

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL080621\  
 Data File : PL068799.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 06 Aug 2021 16:31  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 09 00:52:41 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL080521.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Aug 06 03:02:43 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2    | Resp#1   | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|--------|---------|----------|----------|--------|----------|
| -----                       |                 |        |         |          |          |        |          |
| System Monitoring Compounds |                 |        |         |          |          |        |          |
| 1)                          | SA Tetrachlo... | 4.638  | 5.569   | 8214062  | 22659512 | 19.858 | 22.317   |
| 28)                         | SA Decachlor... | 10.409 | 11.489  | 11547076 | 20642648 | 20.093 | 21.276   |
| Target Compounds            |                 |        |         |          |          |        |          |
| 15)                         | B Endosulfa...  | 0.000  | 9.215   | 0        | 1001655  | N.D.   | 1.092 #  |
| 17)                         | MA 4,4'-DDT     | 0.000  | 9.444f  | 0        | 39992    | N.D.   | 0.042 #  |
| 19)                         | B Endosulfa...  | 0.000  | 9.592f  | 0        | 87342    | N.D.   | 0.096 #  |
| 20)                         | A Methoxychlor  | 9.093  | 0.000   | 2541337  | 0        | 8.118  | N.D. #   |
| 22)                         | Mirex           | 0.000  | 10.570f | 0        | 38824    | N.D.   | 0.049 #  |
| 23)                         | Chlordane-1     | 0.000  | 6.974f  | 0        | 441752   | N.D.   | 10.476 # |
| -----                       |                 |        |         |          |          |        |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL080621\  
Data File : PL068799.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 06 Aug 2021 16:31  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 09 00:52:41 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL080521.M  
Quant Title : GC Extractables  
QLast Update : Fri Aug 06 03:02:43 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

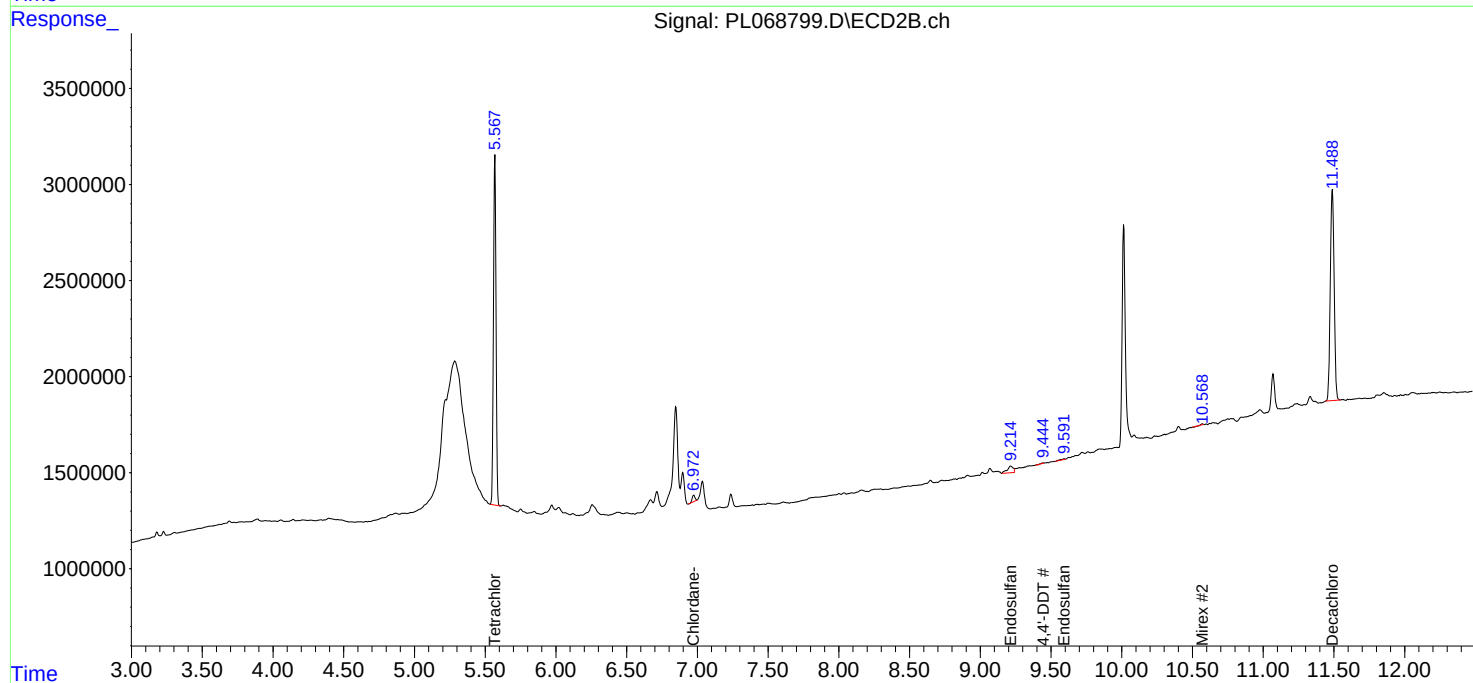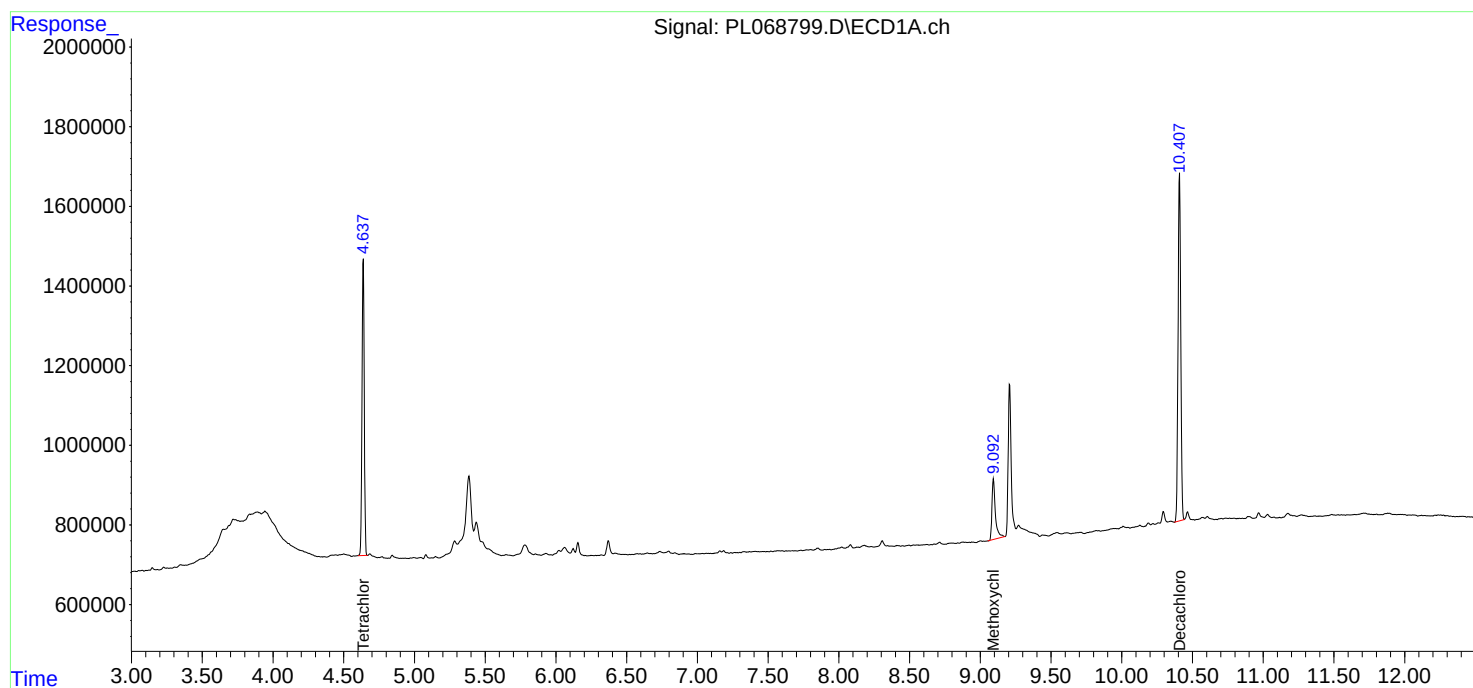


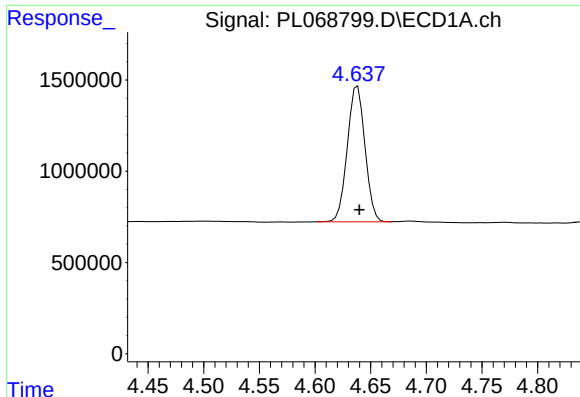

#1 Tetrachloro-m-xylene


R.T.: 4.638 min  
Delta R.T.: -0.002 min  
Response: 8214062  
Conc: 19.86 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

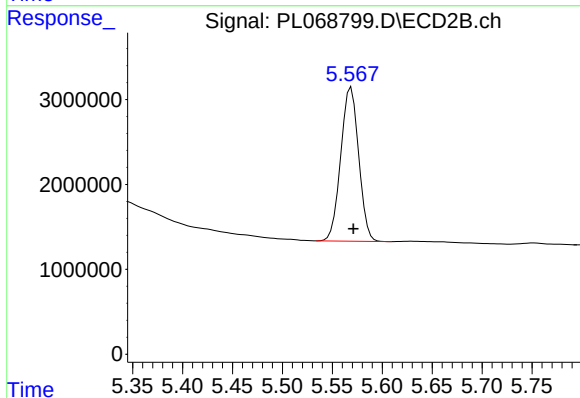


#1 Tetrachloro-m-xylene

R.T.: 5.569 min  
Delta R.T.: -0.002 min  
Response: 22659512  
Conc: 22.32 ng/ml

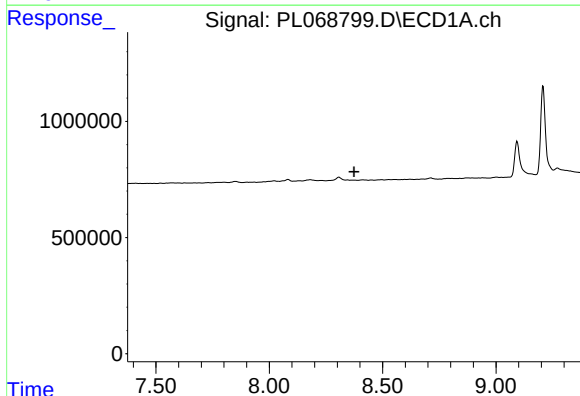


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 8.375 min  
Response: 0  
Conc: N.D.

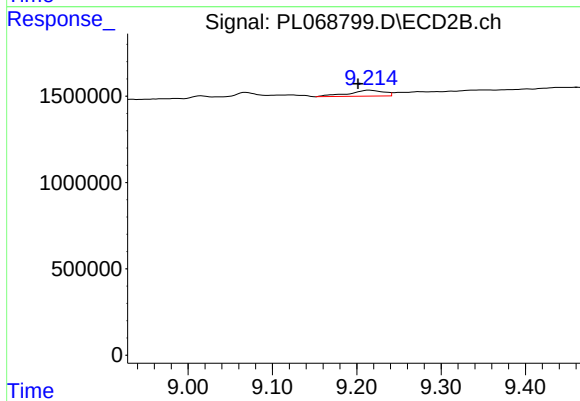

#15 Endosulfan II


R.T.: 9.215 min  
Delta R.T.: 0.014 min  
Response: 1001655  
Conc: 1.09 ng/ml

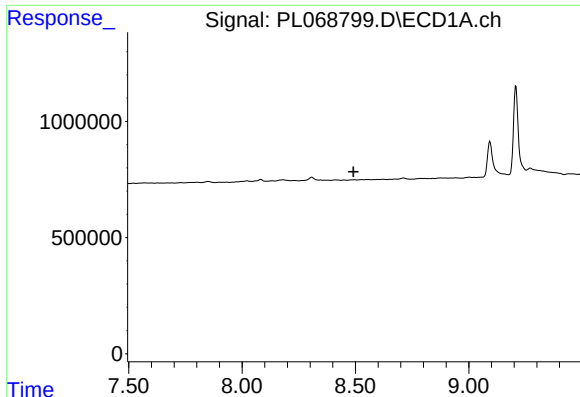

#17 4,4'-DDT


R.T.: 0.000 min  
Exp R.T.: 8.492 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

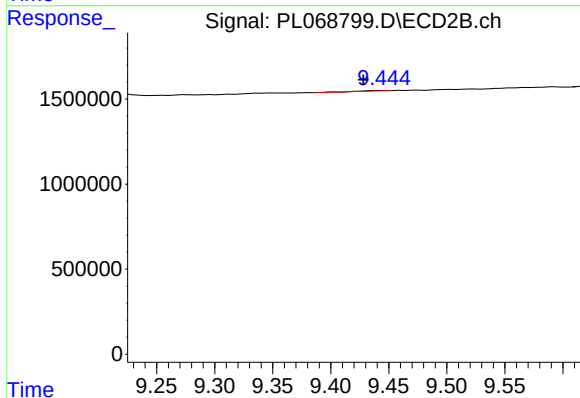


#17 4,4'-DDT

R.T.: 9.444 min  
Delta R.T.: 0.015 min  
Response: 39992  
Conc: 0.04 ng/ml

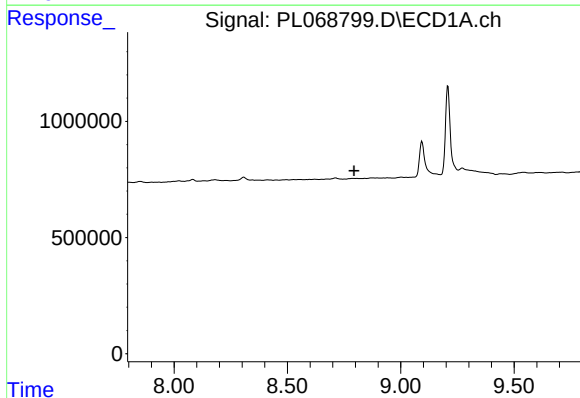


#19 Endosulfan Sulfate

R.T.: 0.000 min  
Exp R.T.: 8.794 min  
Response: 0  
Conc: N.D.

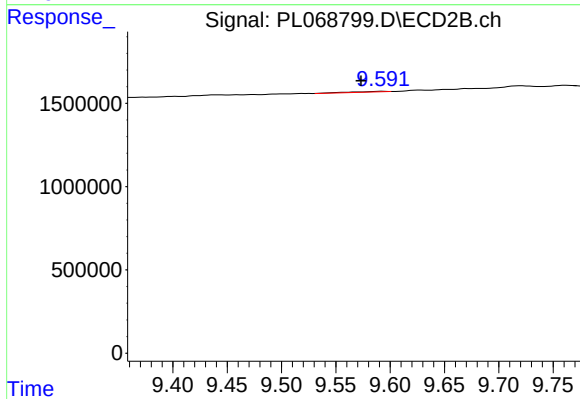

#19 Endosulfan Sulfate


R.T.: 9.592 min  
Delta R.T.: 0.019 min  
Response: 87342  
Conc: 0.10 ng/ml

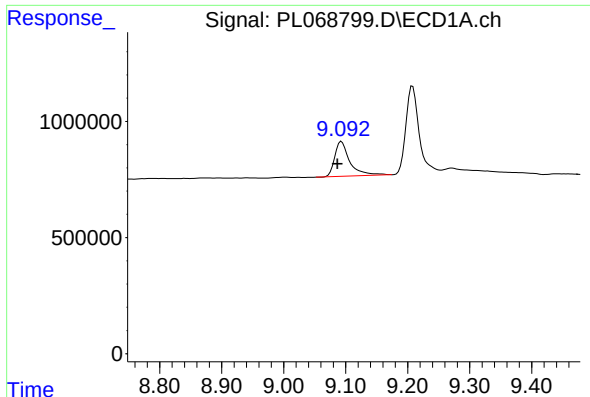

#20 Methoxychlor


R.T.: 9.093 min  
Delta R.T.: 0.007 min  
Response: 2541337  
Conc: 8.12 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

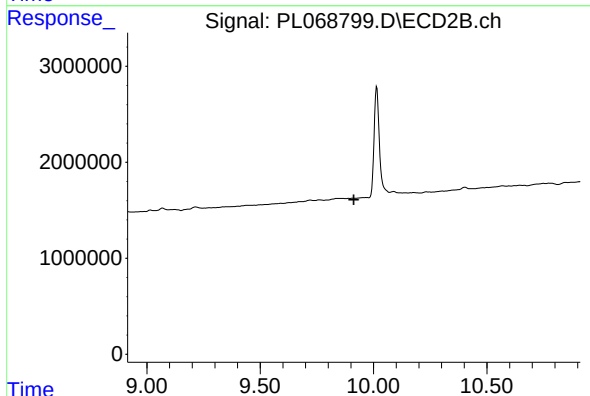


#20 Methoxychlor

R.T.: 0.000 min  
Exp R.T. : 9.913 min  
Response: 0  
Conc: N.D.

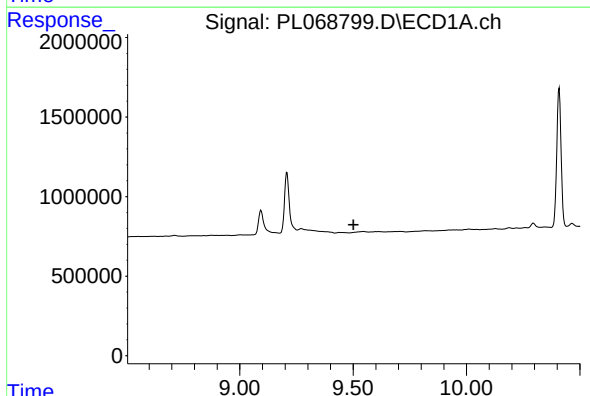


#22 Mirex

R.T.: 0.000 min  
Exp R.T. : 9.502 min  
Response: 0  
Conc: N.D.

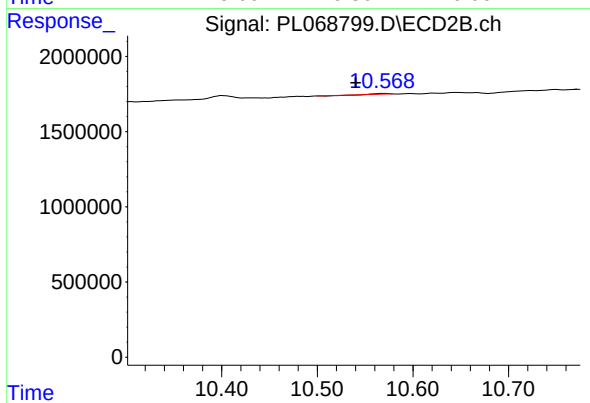

#22 Mirex


R.T.: 10.570 min  
Delta R.T.: 0.030 min  
Response: 38824  
Conc: 0.05 ng/ml

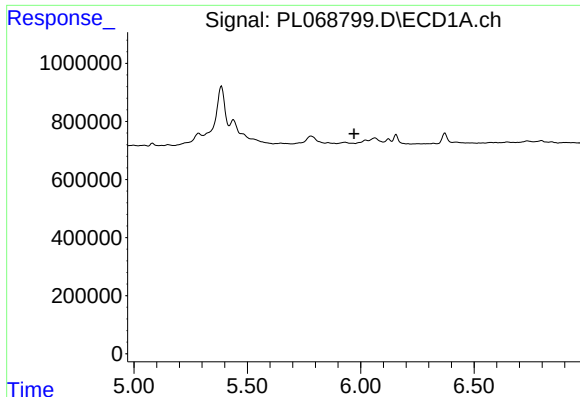

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T.: 5.971 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

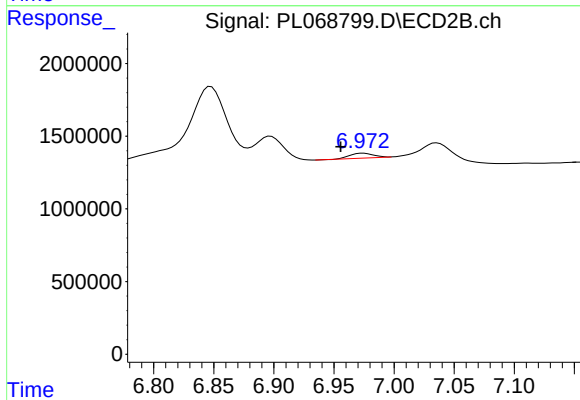


#23 Chlordane-1

R.T.: 6.974 min  
Delta R.T.: 0.019 min  
Response: 441752  
Conc: 10.48 ng/ml

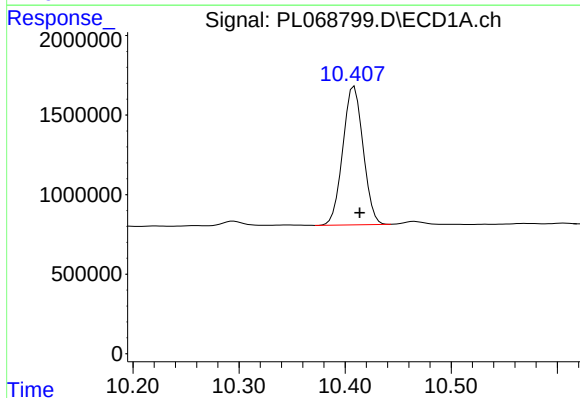

#28 Decachlorobiphenyl

R.T.: 10.409 min  
Delta R.T.: -0.005 min  
Response: 11547076  
Conc: 20.09 ng/ml

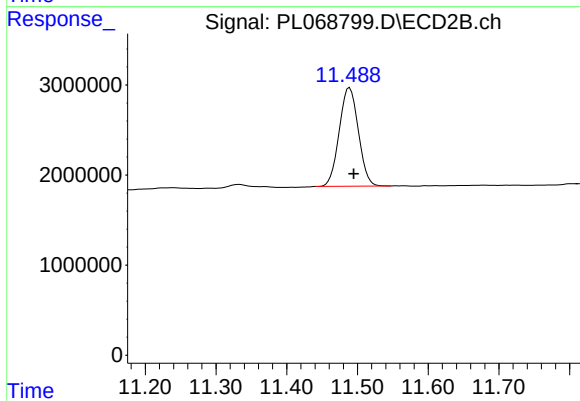

#28 Decachlorobiphenyl

R.T.: 11.489 min  
Delta R.T.: -0.006 min  
Response: 20642648  
Conc: 21.28 ng/ml