

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 16:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:52:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.569	8214062	22659512	19.858	22.317
28)	SA Decachlor...	10.409	11.489	11547076	20642648	20.093	21.276
Target Compounds							
15)	B Endosulfa...	0.000	9.215	0	1001655	N.D.	1.092 #
17)	MA 4,4'-DDT	0.000	9.444f	0	39992	N.D.	0.042 #
19)	B Endosulfa...	0.000	9.592f	0	87342	N.D.	0.096 #
20)	A Methoxychlor	9.093	0.000	2541337	0	8.118	N.D. #
22)	Mirex	0.000	10.570f	0	38824	N.D.	0.049 #
23)	Chlordane-1	0.000	6.974f	0	441752	N.D.	10.476 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 16:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:52:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

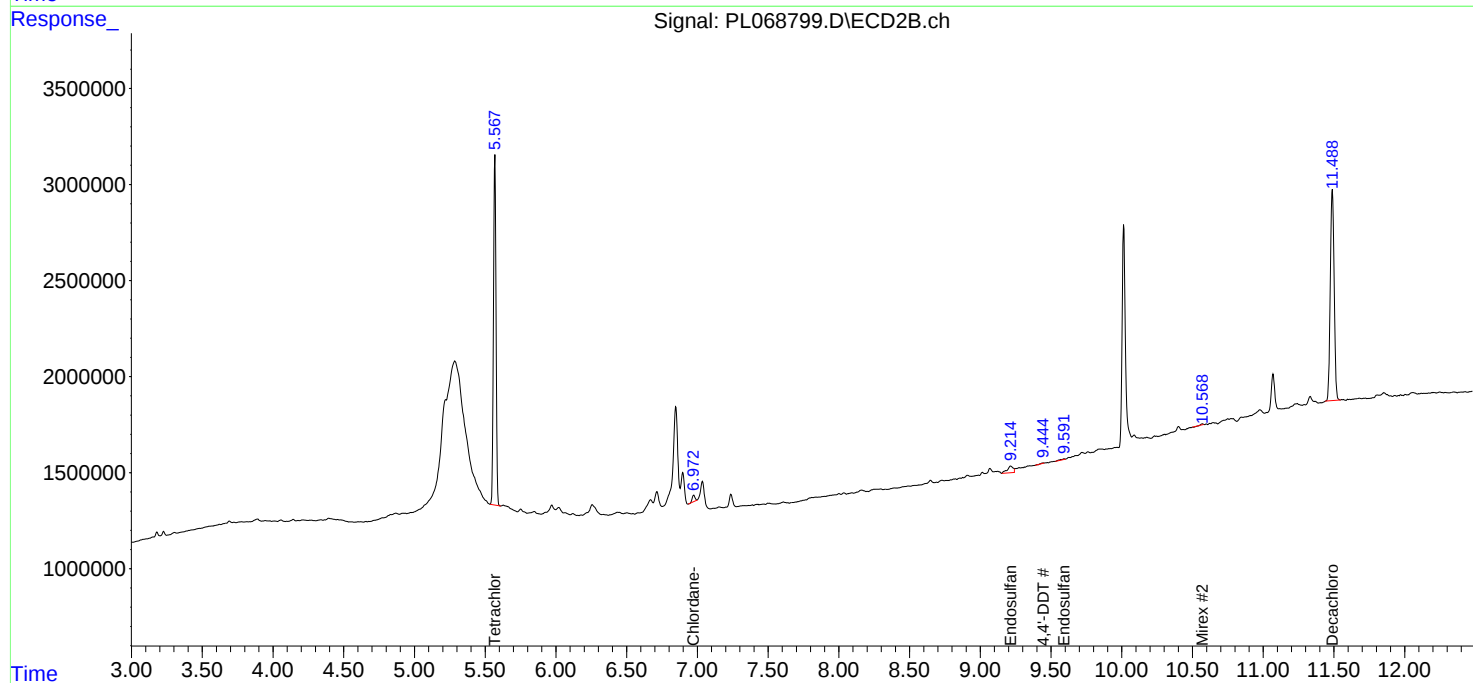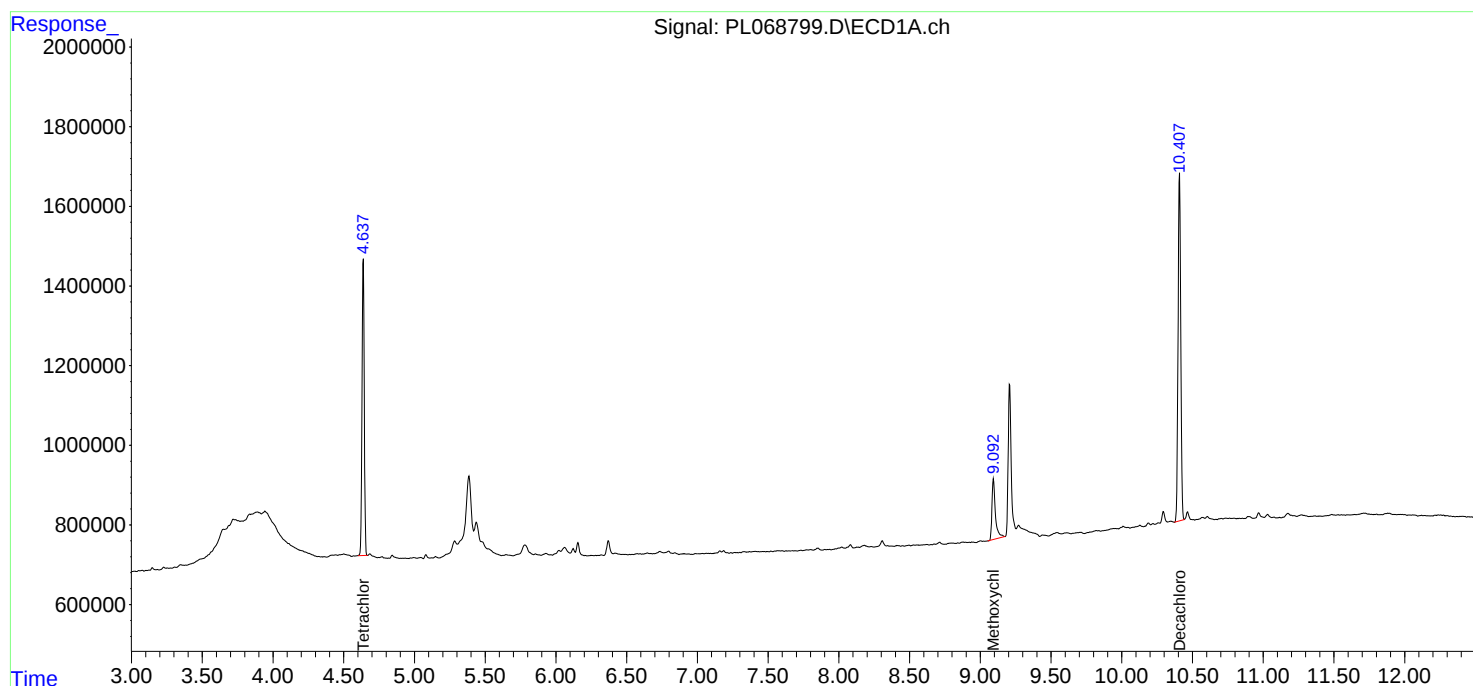


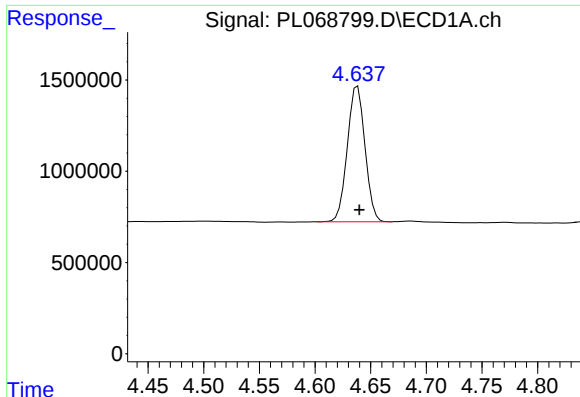

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 8214062
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

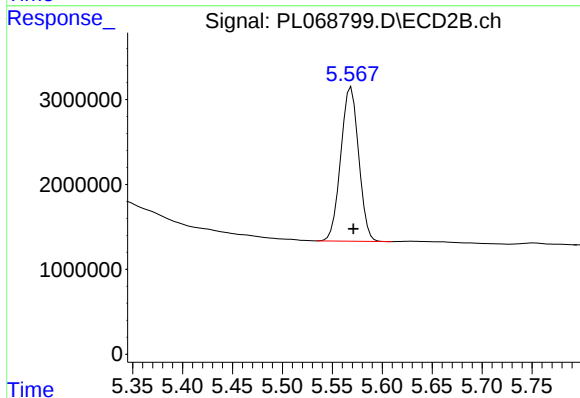


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 22659512
Conc: 22.32 ng/ml

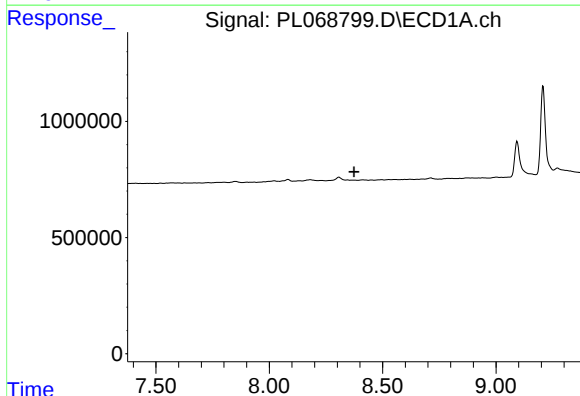


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

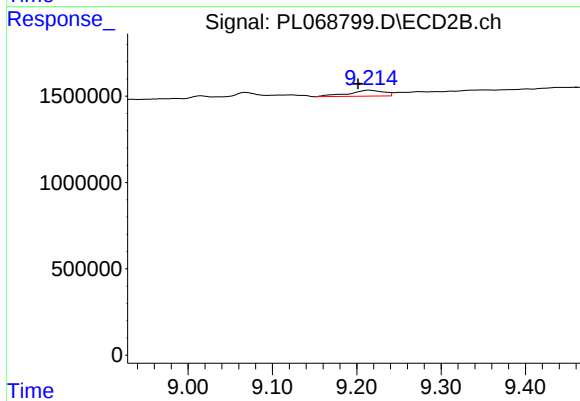

#15 Endosulfan II


R.T.: 9.215 min
Delta R.T.: 0.014 min
Response: 1001655
Conc: 1.09 ng/ml

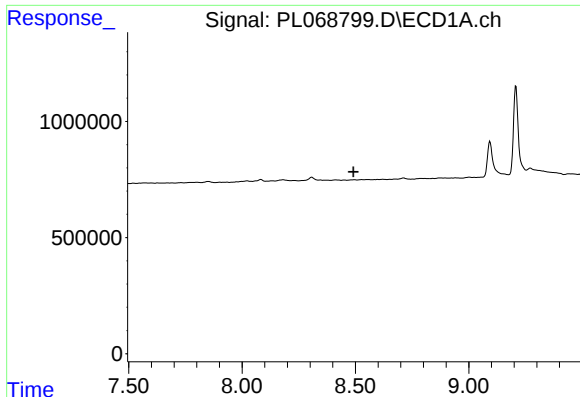

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

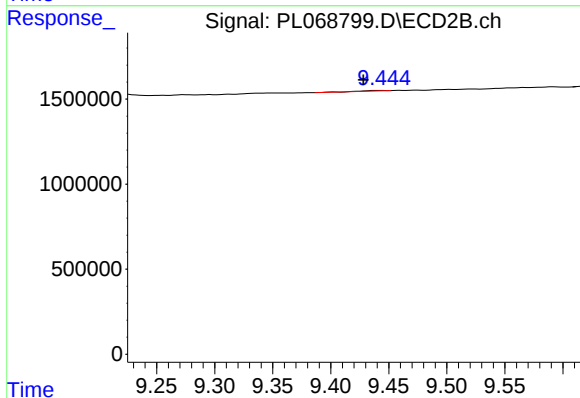


#17 4,4'-DDT

R.T.: 9.444 min
Delta R.T.: 0.015 min
Response: 39992
Conc: 0.04 ng/ml

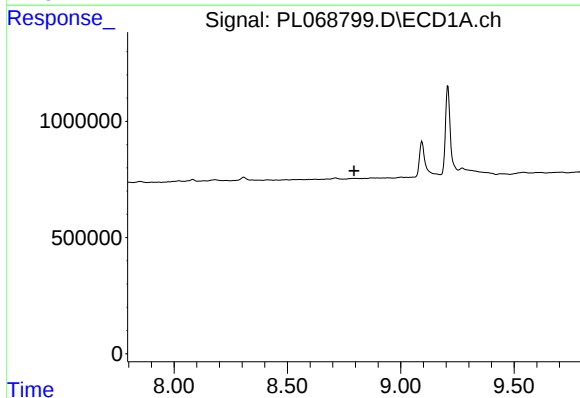


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

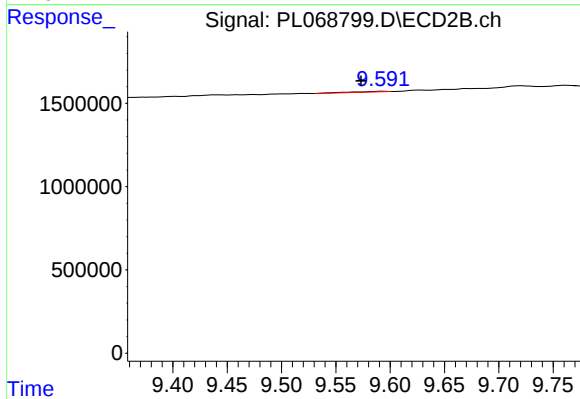

#19 Endosulfan Sulfate


R.T.: 9.592 min
Delta R.T.: 0.019 min
Response: 87342
Conc: 0.10 ng/ml

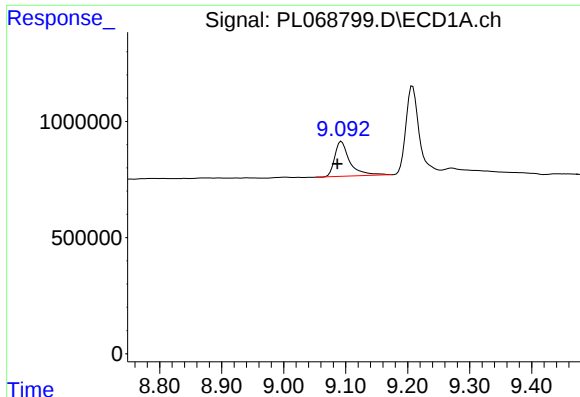

#20 Methoxychlor


R.T.: 9.093 min
Delta R.T.: 0.007 min
Response: 2541337
Conc: 8.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

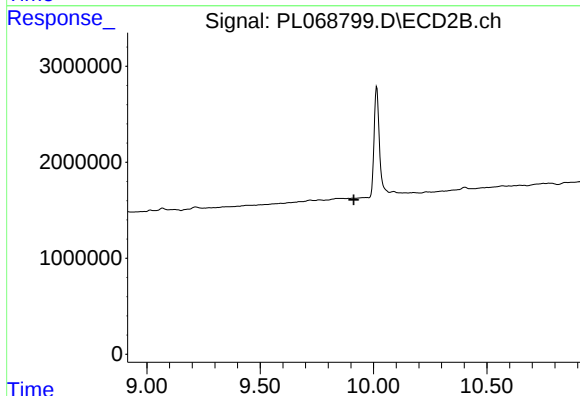


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.913 min
Response: 0
Conc: N.D.

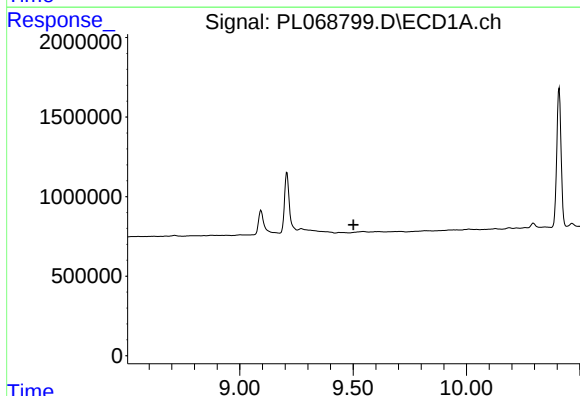


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

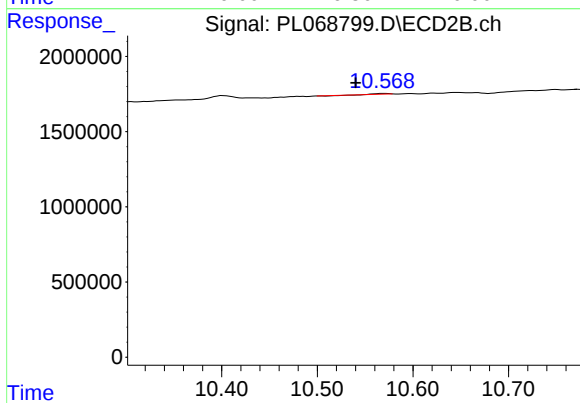

#22 Mirex


R.T.: 10.570 min
Delta R.T.: 0.030 min
Response: 38824
Conc: 0.05 ng/ml

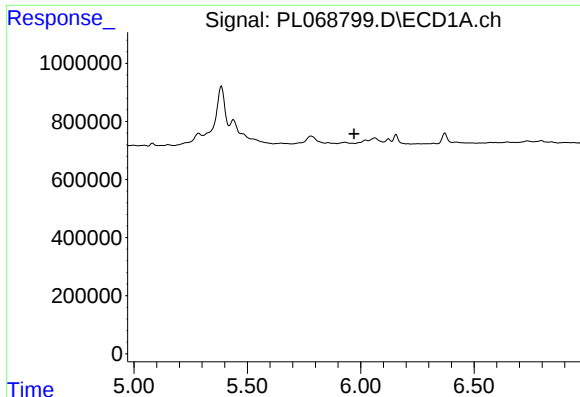

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

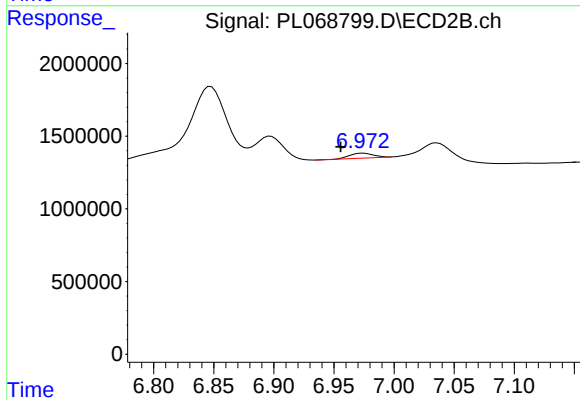


#23 Chlordane-1

R.T.: 6.974 min
Delta R.T.: 0.019 min
Response: 441752
Conc: 10.48 ng/ml

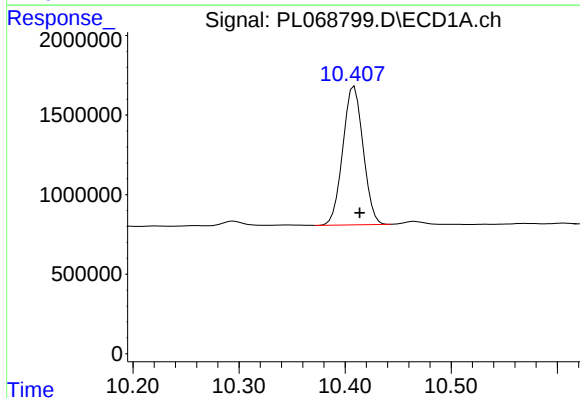

#28 Decachlorobiphenyl

R.T.: 10.409 min
Delta R.T.: -0.005 min
Response: 11547076
Conc: 20.09 ng/ml

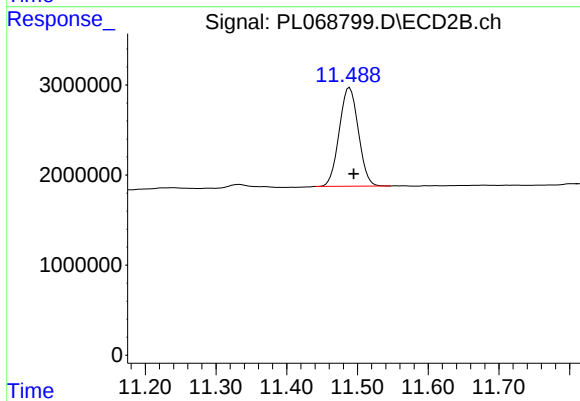

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.006 min
Response: 20642648
Conc: 21.28 ng/ml