

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 19:03
 Operator : AR\AJ
 Sample : PB138237BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138237BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:53:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.568	8046729	21954082	19.453	21.622
28)	SA Decachlor...	10.407	11.488	11766636	20056244	20.475	20.671
Target Compounds							
3)	MA gamma-BHC...	5.783	0.000	605138	0	1.115	N.D. #
9)	A Endosulfan I	0.000	8.460f	0	52047	N.D.	0.049 #
11)	B alpha-Chl...	0.000	8.394	0	64274	N.D.	0.056 #
13)	MA Dieldrin	0.000	8.727	0	137431	N.D.	0.127 #
15)	B Endosulfa...	0.000	9.214	0	394581	N.D.	0.430 #
21)	B Endrin ke...	0.000	10.088f	0	130922	N.D.	0.129 #
23)	Chlordane-1	0.000	6.974f	0	548112	N.D.	12.998 #
26)	Chlordane-4	0.000	8.394	0	64274	N.D.	0.324 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 19:03
Operator : AR\AJ
Sample : PB138237BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB138237BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:53:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

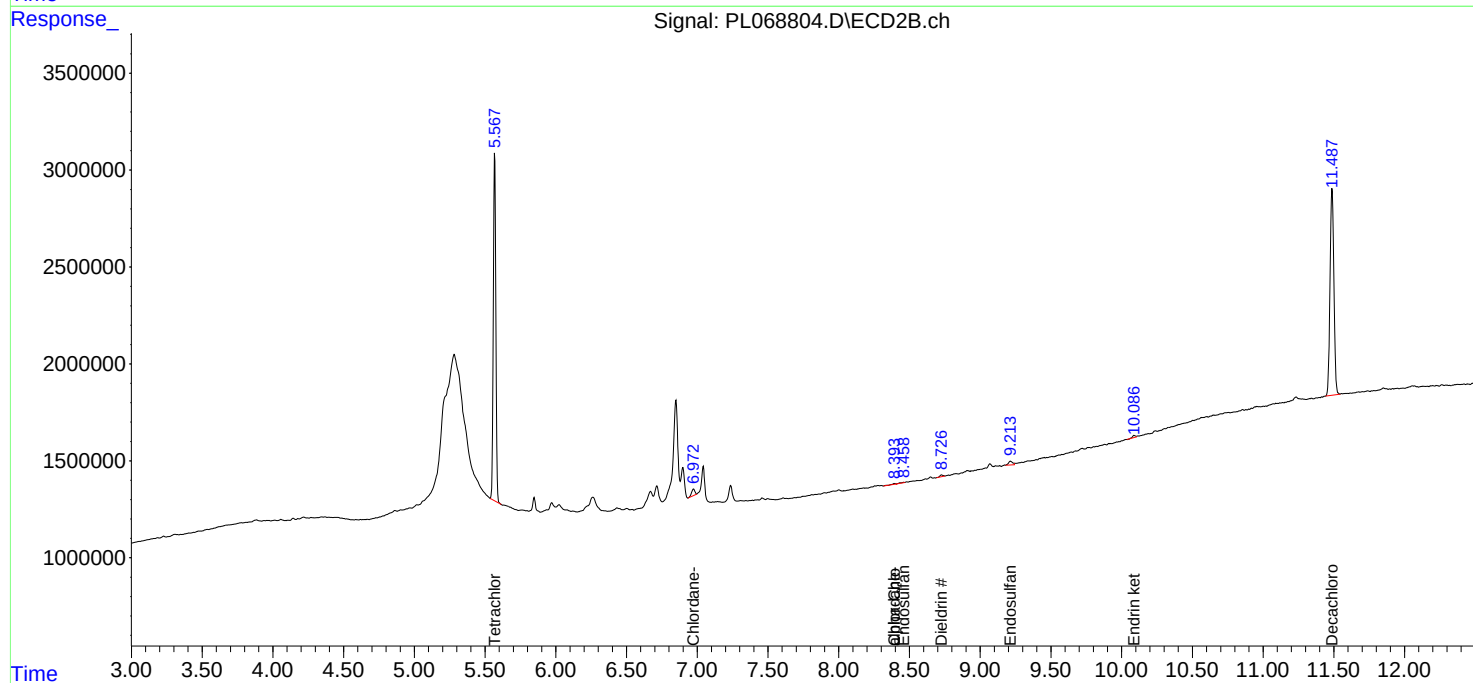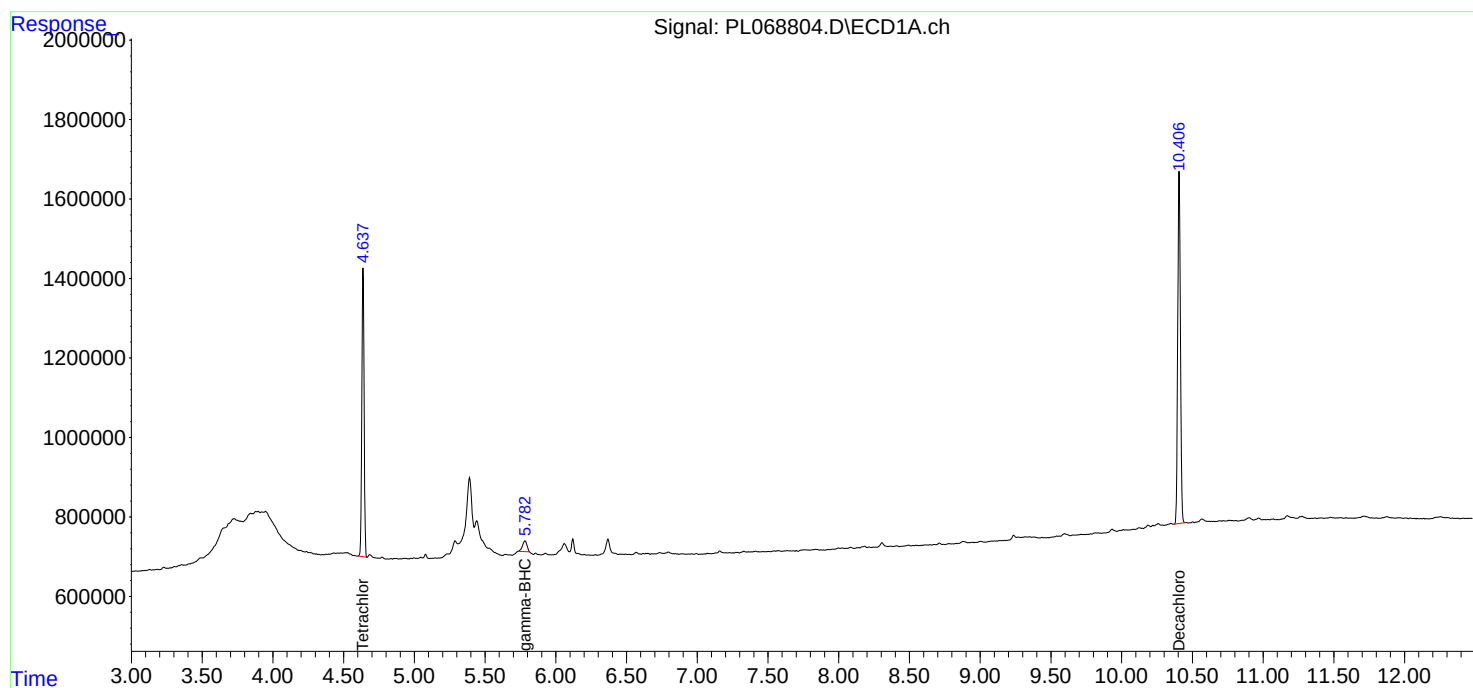


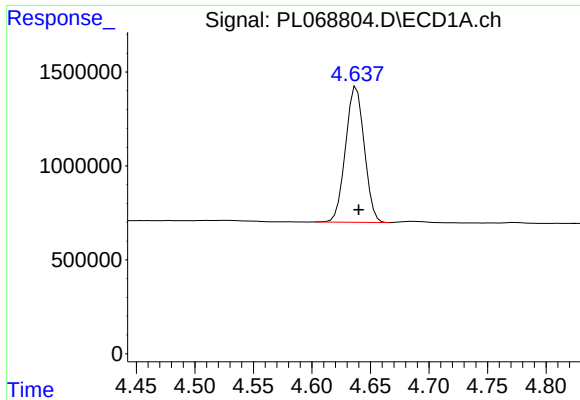

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 8046729
Conc: 19.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138237BL

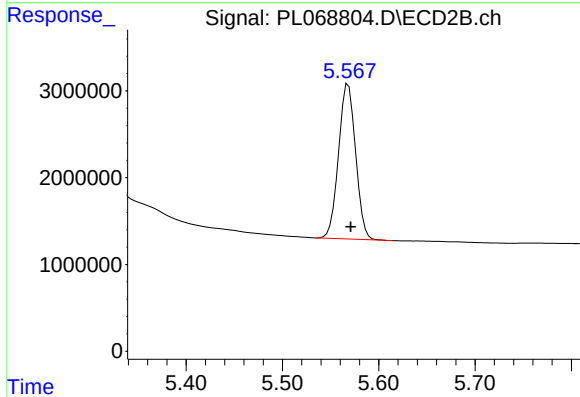


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 21954082
Conc: 21.62 ng/ml

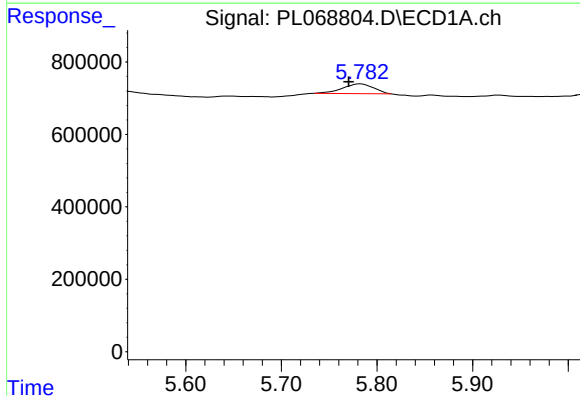


#3 gamma-BHC (Lindane)

R.T.: 5.783 min
Delta R.T.: 0.012 min
Response: 605138
Conc: 1.11 ng/ml

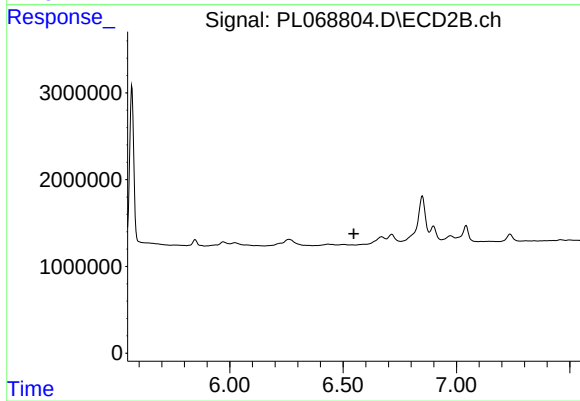

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.547 min
Response: 0
Conc: N.D.

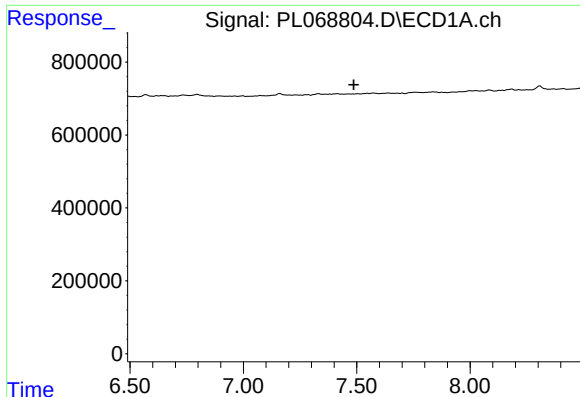

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138237BL

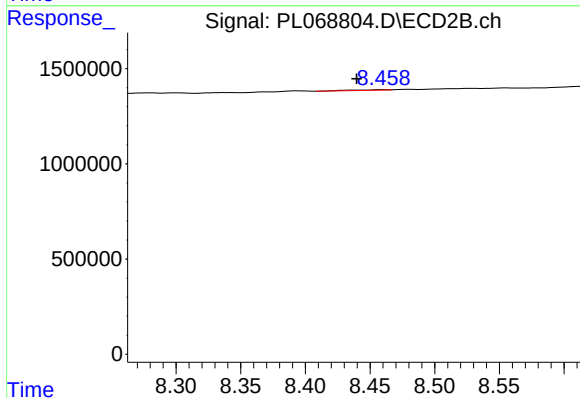


#9 Endosulfan I

R.T.: 8.460 min
Delta R.T.: 0.020 min
Response: 52047
Conc: 0.05 ng/ml

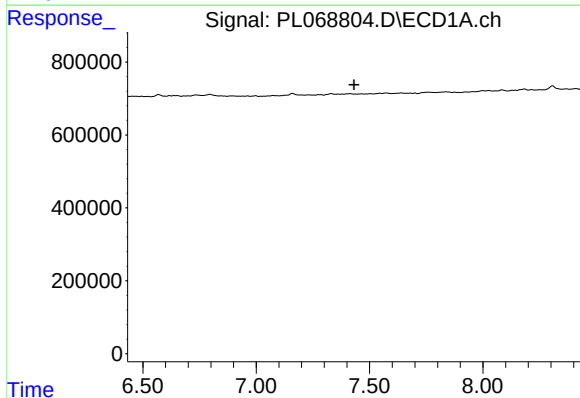


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

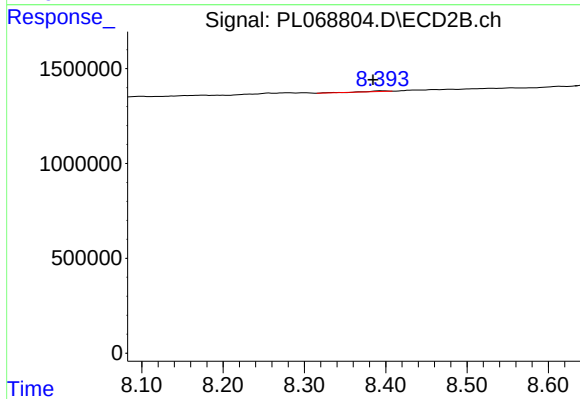

#11 alpha-Chlordane


R.T.: 8.394 min
Delta R.T.: 0.010 min
Response: 64274
Conc: 0.06 ng/ml

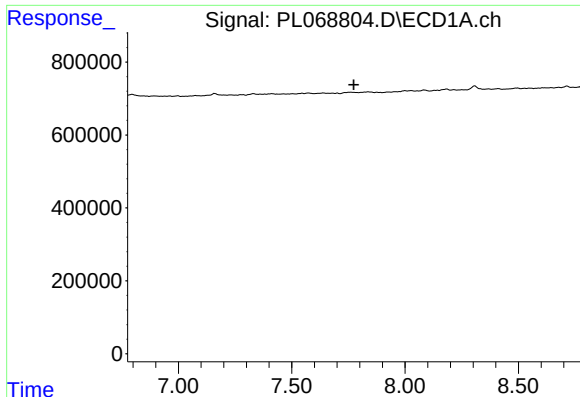

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138237BL

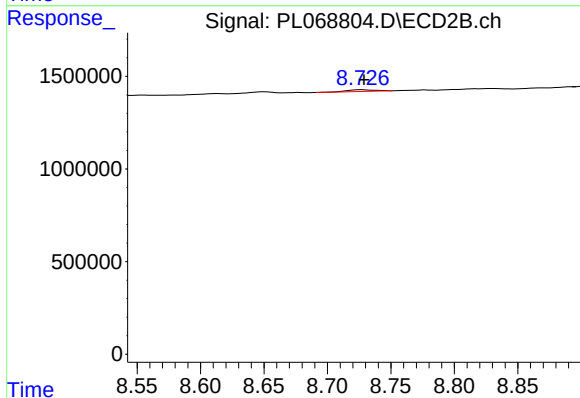


#13 Dieldrin

R.T.: 8.727 min
Delta R.T.: -0.002 min
Response: 137431
Conc: 0.13 ng/ml

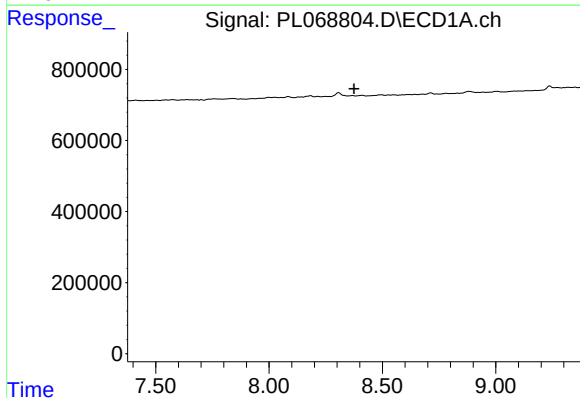


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

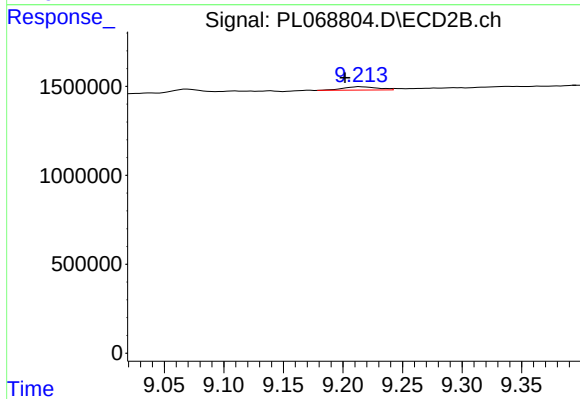

#15 Endosulfan II


R.T.: 9.214 min
Delta R.T.: 0.013 min
Response: 394581
Conc: 0.43 ng/ml

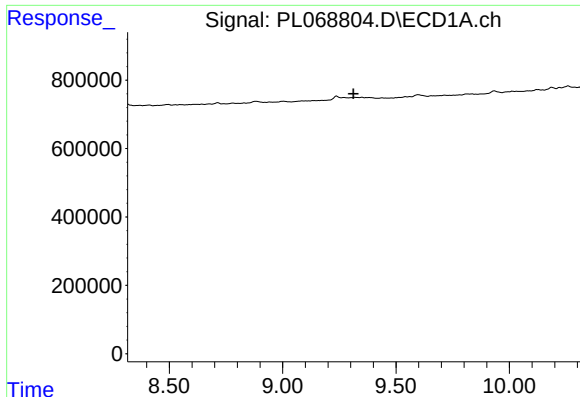

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138237BL

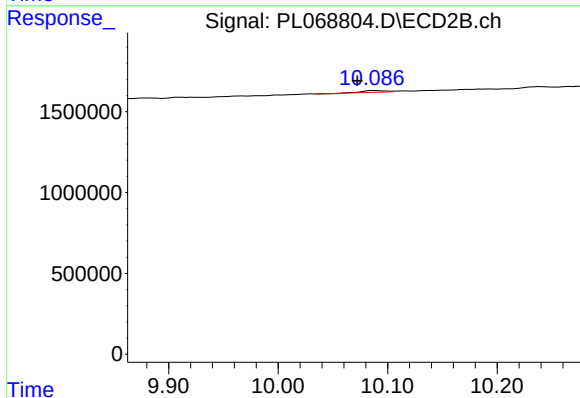


#21 Endrin ketone

R.T.: 10.088 min
Delta R.T.: 0.015 min
Response: 130922
Conc: 0.13 ng/ml

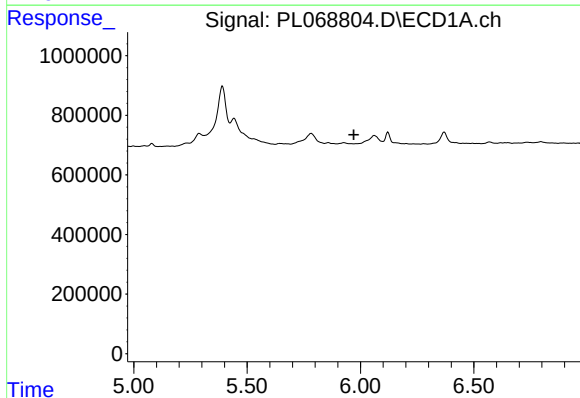


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

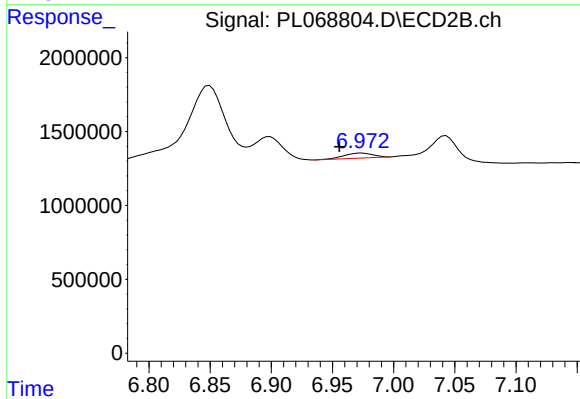

#23 Chlordane-1


R.T.: 6.974 min
Delta R.T.: 0.018 min
Response: 548112
Conc: 13.00 ng/ml

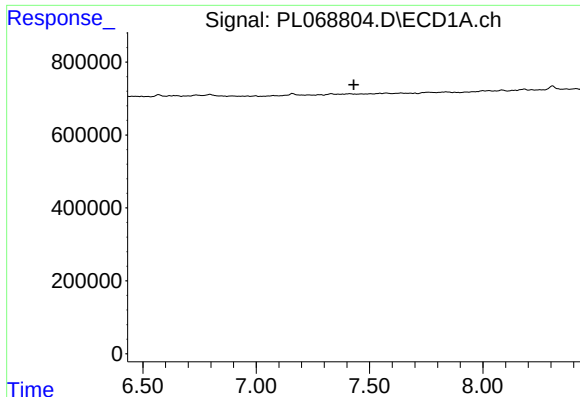

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138237BL

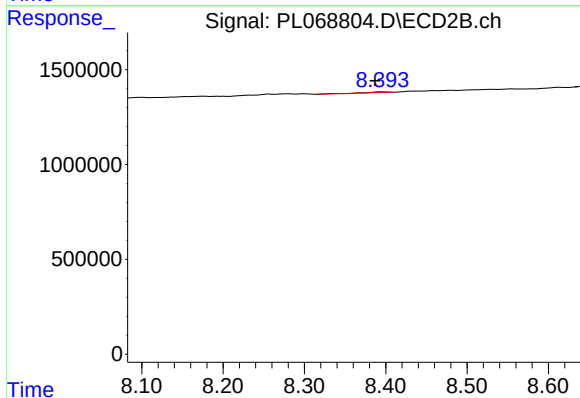


#26 Chlordane-4

R.T.: 8.394 min
Delta R.T.: 0.007 min
Response: 64274
Conc: 0.32 ng/ml

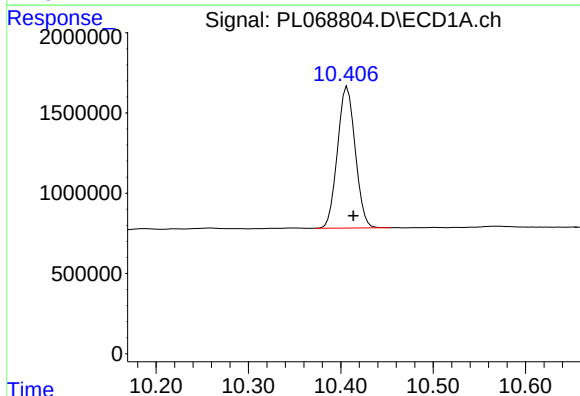

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.006 min
Response: 11766636
Conc: 20.47 ng/ml

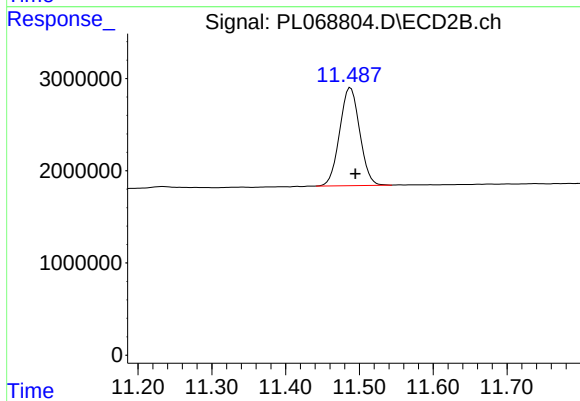

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 20056244
Conc: 20.67 ng/ml