

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 21:17
 Operator : AR\AJ
 Sample : M3296-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:55:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.568	11378796	30301862	27.509	29.844
28)	SA Decachlor...	10.408	11.488	13856554	25783653	24.111	26.574
Target Compounds							
9)	A Endosulfan I	0.000	8.455f	0	68839	N.D.	0.065 #
11)	B alpha-Chl...	0.000	8.392	0	56490	N.D.	0.049 #
13)	MA Dieldrin	0.000	8.724	0	58513	N.D.	0.054 #
15)	B Endosulfa...	0.000	9.216	0	2047148	N.D.	2.232 #
19)	B Endosulfa...	0.000	9.578	0	107141	N.D.	0.118 #
21)	B Endrin ke...	0.000	10.095f	0	112426	N.D.	0.110 #
23)	Chlordane-1	0.000	6.976f	0	347569	N.D.	8.242 #
26)	Chlordane-4	0.000	8.392	0	56490	N.D.	0.285 #
27)	Chlordane-5	0.000	9.289	0	186071	N.D.	5.372 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 21:17
Operator : AR\AJ
Sample : M3296-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:55:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

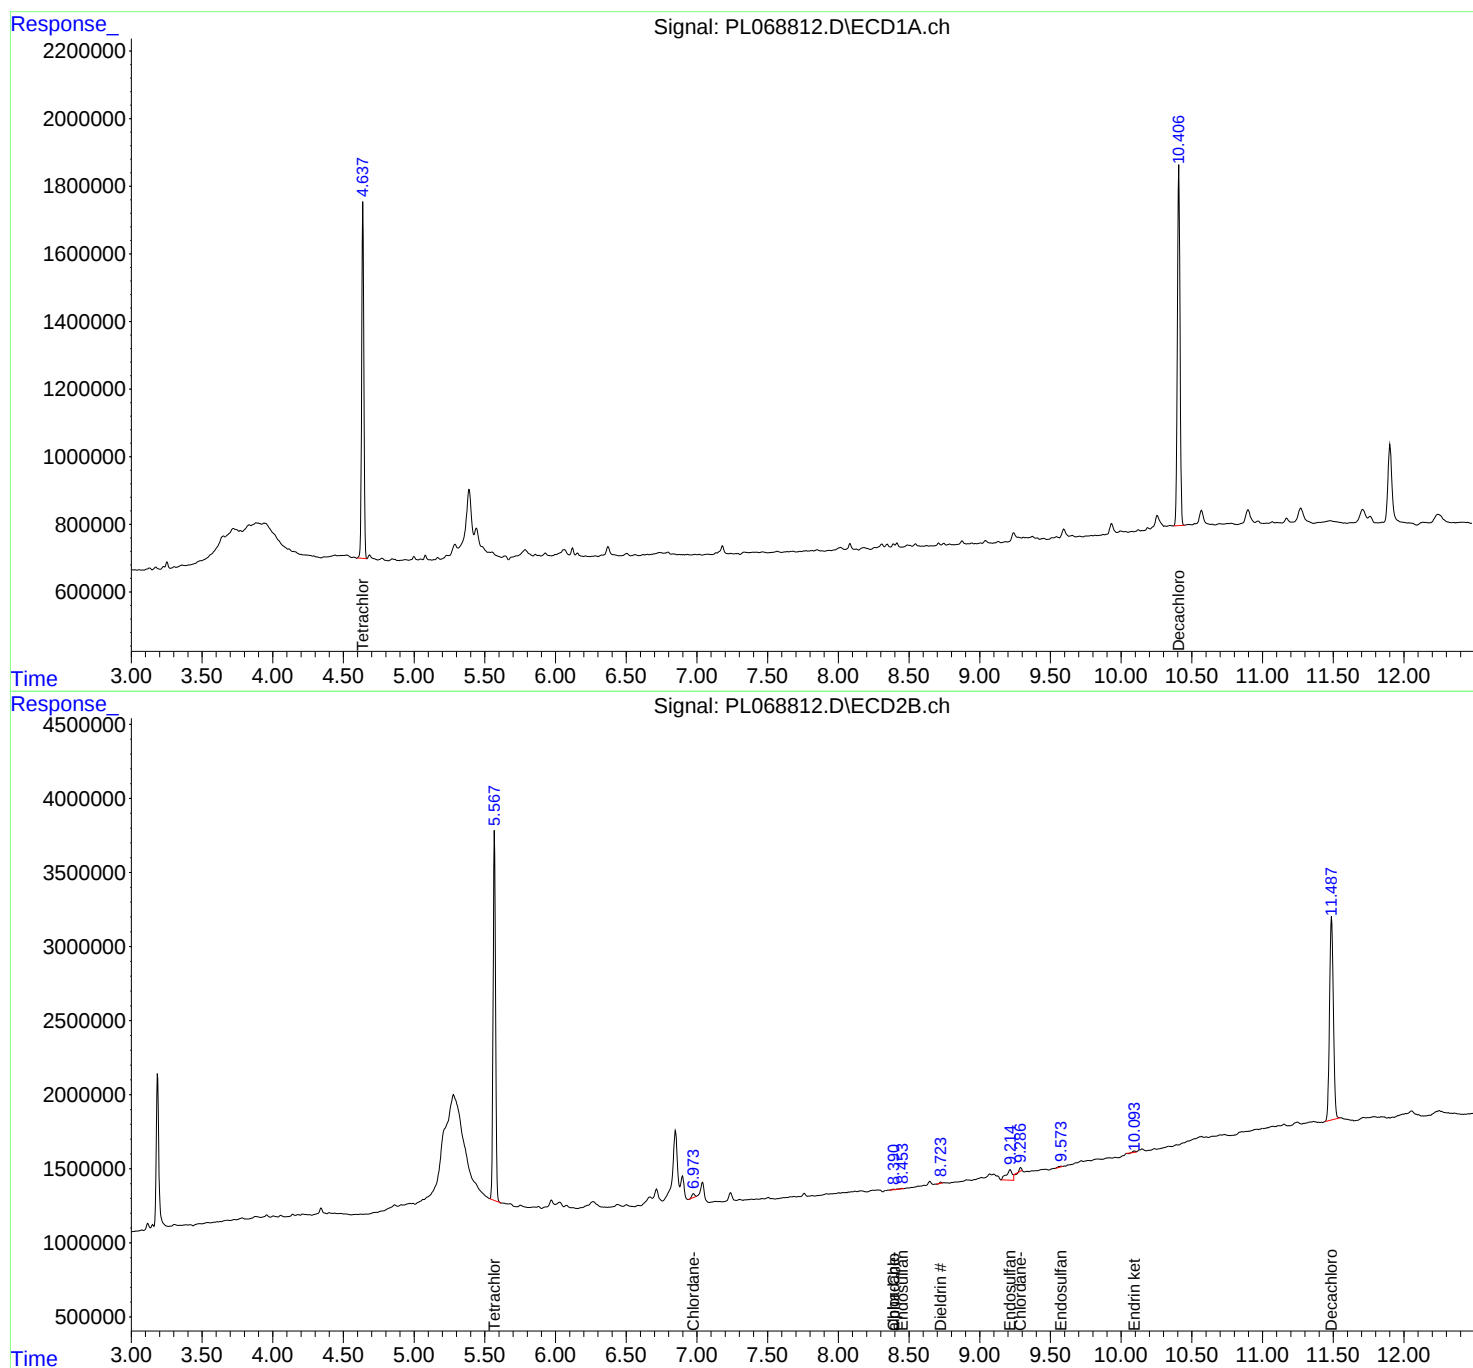


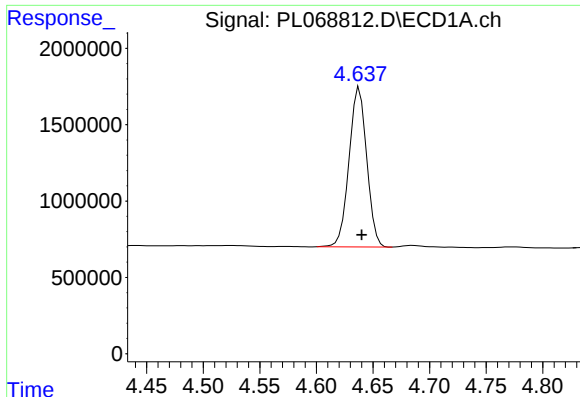

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 11378796
Conc: 27.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

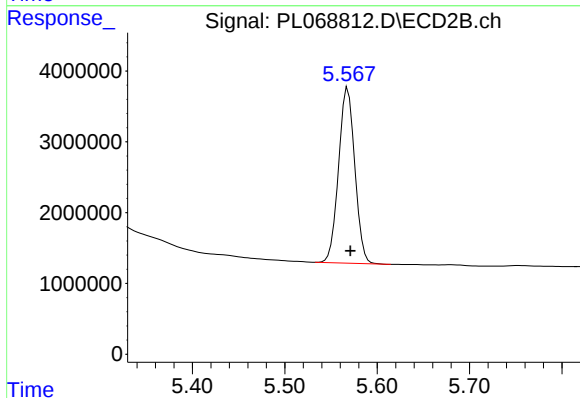


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 30301862
Conc: 29.84 ng/ml

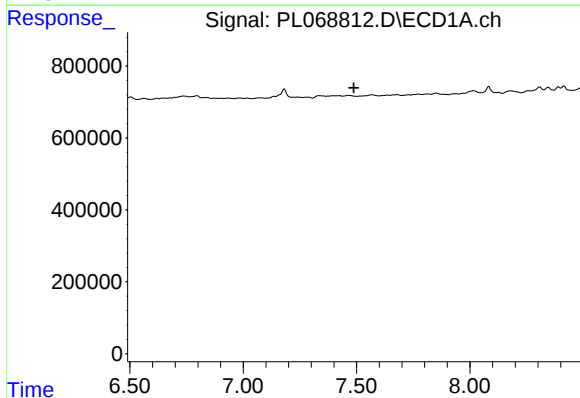


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

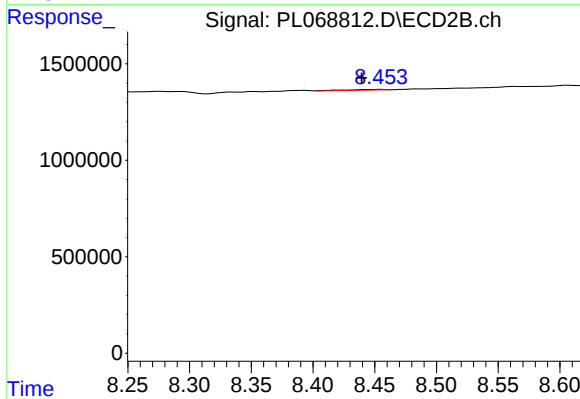

#9 Endosulfan I


R.T.: 8.455 min
Delta R.T.: 0.015 min
Response: 68839
Conc: 0.07 ng/ml

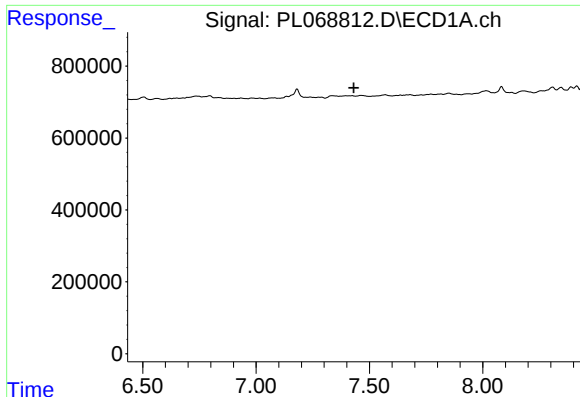

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

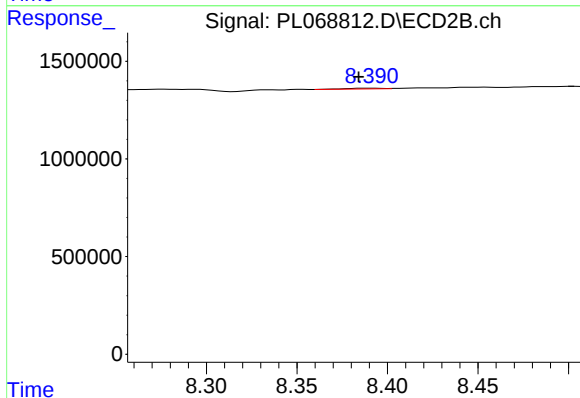


#11 alpha-Chlordane

R.T.: 8.392 min
Delta R.T.: 0.007 min
Response: 56490
Conc: 0.05 ng/ml

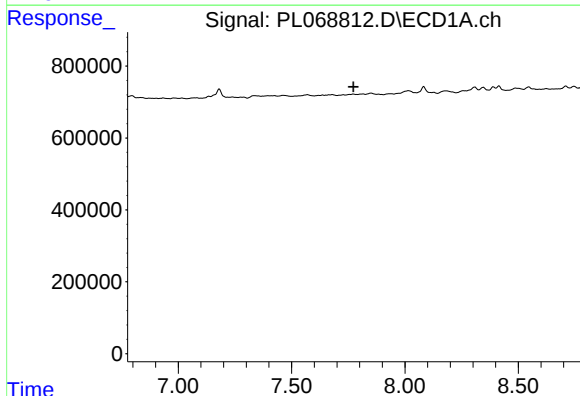


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

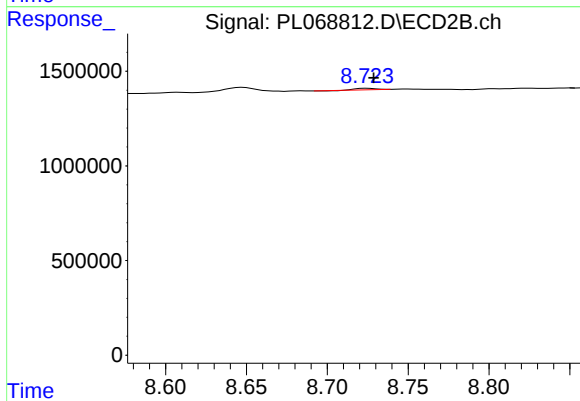

#13 Dieldrin


R.T.: 8.724 min
Delta R.T.: -0.004 min
Response: 58513
Conc: 0.05 ng/ml

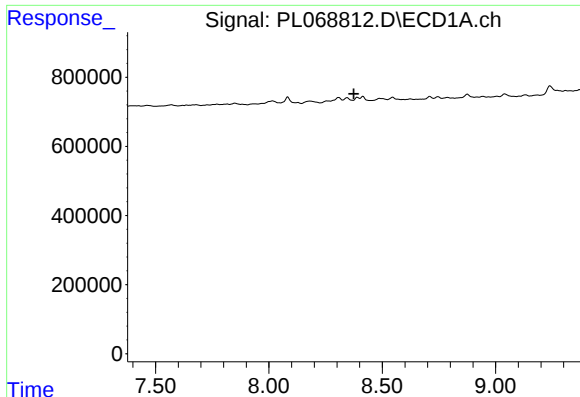

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

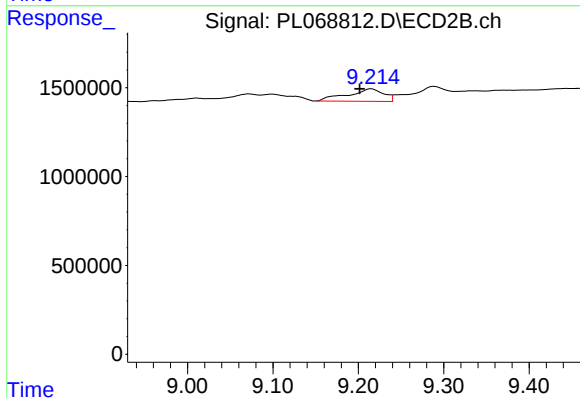


#15 Endosulfan II

R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 2047148
Conc: 2.23 ng/ml

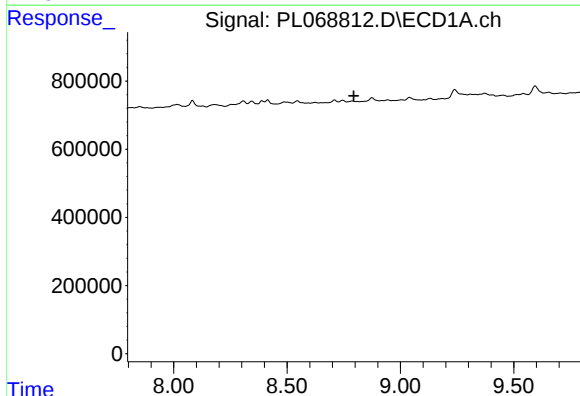


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

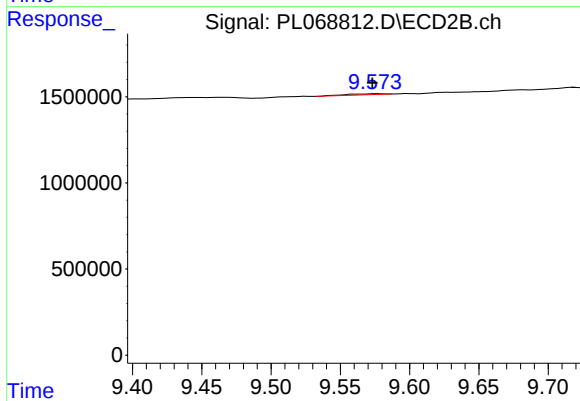

#19 Endosulfan Sulfate


R.T.: 9.578 min
Delta R.T.: 0.004 min
Response: 107141
Conc: 0.12 ng/ml

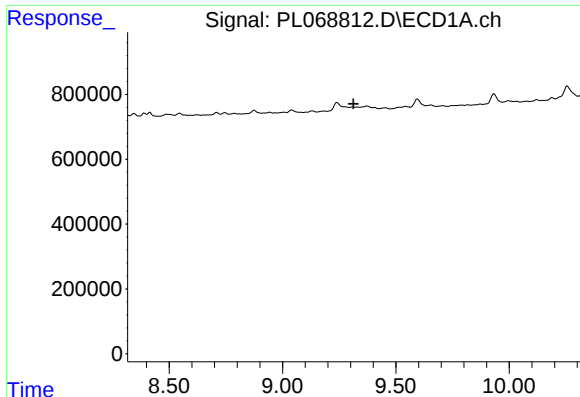

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

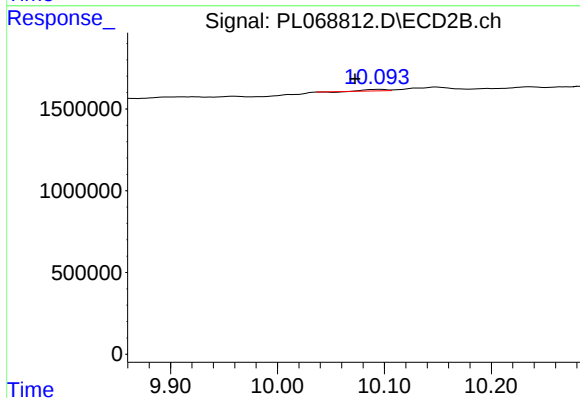


#21 Endrin ketone

R.T.: 10.095 min
Delta R.T.: 0.023 min
Response: 112426
Conc: 0.11 ng/ml

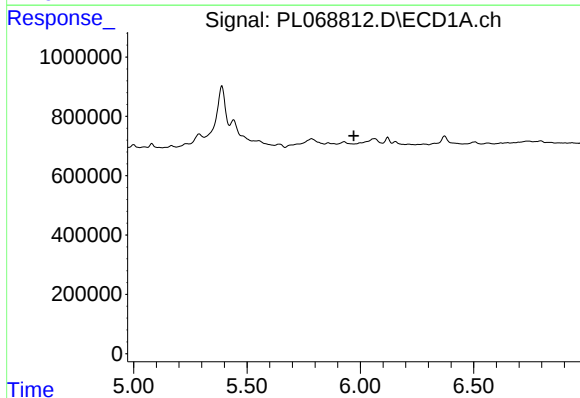


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

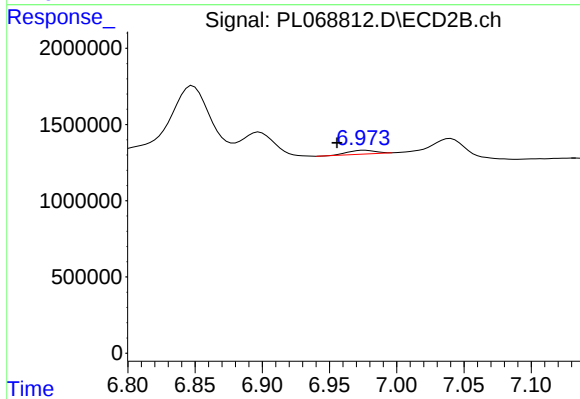

#23 Chlordane-1


R.T.: 6.976 min
Delta R.T.: 0.020 min
Response: 347569
Conc: 8.24 ng/ml

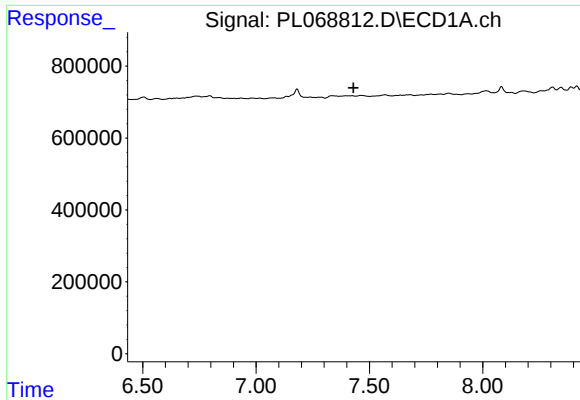

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

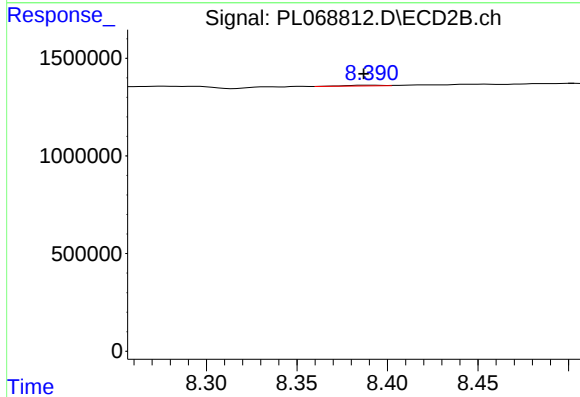


#26 Chlordane-4

R.T.: 8.392 min
Delta R.T.: 0.005 min
Response: 56490
Conc: 0.28 ng/ml

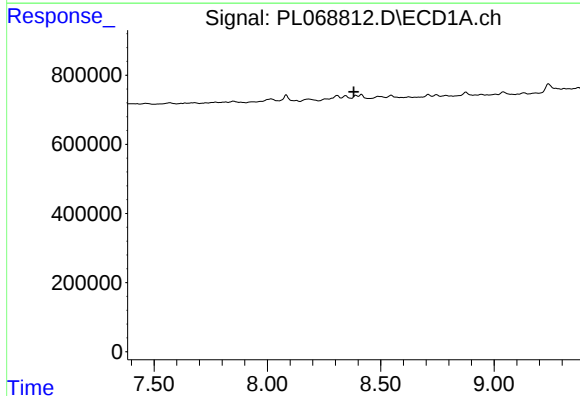


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.380 min
Response: 0
Conc: N.D.

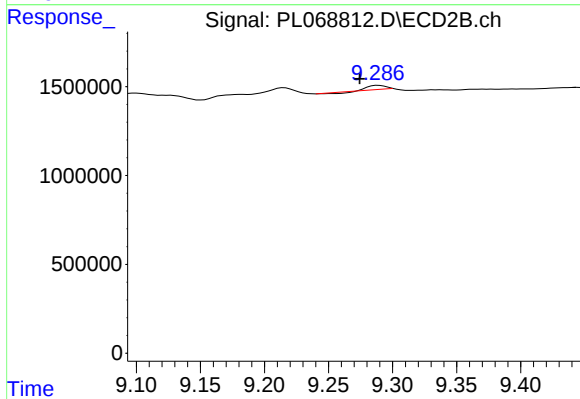

#27 Chlordane-5


R.T.: 9.289 min
Delta R.T.: 0.015 min
Response: 186071
Conc: 5.37 ng/ml

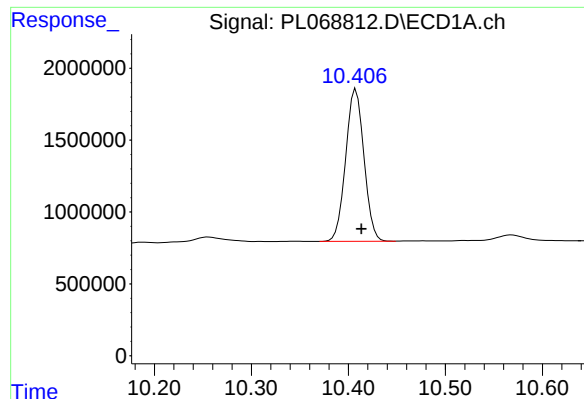

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.006 min
Response: 13856554
Conc: 24.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

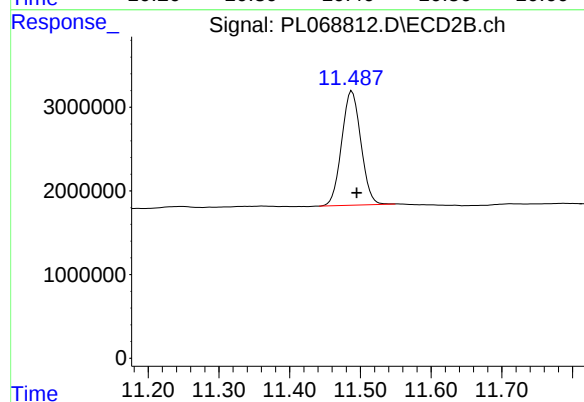

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.006 min
Response: 25783653
Conc: 26.57 ng/ml