

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 22:06
 Operator : AR\AJ
 Sample : M3299-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210560-COM-33

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:56:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.568	6409802	17076845	15.496	16.819
28)	SA Decachlor...	10.408	11.489	7946224	14249435	13.827	14.686
Target Compounds							
10)	B gamma-Chl...	0.000	8.322f	0	266686	N.D.	0.233 #
15)	B Endosulfa...	0.000	9.215	0	319527	N.D.	0.348 #
20)	A Methoxychlor	0.000	9.900	0	386579	N.D.	0.743 #
21)	B Endrin ke...	0.000	10.082	0	302138	N.D.	0.297 #
22)	Mirex	0.000	10.563f	0	102239	N.D.	0.129 #
23)	Chlordane-1	0.000	6.978f	0	114415	N.D.	2.713 #
25)	Chlordane-3	0.000	8.322f	0	266686	N.D.	1.633 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 22:06
Operator : AR\AJ
Sample : M3299-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:56:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

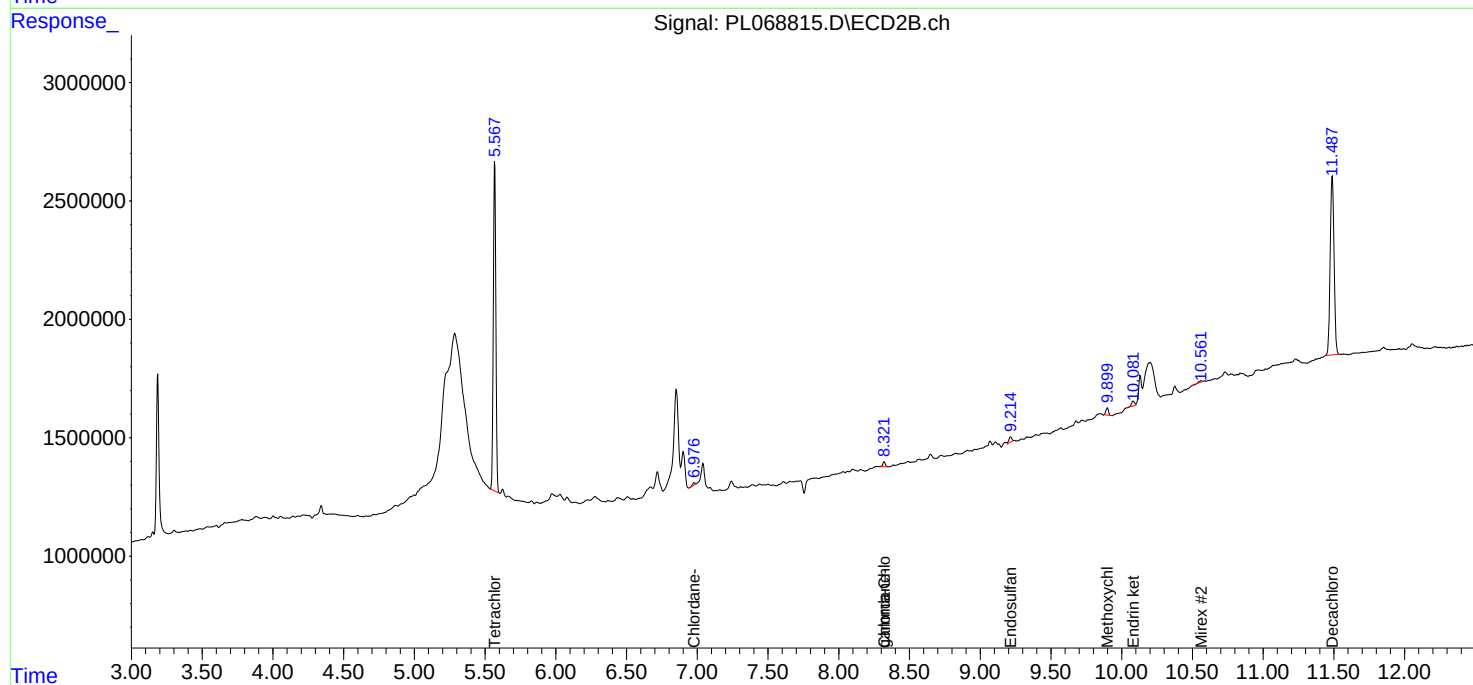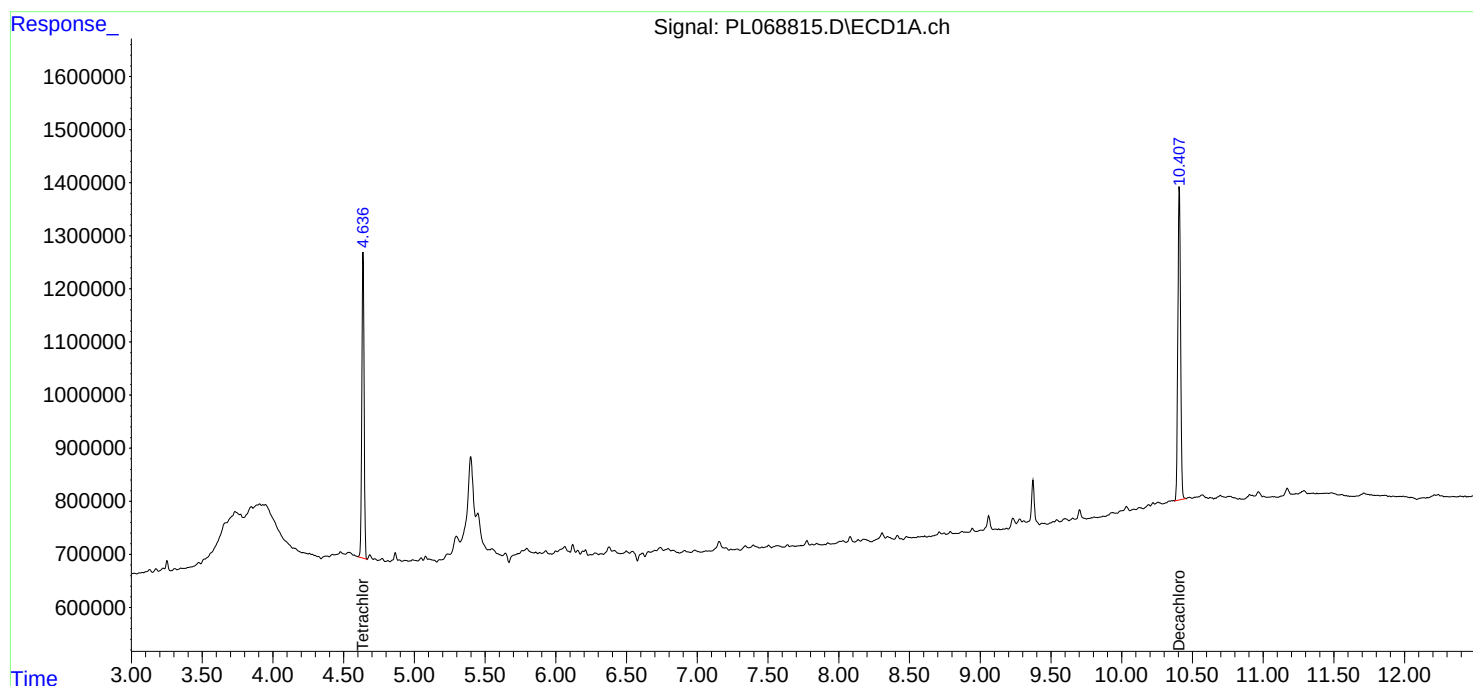


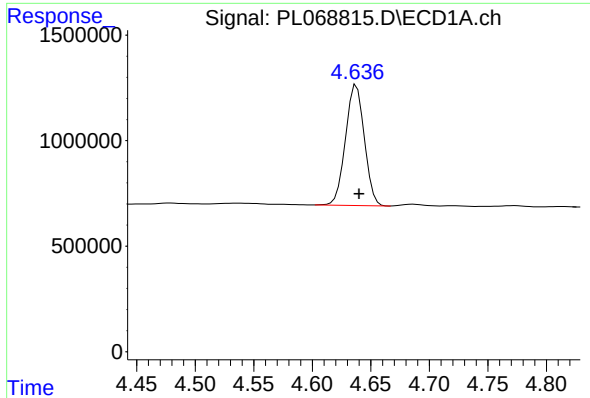

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 6409802
Conc: 15.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

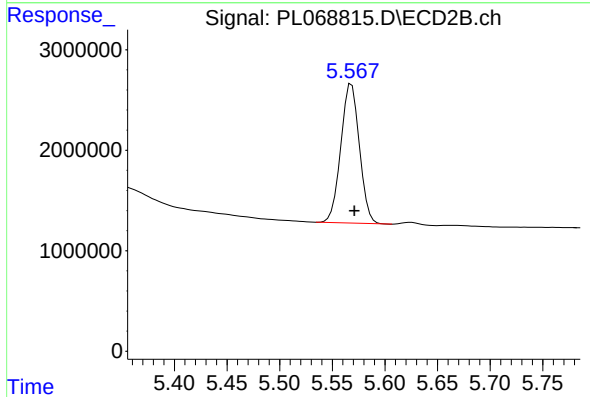


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 17076845
Conc: 16.82 ng/ml

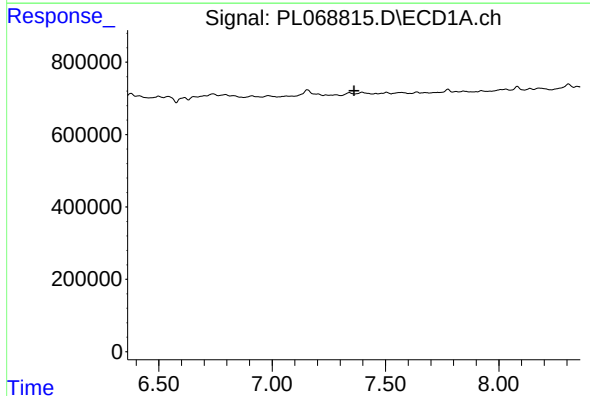


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

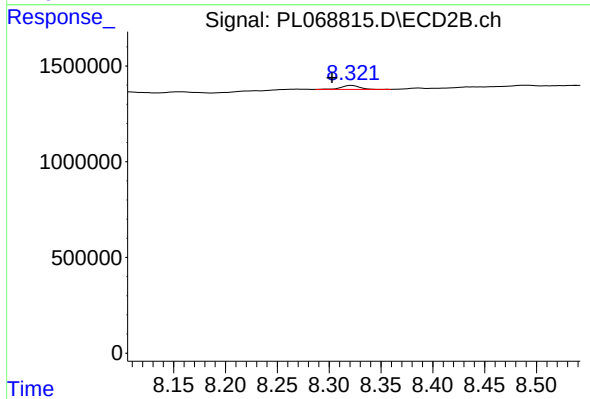

#10 gamma-Chlordane


R.T.: 8.322 min
Delta R.T.: 0.019 min
Response: 266686
Conc: 0.23 ng/ml

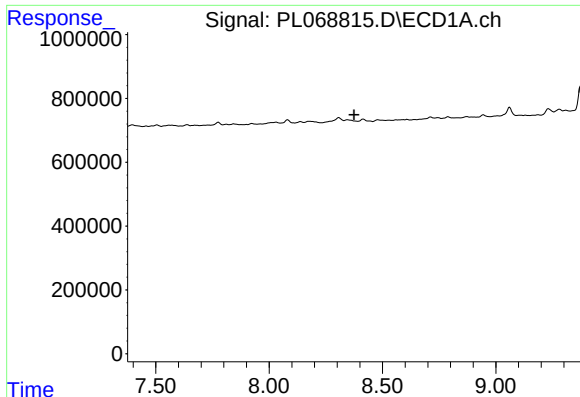

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

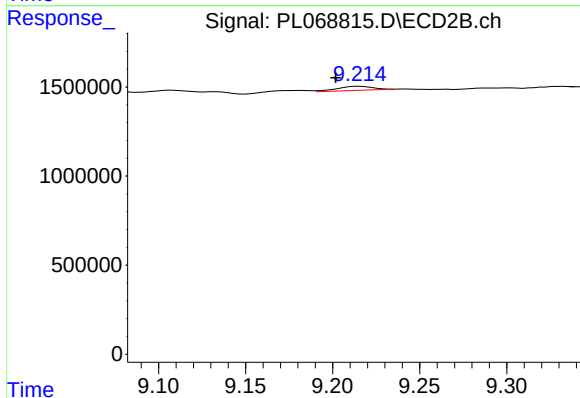


#15 Endosulfan II

R.T.: 9.215 min
Delta R.T.: 0.014 min
Response: 319527
Conc: 0.35 ng/ml

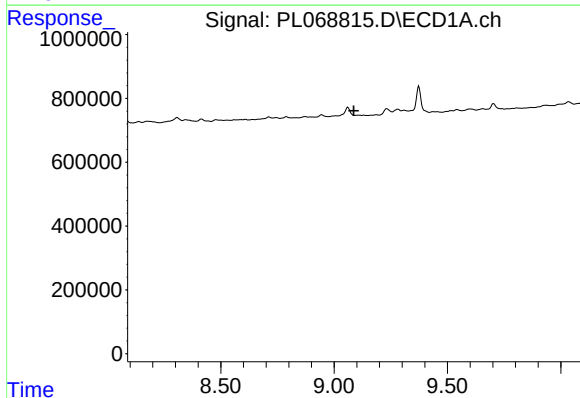


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

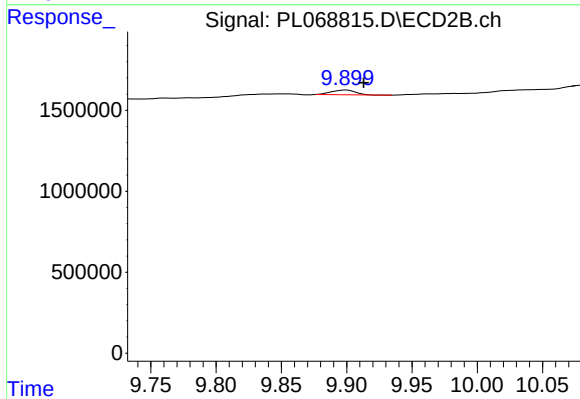

#20 Methoxychlor


R.T.: 9.900 min
Delta R.T.: -0.013 min
Response: 386579
Conc: 0.74 ng/ml

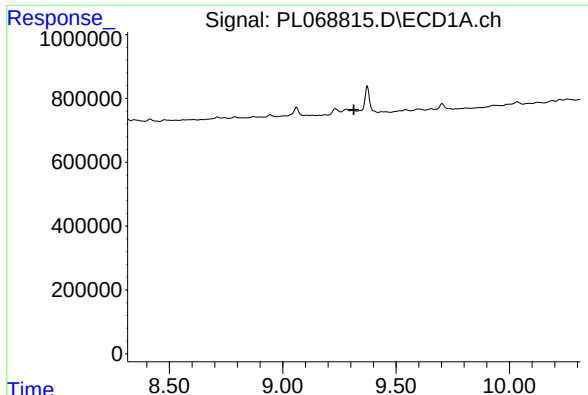

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

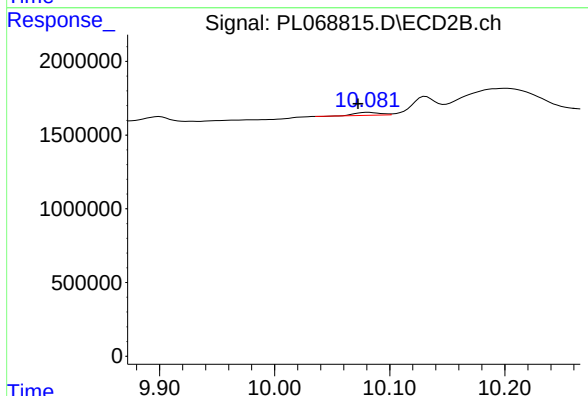


#21 Endrin ketone

R.T.: 10.082 min
Delta R.T.: 0.009 min
Response: 302138
Conc: 0.30 ng/ml

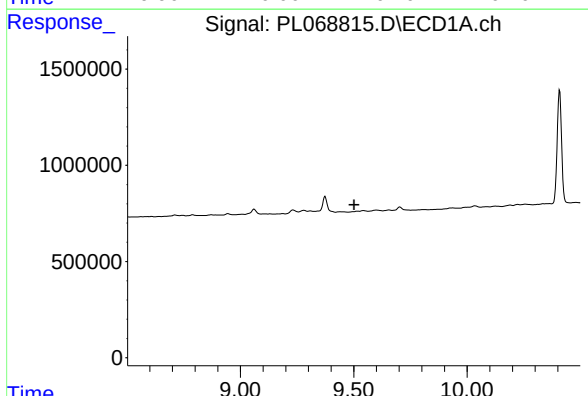


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

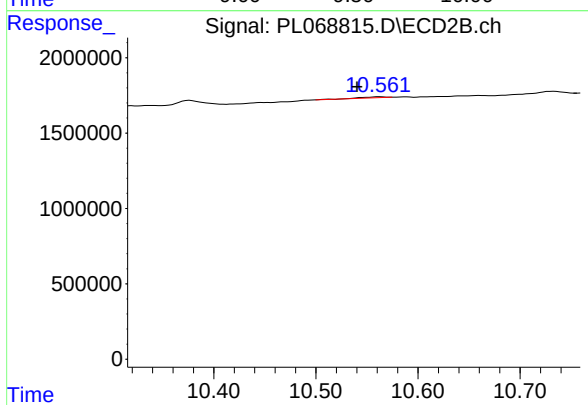

#22 Mirex


R.T.: 10.563 min
Delta R.T.: 0.022 min
Response: 102239
Conc: 0.13 ng/ml

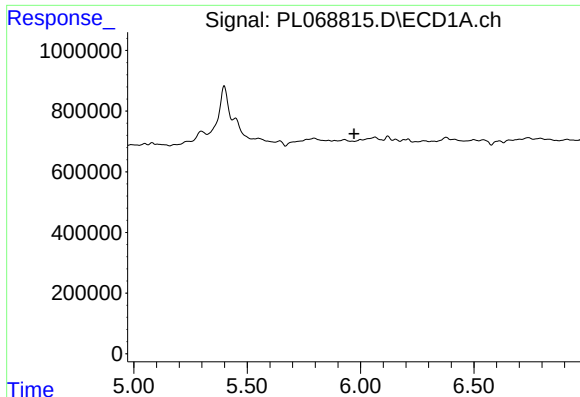

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

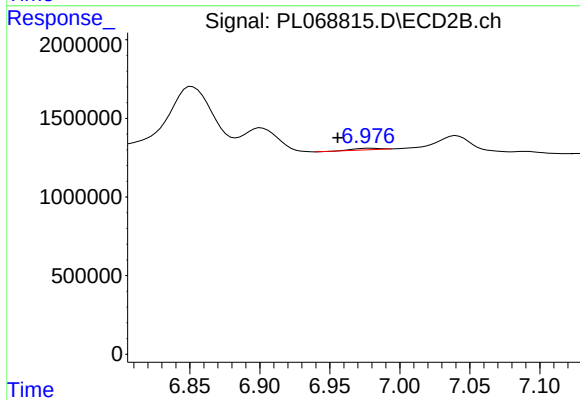


#23 Chlordane-1

R.T.: 6.978 min
Delta R.T.: 0.023 min
Response: 114415
Conc: 2.71 ng/ml

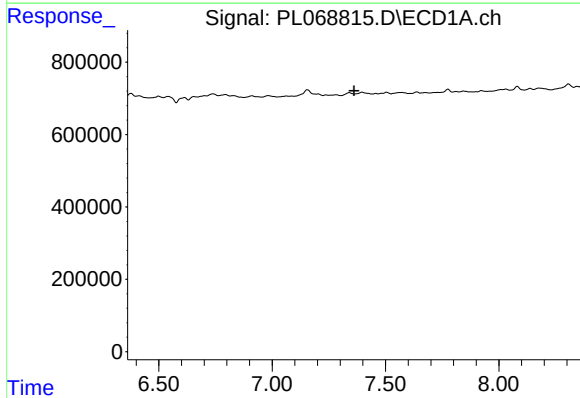


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

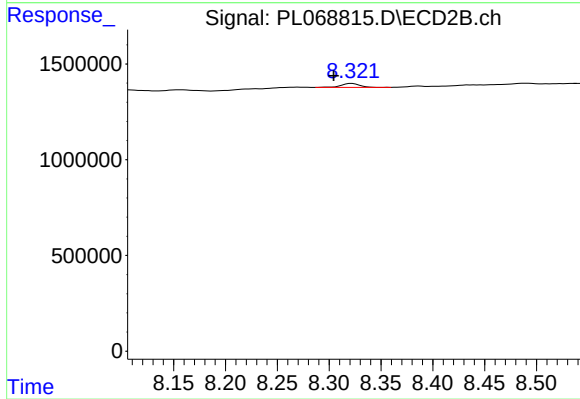

#25 Chlordane-3


R.T.: 8.322 min
Delta R.T.: 0.017 min
Response: 266686
Conc: 1.63 ng/ml

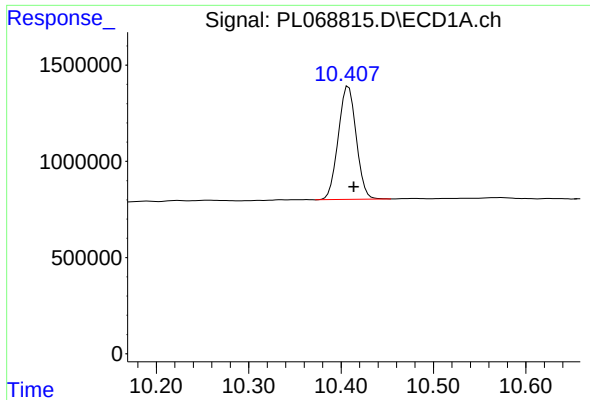

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.006 min
Response: 7946224
Conc: 13.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210560-COM-33

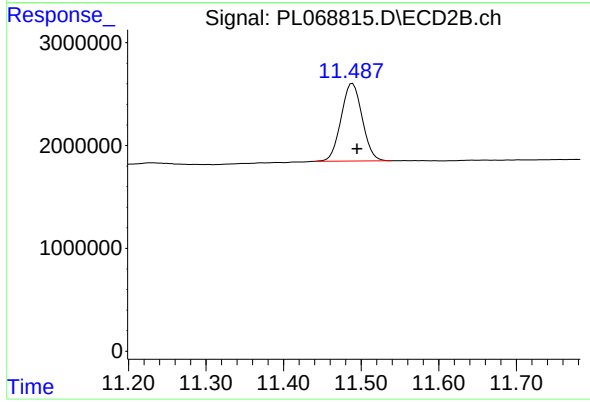

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.006 min
Response: 14249435
Conc: 14.69 ng/ml