

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 22:23
 Operator : AR\AJ
 Sample : M3299-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210562-COM-35

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:56:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.568	5010144	13098441	12.112	12.901
28)	SA Decachlor...	10.408	11.488	6038356	10570985	10.507	10.895
Target Compounds							
8)	B Heptachlo...	0.000	8.030	0	170337	N.D.	0.147 #
12)	B 4,4'-DDE	0.000	8.567	0	140614	N.D.	0.133 #
15)	B Endosulfa...	0.000	9.216	0	507902	N.D.	0.554 #
20)	A Methoxychlor	0.000	9.896f	0	196410	N.D.	0.377 #
21)	B Endrin ke...	0.000	10.088f	0	117145	N.D.	0.115 #
22)	Mirex	0.000	10.566f	0	185056	N.D.	0.234 #
23)	Chlordane-1	0.000	6.981f	0	213590	N.D.	5.065 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 22:23
Operator : AR\AJ
Sample : M3299-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:56:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

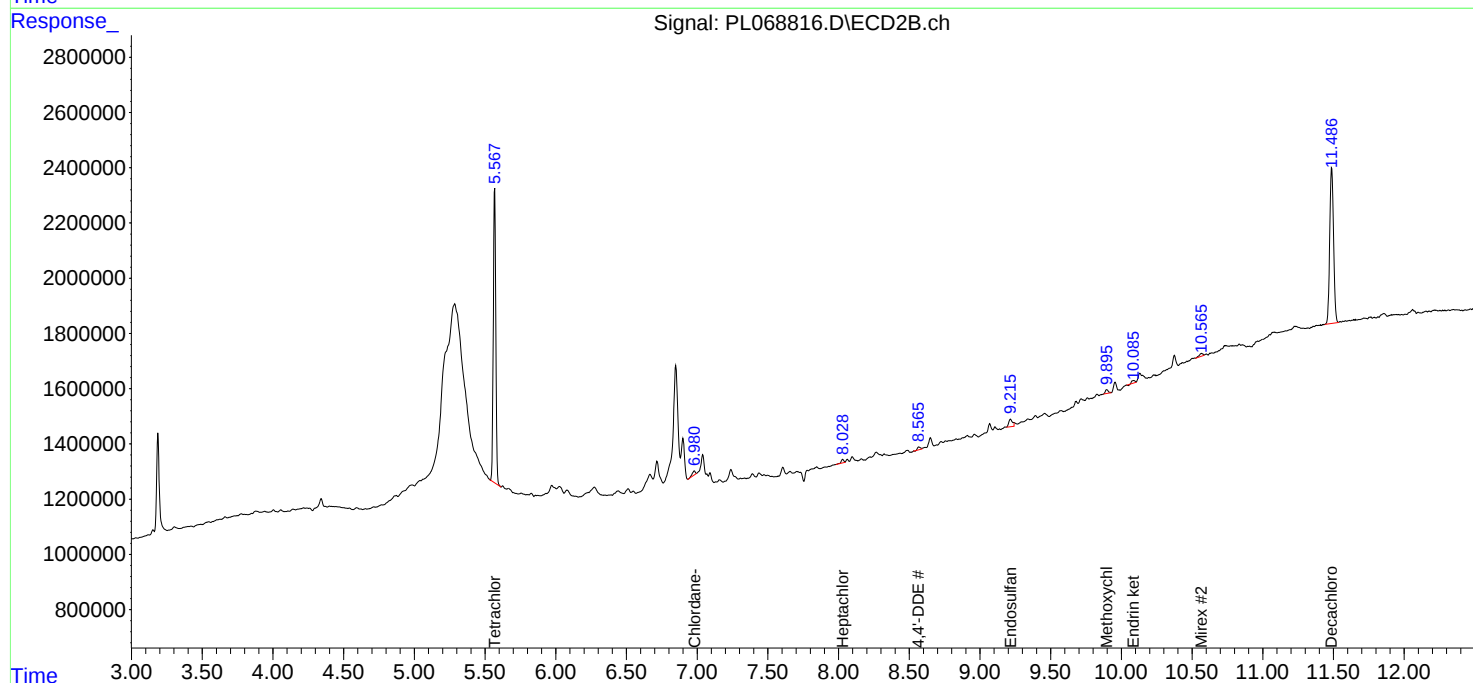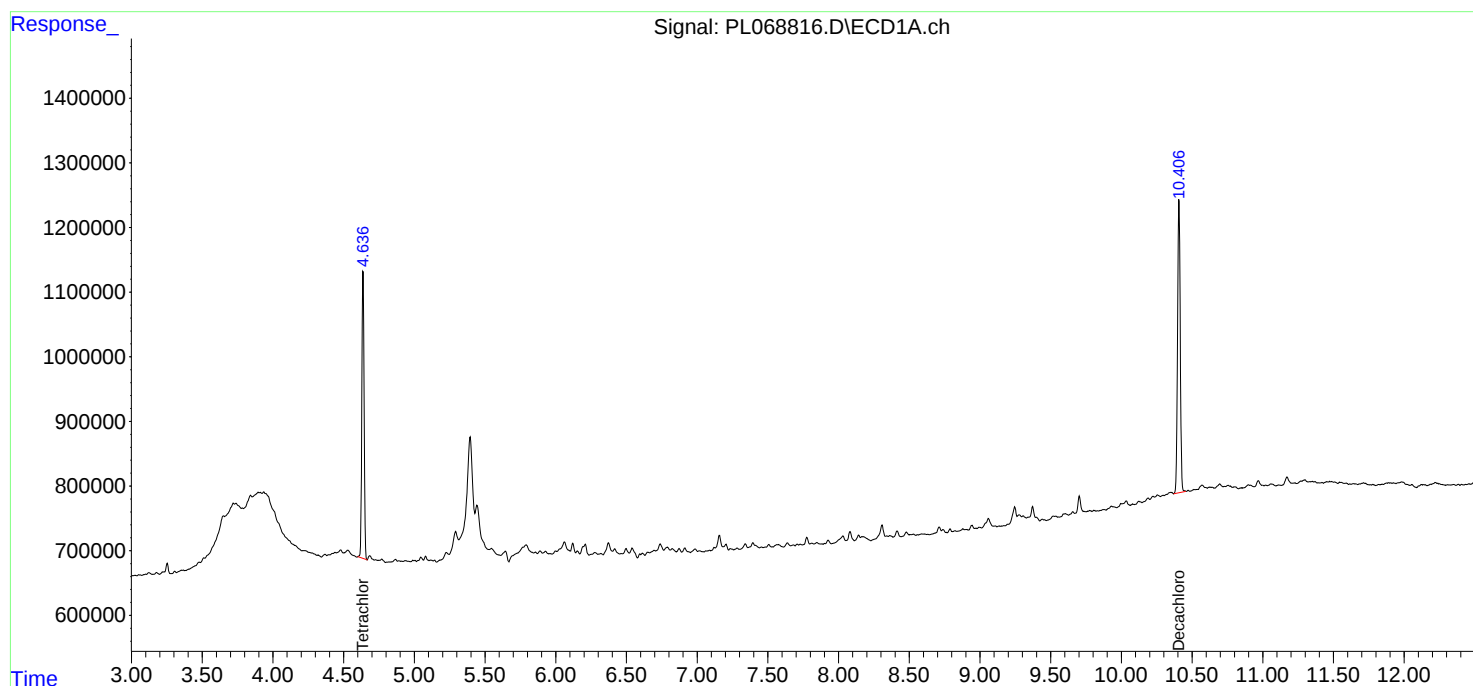


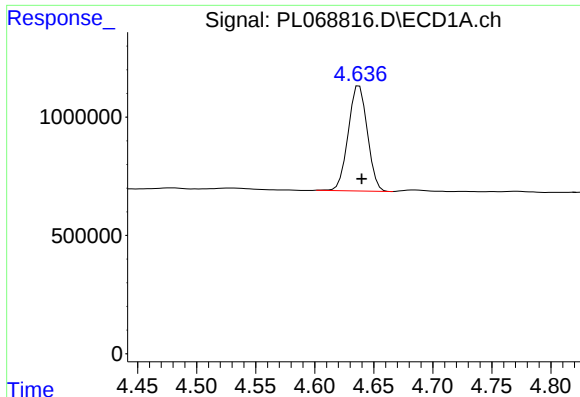

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 5010144
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

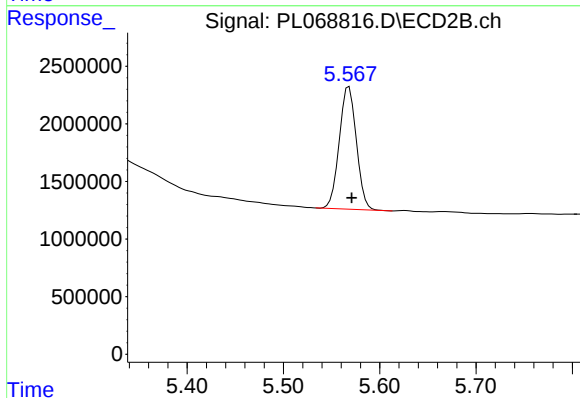


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 13098441
Conc: 12.90 ng/ml

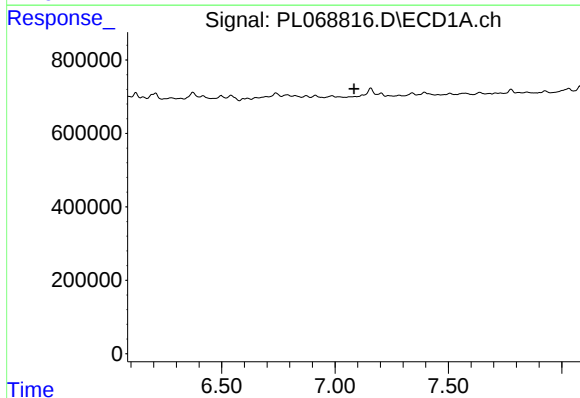


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

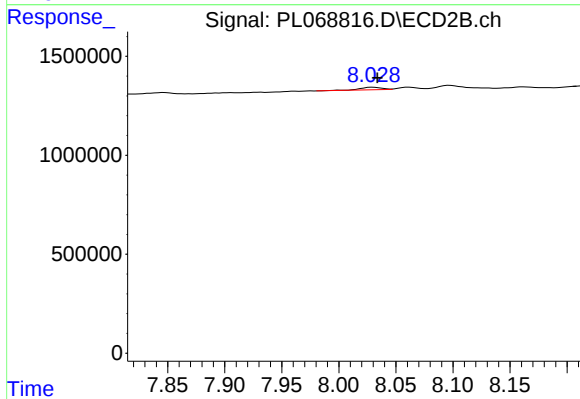

#8 Heptachlor epoxide


R.T.: 8.030 min
Delta R.T.: -0.004 min
Response: 170337
Conc: 0.15 ng/ml

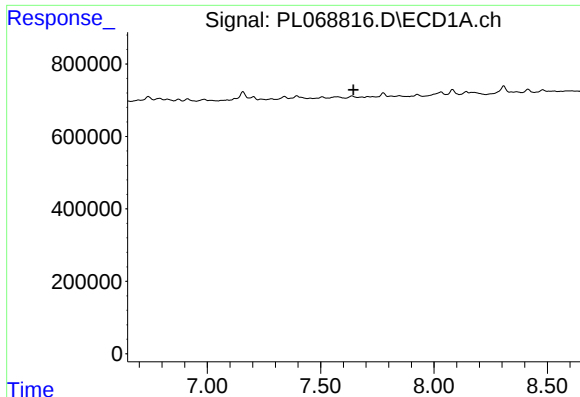

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

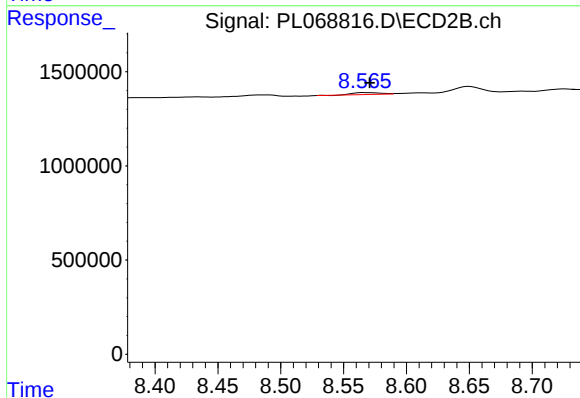


#12 4,4'-DDE

R.T.: 8.567 min
Delta R.T.: -0.004 min
Response: 140614
Conc: 0.13 ng/ml

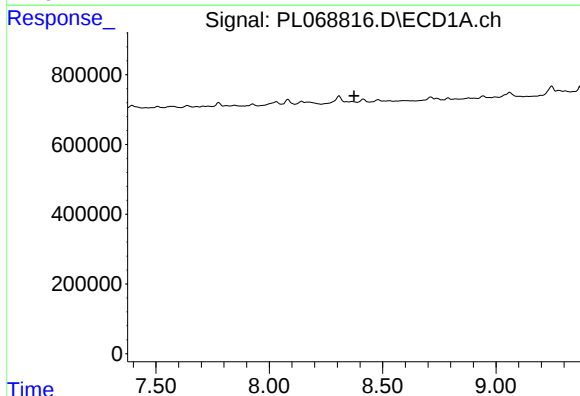


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

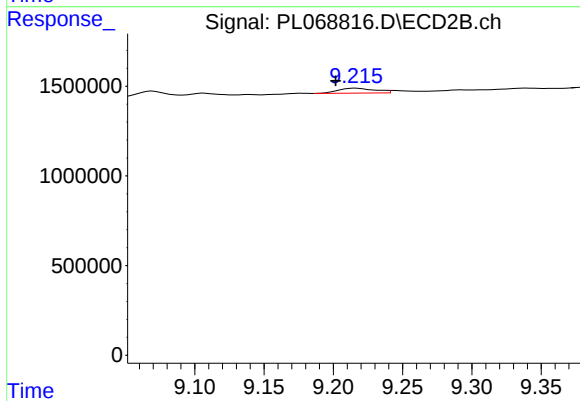

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 507902
Conc: 0.55 ng/ml

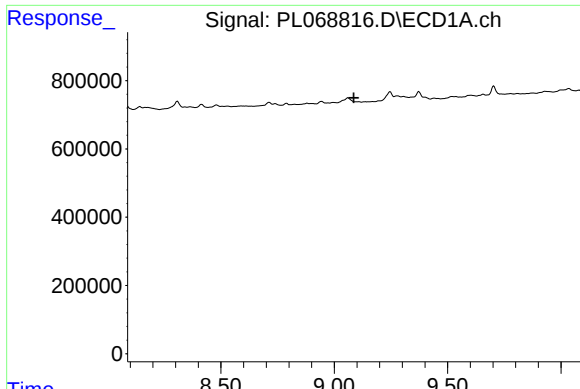

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

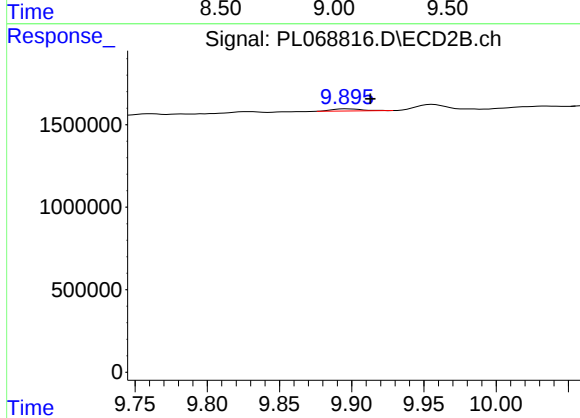


#20 Methoxychlor

R.T.: 9.896 min
Delta R.T.: -0.017 min
Response: 196410
Conc: 0.38 ng/ml

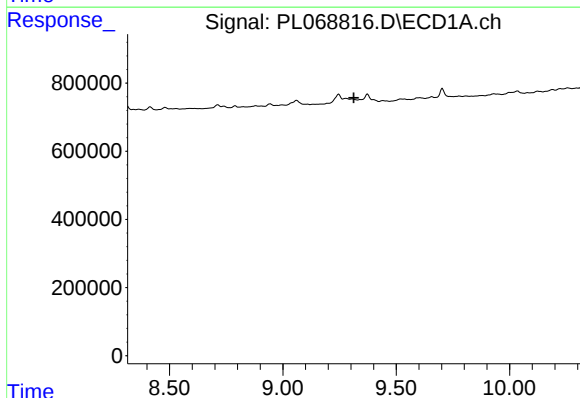


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

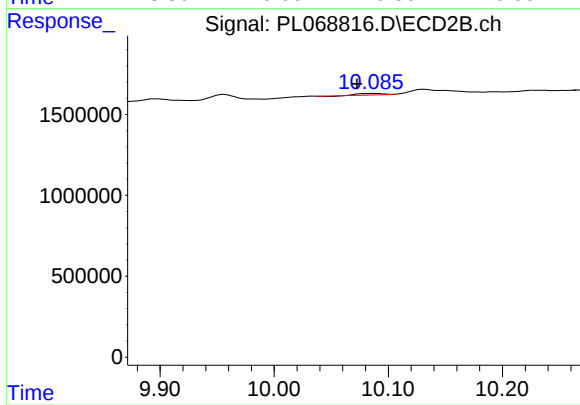

#21 Endrin ketone


R.T.: 10.088 min
Delta R.T.: 0.015 min
Response: 117145
Conc: 0.12 ng/ml

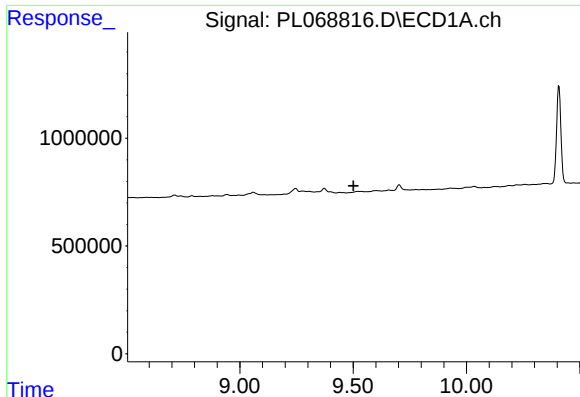

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

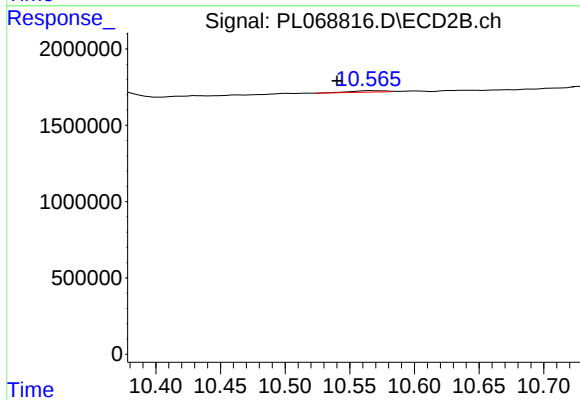


#22 Mirex

R.T.: 10.566 min
Delta R.T.: 0.026 min
Response: 185056
Conc: 0.23 ng/ml

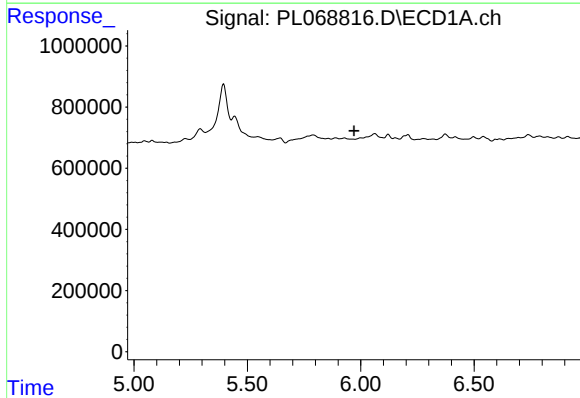


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

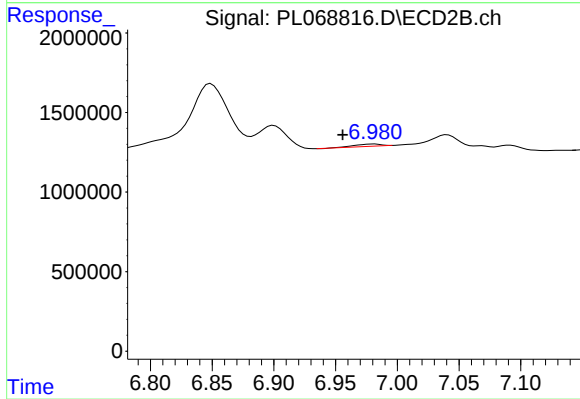

#23 Chlordane-1


R.T.: 6.981 min
Delta R.T.: 0.025 min
Response: 213590
Conc: 5.07 ng/ml

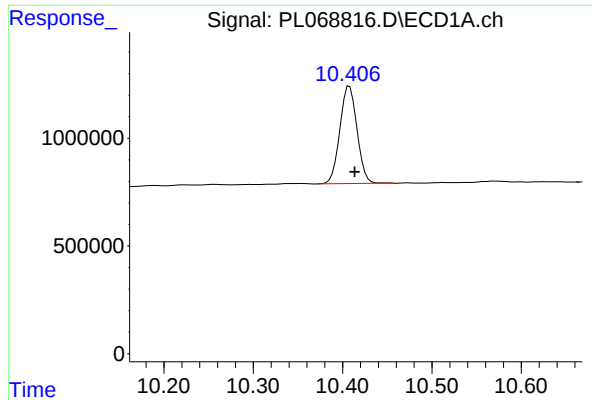

#28 Decachlorobiphenyl

R.T.: 10.408 min
Delta R.T.: -0.006 min
Response: 6038356
Conc: 10.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210562-COM-35

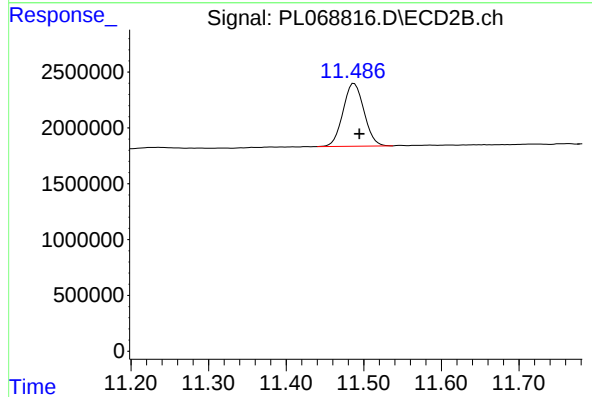

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 10570985
Conc: 10.90 ng/ml