

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
 Data File : PL068817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 22:40
 Operator : AR\AJ
 Sample : M3305-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SA-01-080521

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:56:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	3938866	10173723	9.522	10.020
28)	SA Decachlor...	10.407	11.487	6030435	10809946	10.493	11.141
Target Compounds							
8)	B Heptachlo...	0.000	8.037	0	125761	N.D.	0.109 #
11)	B alpha-Chl...	0.000	8.383	0	173998	N.D.	0.152 #
13)	MA Dieldrin	0.000	8.728	0	109488	N.D.	0.101 #
15)	B Endosulfa...	0.000	9.218f	0	795352	N.D.	0.867 #
21)	B Endrin ke...	0.000	10.089f	0	223091	N.D.	0.219 #
22)	Mirex	0.000	10.570f	0	171833	N.D.	0.217 #
23)	Chlordane-1	0.000	6.981f	0	114905	N.D.	2.725 #
26)	Chlordane-4	0.000	8.383	0	173998	N.D.	0.877 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080621\
Data File : PL068817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 22:40
Operator : AR\AJ
Sample : M3305-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:56:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

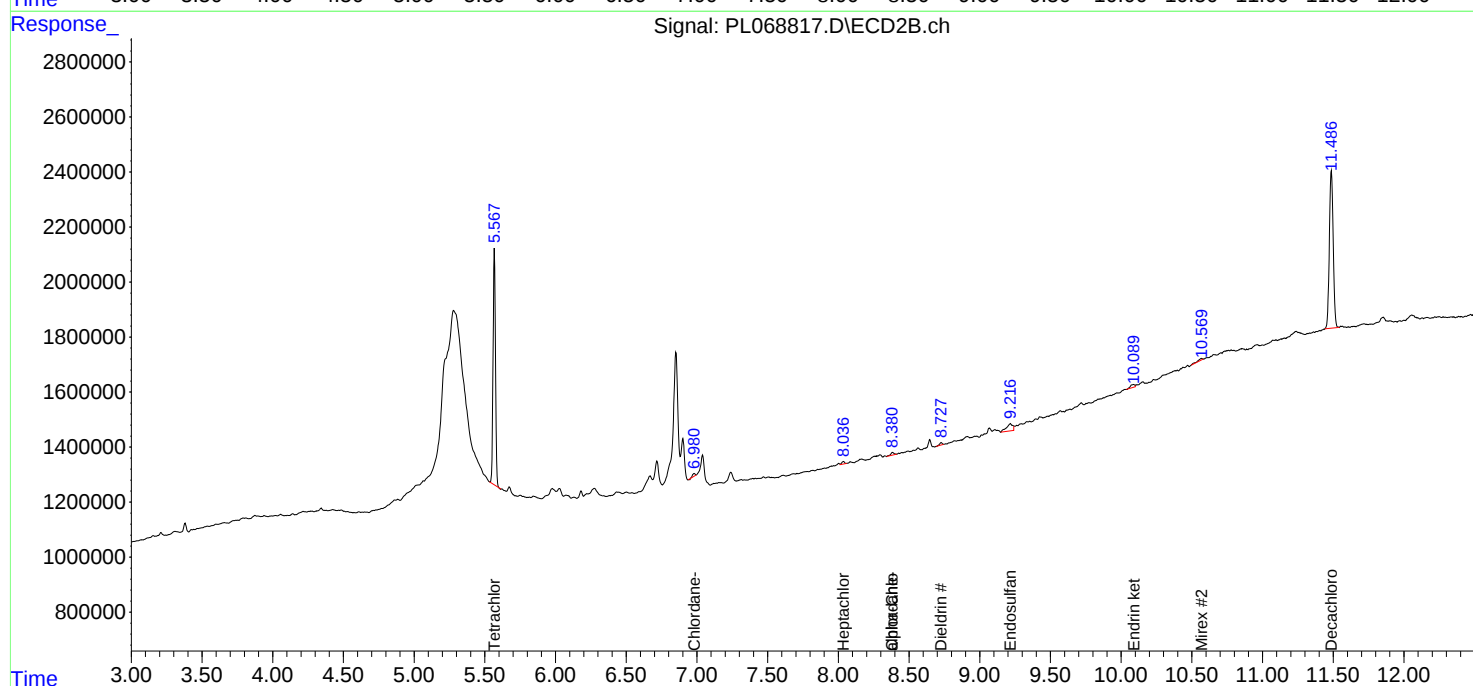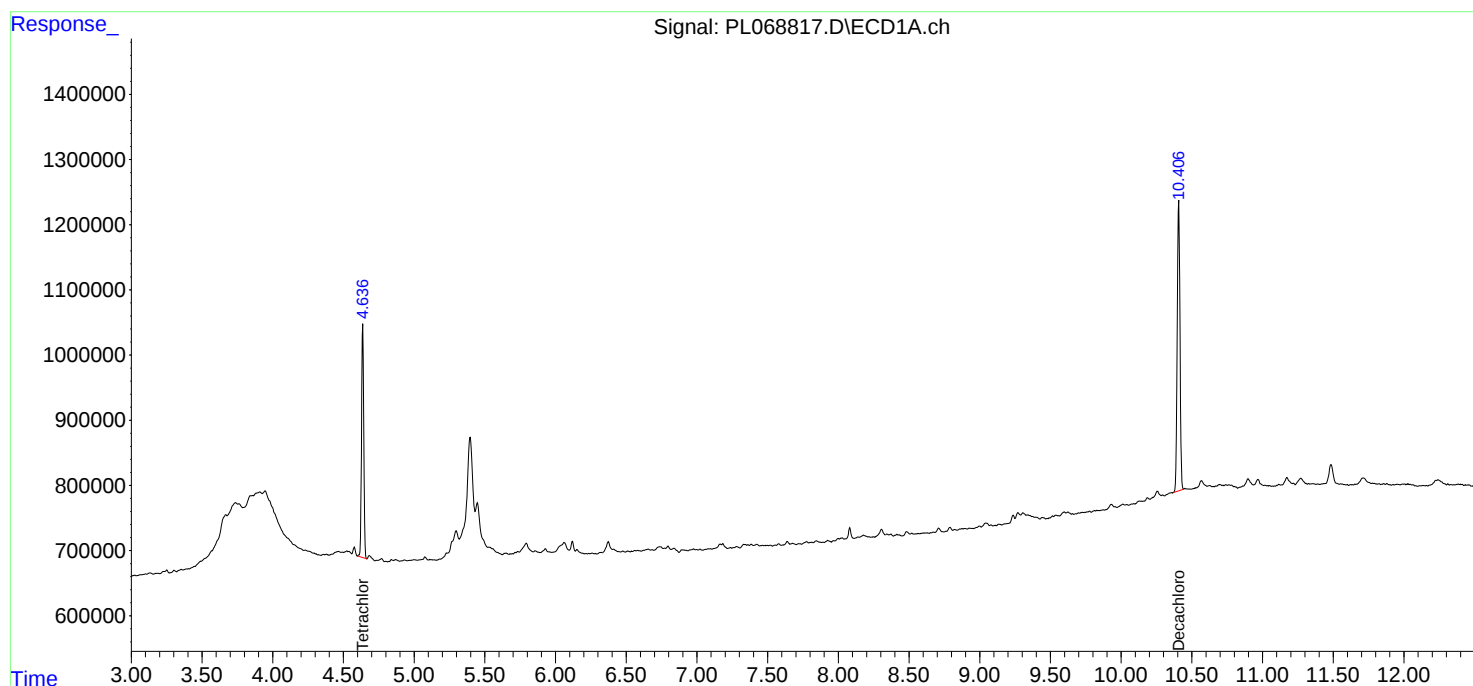


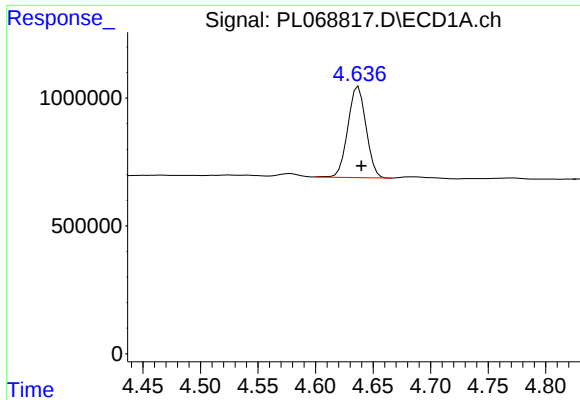

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 3938866
Conc: 9.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

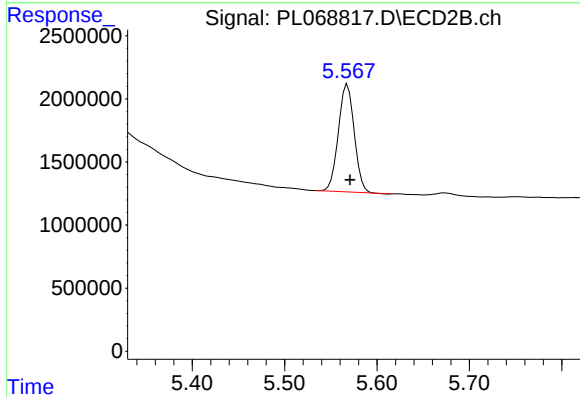


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 10173723
Conc: 10.02 ng/ml

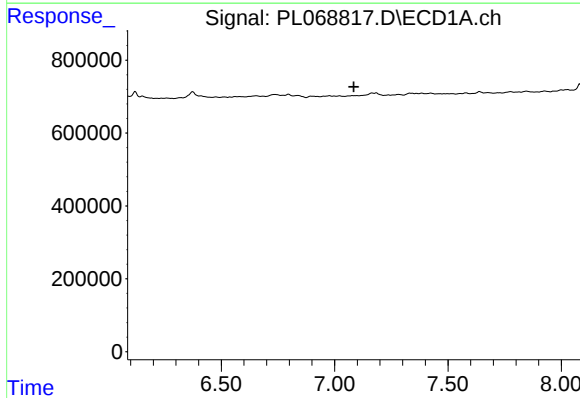


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

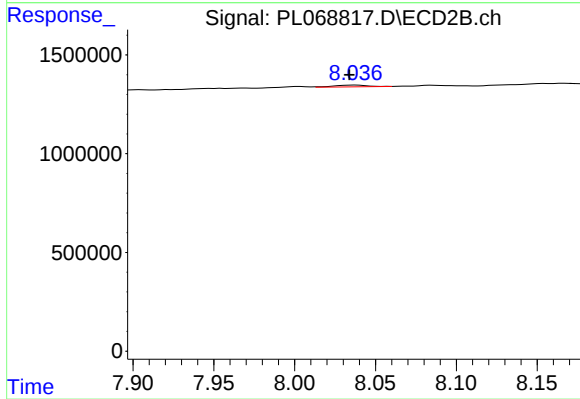

#8 Heptachlor epoxide


R.T.: 8.037 min
Delta R.T.: 0.003 min
Response: 125761
Conc: 0.11 ng/ml

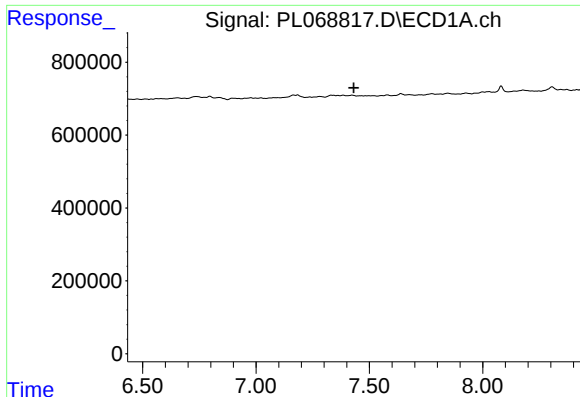

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

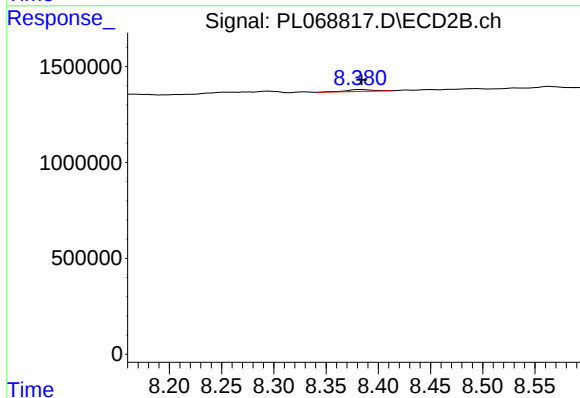


#11 alpha-Chlordane

R.T.: 8.383 min
Delta R.T.: -0.001 min
Response: 173998
Conc: 0.15 ng/ml

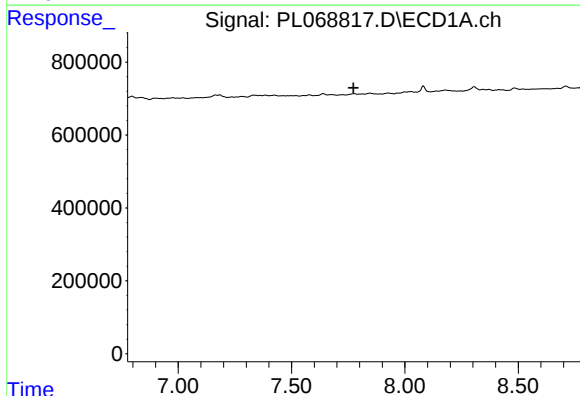


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

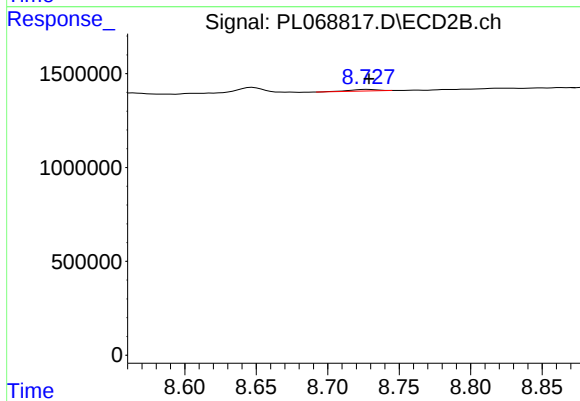

#13 Dieldrin


R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 109488
Conc: 0.10 ng/ml

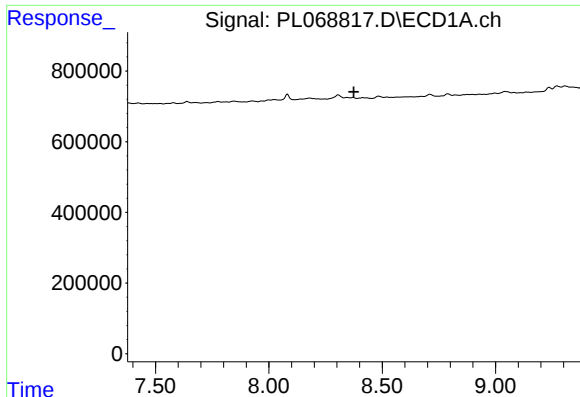

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

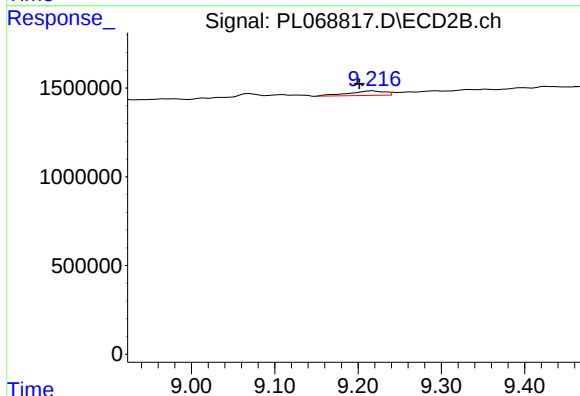


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.016 min
Response: 795352
Conc: 0.87 ng/ml

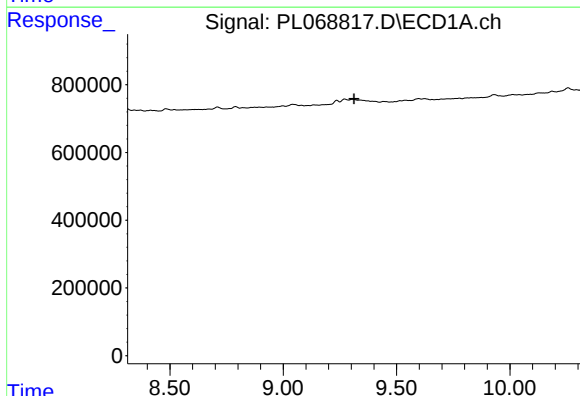


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

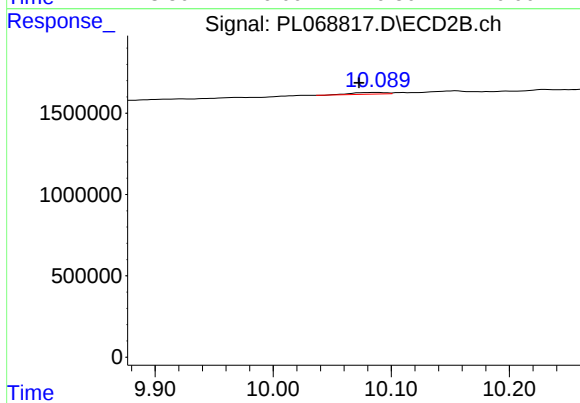

#21 Endrin ketone


R.T.: 10.089 min
Delta R.T.: 0.016 min
Response: 223091
Conc: 0.22 ng/ml

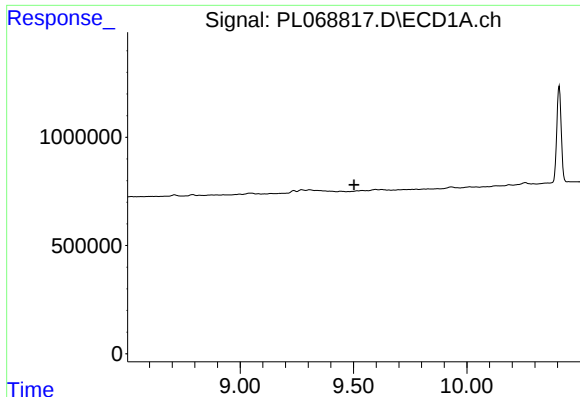

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

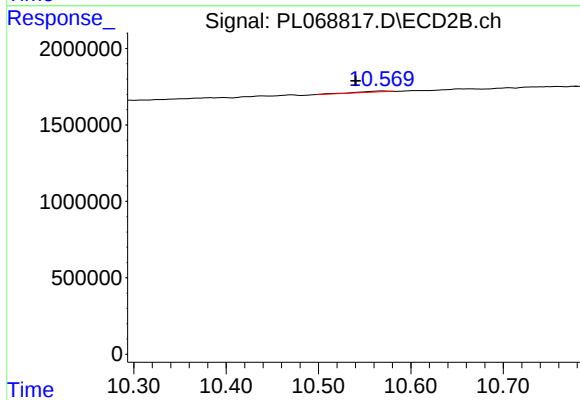


#22 Mirex

R.T.: 10.570 min
Delta R.T.: 0.030 min
Response: 171833
Conc: 0.22 ng/ml

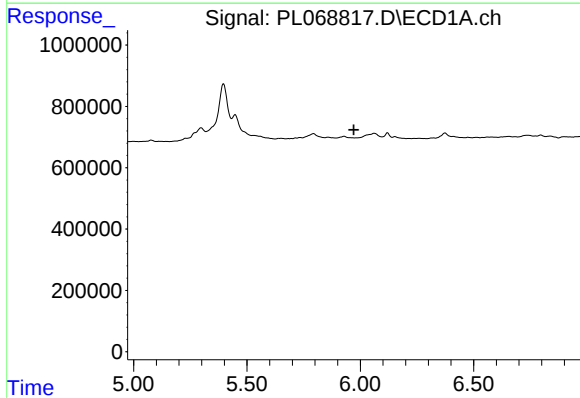


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

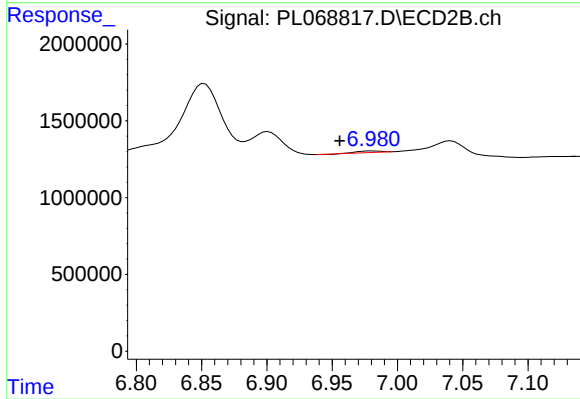

#23 Chlordane-1


R.T.: 6.981 min
Delta R.T.: 0.025 min
Response: 114905
Conc: 2.72 ng/ml

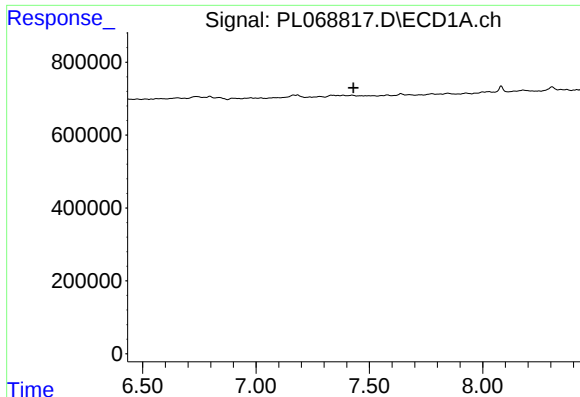

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SA-01-080521

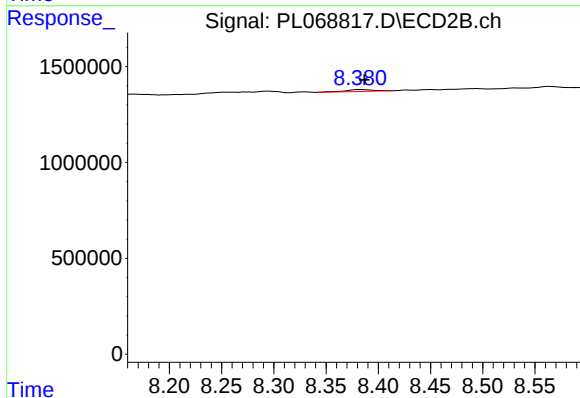


#26 Chlordane-4

R.T.: 8.383 min
Delta R.T.: -0.004 min
Response: 173998
Conc: 0.88 ng/ml

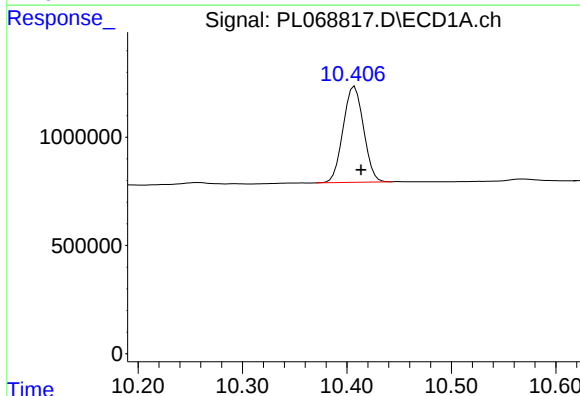

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.006 min
Response: 6030435
Conc: 10.49 ng/ml

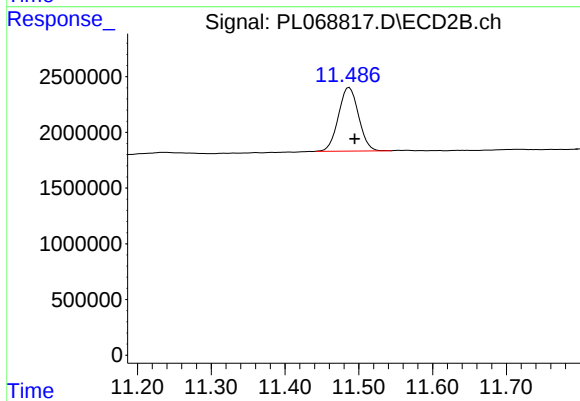

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 10809946
Conc: 11.14 ng/ml