

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080624\
 Data File : PL090833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 19:55
 Operator : AR\AJ
 Sample : P3474-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-A2-COMP

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/07/2024
 Supervised By : Ankita Jodhani 08/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 02:19:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 06 10:55:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.786	38658202	35330099	19.966m	20.436
28) SA Decachlor...	9.053	7.926	26155400	28962733	18.205	17.352

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080624\
Data File : PL090833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 19:55
Operator : AR\AJ
Sample : P3474-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-A2-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/07/2024
Supervised By : Ankita Jodhani 08/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 02:19:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Tue Aug 06 10:55:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

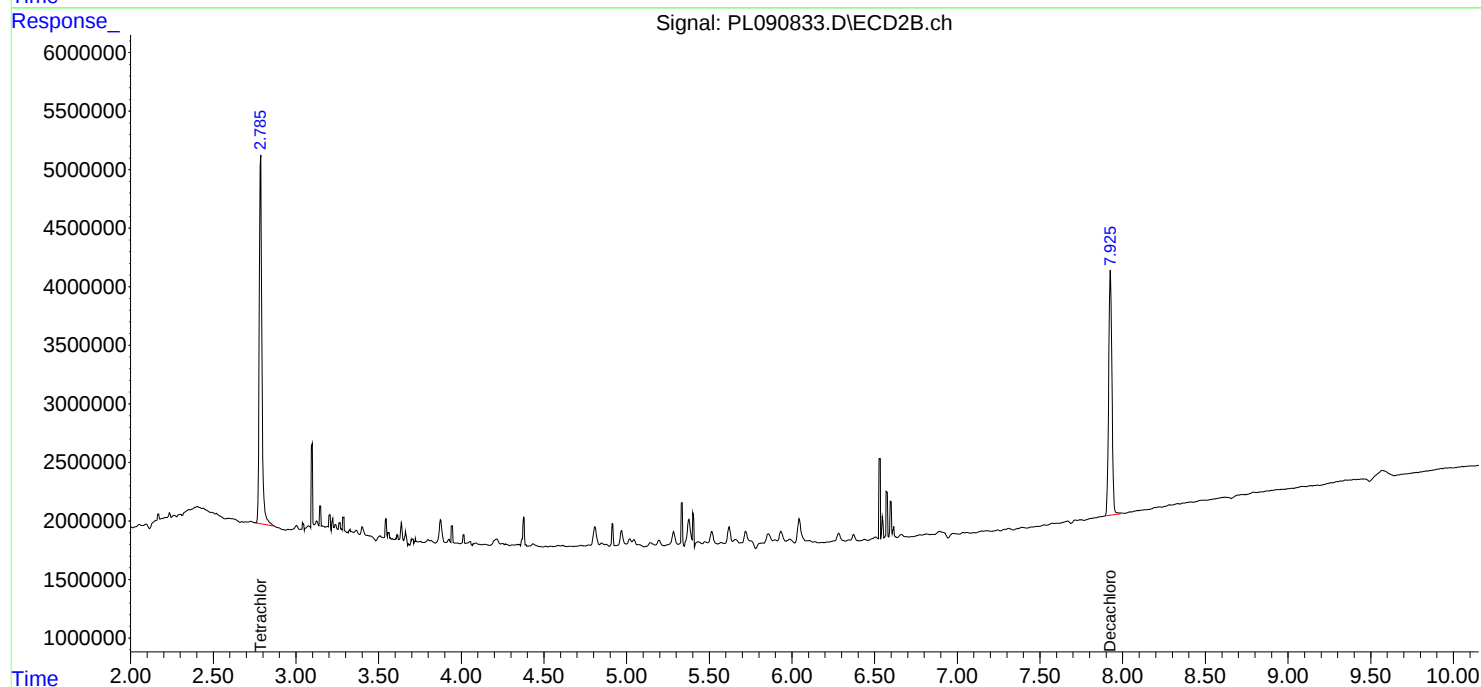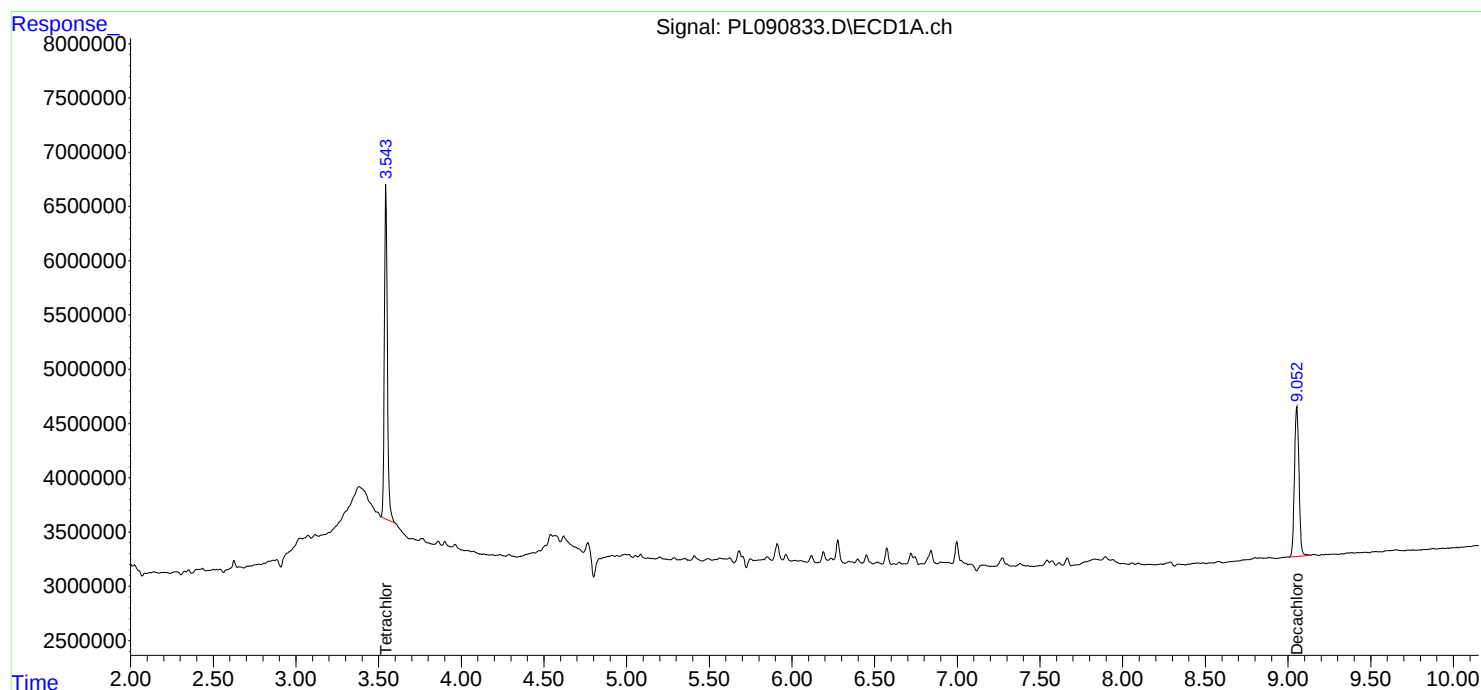

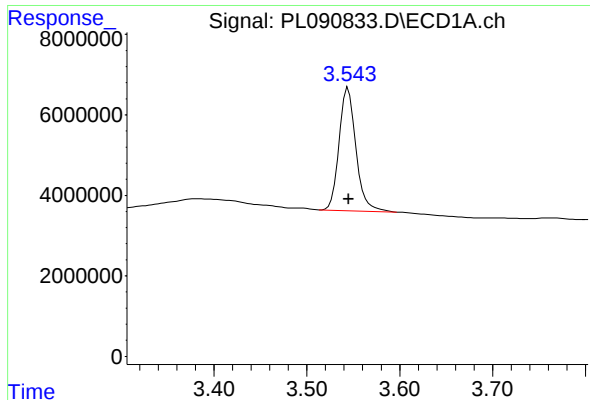


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.002 min
Response: 38658202
Conc: 19.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-A2-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/07/2024
Supervised By :Ankita Jodhani 08/07/2024

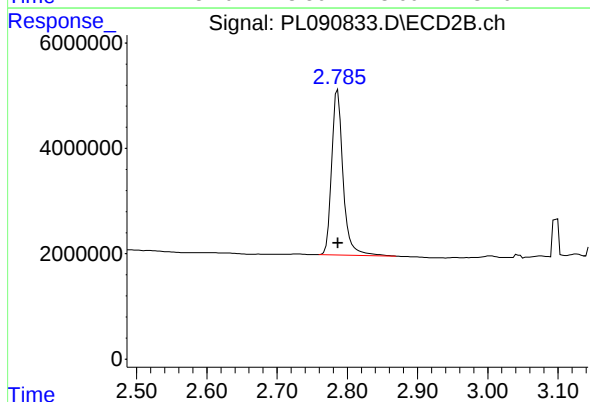


#1 Tetrachloro-m-xylene

R.T.: 2.786 min
Delta R.T.: 0.000 min
Response: 35330099
Conc: 20.44 ng/ml

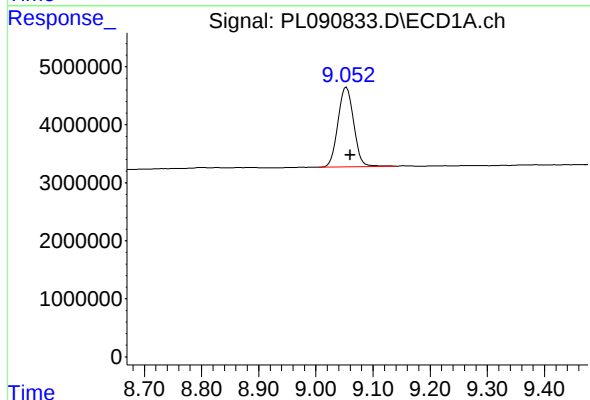

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.007 min
Response: 26155400
Conc: 18.20 ng/ml

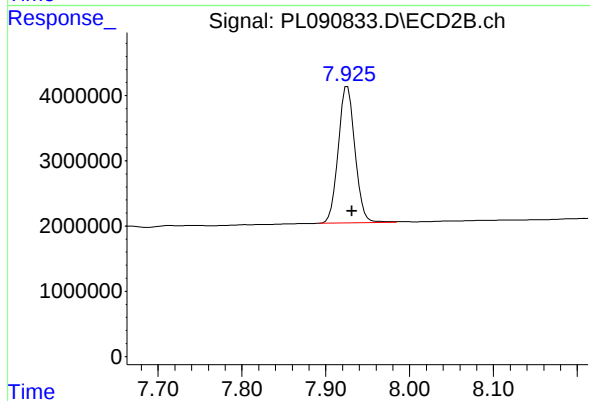

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.005 min
Response: 28962733
Conc: 17.35 ng/ml