

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
 Data File : PL096720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2025 13:22
 Operator : AR\AJ
 Sample : Q2772-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 22:30:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	2.825	57825225	73430539	18.180	15.369
28)	SA Decachlor...	9.010	7.988	50809366	100.4E6	21.307	23.145
Target Compounds							
19)	B Endosulfa...	0.000	6.421f	0	16107701	N.D.	3.167 #
23)	Chlordane-1	0.000	3.849	0	8798309	N.D.	41.969 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
Data File : PL096720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2025 13:22
Operator : AR\AJ
Sample : Q2772-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 22:30:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

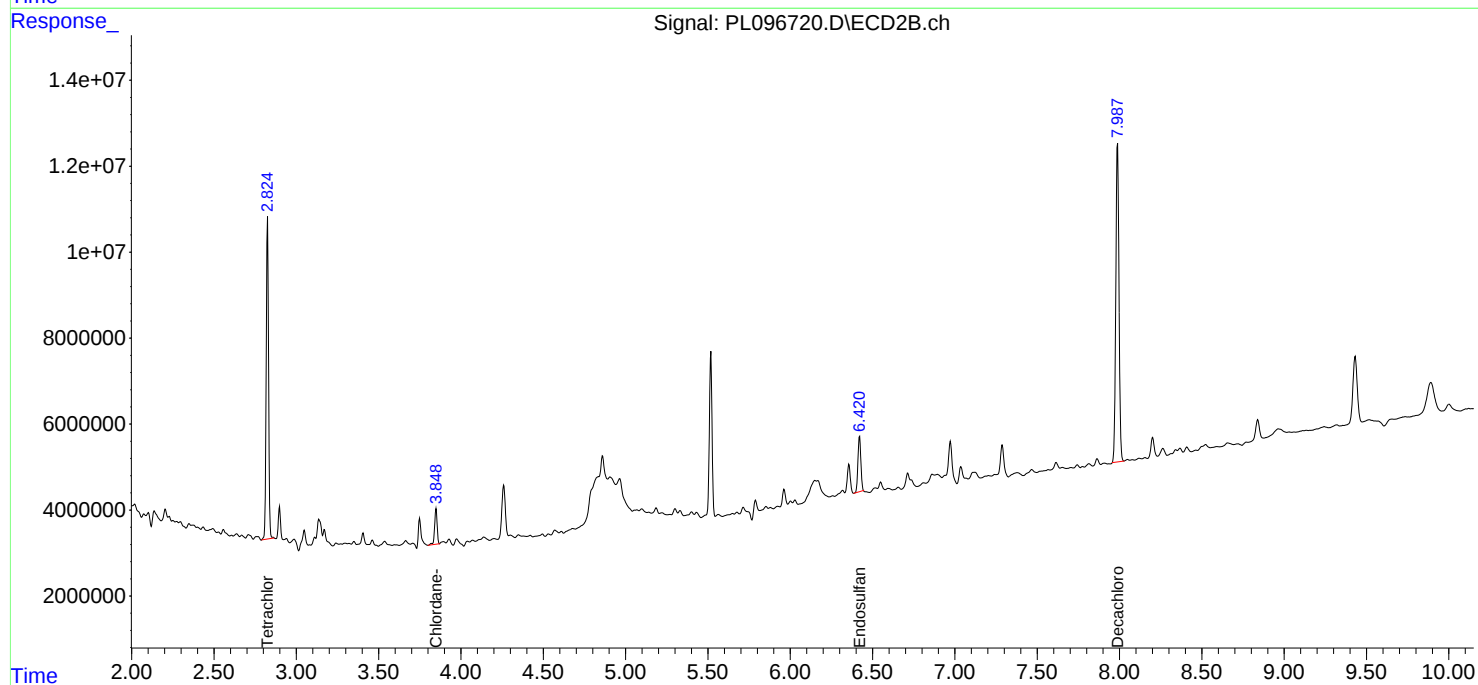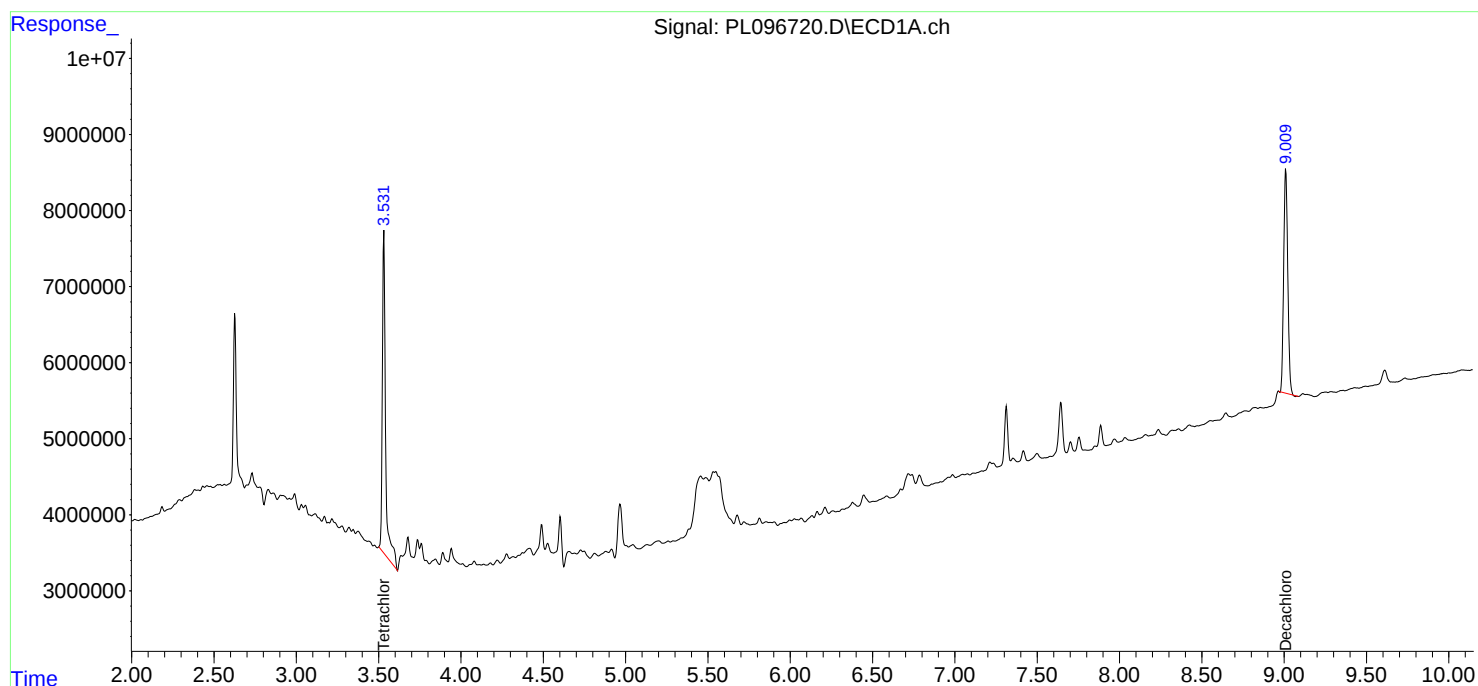


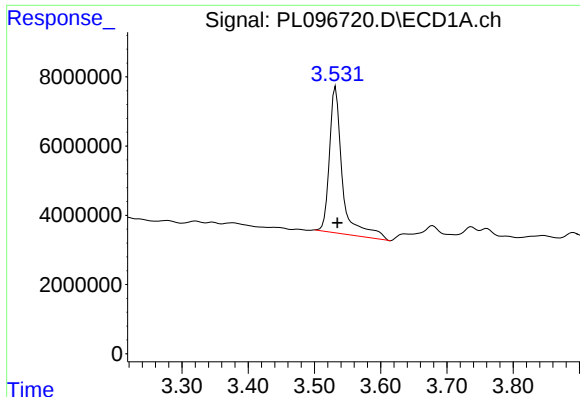

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.003 min
Response: 57825225
Conc: 18.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

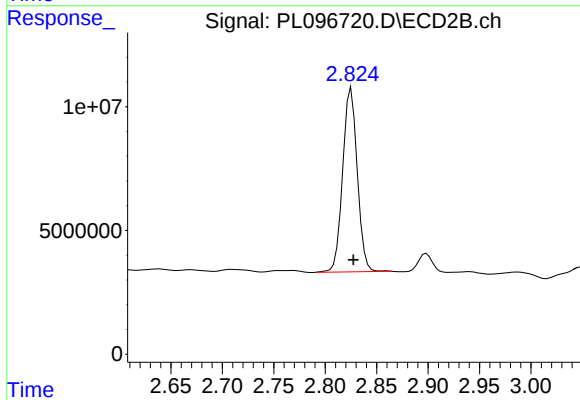


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.002 min
Response: 73430539
Conc: 15.37 ng/ml

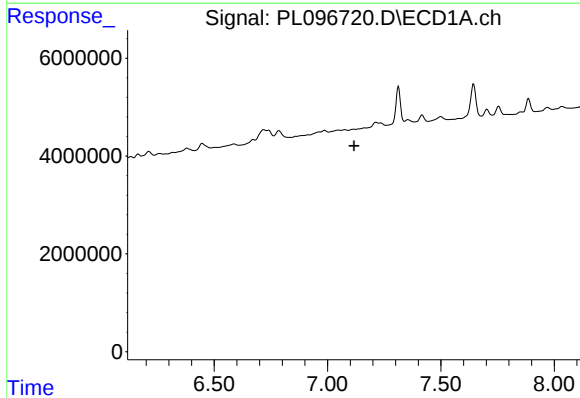


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.118 min
Response: 0
Conc: N.D.

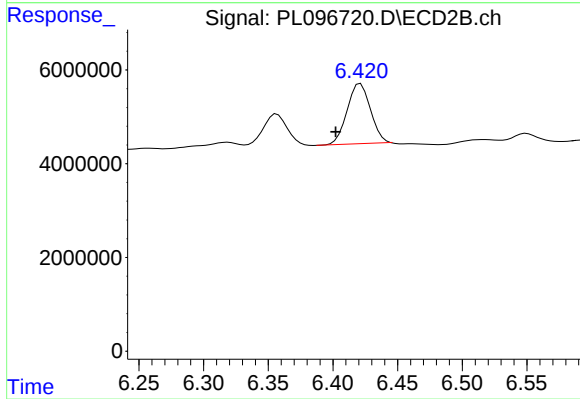

#19 Endosulfan Sulfate


R.T.: 6.421 min
Delta R.T.: 0.019 min
Response: 16107701
Conc: 3.17 ng/ml

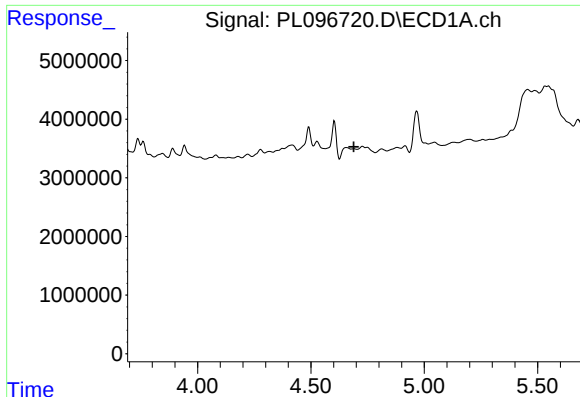

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.689 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

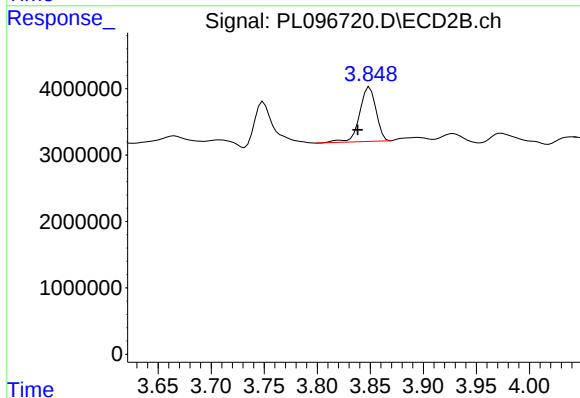


#23 Chlordane-1

R.T.: 3.849 min
Delta R.T.: 0.011 min
Response: 8798309
Conc: 41.97 ng/ml

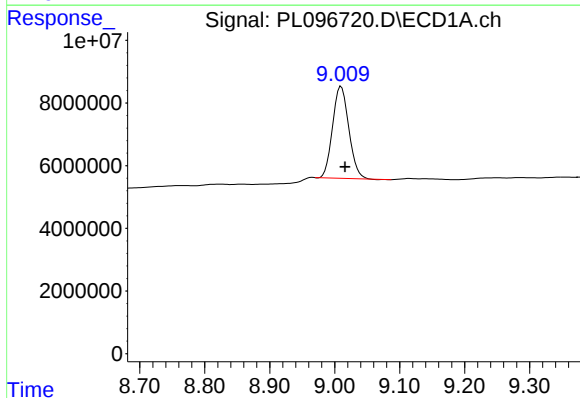

#28 Decachlorobiphenyl

R.T.: 9.010 min
Delta R.T.: -0.006 min
Response: 50809366
Conc: 21.31 ng/ml

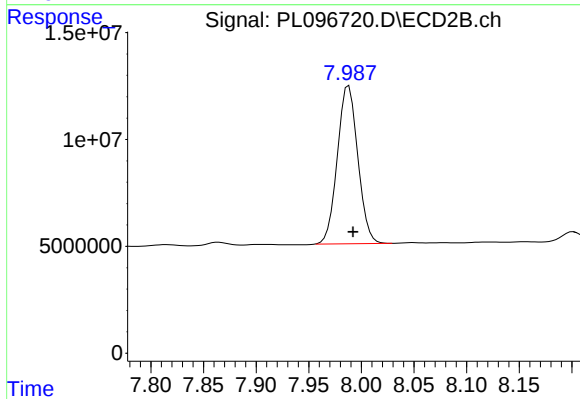

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.004 min
Response: 100408798
Conc: 23.14 ng/ml