

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
 Data File : PL096726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2025 14:43
 Operator : AR\AJ
 Sample : Q2774-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 22:31:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	2.827	32537956	37422095	10.230	7.833
28)	SA Decachlor...	9.007	7.987	36690745	63349017	15.386	14.602
Target Compounds							
10)	B gamma-Chl...	5.914	5.075f	8231594	14441663	2.163	2.456
11)	B alpha-Chl...	6.000	0.000	19357329	0	5.022	N.D. #
12)	B 4,4'-DDE	6.163	5.301	3513754	8080170	1.094	1.465 #
16)	A 4,4'-DDD	6.687	0.000	3852910	0	1.524	N.D. #
17)	MA 4,4'-DDT	6.985	6.104	14153935	23697158	4.936	4.685
25)	Chlordane-3	5.914	5.075f	8231594	14441663	12.324	20.770 #
26)	Chlordane-4	6.000	0.000	19357329	0	23.387	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
Data File : PL096726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2025 14:43
Operator : AR\AJ
Sample : Q2774-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 22:31:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

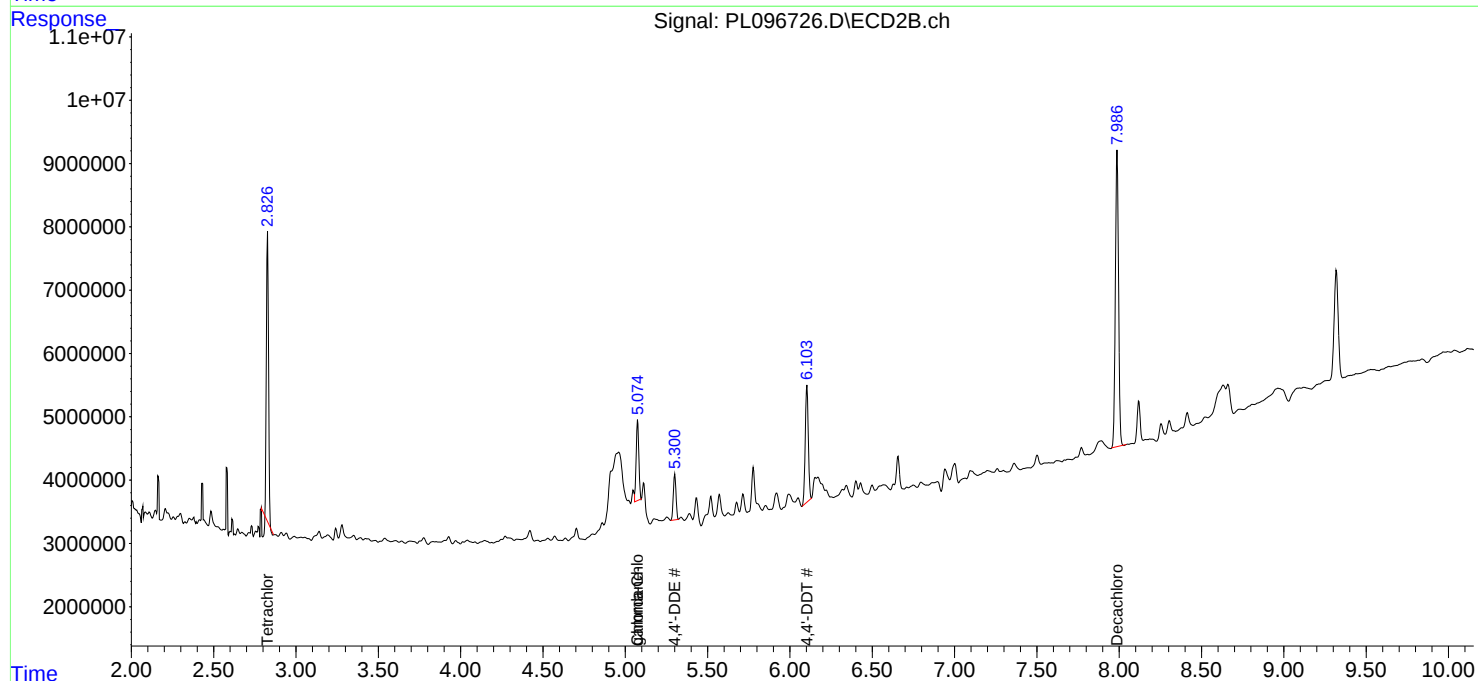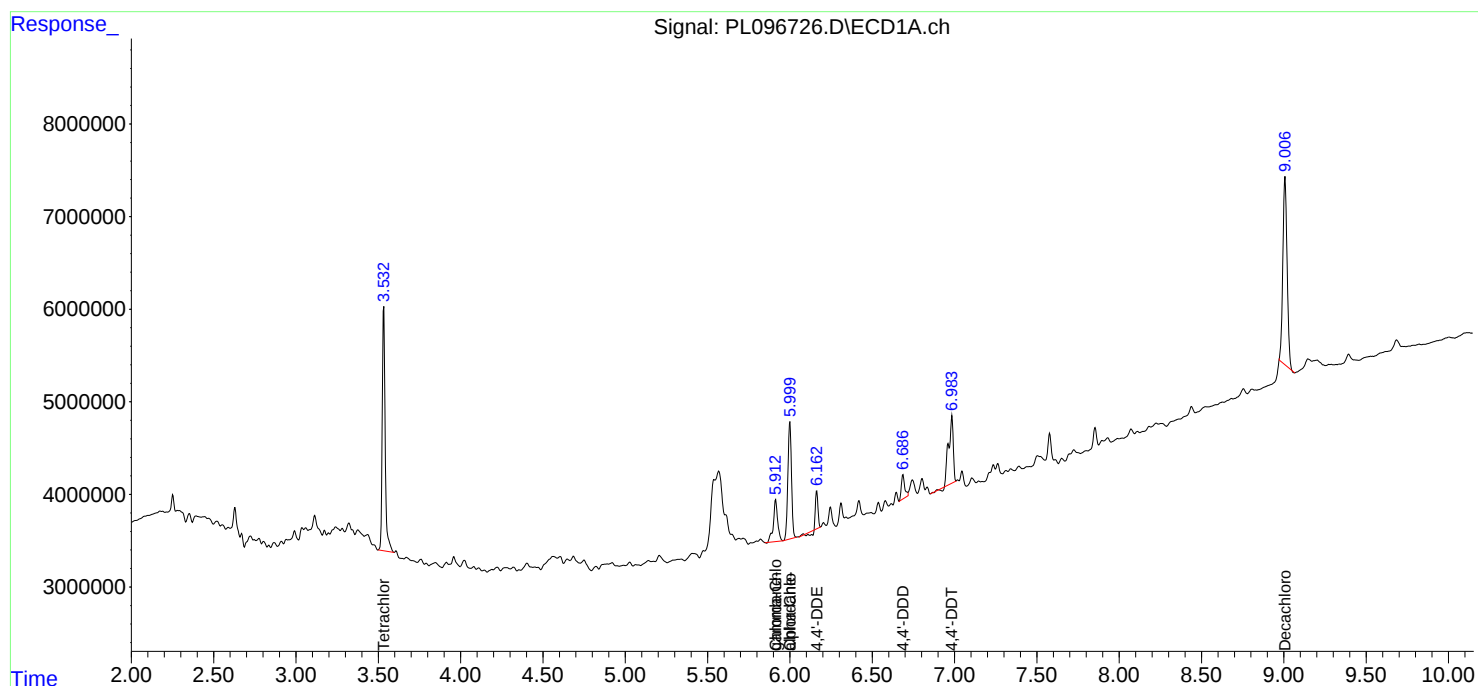


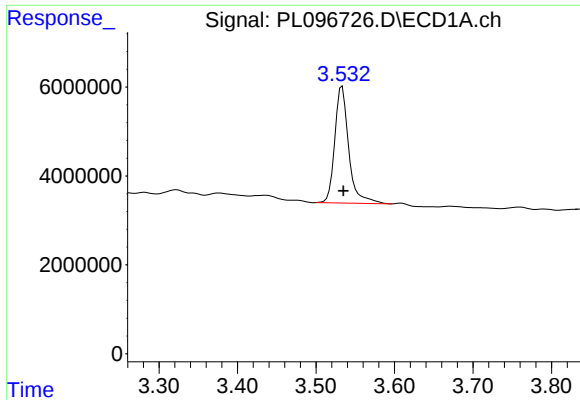

#1 Tetrachloro-m-xylene


R.T.: 3.533 min
Delta R.T.: -0.002 min
Response: 32537956
Conc: 10.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
248

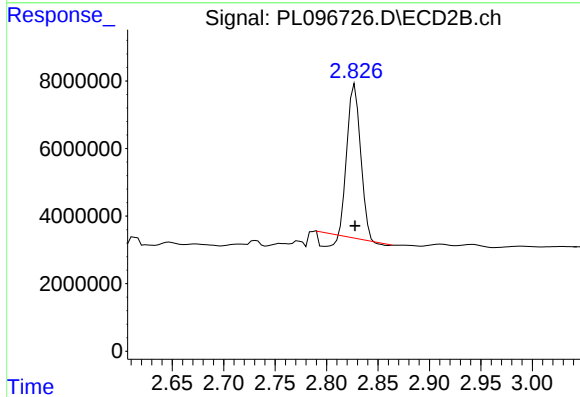


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 37422095
Conc: 7.83 ng/ml

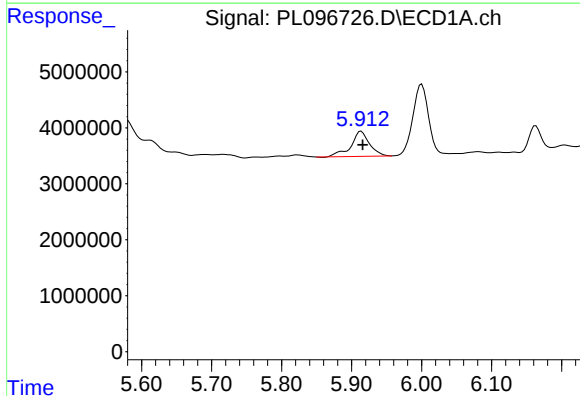


#10 gamma-Chlordane

R.T.: 5.914 min
Delta R.T.: -0.002 min
Response: 8231594
Conc: 2.16 ng/ml

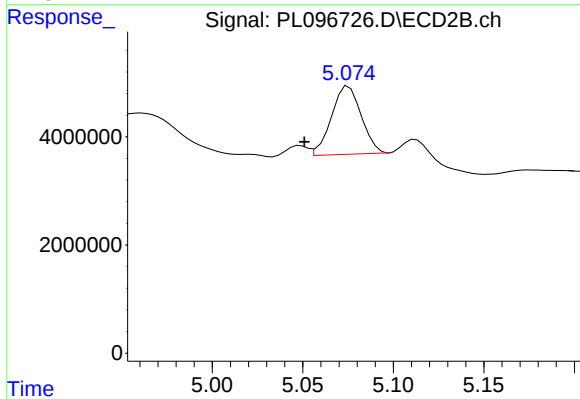

#10 gamma-Chlordane


R.T.: 5.075 min
Delta R.T.: 0.025 min
Response: 14441663
Conc: 2.46 ng/ml

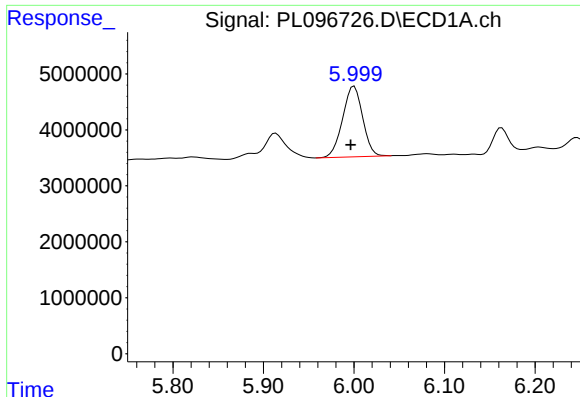

#11 alpha-Chlordane


R.T.: 6.000 min
Delta R.T.: 0.004 min
Response: 19357329
Conc: 5.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
248

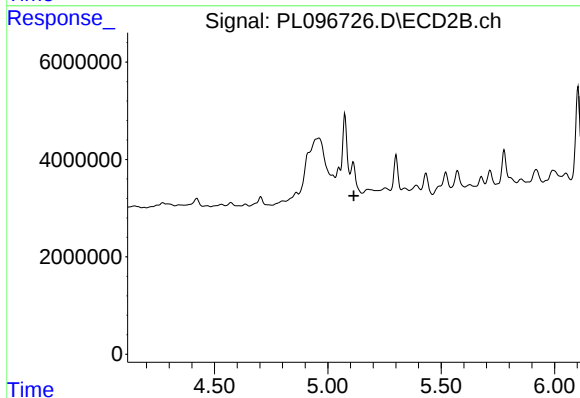


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

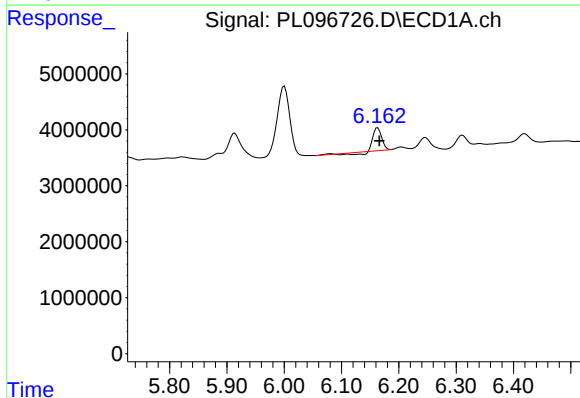


#12 4,4'-DDE

R.T.: 6.163 min
Delta R.T.: -0.003 min
Response: 3513754
Conc: 1.09 ng/ml

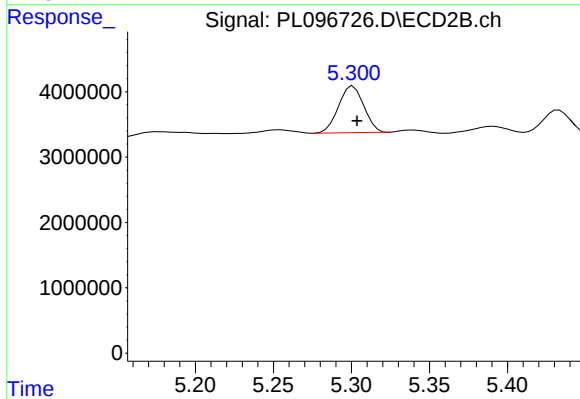

#12 4,4'-DDE


R.T.: 5.301 min
Delta R.T.: -0.002 min
Response: 8080170
Conc: 1.47 ng/ml

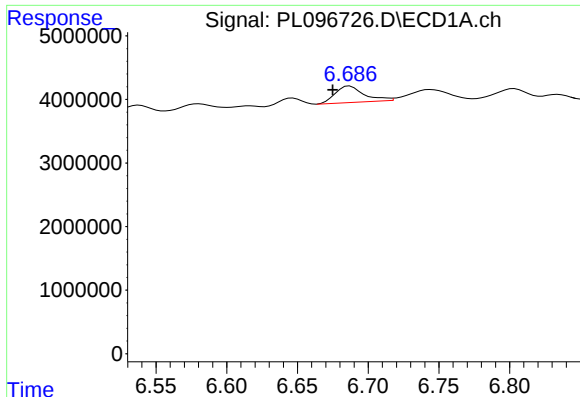

#16 4,4'-DDD


R.T.: 6.687 min
Delta R.T.: 0.012 min
Response: 3852910
Conc: 1.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
248

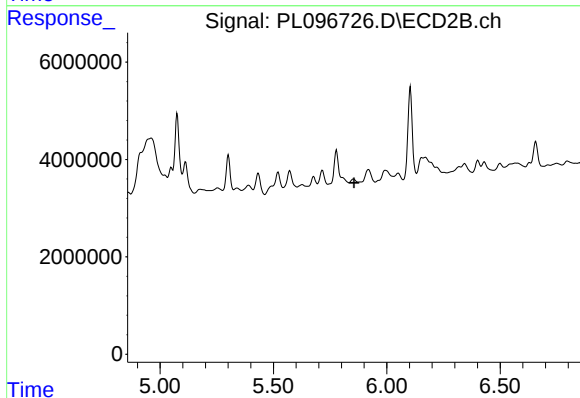


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.856 min
Response: 0
Conc: N.D.

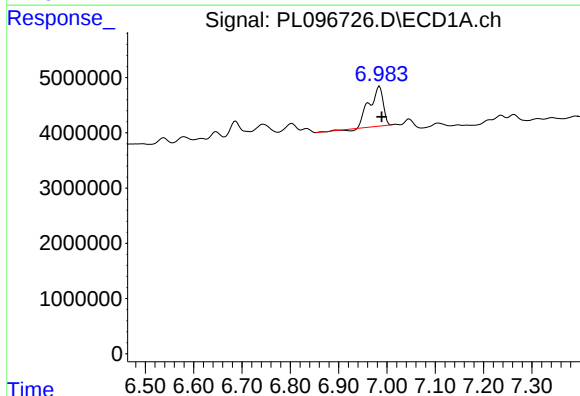


#17 4,4'-DDT

R.T.: 6.985 min
Delta R.T.: -0.005 min
Response: 14153935
Conc: 4.94 ng/ml

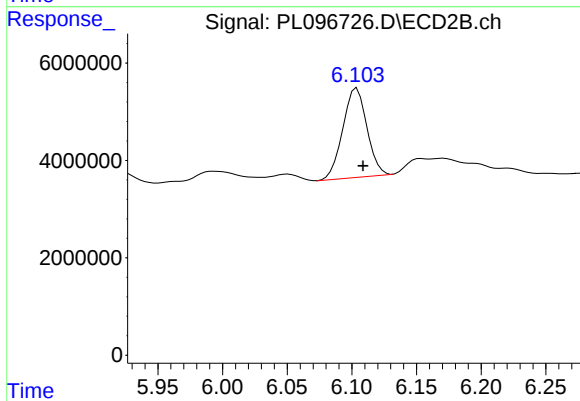

#17 4,4'-DDT


R.T.: 6.104 min
Delta R.T.: -0.005 min
Response: 23697158
Conc: 4.68 ng/ml

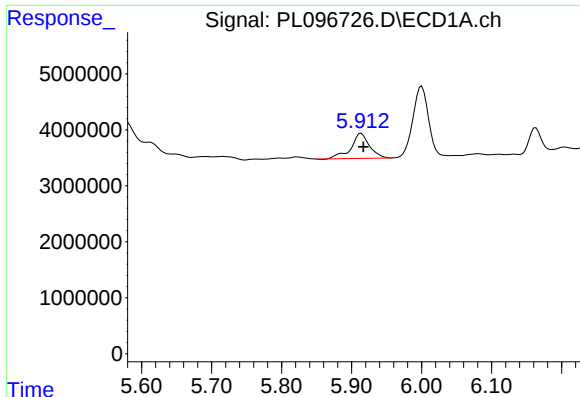

#25 Chlordane-3


R.T.: 5.914 min
Delta R.T.: -0.003 min
Response: 8231594
Conc: 12.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
248

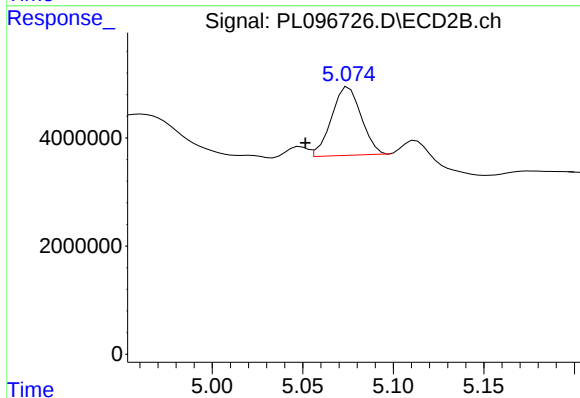


#25 Chlordane-3

R.T.: 5.075 min
Delta R.T.: 0.024 min
Response: 14441663
Conc: 20.77 ng/ml

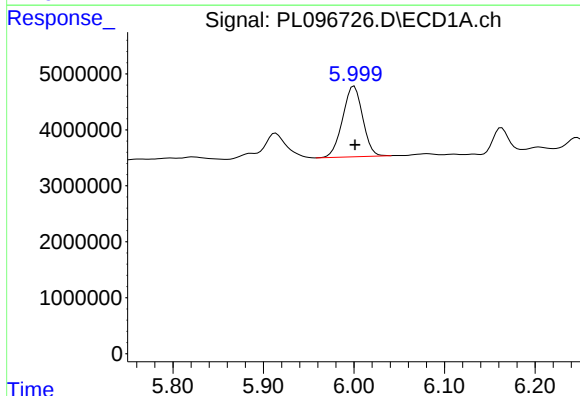


#26 Chlordane-4

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 19357329
Conc: 23.39 ng/ml

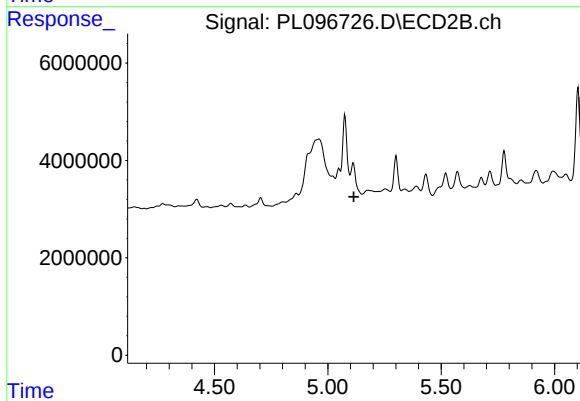

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

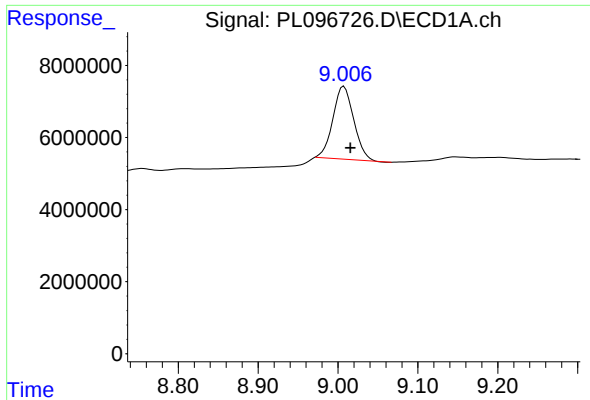

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.008 min
Response: 36690745
Conc: 15.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
248

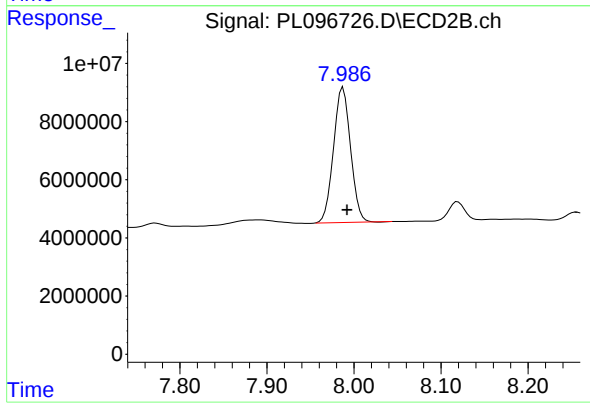

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 63349017
Conc: 14.60 ng/ml