

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
 Data File : PL096731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2025 15:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 22:32:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.532	2.826	70533890	117.3E6	22.175	24.545
28)	SA Decachlor...	9.007	7.987	51847722	96234409	21.742	22.182
Target Compounds							
14)	MA Endrin	0.000	5.714	0	9693371	N.D.	1.793 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080625\
Data File : PL096731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2025 15:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 22:32:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

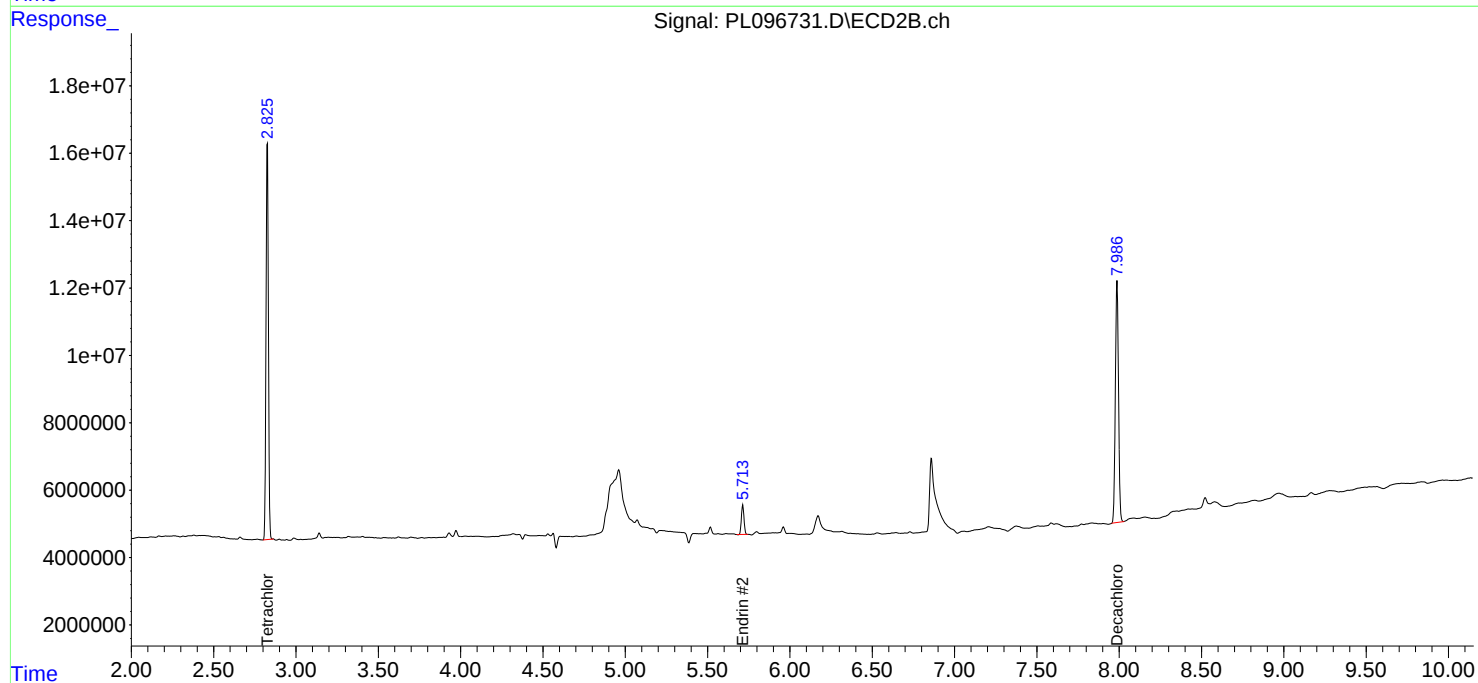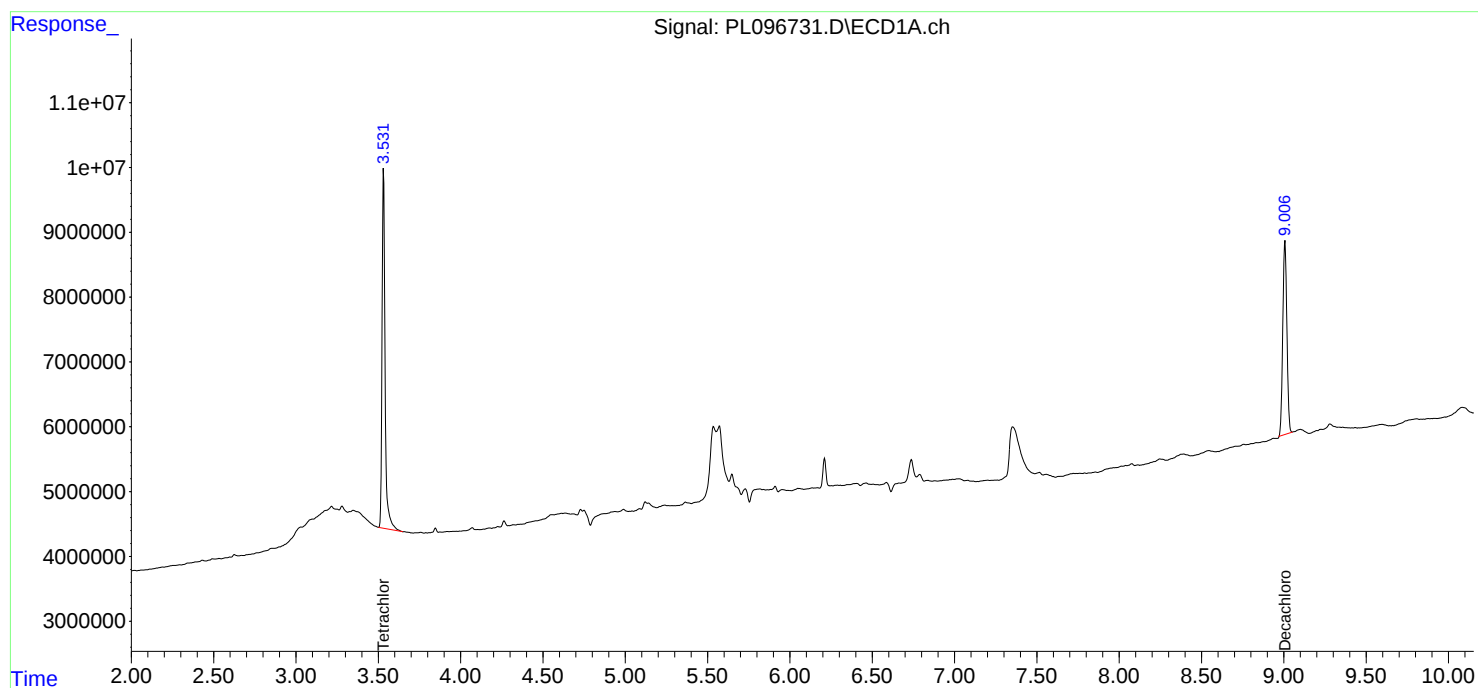


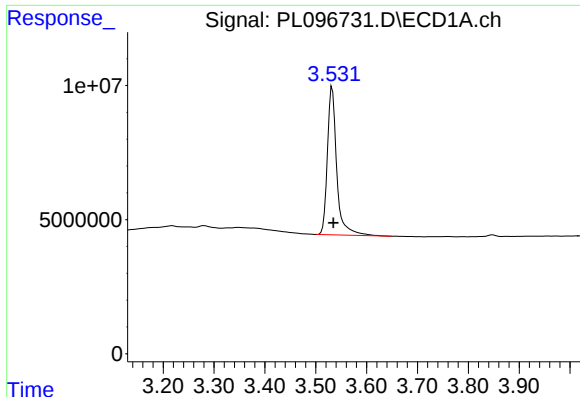

#1 Tetrachloro-m-xylene


R.T.: 3.532 min
Delta R.T.: -0.003 min
Response: 70533890
Conc: 22.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

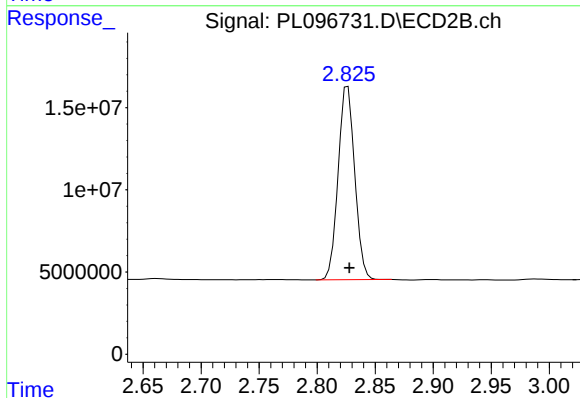


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.001 min
Response: 117268745
Conc: 24.54 ng/ml

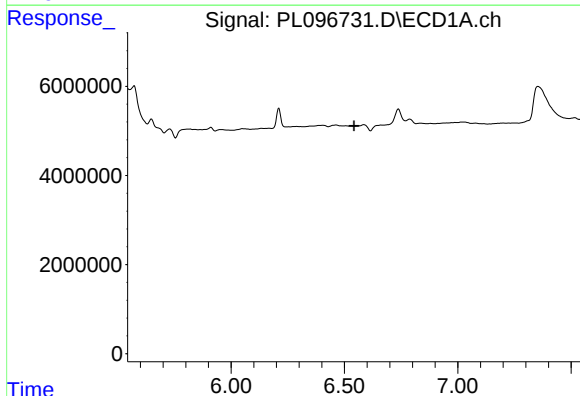


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

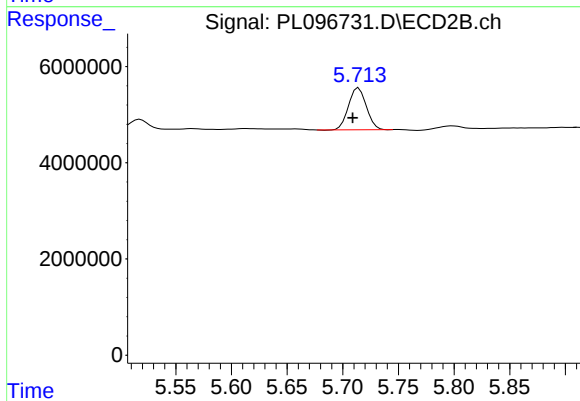

#14 Endrin


R.T.: 5.714 min
Delta R.T.: 0.005 min
Response: 9693371
Conc: 1.79 ng/ml

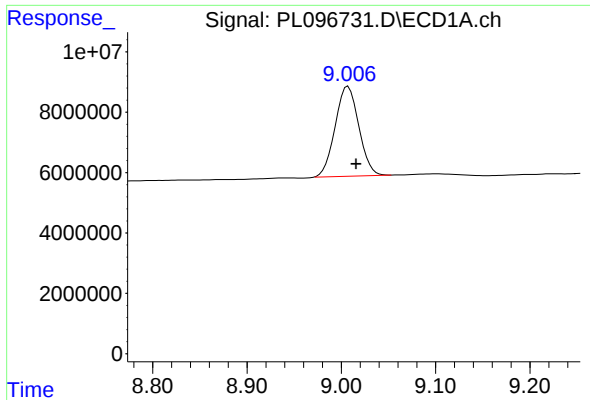

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.009 min
Response: 51847722
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

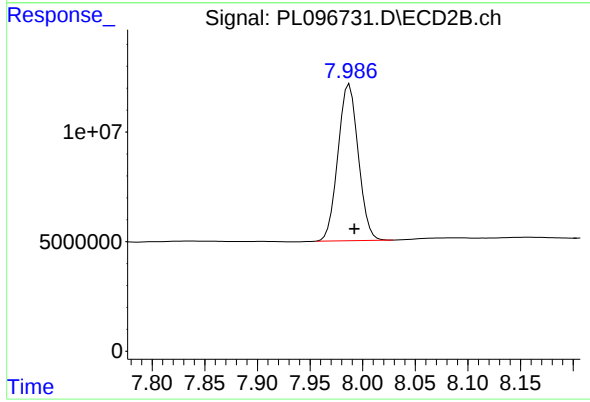

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 96234409
Conc: 22.18 ng/ml