

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
 Data File : PL051143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 08:40
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 01:18:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
4)	MA	Heptachlor	4.329f	0.000	20456334	0	1.247	N.D.	#
7)	B	delta-BHC	4.477	0.000	1818005	0	0.111	N.D.	#
12)	B	4,4'-DDE	5.447f	0.000	24974130	0	1.667	N.D.	#
13)	MA	Dieldrin	5.556	0.000	15447648	0	0.997	N.D.	#
16)	A	4,4'-DDD	5.942	0.000	16956379	0	1.415	N.D.	#
17)	MA	4,4'-DDT	6.176	0.000	153.4E6	0	12.382	N.D.	#
18)	B	Endrin al...	6.255	0.000	18257457	0	1.583	N.D.	#
20)	A	Methoxychlor	6.729f	0.000	12857538	0	2.061	N.D.	#
21)	B	Endrin ke...	6.937	0.000	51626165	0	3.775	N.D.	#
24)		Chlordane-2	4.652	0.000	52180413	0	116.577	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
Data File : PL051143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 08:40
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 01:18:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

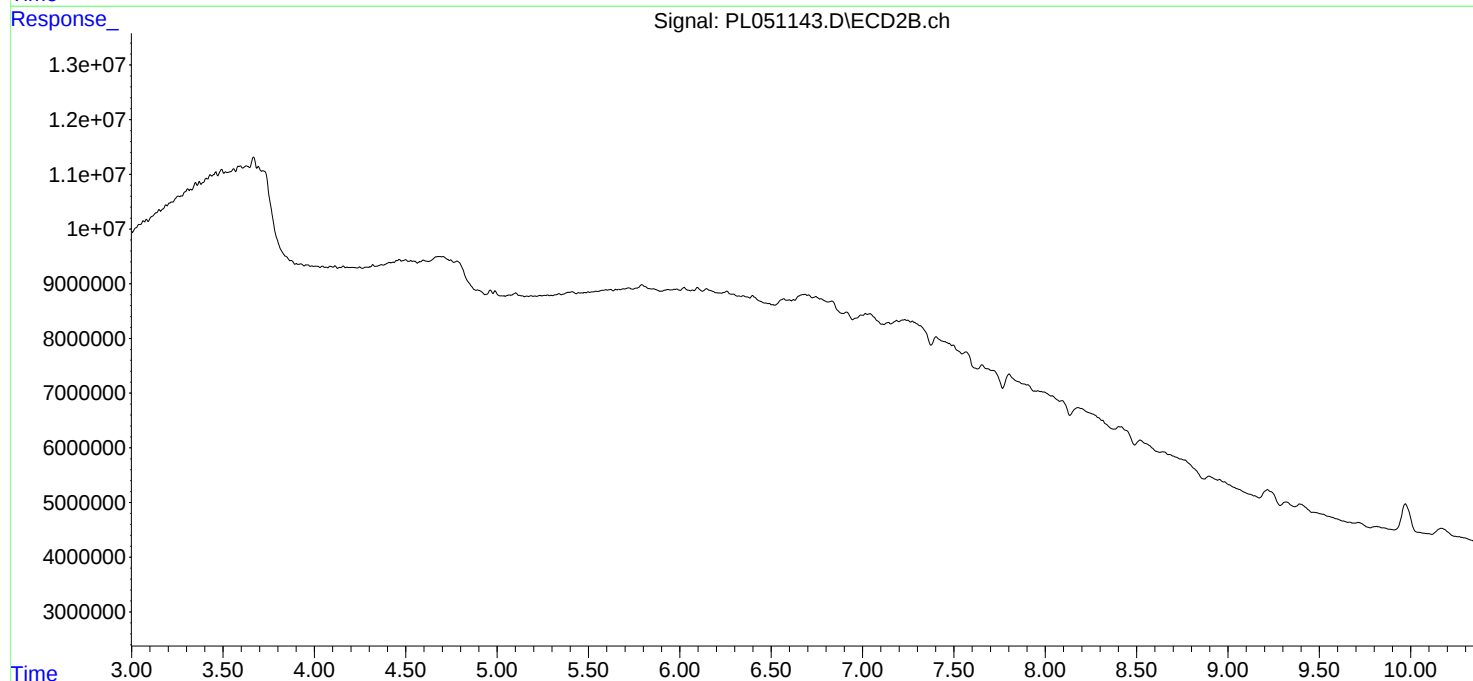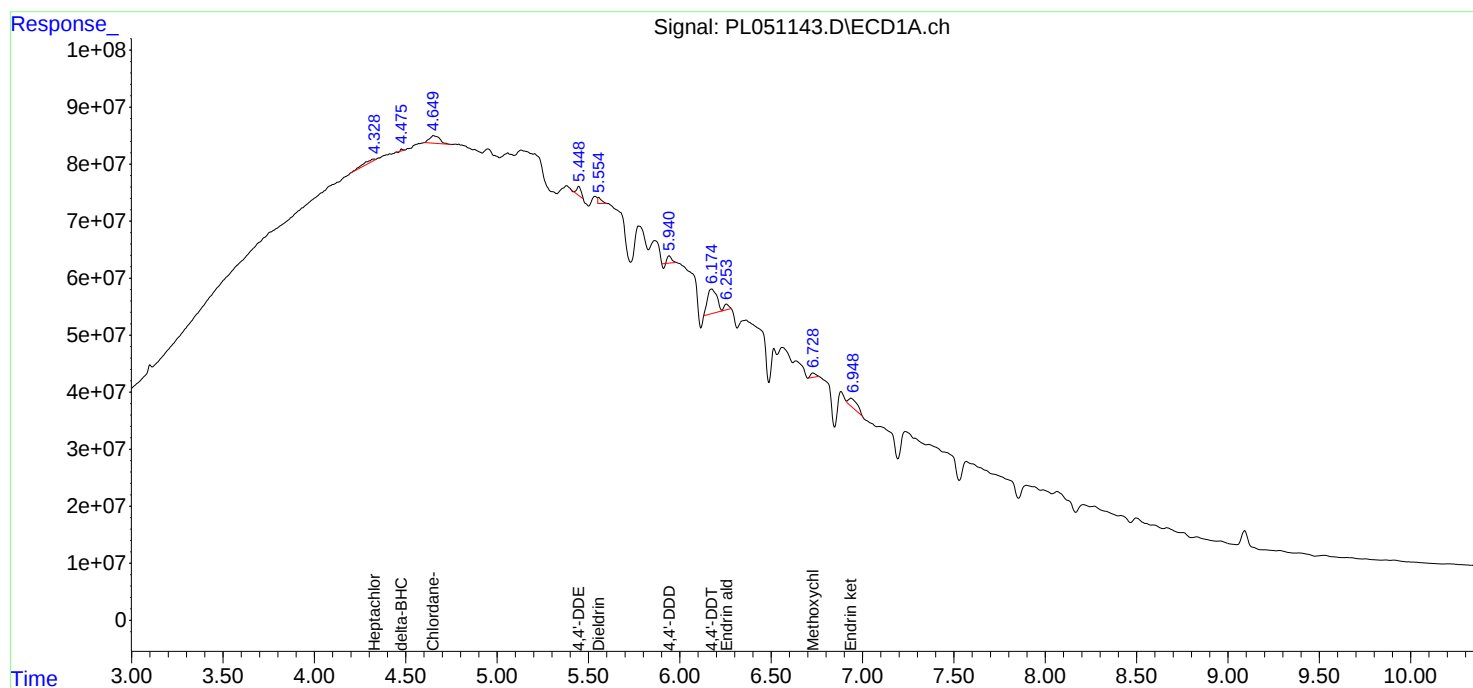


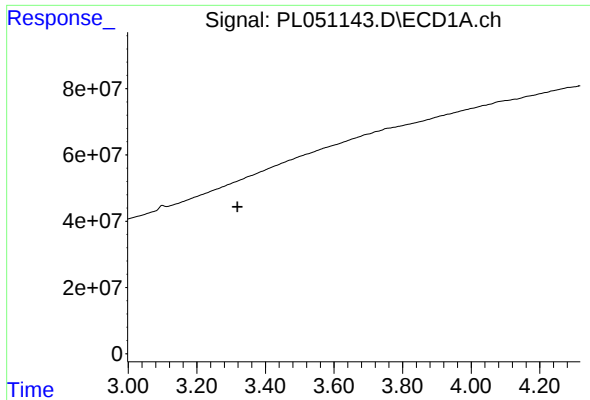

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

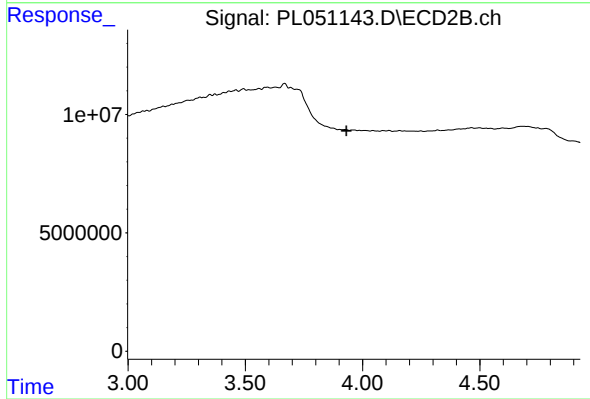


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

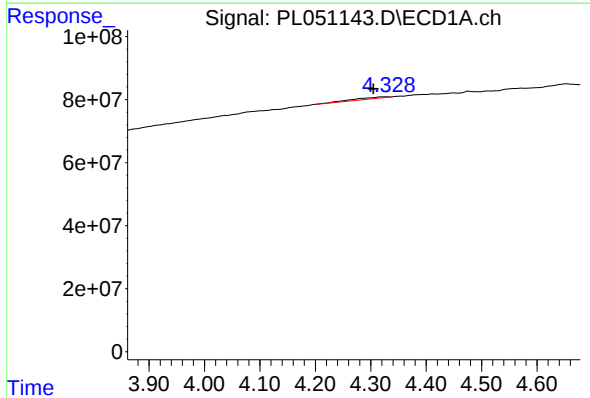


#4 Heptachlor

R.T.: 4.329 min
Delta R.T.: 0.023 min
Response: 20456334
Conc: 1.25 ng/ml

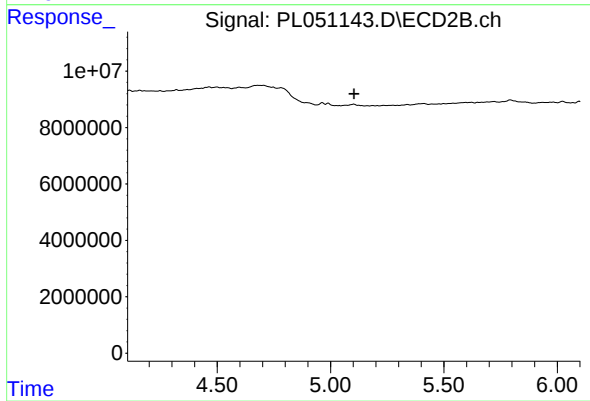

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.104 min
Response: 0
Conc: N.D.

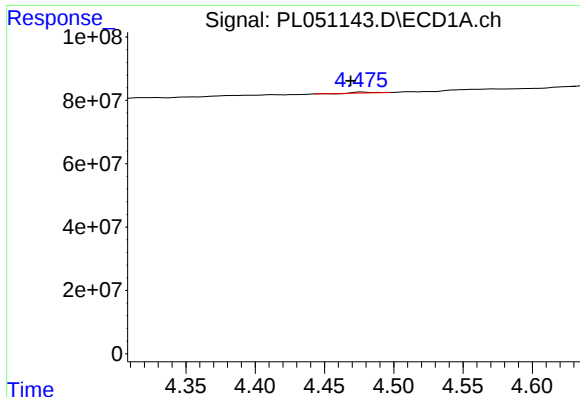

#7 delta-BHC


R.T.: 4.477 min
Delta R.T.: 0.008 min
Response: 1818005
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

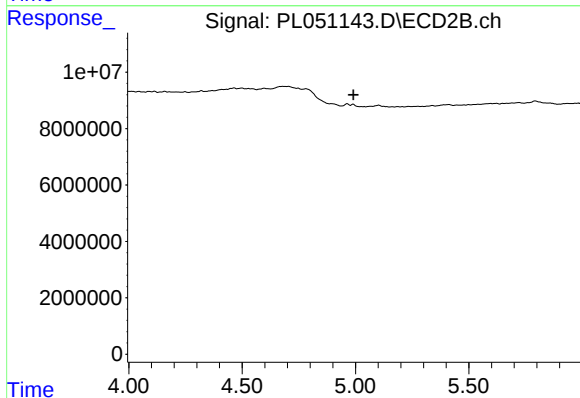


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.991 min
Response: 0
Conc: N.D.

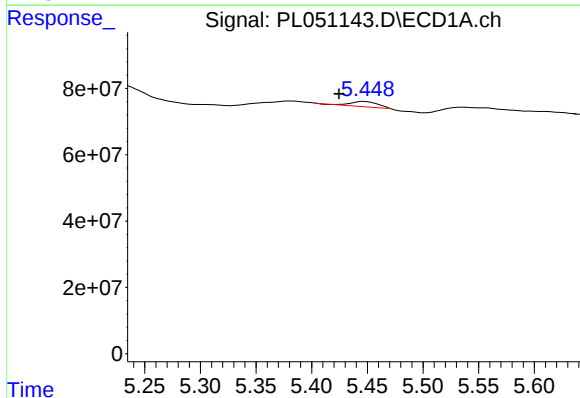


#12 4,4'-DDE

R.T.: 5.447 min
Delta R.T.: 0.022 min
Response: 24974130
Conc: 1.67 ng/ml

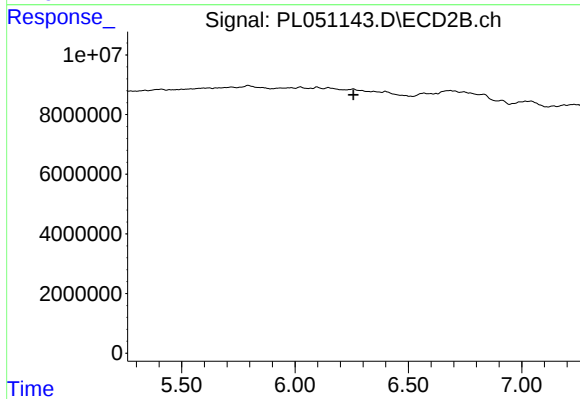

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.258 min
Response: 0
Conc: N.D.

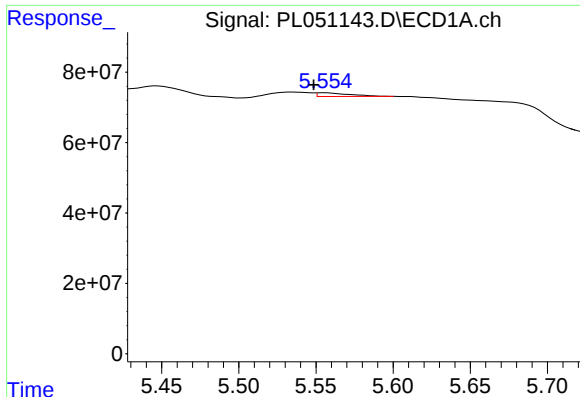

#13 Dieldrin


R.T.: 5.556 min
Delta R.T.: 0.007 min
Response: 15447648
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

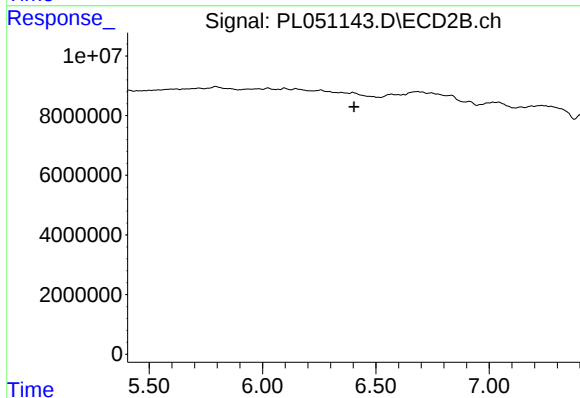


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

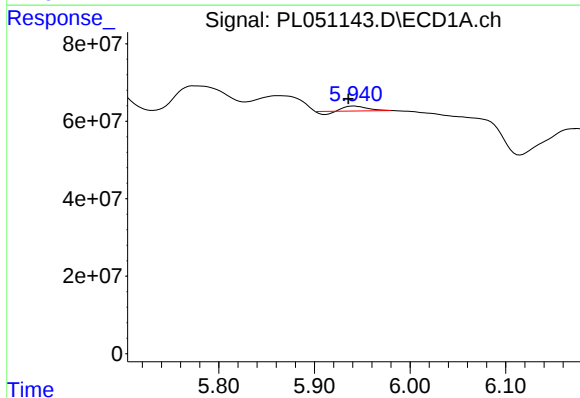


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.006 min
Response: 16956379
Conc: 1.41 ng/ml

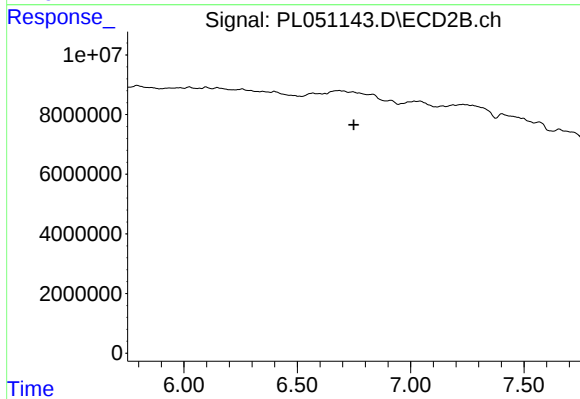

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

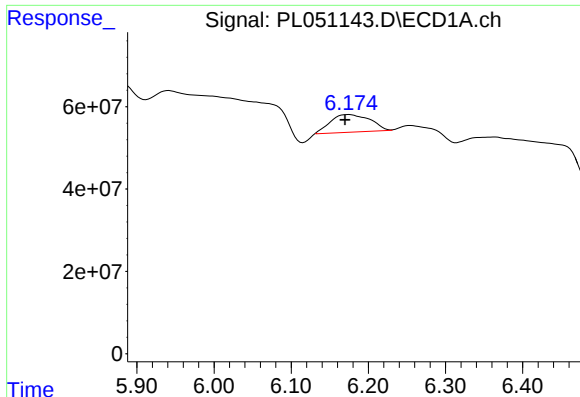

#17 4,4'-DDT


R.T.: 6.176 min
Delta R.T.: 0.006 min
Response: 153362042
Conc: 12.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

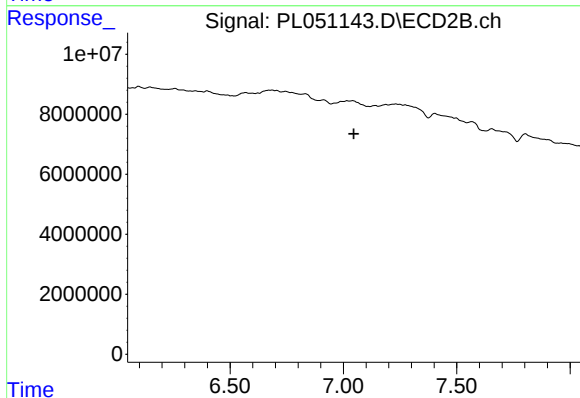


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

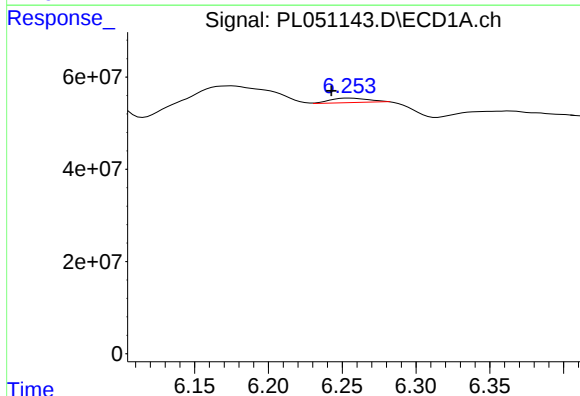


#18 Endrin aldehyde

R.T.: 6.255 min
Delta R.T.: 0.012 min
Response: 18257457
Conc: 1.58 ng/ml

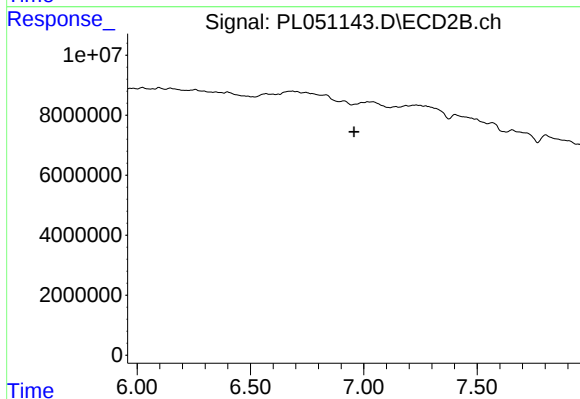

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

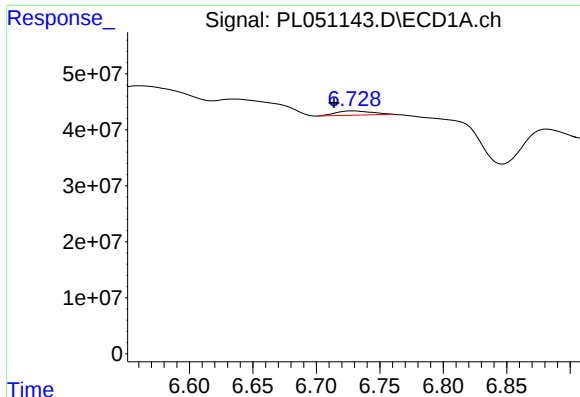

#20 Methoxychlor


R.T.: 6.729 min
Delta R.T.: 0.015 min
Response: 12857538
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

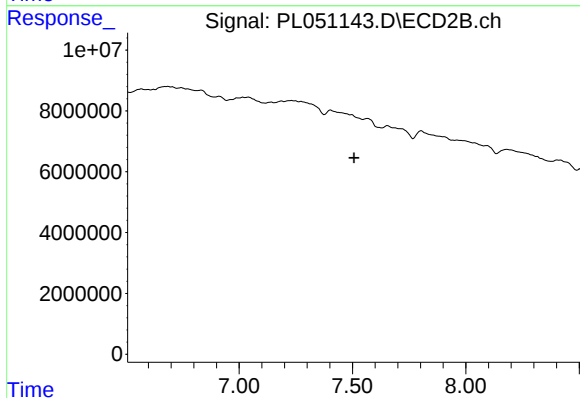


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

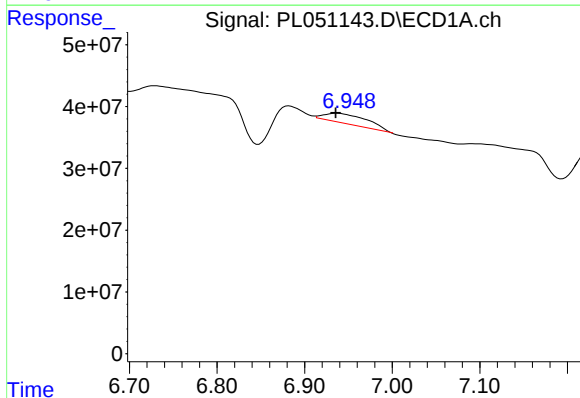


#21 Endrin ketone

R.T.: 6.937 min
Delta R.T.: 0.001 min
Response: 51626165
Conc: 3.77 ng/ml

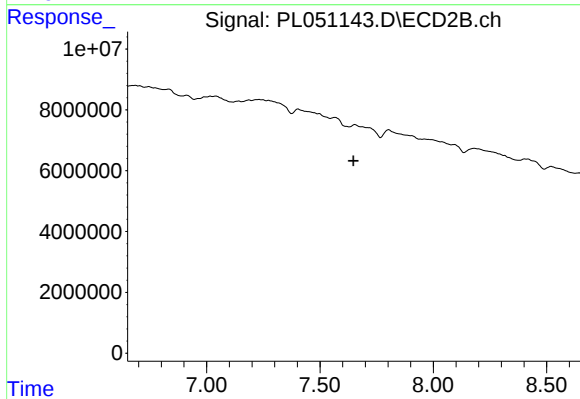

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.648 min
Response: 0
Conc: N.D.

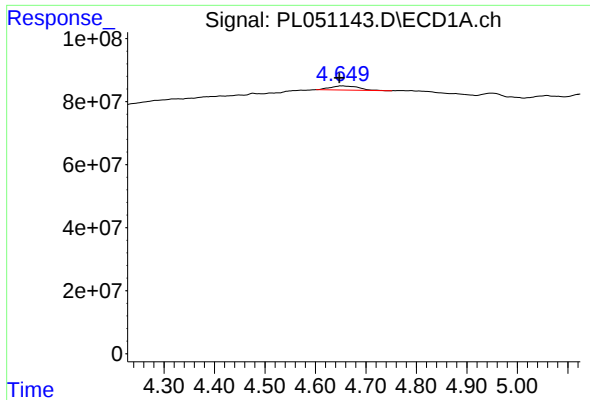

#24 Chlordane-2


R.T.: 4.652 min
Delta R.T.: 0.004 min
Response: 52180413
Conc: 116.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

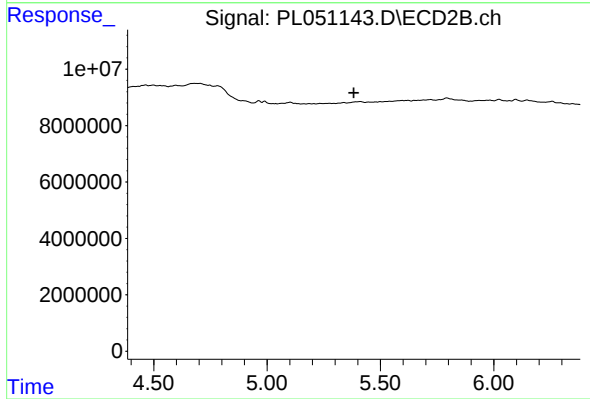


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.383 min
Response: 0
Conc: N.D.

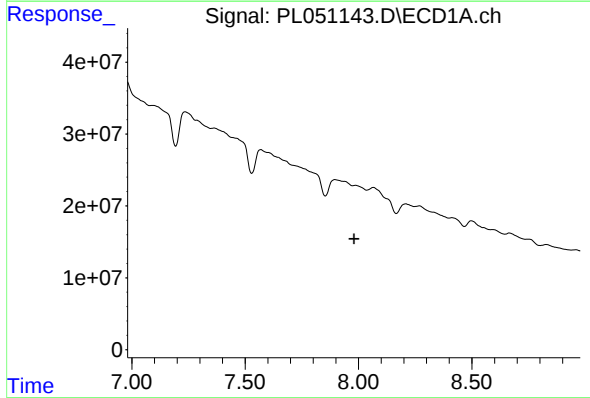

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

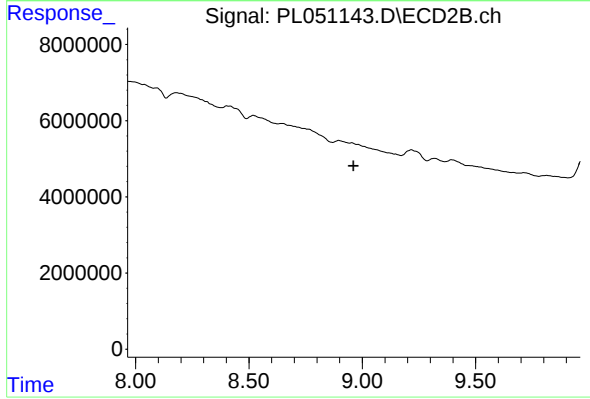

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.