

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
 Data File : PL051157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 15:57
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 01:55:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	243.9E6	64161220	24.274	22.487
28)	SA Decachlor...	7.980	8.958	255.7E6	64888558	25.249	22.946
Target Compounds							
8)	B Heptachlo...	0.000	5.789	0	19061944	N.D.	4.984 #
13)	MA Dieldrin	5.546	0.000	22669100	0	1.463	N.D. #
15)	B Endosulfa...	6.071	0.000	7770896	0	0.555	N.D. #
27)	Chlordane-5	6.071	0.000	7770896	0	15.299	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
Data File : PL051157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 15:57
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 01:55:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

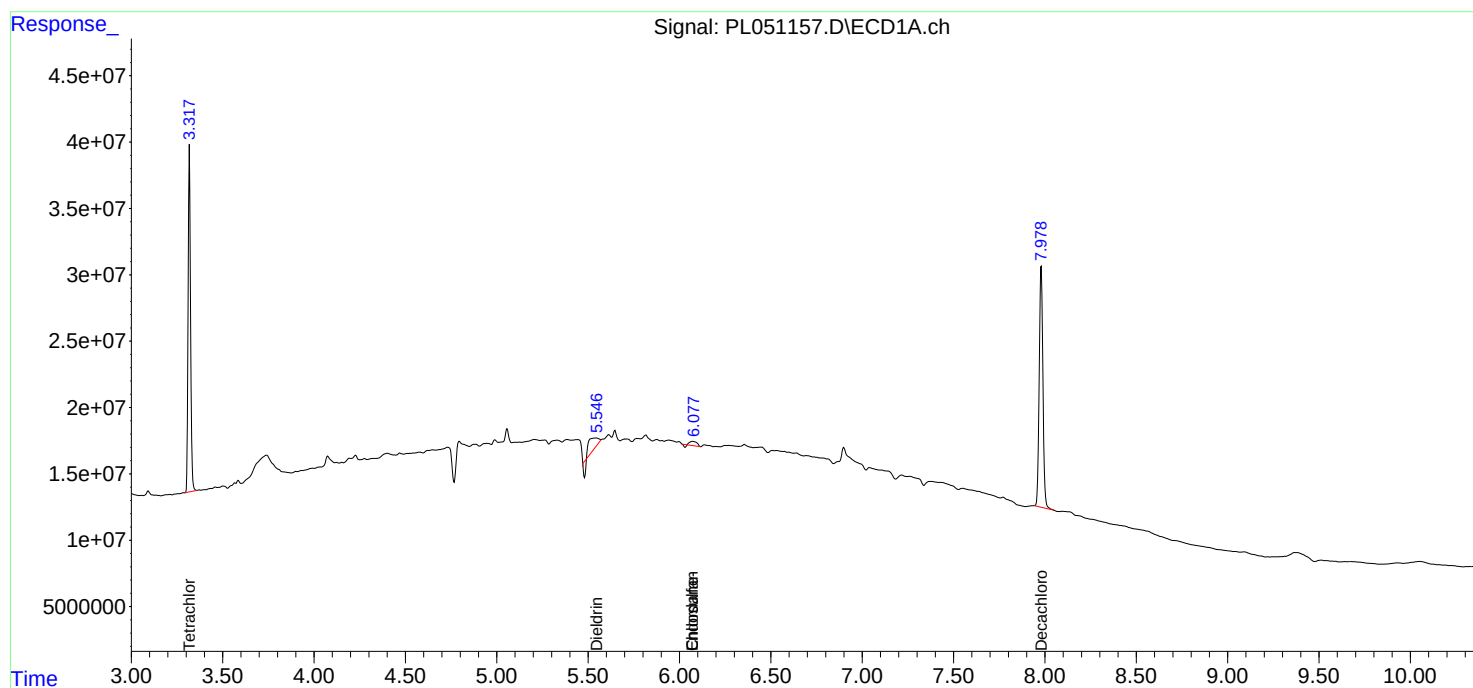


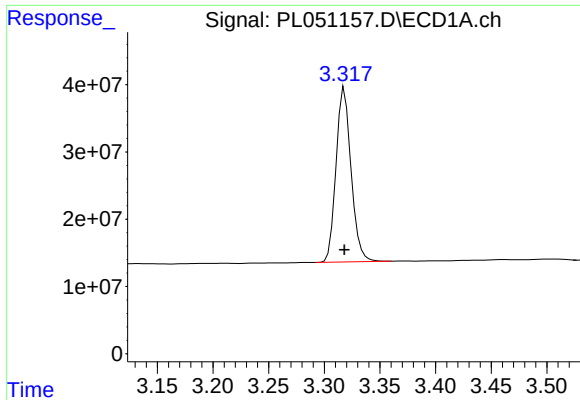

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 243902206
Conc: 24.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

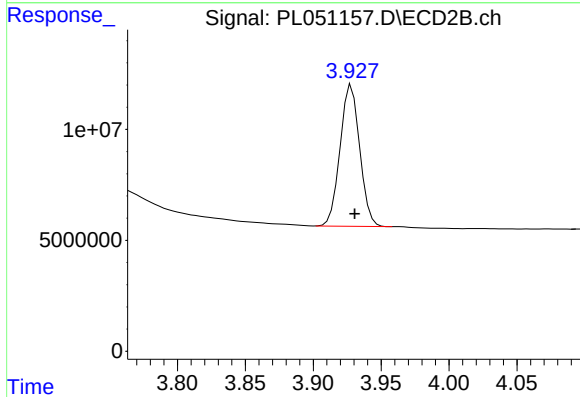


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 64161220
Conc: 22.49 ng/ml

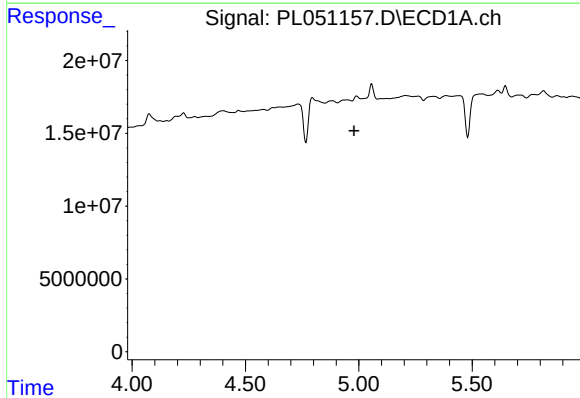


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

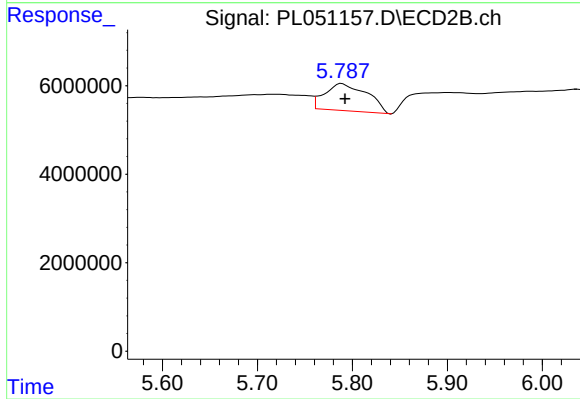

#8 Heptachlor epoxide


R.T.: 5.789 min
Delta R.T.: -0.004 min
Response: 19061944
Conc: 4.98 ng/ml

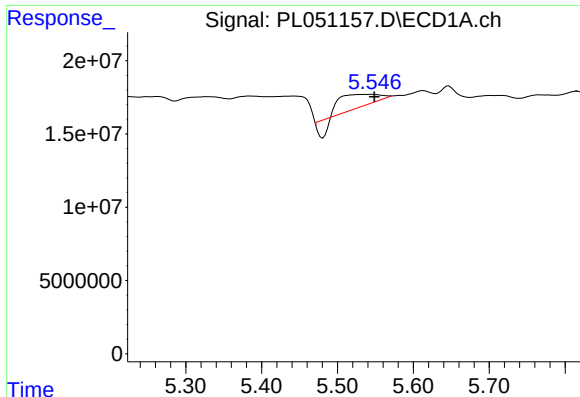

#13 Dieldrin


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 22669100
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

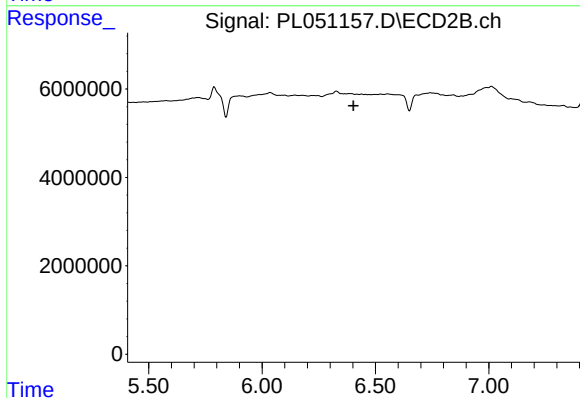


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

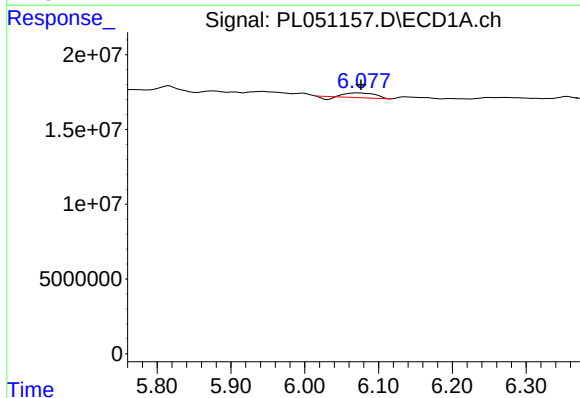


#15 Endosulfan II

R.T.: 6.071 min
Delta R.T.: -0.005 min
Response: 7770896
Conc: 0.56 ng/ml

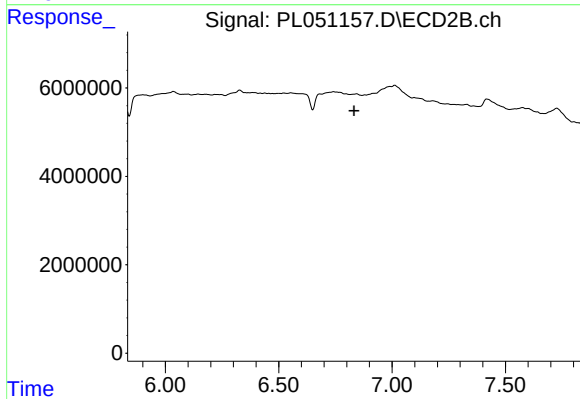

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.833 min
Response: 0
Conc: N.D.

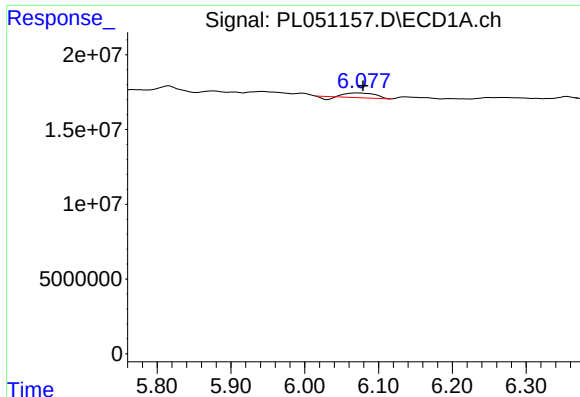

#27 Chlordane-5


R.T.: 6.071 min
Delta R.T.: -0.008 min
Response: 7770896
Conc: 15.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

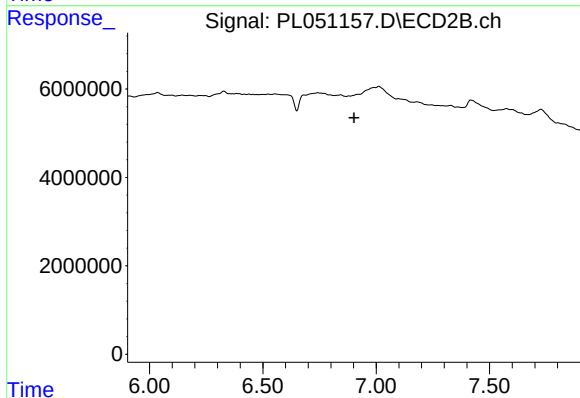


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.902 min
Response: 0
Conc: N.D.

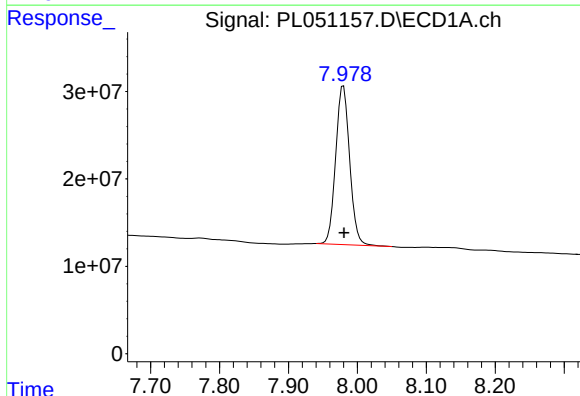

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 255650492
Conc: 25.25 ng/ml

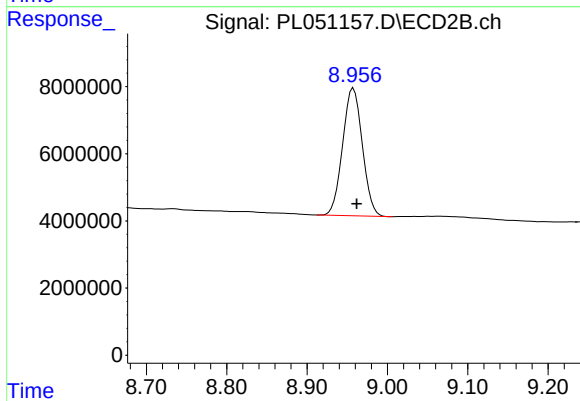

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 64888558
Conc: 22.95 ng/ml