

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
 Data File : PL051182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2019 22:13
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 02:05:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	239.6E6	65529946	23.851	22.967
28)	SA Decachlor...	7.980	8.959	258.9E6	66756147	25.569	23.606
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	5321197	N.D.	3.078 #
8)	B Heptachlo...	0.000	5.790	0	16189390	N.D.	4.233 #
9)	A Endosulfan I	5.328f	0.000	7852097	0	0.540	N.D. #
13)	MA Dieldrin	5.542	0.000	31895395	0	2.058	N.D. #
15)	B Endosulfa...	6.071	0.000	9715068	0	0.694	N.D. #
27)	Chlordane-5	6.071	0.000	9715068	0	19.127	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
Data File : PL051182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2019 22:13
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 02:05:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

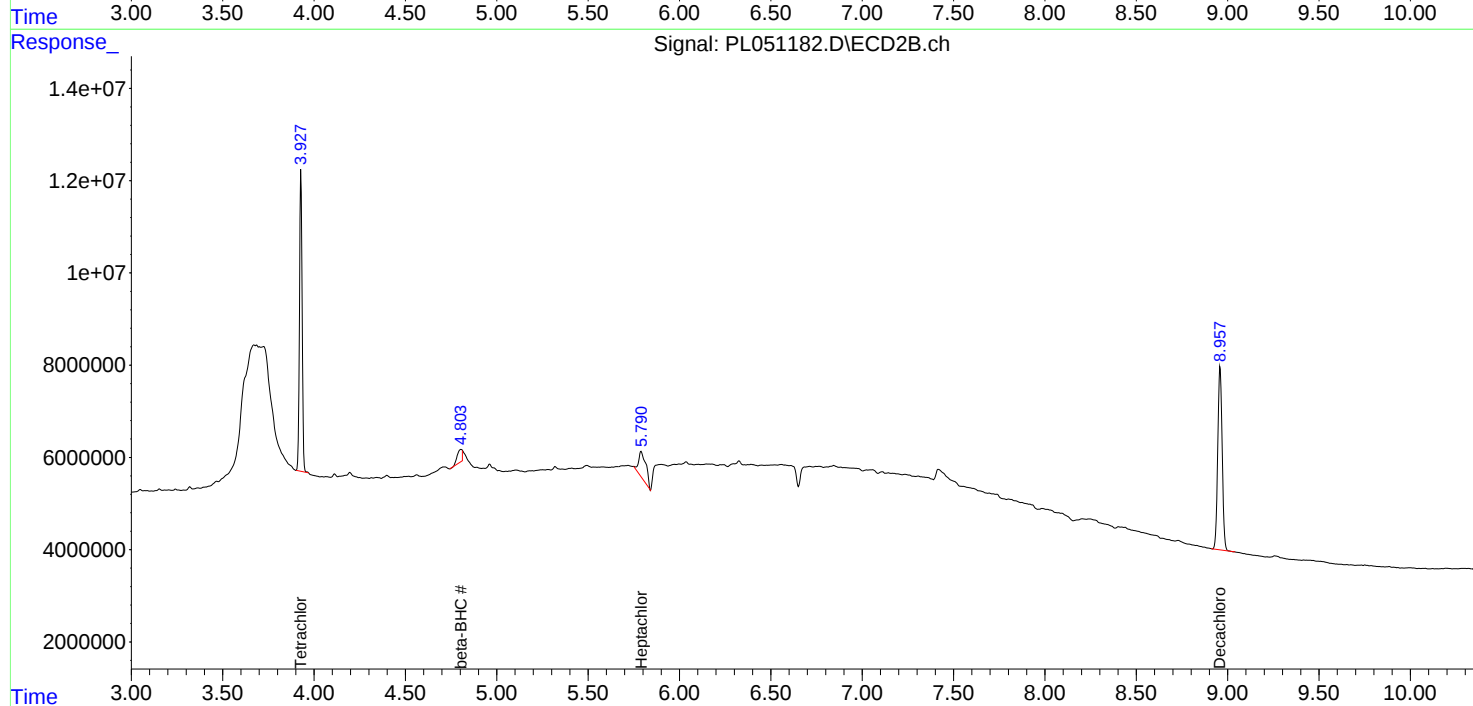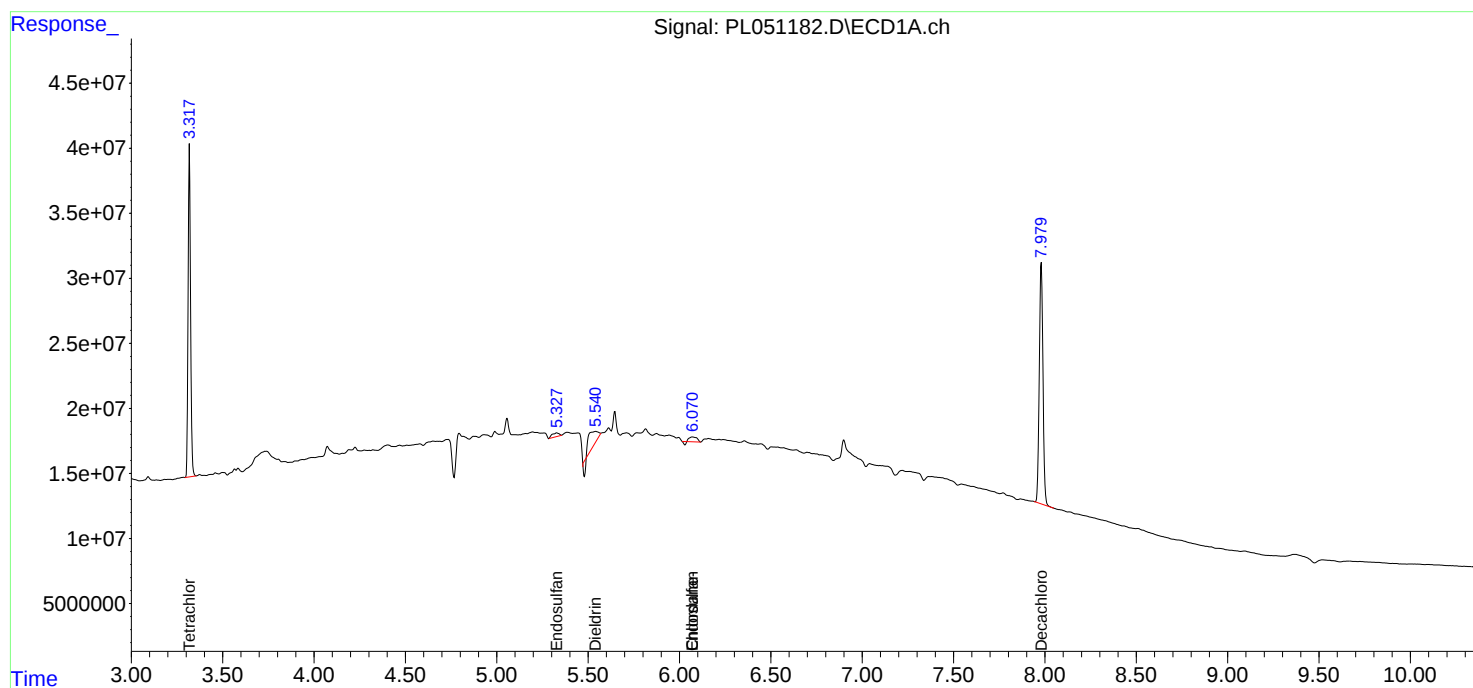


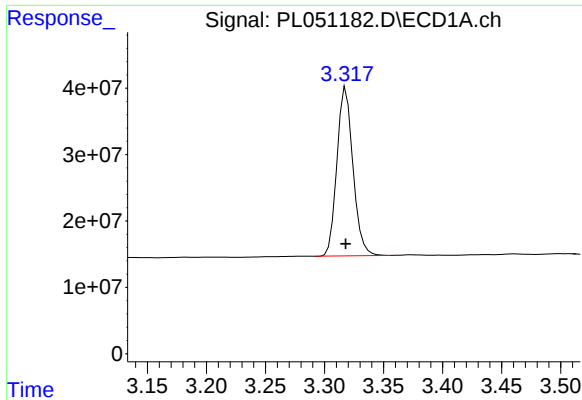

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 239648787
Conc: 23.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

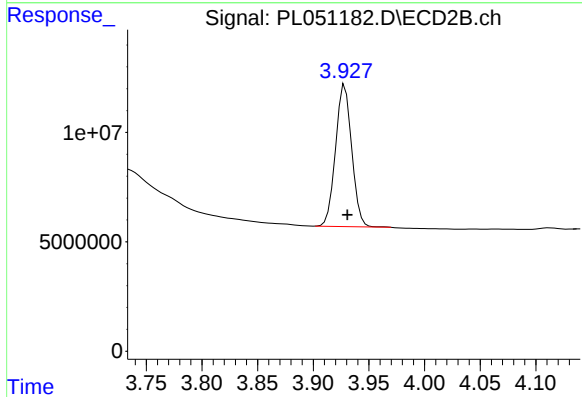


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 65529946
Conc: 22.97 ng/ml

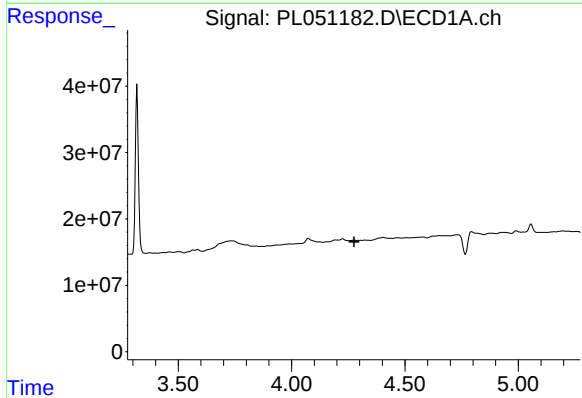


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

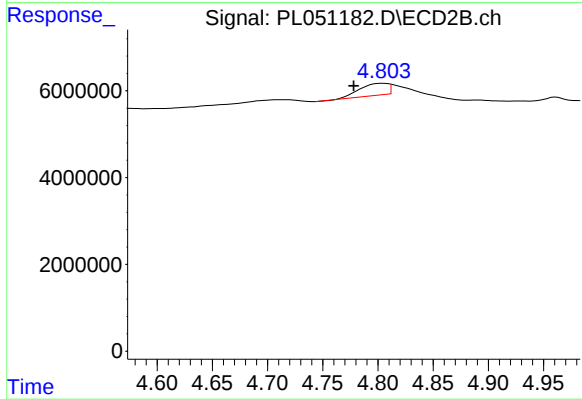

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 5321197
Conc: 3.08 ng/ml

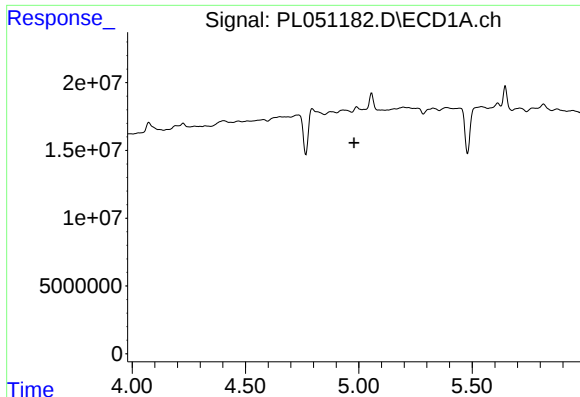

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

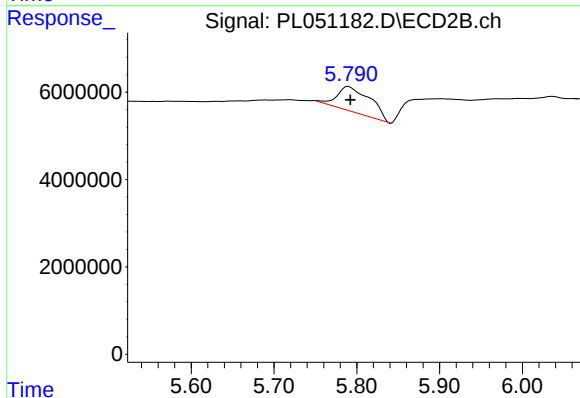


#8 Heptachlor epoxide

R.T.: 5.790 min
Delta R.T.: -0.003 min
Response: 16189390
Conc: 4.23 ng/ml

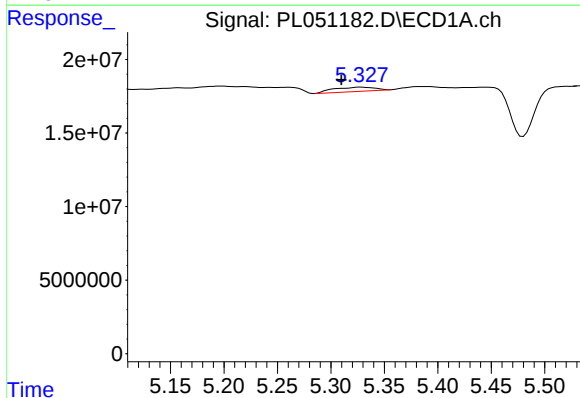


#9 Endosulfan I

R.T.: 5.328 min
Delta R.T.: 0.018 min
Response: 7852097
Conc: 0.54 ng/ml

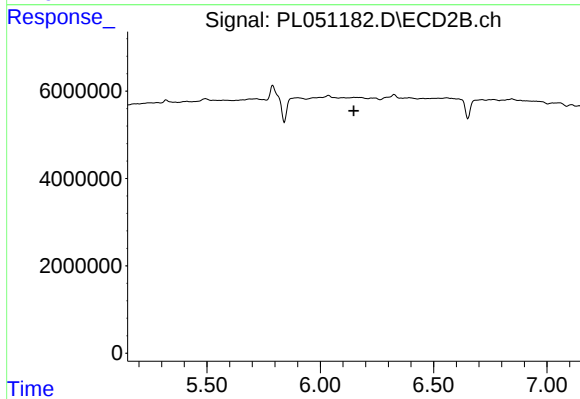

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

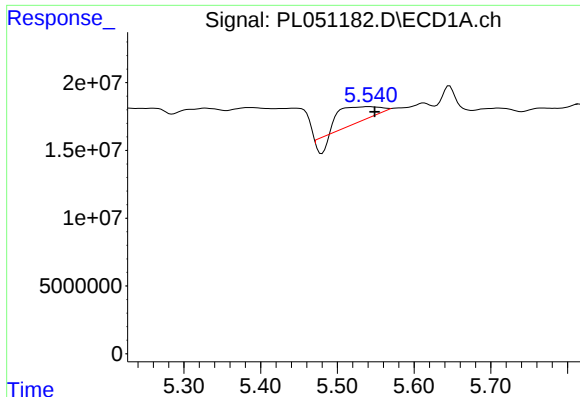

#13 Dieldrin


R.T.: 5.542 min
Delta R.T.: -0.006 min
Response: 31895395
Conc: 2.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

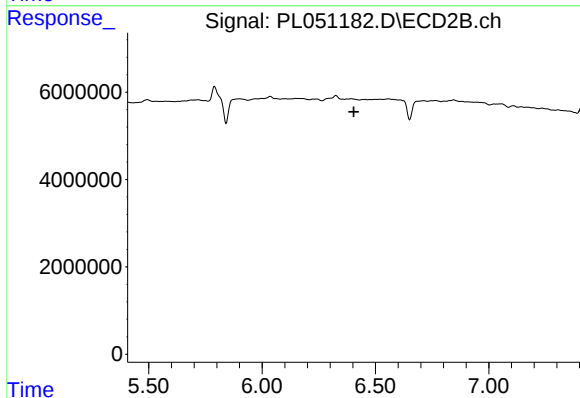


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

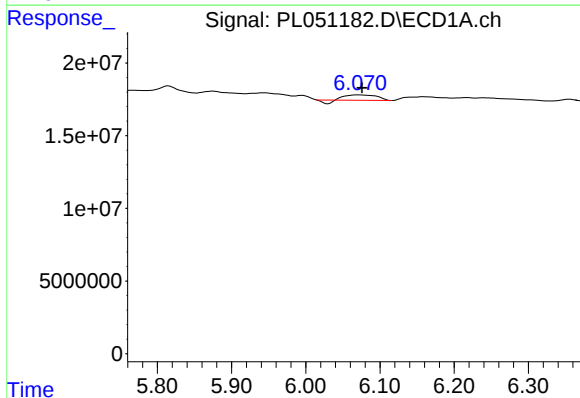


#15 Endosulfan II

R.T.: 6.071 min
Delta R.T.: -0.005 min
Response: 9715068
Conc: 0.69 ng/ml

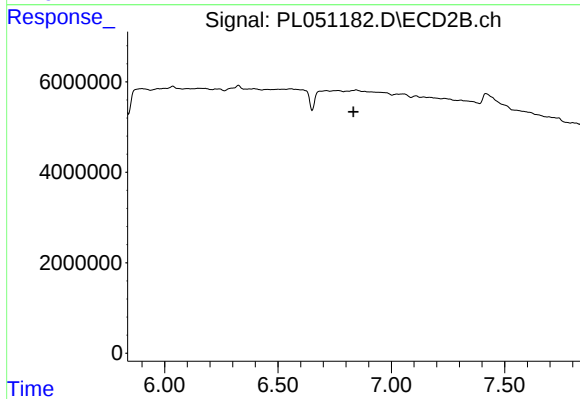

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.833 min
Response: 0
Conc: N.D.

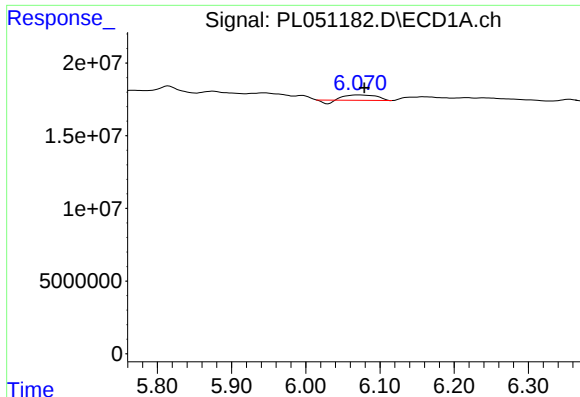

#27 Chlordane-5


R.T.: 6.071 min
Delta R.T.: -0.008 min
Response: 9715068
Conc: 19.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

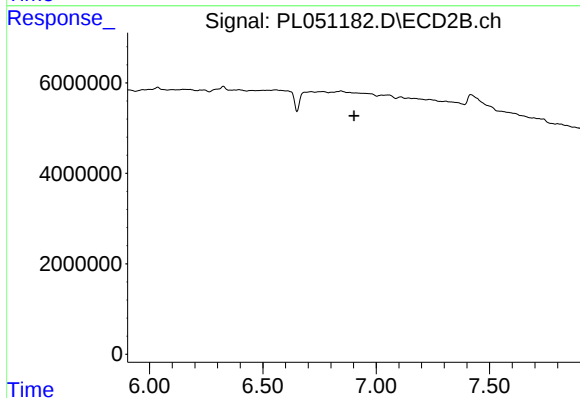


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

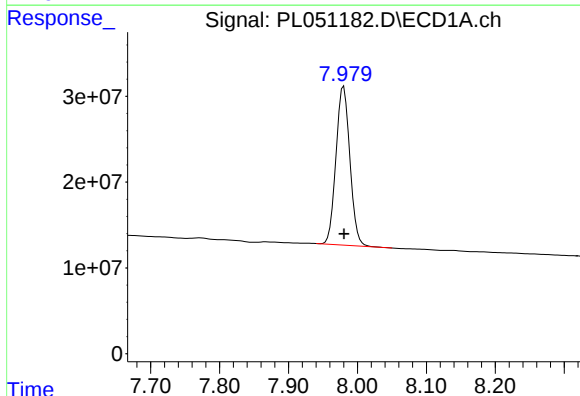

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: 0.000 min
Response: 258894281
Conc: 25.57 ng/ml

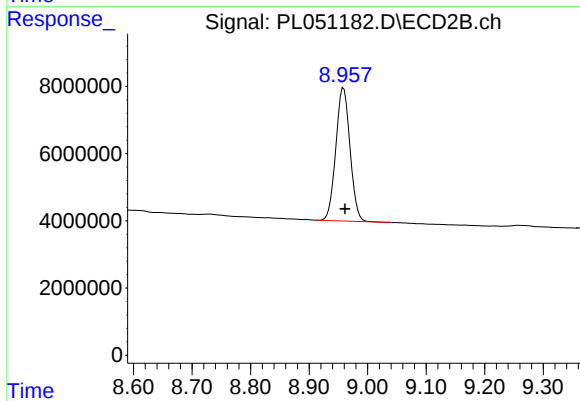

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 66756147
Conc: 23.61 ng/ml