

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
 Data File : PL051190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2019 00:14
 Operator : SM\AJ
 Sample : K4148-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-BH-3-ELU-20190612

Manual Integrations
 APPROVED

Ankita
 8/8/2019 2:44:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 02:09:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.928	185.6E6	56459852	18.471m	19.788
28)	SA Decachlor...	7.979	8.957	156.9E6	44350319	15.495	15.683
Target Compounds							
13)	MA Dieldrin	5.541	6.400	9479947	5587824	0.612m	1.578m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080719\
Data File : PL051190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2019 00:14
Operator : SM\AJ
Sample : K4148-10
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-BH-3-ELU-20190612


Manual Integrations
APPROVED

Ankita
8/8/2019 2:44:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 02:09:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

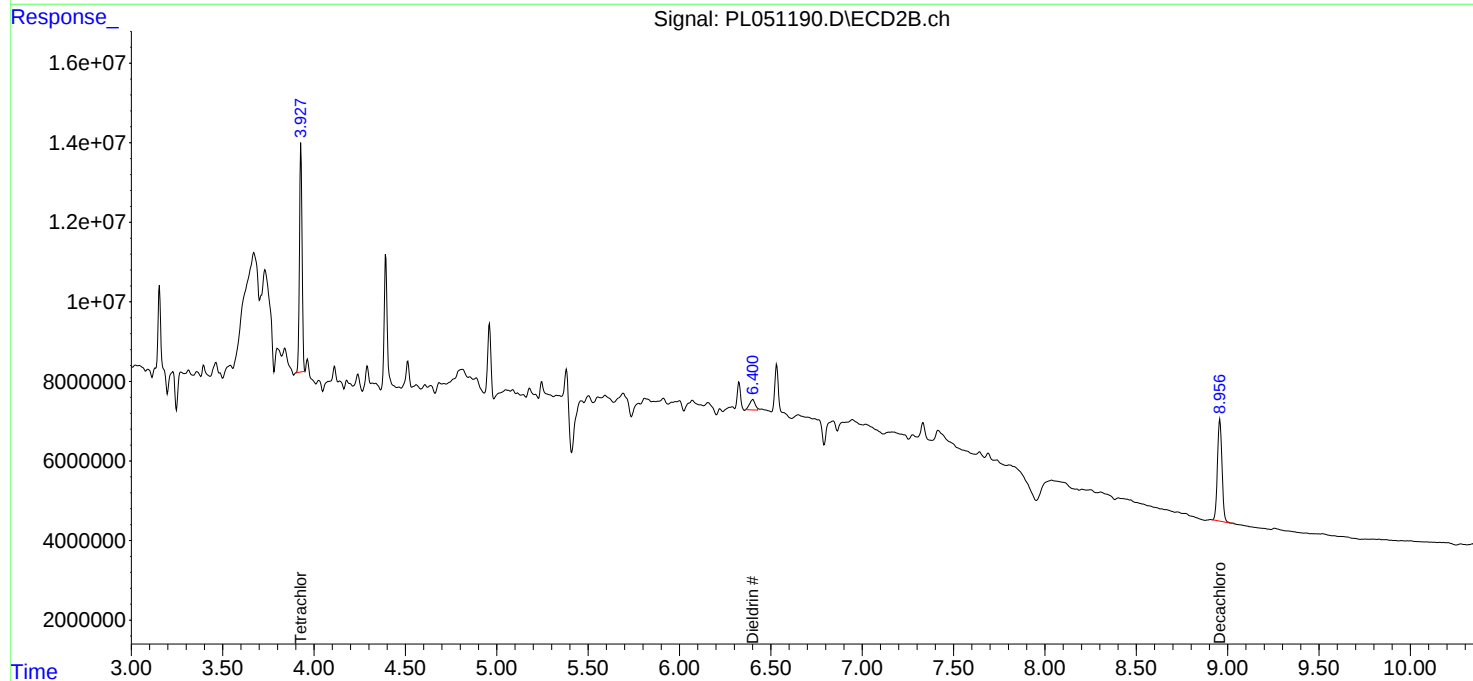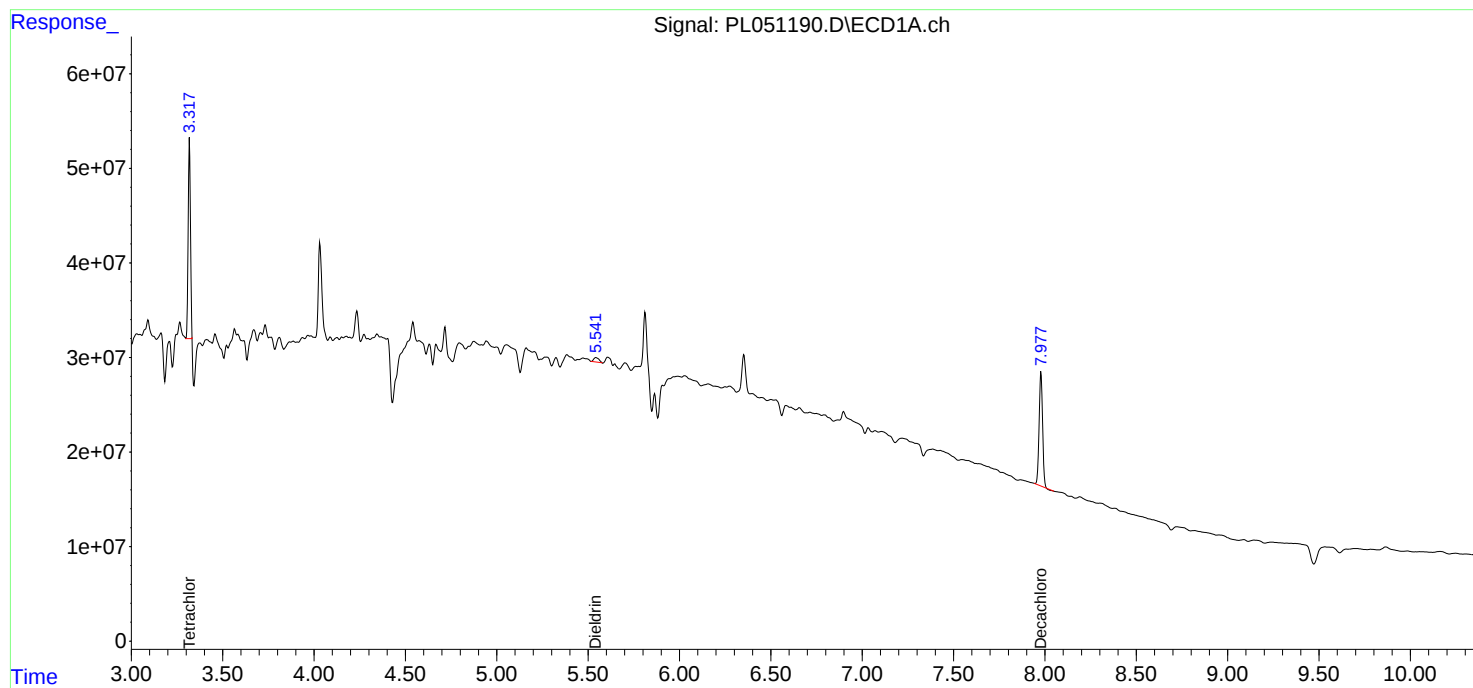

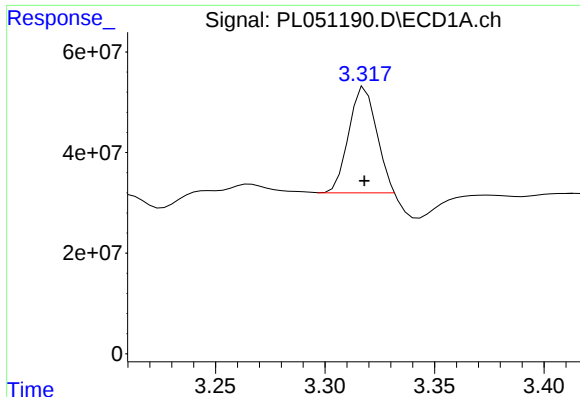

#1 Tetrachloro-m-xylene

R.T.: 3.317 min

Delta R.T.: 0.000 min


Response: 185594280

Conc: 18.47 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMP-BH-3-ELU-20190612

Manual Integrations
APPROVED

Ankita
8/8/2019 2:44:25 PM

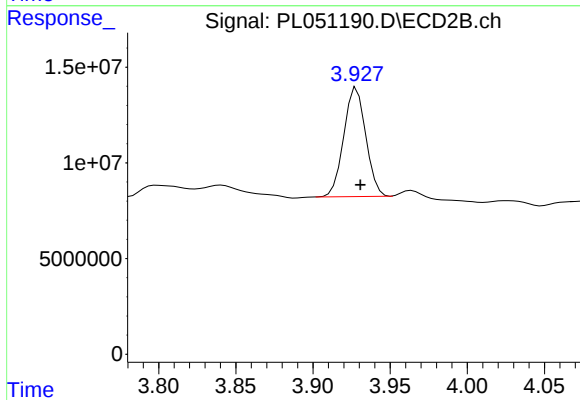


#1 Tetrachloro-m-xylene

R.T.: 3.928 min

Delta R.T.: -0.002 min

Response: 56459852

Conc: 19.79 ng/ml

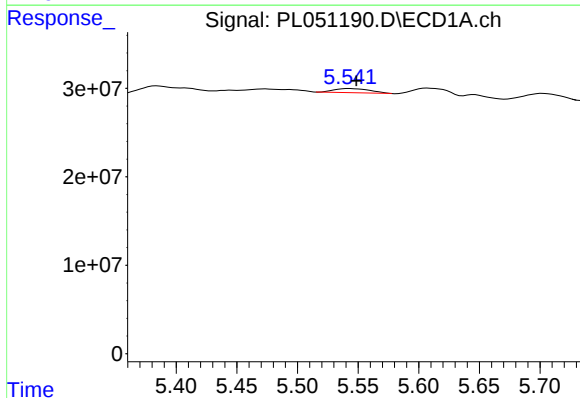


#13 Dieldrin

R.T.: 5.541 min

Delta R.T.: -0.007 min

Response: 9479947

Conc: 0.61 ng/ml m

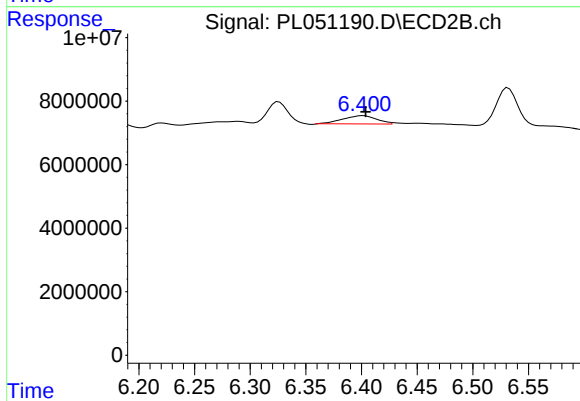


#13 Dieldrin

R.T.: 6.400 min

Delta R.T.: -0.004 min

Response: 5587824

Conc: 1.58 ng/ml m

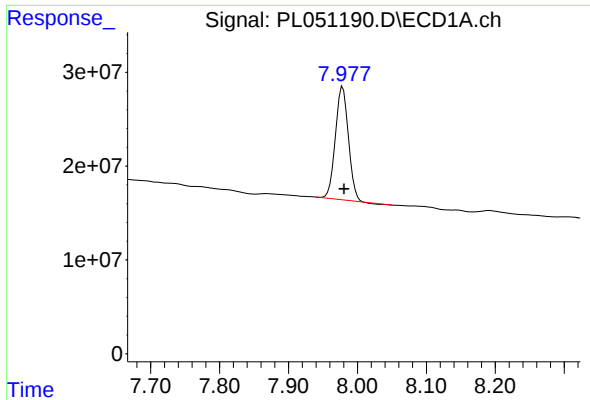


#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 156893182
Conc: 15.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-BH-3-ELU-20190612

Manual Integrations
APPROVED

Ankita
8/8/2019 2:44:25 PM

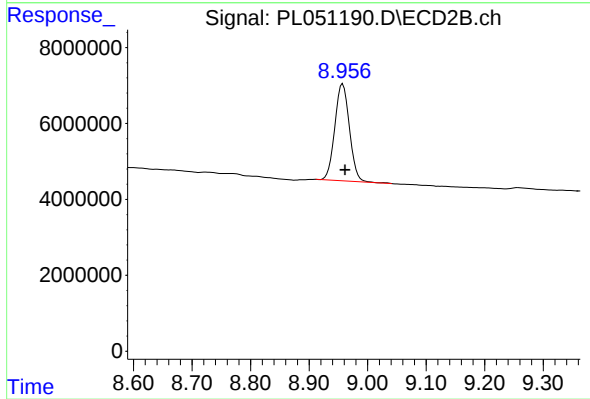

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.004 min
Response: 44350319
Conc: 15.68 ng/ml