

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080720\
 Data File : PL060573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2020 17:56
 Operator : DD\AJ
 Sample : L3508-01 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-080620

Manual Integrations
 APPROVED

Ankita
 8/10/2020 1:04:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 00:07:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 30 04:13:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	2363364	3461757	1.186m	1.324m
28)	SA Decachlor...	8.217	9.097	2380958	3013508	1.560m	1.675m
Target Compounds							
12)	B 4,4'-DDE	5.625	6.353	4264744	7318693	2.530m	2.767
17)	MA 4,4'-DDT	6.382	7.145	1147008	2521465	0.840m	1.247m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080720\
Data File : PL060573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2020 17:56
Operator : DD\AJ
Sample : L3508-01 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-04-080620


Manual Integrations
APPROVED

Ankita
8/10/2020 1:04:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 00:07:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL073020.M
Quant Title : GC Extractables
QLast Update : Thu Jul 30 04:13:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

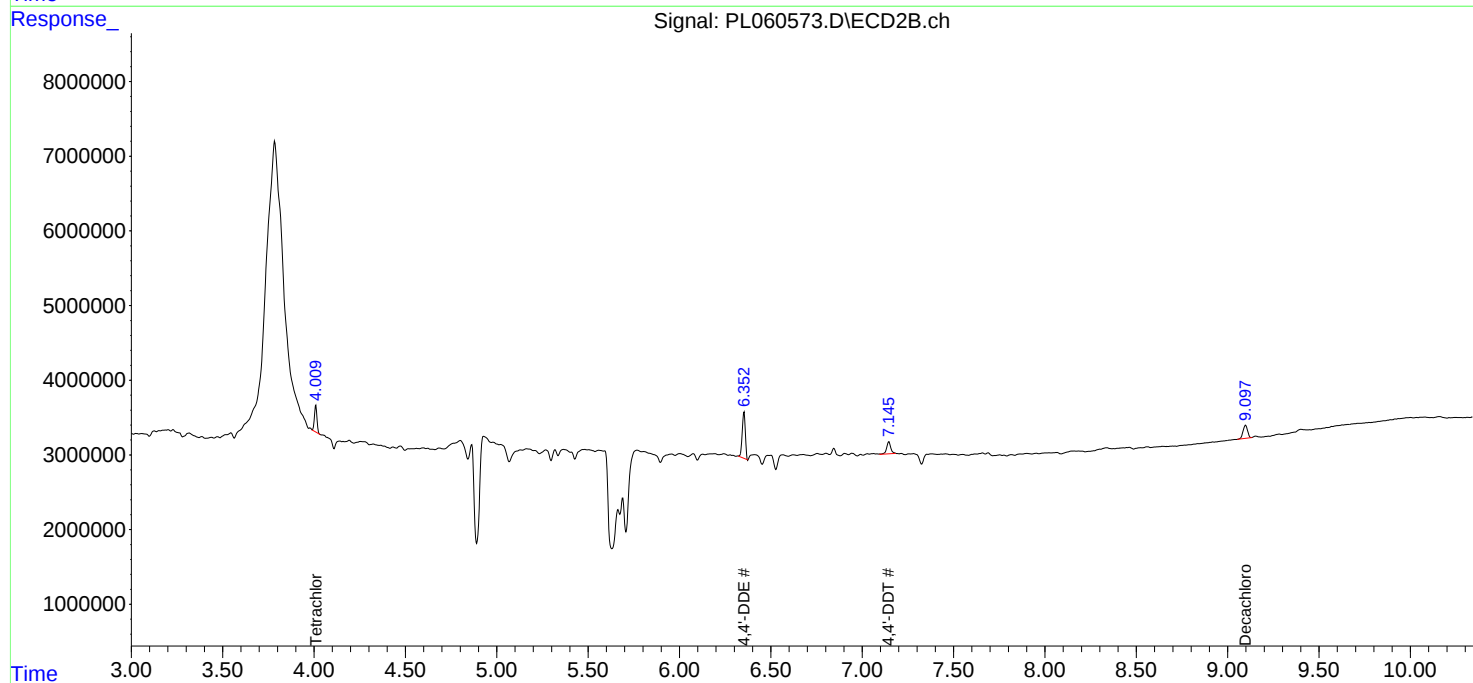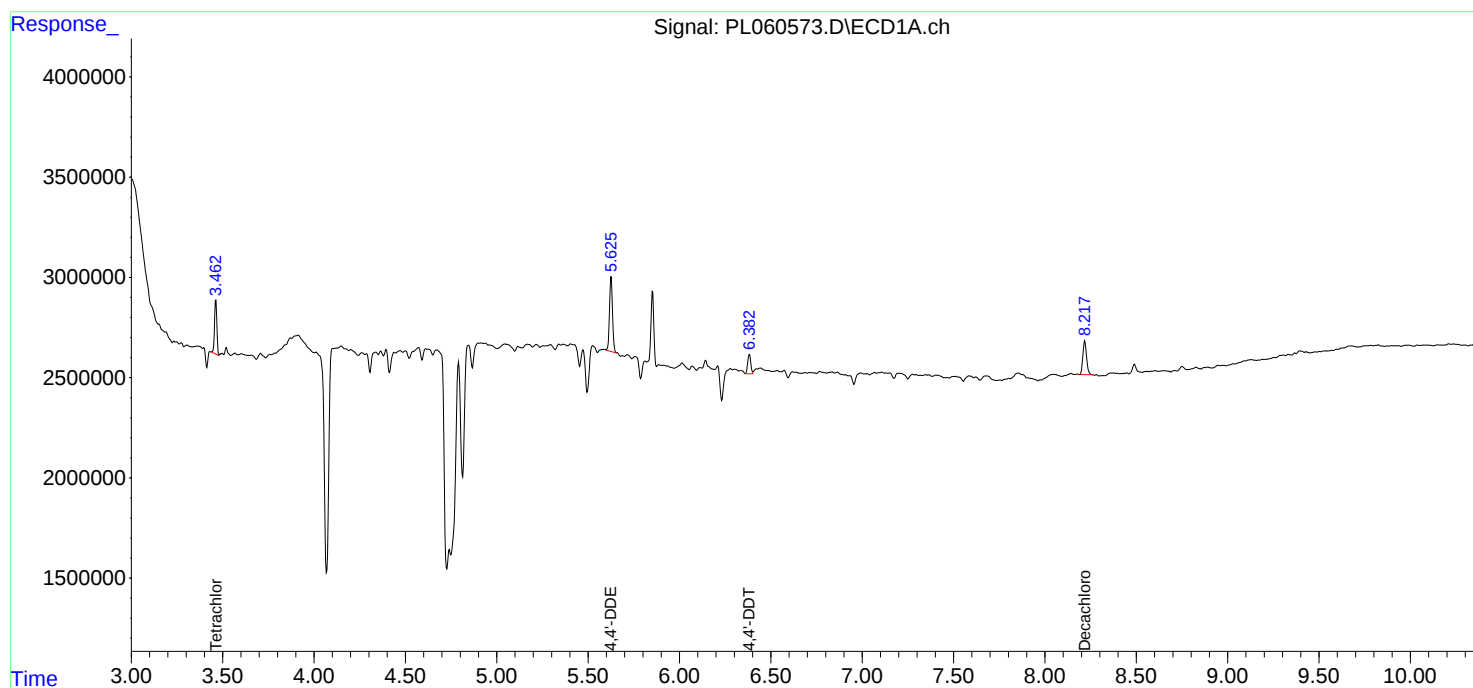

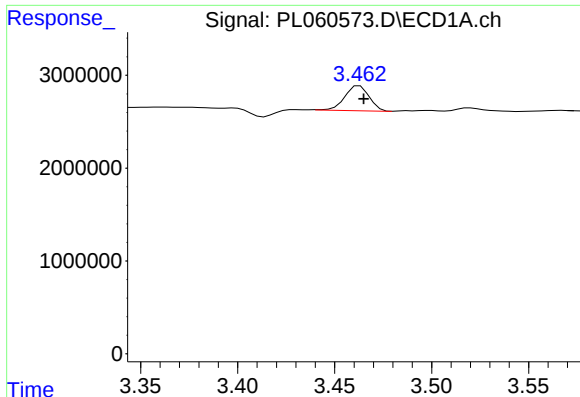


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: -0.003 min
Response: 2363364
Conc: 1.19 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-04-080620


Manual Integrations
APPROVED

Ankita
8/10/2020 1:04:44 PM

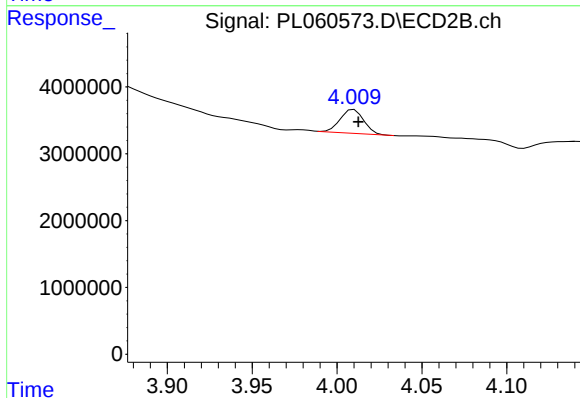


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: -0.004 min
Response: 3461757
Conc: 1.32 ng/ml m

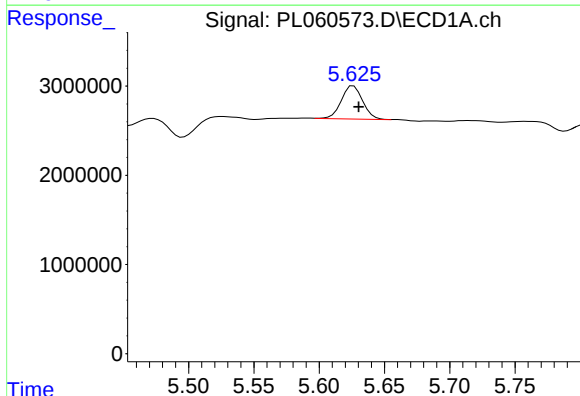


#12 4,4'-DDE

R.T.: 5.625 min
Delta R.T.: -0.005 min
Response: 4264744
Conc: 2.53 ng/ml m

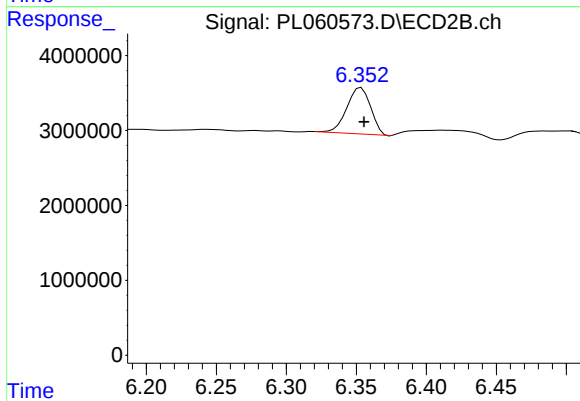

#12 4,4'-DDE

R.T.: 6.353 min
Delta R.T.: -0.002 min
Response: 7318693
Conc: 2.77 ng/ml m

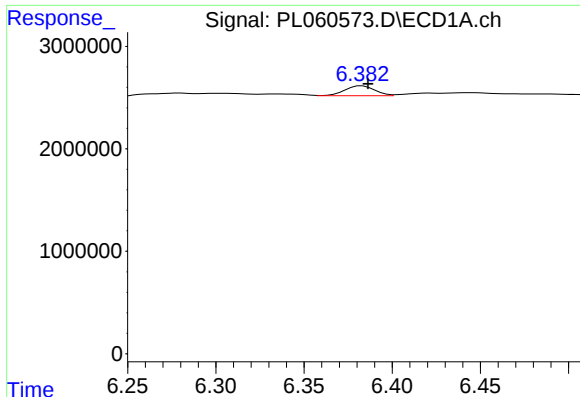


#17 4,4'-DDT

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 1147008
Conc: 0.84 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-04-080620


Manual Integrations
APPROVED

Ankita
8/10/2020 1:04:44 PM

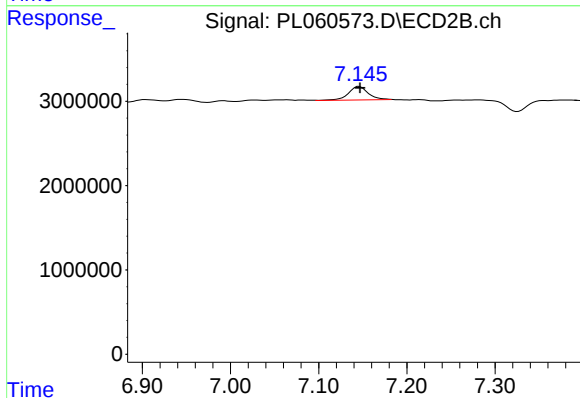


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.002 min
Response: 2521465
Conc: 1.25 ng/ml m

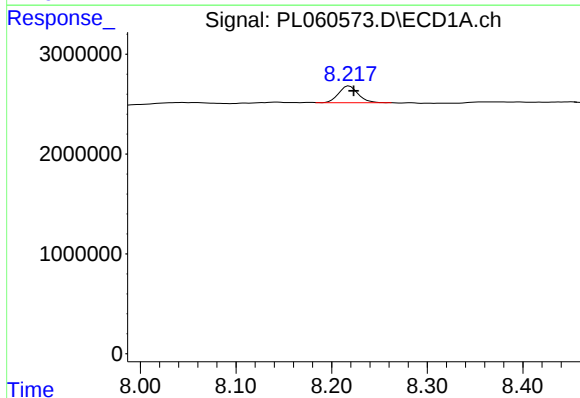

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: -0.006 min
Response: 2380958
Conc: 1.56 ng/ml m

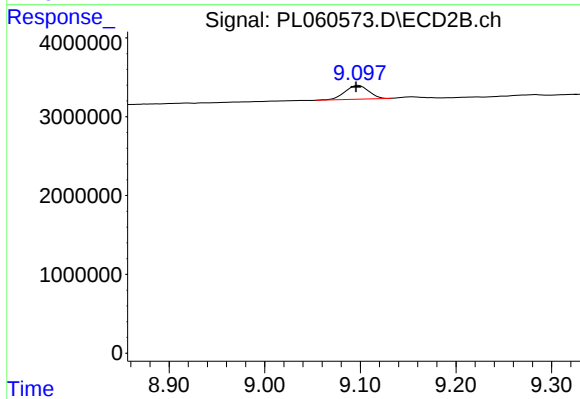

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.001 min
Response: 3013508
Conc: 1.68 ng/ml m