

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080725\
 Data File : PL096741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Aug 2025 12:13
 Operator : AR\AJ
 Sample : Q2774-13 DL2 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 254DL2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 22:40:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
9) A	Endosulfan I	0.000	5.175	0	4282051	N.D.	0.774 #
10) B	gamma-Chl...	5.912	5.048	17031908	8549084	4.476	1.454 #
11) B	alpha-Chl...	5.995	5.112	21777892	31309568	5.650	5.308
12) B	4,4'-DDE	6.163	5.301	9880335	25369176	3.077	4.601 #
14) MA	Endrin	0.000	5.716	0	11178203	N.D.	2.068 #
16) A	4,4'-DDD	6.671	5.853	7763053	7453269	3.070	1.584 #
17) MA	4,4'-DDT	6.984	6.106	137.1E6	263.7E6	47.817	52.132
25)	Chlordane-3	5.912	5.048	17031908	8549084	25.499	12.295 #
26)	Chlordane-4	5.995	5.112	21777892	31309568	26.311	50.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080725\
Data File : PL096741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Aug 2025 12:13
Operator : AR\AJ
Sample : Q2774-13 DL2 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
254DL2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 22:40:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

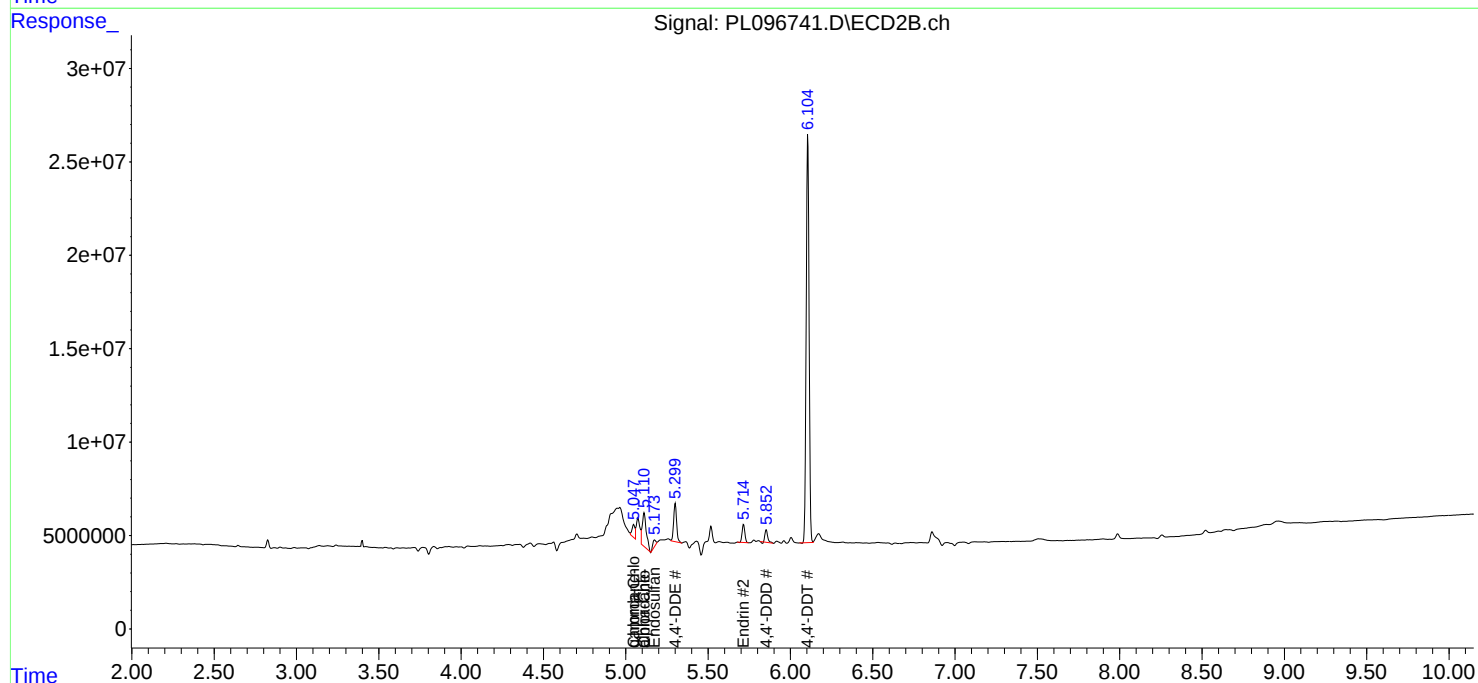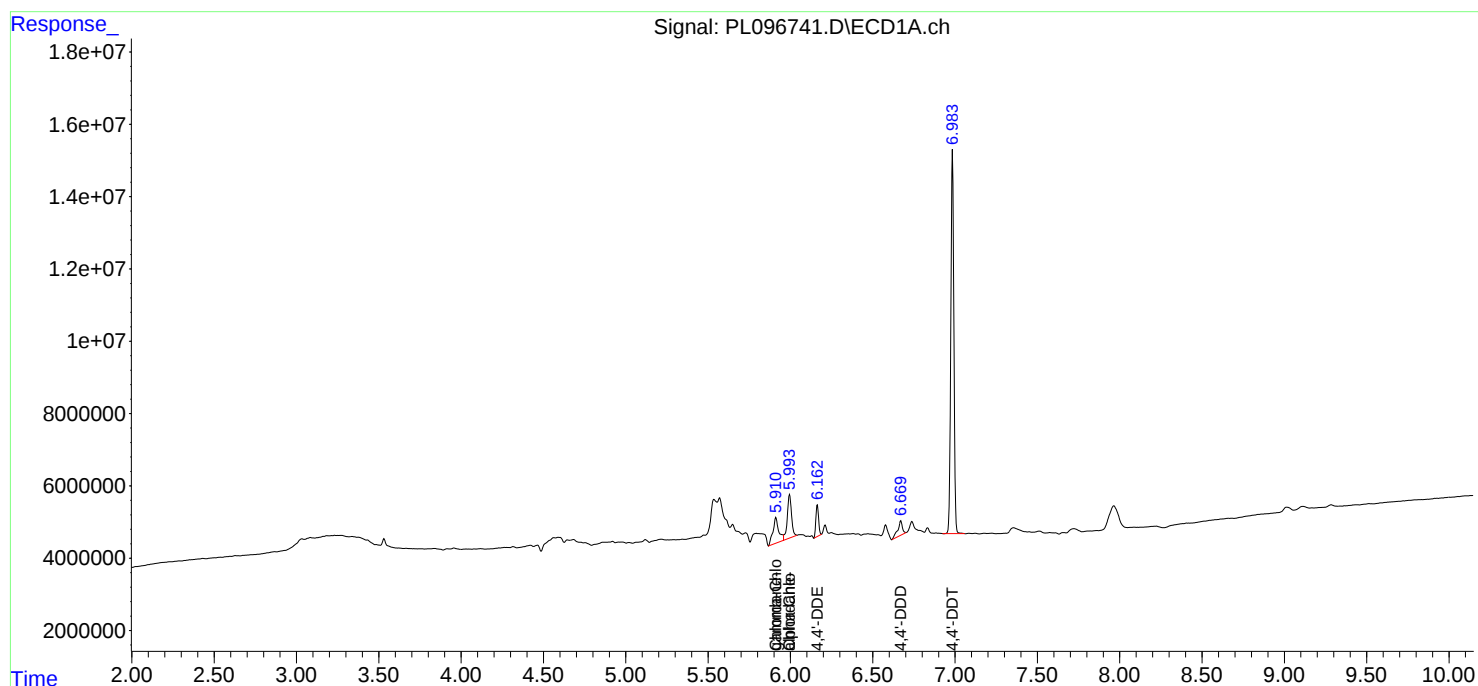


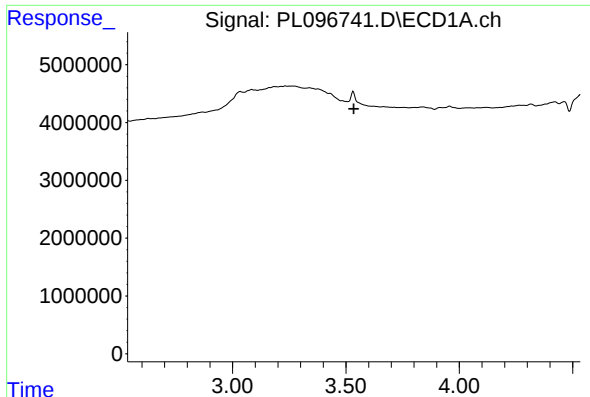

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
254DL2

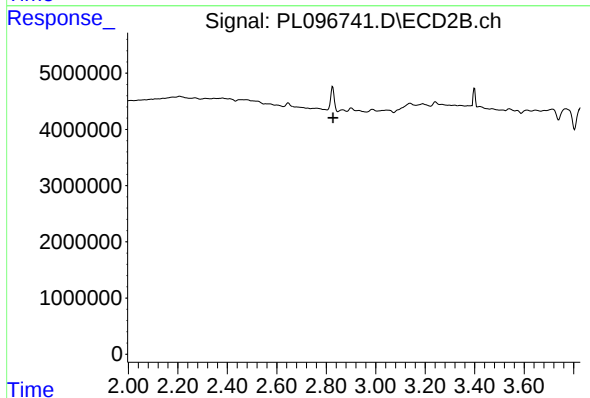


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.828 min
Response: 0
Conc: N.D.

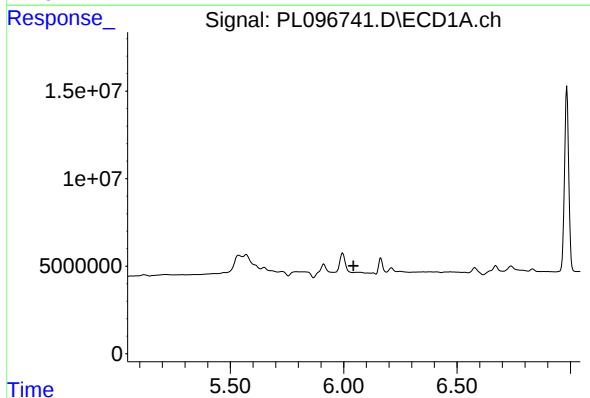


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.044 min
Response: 0
Conc: N.D.

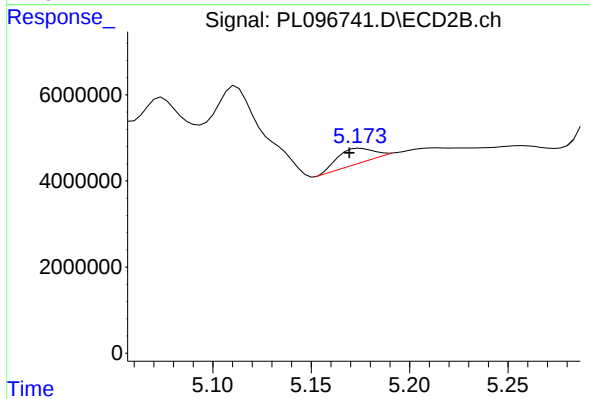

#9 Endosulfan I


R.T.: 5.175 min
Delta R.T.: 0.006 min
Response: 4282051
Conc: 0.77 ng/ml

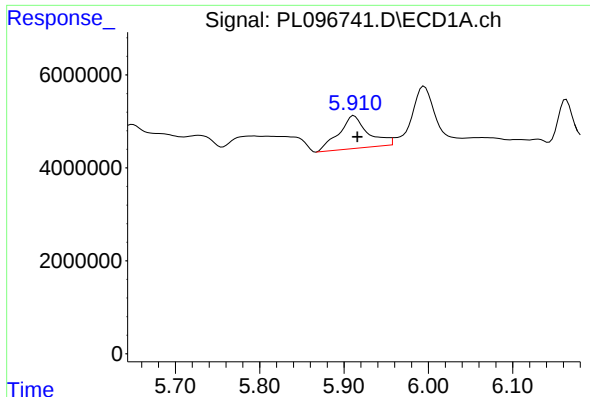

#10 gamma-Chlordane


R.T.: 5.912 min
Delta R.T.: -0.004 min
Response: 17031908
Conc: 4.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
254DL2

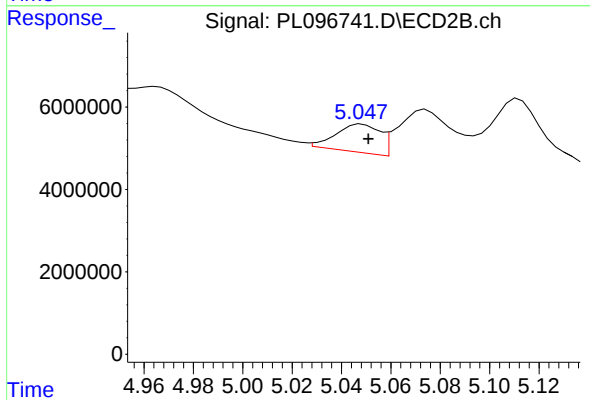


#10 gamma-Chlordane

R.T.: 5.048 min
Delta R.T.: -0.003 min
Response: 8549084
Conc: 1.45 ng/ml

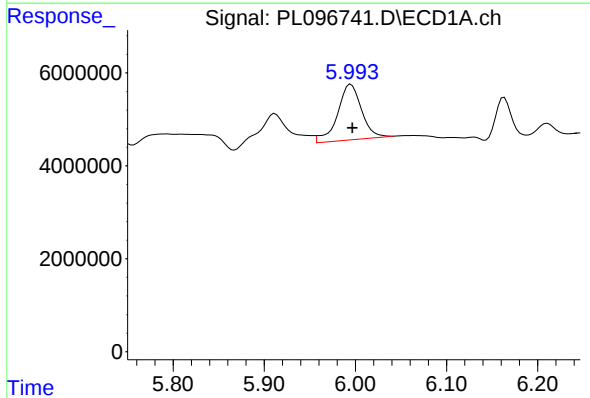


#11 alpha-Chlordane

R.T.: 5.995 min
Delta R.T.: -0.001 min
Response: 21777892
Conc: 5.65 ng/ml

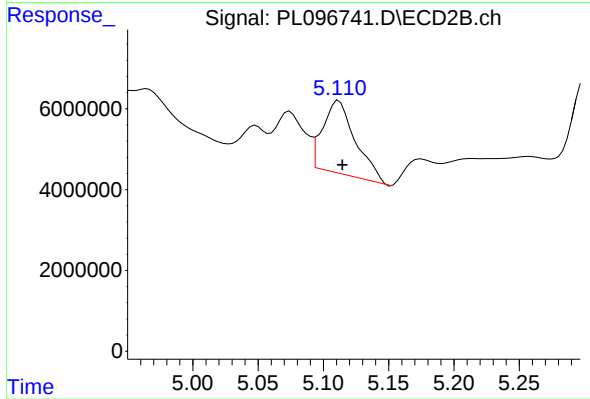

#11 alpha-Chlordane


R.T.: 5.112 min
Delta R.T.: -0.003 min
Response: 31309568
Conc: 5.31 ng/ml

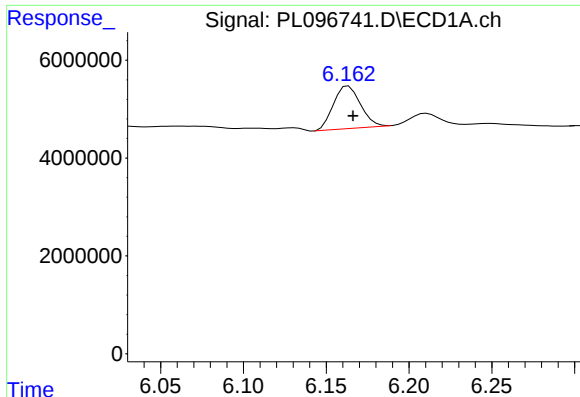

#12 4,4'-DDE


R.T.: 6.163 min
Delta R.T.: -0.003 min
Response: 9880335
Conc: 3.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
254DL2

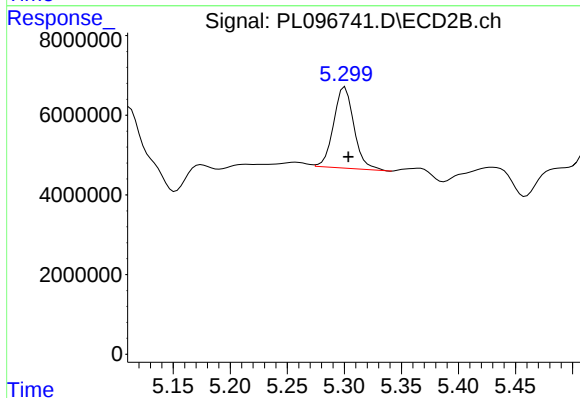


#12 4,4'-DDE

R.T.: 5.301 min
Delta R.T.: -0.003 min
Response: 25369176
Conc: 4.60 ng/ml

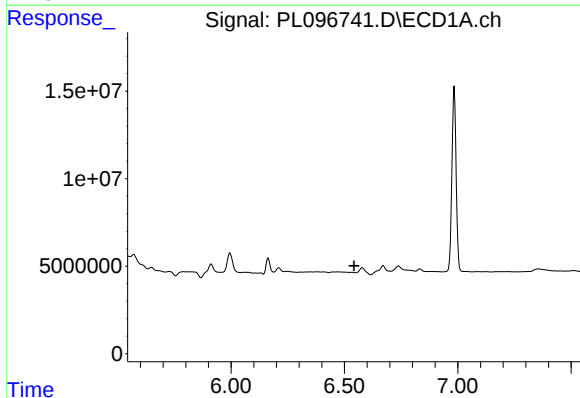


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

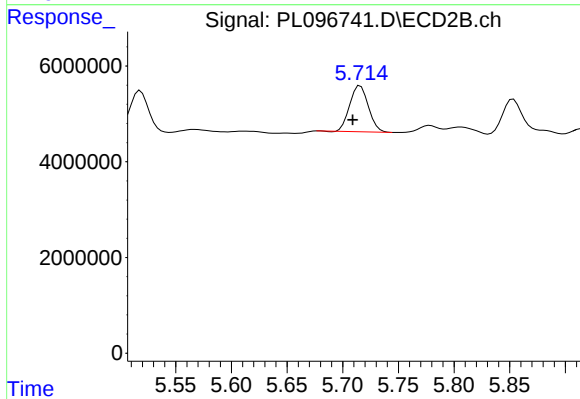

#14 Endrin


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 11178203
Conc: 2.07 ng/ml

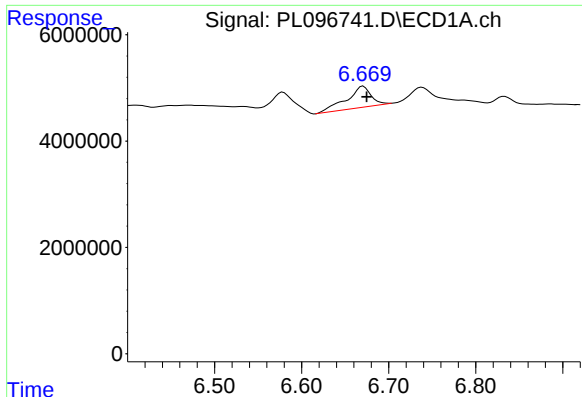

#16 4,4'-DDD


R.T.: 6.671 min
Delta R.T.: -0.004 min
Response: 7763053
Conc: 3.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
254DL2

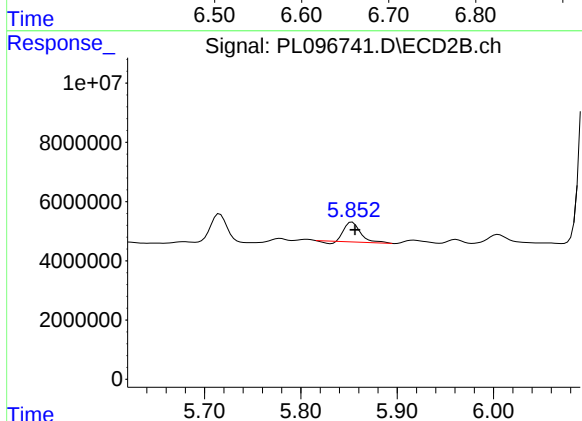


#16 4,4'-DDD

R.T.: 5.853 min
Delta R.T.: -0.003 min
Response: 7453269
Conc: 1.58 ng/ml

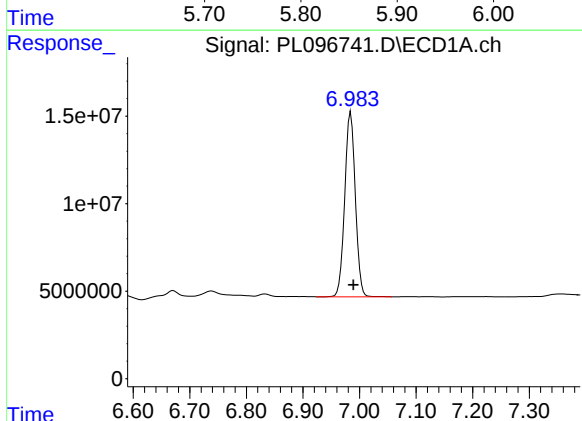


#17 4,4'-DDT

R.T.: 6.984 min
Delta R.T.: -0.005 min
Response: 137123432
Conc: 47.82 ng/ml

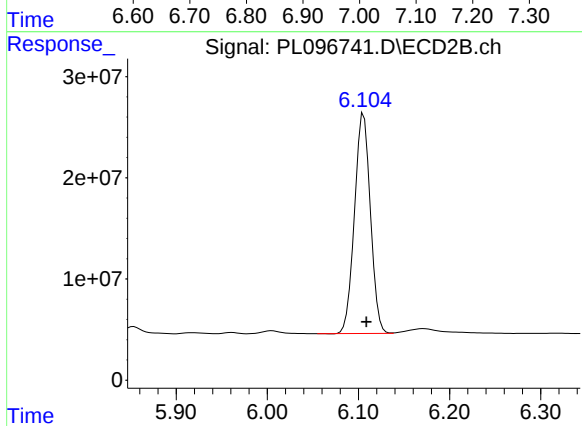

#17 4,4'-DDT


R.T.: 6.106 min
Delta R.T.: -0.003 min
Response: 263701148
Conc: 52.13 ng/ml

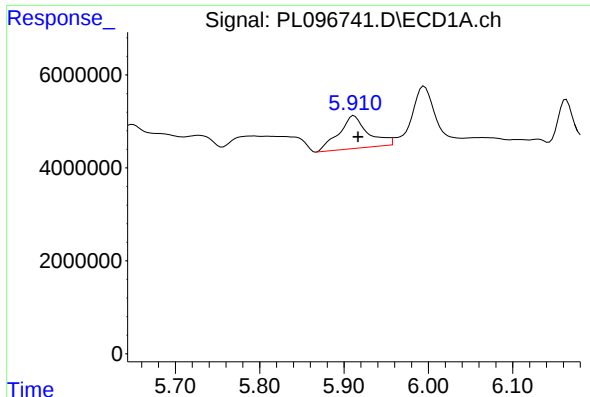

#25 Chlordane-3


R.T.: 5.912 min
Delta R.T.: -0.005 min
Response: 17031908
Conc: 25.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
254DL2

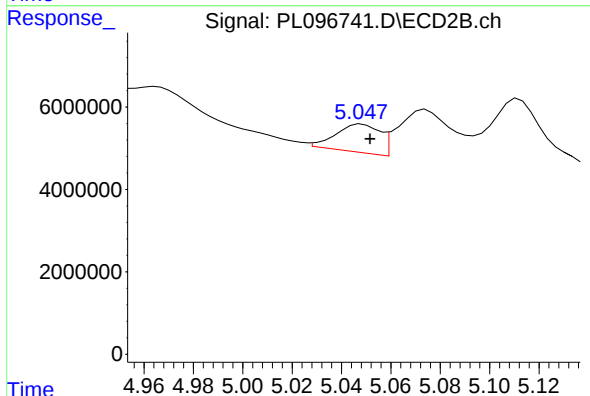


#25 Chlordane-3

R.T.: 5.048 min
Delta R.T.: -0.003 min
Response: 8549084
Conc: 12.30 ng/ml

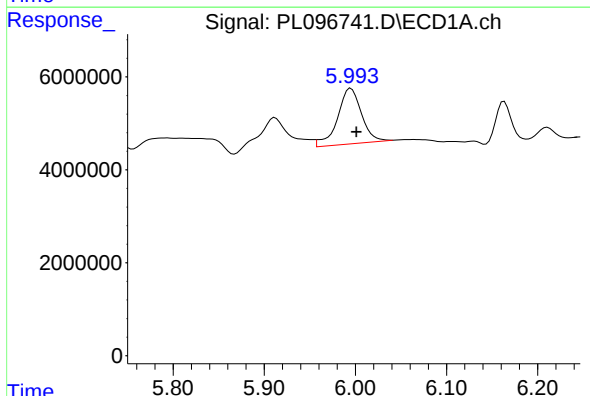


#26 Chlordane-4

R.T.: 5.995 min
Delta R.T.: -0.006 min
Response: 21777892
Conc: 26.31 ng/ml

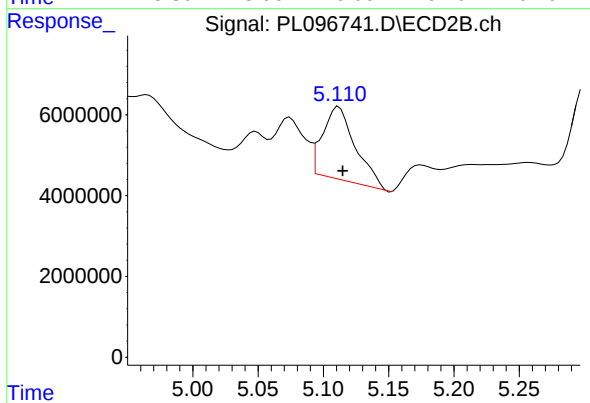

#26 Chlordane-4


R.T.: 5.112 min
Delta R.T.: -0.003 min
Response: 31309568
Conc: 50.31 ng/ml

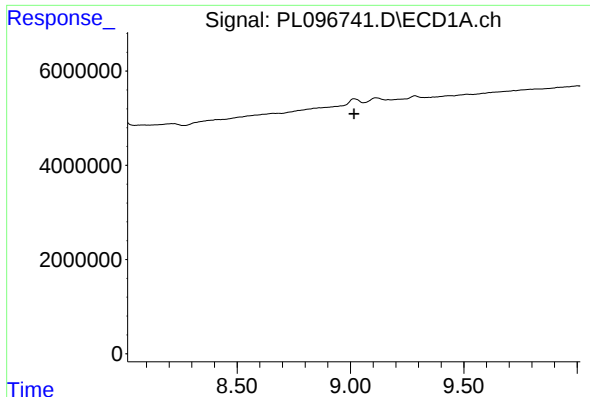

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.016 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
254DL2

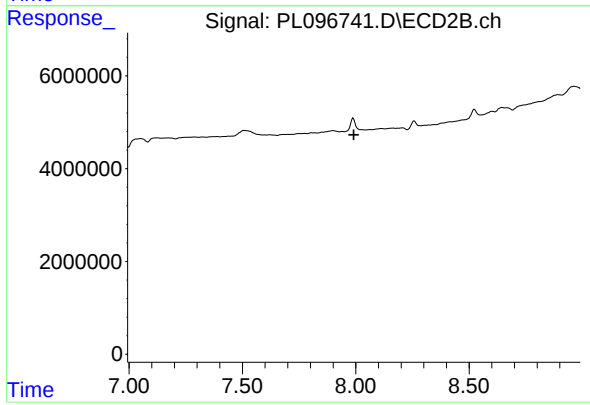

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.992 min
Response: 0
Conc: N.D.