


Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Quant Time: Aug 03 15:48:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

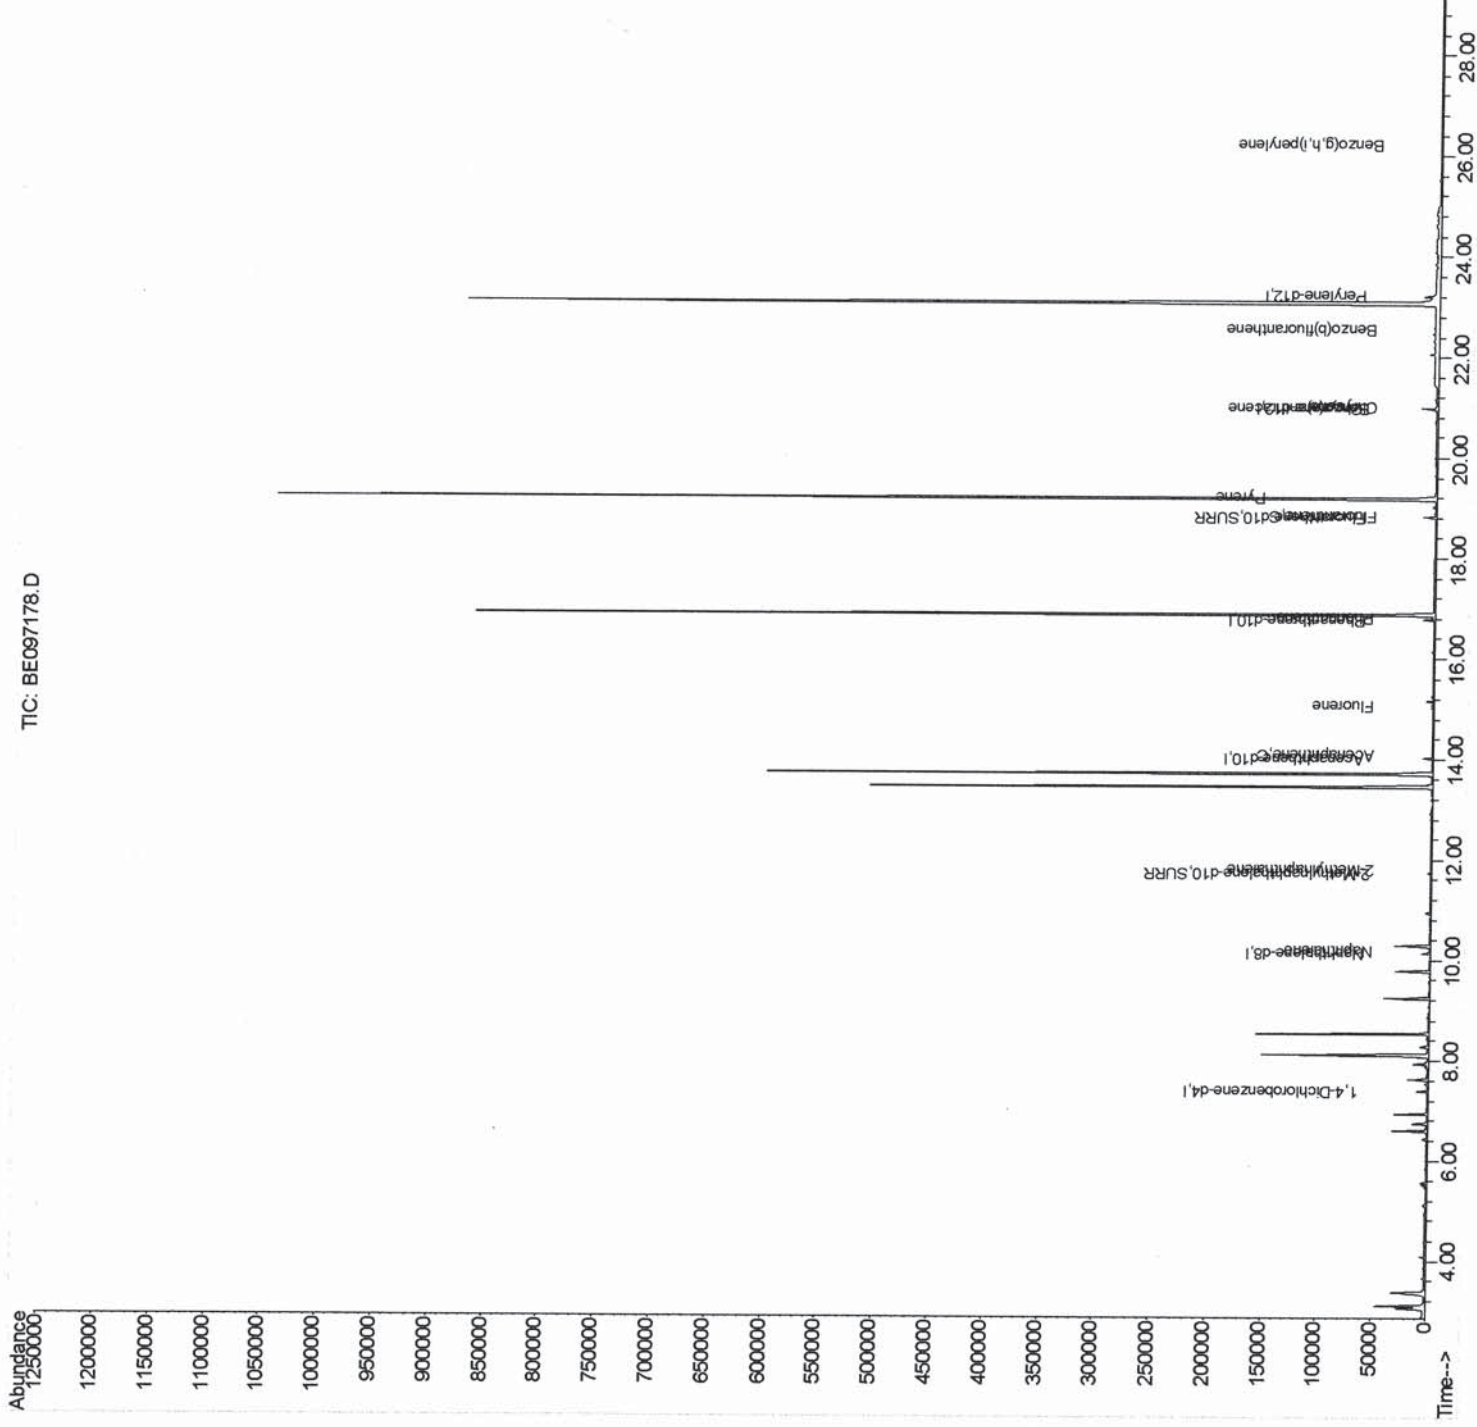

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 03 15:06:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

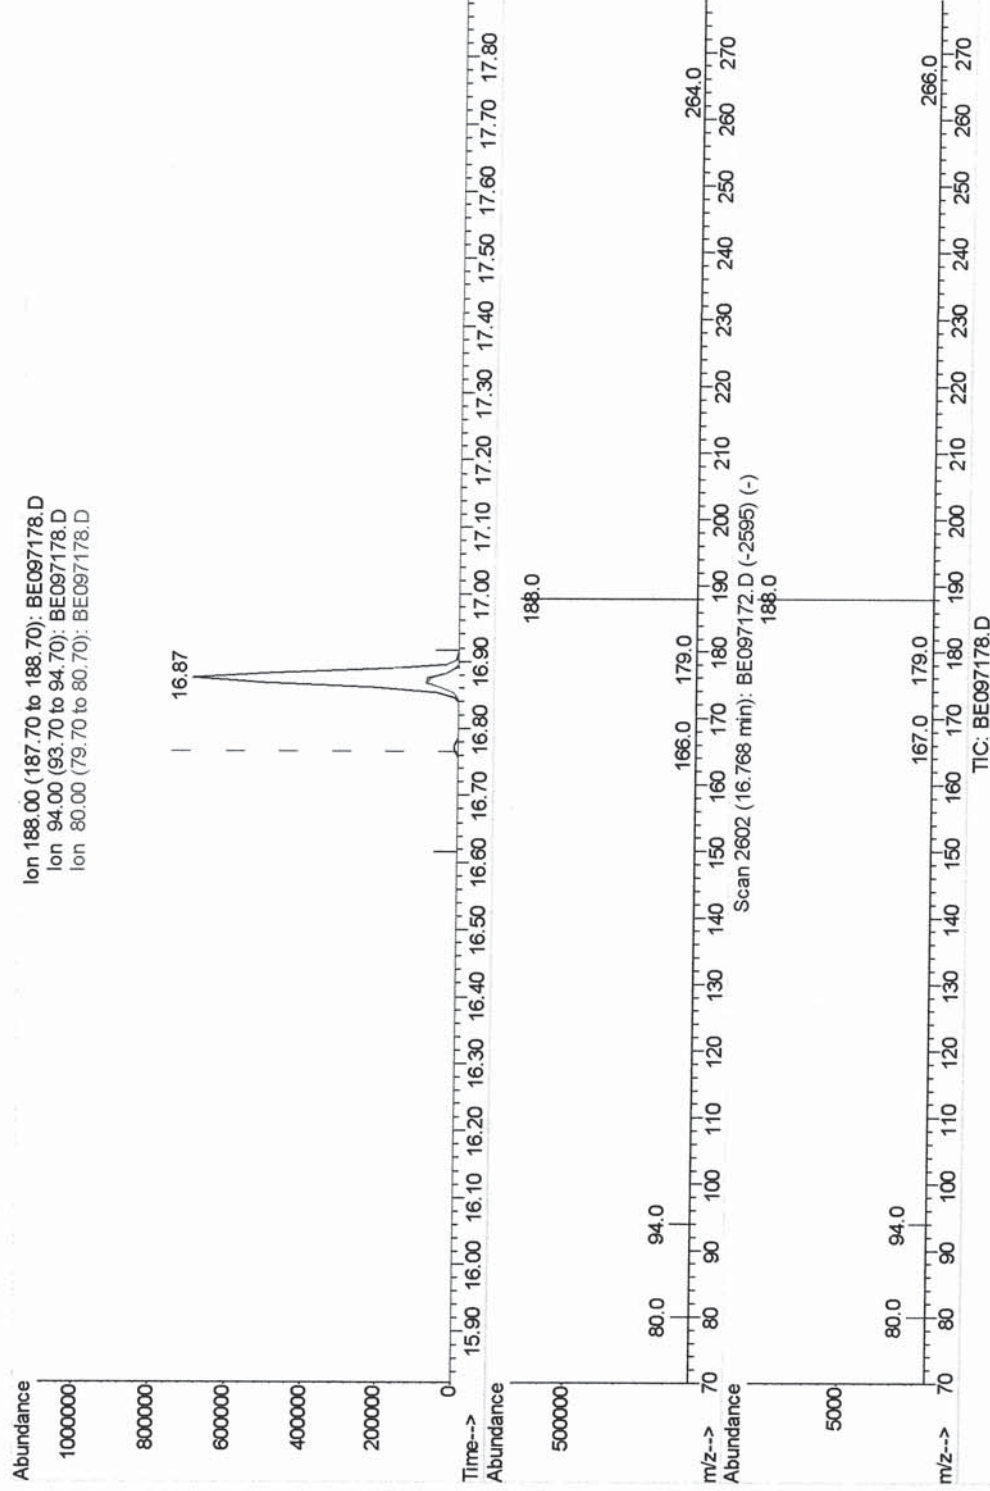

(10) Phenanthrene-d10 (l)
 16.874min (+0.105) 0.40ng/ul


response 919092

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.92
80.00	11.80	10.58
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 03 15:06:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

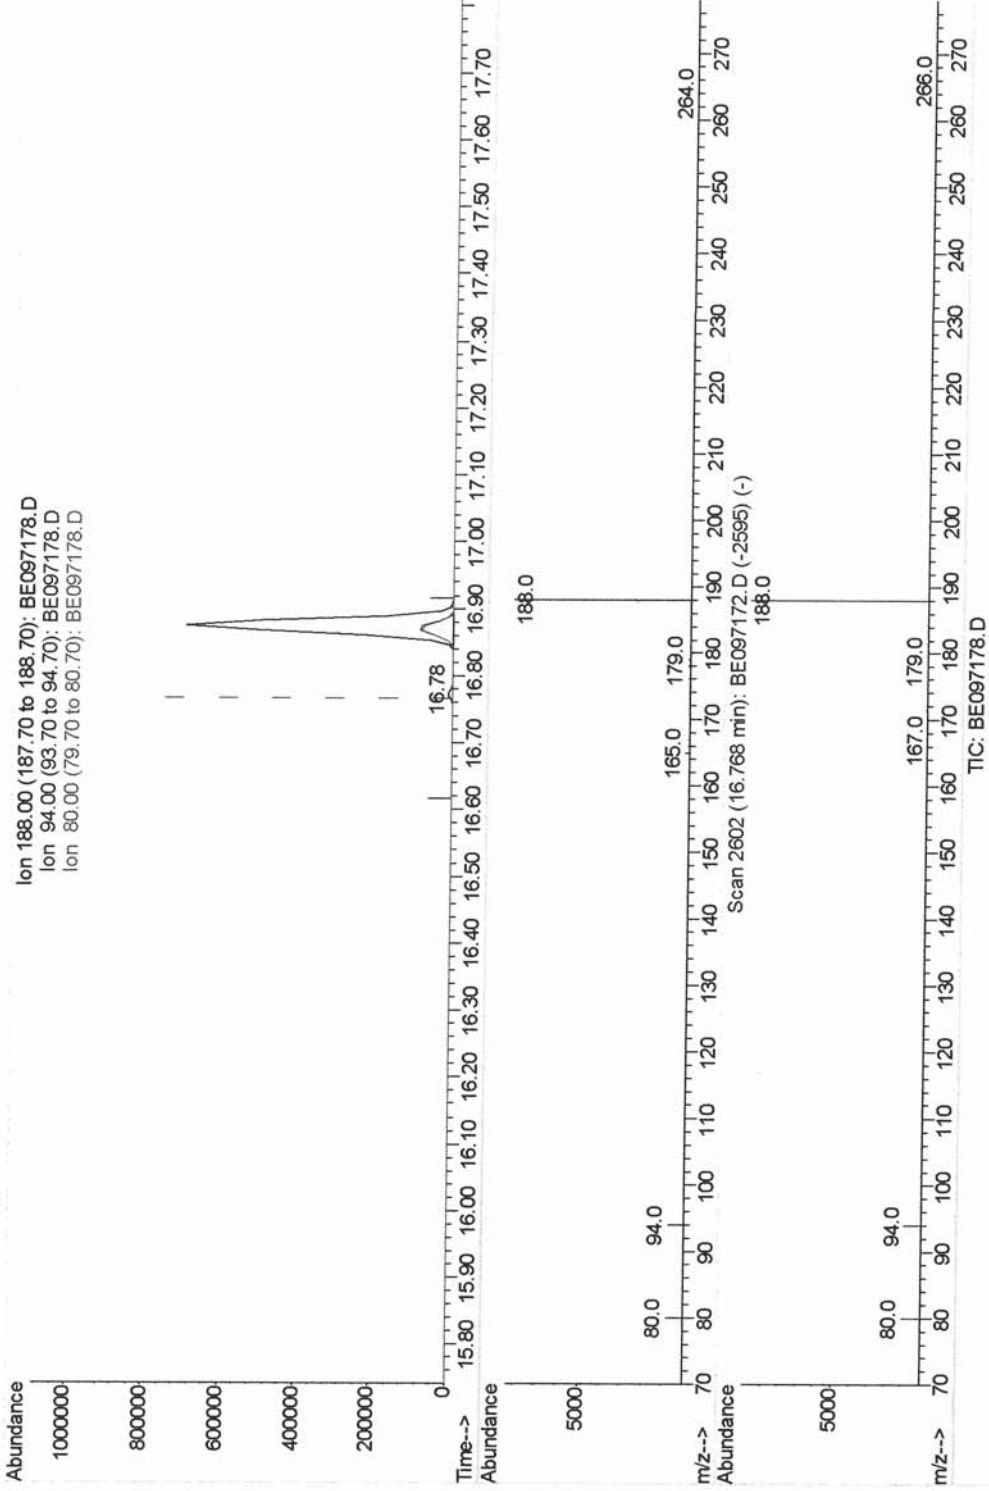

(10) Phenanthrene-d10 (I)

16.775min (+0.006) 0.40ng/ul m


response 12037

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.81
80.00	11.80	10.43
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 03 15:39:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

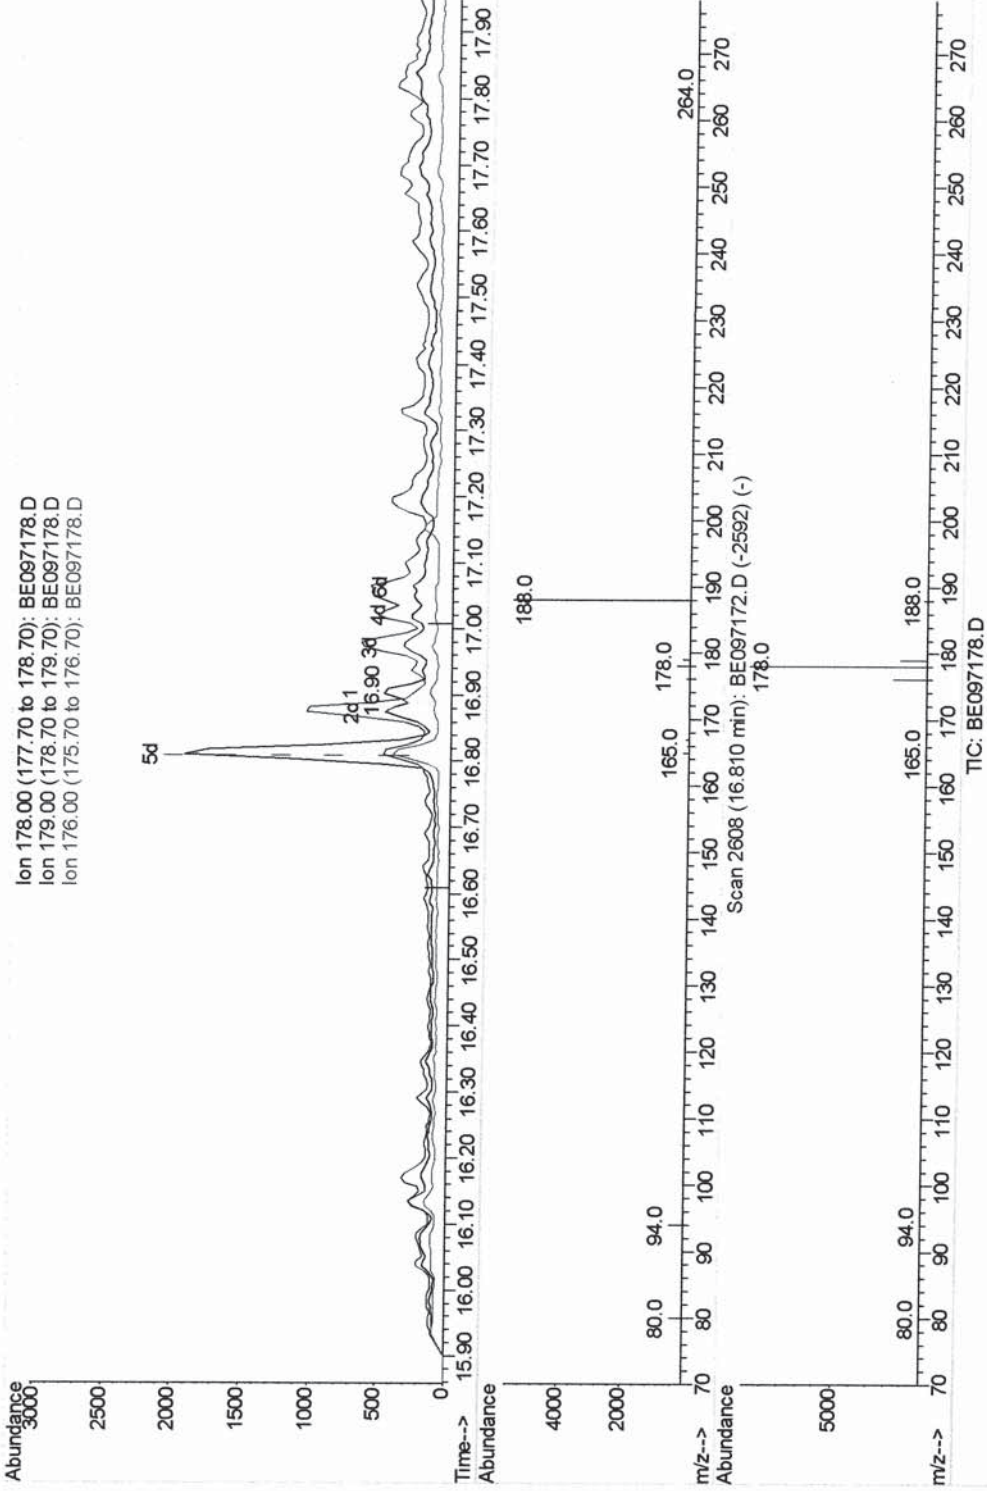

(12) Phenanthrene

16.902min (+0.091) 0.02ng/ul


response 499

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	56.59#
176.00	17.00	32.86#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 03 15:39:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

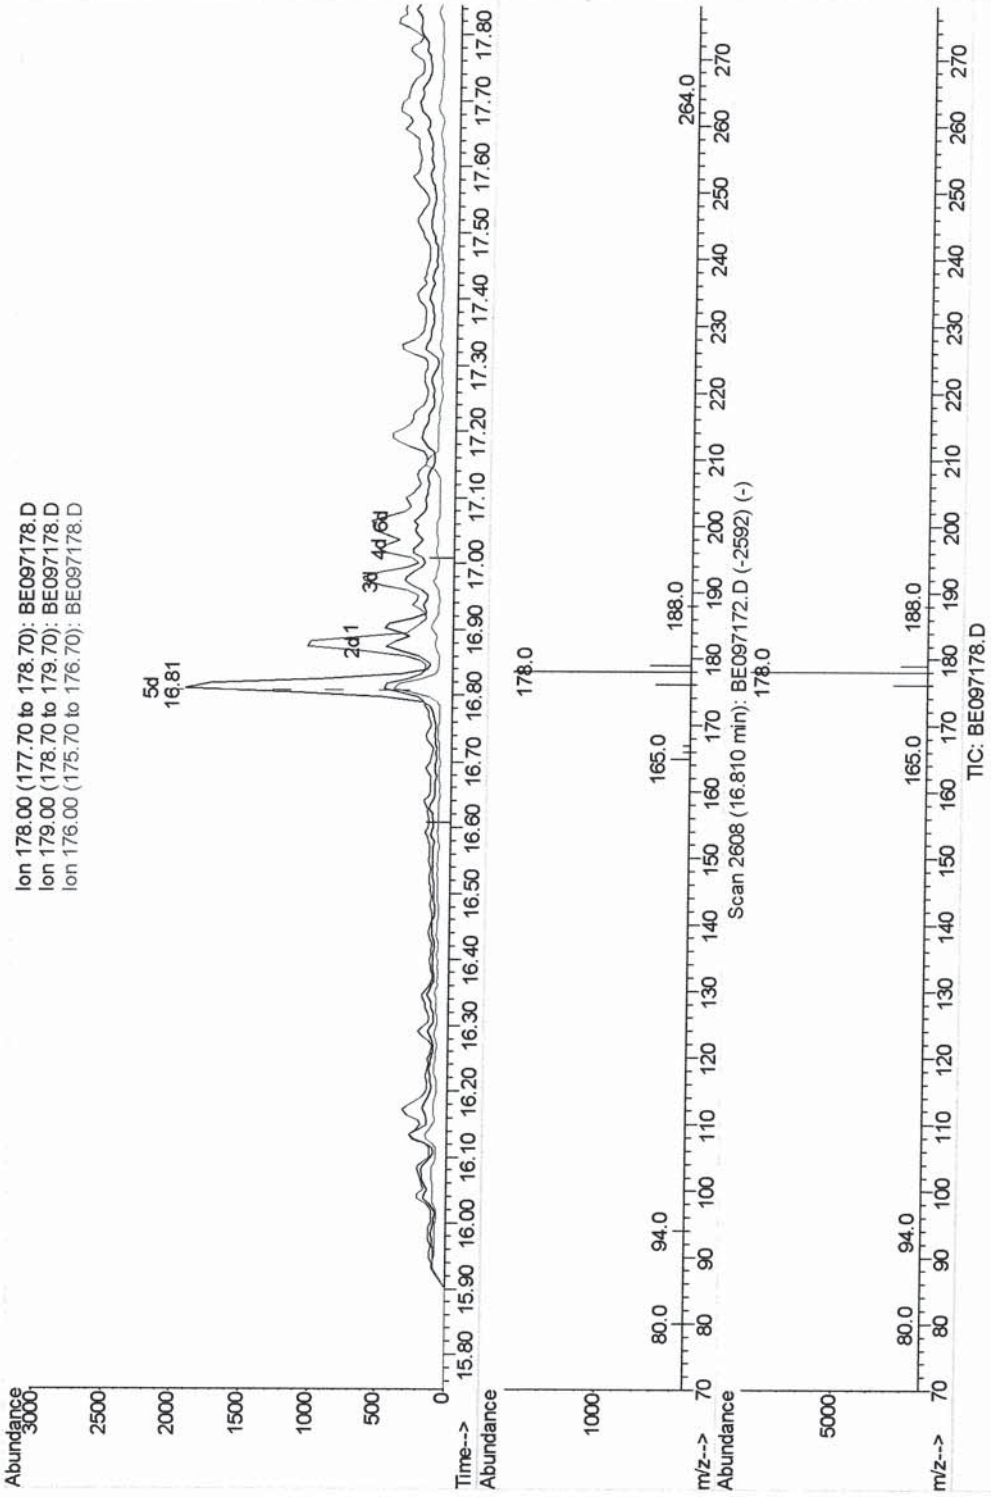

(12) Phenanthrene

16.810min (-0.001) 0.09ng/ul m


response 2699

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	25.39
176.00	17.00	21.78#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080318\
 Data File : BE097178.D
 Acq On : 3 Aug 2018 13:01
 Operator : SJ/JU
 Sample : J4172-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 03 15:39:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 11:26:05 2018
 Response via : Initial Calibration

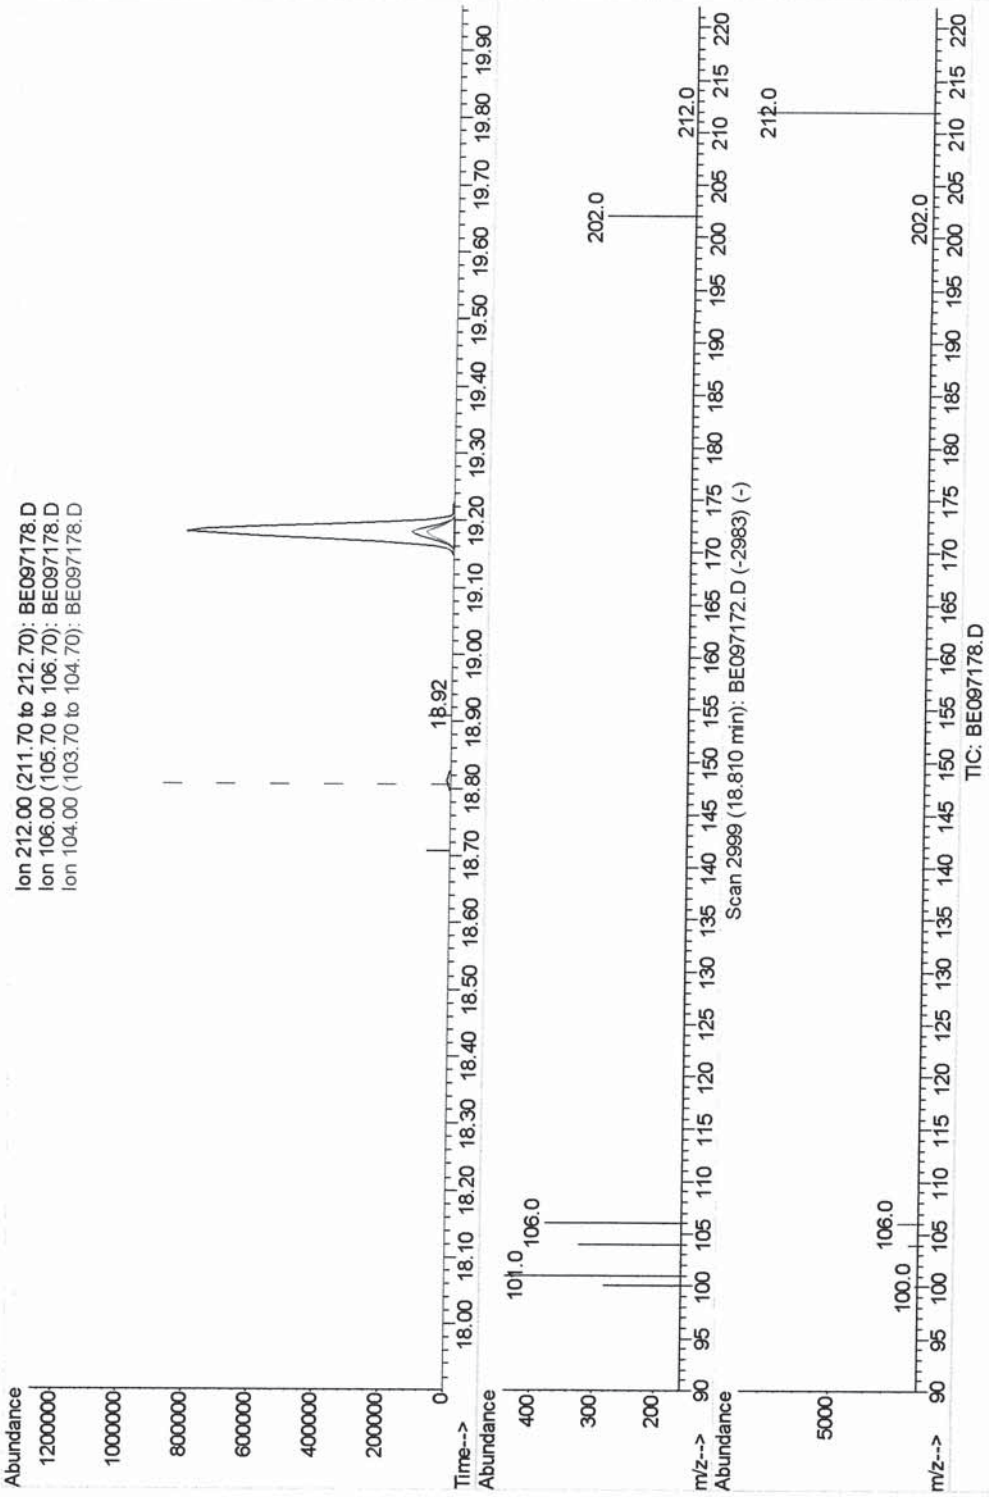

(14) Fluoranthene-d10 (SURR)

18.921min (+0.111) 0.00ng/ul

response 107

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	173.83#
104.00	15.60	316.82#
0.00	0.00	0.00

18.M

