

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 13:46
 Operator : AJ\SJ
 Sample : PB111851BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:51:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.331	3.926	142.9E6	55561211	19.186	21.167
28)	SA Decachlor...	7.999	8.937	144.3E6	54429775	19.026	22.267
Target Compounds							
3)	MA gamma-BHC...	0.000	4.624f	0	1686195	N.D.	0.467 #
6)	B beta-BHC	0.000	4.760	0	1851771	N.D.	1.221 #
7)	B delta-BHC	0.000	4.956	0	1020521	N.D.	0.308 #
8)	B Heptachlo...	0.000	5.796	0	3252889	N.D.	1.145 #
14)	MA Endrin	0.000	6.658f	0	1609897	N.D.	0.674 #
15)	B Endosulfa...	0.000	6.826	0	1167360	N.D.	0.486 #
16)	A 4,4'-DDD	0.000	6.658f	0	1609897	N.D.	0.752 #
23)	Chlordane-1	4.108	4.956	13895883	1020521	40.132	8.806 #
27)	Chlordane-5	0.000	6.826	0	1167360	N.D.	13.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 13:46
Operator : AJ\SJ
Sample : PB111851BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:51:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

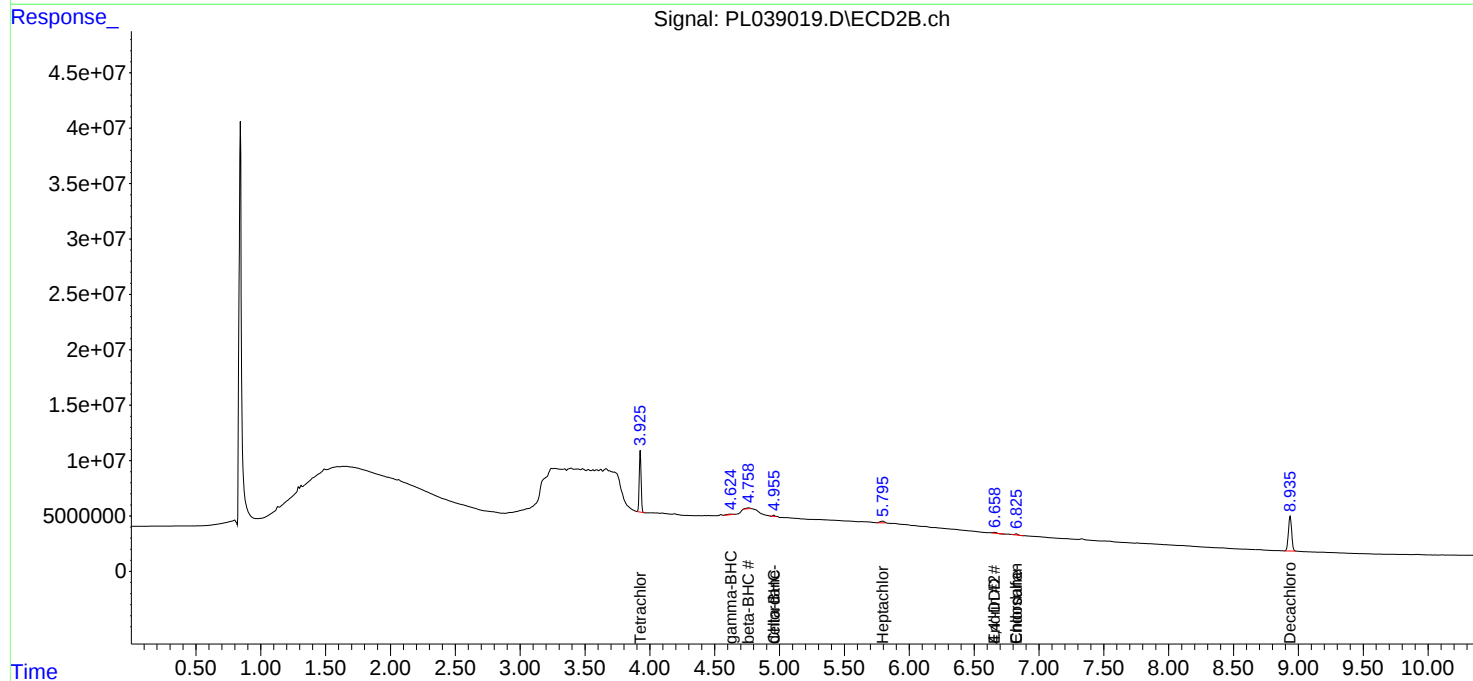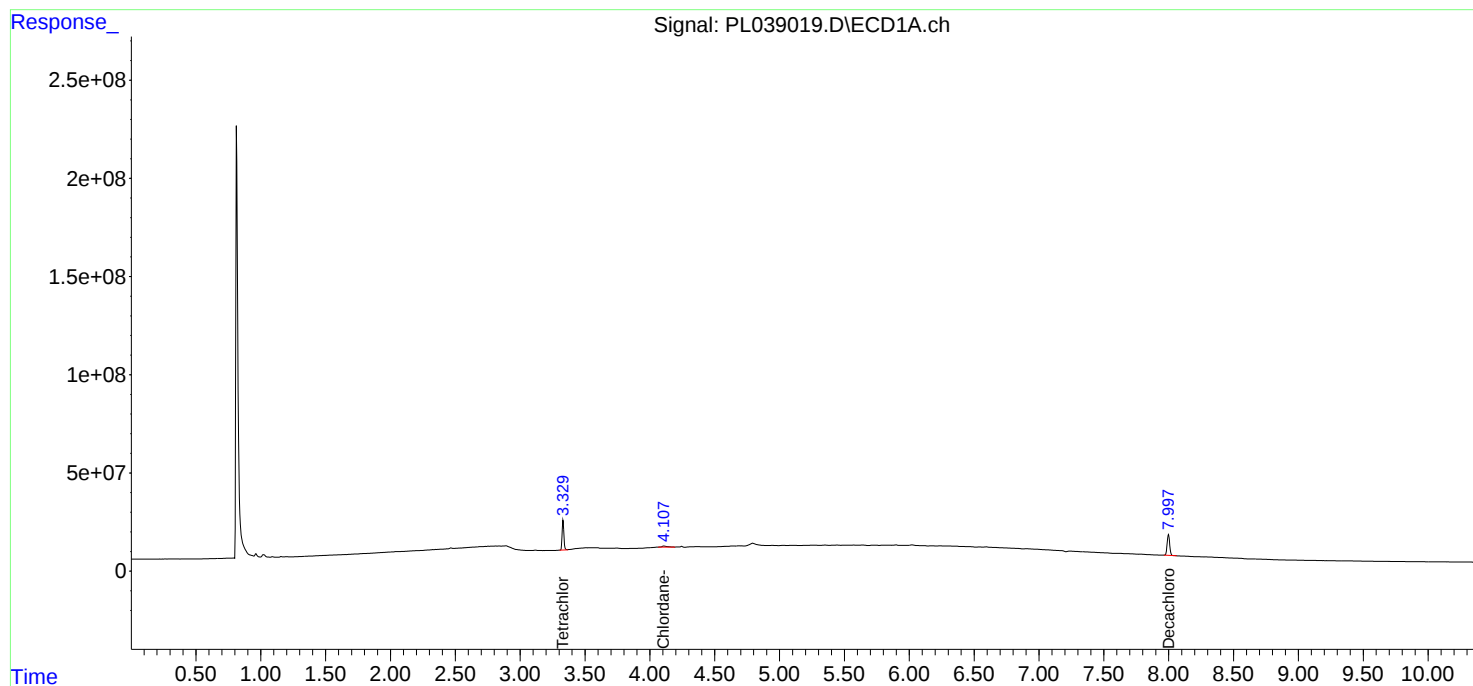


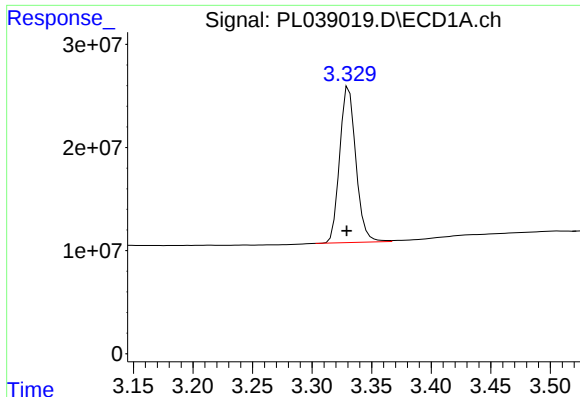

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: 0.002 min
Response: 142867800
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

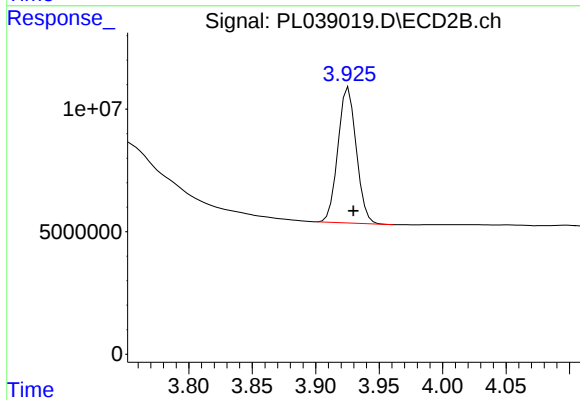


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 55561211
Conc: 21.17 ng/ml

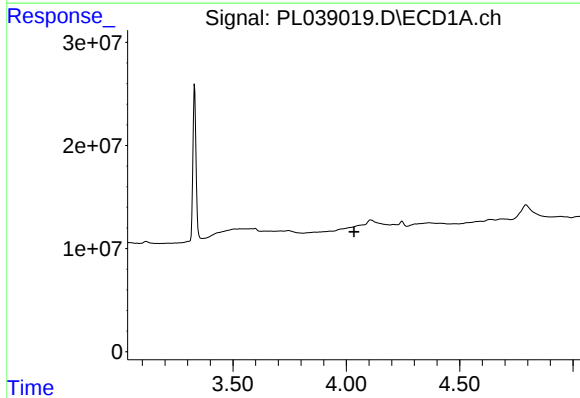


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

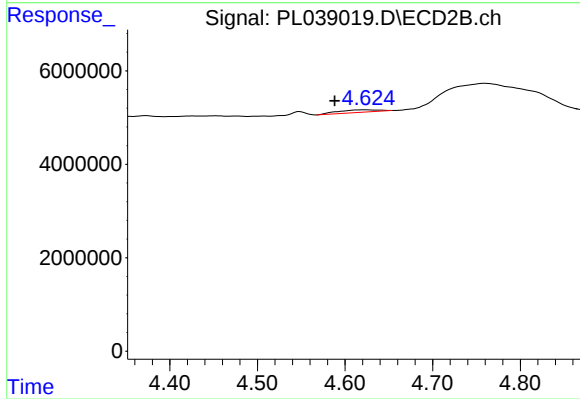

#3 gamma-BHC (Lindane)


R.T.: 4.624 min
Delta R.T.: 0.036 min
Response: 1686195
Conc: 0.47 ng/ml

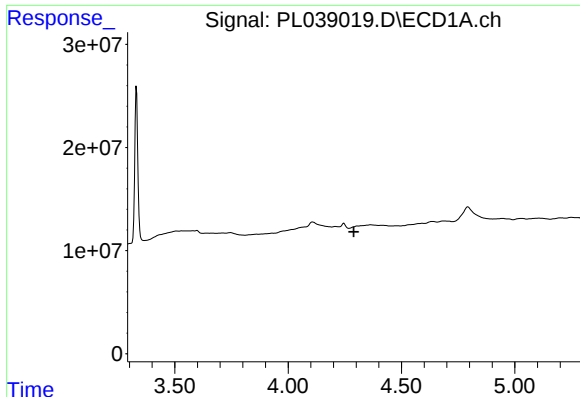

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

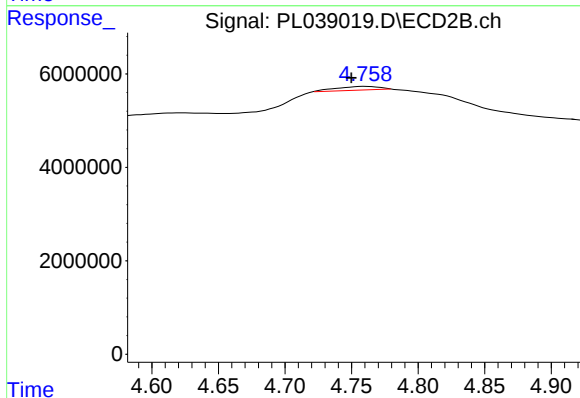


#6 beta-BHC

R.T.: 4.760 min
Delta R.T.: 0.010 min
Response: 1851771
Conc: 1.22 ng/ml

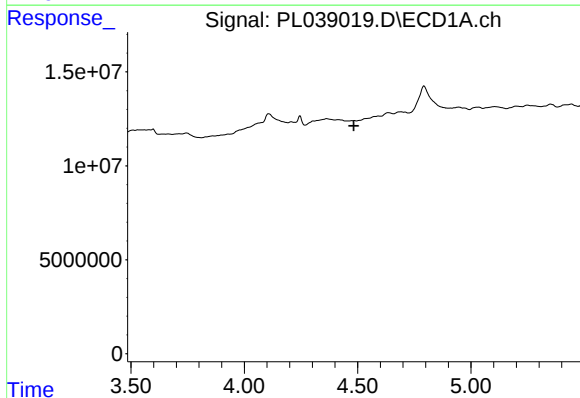


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

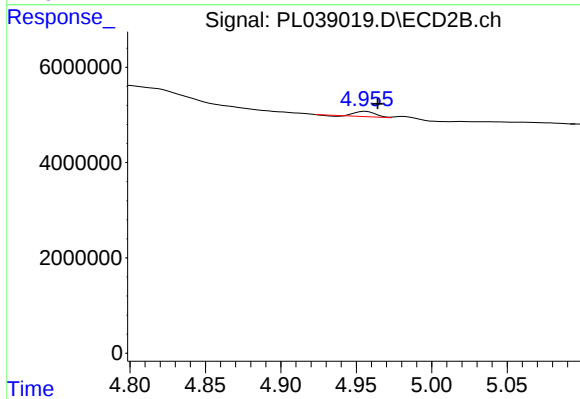

#7 delta-BHC


R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 1020521
Conc: 0.31 ng/ml

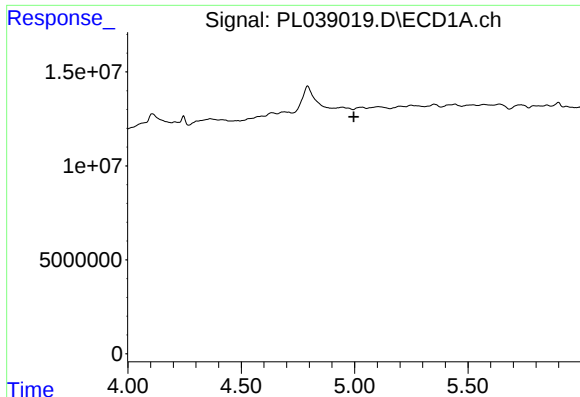

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

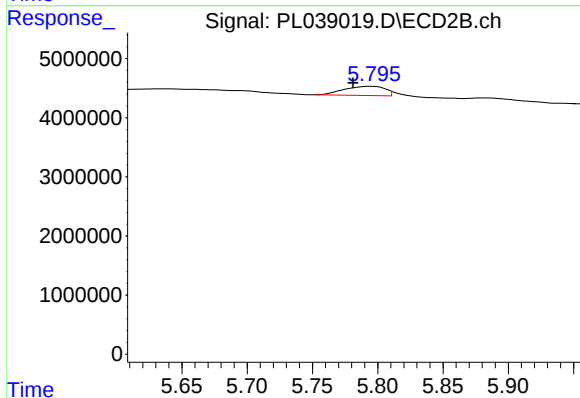


#8 Heptachlor epoxide

R.T.: 5.796 min
Delta R.T.: 0.015 min
Response: 3252889
Conc: 1.14 ng/ml

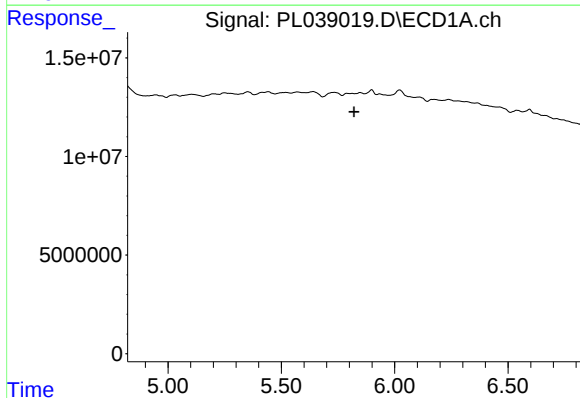


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.821 min
Response: 0
Conc: N.D.

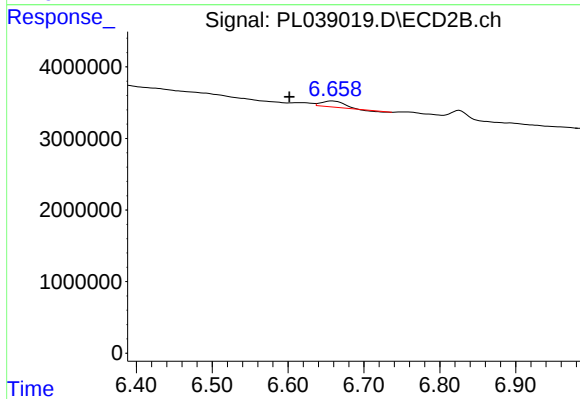

#14 Endrin


R.T.: 6.658 min
Delta R.T.: 0.056 min
Response: 1609897
Conc: 0.67 ng/ml

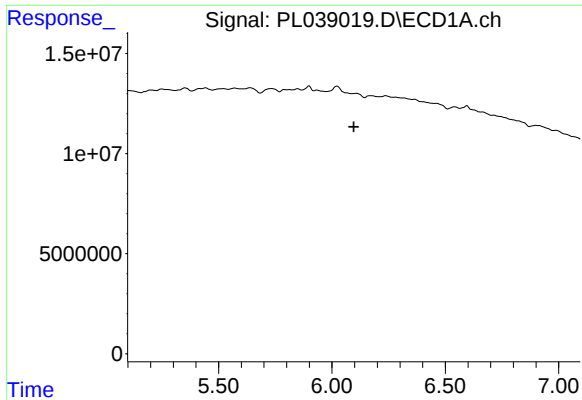

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

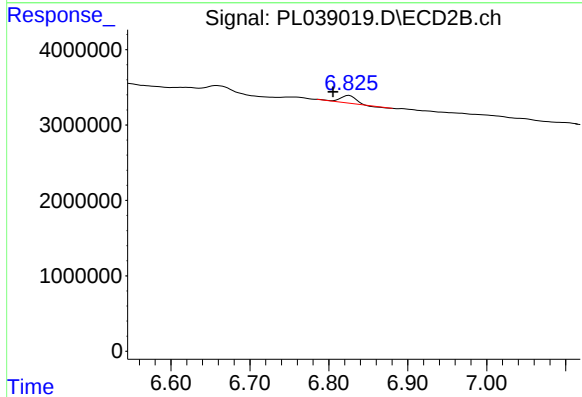


#15 Endosulfan II

R.T.: 6.826 min
Delta R.T.: 0.020 min
Response: 1167360
Conc: 0.49 ng/ml

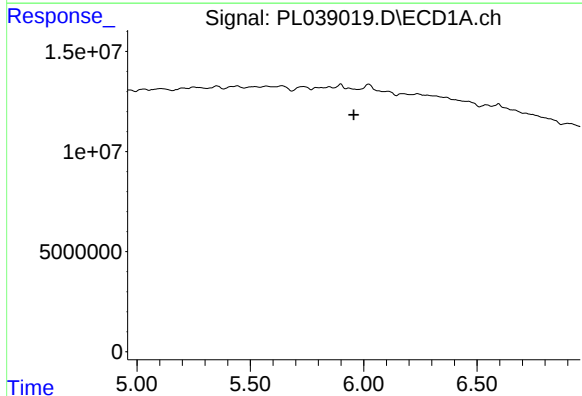


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

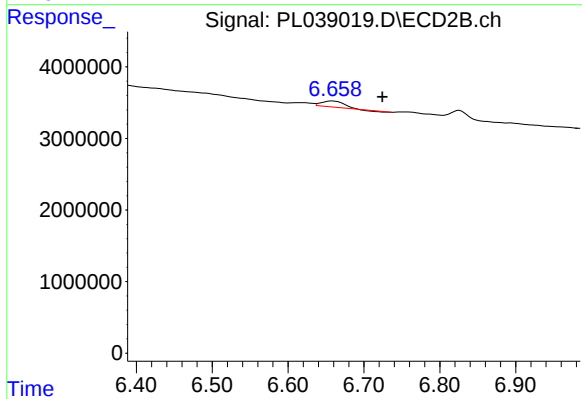

#16 4,4'-DDD


R.T.: 6.658 min
Delta R.T.: -0.067 min
Response: 1609897
Conc: 0.75 ng/ml

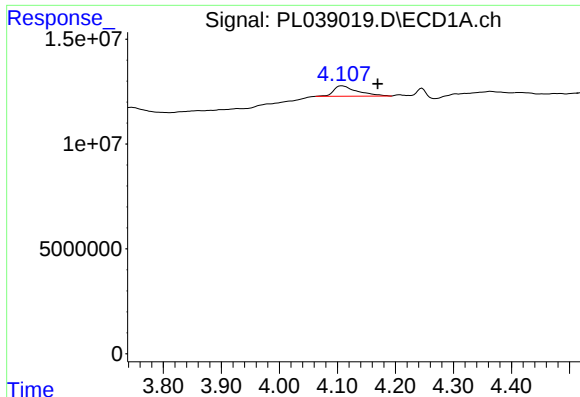

#23 Chlordane-1


R.T.: 4.108 min
Delta R.T.: -0.061 min
Response: 13895883
Conc: 40.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

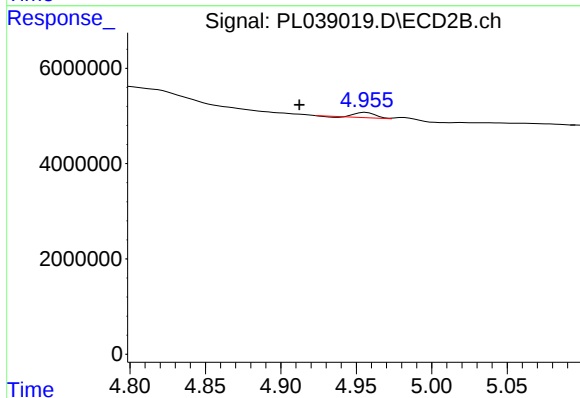


#23 Chlordane-1

R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 1020521
Conc: 8.81 ng/ml

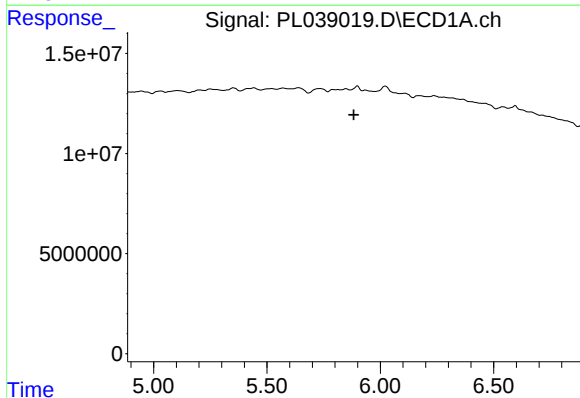


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

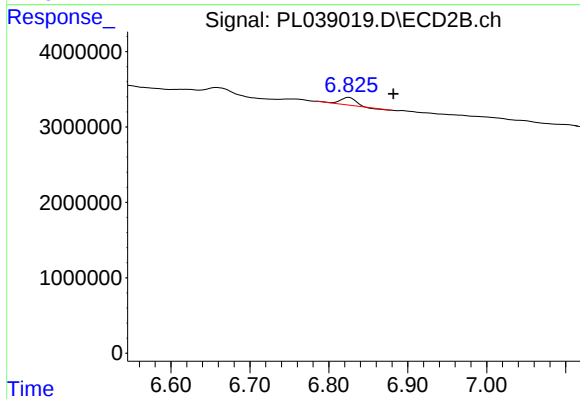

#27 Chlordane-5


R.T.: 6.826 min
Delta R.T.: -0.056 min
Response: 1167360
Conc: 13.03 ng/ml

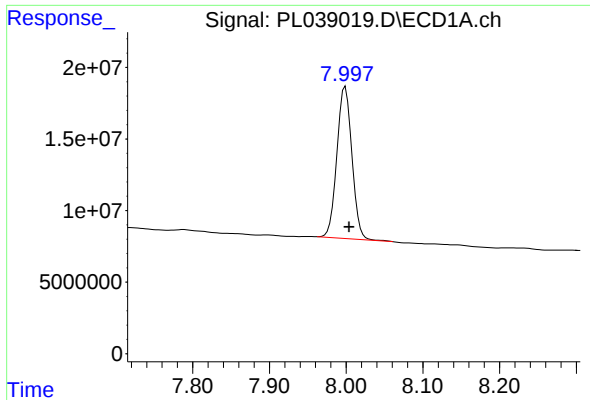

#28 Decachlorobiphenyl

R.T.: 7.999 min
Delta R.T.: -0.005 min
Response: 144327157
Conc: 19.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

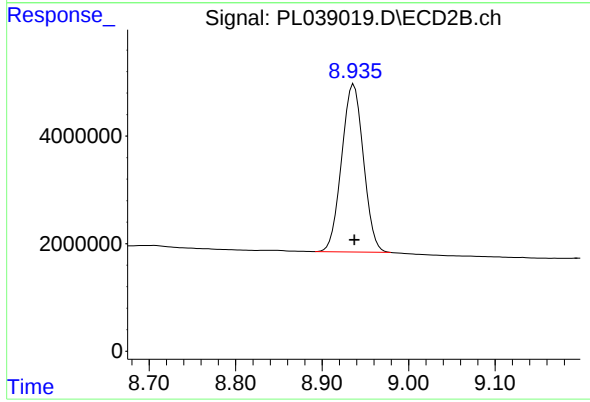

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 54429775
Conc: 22.27 ng/ml