

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 18:18
 Operator : AJ\SJ
 Sample : J4275-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:07:39 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	161.8E6	66372297	21.735	25.285
28)	SA Decachlor...	7.990	8.935	142.7E6	56042197	18.805	22.926
Target Compounds							
2)	A alpha-BHC	0.000	4.276f	0	2779438	N.D.	0.718 #
3)	MA gamma-BHC...	0.000	4.548f	0	2935564	N.D.	0.813 #
7)	B delta-BHC	0.000	4.957	0	7840016	N.D.	2.364 #
8)	B Heptachlo...	0.000	5.801	0	306778	N.D.	0.108 #
15)	B Endosulfa...	0.000	6.829	0	541280	N.D.	0.225 #
20)	A Methoxychlor	0.000	7.475	0	214615	N.D.	0.188 #
23)	Chlordane-1	4.238	4.918	22023084	24098	63.604	0.208 #
27)	Chlordane-5	0.000	6.829	0	541280	N.D.	6.042 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 18:18
Operator : AJ\SJ
Sample : J4275-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:07:39 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

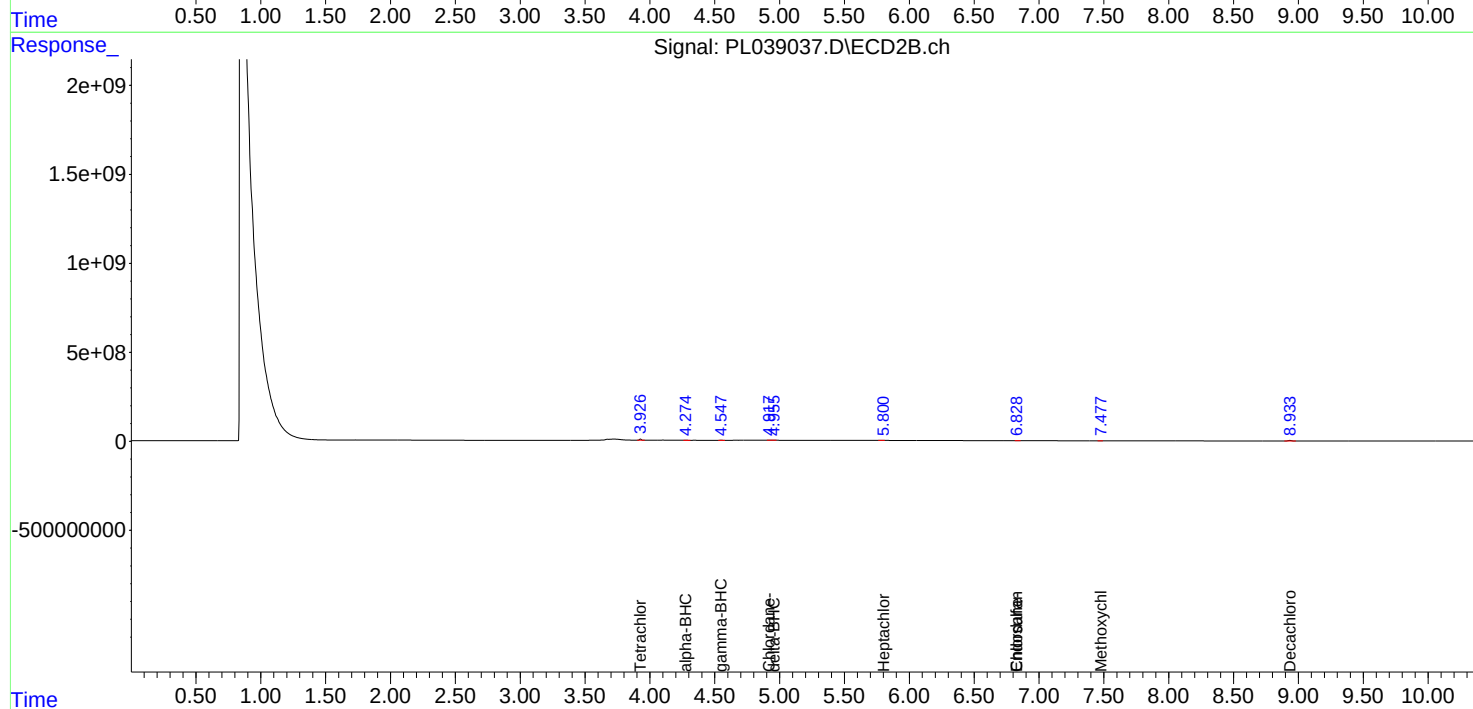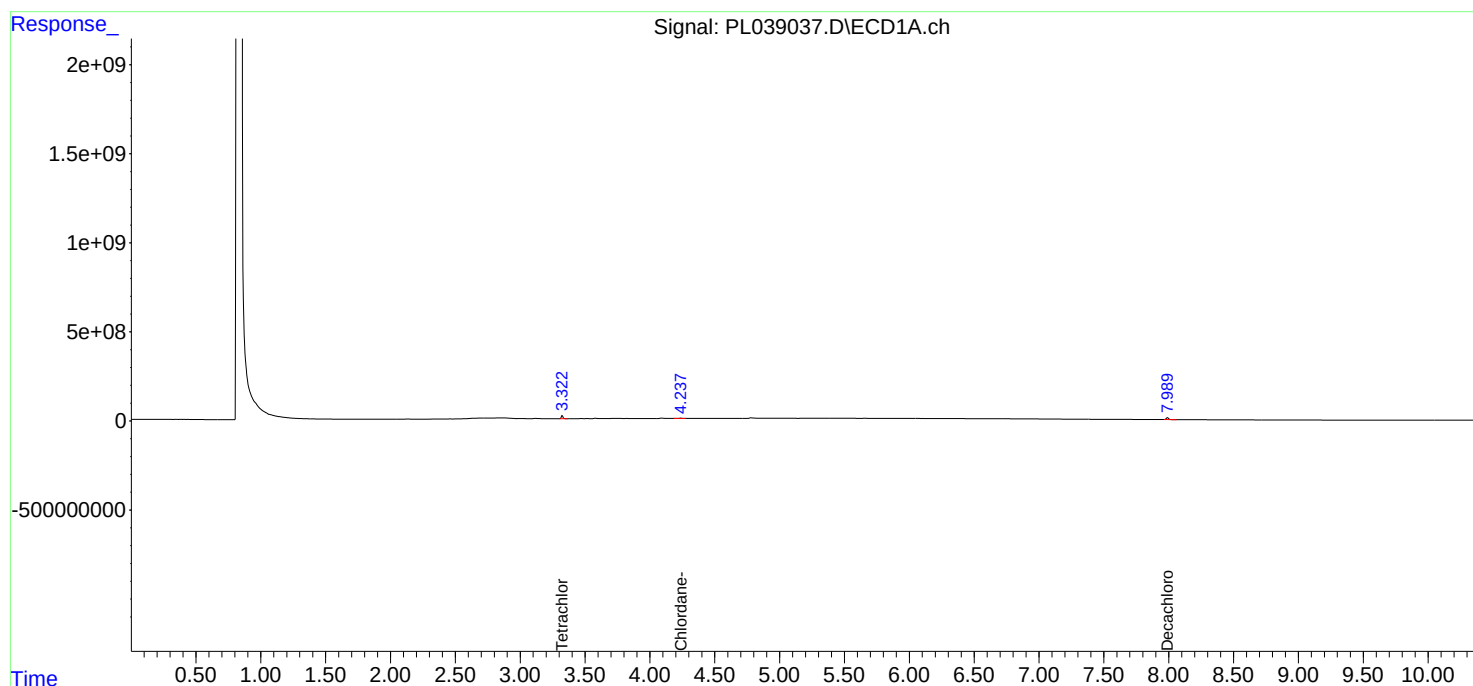


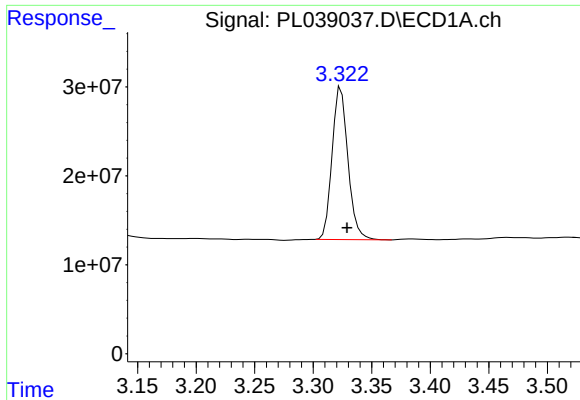

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 161845498
Conc: 21.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

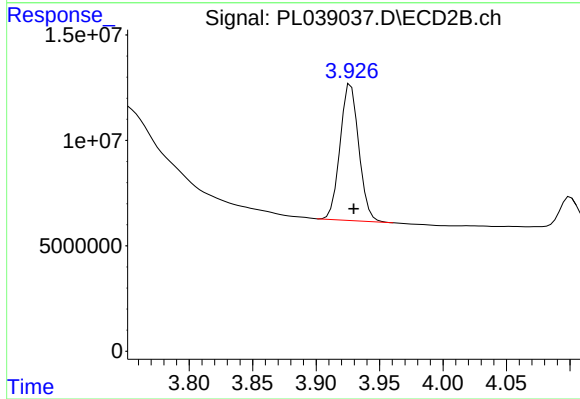


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 66372297
Conc: 25.29 ng/ml

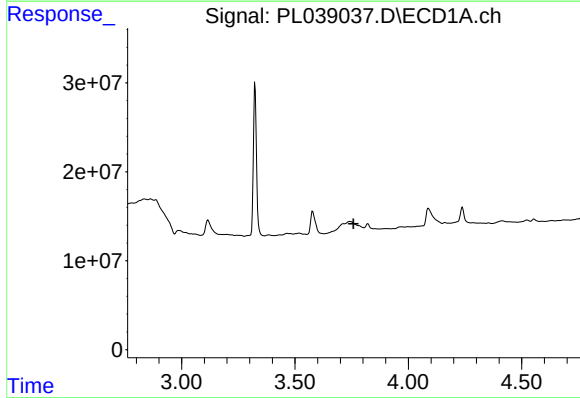


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

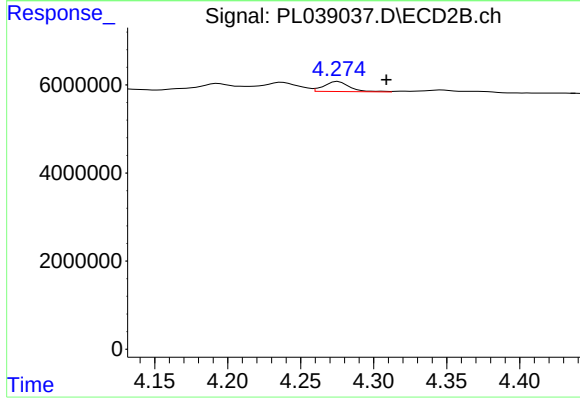

#2 alpha-BHC


R.T.: 4.276 min
Delta R.T.: -0.033 min
Response: 2779438
Conc: 0.72 ng/ml

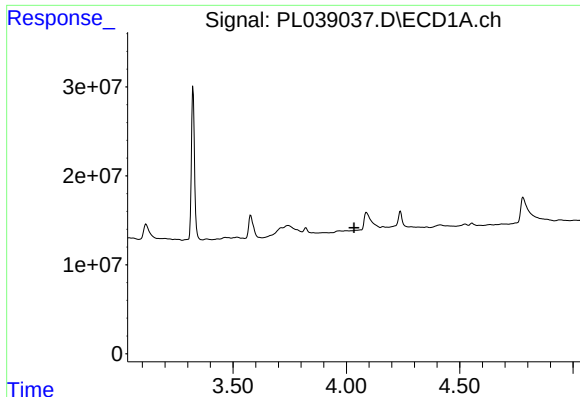

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

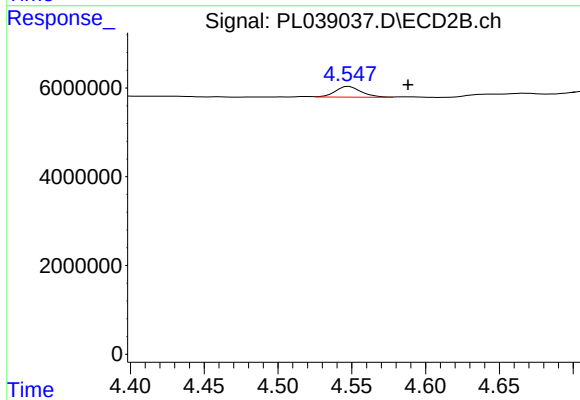


#3 gamma-BHC (Lindane)

R.T.: 4.548 min
Delta R.T.: -0.040 min
Response: 2935564
Conc: 0.81 ng/ml

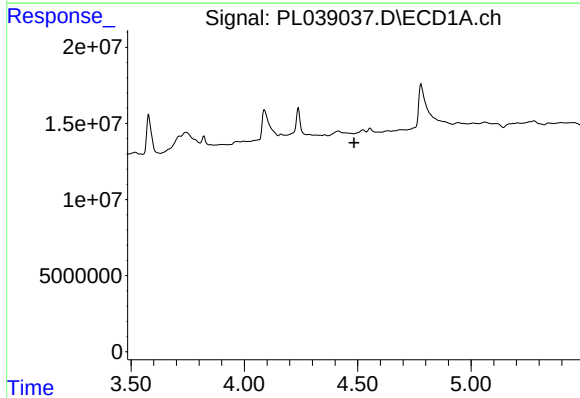


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

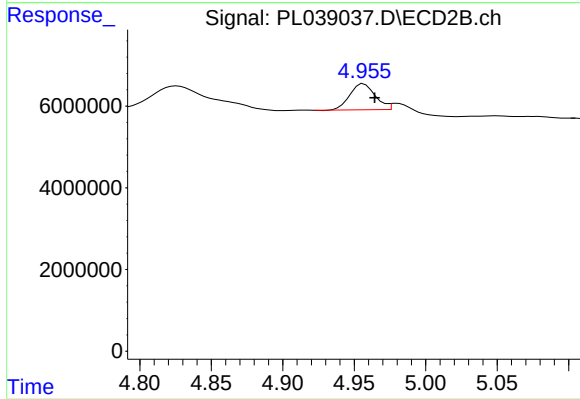

#7 delta-BHC


R.T.: 4.957 min
Delta R.T.: -0.008 min
Response: 7840016
Conc: 2.36 ng/ml

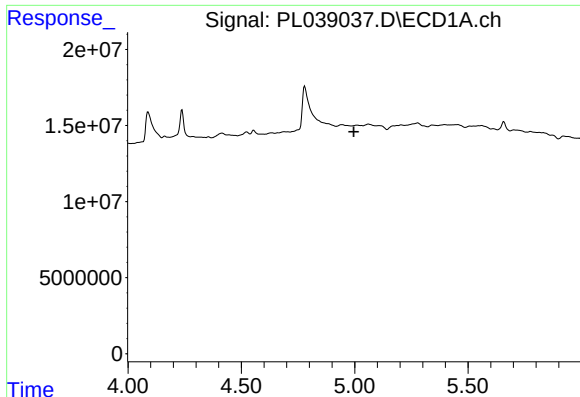

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

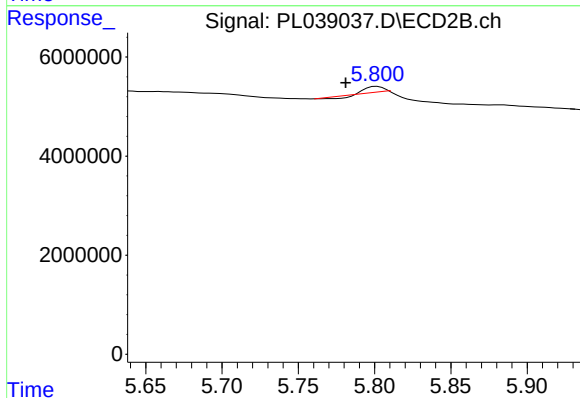


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 306778
Conc: 0.11 ng/ml

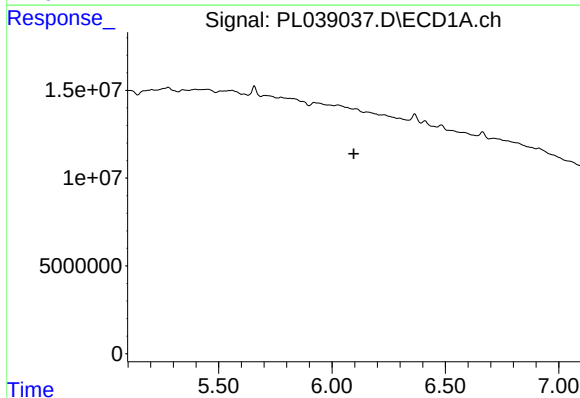


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.

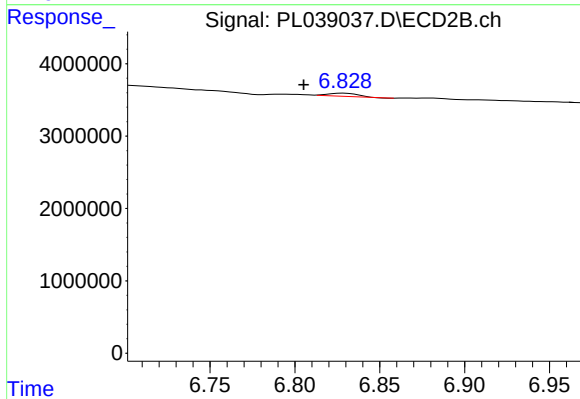

#15 Endosulfan II


R.T.: 6.829 min
Delta R.T.: 0.024 min
Response: 541280
Conc: 0.23 ng/ml

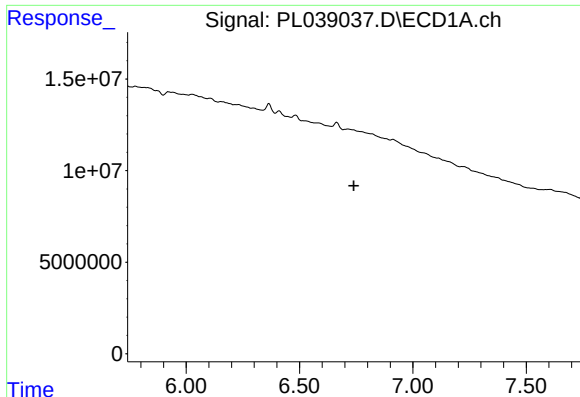

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.739 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

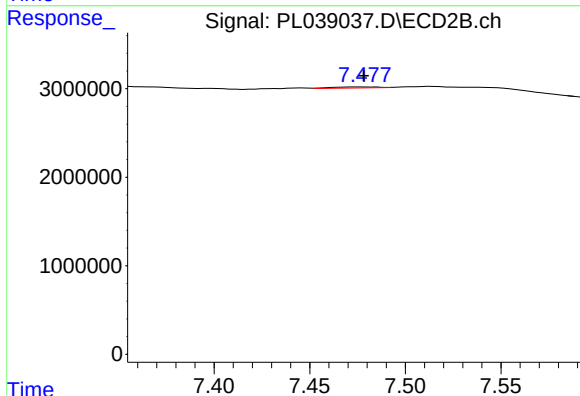


#20 Methoxychlor

R.T.: 7.475 min
Delta R.T.: -0.003 min
Response: 214615
Conc: 0.19 ng/ml

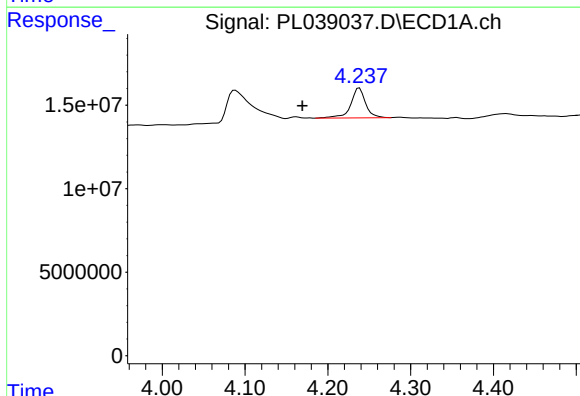


#23 Chlordane-1

R.T.: 4.238 min
Delta R.T.: 0.069 min
Response: 22023084
Conc: 63.60 ng/ml

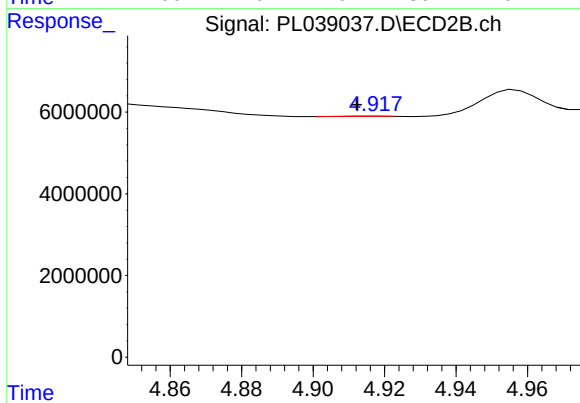

#23 Chlordane-1


R.T.: 4.918 min
Delta R.T.: 0.006 min
Response: 24098
Conc: 0.21 ng/ml

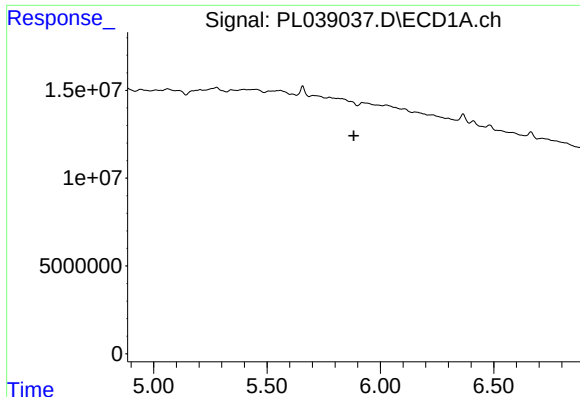

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

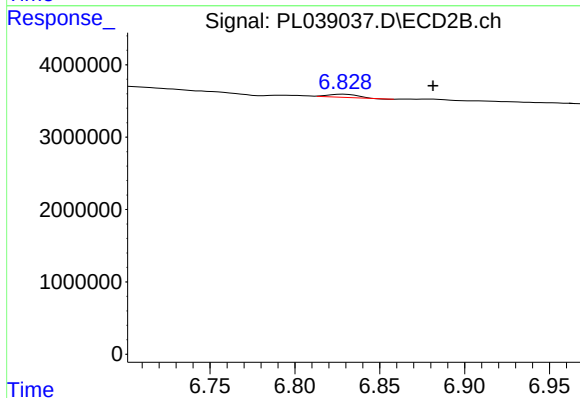


#27 Chlordane-5

R.T.: 6.829 min
Delta R.T.: -0.053 min
Response: 541280
Conc: 6.04 ng/ml

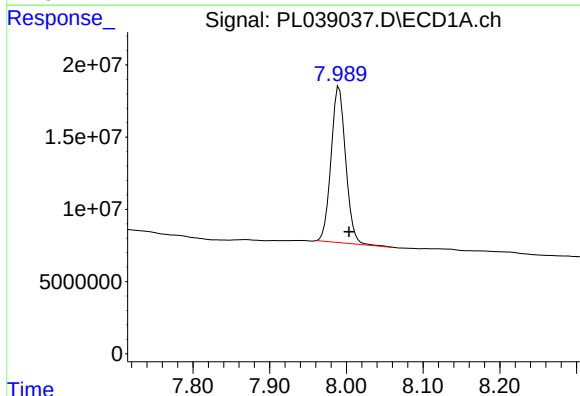

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 142652661
Conc: 18.81 ng/ml

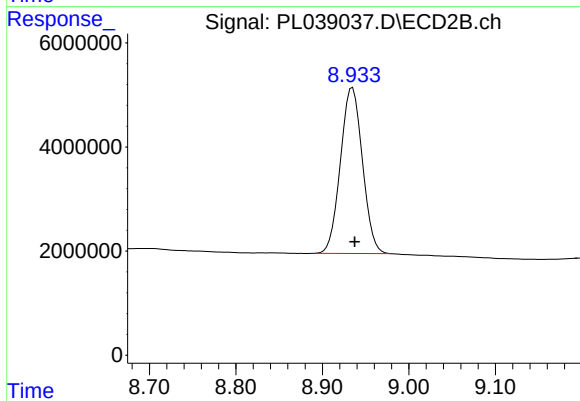

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 56042197
Conc: 22.93 ng/ml