

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 18:33
 Operator : AJ\SJ
 Sample : J4275-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:07:56 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	159.5E6	65763234	21.415	25.053
28)	SA Decachlor...	7.990	8.934	136.8E6	54379336	18.028	22.246
Target Compounds							
2)	A alpha-BHC	0.000	4.324	0	308372	N.D.	0.080 #
3)	MA gamma-BHC...	0.000	4.555f	0	921907	N.D.	0.255 #
4)	MA Heptachlor	0.000	5.156f	0	1439795	N.D.	0.450 #
7)	B delta-BHC	0.000	4.956	0	5818924	N.D.	1.754 #
8)	B Heptachlo...	4.942f	5.801	1833825	1027411	0.194	0.362 #
15)	B Endosulfa...	0.000	6.827	0	15702	N.D.	0.007 #
23)	Chlordane-1	4.237	4.916	31569475	31069	91.175	0.268 #
27)	Chlordane-5	0.000	6.827	0	15702	N.D.	0.175 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 18:33
Operator : AJ\SJ
Sample : J4275-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:07:56 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

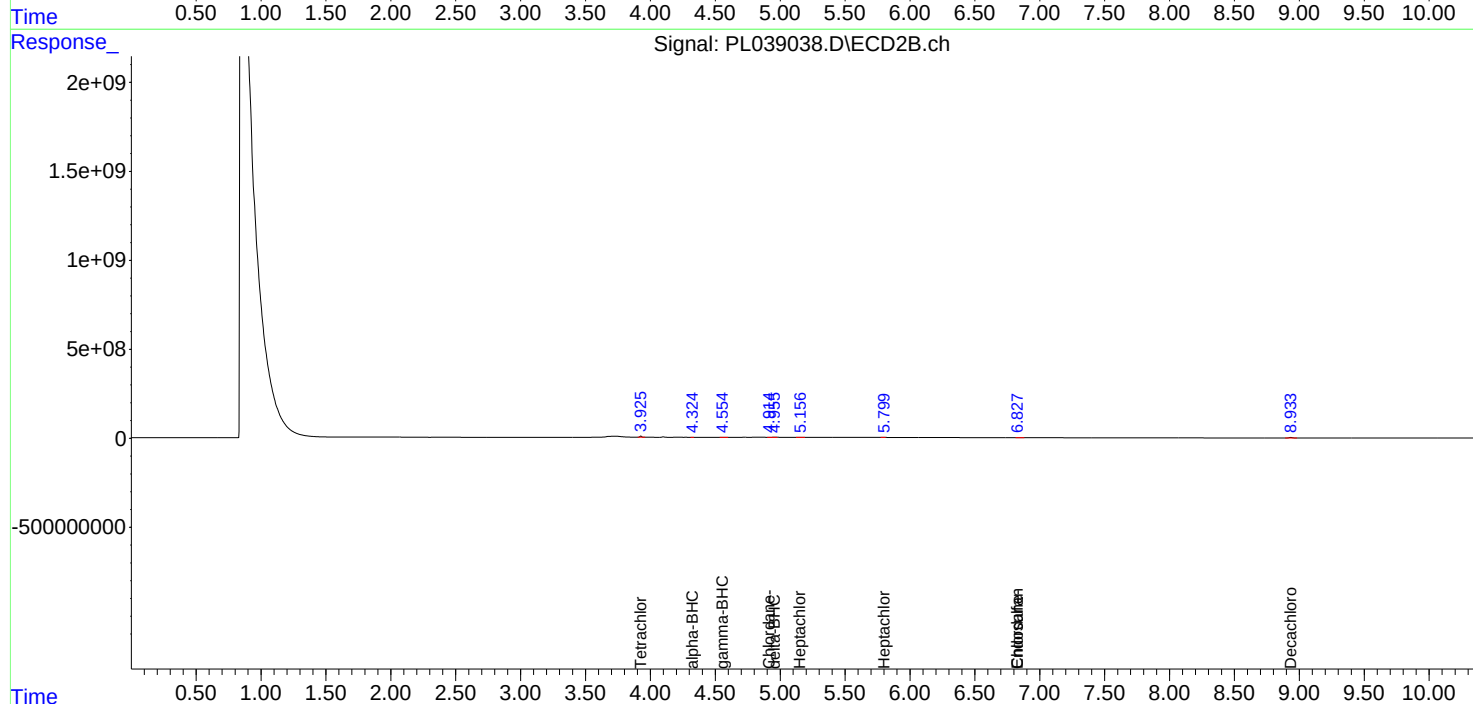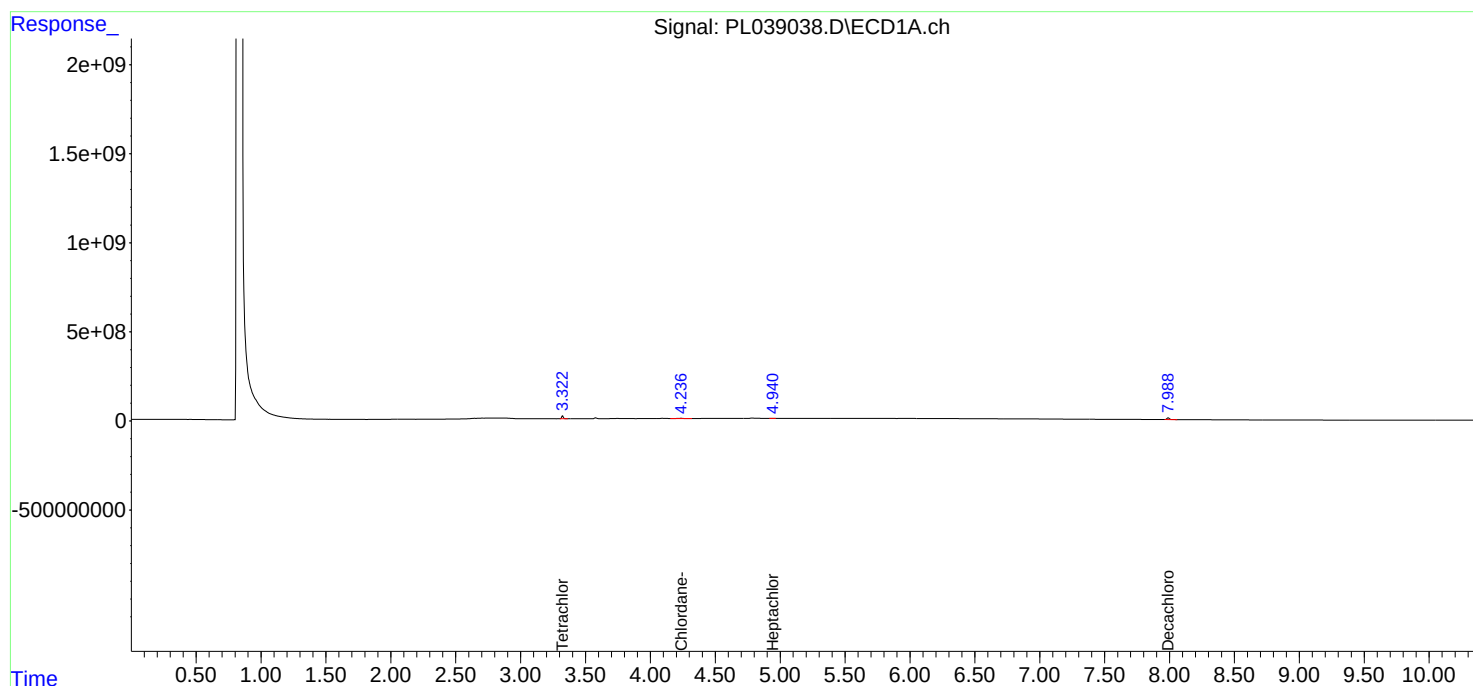


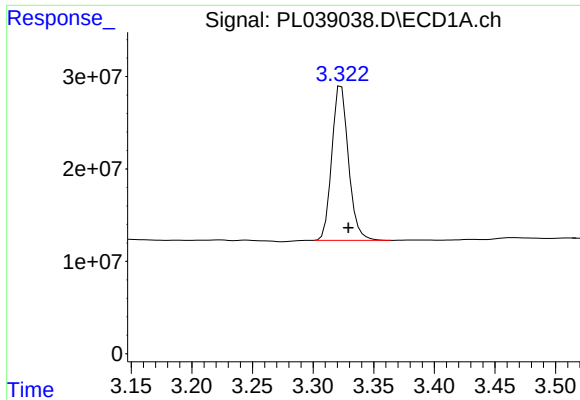

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 159466192
Conc: 21.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

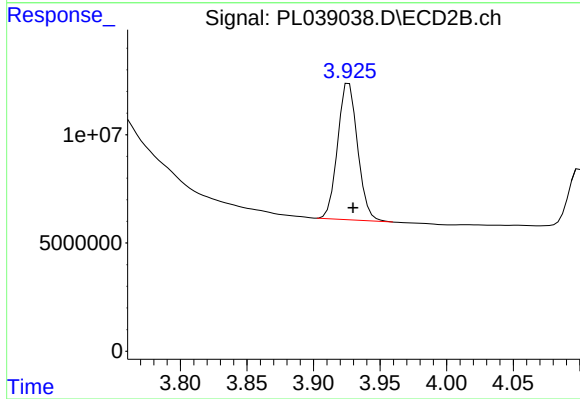


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 65763234
Conc: 25.05 ng/ml

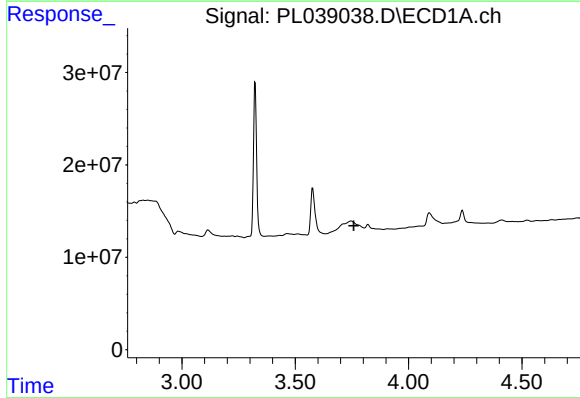


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

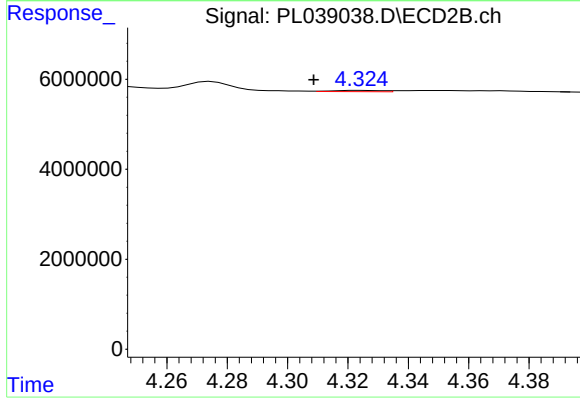

#2 alpha-BHC


R.T.: 4.324 min
Delta R.T.: 0.016 min
Response: 308372
Conc: 0.08 ng/ml

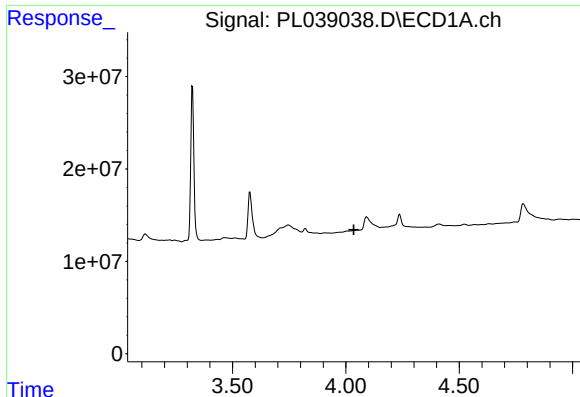

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

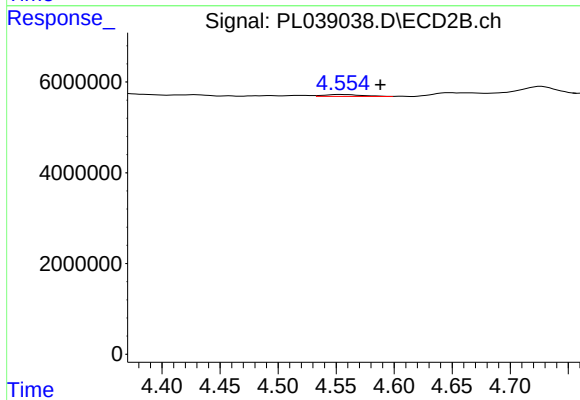


#3 gamma-BHC (Lindane)

R.T.: 4.555 min
Delta R.T.: -0.034 min
Response: 921907
Conc: 0.26 ng/ml

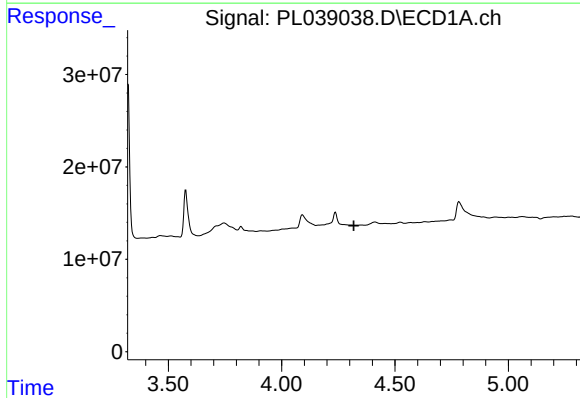


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

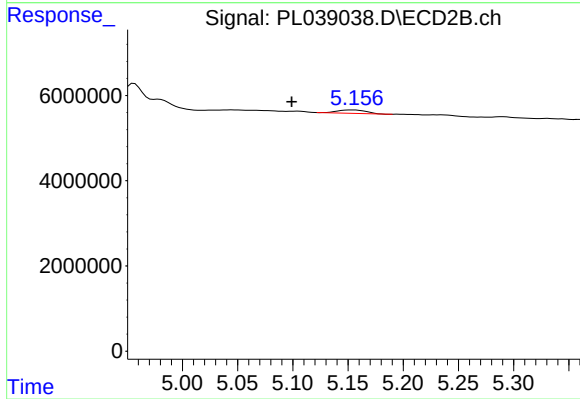

#4 Heptachlor


R.T.: 5.156 min
Delta R.T.: 0.057 min
Response: 1439795
Conc: 0.45 ng/ml

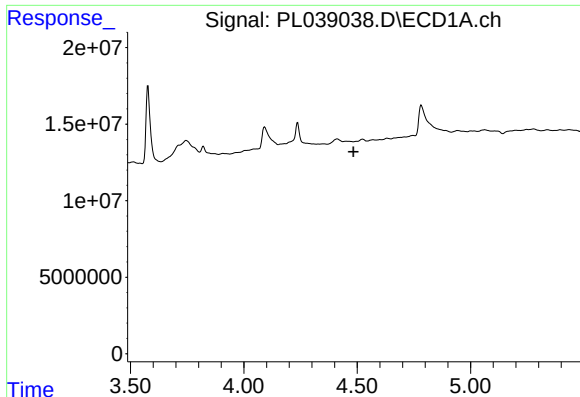

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

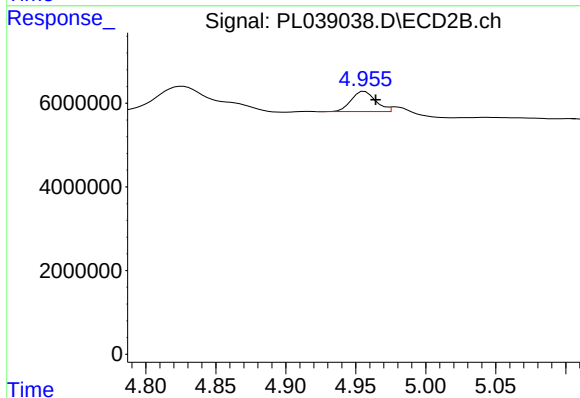


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 5818924
Conc: 1.75 ng/ml

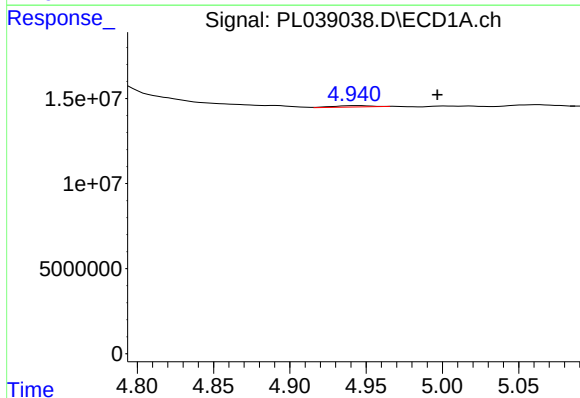


#8 Heptachlor epoxide

R.T.: 4.942 min
Delta R.T.: -0.055 min
Response: 1833825
Conc: 0.19 ng/ml

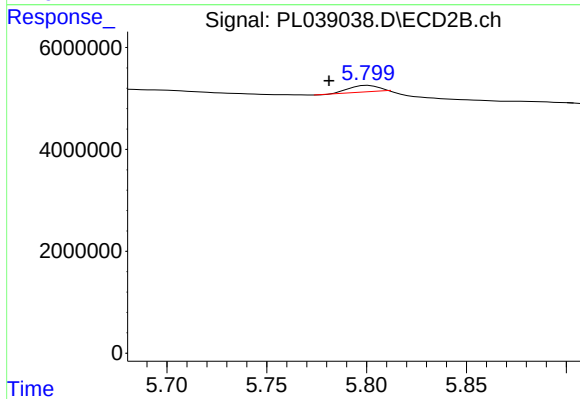

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 1027411
Conc: 0.36 ng/ml

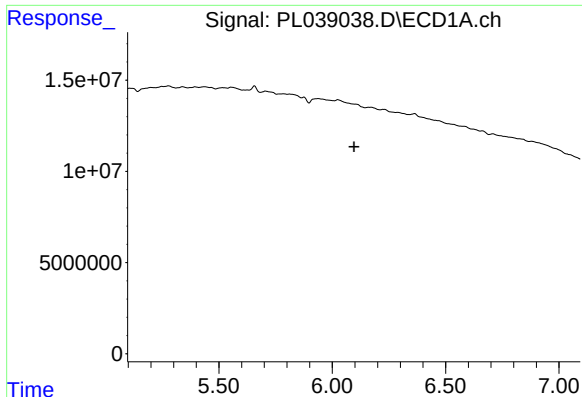

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

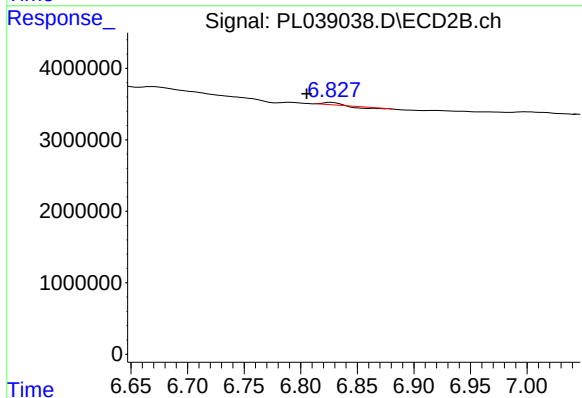


#15 Endosulfan II

R.T.: 6.827 min
Delta R.T.: 0.022 min
Response: 15702
Conc: 0.01 ng/ml

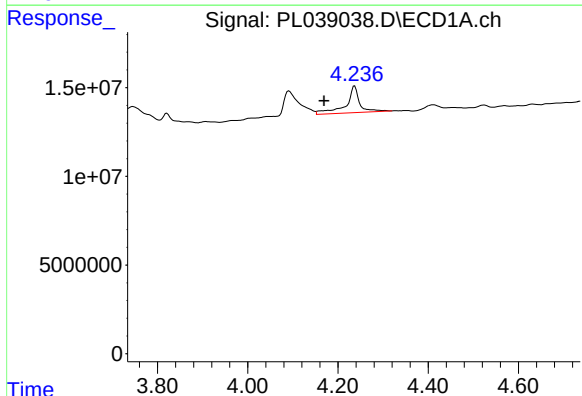


#23 Chlordane-1

R.T.: 4.237 min
Delta R.T.: 0.068 min
Response: 31569475
Conc: 91.18 ng/ml

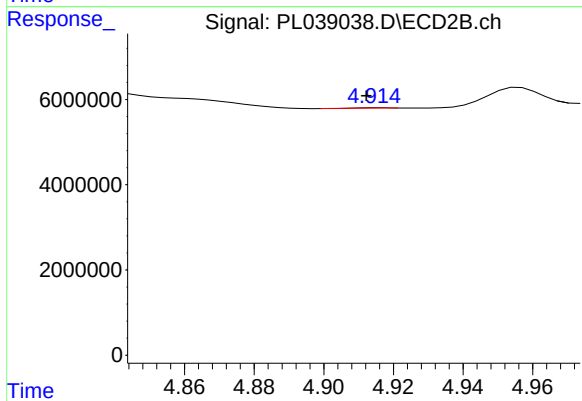

#23 Chlordane-1


R.T.: 4.916 min
Delta R.T.: 0.004 min
Response: 31069
Conc: 0.27 ng/ml

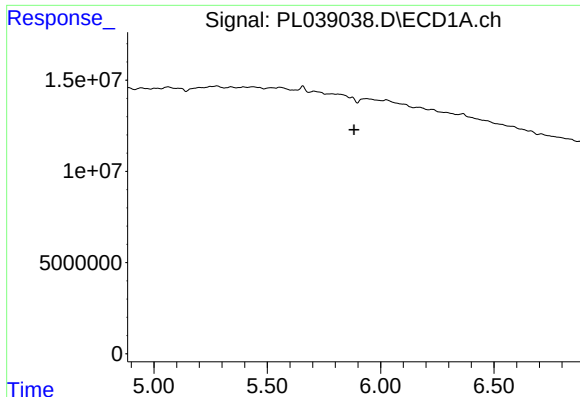

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

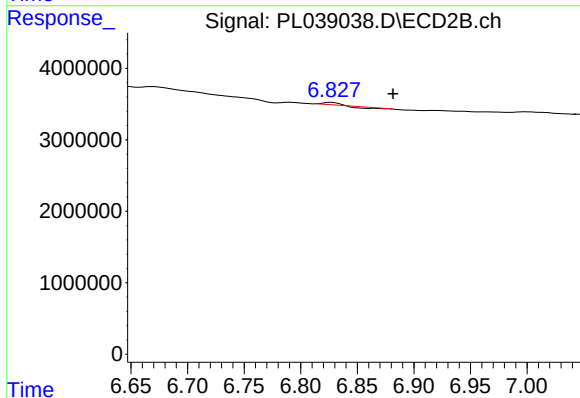


#27 Chlorodane-5

R.T.: 6.827 min
Delta R.T.: -0.054 min
Response: 15702
Conc: 0.18 ng/ml

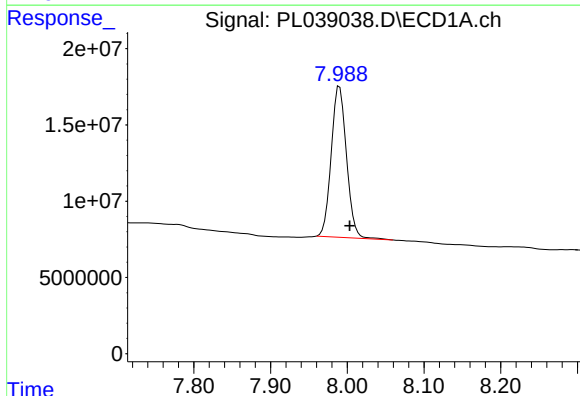

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 136755488
Conc: 18.03 ng/ml

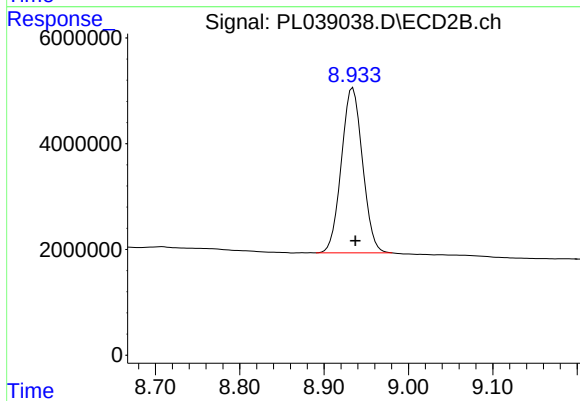

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 54379336
Conc: 22.25 ng/ml