

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 18:47
 Operator : AJ\SJ
 Sample : J4276-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:08:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	154.8E6	64543059	20.794	24.588
28)	SA Decachlor...	7.991	8.935	124.8E6	49736545	16.446	20.347
Target Compounds							
2)	A alpha-BHC	0.000	4.275f	0	3033770	N.D.	0.784 #
3)	MA gamma-BHC...	0.000	4.561f	0	592871	N.D.	0.164 #
4)	MA Heptachlor	0.000	5.056f	0	9133	N.D.	0.003 #
7)	B delta-BHC	0.000	4.956	0	6126658	N.D.	1.847 #
8)	B Heptachlo...	0.000	5.765	0	196969	N.D.	0.069 #
17)	MA 4,4'-DDT	0.000	6.981f	0	471586	N.D.	0.221 #
18)	B Endrin al...	0.000	6.921	0	613349	N.D.	0.314 #
23)	Chlordane-1	4.238	4.956	26733673	6126658	77.209	52.868 #
27)	Chlordane-5	0.000	6.921	0	613349	N.D.	6.847 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 18:47
Operator : AJ\SJ
Sample : J4276-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:08:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

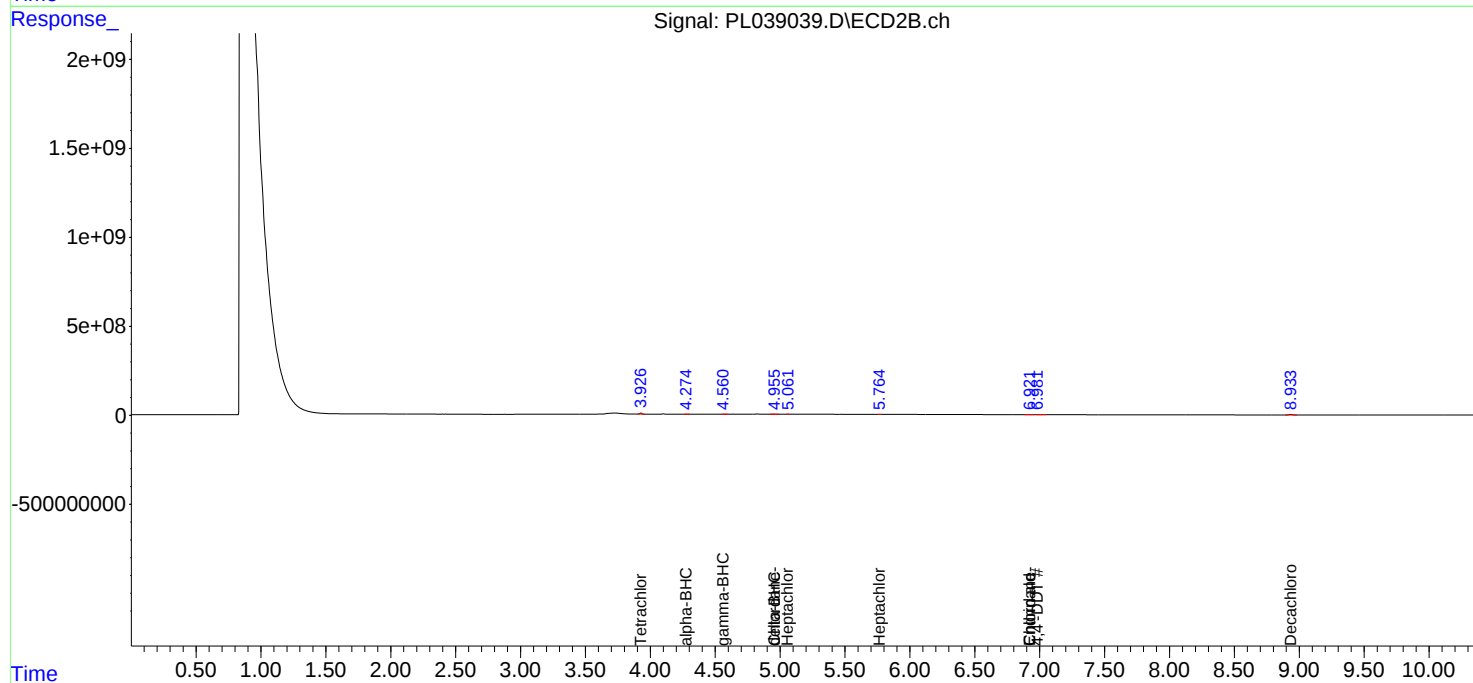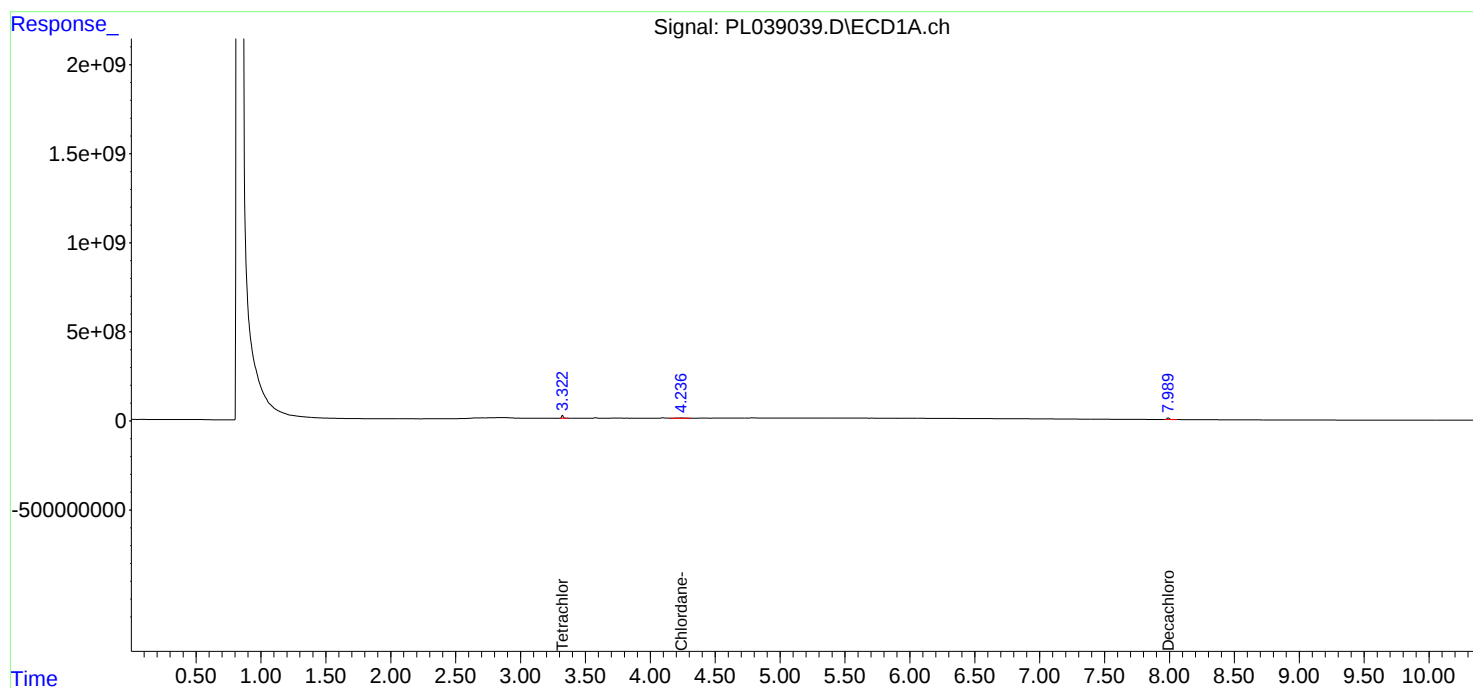


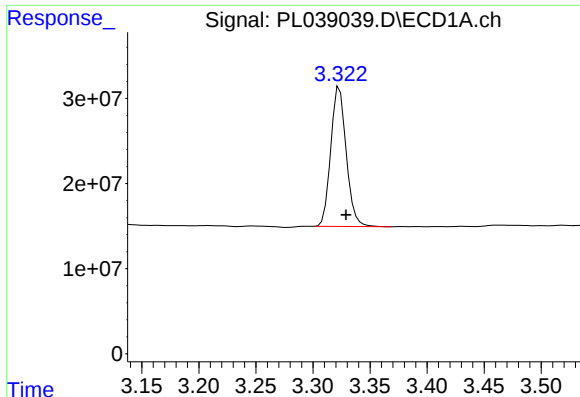

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 154842626
Conc: 20.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

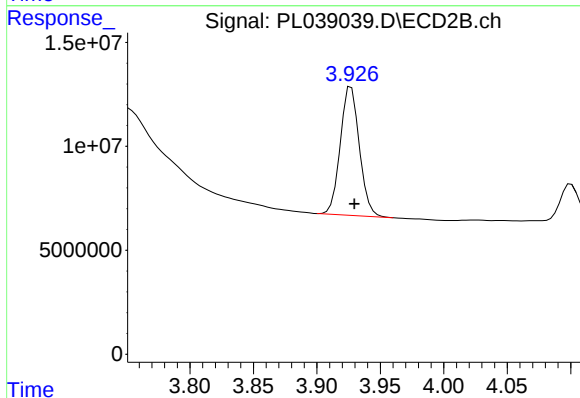


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 64543059
Conc: 24.59 ng/ml

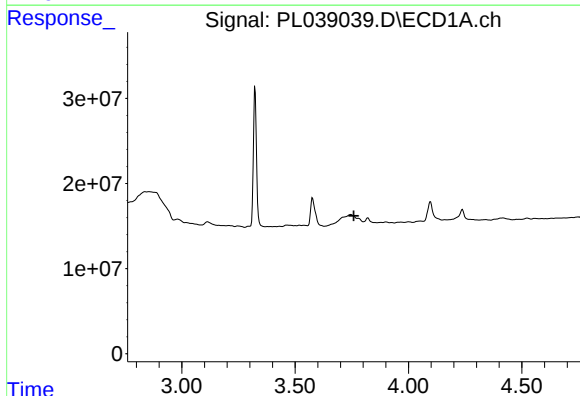


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

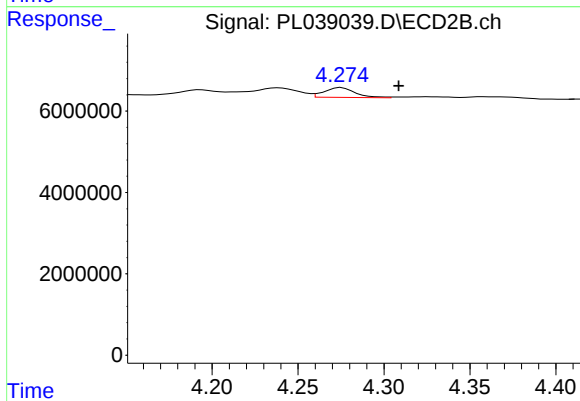

#2 alpha-BHC


R.T.: 4.275 min
Delta R.T.: -0.033 min
Response: 3033770
Conc: 0.78 ng/ml

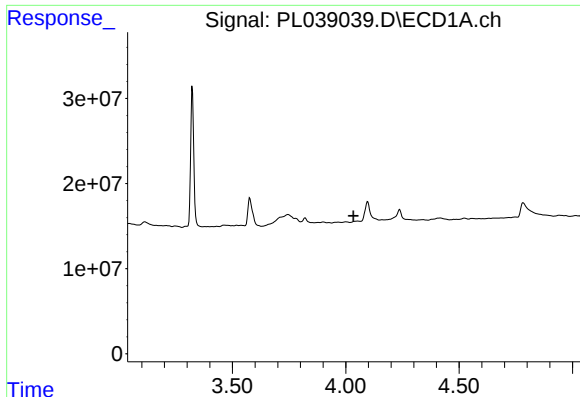

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

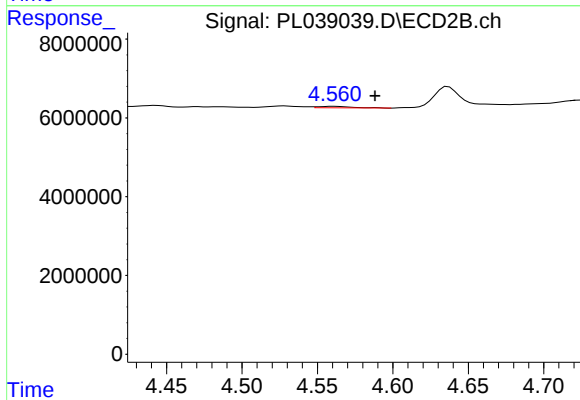


#3 gamma-BHC (Lindane)

R.T.: 4.561 min
Delta R.T.: -0.027 min
Response: 592871
Conc: 0.16 ng/ml

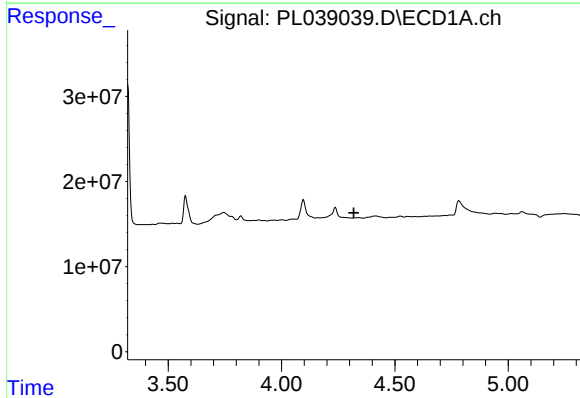


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

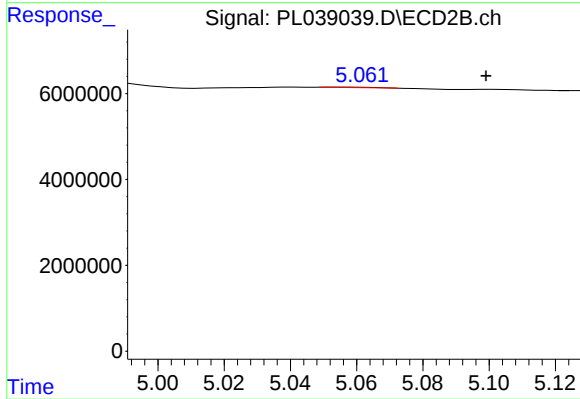

#4 Heptachlor


R.T.: 5.056 min
Delta R.T.: -0.043 min
Response: 9133
Conc: 0.00 ng/ml

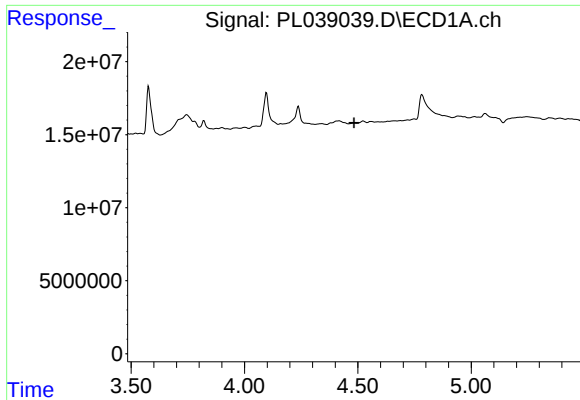

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

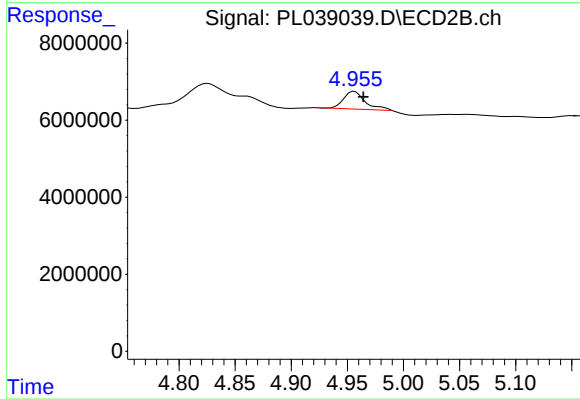


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 6126658
Conc: 1.85 ng/ml

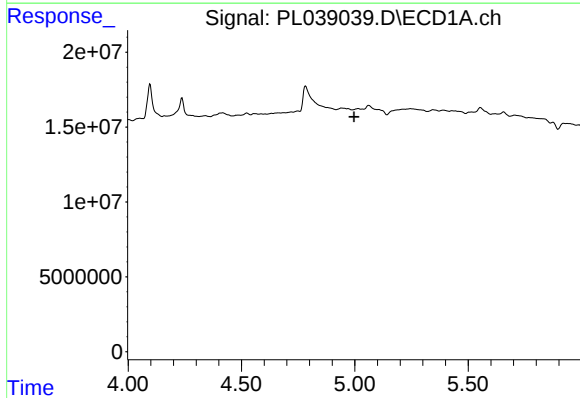


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.997 min
Response: 0
Conc: N.D.

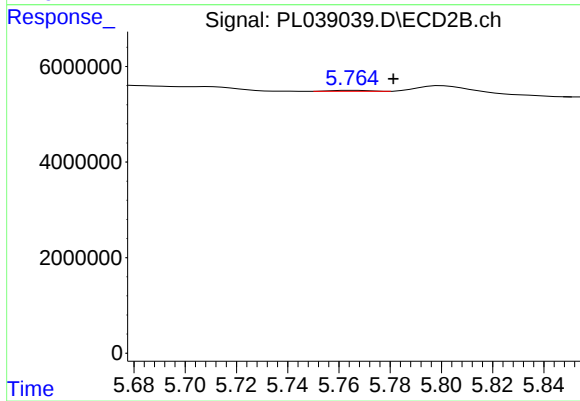

#8 Heptachlor epoxide


R.T.: 5.765 min
Delta R.T.: -0.016 min
Response: 196969
Conc: 0.07 ng/ml

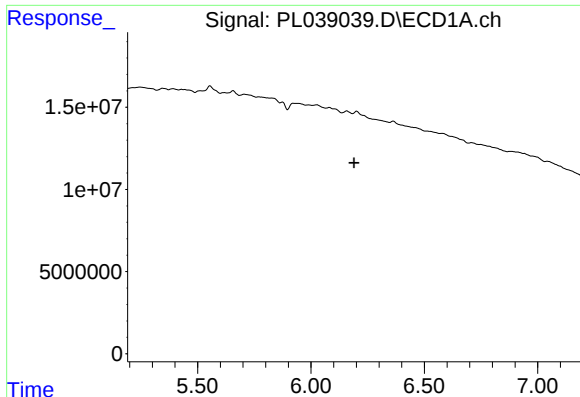

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

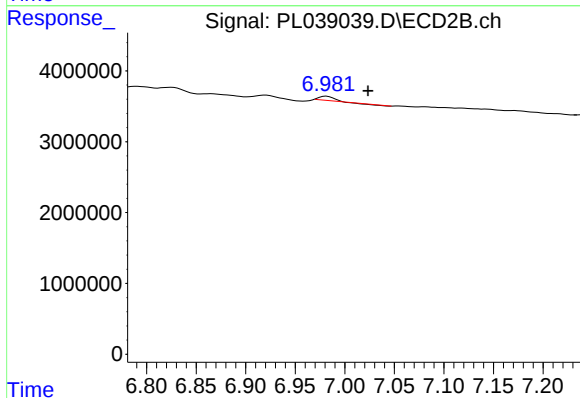


#17 4,4'-DDT

R.T.: 6.981 min
Delta R.T.: -0.042 min
Response: 471586
Conc: 0.22 ng/ml

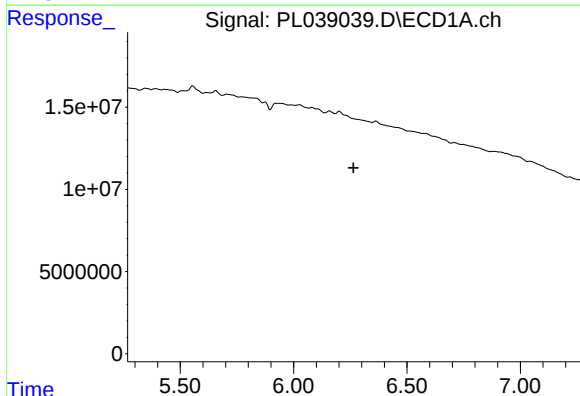


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

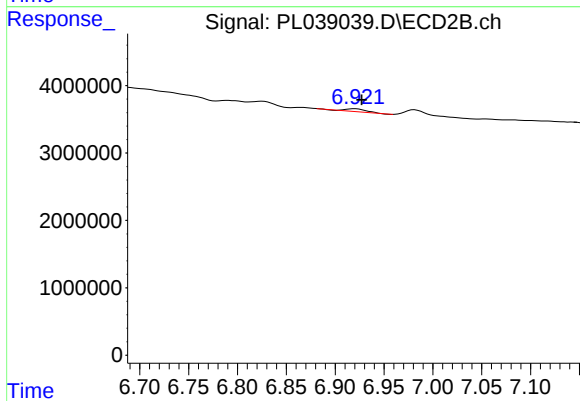

#18 Endrin aldehyde


R.T.: 6.921 min
Delta R.T.: -0.006 min
Response: 613349
Conc: 0.31 ng/ml

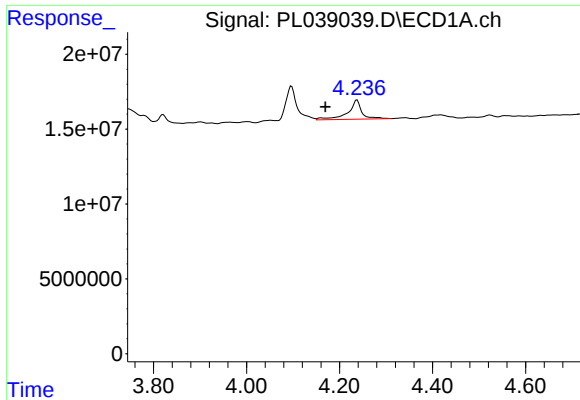

#23 Chlordane-1


R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 26733673
Conc: 77.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

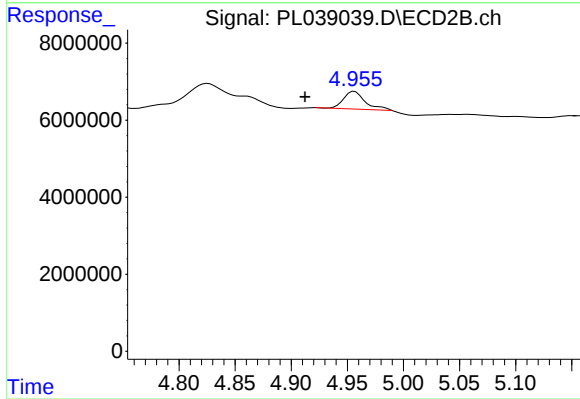


#23 Chlordane-1

R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 6126658
Conc: 52.87 ng/ml

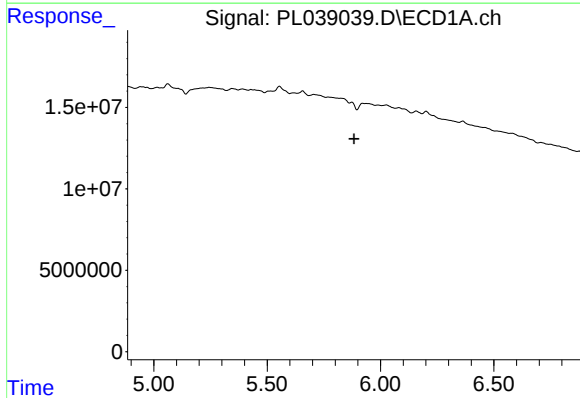


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 5.883 min
Response: 0
Conc: N.D.

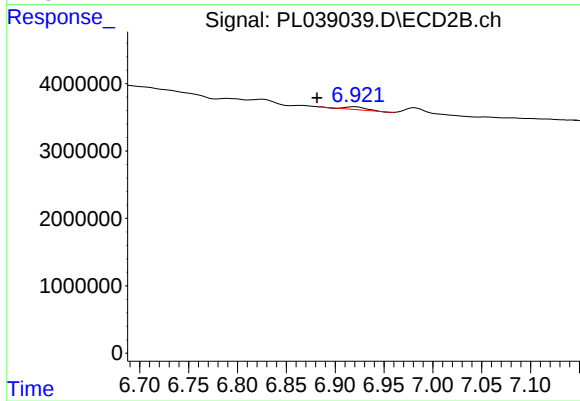

#27 Chlordane-5


R.T.: 6.921 min
Delta R.T.: 0.039 min
Response: 613349
Conc: 6.85 ng/ml

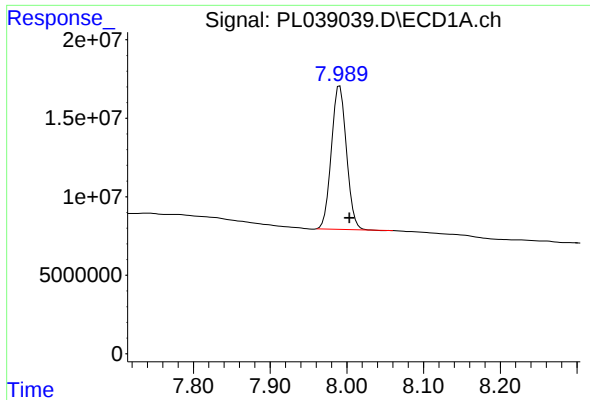

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.013 min
Response: 124757126
Conc: 16.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

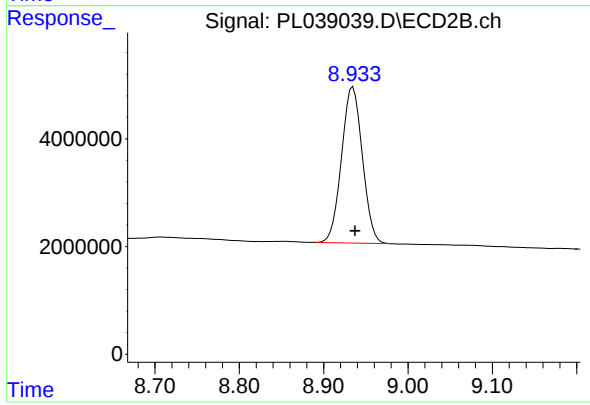

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.003 min
Response: 49736545
Conc: 20.35 ng/ml