

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 21:37
 Operator : AJ\SJ
 Sample : PB111857BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:12:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	181.6E6	72640623	24.387	27.673
28)	SA Decachlor...	7.991	8.936	153.6E6	60765681	20.248	24.859
Target Compounds							
2)	A alpha-BHC	0.000	4.317	0	2137334	N.D.	0.552 #
6)	B beta-BHC	4.240f	0.000	14195278	0	3.007	N.D. #
7)	B delta-BHC	0.000	4.955	0	2952119	N.D.	0.890 #
8)	B Heptachlo...	0.000	5.801	0	433634	N.D.	0.153 #
16)	A 4,4'-DDD	0.000	6.675f	0	1211001	N.D.	0.566 #
19)	B Endosulfa...	6.483	0.000	10081849	0	1.335	N.D. #
20)	A Methoxychlor	0.000	7.441f	0	453485	N.D.	0.398 #
23)	Chlordane-1	0.000	4.914	0	117072	N.D.	1.010 #
24)	Chlordane-2	0.000	5.310	0	190147	N.D.	1.588 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 21:37
Operator : AJ\SJ
Sample : PB111857BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:12:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

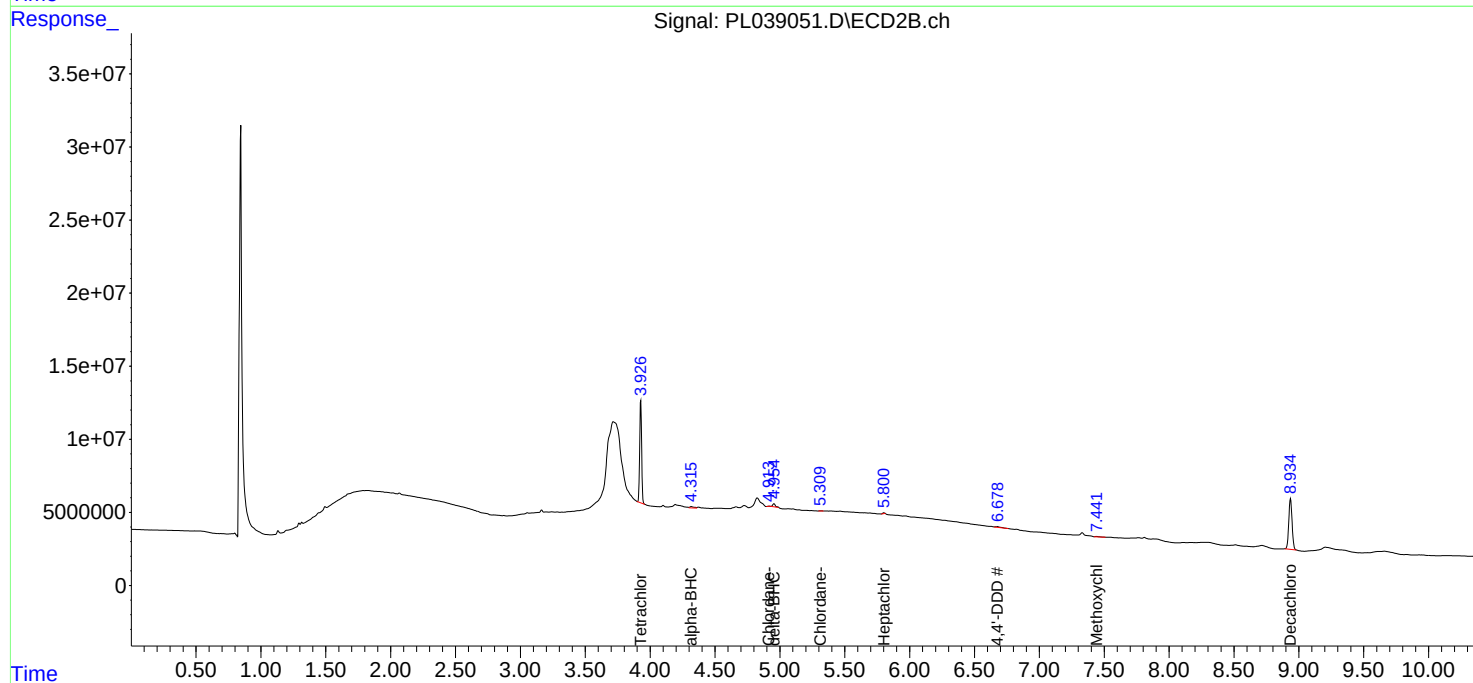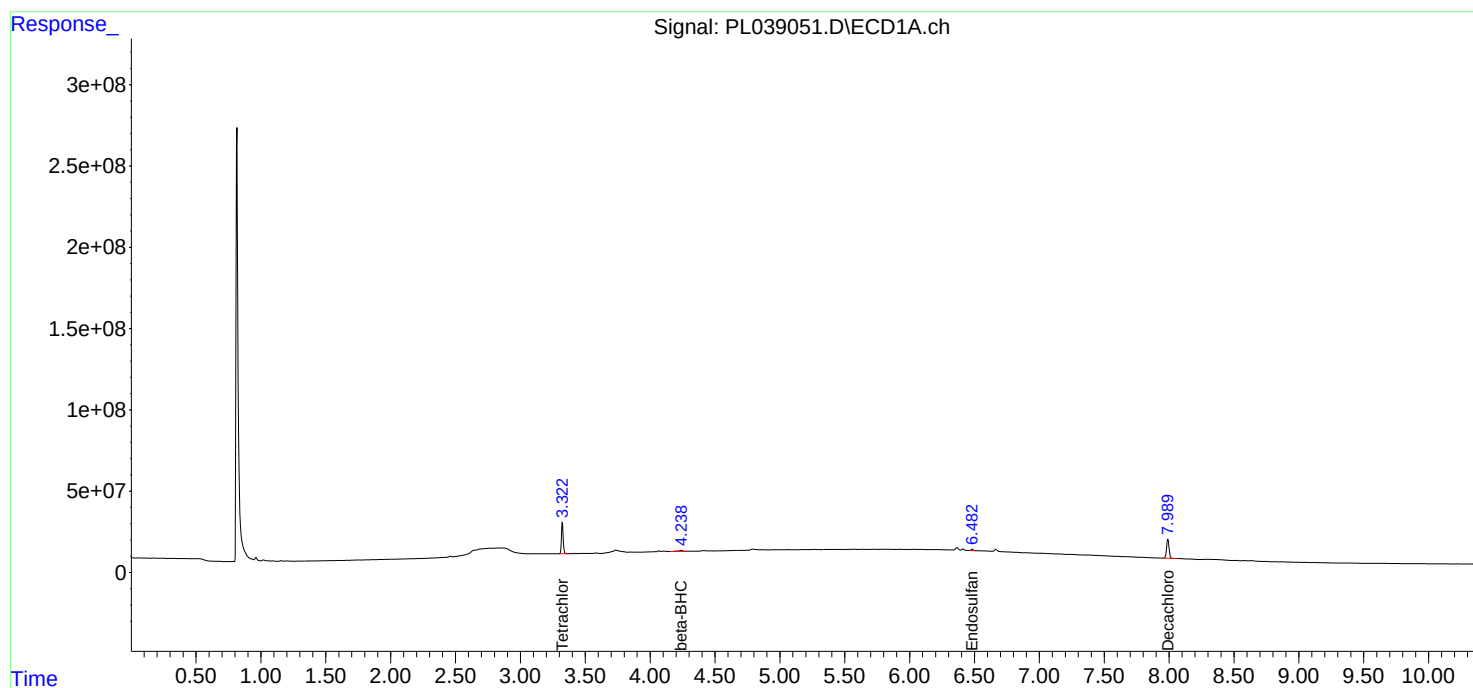


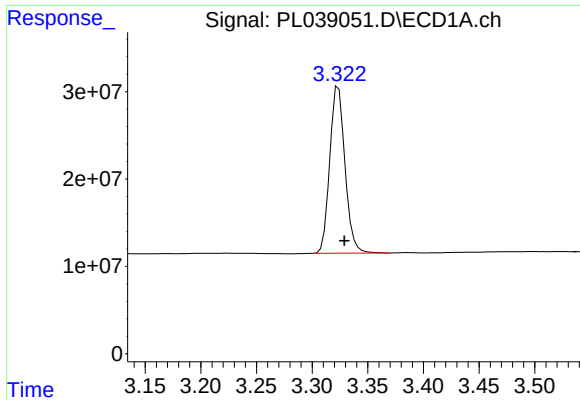

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 181596766
Conc: 24.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

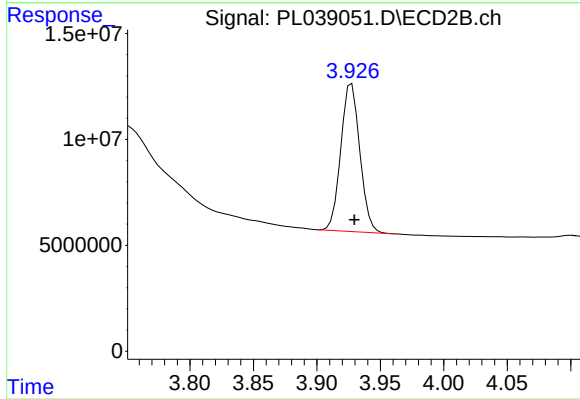


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.002 min
Response: 72640623
Conc: 27.67 ng/ml

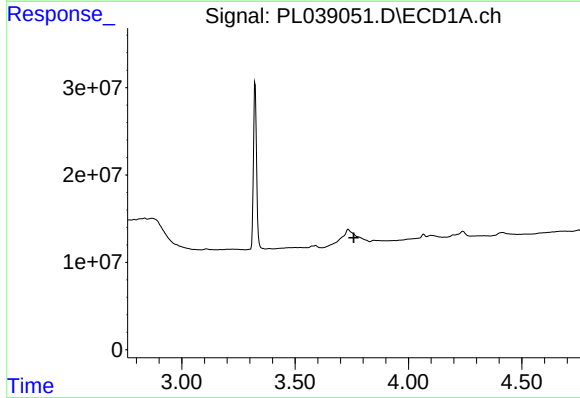


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

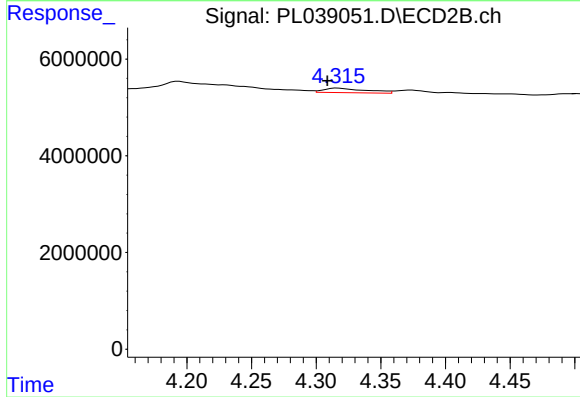

#2 alpha-BHC


R.T.: 4.317 min
Delta R.T.: 0.008 min
Response: 2137334
Conc: 0.55 ng/ml

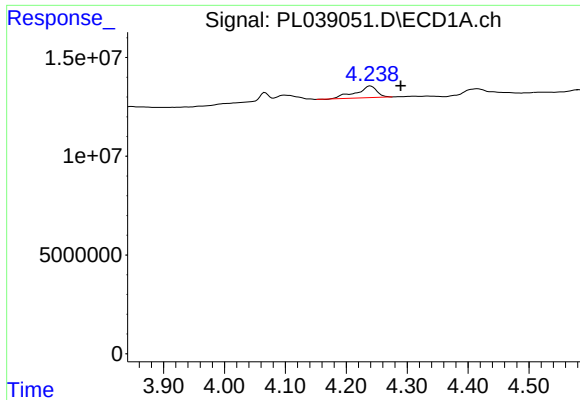

#6 beta-BHC


R.T.: 4.240 min
Delta R.T.: -0.049 min
Response: 14195278
Conc: 3.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

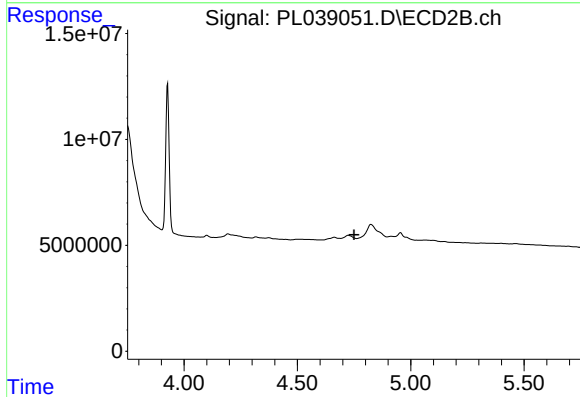


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.750 min
Response: 0
Conc: N.D.

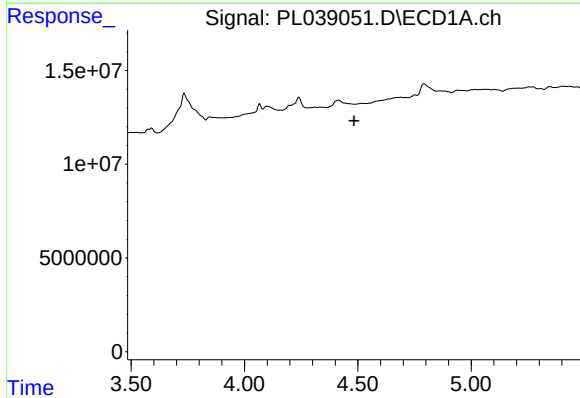


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

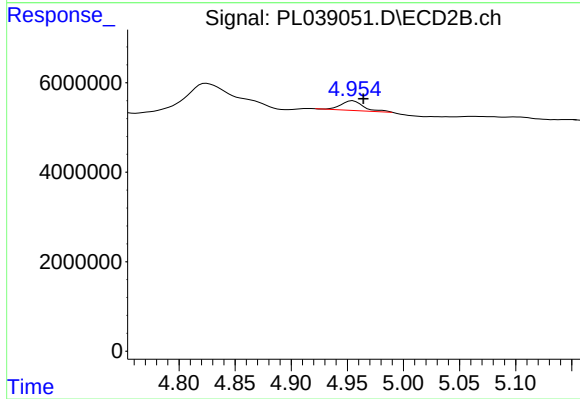

#7 delta-BHC


R.T.: 4.955 min
Delta R.T.: -0.009 min
Response: 2952119
Conc: 0.89 ng/ml

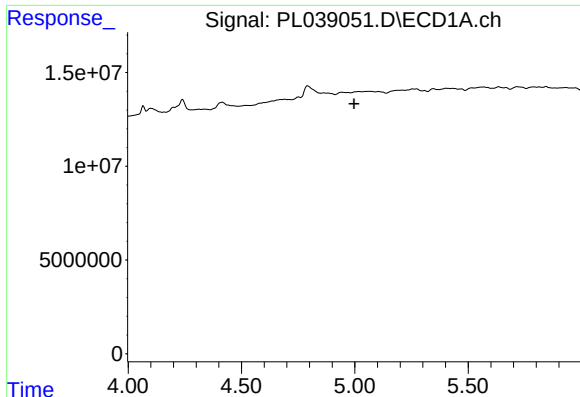

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

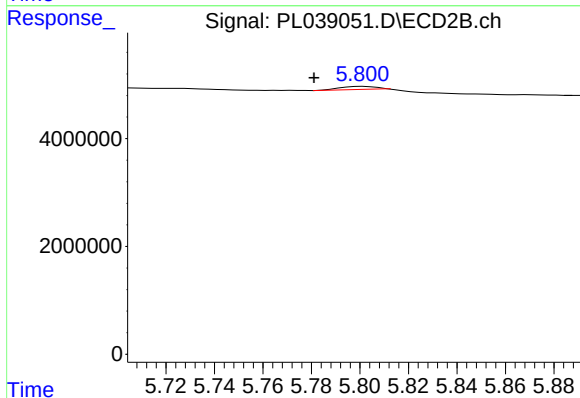


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 433634
Conc: 0.15 ng/ml

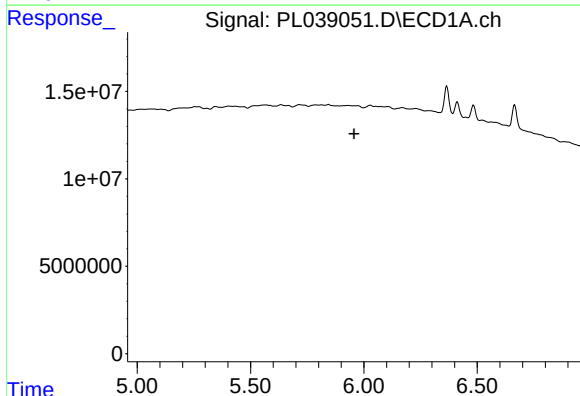


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

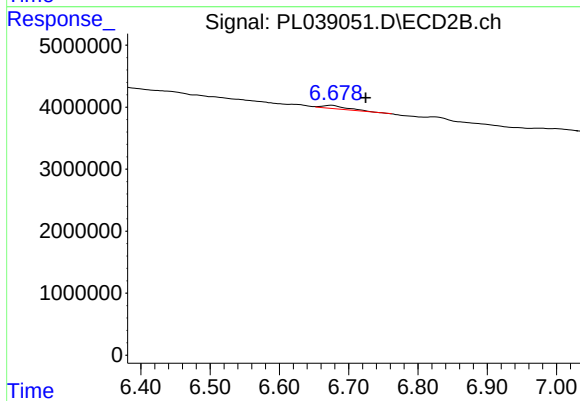

#16 4,4'-DDD


R.T.: 6.675 min
Delta R.T.: -0.049 min
Response: 1211001
Conc: 0.57 ng/ml

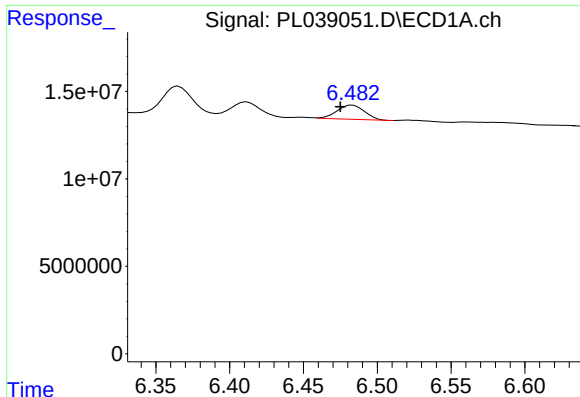

#19 Endosulfan Sulfate


R.T.: 6.483 min
Delta R.T.: 0.008 min
Response: 10081849
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

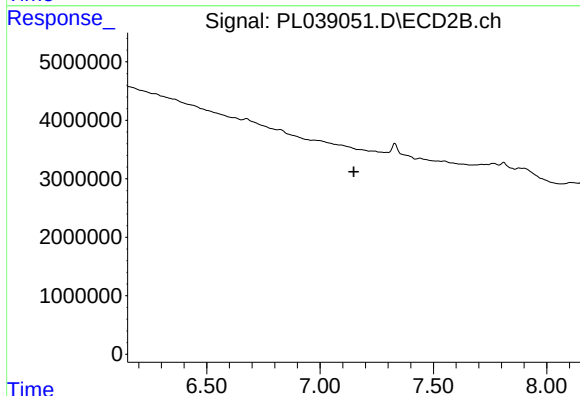


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

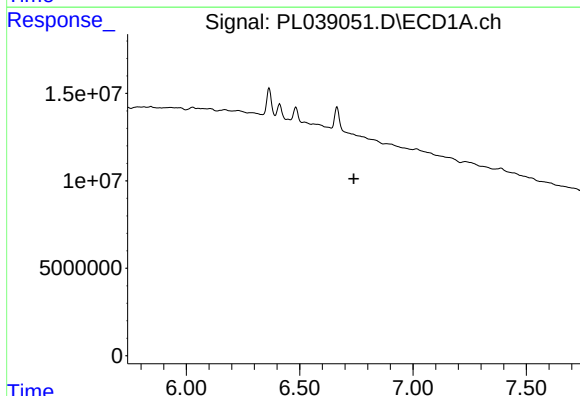


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.739 min
Response: 0
Conc: N.D.

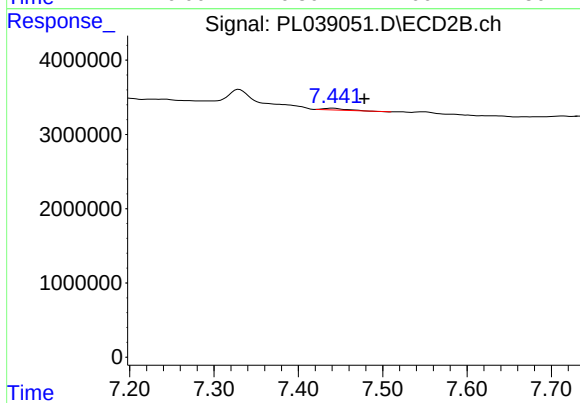

#20 Methoxychlor


R.T.: 7.441 min
Delta R.T.: -0.037 min
Response: 453485
Conc: 0.40 ng/ml

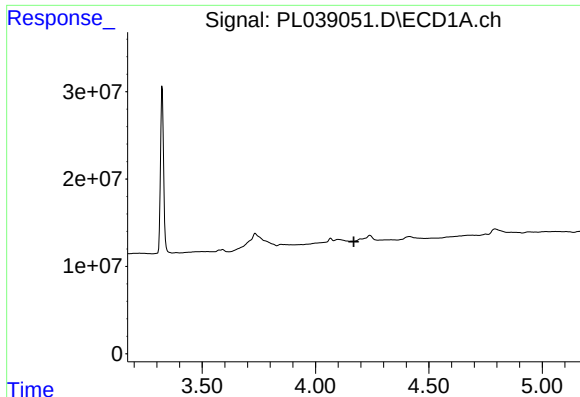

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

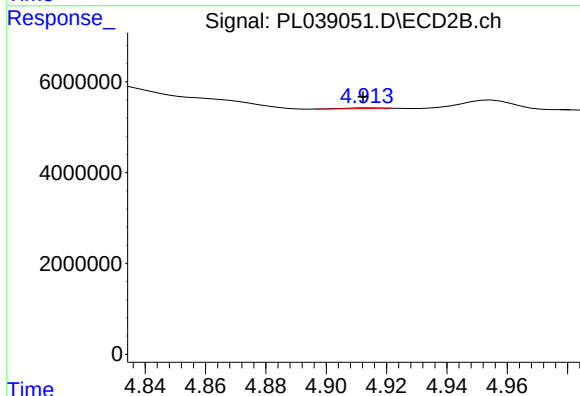


#23 Chlordane-1

R.T.: 4.914 min
Delta R.T.: 0.002 min
Response: 117072
Conc: 1.01 ng/ml

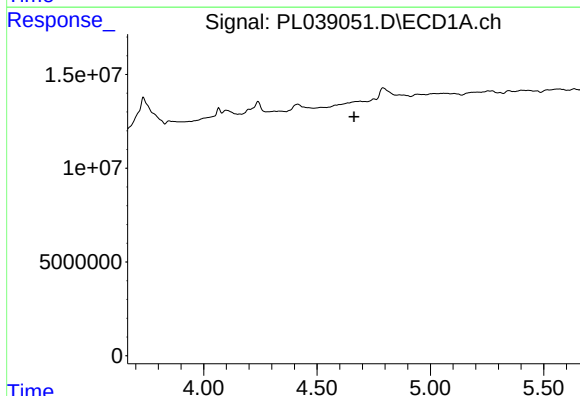


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.663 min
Response: 0
Conc: N.D.

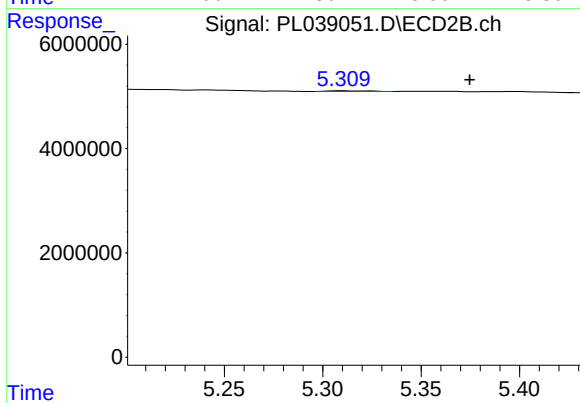

#24 Chlordane-2


R.T.: 5.310 min
Delta R.T.: -0.064 min
Response: 190147
Conc: 1.59 ng/ml

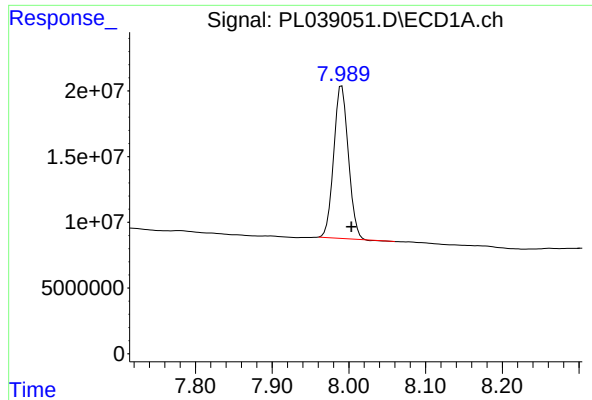

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.013 min
Response: 153600911
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

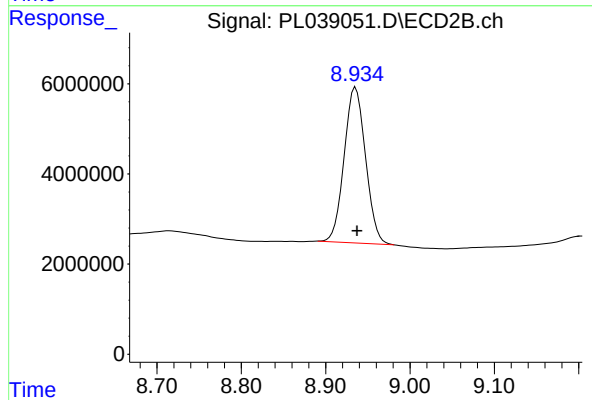

#28 Decachlorobiphenyl

R.T.: 8.936 min
Delta R.T.: -0.002 min
Response: 60765681
Conc: 24.86 ng/ml