

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 14:28
 Operator : AJ\SJ
 Sample : J4276-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-02-080718

Manual Integrations
 APPROVED

Sohil
 8/9/2018 9:58:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:52:27 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.926	87648245	31874008	11.771	12.143
28)	SA Decachlor...	7.990	8.933	84124223	39079676	11.090	15.987 #
Target Compounds							
12)	B 4,4'-DDE	5.434	6.239	43150424	10801748	4.501	4.039
17)	MA 4,4'-DDT	6.179	7.018	40315002	13047596	5.427	6.120m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 14:28
Operator : AJ\SJ
Sample : J4276-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
OK-02-080718


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:52:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

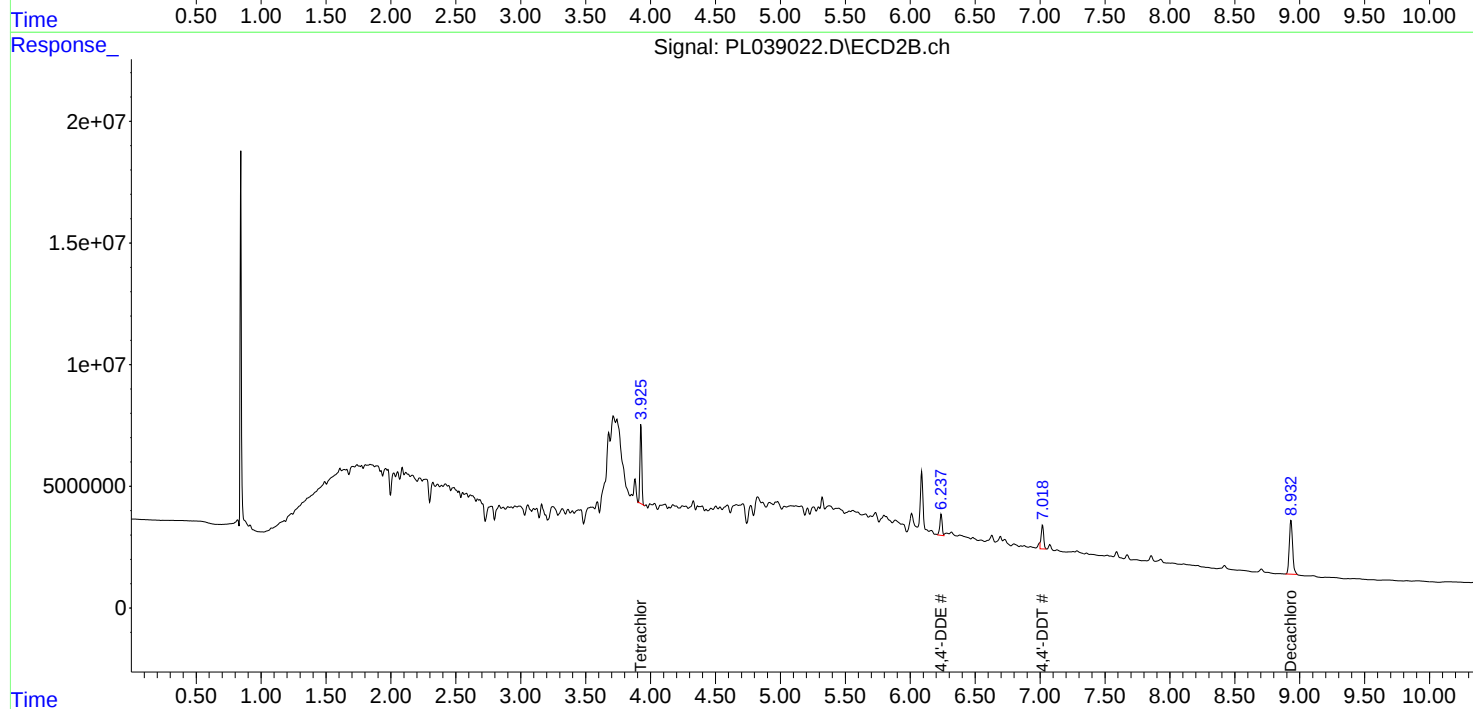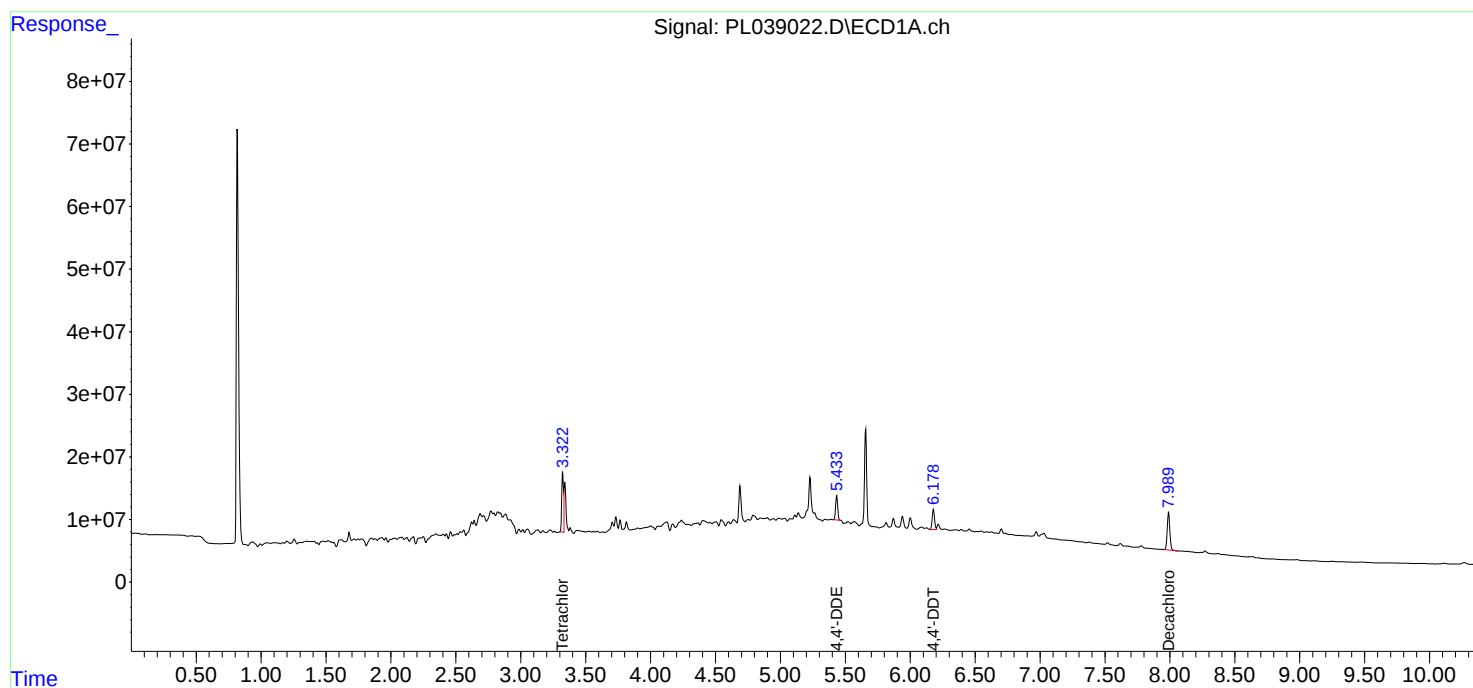

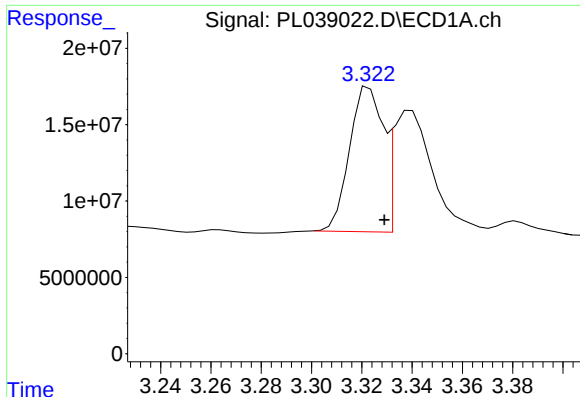


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 87648245
Conc: 11.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-080718


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:20 AM

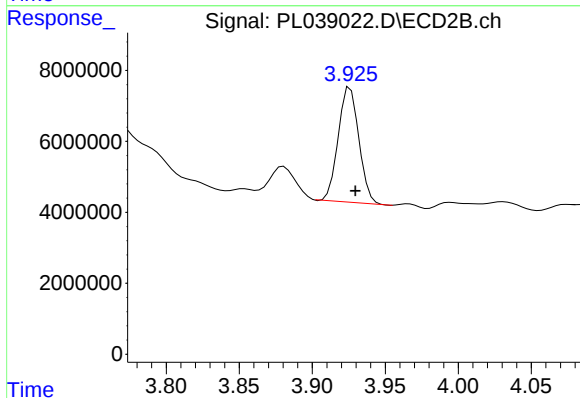


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 31874008
Conc: 12.14 ng/ml

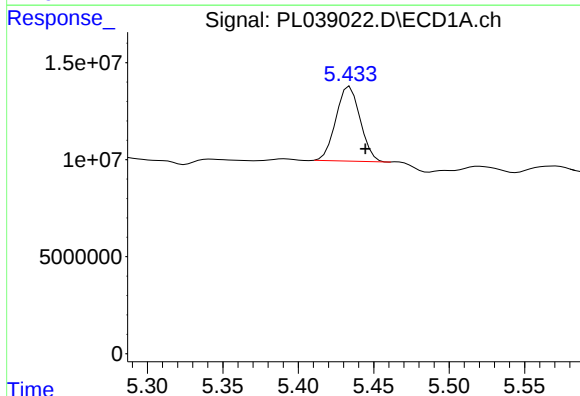


#12 4,4'-DDE

R.T.: 5.434 min
Delta R.T.: -0.010 min
Response: 43150424
Conc: 4.50 ng/ml

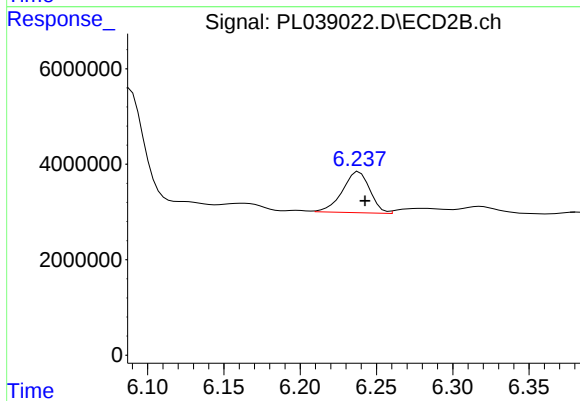

#12 4,4'-DDE

R.T.: 6.239 min
Delta R.T.: -0.004 min
Response: 10801748
Conc: 4.04 ng/ml

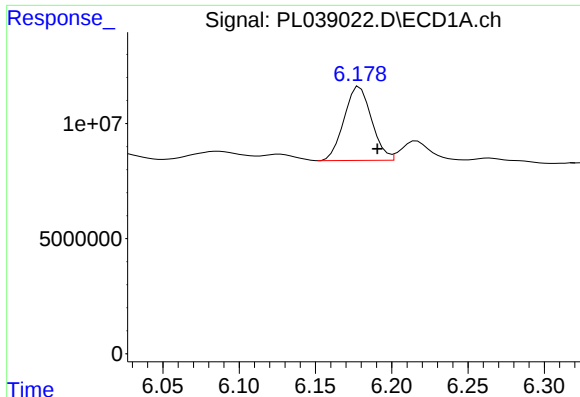


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: -0.011 min
Response: 40315002
Conc: 5.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-02-080718


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:20 AM

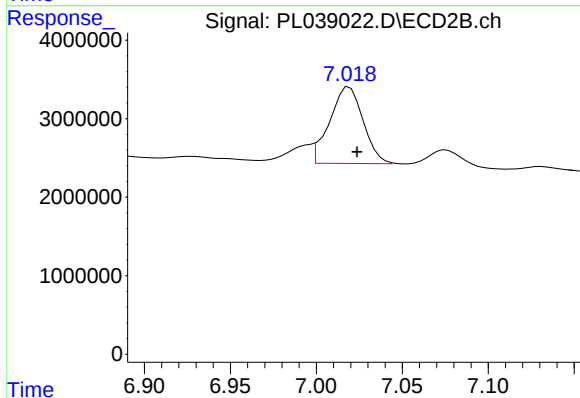


#17 4,4'-DDT

R.T.: 7.018 min
Delta R.T.: -0.006 min
Response: 13047596
Conc: 6.12 ng/ml m

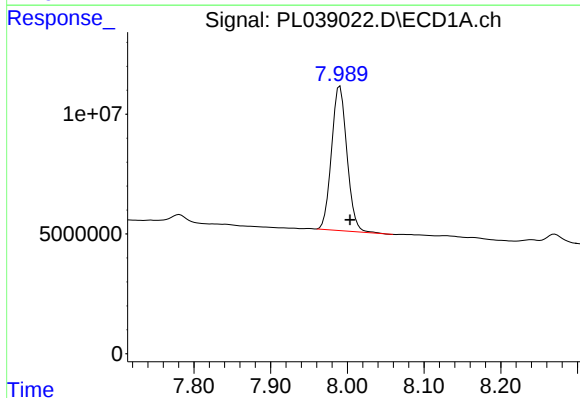

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.013 min
Response: 84124223
Conc: 11.09 ng/ml

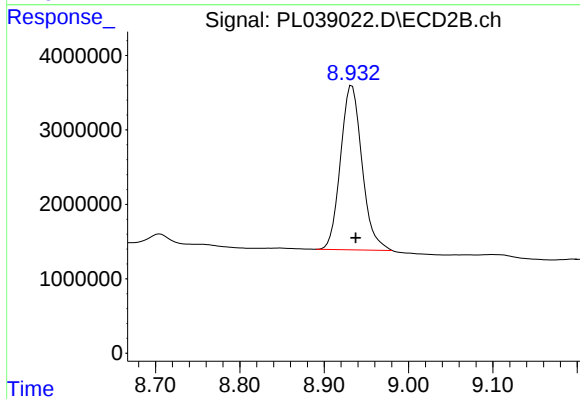

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 39079676
Conc: 15.99 ng/ml