

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
 Data File : PL039032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2018 17:07
 Operator : AJ\SJ
 Sample : PB111859BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB111859BS

Manual Integrations
 APPROVED

Sohil
 8/9/2018 9:58:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:05:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	116.1E6	45513306	15.592	17.339
2)	SA Decachlor...	7.990	8.933	89683865	39535665	11.822	16.174 #
Target Compounds							
2)	A alpha-BHC	3.753	4.306	504.8E6	189.6E6	42.728	48.983
3)	MA gamma-BHC...	4.027	4.585	460.2E6	170.8E6	43.896m	47.288
4)	MA Heptachlor	4.311	5.096	460.1E6	162.3E6	43.256	50.794
5)	MB Aldrin	4.550	5.397	451.2E6	149.1E6	43.104	48.313
6)	B beta-BHC	4.283	4.748	205.0E6	76793381	43.422	50.626
7)	B delta-BHC	4.476	4.962	478.8E6	167.3E6	44.110	50.440
8)	B Heptachlo...	4.986	5.778	410.1E6	132.3E6	43.498m	46.562
9)	A Endosulfan I	5.318	6.130	382.6E6	116.6E6	44.235	45.354
10)	B gamma-Chl...	5.209	6.010	425.4E6	130.7E6	43.037	45.069
11)	B alpha-Chl...	5.266	6.084	409.8E6	129.4E6	43.291	45.149
12)	B 4,4'-DDE	5.433	6.239	409.9E6	123.1E6	42.749m	46.036
13)	MA Dieldrin	5.557	6.382	406.4E6	119.1E6	42.292	43.775m
14)	MA Endrin	5.810	6.597	338.0E6	100.1E6	38.906	41.898m
15)	B Endosulfa...	6.084	6.802	321.9E6	98653484	40.595m	41.082
16)	A 4,4'-DDD	5.946	6.722	301.2E6	88620861	41.062	41.403
17)	MA 4,4'-DDT	6.179	7.020	286.0E6	88578484	38.496	41.546
18)	B Endrin al...	6.253	6.925	259.4E6	85491921	40.740	43.811
19)	B Endosulfa...	6.464	7.147	306.0E6	95265283	40.510	43.704
20)	A Methoxychlor	6.728	7.476	150.3E6	49228098	39.064	43.233
21)	B Endrin ke...	6.947	7.611	309.7E6	98145183	39.478	41.176

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080818\
Data File : PL039032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2018 17:07
Operator : AJ\SJ
Sample : PB111859BS
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:05:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

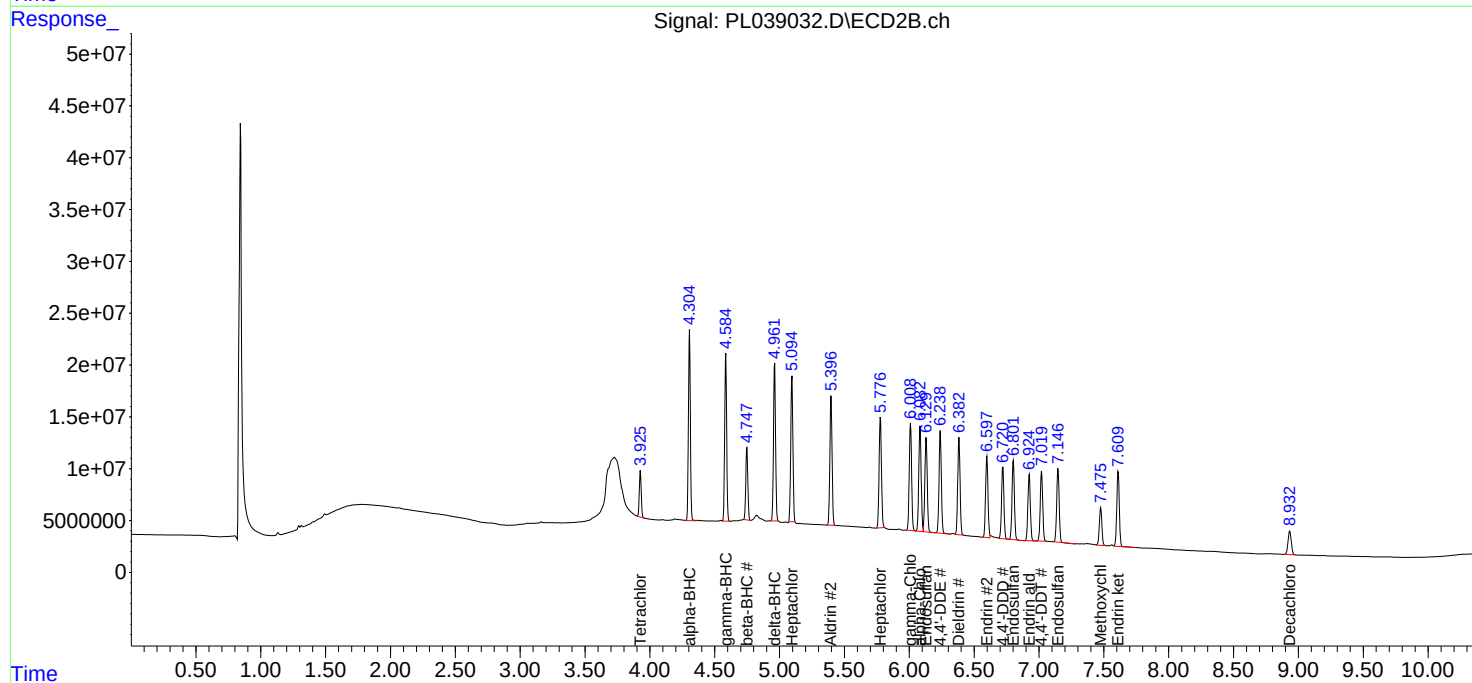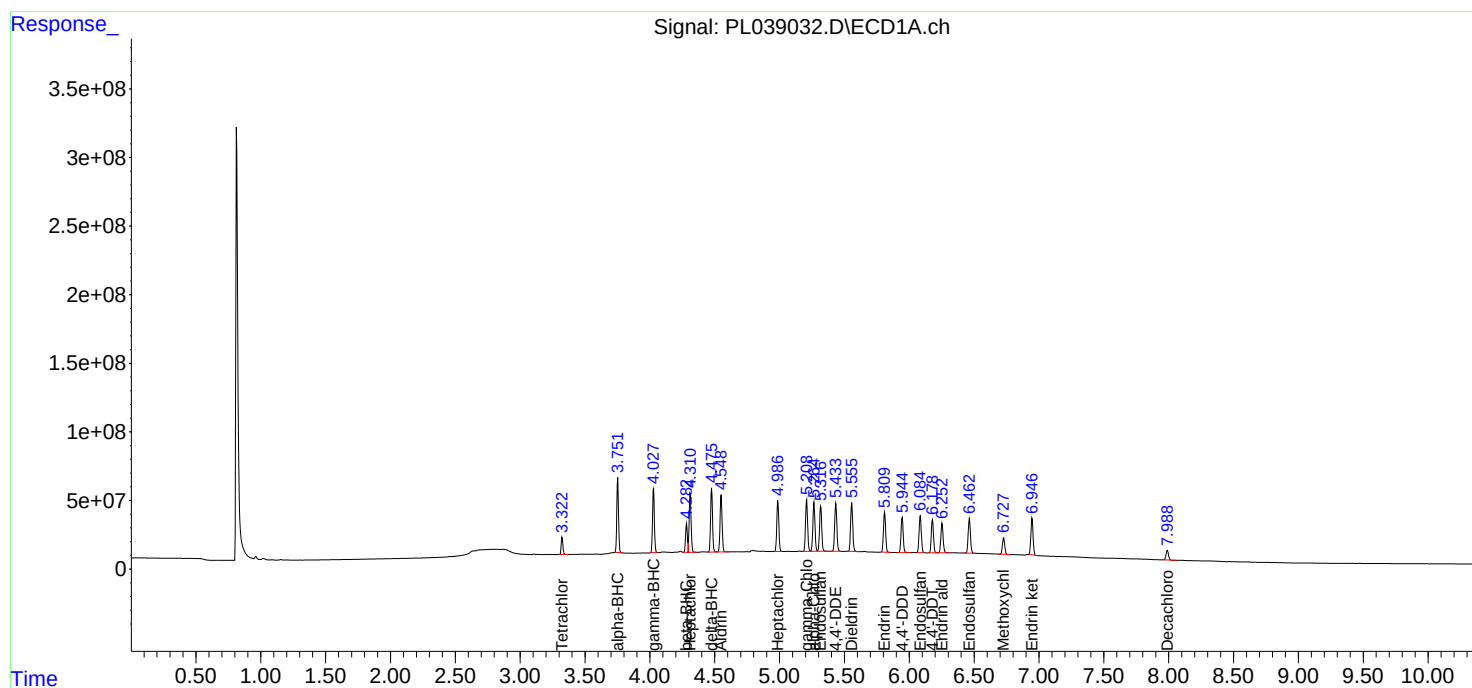

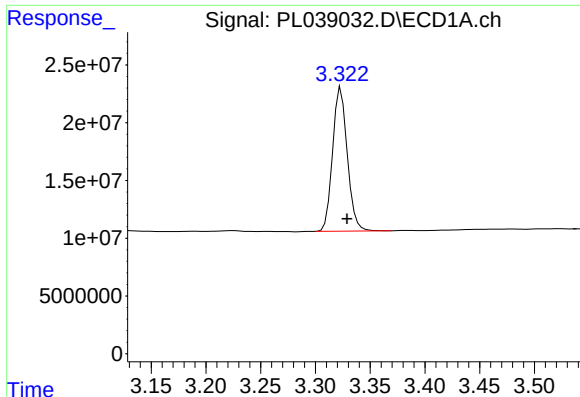


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 116103872
Conc: 15.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

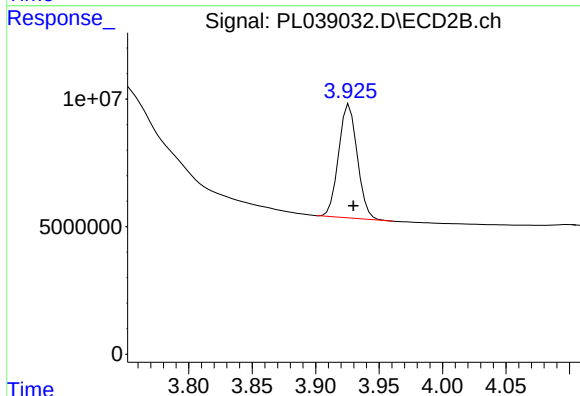


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 45513306
Conc: 17.34 ng/ml

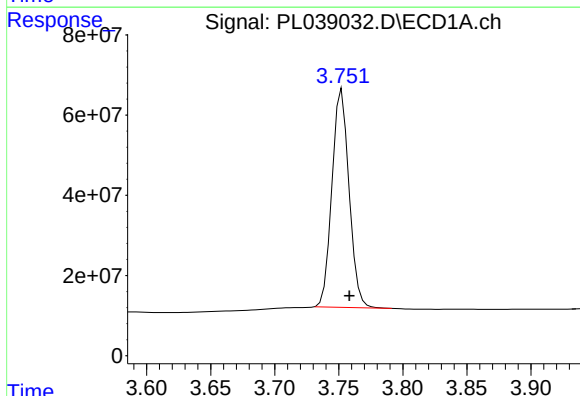


#2 alpha-BHC

R.T.: 3.753 min
Delta R.T.: -0.006 min
Response: 504845186
Conc: 42.73 ng/ml

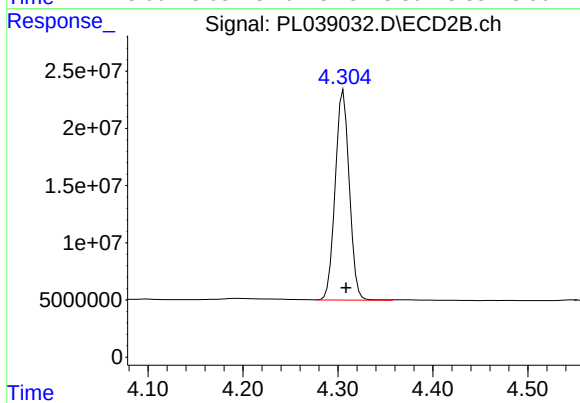

#2 alpha-BHC

R.T.: 4.306 min
Delta R.T.: -0.003 min
Response: 189572500
Conc: 48.98 ng/ml

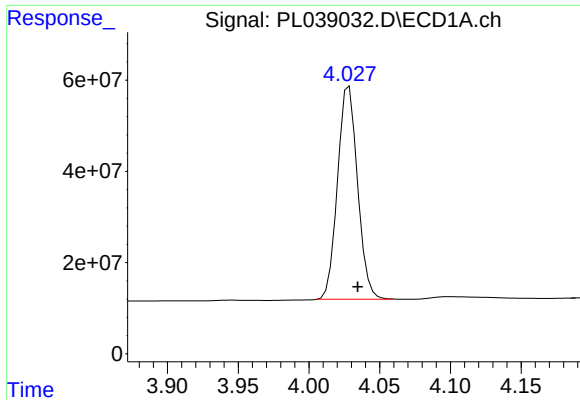


#3 gamma-BHC (Lindane)

R.T.: 4.027 min
Delta R.T.: -0.007 min
Response: 460197871
Conc: 43.90 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

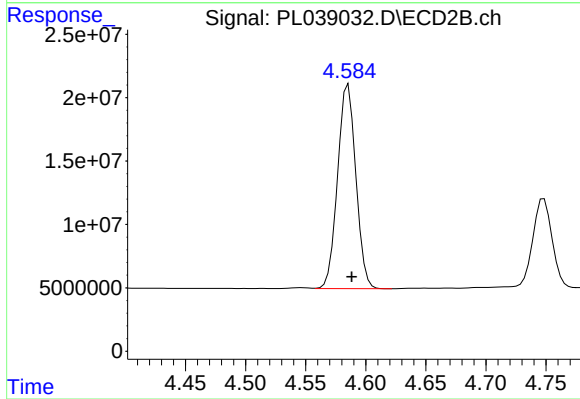


#3 gamma-BHC (Lindane)

R.T.: 4.585 min
Delta R.T.: -0.003 min
Response: 170794016
Conc: 47.29 ng/ml

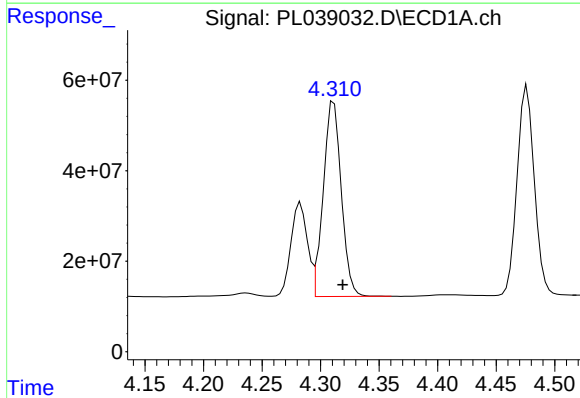


#4 Heptachlor

R.T.: 4.311 min
Delta R.T.: -0.008 min
Response: 460129739
Conc: 43.26 ng/ml

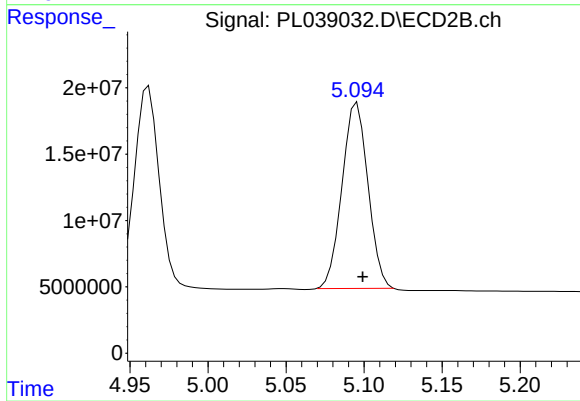

#4 Heptachlor

R.T.: 5.096 min
Delta R.T.: -0.004 min
Response: 162349462
Conc: 50.79 ng/ml

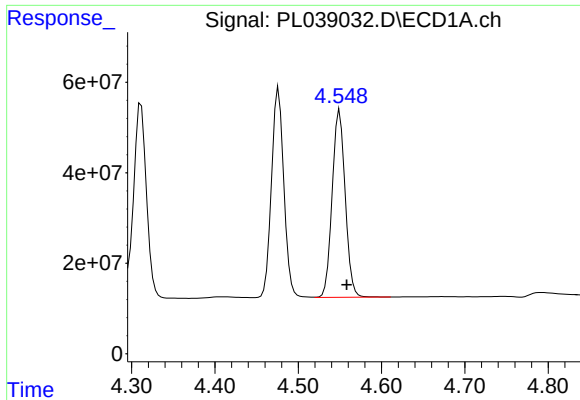

#5 Aldrin

R.T.: 4.550 min

Delta R.T.: -0.009 min


Response: 451180662

Conc: 43.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS

Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

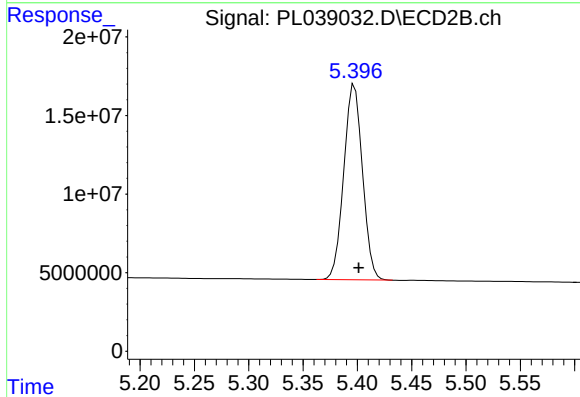


#5 Aldrin

R.T.: 5.397 min

Delta R.T.: -0.004 min

Response: 149104057

Conc: 48.31 ng/ml

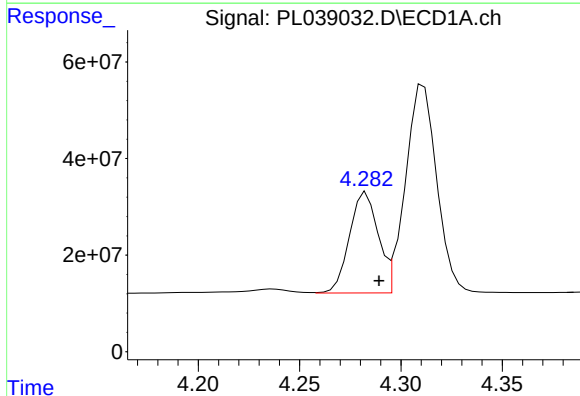


#6 beta-BHC

R.T.: 4.283 min

Delta R.T.: -0.006 min

Response: 204967065

Conc: 43.42 ng/ml

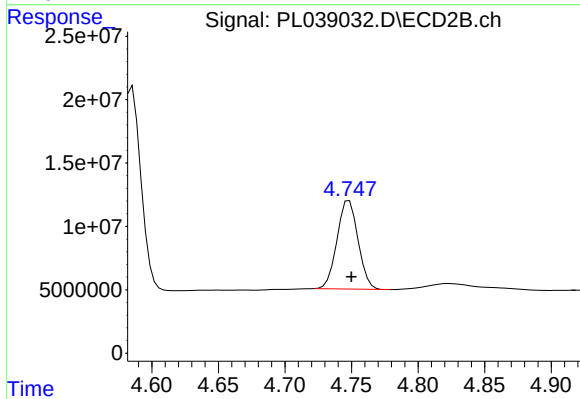


#6 beta-BHC

R.T.: 4.748 min

Delta R.T.: -0.002 min

Response: 76793381

Conc: 50.63 ng/ml

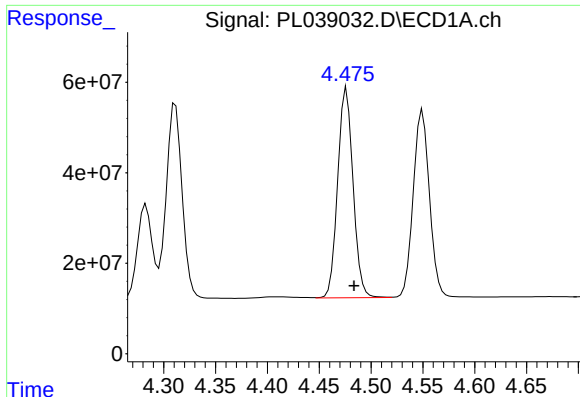


#7 delta-BHC

R.T.: 4.476 min
Delta R.T.: -0.007 min
Response: 478782594
Conc: 44.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

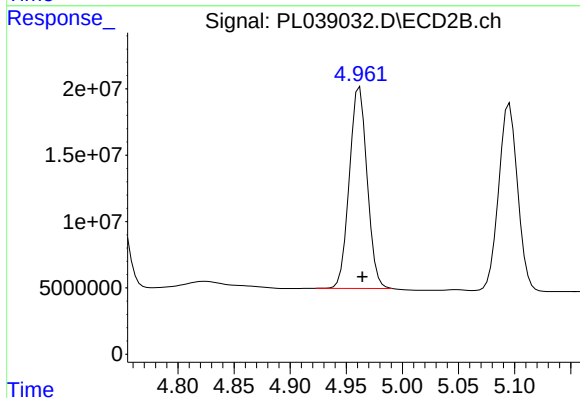


#7 delta-BHC

R.T.: 4.962 min
Delta R.T.: -0.002 min
Response: 167289250
Conc: 50.44 ng/ml

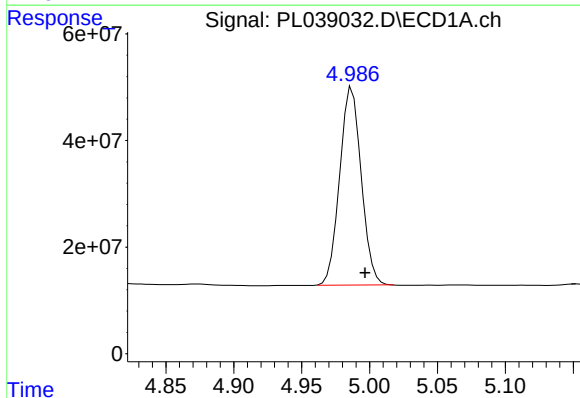


#8 Heptachlor epoxide

R.T.: 4.986 min
Delta R.T.: -0.011 min
Response: 410116461
Conc: 43.50 ng/ml m

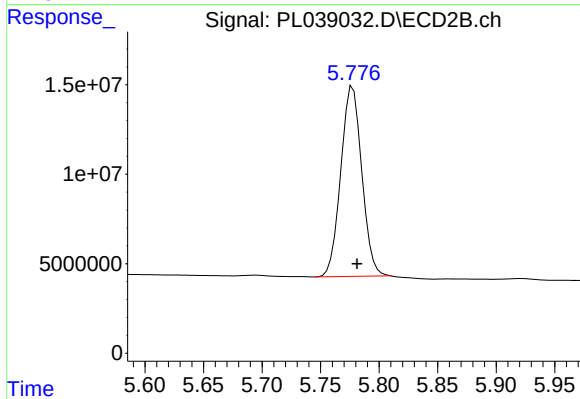

#8 Heptachlor epoxide

R.T.: 5.778 min
Delta R.T.: -0.004 min
Response: 132325744
Conc: 46.56 ng/ml

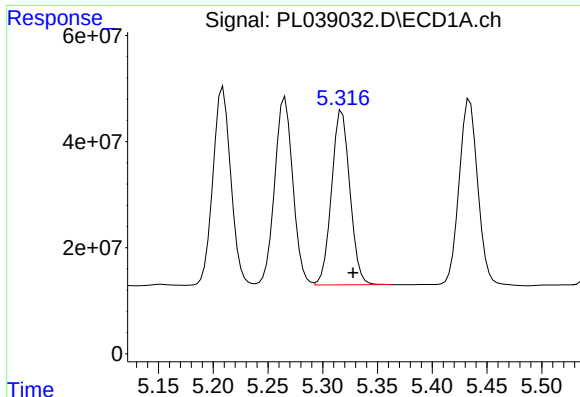


#9 Endosulfan I

R.T.: 5.318 min
Delta R.T.: -0.010 min
Response: 382618228
Conc: 44.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

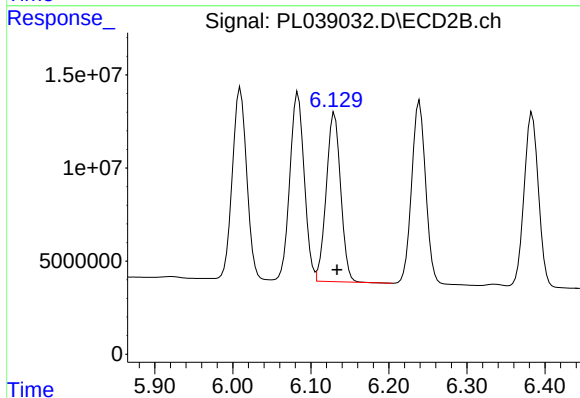


#9 Endosulfan I

R.T.: 6.130 min
Delta R.T.: -0.003 min
Response: 116640805
Conc: 45.35 ng/ml

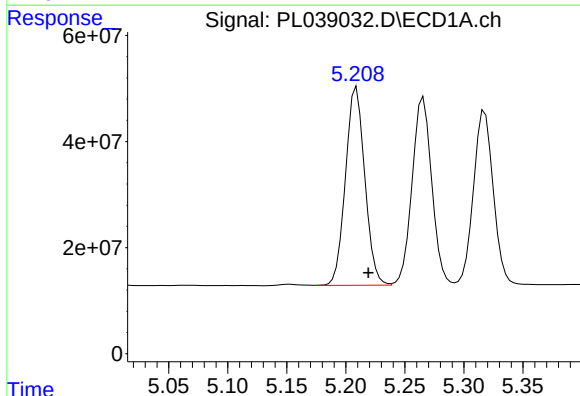


#10 gamma-Chlordane

R.T.: 5.209 min
Delta R.T.: -0.010 min
Response: 425377488
Conc: 43.04 ng/ml

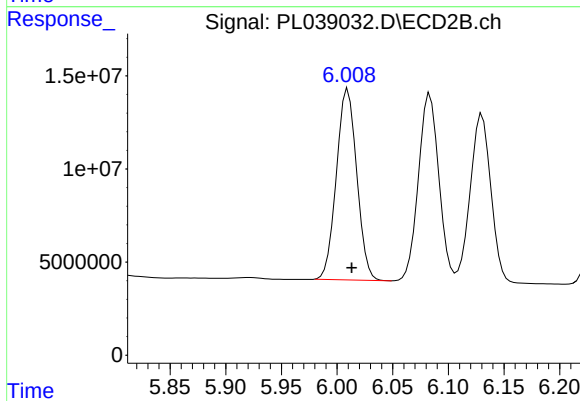

#10 gamma-Chlordane

R.T.: 6.010 min
Delta R.T.: -0.003 min
Response: 130664119
Conc: 45.07 ng/ml

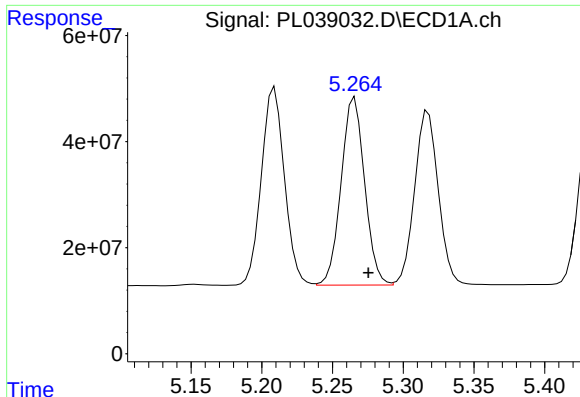


#11 alpha-Chlordane

R.T.: 5.266 min
Delta R.T.: -0.010 min
Response: 409783945
Conc: 43.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

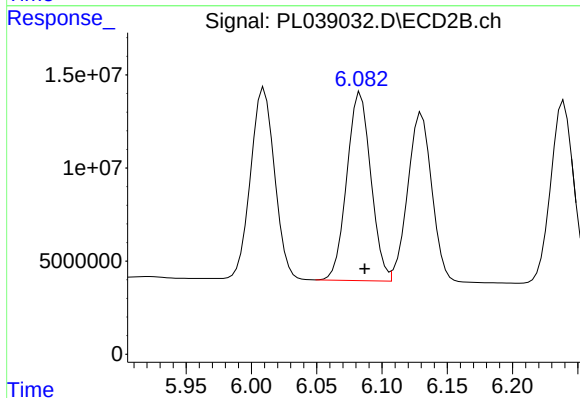


#11 alpha-Chlordane

R.T.: 6.084 min
Delta R.T.: -0.003 min
Response: 129407423
Conc: 45.15 ng/ml

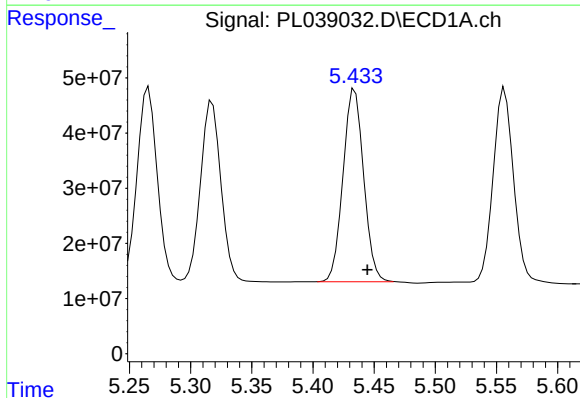


#12 4,4'-DDE

R.T.: 5.433 min
Delta R.T.: -0.012 min
Response: 409870904
Conc: 42.75 ng/ml m

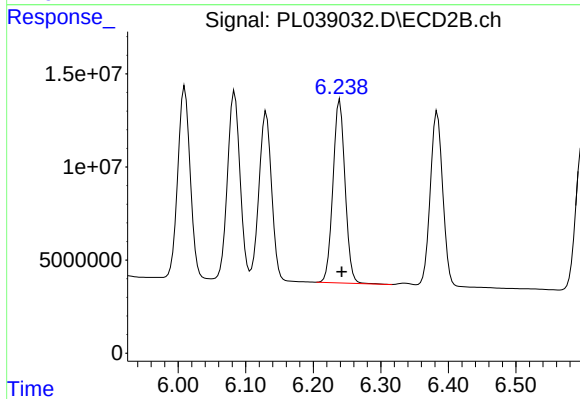

#12 4,4'-DDE

R.T.: 6.239 min
Delta R.T.: -0.003 min
Response: 123103581
Conc: 46.04 ng/ml

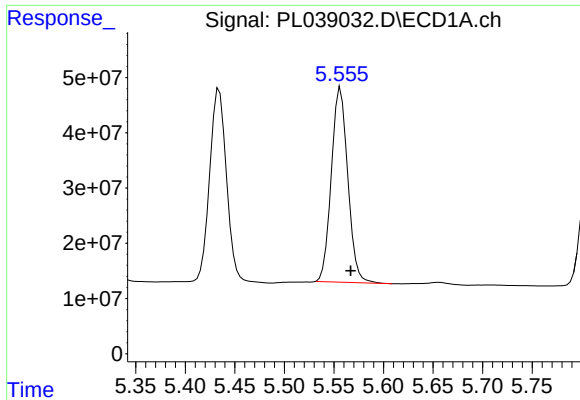


#13 Dieldrin

R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 406436147
Conc: 42.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

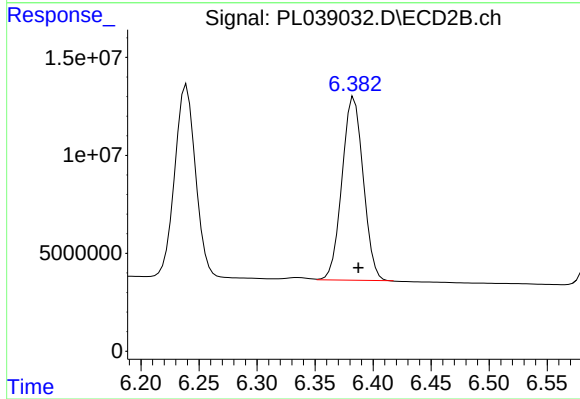


#13 Dieldrin

R.T.: 6.382 min
Delta R.T.: -0.005 min
Response: 119145361
Conc: 43.77 ng/ml m

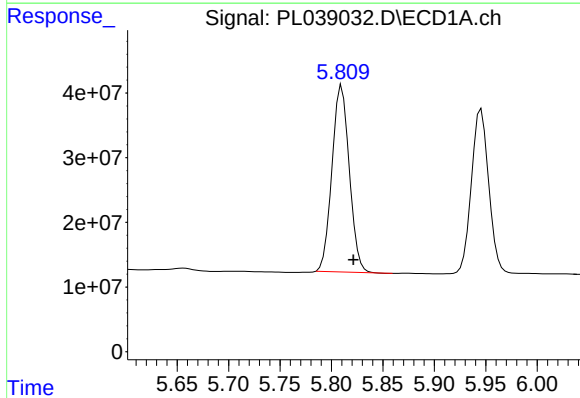


#14 Endrin

R.T.: 5.810 min
Delta R.T.: -0.011 min
Response: 338030950
Conc: 38.91 ng/ml

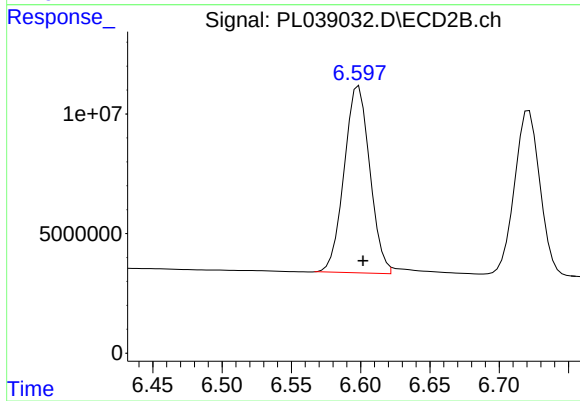

#14 Endrin

R.T.: 6.597 min
Delta R.T.: -0.005 min
Response: 100058129
Conc: 41.90 ng/ml m

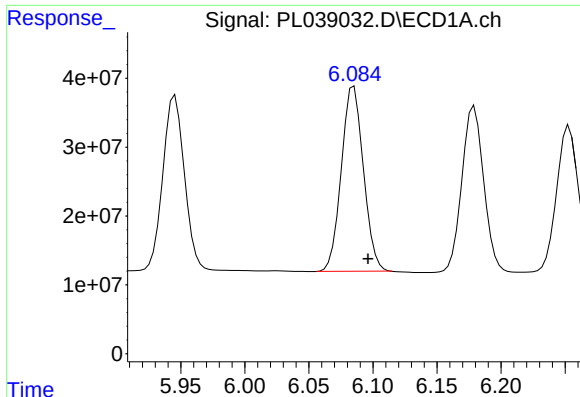


#15 Endosulfan II

R.T.: 6.084 min
Delta R.T.: -0.012 min
Response: 321925547
Conc: 40.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

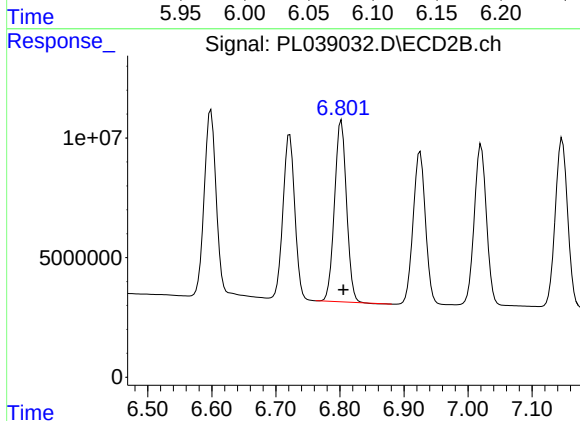


#15 Endosulfan II

R.T.: 6.802 min
Delta R.T.: -0.003 min
Response: 98653484
Conc: 41.08 ng/ml

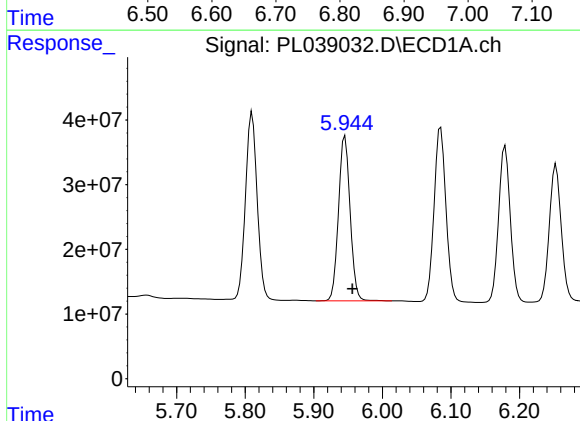


#16 4,4'-DDD

R.T.: 5.946 min
Delta R.T.: -0.011 min
Response: 301213992
Conc: 41.06 ng/ml

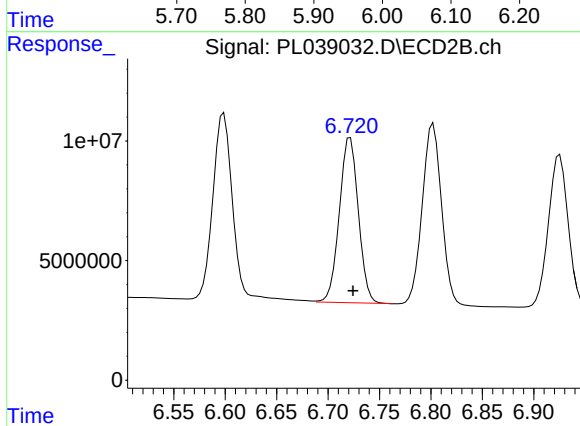

#16 4,4'-DDD

R.T.: 6.722 min
Delta R.T.: -0.003 min
Response: 88620861
Conc: 41.40 ng/ml

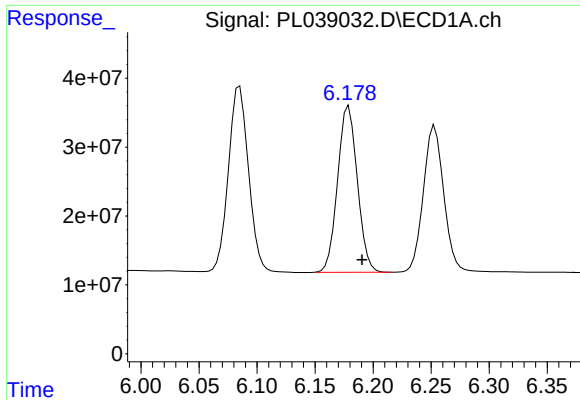


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: -0.011 min
Response: 285975624
Conc: 38.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

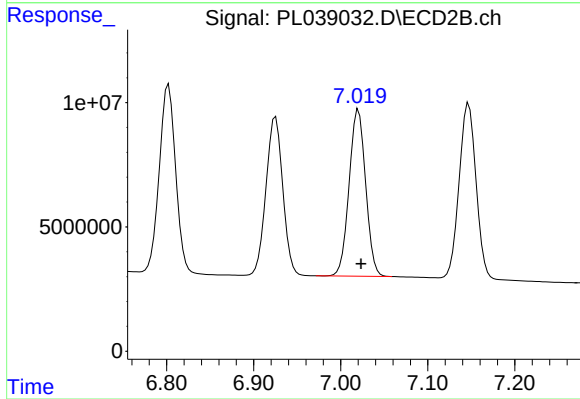


#17 4,4'-DDT

R.T.: 7.020 min
Delta R.T.: -0.003 min
Response: 88578484
Conc: 41.55 ng/ml

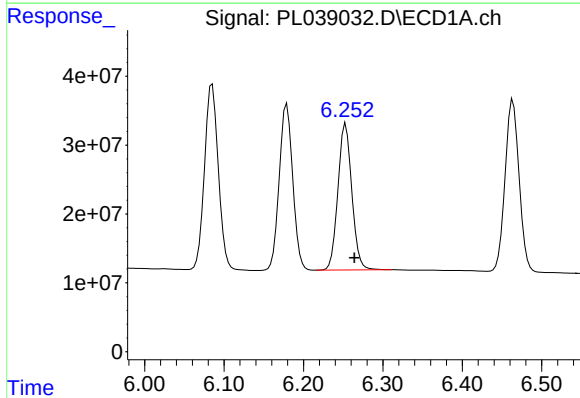


#18 Endrin aldehyde

R.T.: 6.253 min
Delta R.T.: -0.011 min
Response: 259413898
Conc: 40.74 ng/ml

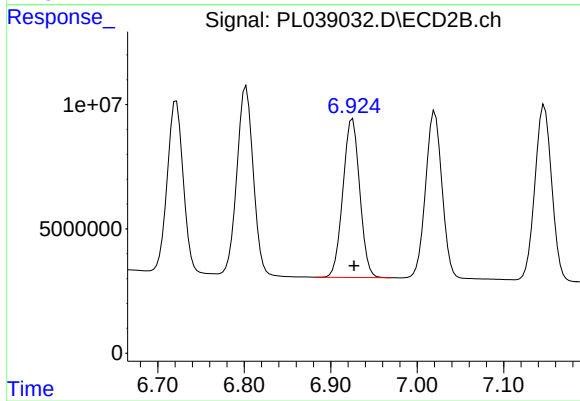

#18 Endrin aldehyde

R.T.: 6.925 min
Delta R.T.: -0.002 min
Response: 85491921
Conc: 43.81 ng/ml

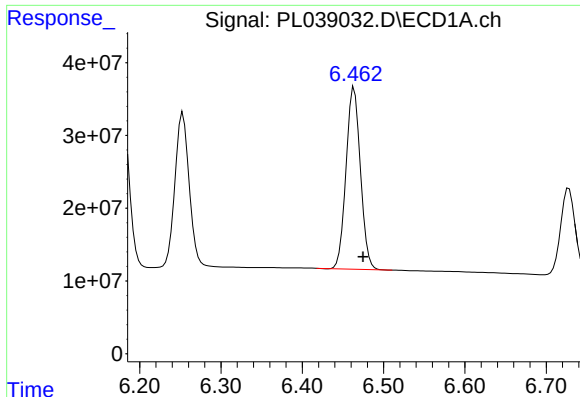


#19 Endosulfan Sulfate

R.T.: 6.464 min
Delta R.T.: -0.011 min
Response: 305987664
Conc: 40.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

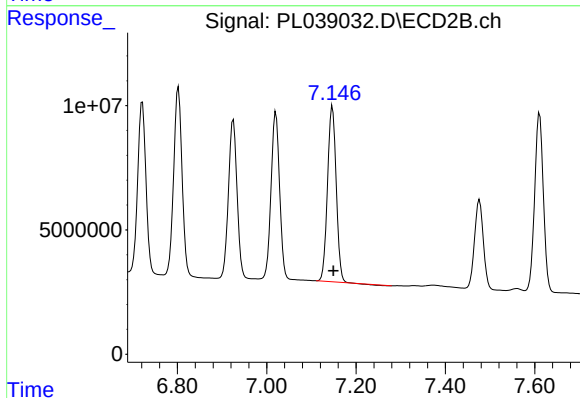


#19 Endosulfan Sulfate

R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 95265283
Conc: 43.70 ng/ml

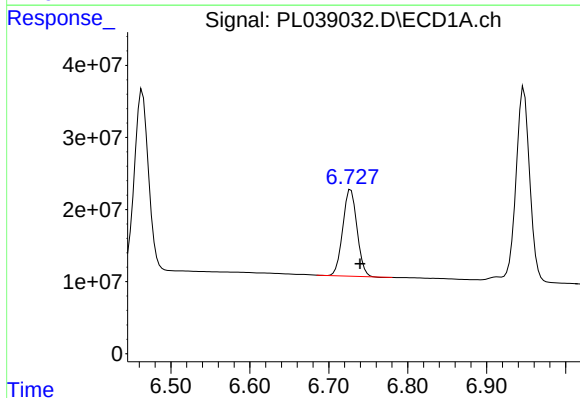


#20 Methoxychlor

R.T.: 6.728 min
Delta R.T.: -0.012 min
Response: 150296544
Conc: 39.06 ng/ml

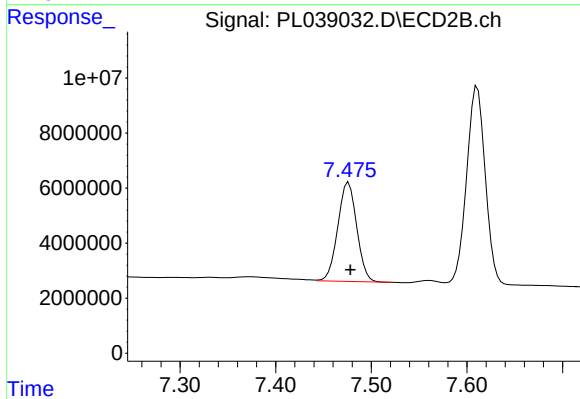

#20 Methoxychlor

R.T.: 7.476 min
Delta R.T.: -0.002 min
Response: 49228098
Conc: 43.23 ng/ml

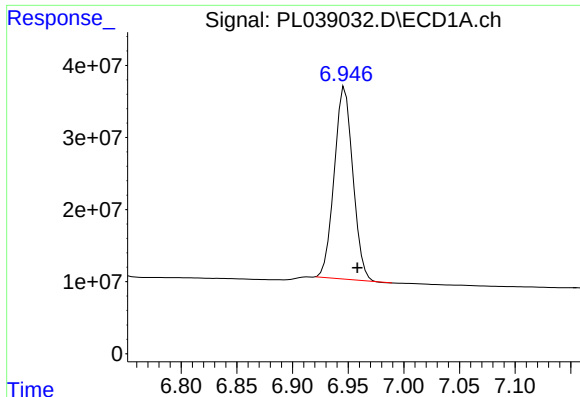


#21 Endrin ketone

R.T.: 6.947 min
Delta R.T.: -0.011 min
Response: 309745107
Conc: 39.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111859BS


Manual Integrations
APPROVED

Sohil
8/9/2018 9:58:28 AM

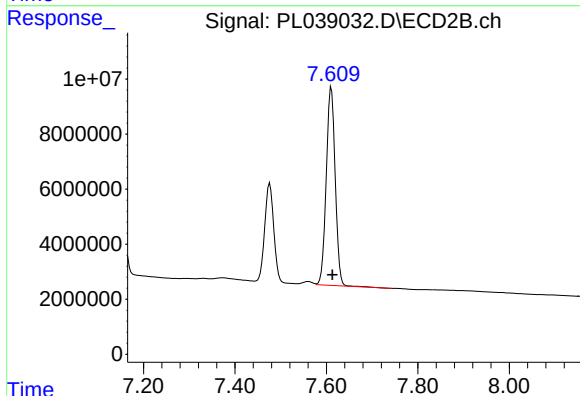


#21 Endrin ketone

R.T.: 7.611 min
Delta R.T.: -0.002 min
Response: 98145183
Conc: 41.18 ng/ml

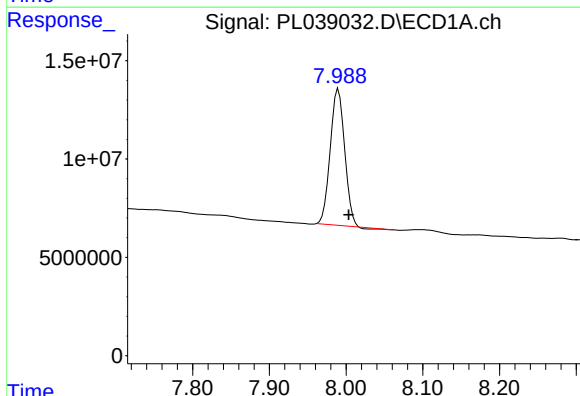

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 89683865
Conc: 11.82 ng/ml

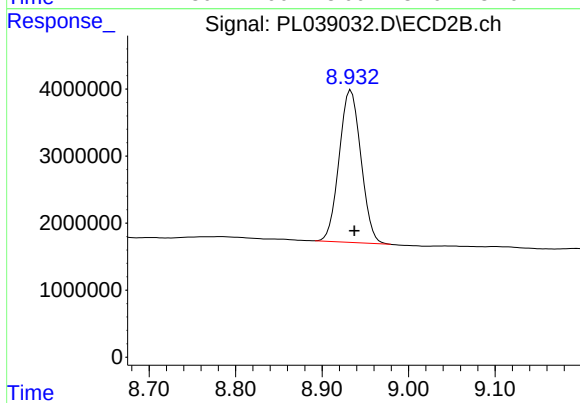

#28 Decachlorobiphenyl

R.T.: 8.933 min
Delta R.T.: -0.004 min
Response: 39535665
Conc: 16.17 ng/ml