

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080819\
 Data File : PL051196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 01:52
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 06:38:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.008f	5.790	2469650	17081818	0.167 4.466 #
9) A	Endosulfan I	5.335f	0.000	15126871	0	1.040 N.D. #
10) B	gamma-Chl...	5.198	0.000	84810532	0	5.373 N.D. #
11) B	alpha-Chl...	5.235f	0.000	185.9E6	0	12.184 N.D. #
13) MA	Dieldrin	5.527f	0.000	9965019	0	0.643 N.D. #
14) MA	Endrin	0.000	6.623	0	6968823	N.D. 2.247 #
17) MA	4,4'-DDT	6.197f	0.000	210.7E6	0	17.014 N.D. #
25)	Chlordane-3	5.198	0.000	84810532	0	60.588 N.D. #
26)	Chlordane-4	5.235f	0.000	185.9E6	0	140.932 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080819\
Data File : PL051196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 01:52
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 06:38:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

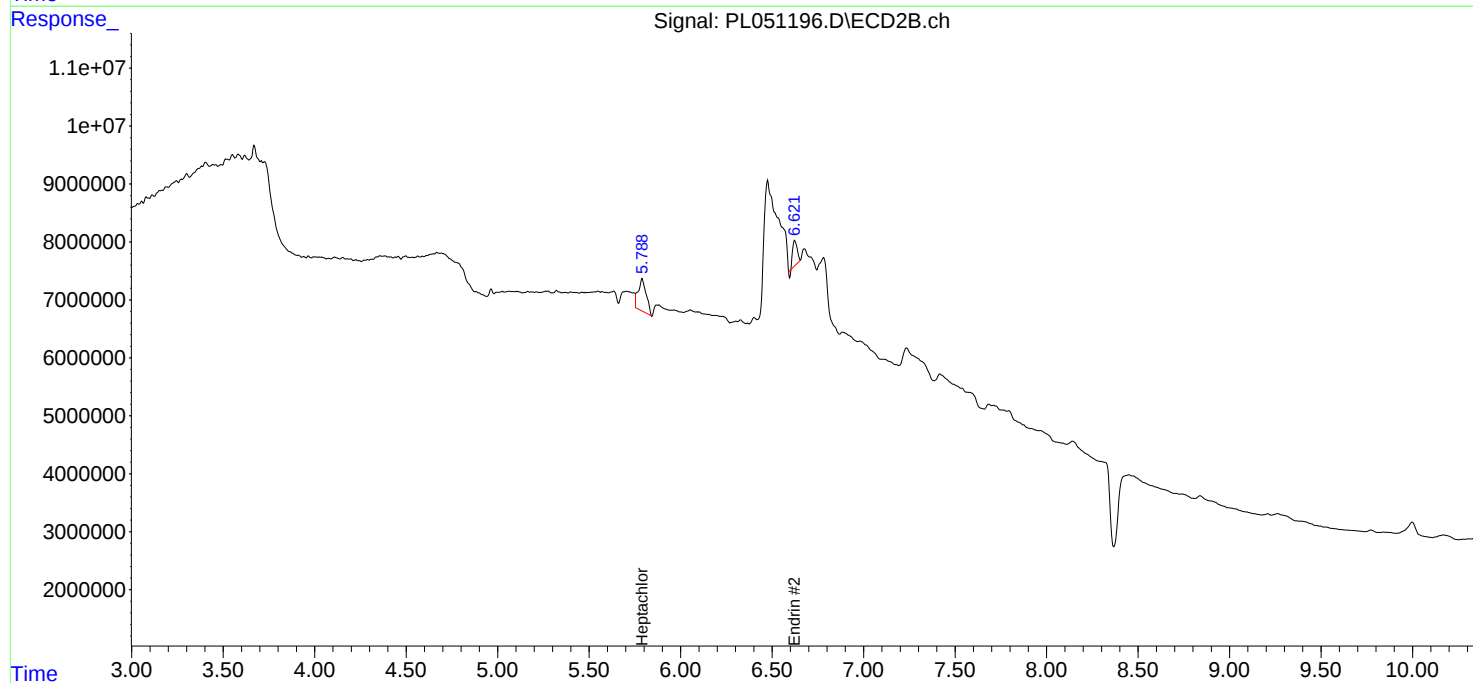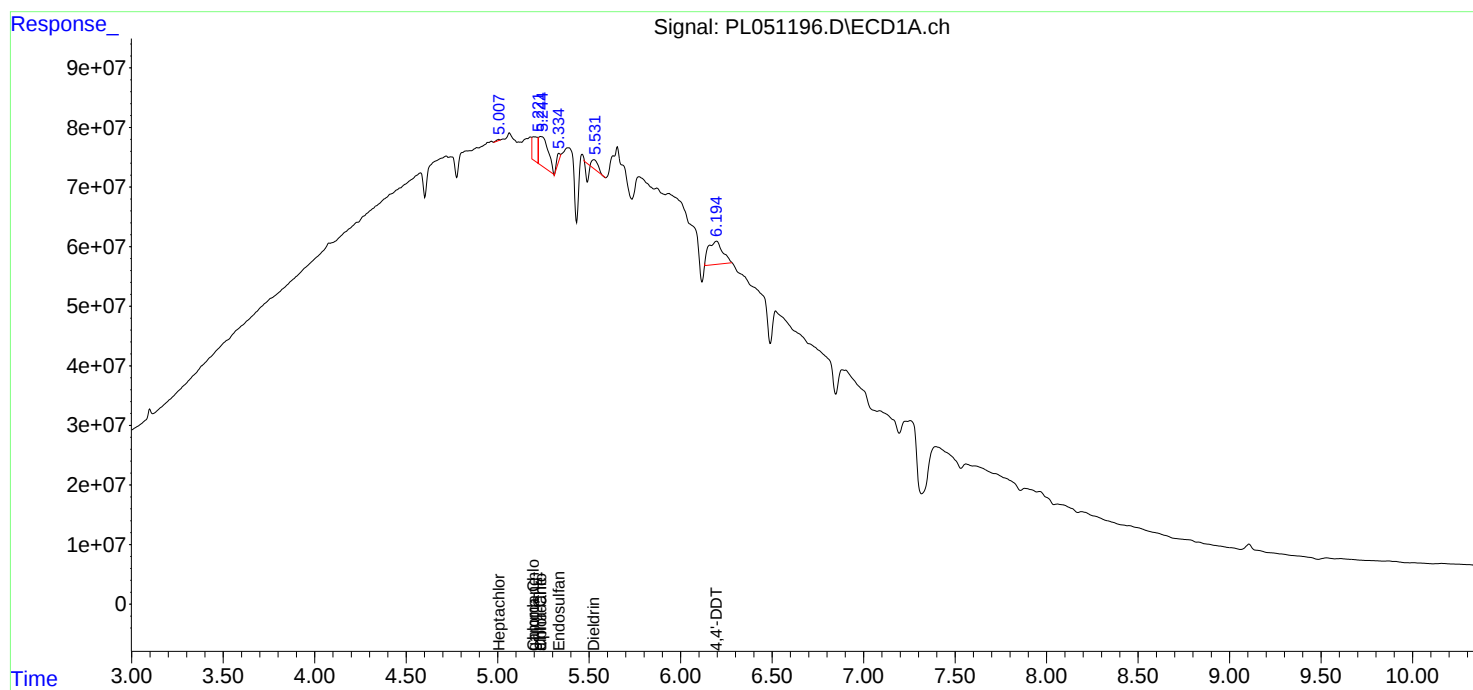


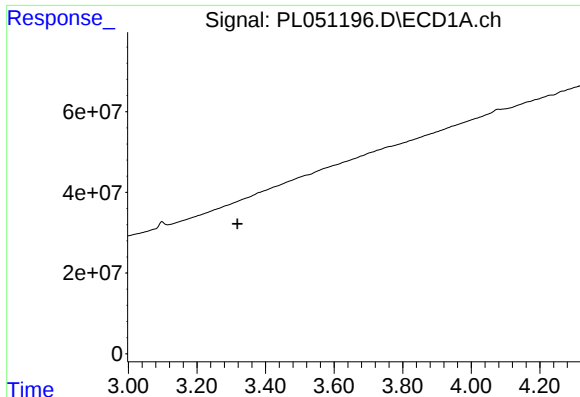

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

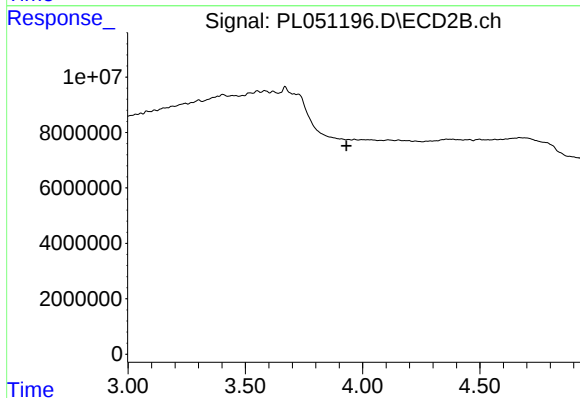


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

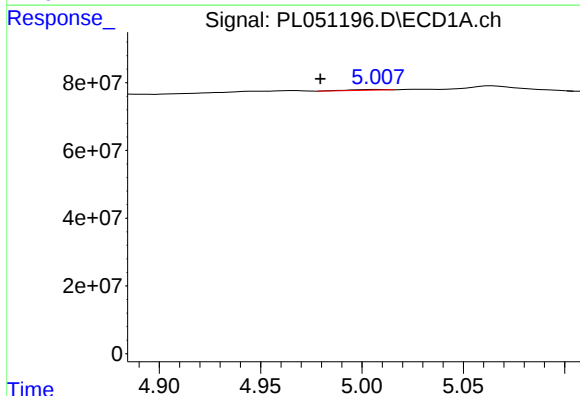


#8 Heptachlor epoxide

R.T.: 5.008 min
Delta R.T.: 0.028 min
Response: 2469650
Conc: 0.17 ng/ml

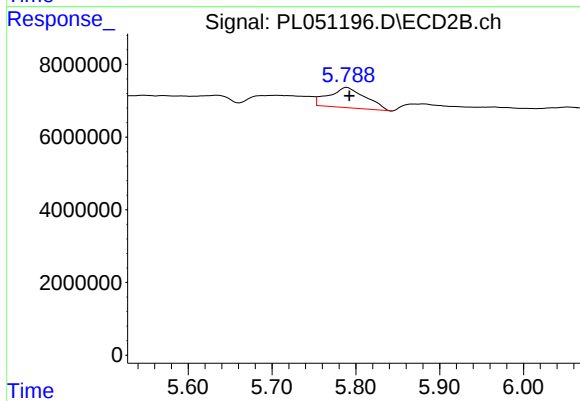

#8 Heptachlor epoxide


R.T.: 5.790 min
Delta R.T.: -0.003 min
Response: 17081818
Conc: 4.47 ng/ml

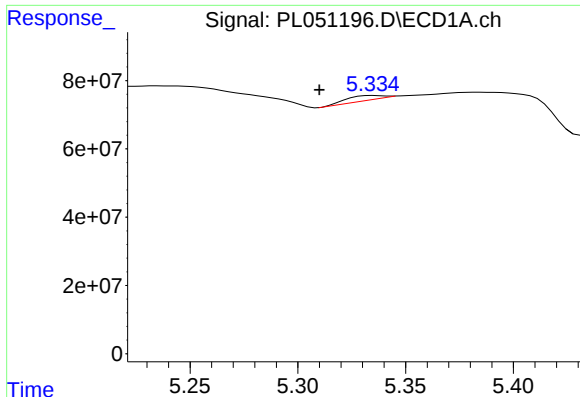

#9 Endosulfan I


R.T.: 5.335 min
Delta R.T.: 0.025 min
Response: 15126871
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

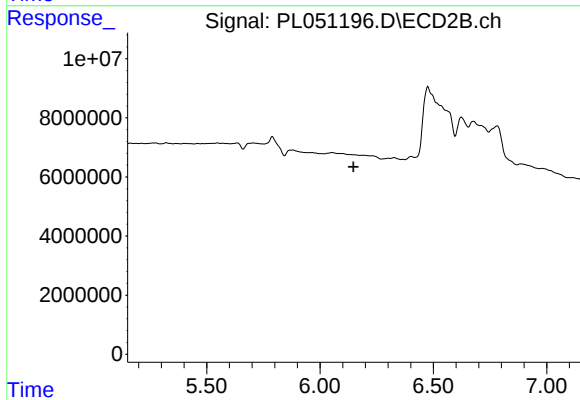


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

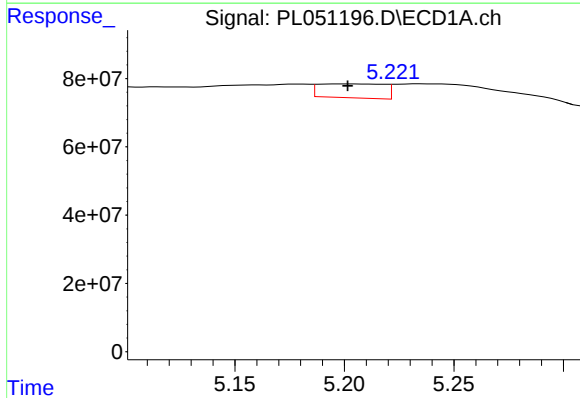


#10 gamma-Chlordane

R.T.: 5.198 min
Delta R.T.: -0.004 min
Response: 84810532
Conc: 5.37 ng/ml

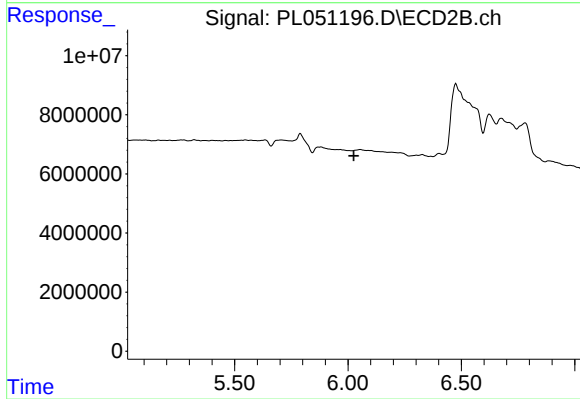

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

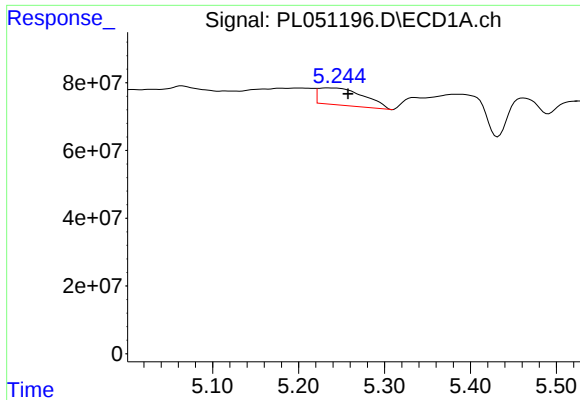

#11 alpha-Chlordane


R.T.: 5.235 min
Delta R.T.: -0.023 min
Response: 185886068
Conc: 12.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

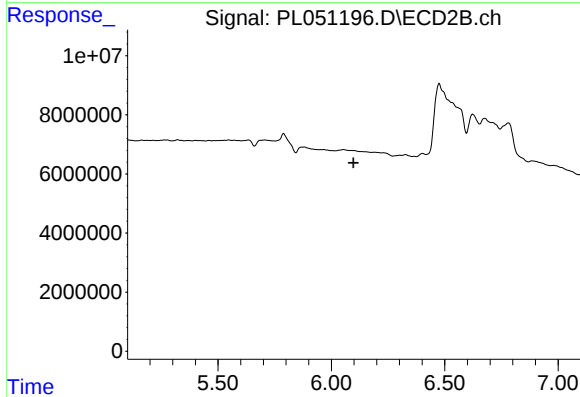


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

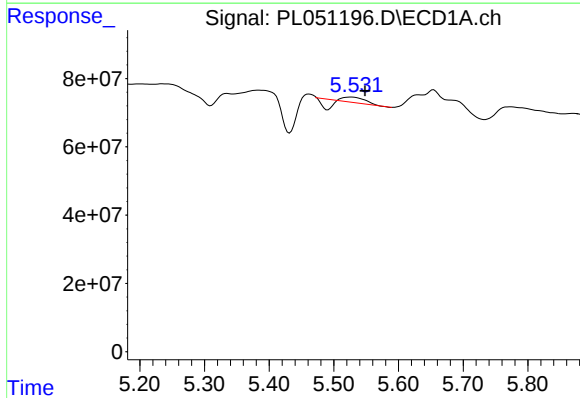


#13 Dieldrin

R.T.: 5.527 min
Delta R.T.: -0.022 min
Response: 9965019
Conc: 0.64 ng/ml

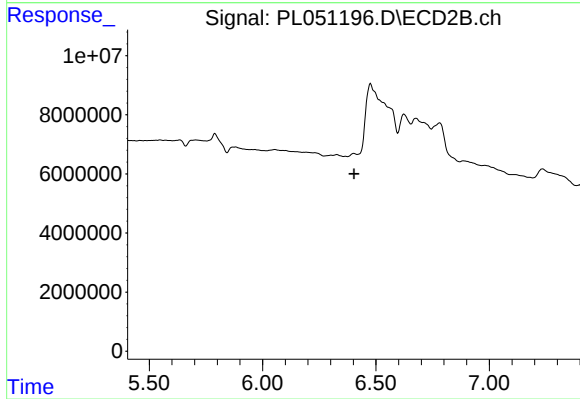

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

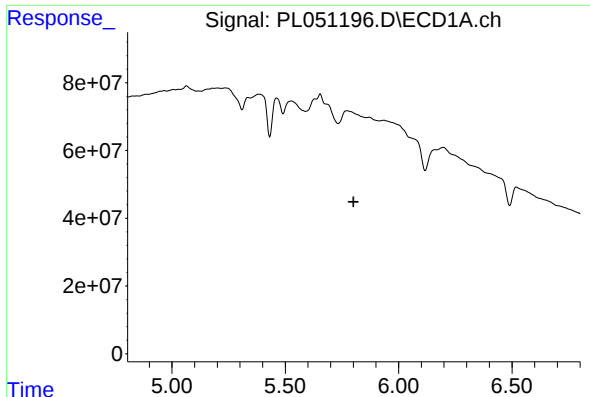

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

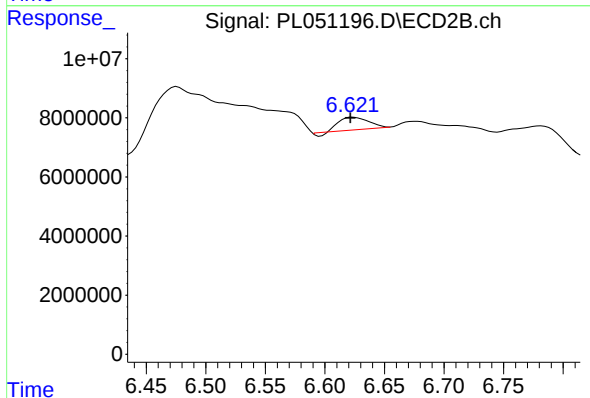


#14 Endrin

R.T.: 6.623 min
Delta R.T.: 0.002 min
Response: 6968823
Conc: 2.25 ng/ml

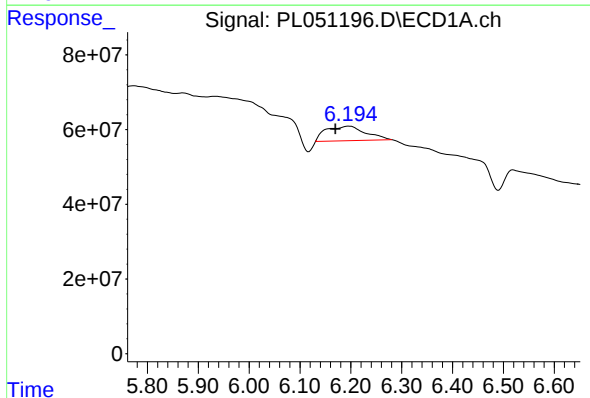


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.027 min
Response: 210736768
Conc: 17.01 ng/ml

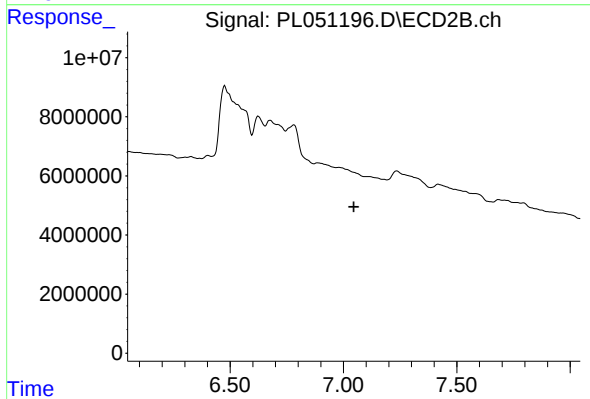

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.046 min
Response: 0
Conc: N.D.

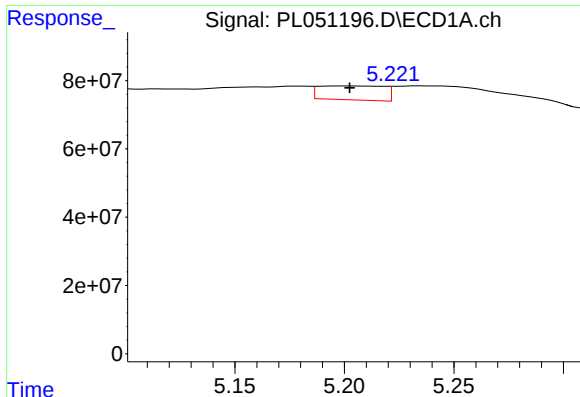

#25 Chlordane-3


R.T.: 5.198 min
Delta R.T.: -0.005 min
Response: 84810532
Conc: 60.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

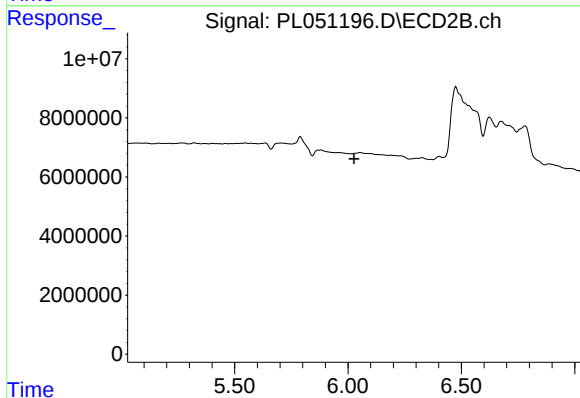


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

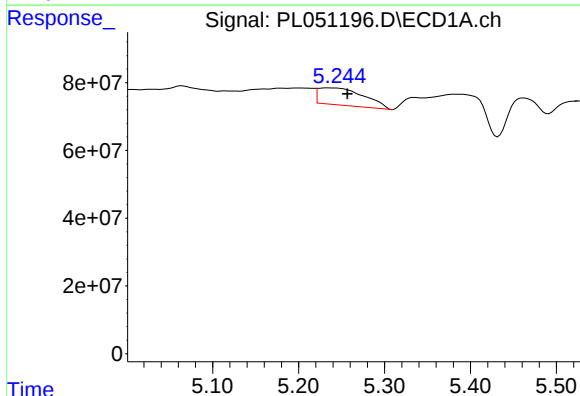


#26 Chlordane-4

R.T.: 5.235 min
Delta R.T.: -0.022 min
Response: 185886068
Conc: 140.93 ng/ml

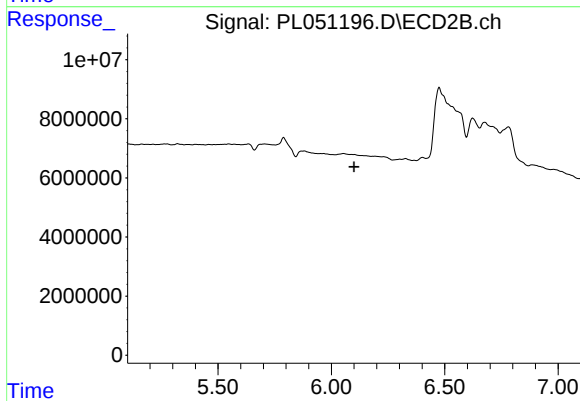

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

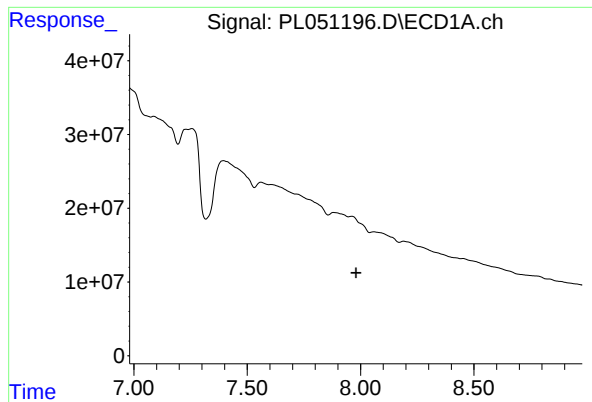

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

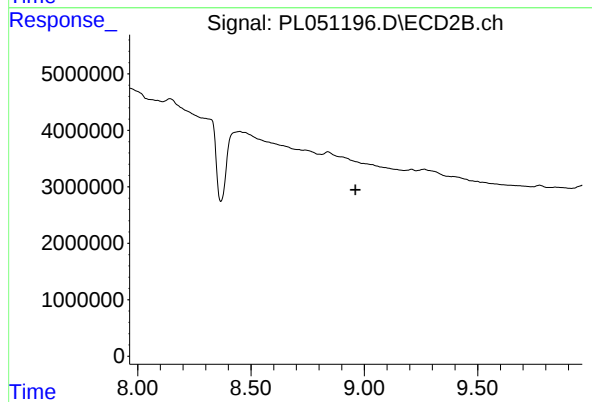

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.