

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 18:30
 Operator : AR\AJ
 Sample : PSTDICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 06:53:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 06:52:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.637	50269960	146.7E6	50.000	50.000
28)	SA Decachlor...	8.907	7.740	38138703	112.6E6	50.000	50.000
Target Compounds							
2)	A alpha-BHC	3.884	3.130	71894340	220.0E6	50.000	50.000
3)	MA gamma-BHC...	4.219	3.454	65930871	198.4E6	50.000	50.000
4)	MA Heptachlor	4.795	3.788	61982363	183.9E6	50.000	50.000
5)	MB Aldrin	5.136	4.062	58302997	182.6E6	50.000	50.000
6)	B beta-BHC	4.430	3.753	28863408	78835480	50.000	50.000
7)	B delta-BHC	4.674	3.977	59275760	197.8E6	50.000	50.000
8)	B Heptachlo...	5.568	4.561	50782879	155.3E6	50.000	50.000
9)	A Endosulfan I	5.954	4.927	46492607	139.2E6	50.000	50.000
10)	B gamma-Chl...	5.823	4.810	50931698	155.3E6	50.000	50.000
11)	B alpha-Chl...	5.900	4.873	50679184	151.2E6	50.000	50.000
12)	B 4,4'-DDE	6.080	5.067	44822329	147.2E6	50.000	50.000
13)	MA Dieldrin	6.231	5.190	49701189	152.7E6	50.000	50.000
14)	MA Endrin	6.463	5.462	41852829	129.1E6	50.000	50.000
15)	B Endosulfa...	6.691	5.758	43523117	128.7E6	50.000	50.000
16)	A 4,4'-DDD	6.604	5.619	37871228	114.9E6	50.000	50.000
17)	MA 4,4'-DDT	6.914	5.868	39794789	117.7E6	50.000	50.000
18)	B Endrin al...	6.821	5.937	36797292	99437005	50.000	50.000
19)	B Endosulfa...	7.054	6.160	42007966	116.9E6	50.000	50.000
20)	A Methoxychlor	7.395	6.446	22914413	61239254	50.000	50.000
21)	B Endrin ke...	7.543	6.660	46481501	130.1E6	50.000	50.000
22)	Mirex	8.003	6.837	35219687	95707135	50.000	50.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 18:30
Operator : AR\AJ
Sample : PSTDICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 06:53:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 06:52:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

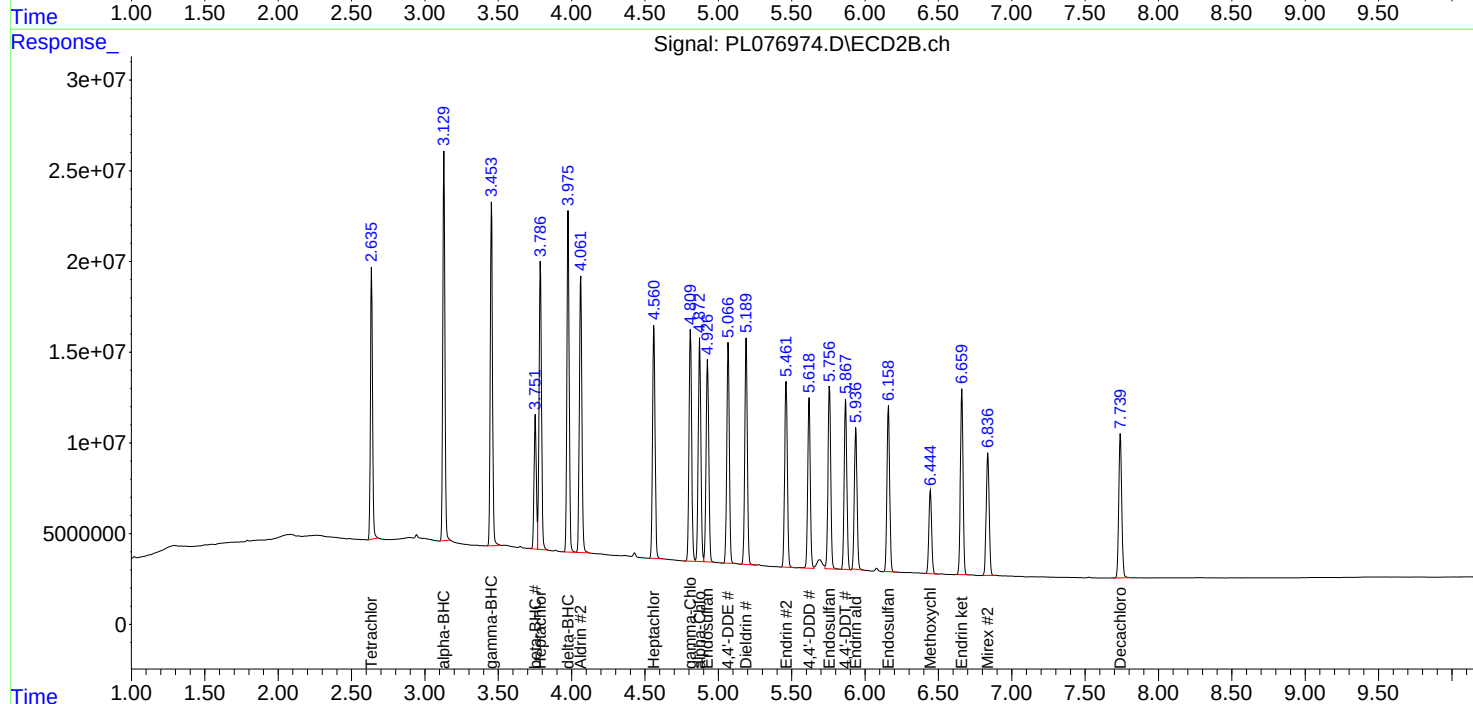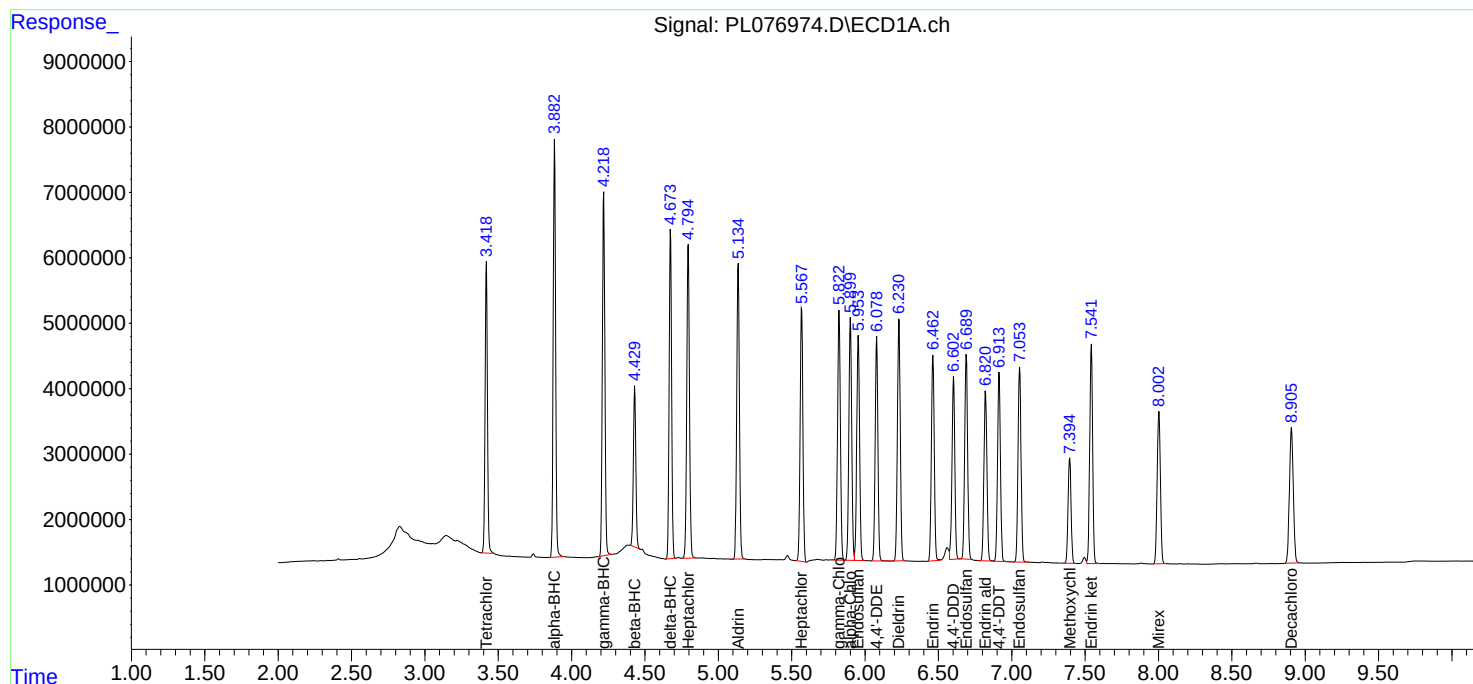


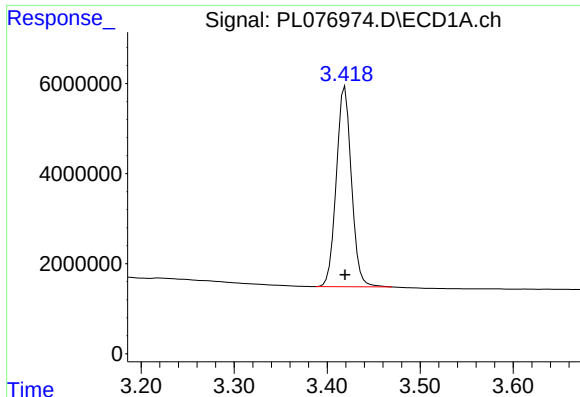

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 50269960
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

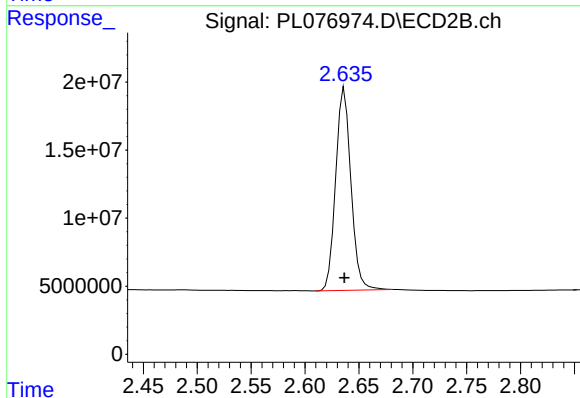


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 146707249
Conc: 50.00 ng/ml

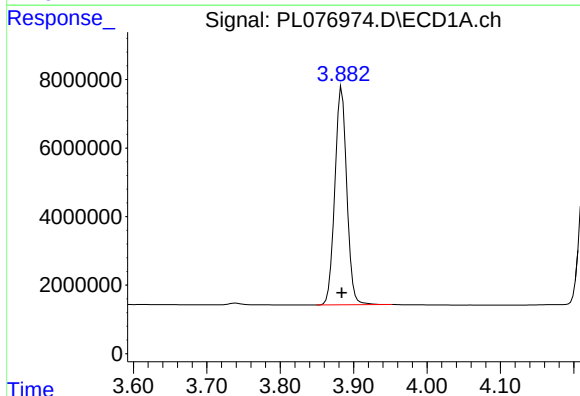


#2 alpha-BHC

R.T.: 3.884 min
Delta R.T.: 0.000 min
Response: 71894340
Conc: 50.00 ng/ml

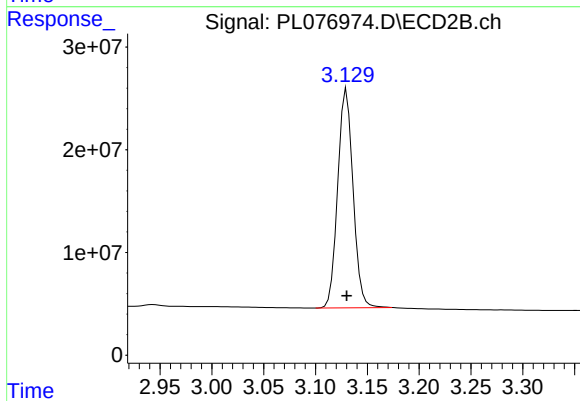

#2 alpha-BHC


R.T.: 3.130 min
Delta R.T.: 0.000 min
Response: 219962490
Conc: 50.00 ng/ml

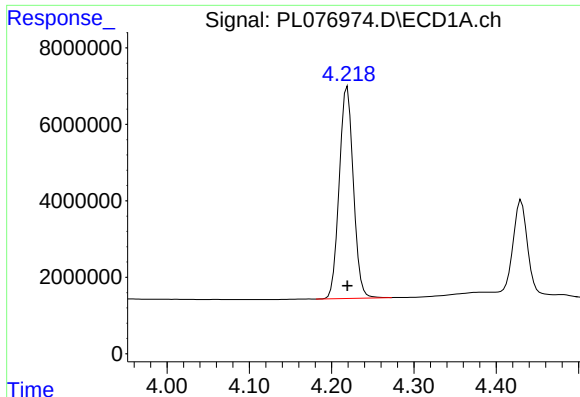

#3 gamma-BHC (Lindane)


R.T.: 4.219 min
Delta R.T.: 0.000 min
Response: 65930871
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

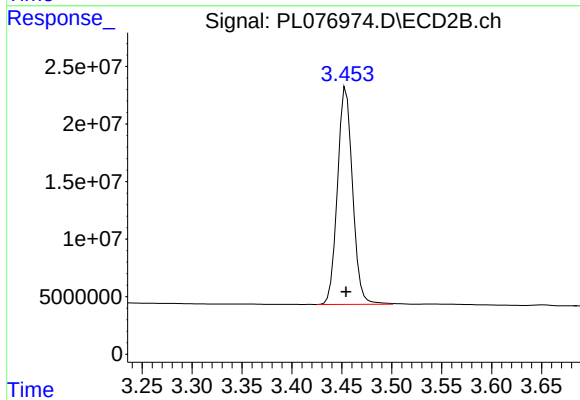


#3 gamma-BHC (Lindane)

R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 198410664
Conc: 50.00 ng/ml

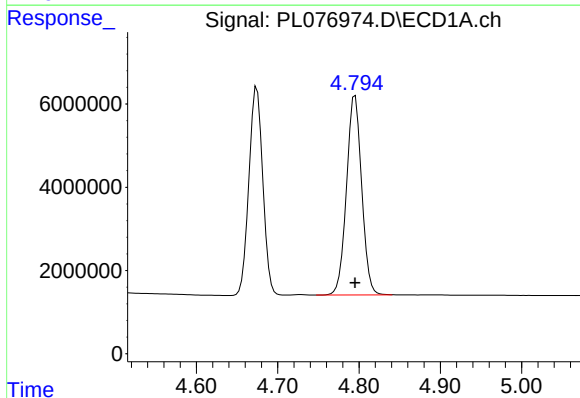


#4 Heptachlor

R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 61982363
Conc: 50.00 ng/ml

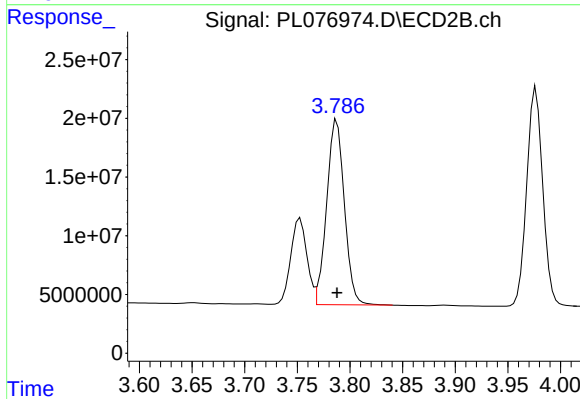

#4 Heptachlor


R.T.: 3.788 min
Delta R.T.: 0.000 min
Response: 183885482
Conc: 50.00 ng/ml

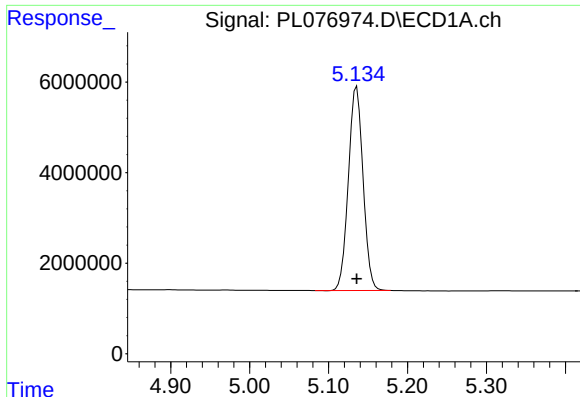

#5 Aldrin


R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 58302997
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

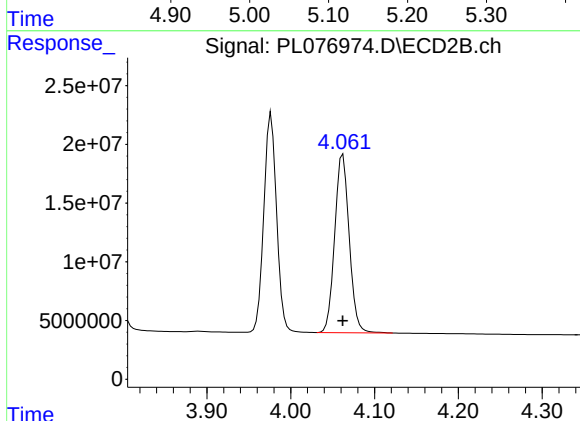


#5 Aldrin

R.T.: 4.062 min
Delta R.T.: 0.000 min
Response: 182608852
Conc: 50.00 ng/ml

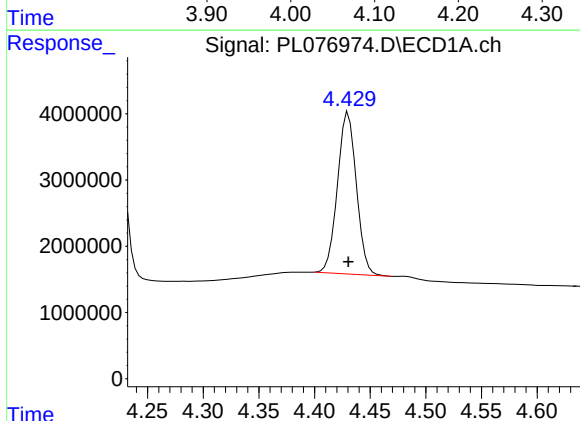


#6 beta-BHC

R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 28863408
Conc: 50.00 ng/ml

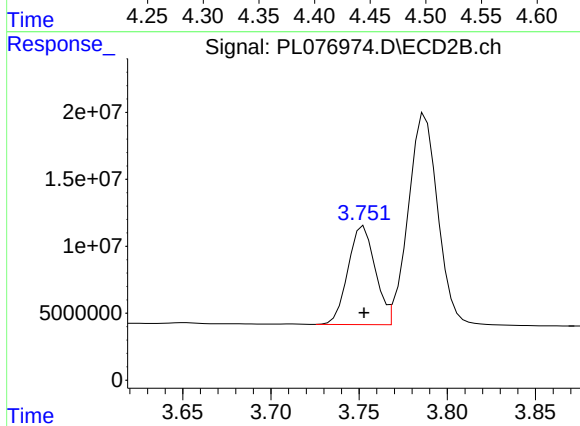

#6 beta-BHC


R.T.: 3.753 min
Delta R.T.: 0.000 min
Response: 78835480
Conc: 50.00 ng/ml

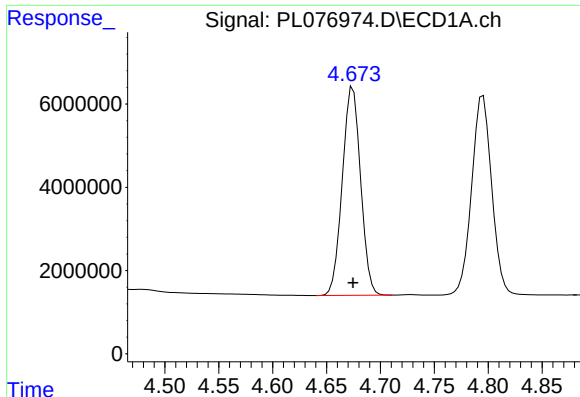

#7 delta-BHC


R.T.: 4.674 min
Delta R.T.: 0.000 min
Response: 59275760
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

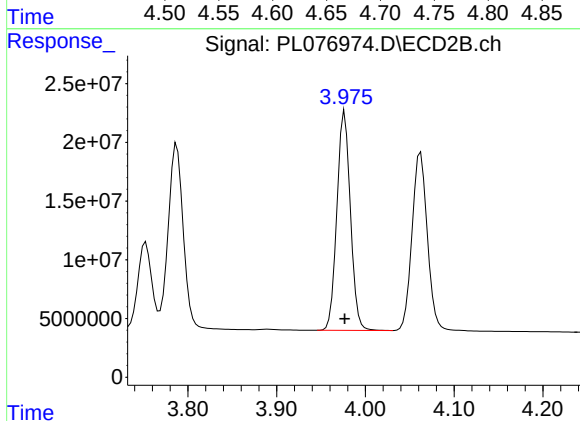


#7 delta-BHC

R.T.: 3.977 min
Delta R.T.: 0.000 min
Response: 197841142
Conc: 50.00 ng/ml

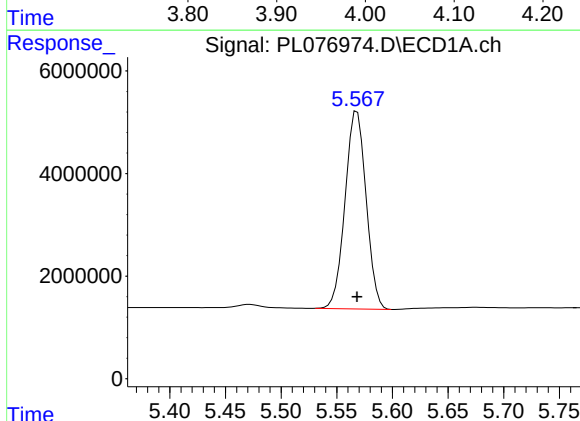


#8 Heptachlor epoxide

R.T.: 5.568 min
Delta R.T.: 0.000 min
Response: 50782879
Conc: 50.00 ng/ml

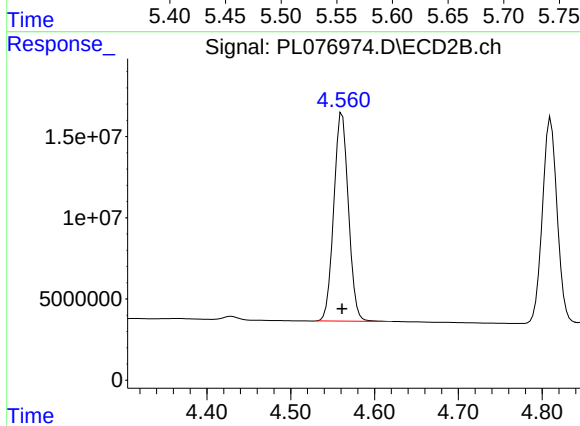

#8 Heptachlor epoxide


R.T.: 4.561 min
Delta R.T.: 0.000 min
Response: 155338515
Conc: 50.00 ng/ml

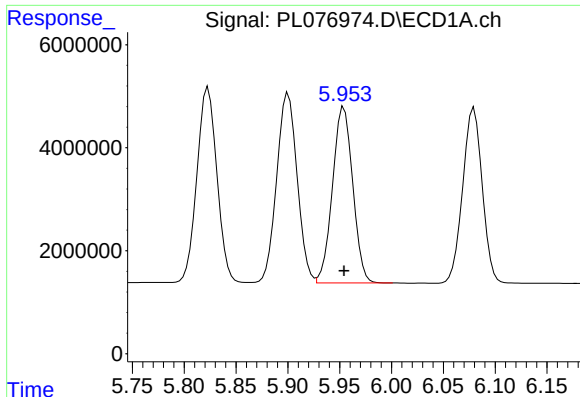

#9 Endosulfan I


R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 46492607
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

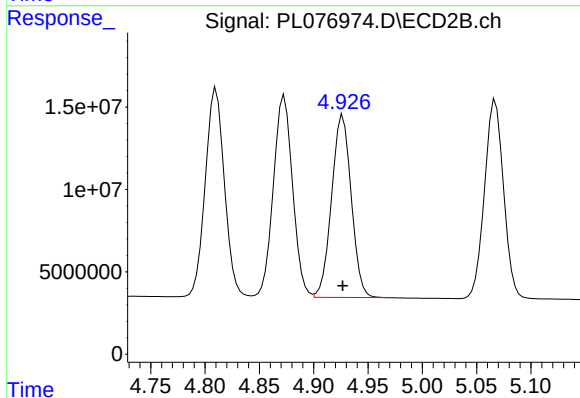


#9 Endosulfan I

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 139230280
Conc: 50.00 ng/ml

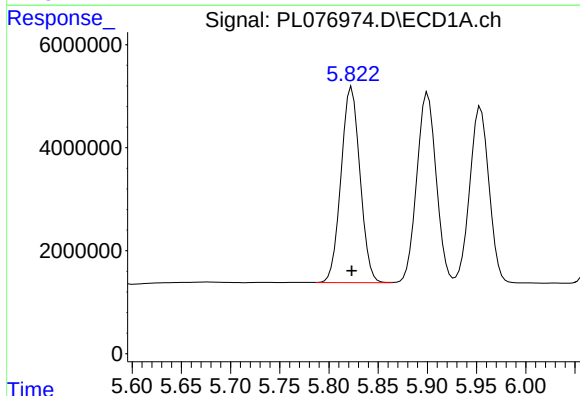


#10 gamma-Chlordane

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 50931698
Conc: 50.00 ng/ml

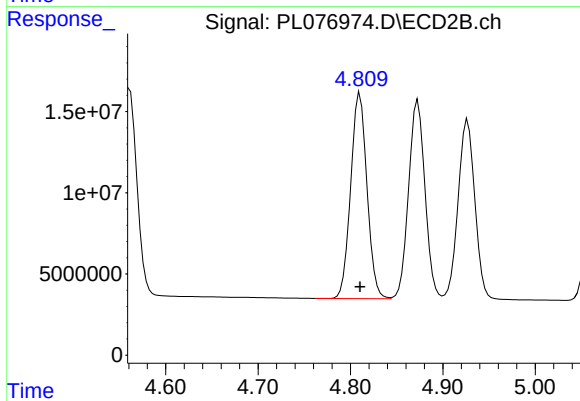

#10 gamma-Chlordane


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 155308265
Conc: 50.00 ng/ml

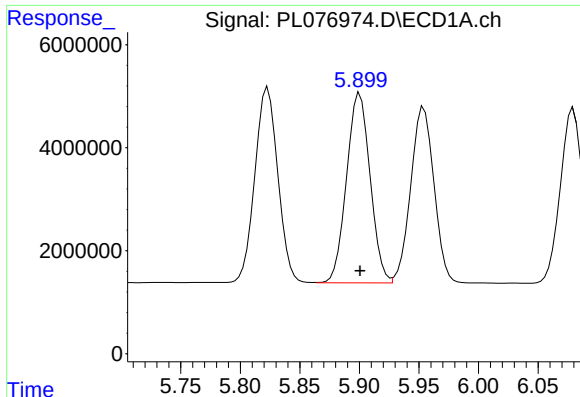

#11 alpha-Chlordane


R.T.: 5.900 min
Delta R.T.: 0.000 min
Response: 50679184
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

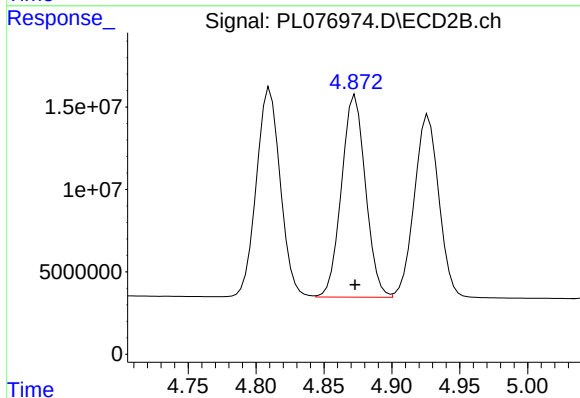


#11 alpha-Chlordane

R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 151176694
Conc: 50.00 ng/ml

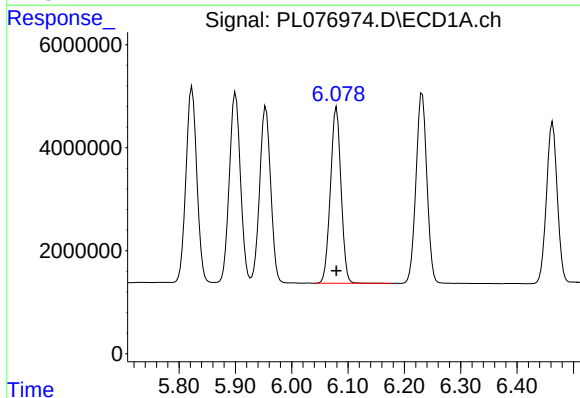


#12 4,4'-DDE

R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 44822329
Conc: 50.00 ng/ml

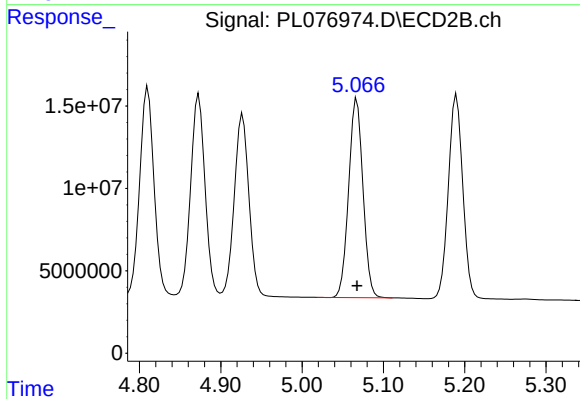

#12 4,4'-DDE


R.T.: 5.067 min
Delta R.T.: 0.000 min
Response: 147244440
Conc: 50.00 ng/ml

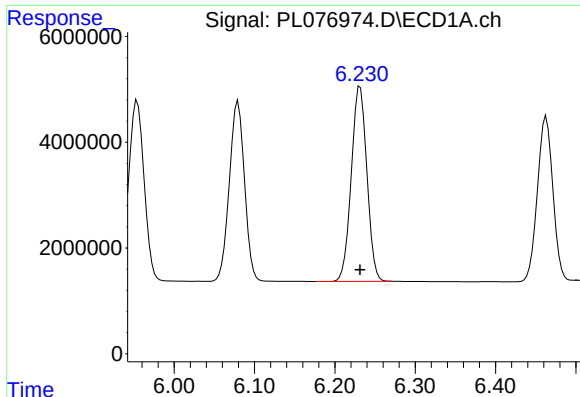

#13 Dieldrin


R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 49701189
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

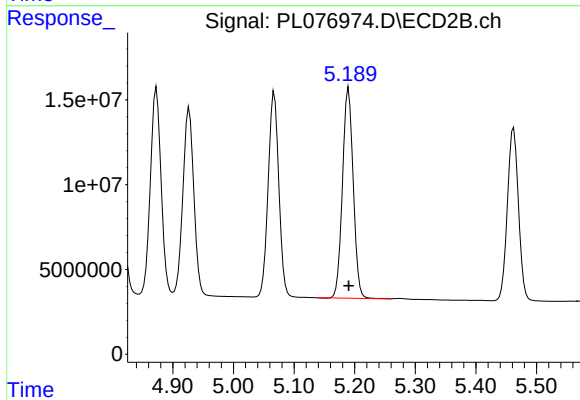


#13 Dieldrin

R.T.: 5.190 min
Delta R.T.: 0.000 min
Response: 152681662
Conc: 50.00 ng/ml

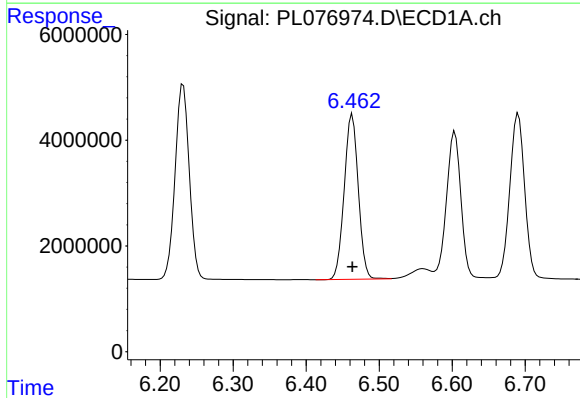


#14 Endrin

R.T.: 6.463 min
Delta R.T.: 0.000 min
Response: 41852829
Conc: 50.00 ng/ml

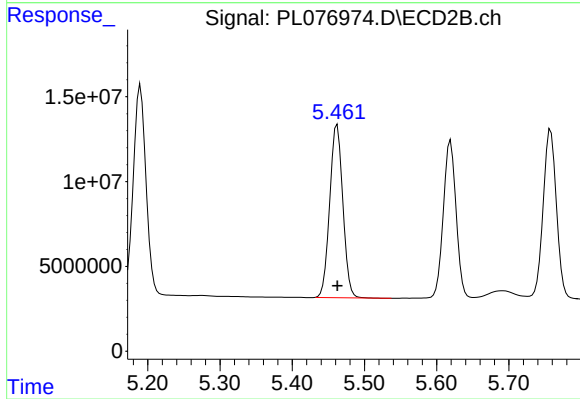

#14 Endrin


R.T.: 5.462 min
Delta R.T.: 0.000 min
Response: 129115139
Conc: 50.00 ng/ml

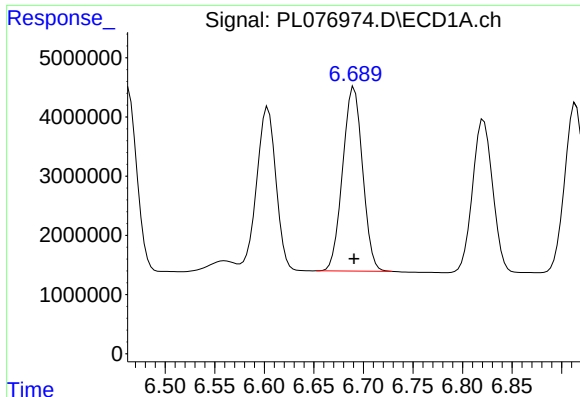

#15 Endosulfan II


R.T.: 6.691 min
Delta R.T.: 0.000 min
Response: 43523117
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

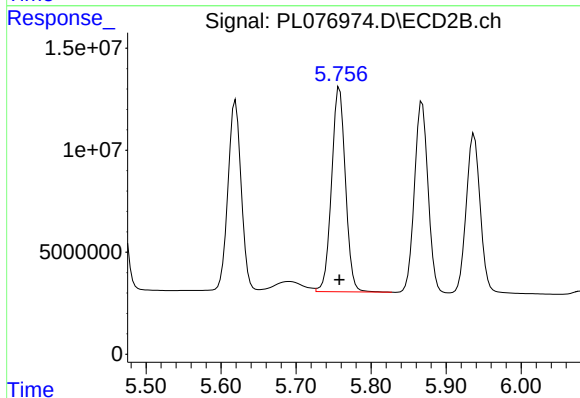


#15 Endosulfan II

R.T.: 5.758 min
Delta R.T.: 0.000 min
Response: 128684860
Conc: 50.00 ng/ml

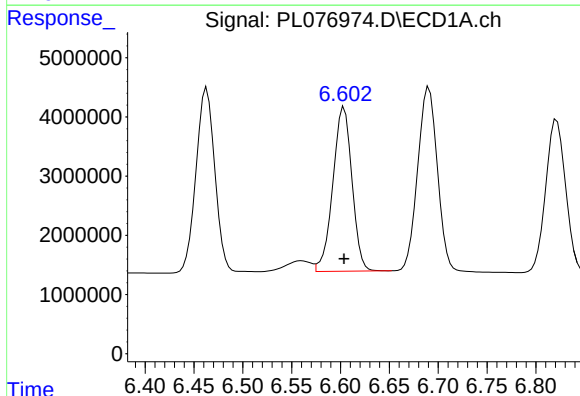


#16 4,4'-DDD

R.T.: 6.604 min
Delta R.T.: 0.000 min
Response: 37871228
Conc: 50.00 ng/ml

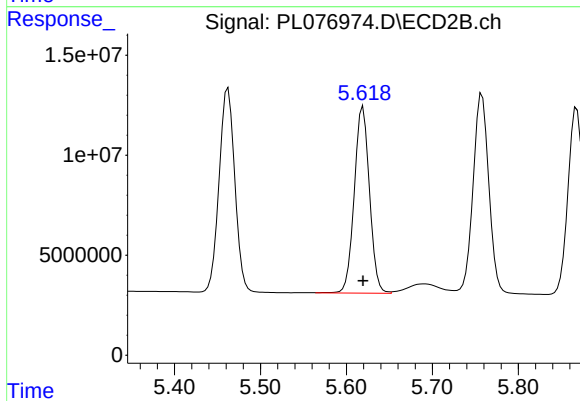

#16 4,4'-DDD


R.T.: 5.619 min
Delta R.T.: 0.000 min
Response: 114918308
Conc: 50.00 ng/ml

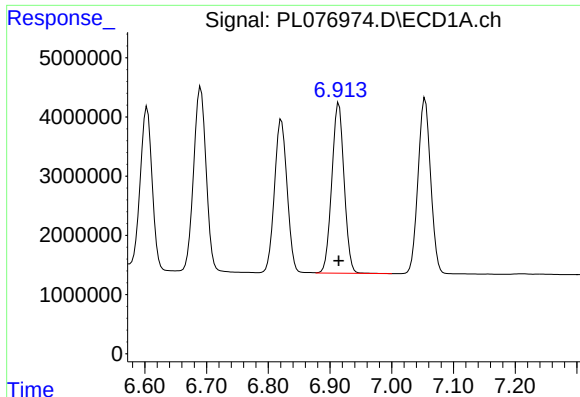

#17 4,4'-DDT


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 39794789
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

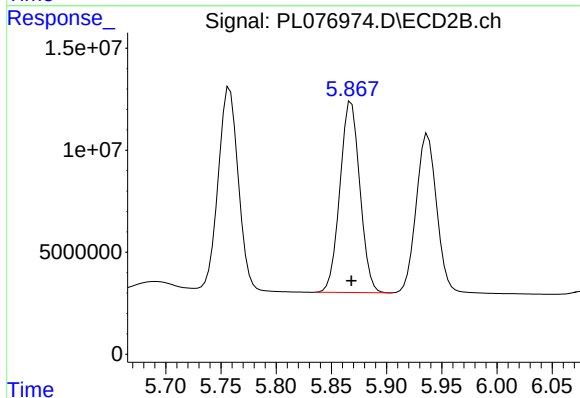


#17 4,4'-DDT

R.T.: 5.868 min
Delta R.T.: 0.000 min
Response: 117683823
Conc: 50.00 ng/ml

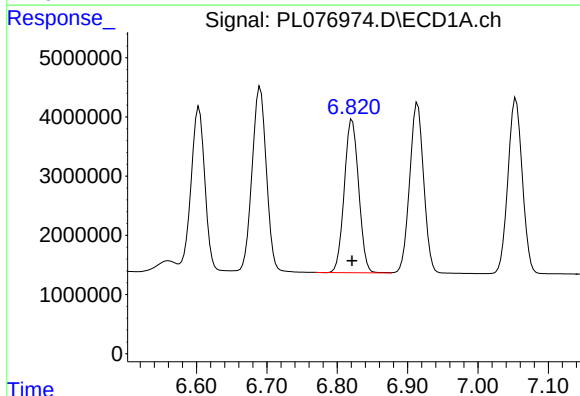


#18 Endrin aldehyde

R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 36797292
Conc: 50.00 ng/ml

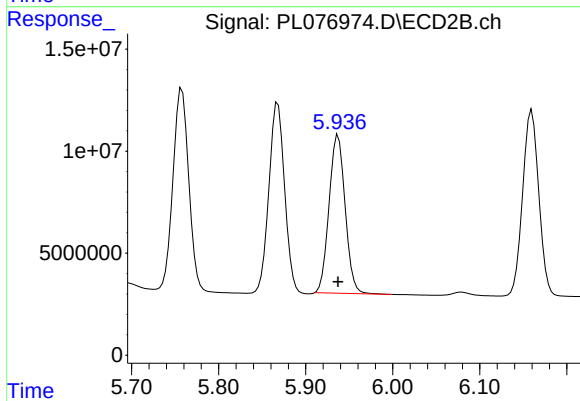

#18 Endrin aldehyde


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 99437005
Conc: 50.00 ng/ml

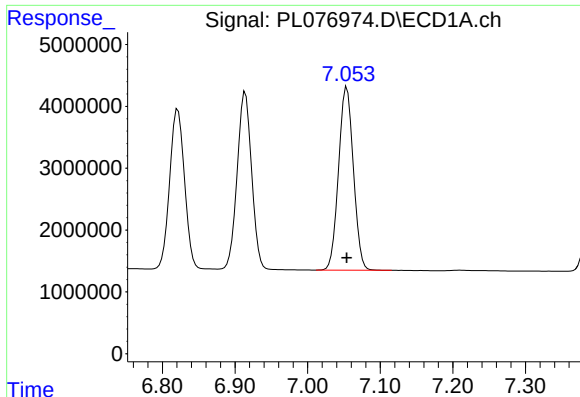

#19 Endosulfan Sulfate


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 42007966
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

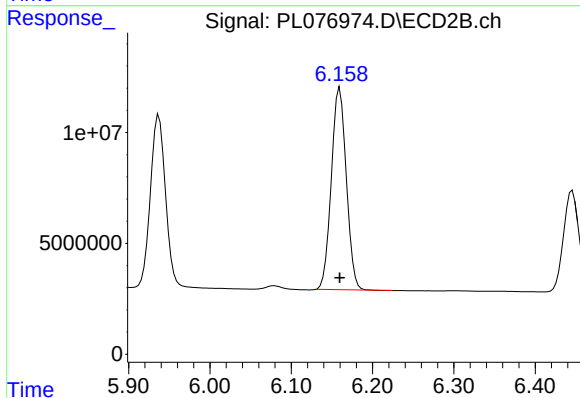


#19 Endosulfan Sulfate

R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 116857079
Conc: 50.00 ng/ml

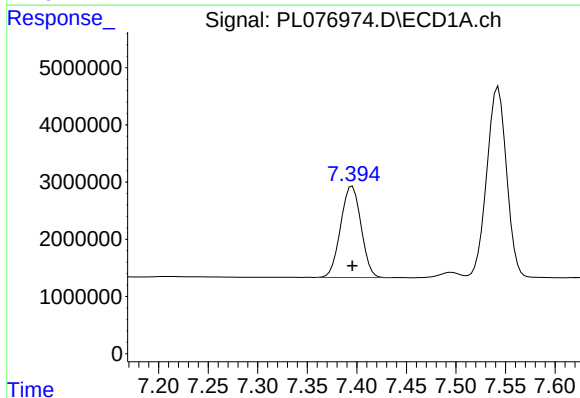


#20 Methoxychlor

R.T.: 7.395 min
Delta R.T.: 0.000 min
Response: 22914413
Conc: 50.00 ng/ml

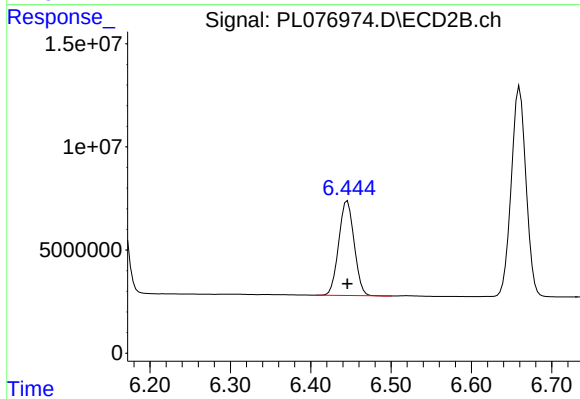

#20 Methoxychlor


R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 61239254
Conc: 50.00 ng/ml

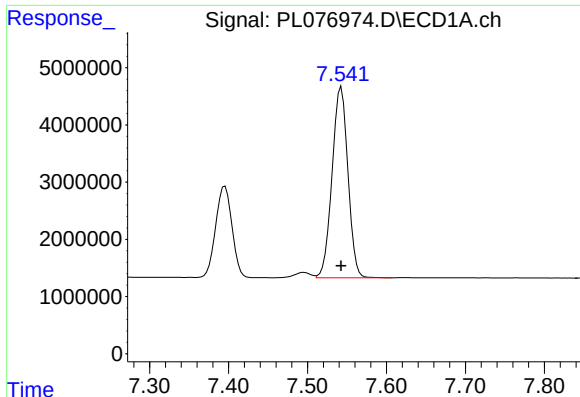

#21 Endrin ketone


R.T.: 7.543 min
Delta R.T.: 0.000 min
Response: 46481501
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

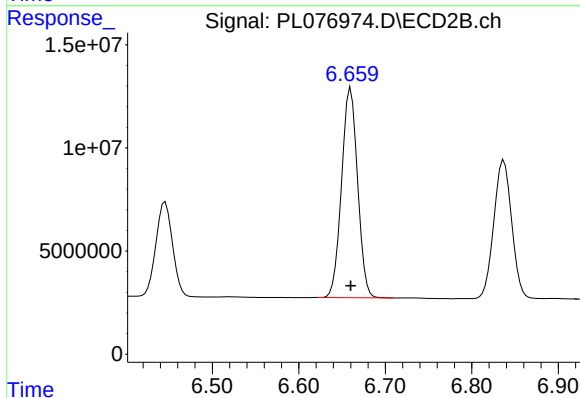


#21 Endrin ketone

R.T.: 6.660 min
Delta R.T.: 0.000 min
Response: 130058756
Conc: 50.00 ng/ml

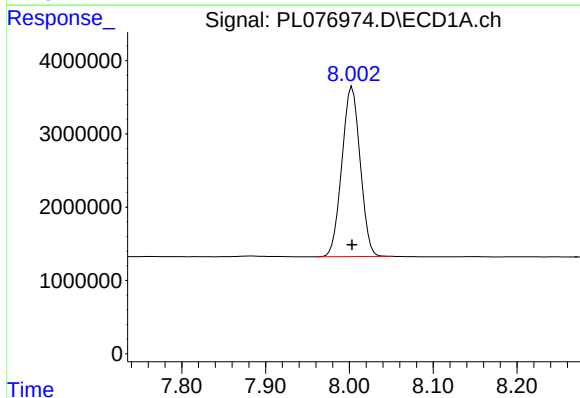


#22 Mirex

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 35219687
Conc: 50.00 ng/ml

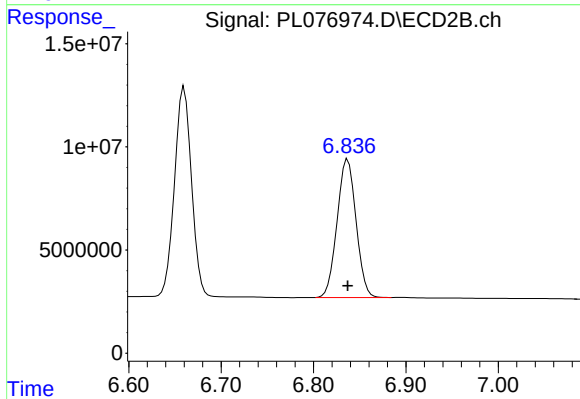

#22 Mirex


R.T.: 6.837 min
Delta R.T.: 0.000 min
Response: 95707135
Conc: 50.00 ng/ml

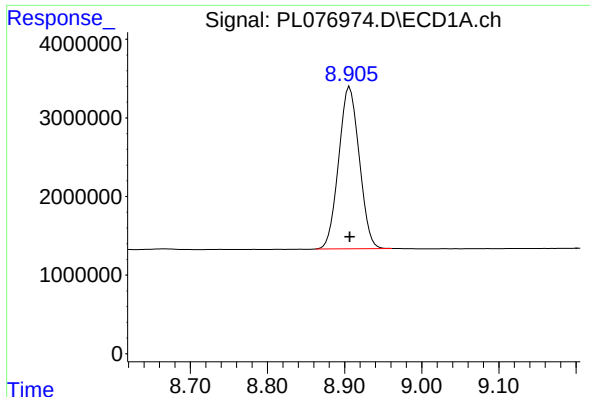

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 38138703
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC050

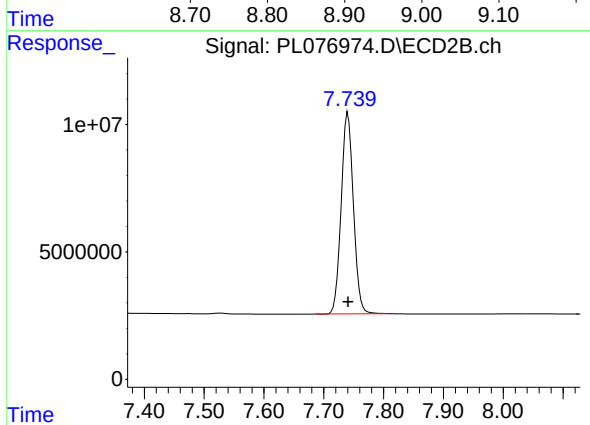

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 112626749
Conc: 50.00 ng/ml