

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 19:12
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:08:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 07:07:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	105.1E6	355.8E6	96.454	94.492
28)	SA Decachlor...	8.907	7.741	75527429	234.3E6	93.660	92.978
Target Compounds							
23)	Chlordane-1	4.579	3.616	37349741	95365978	966.302	956.677
24)	Chlordane-2	5.113	4.187	37914901	106.9E6	927.355	931.158
25)	Chlordane-3	5.824	4.811	148.0E6	315.0E6	1000.689	974.786
26)	Chlordane-4	5.902	4.873	177.5E6	325.8E6	989.759	972.213
27)	Chlordane-5	6.760	5.537	30461253	84485860	960.059	933.424



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 19:12
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:08:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 07:07:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

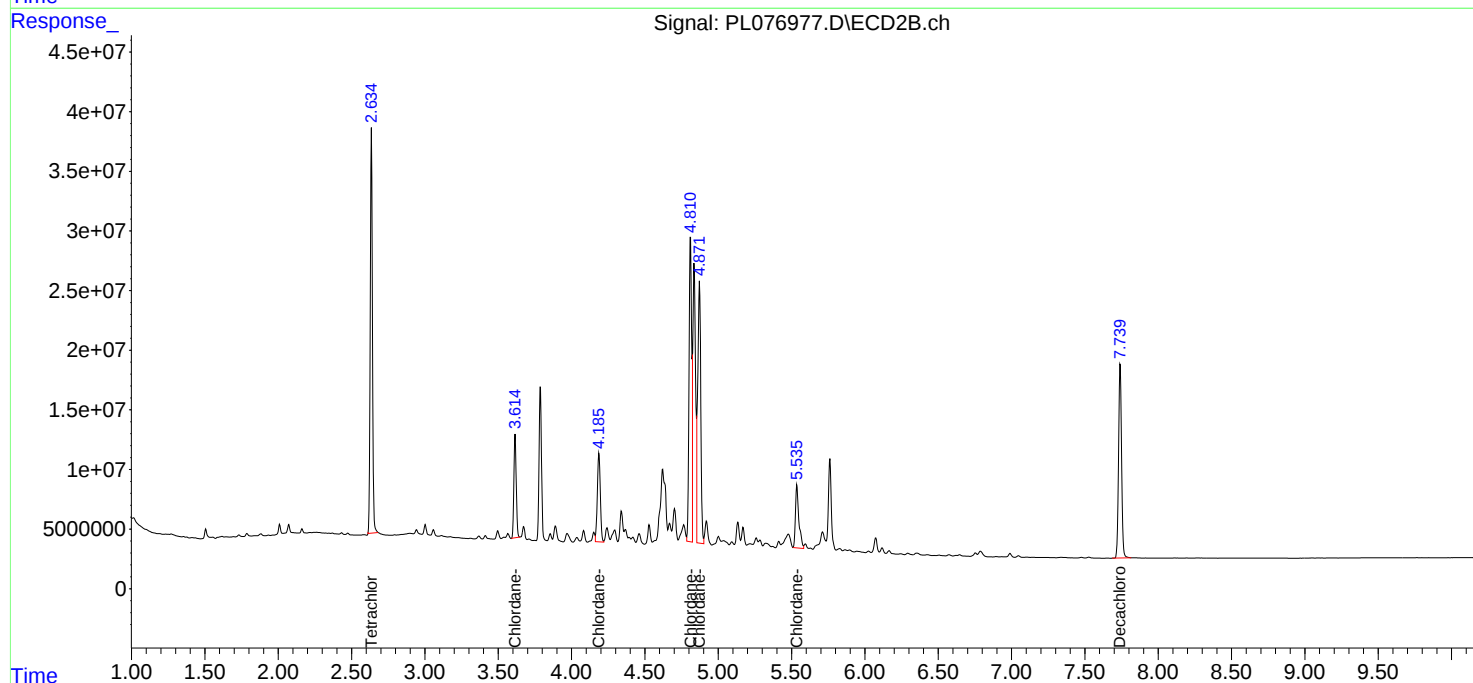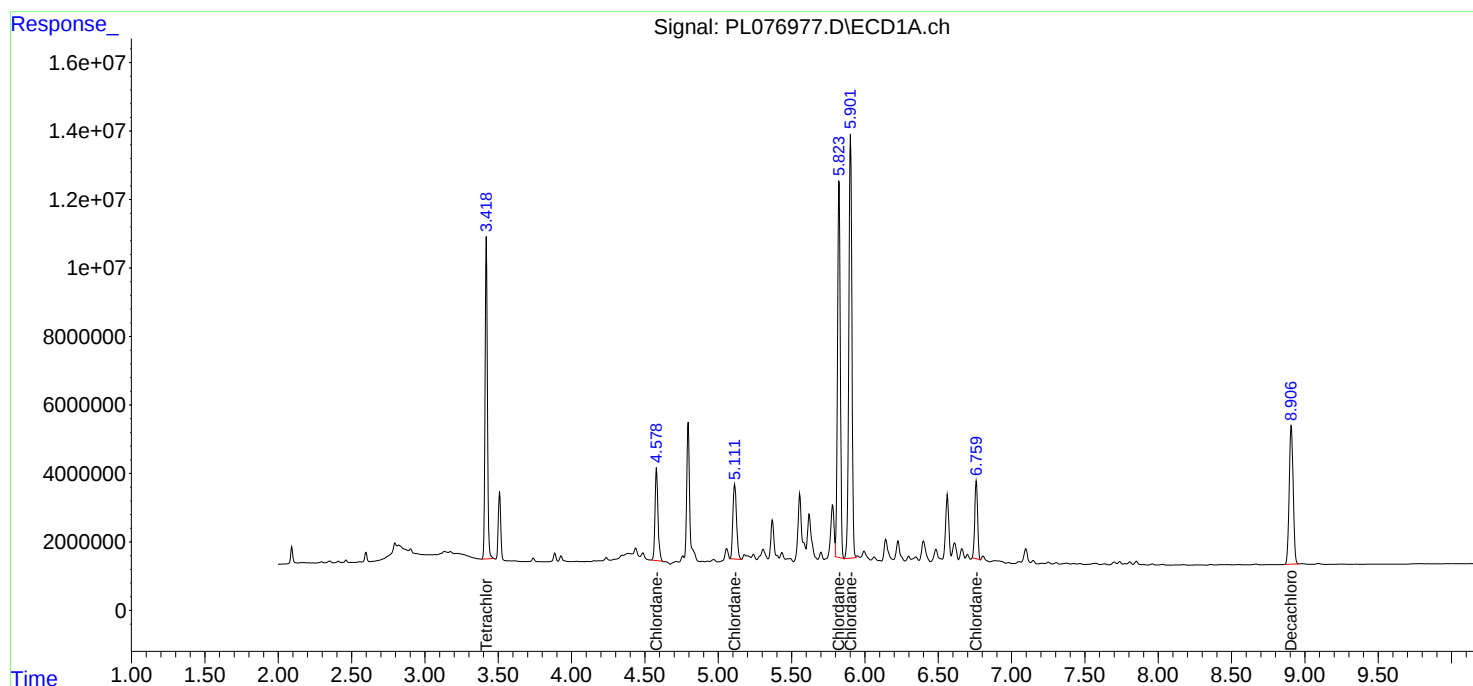


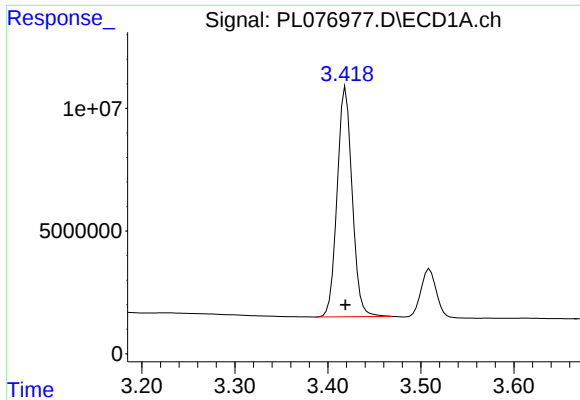

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 105071181
Conc: 96.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

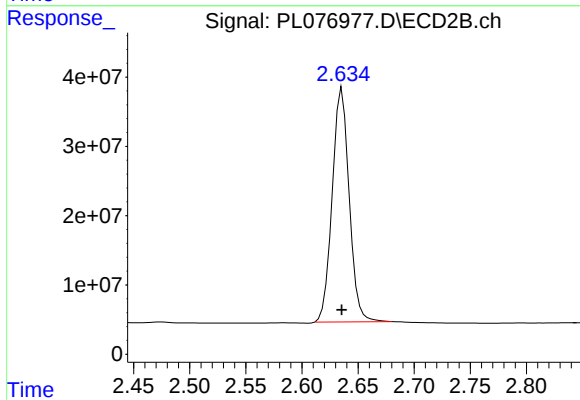


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 355811066
Conc: 94.49 ng/ml

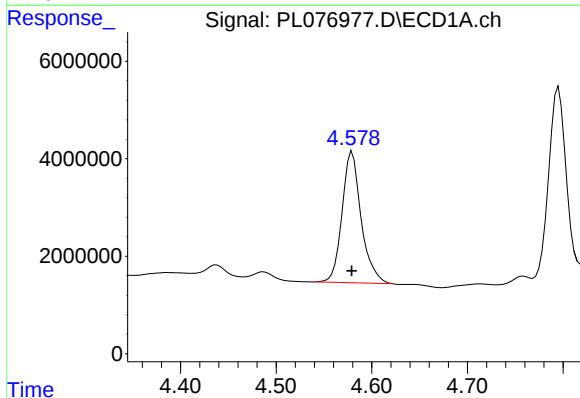


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 37349741
Conc: 966.30 ng/ml

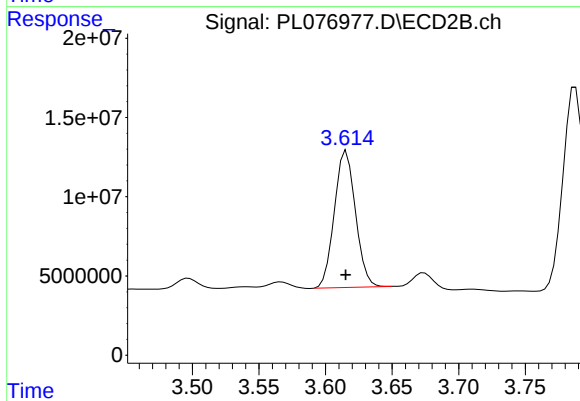

#23 Chlordane-1


R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 95365978
Conc: 956.68 ng/ml

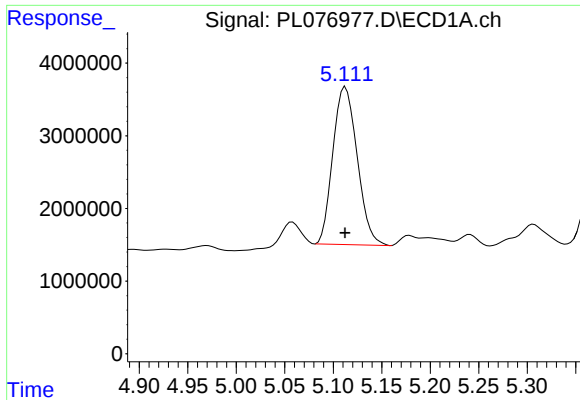

#24 Chlordane-2


R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 37914901
Conc: 927.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

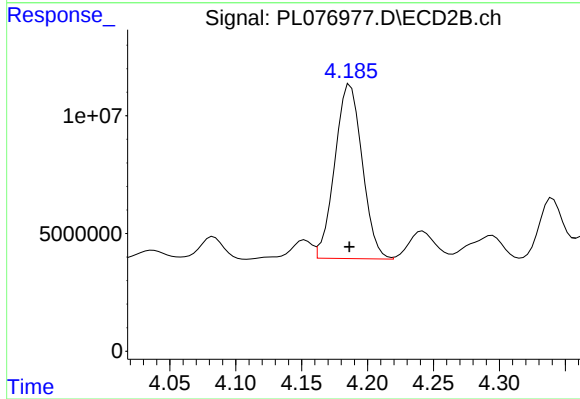


#24 Chlordane-2

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 106923021
Conc: 931.16 ng/ml

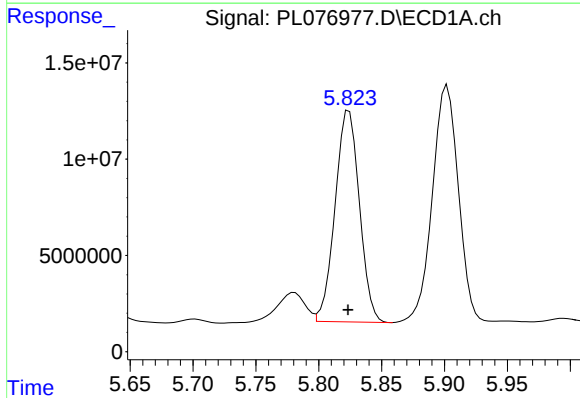


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 147977377
Conc: 1000.69 ng/ml

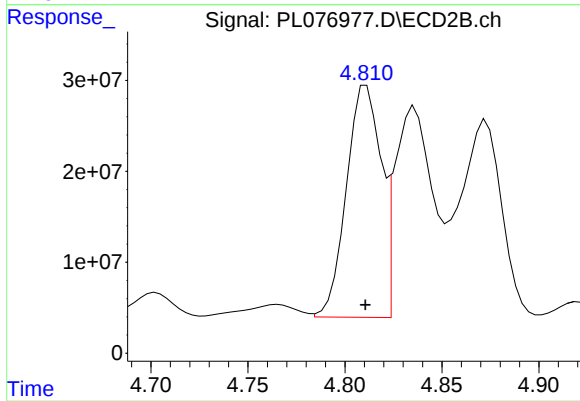

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 314958775
Conc: 974.79 ng/ml

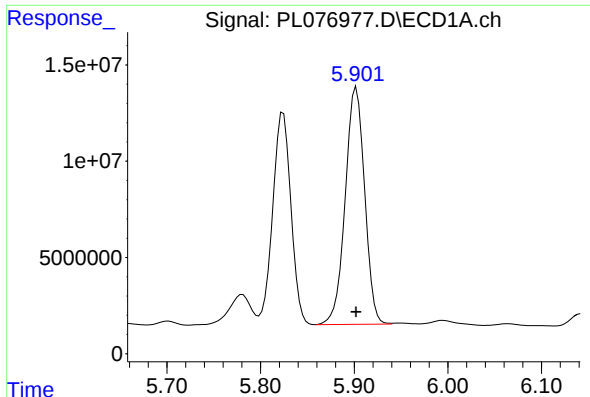

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 177475862
Conc: 989.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

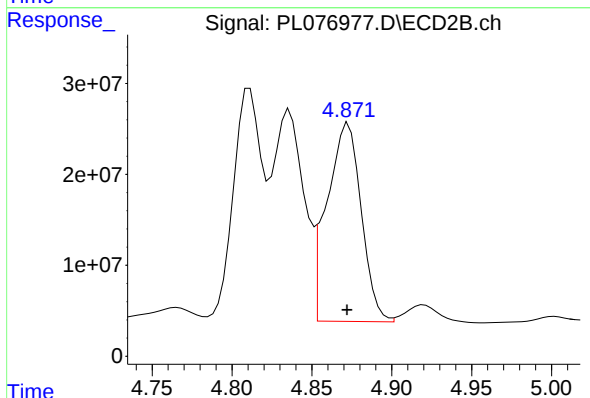


#26 Chlordane-4

R.T.: 4.873 min
Delta R.T.: 0.000 min
Response: 325811895
Conc: 972.21 ng/ml

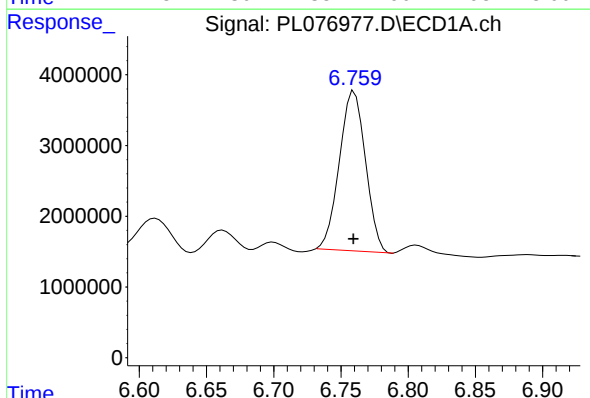


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 30461253
Conc: 960.06 ng/ml

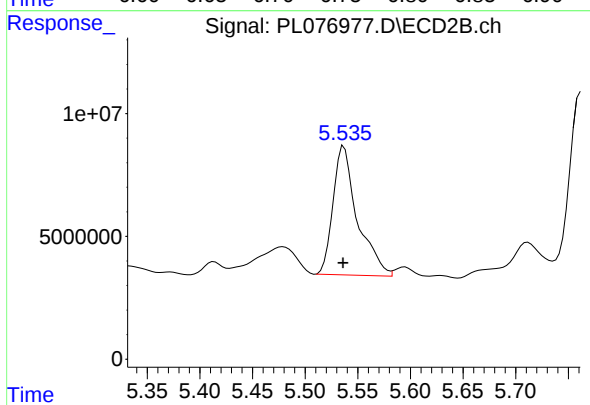

#27 Chlordane-5


R.T.: 5.537 min
Delta R.T.: 0.000 min
Response: 84485860
Conc: 933.42 ng/ml

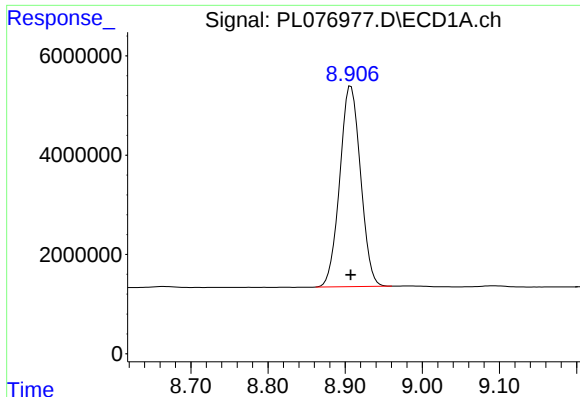

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 75527429
Conc: 93.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

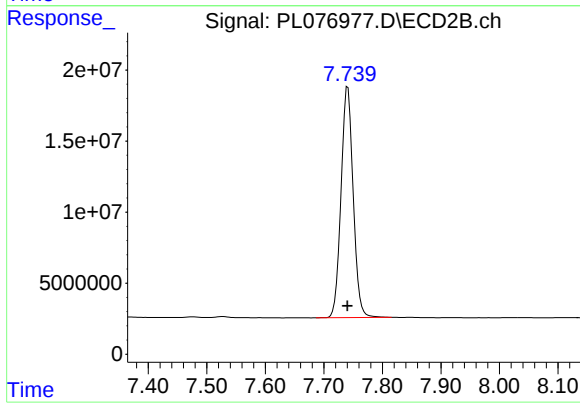

#28 Decachlorobiphenyl

R.T.: 7.741 min
Delta R.T.: 0.000 min
Response: 234253348
Conc: 92.98 ng/ml