

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 19:53
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:09:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 07:07:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.635	26351261	91855075	24.190	24.394
28)	SA Decachlor...	8.907	7.740	21446691	64471990	26.596	25.590
Target Compounds							
23)	Chlordane-1	4.579	3.616	9532479	24506499	246.622	245.840
24)	Chlordane-2	5.112	4.187	10245733	29042340	250.599	252.920
25)	Chlordane-3	5.824	4.811	35382058	78746891	239.269	243.719
26)	Chlordane-4	5.902	4.871	43333180	82411558	241.663	245.914
27)	Chlordane-5	6.760	5.536	7727345	22552835	243.546	249.170



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 19:53
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:09:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 07:07:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

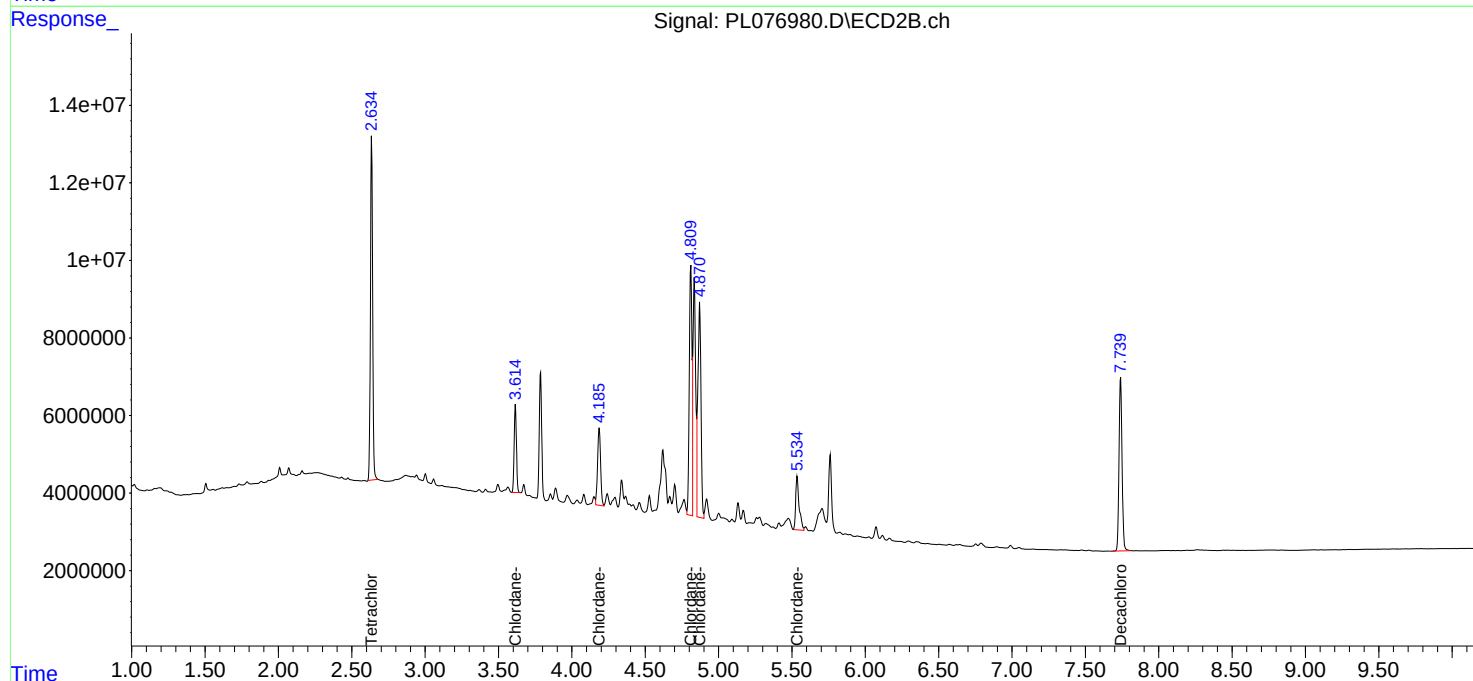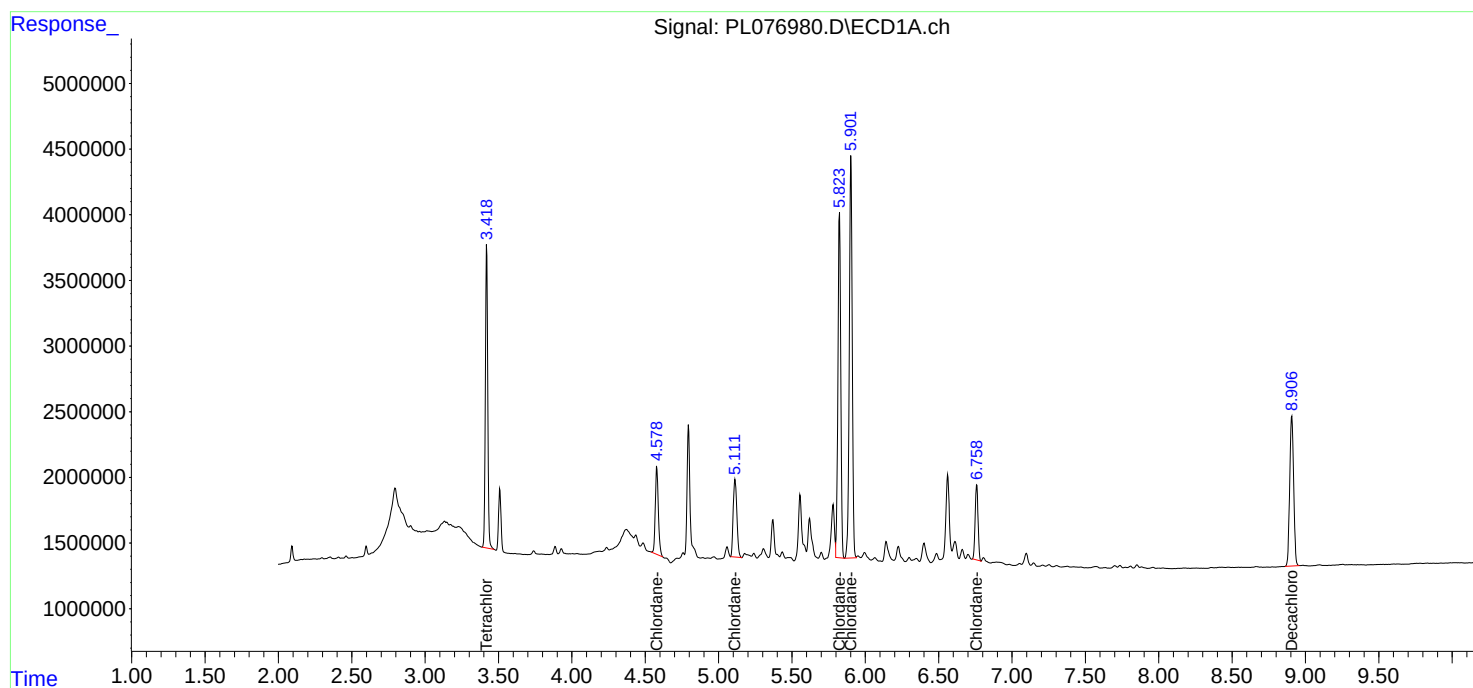


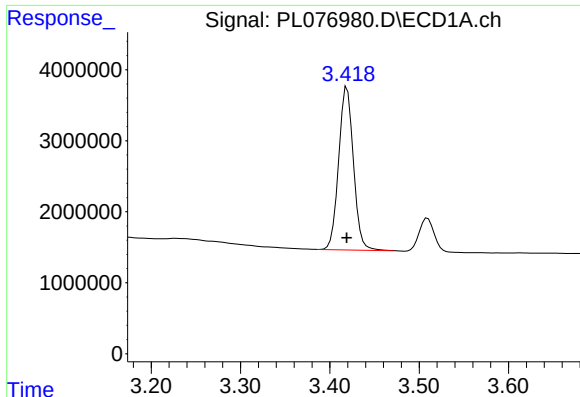

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 26351261
Conc: 24.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

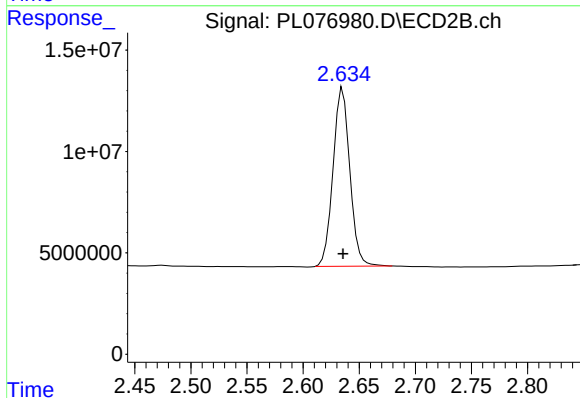


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: 0.000 min
Response: 91855075
Conc: 24.39 ng/ml

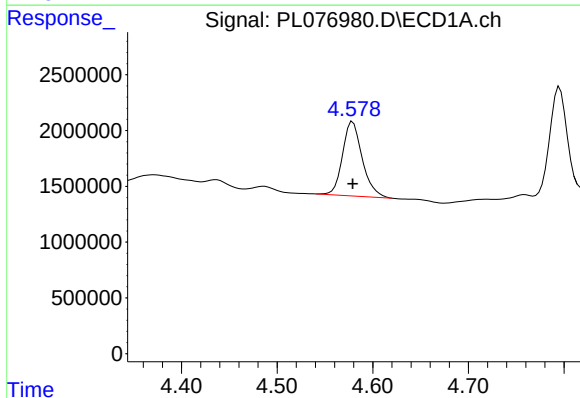


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 9532479
Conc: 246.62 ng/ml

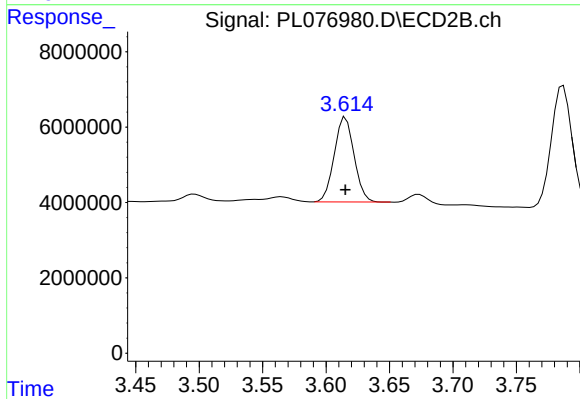

#23 Chlordane-1


R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 24506499
Conc: 245.84 ng/ml

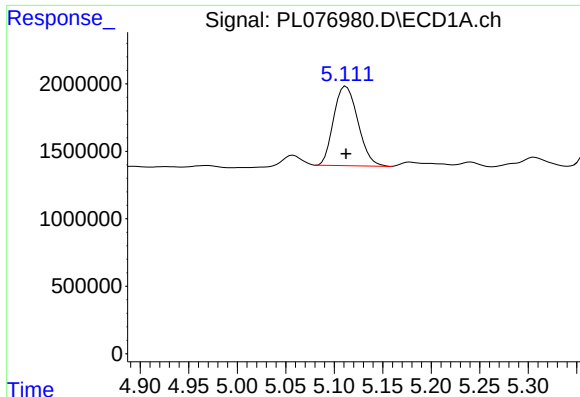

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 10245733
Conc: 250.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

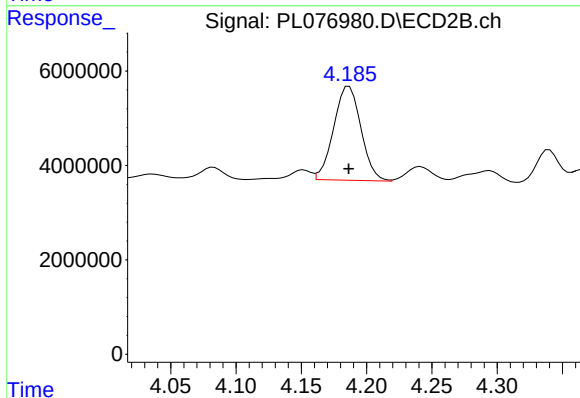


#24 Chlordane-2

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 29042340
Conc: 252.92 ng/ml

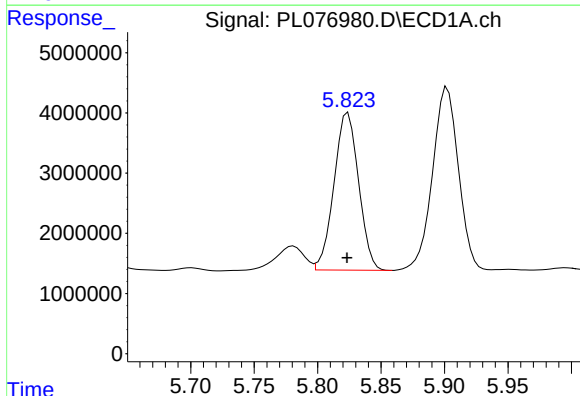


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 35382058
Conc: 239.27 ng/ml

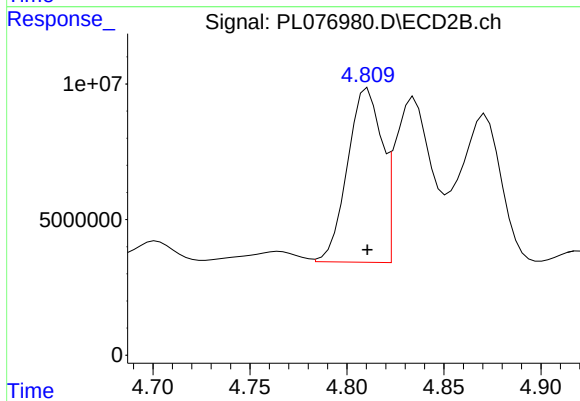

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 78746891
Conc: 243.72 ng/ml

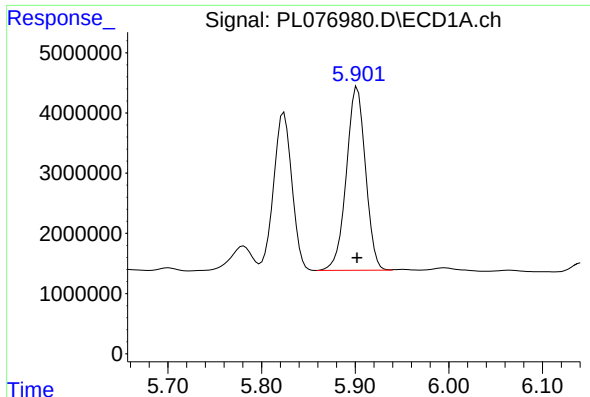

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 43333180
Conc: 241.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

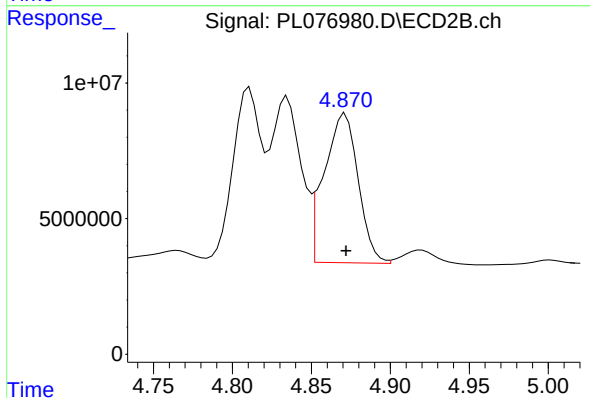


#26 Chlordane-4

R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 82411558
Conc: 245.91 ng/ml

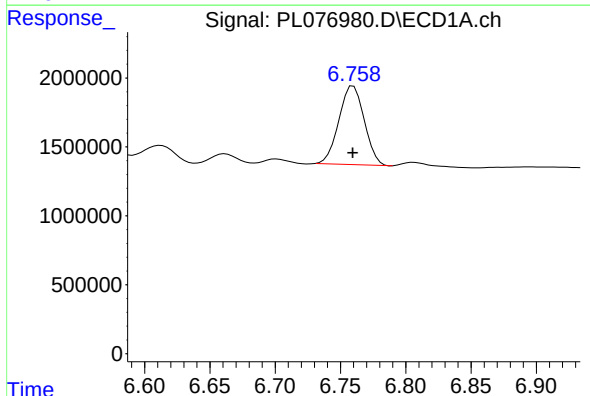


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 7727345
Conc: 243.55 ng/ml

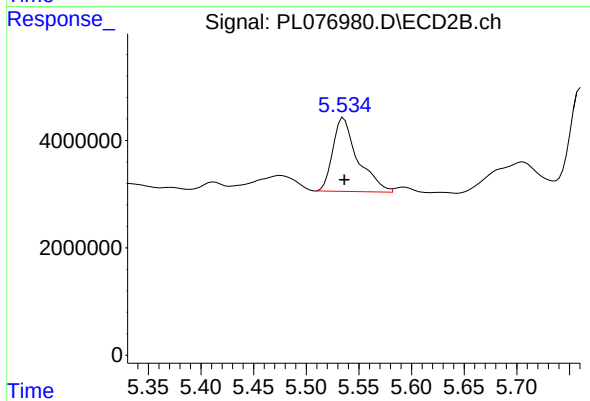

#27 Chlordane-5


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 22552835
Conc: 249.17 ng/ml

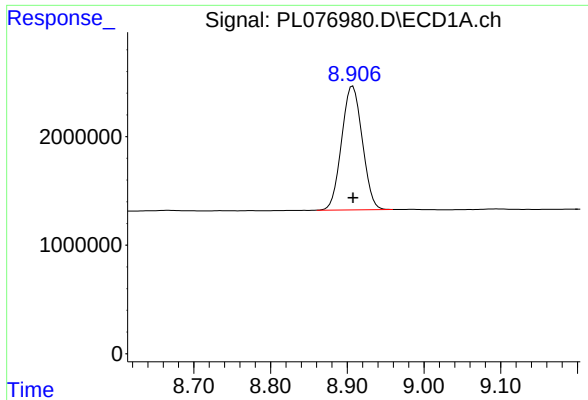

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 21446691
Conc: 26.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

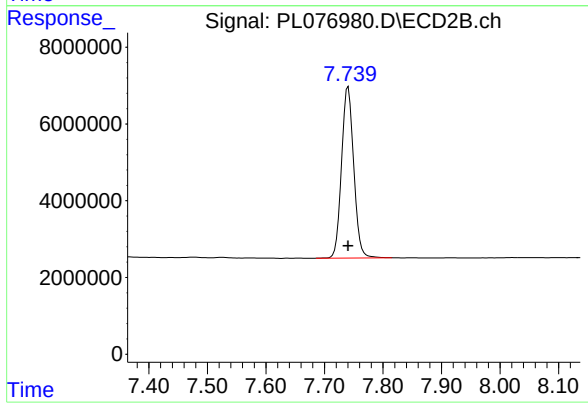

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 64471990
Conc: 25.59 ng/ml