

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 20:07
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:09:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 07:07:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	5101822	17651556	4.683	4.688
28)	SA Decachlor...	8.907	7.739	4393281	13310971	5.448	5.283
Target Compounds							
23)	Chlordane-1	4.578	3.615	1790065	4718097	46.312	47.330
24)	Chlordane-2	5.112	4.186	1971173	6275223	48.213	54.649
25)	Chlordane-3	5.824	4.810	6967954	15262187	47.120	47.236
26)	Chlordane-4	5.902	4.872	8584668	16037895	47.876	47.857
27)	Chlordane-5	6.760	5.535	1351472	5159148	42.595	57.000 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 20:07
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:09:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 07:07:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

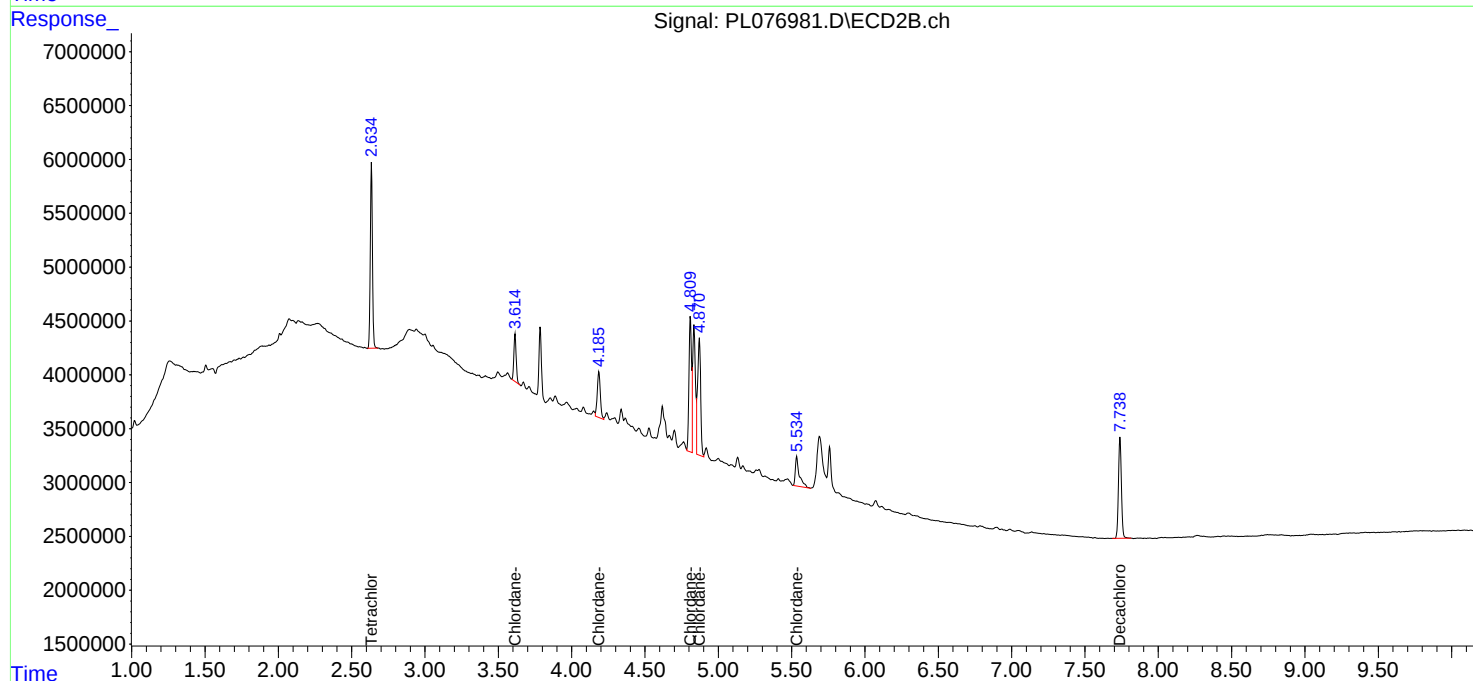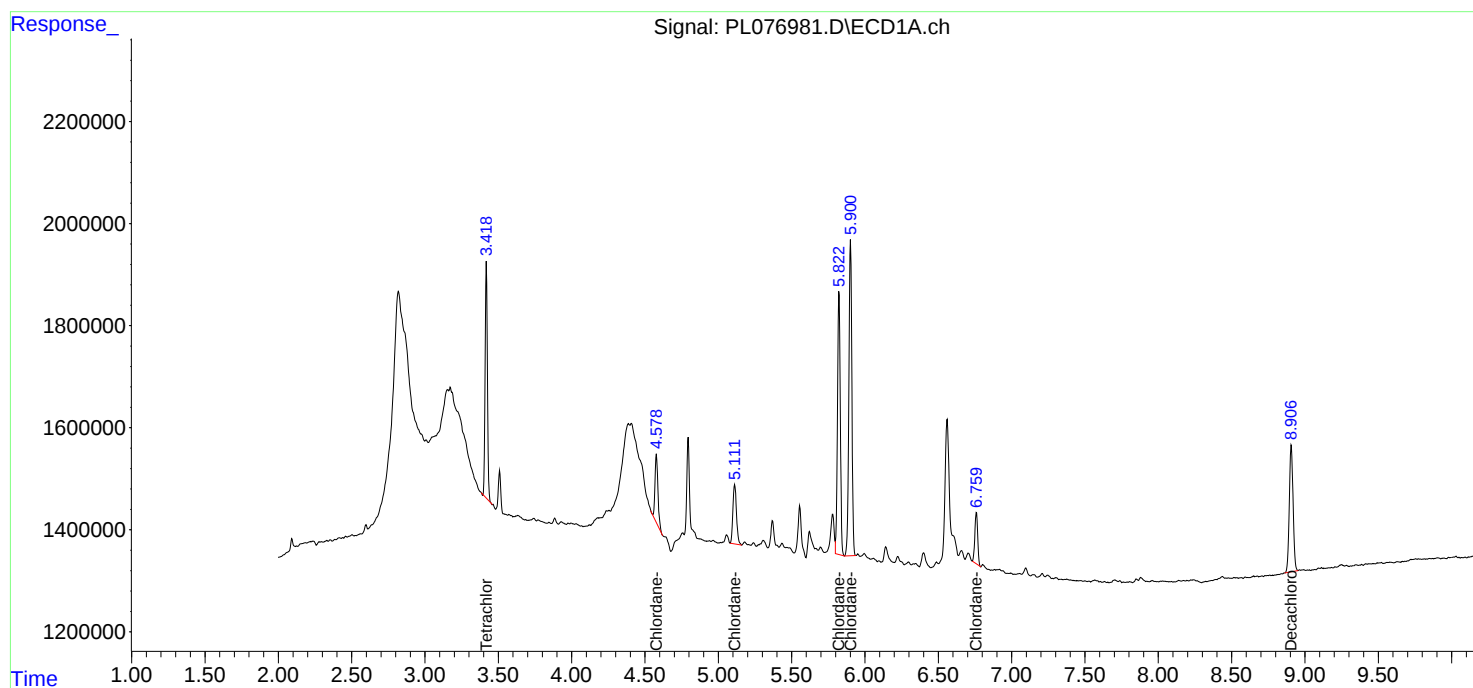


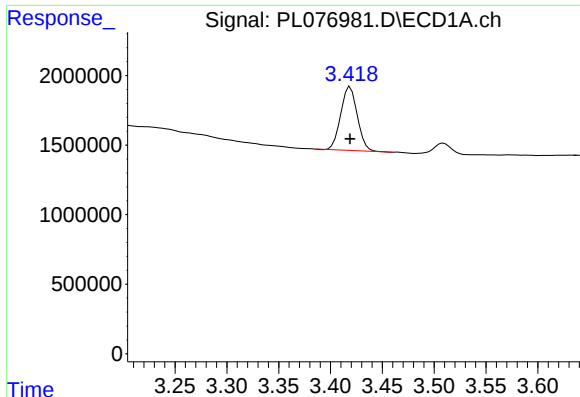

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 5101822
Conc: 4.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

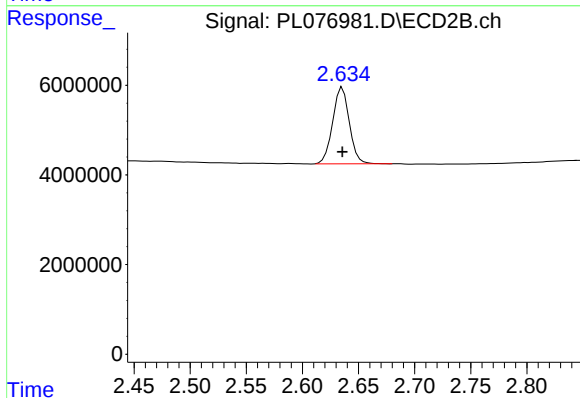


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 17651556
Conc: 4.69 ng/ml

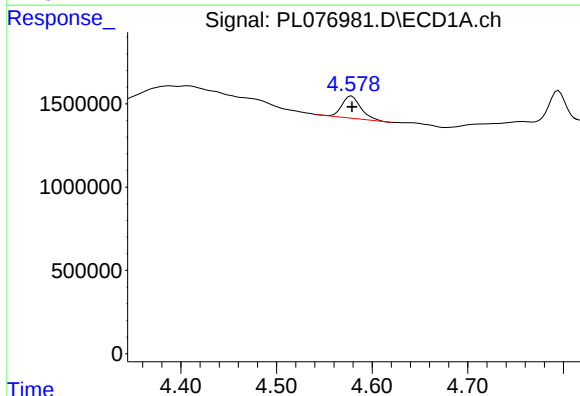


#23 Chlordane-1

R.T.: 4.578 min
Delta R.T.: 0.000 min
Response: 1790065
Conc: 46.31 ng/ml

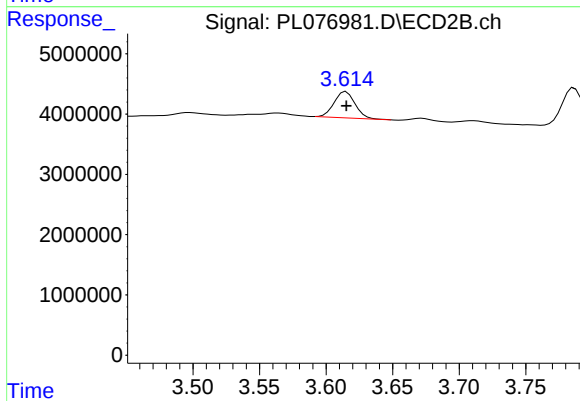

#23 Chlordane-1


R.T.: 3.615 min
Delta R.T.: 0.000 min
Response: 4718097
Conc: 47.33 ng/ml

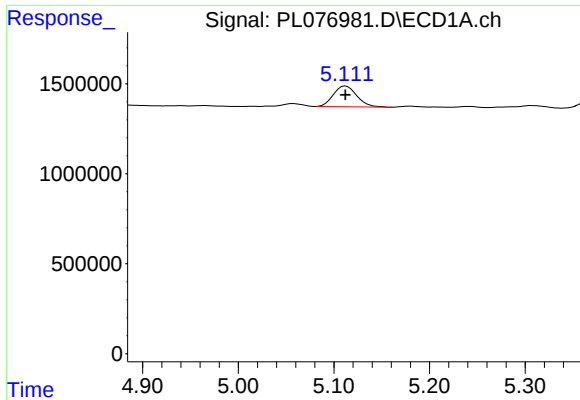

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 1971173
Conc: 48.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

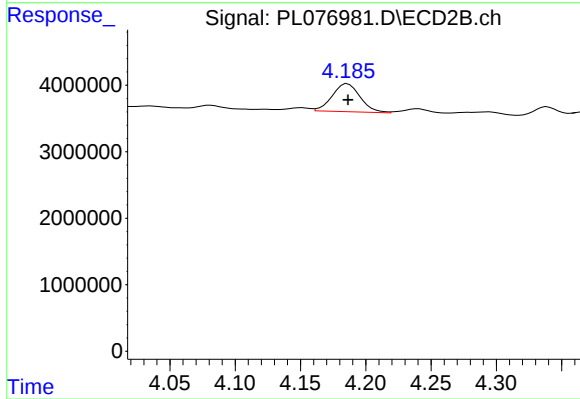


#24 Chlordane-2

R.T.: 4.186 min
Delta R.T.: 0.000 min
Response: 6275223
Conc: 54.65 ng/ml

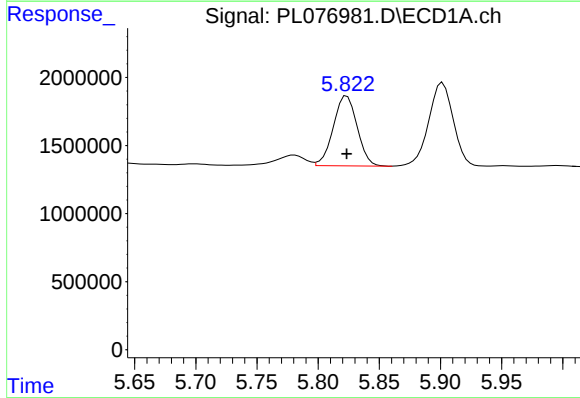


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 6967954
Conc: 47.12 ng/ml

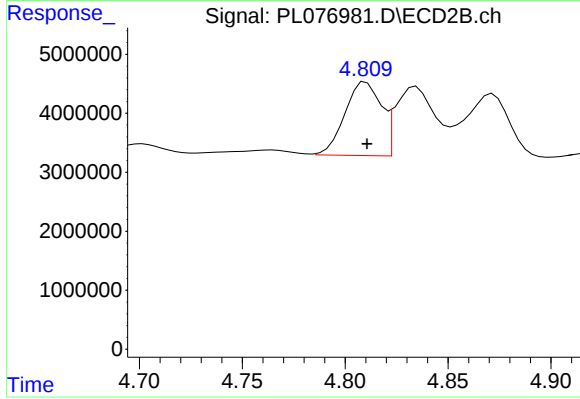

#25 Chlordane-3


R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 15262187
Conc: 47.24 ng/ml

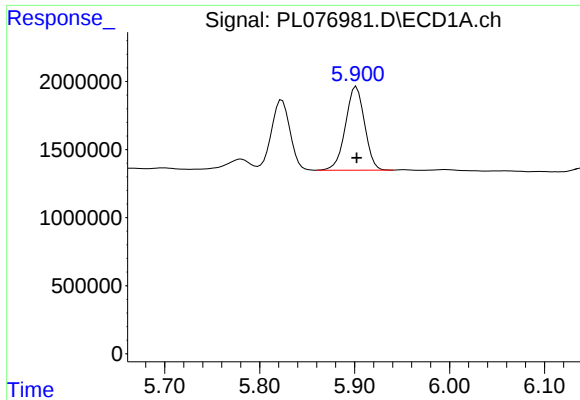

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 8584668
Conc: 47.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

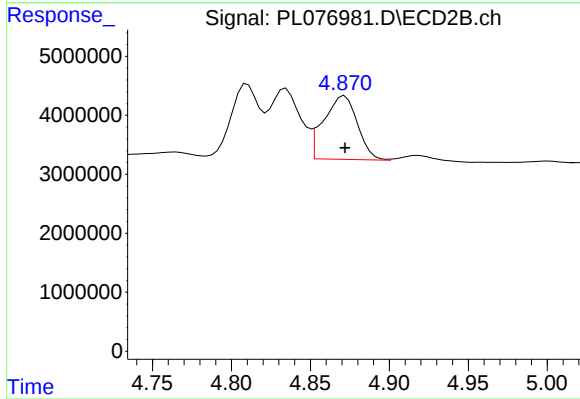


#26 Chlordane-4

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 16037895
Conc: 47.86 ng/ml

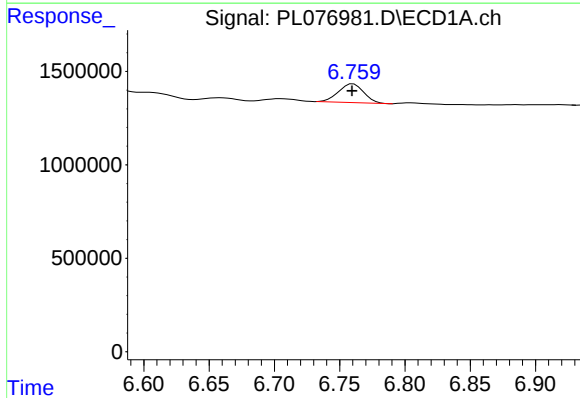


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 1351472
Conc: 42.59 ng/ml

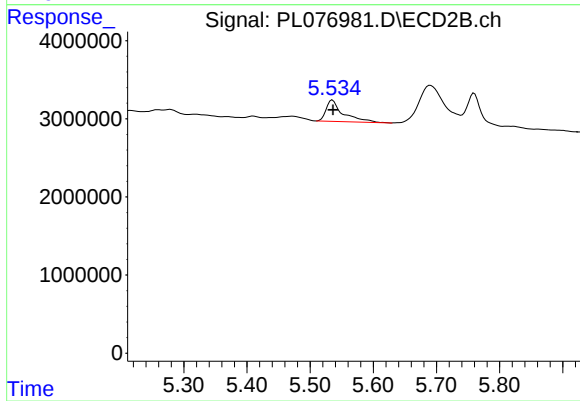

#27 Chlordane-5


R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 5159148
Conc: 57.00 ng/ml

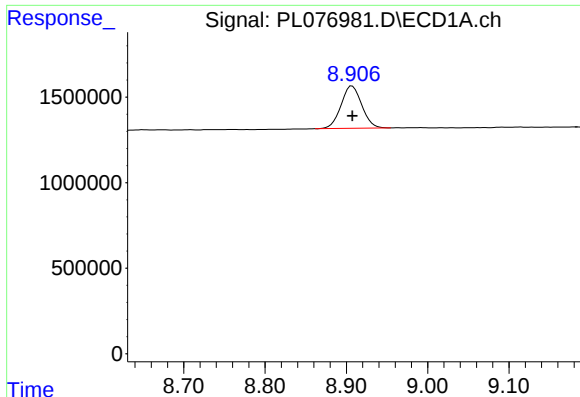

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 4393281
Conc: 5.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

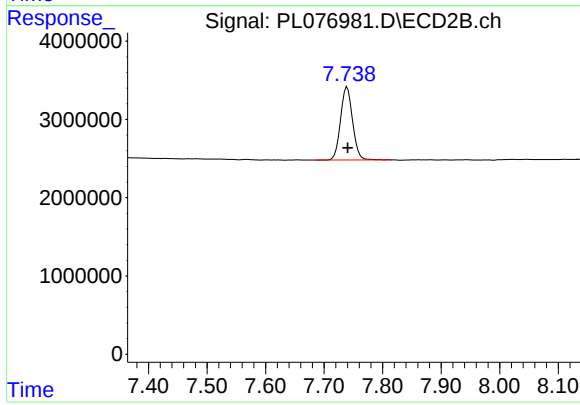

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: -0.001 min
Response: 13310971
Conc: 5.28 ng/ml