

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 21:45
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL080822CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 09:13:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:12:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	54336482	182.8E6	51.266	50.045
28)	SA Decachlor...	8.908	7.740	41133736	123.2E6	50.414	49.124
Target Compounds							
23)	Chlordane-1	4.579	3.616	19394936	48820265	514.494	501.260
24)	Chlordane-2	5.112	4.187	20595075	56072068	518.237	487.528
25)	Chlordane-3	5.824	4.811	74897840	158.7E6	515.223	501.245
26)	Chlordane-4	5.902	4.872	90989883	163.7E6	515.398	496.975
27)	Chlordane-5	6.760	5.536	15981287	43520269	527.458	477.276


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 21:45
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL080822CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 09:13:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:12:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

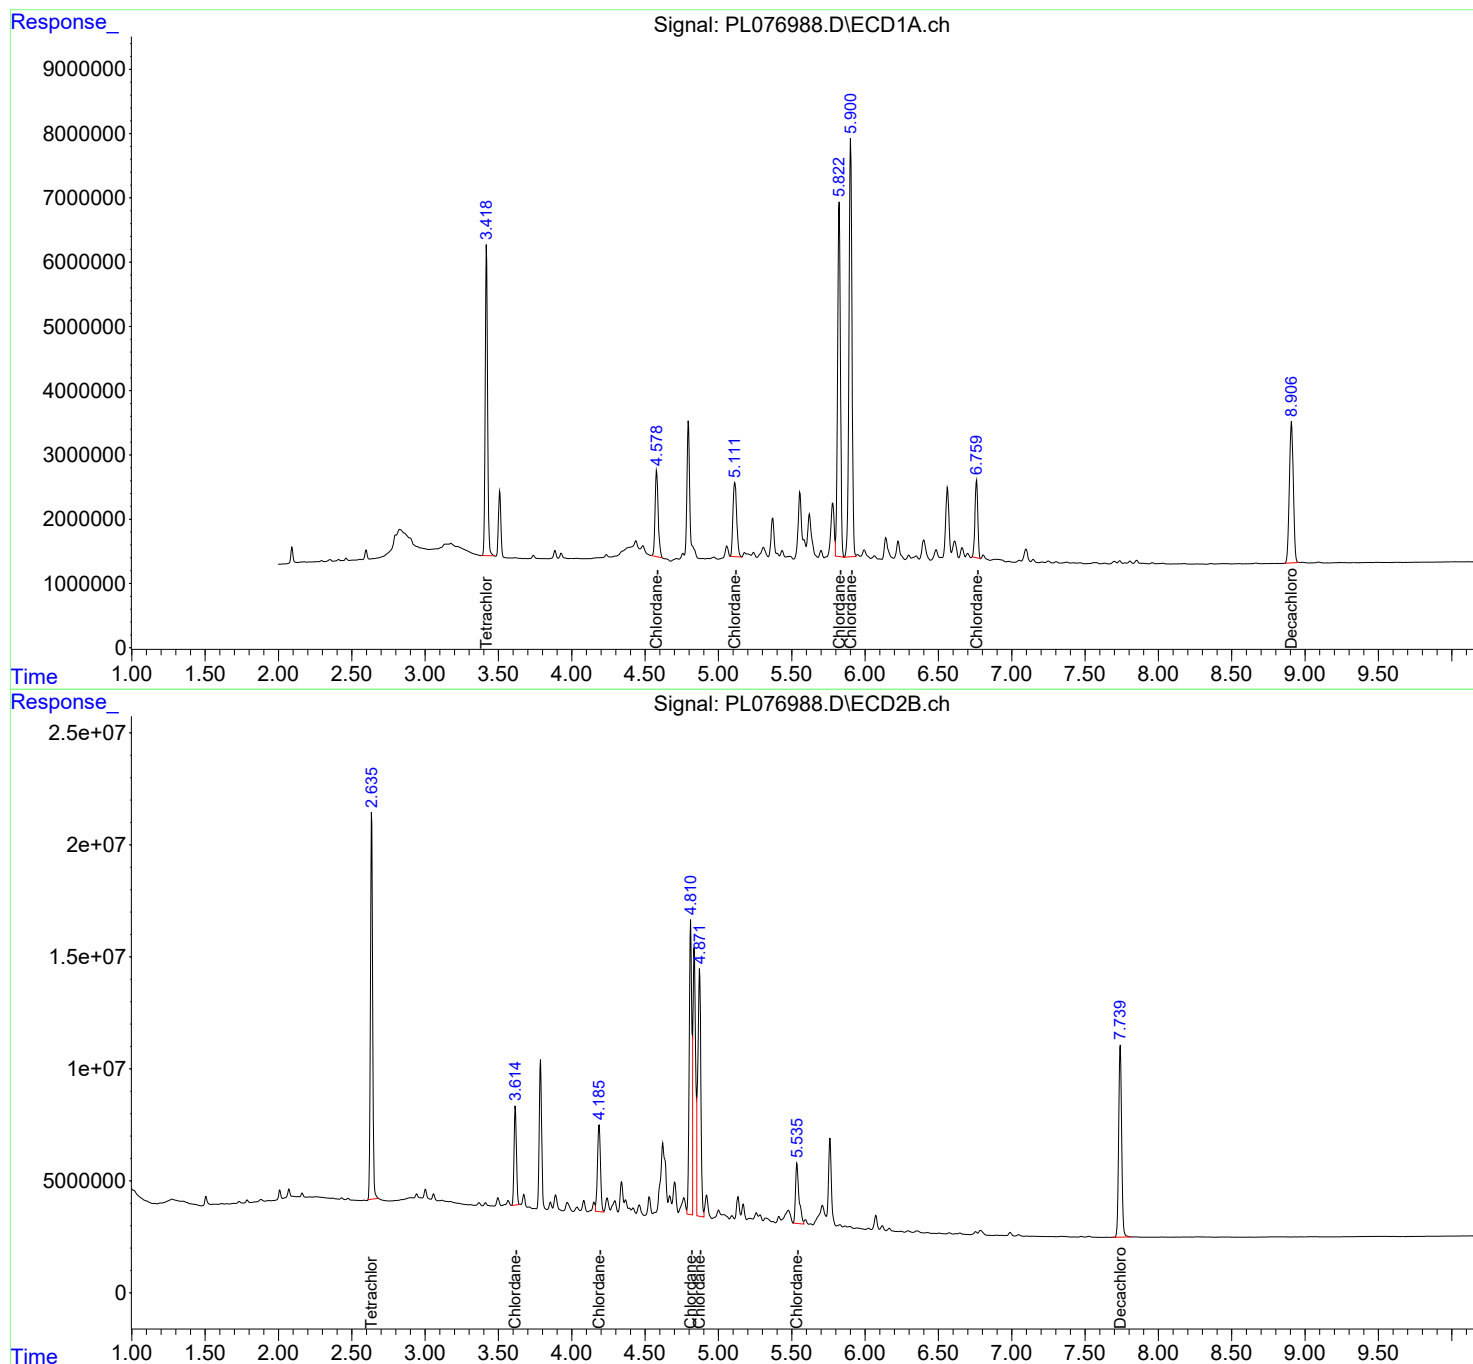


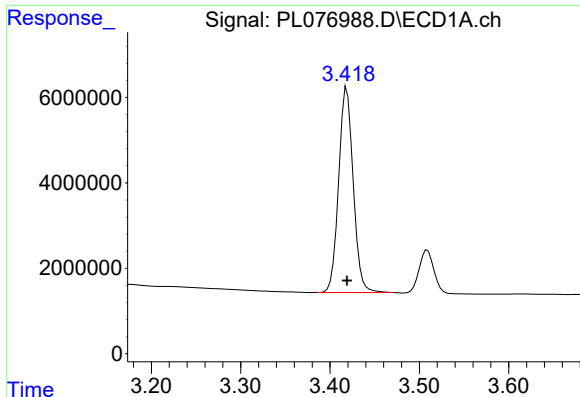

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 54336482
Conc: 51.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080822CHLOR

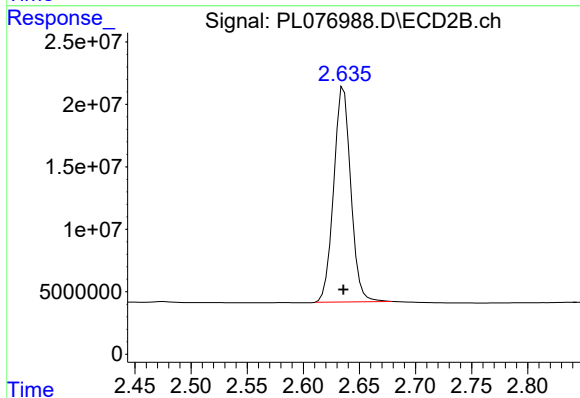


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 182757477
Conc: 50.04 ng/ml

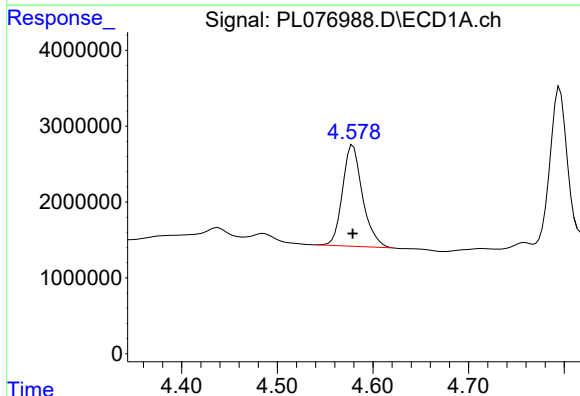


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 19394936
Conc: 514.49 ng/ml

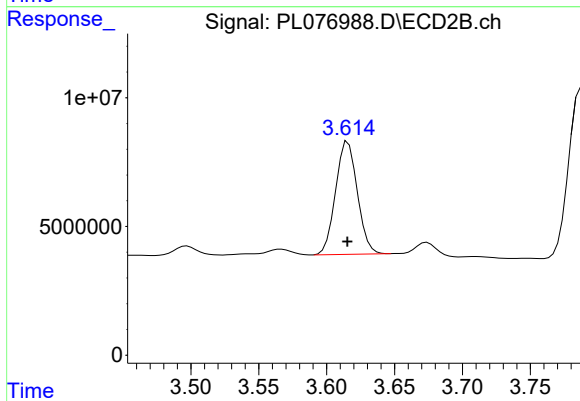

#23 Chlordane-1


R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 48820265
Conc: 501.26 ng/ml

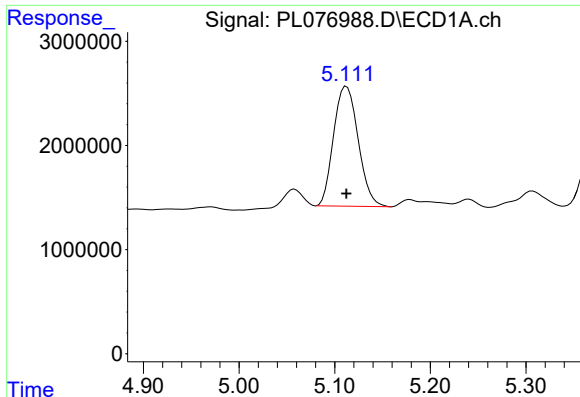

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 20595075
Conc: 518.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080822CHLOR

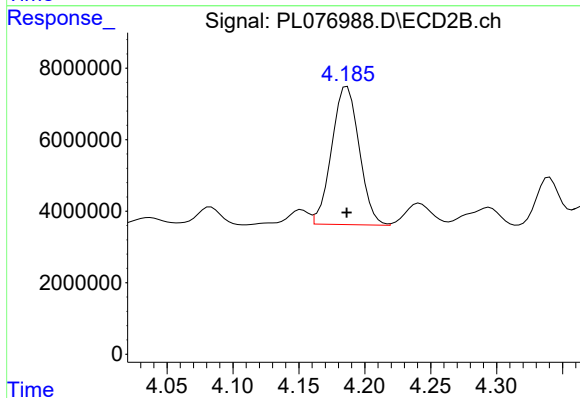


#24 Chlordane-2

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 56072068
Conc: 487.53 ng/ml

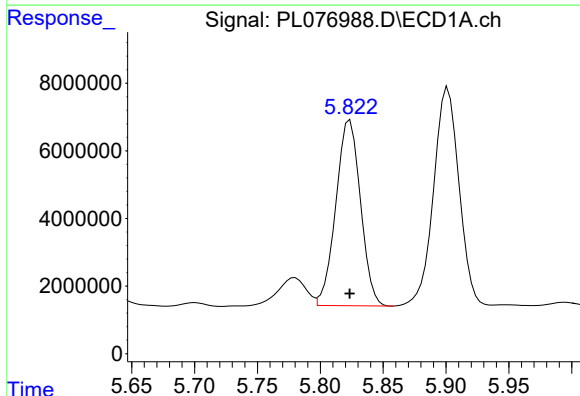


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 74897840
Conc: 515.22 ng/ml

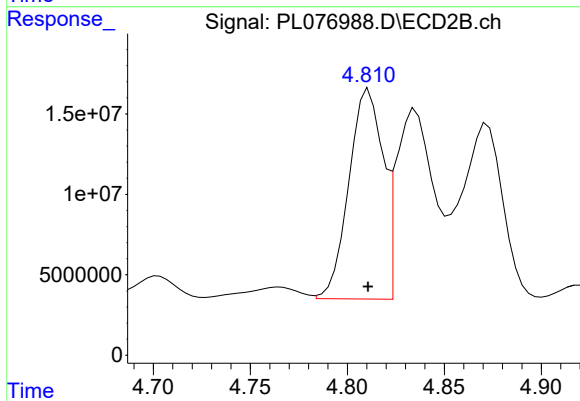

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 158696300
Conc: 501.25 ng/ml

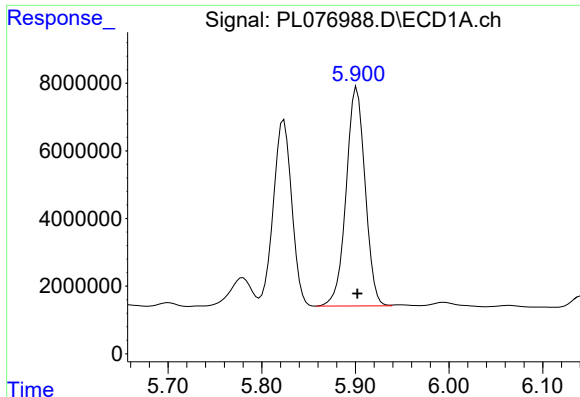

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 90989883
Conc: 515.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080822CHLOR

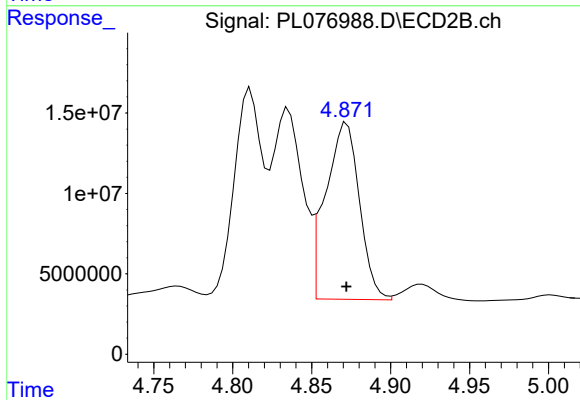


#26 Chlordane-4

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 163684924
Conc: 496.98 ng/ml

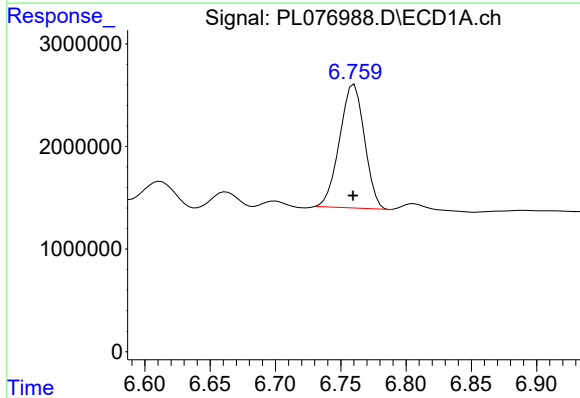


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.001 min
Response: 15981287
Conc: 527.46 ng/ml

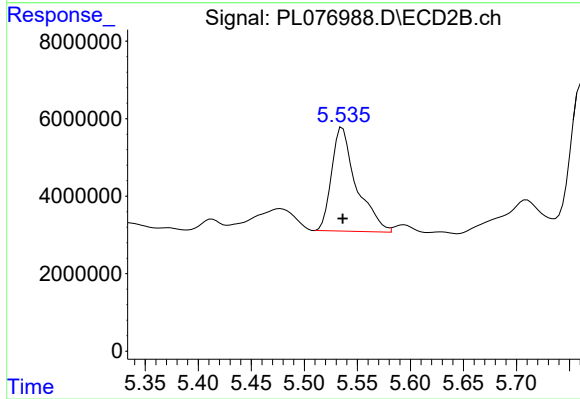

#27 Chlordane-5


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 43520269
Conc: 477.28 ng/ml

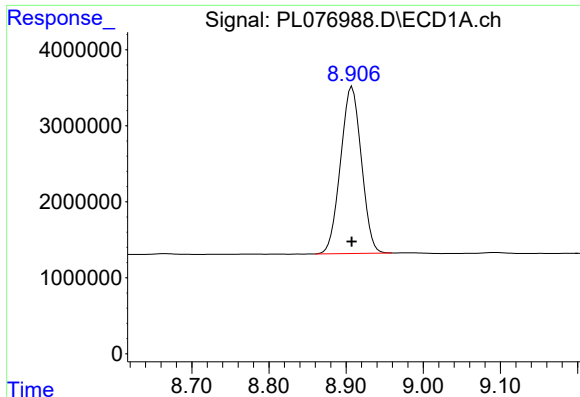

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 41133736
Conc: 50.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL080822CHLOR

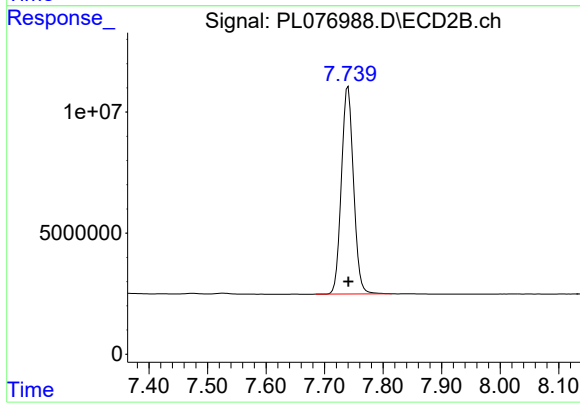

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 123240550
Conc: 49.12 ng/ml