

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 19:25
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:08:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 07:07:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	81374843	279.8E6	74.701	74.318
28)	SA Decachlor...	8.907	7.740	58605530	183.1E6	72.676	72.661
Target Compounds							
23)	Chlordane-1	4.579	3.616	28914174	74652696	748.059	748.889
24)	Chlordane-2	5.112	4.186	29622638	83730360	724.535	729.181
25)	Chlordane-3	5.824	4.811	112.6E6	243.5E6	761.329	753.757
26)	Chlordane-4	5.902	4.872	135.7E6	251.6E6	756.643	750.779
27)	Chlordane-5	6.761	5.536	23523693	65648732	741.405	725.306



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 19:25
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:08:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 07:07:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

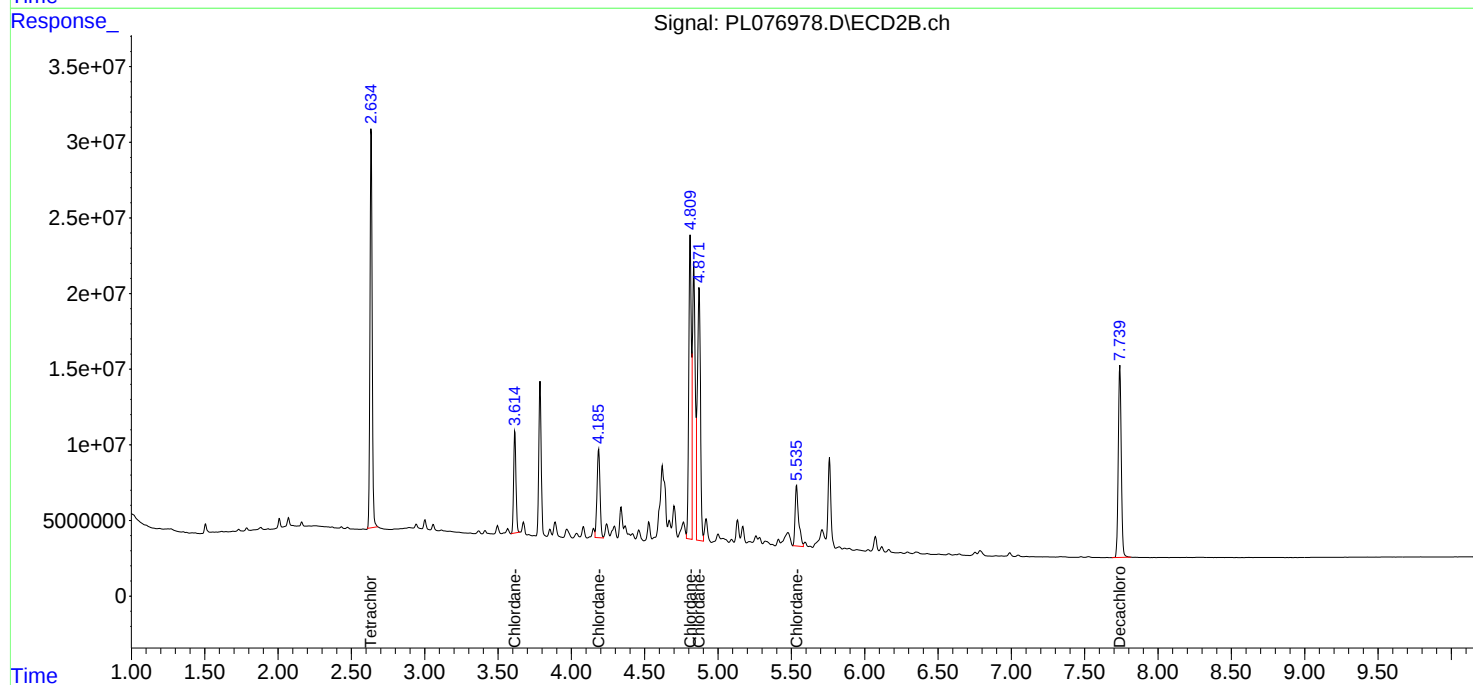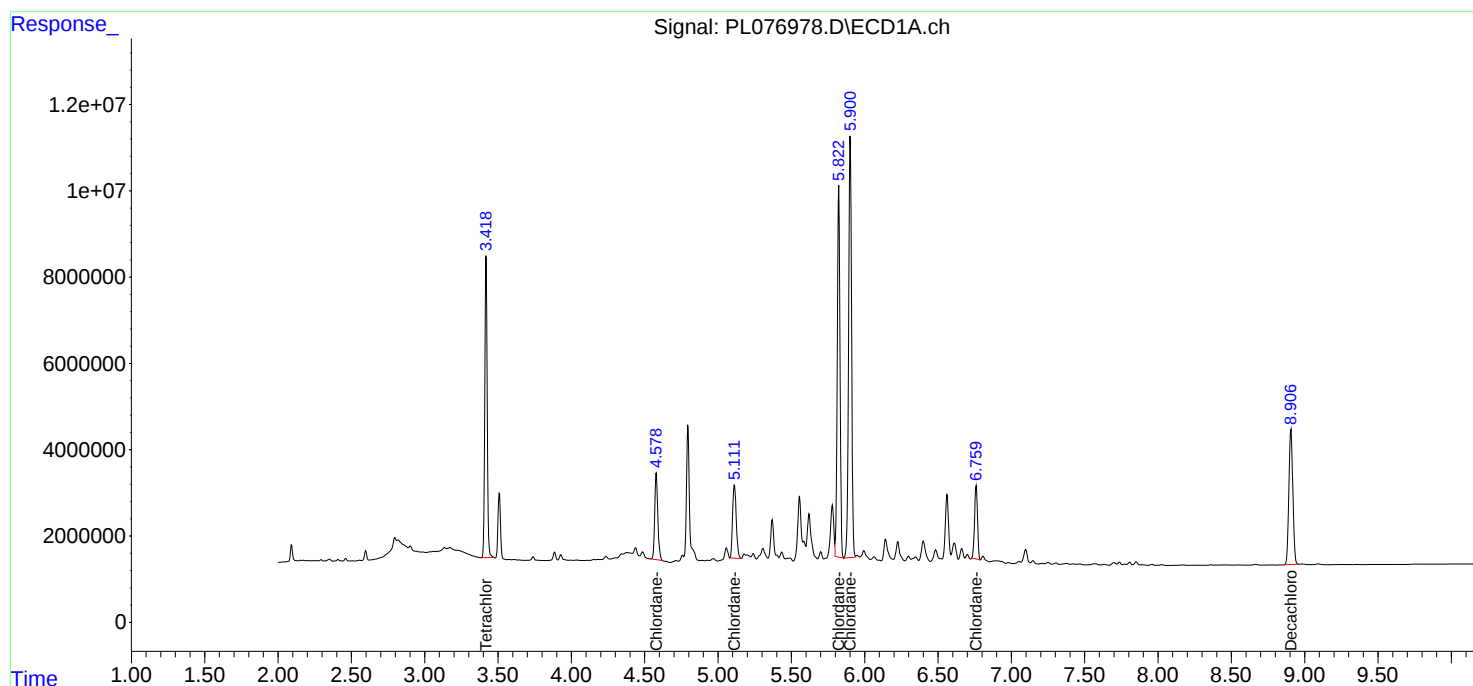


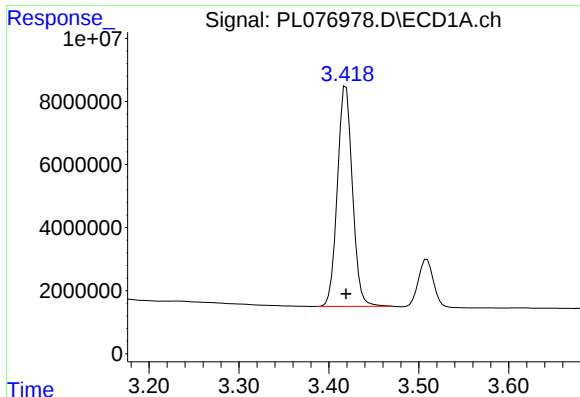

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 81374843
Conc: 74.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

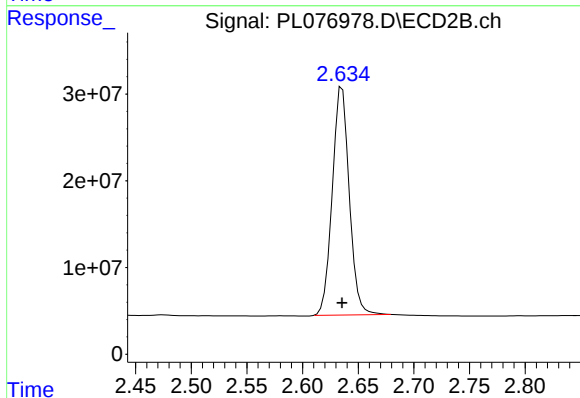


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 279847174
Conc: 74.32 ng/ml

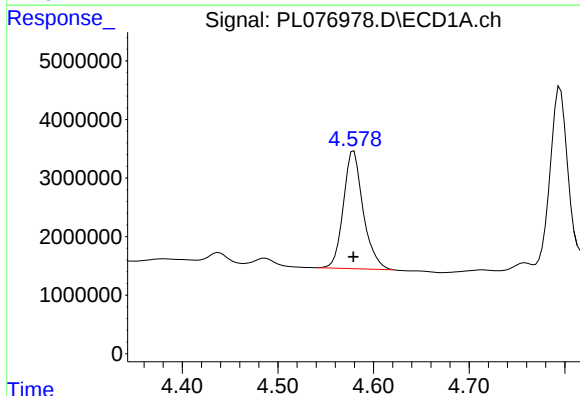


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 28914174
Conc: 748.06 ng/ml

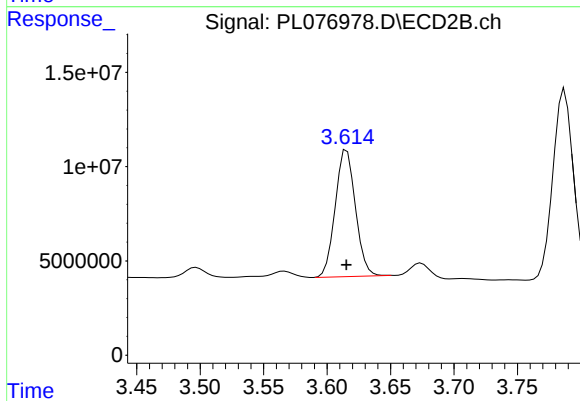

#23 Chlordane-1


R.T.: 3.616 min
Delta R.T.: 0.000 min
Response: 74652696
Conc: 748.89 ng/ml

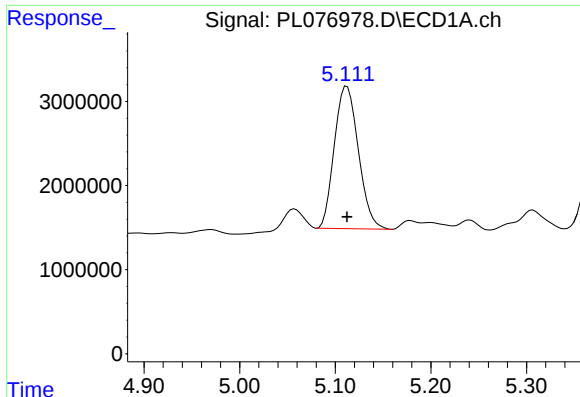

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 29622638
Conc: 724.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

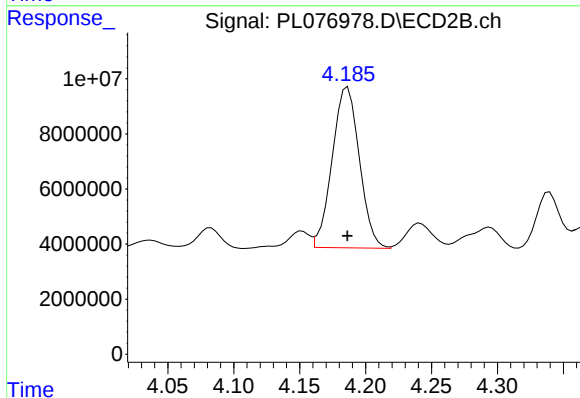


#24 Chlordane-2

R.T.: 4.186 min
Delta R.T.: 0.000 min
Response: 83730360
Conc: 729.18 ng/ml

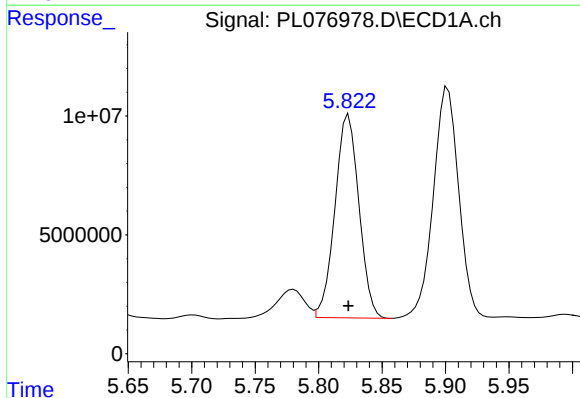


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 112581937
Conc: 761.33 ng/ml

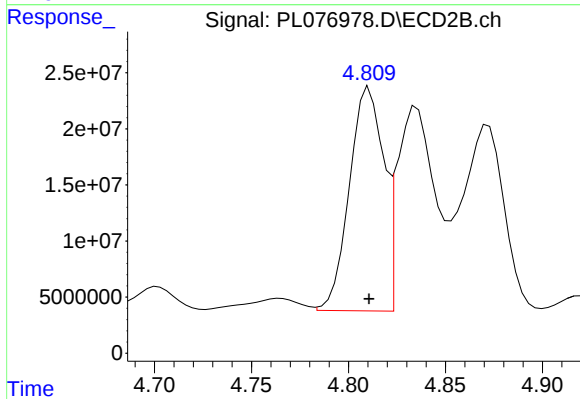

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 243543330
Conc: 753.76 ng/ml

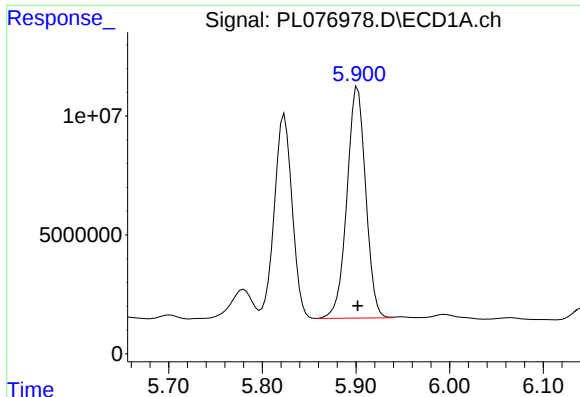

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 135675403
Conc: 756.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

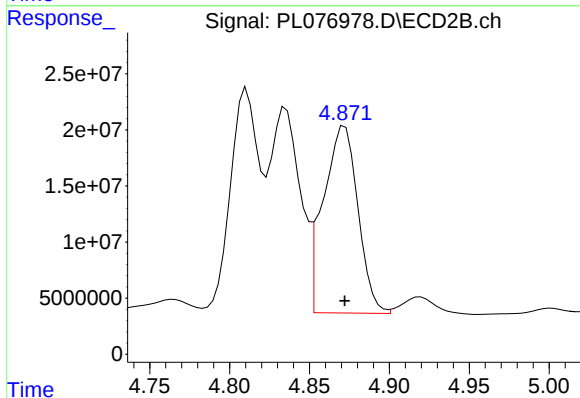


#26 Chlordane-4

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 251604117
Conc: 750.78 ng/ml

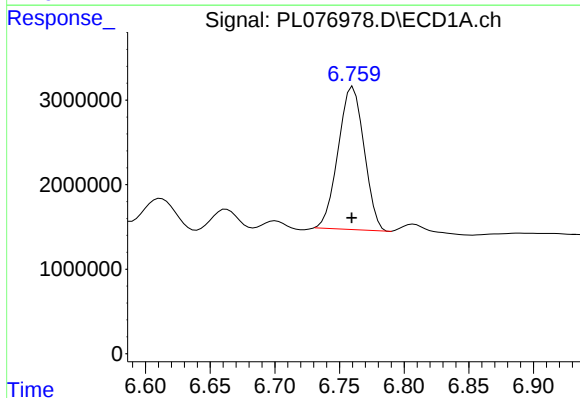


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.001 min
Response: 23523693
Conc: 741.41 ng/ml

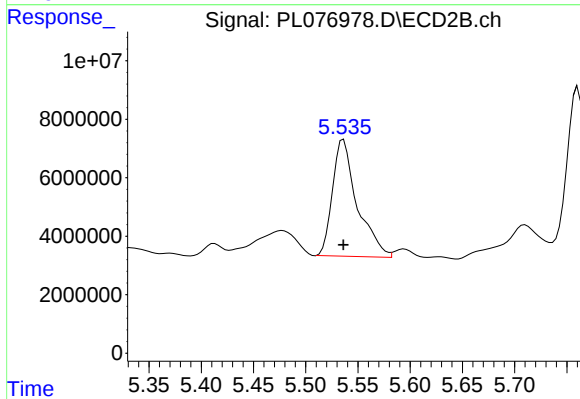

#27 Chlordane-5


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 65648732
Conc: 725.31 ng/ml

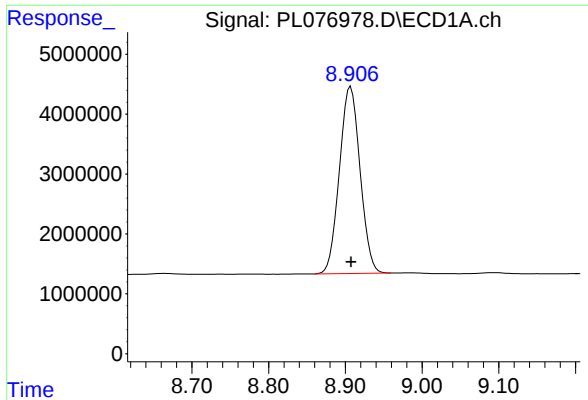

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 58605530
Conc: 72.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

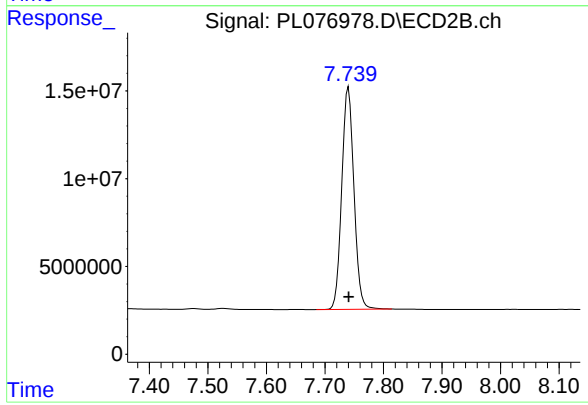

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 183065862
Conc: 72.66 ng/ml