

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
 Data File : PL076979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 19:39
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:08:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 07:07:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	54467020	188.3E6	50.000	50.000
28)	SA Decachlor...	8.907	7.740	40319788	126.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.579	3.615	19326128	49842304	500.000	500.000
24)	Chlordane-2	5.112	4.186	20442503	57414001	500.000	500.000
25)	Chlordane-3	5.823	4.811	73937732	161.6E6	500.000	500.000
26)	Chlordane-4	5.902	4.872	89656101	167.6E6	500.000	500.000
27)	Chlordane-5	6.759	5.536	15864264	45255875	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080822\
Data File : PL076979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 19:39
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:08:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 07:07:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

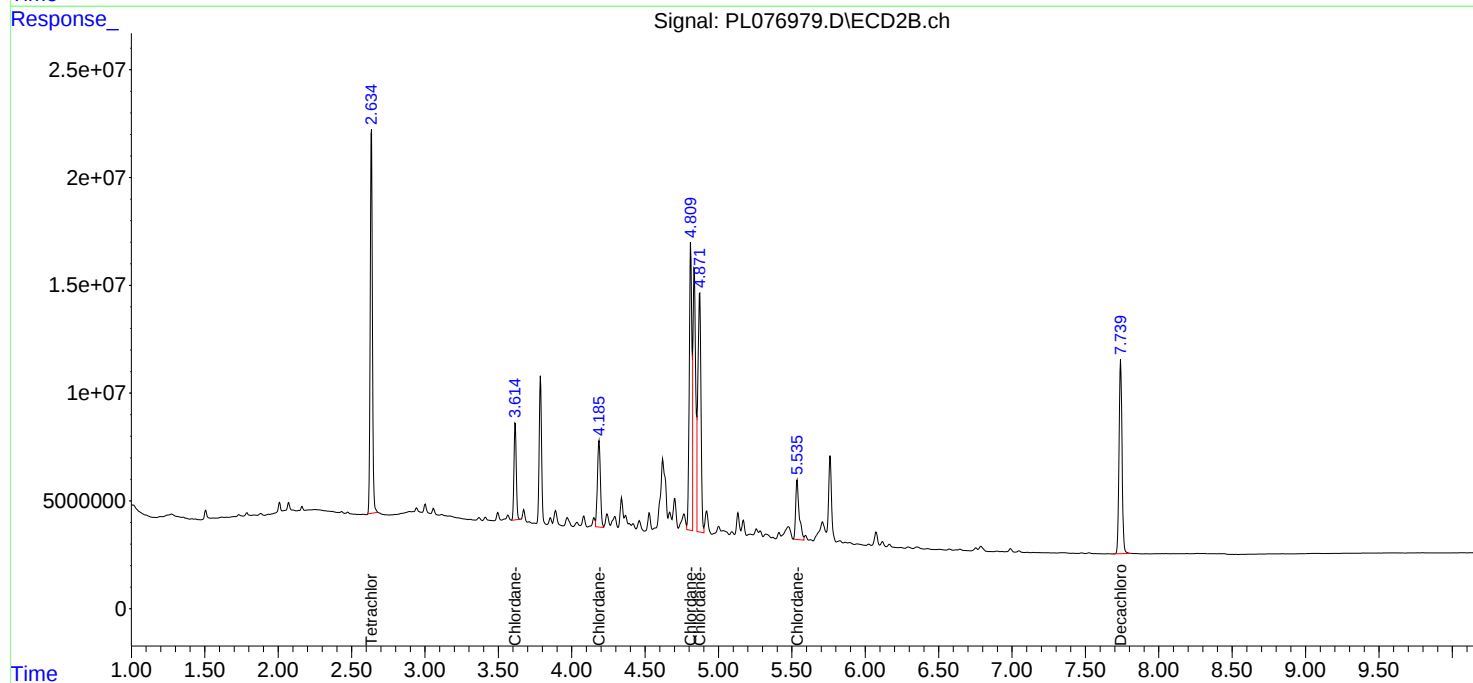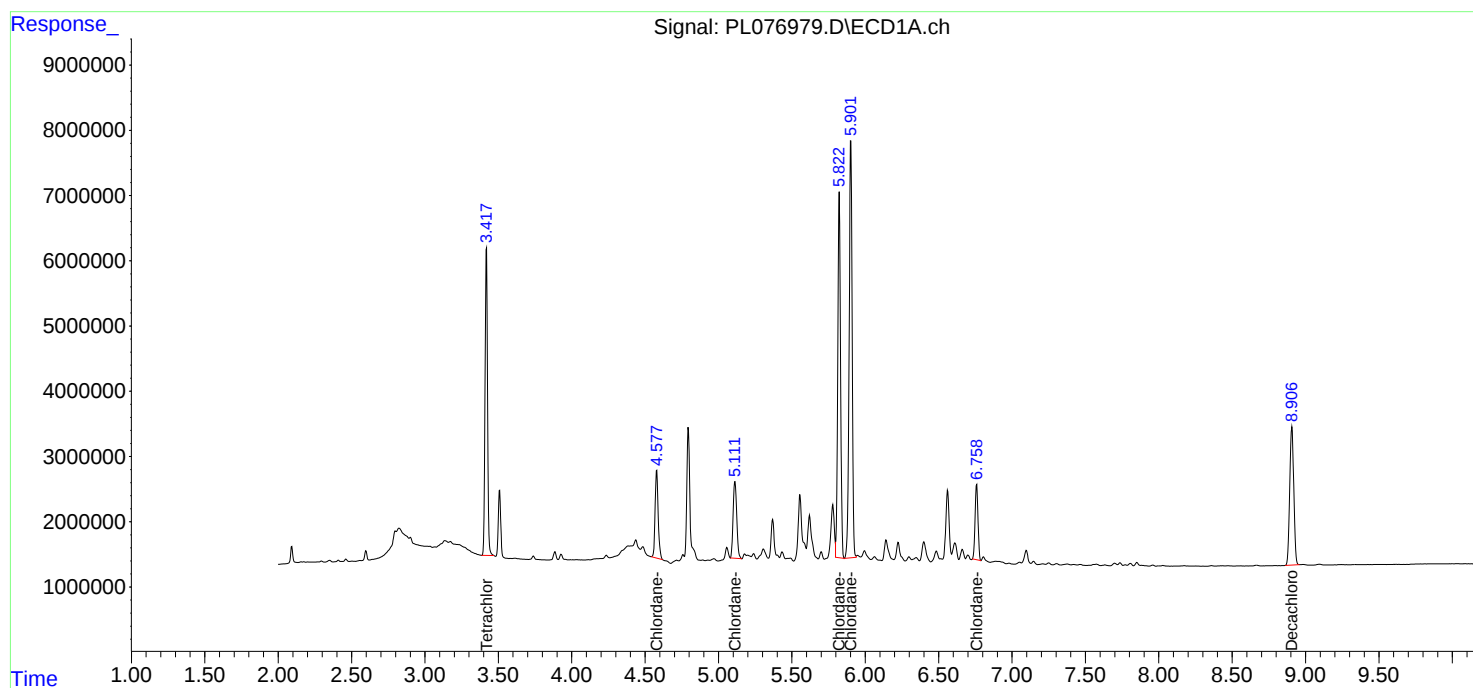


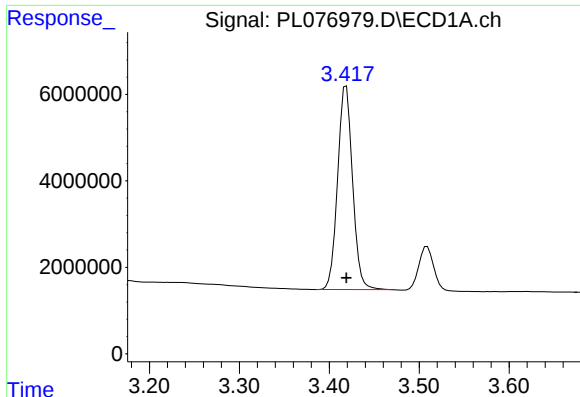

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 54467020
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

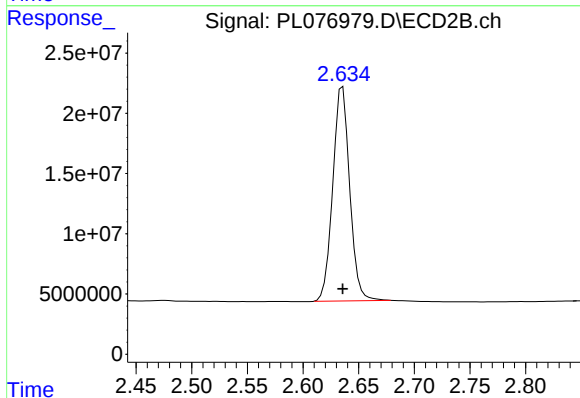


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 188276482
Conc: 50.00 ng/ml

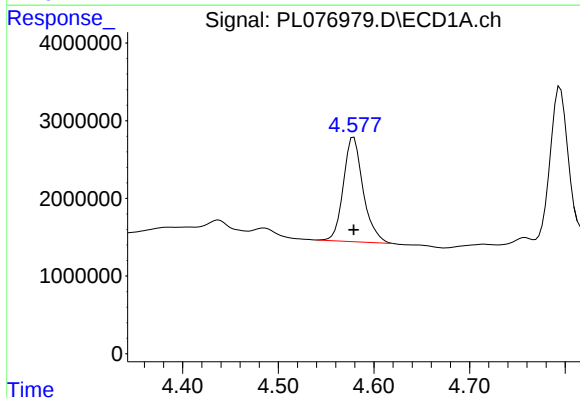


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 19326128
Conc: 500.00 ng/ml

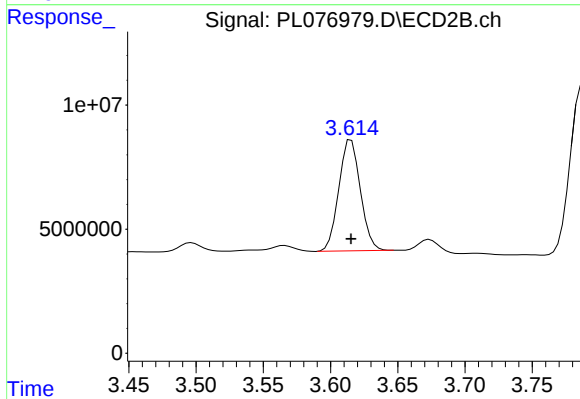

#23 Chlordane-1


R.T.: 3.615 min
Delta R.T.: 0.000 min
Response: 49842304
Conc: 500.00 ng/ml

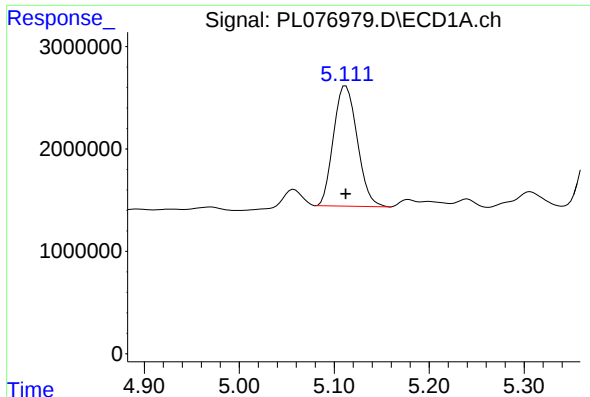

#24 Chlordane-2


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 20442503
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

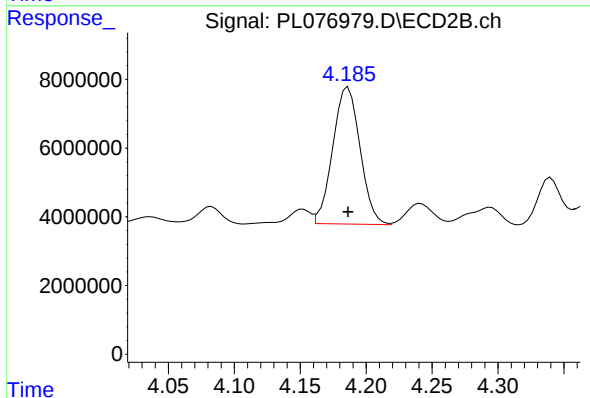


#24 Chlordane-2

R.T.: 4.186 min
Delta R.T.: 0.000 min
Response: 57414001
Conc: 500.00 ng/ml

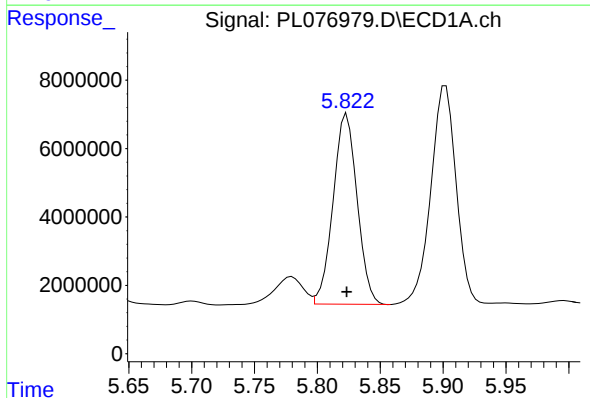


#25 Chlordane-3

R.T.: 5.823 min
Delta R.T.: 0.000 min
Response: 73937732
Conc: 500.00 ng/ml

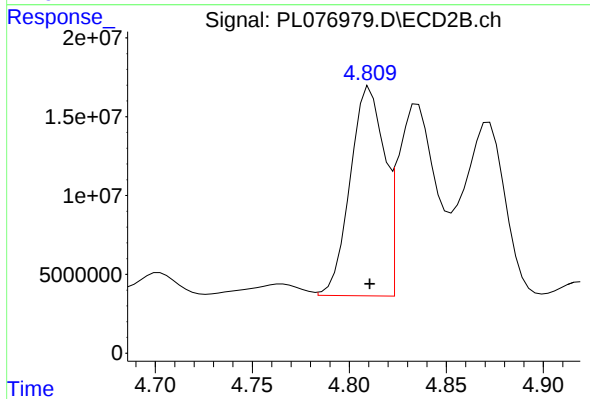

#25 Chlordane-3


R.T.: 4.811 min
Delta R.T.: 0.000 min
Response: 161552855
Conc: 500.00 ng/ml

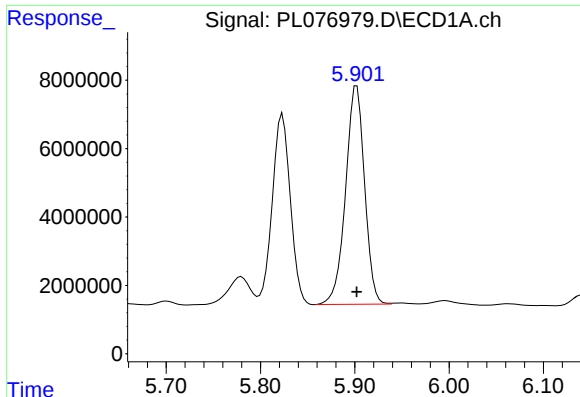

#26 Chlordane-4


R.T.: 5.902 min
Delta R.T.: 0.000 min
Response: 89656101
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

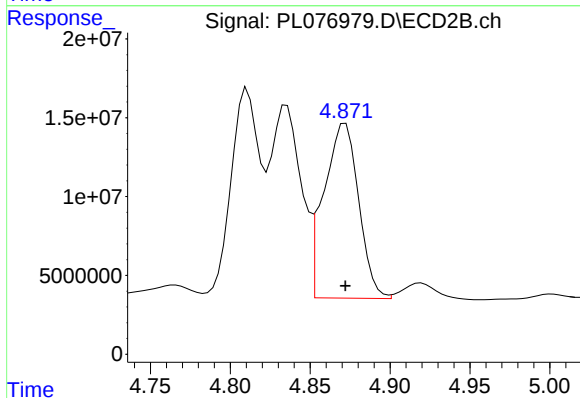


#26 Chlordane-4

R.T.: 4.872 min
Delta R.T.: 0.000 min
Response: 167561965
Conc: 500.00 ng/ml

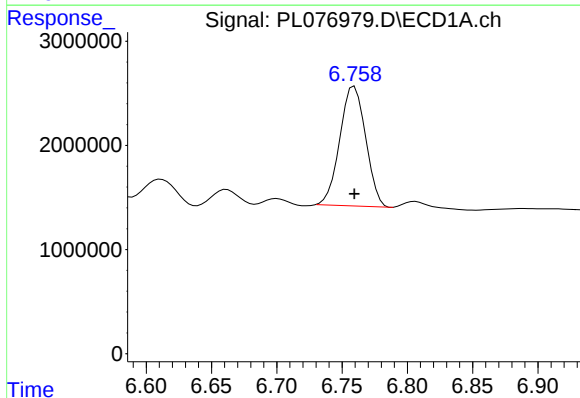


#27 Chlordane-5

R.T.: 6.759 min
Delta R.T.: 0.000 min
Response: 15864264
Conc: 500.00 ng/ml

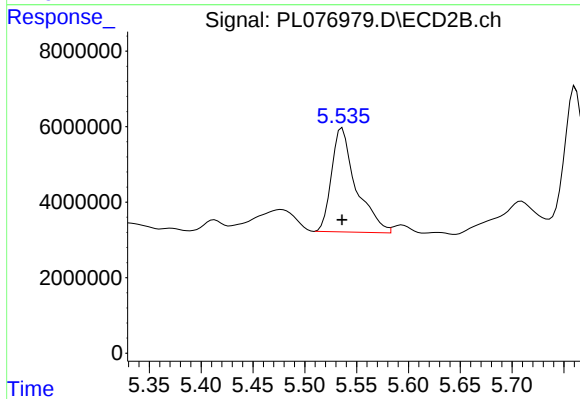

#27 Chlordane-5


R.T.: 5.536 min
Delta R.T.: 0.000 min
Response: 45255875
Conc: 500.00 ng/ml

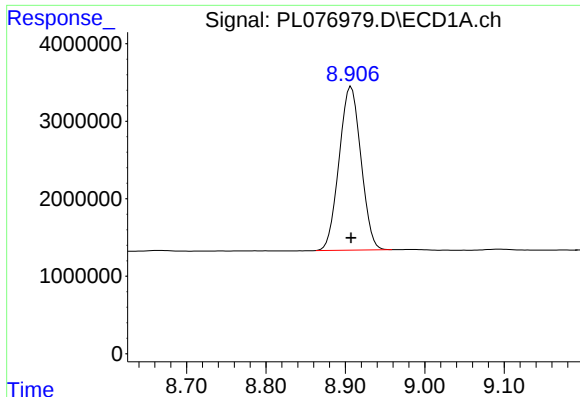

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 40319788
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

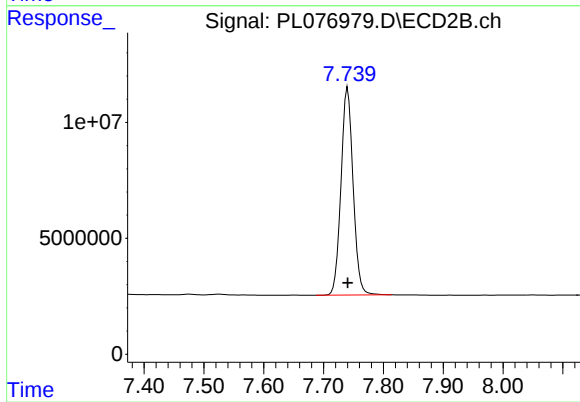

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 125972531
Conc: 50.00 ng/ml