

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080823\
 Data File : PL084583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 16:07
 Operator : AR\AJ
 Sample : 03929-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-PP20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:12:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.686	41132915	19868720	17.703	18.272
28)	SA Decachlor...	9.028	7.868	24207772	18604930	14.878	14.922
Target Compounds							
10)	B gamma-Chl...	5.891	4.900	1168793	588994	0.408	0.434
11)	B alpha-Chl...	5.971	4.966	2185834	1095546	0.774	0.804


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080823\
Data File : PL084583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2023 16:07
Operator : AR\AJ
Sample : 03929-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
B-PP20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:12:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

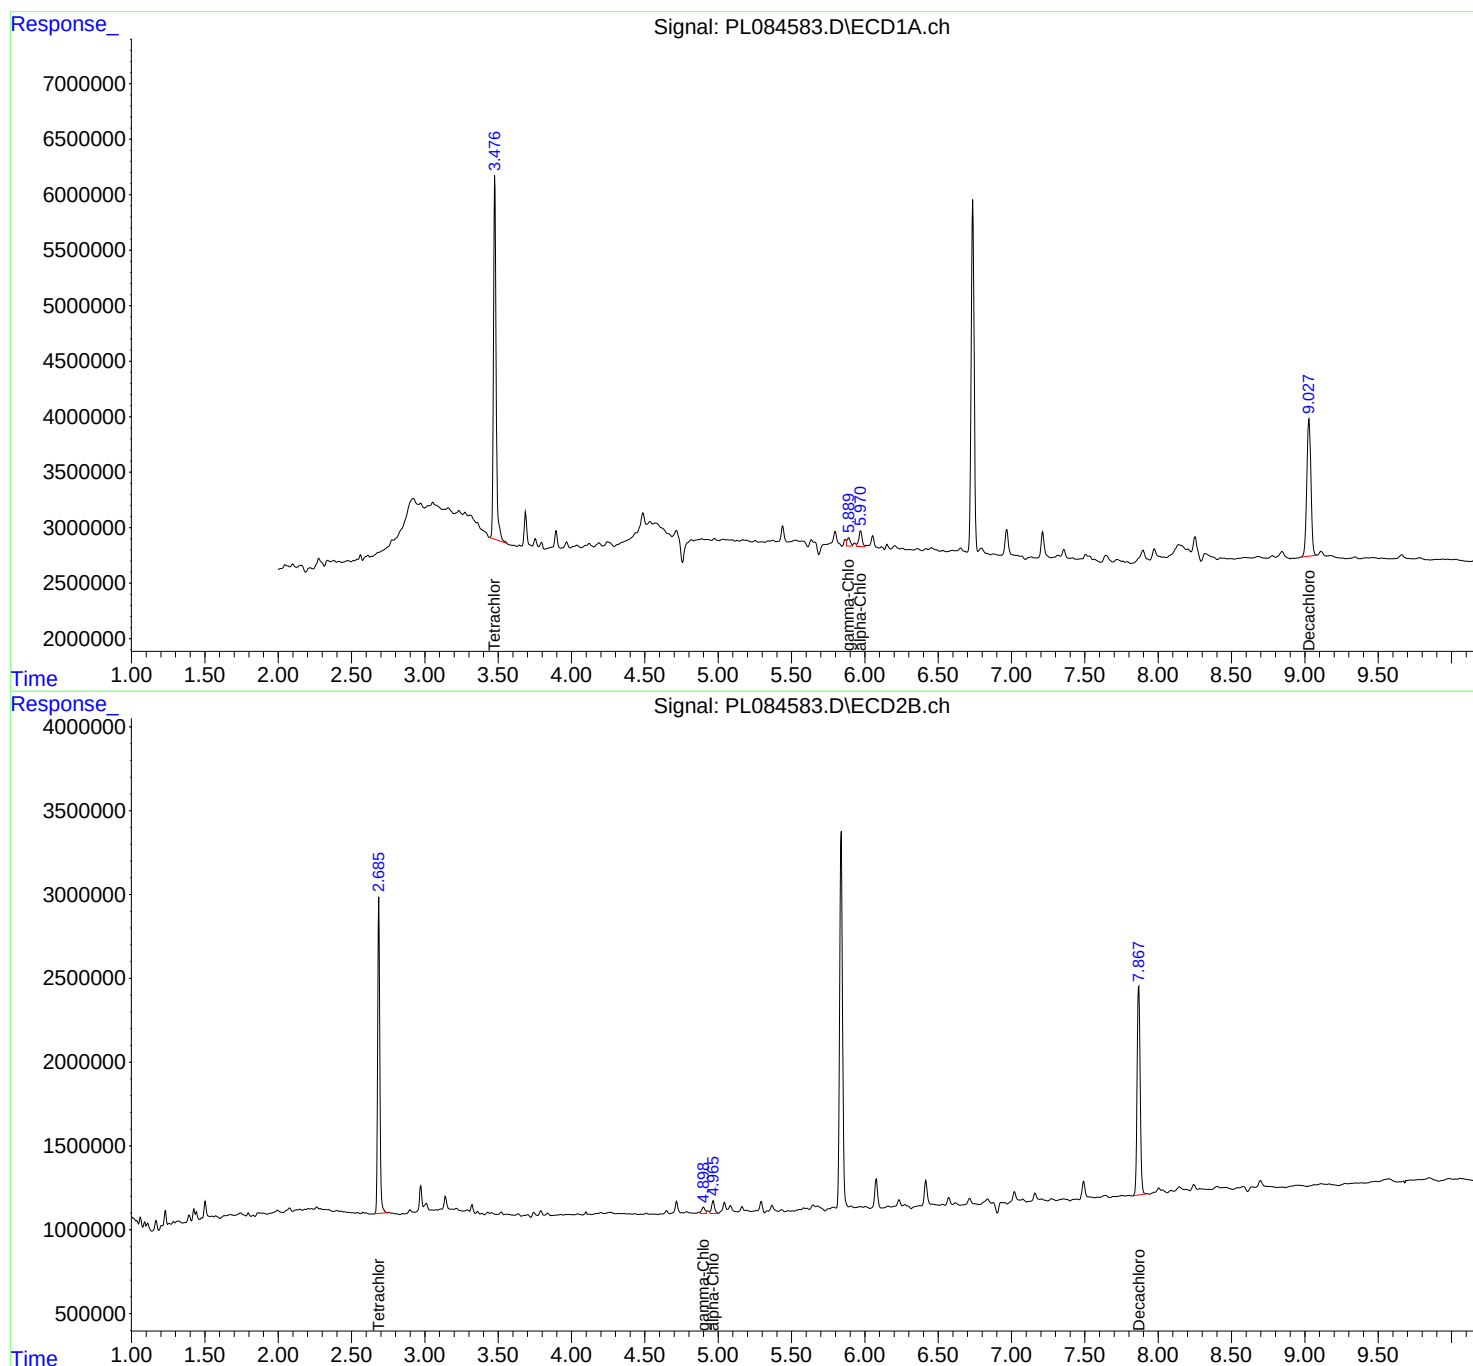


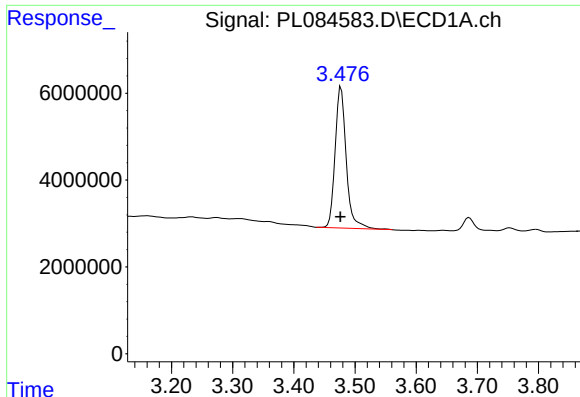

#1 Tetrachloro-m-xylene


R.T.: 3.477 min
Delta R.T.: 0.001 min
Response: 41132915
Conc: 17.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-PP20

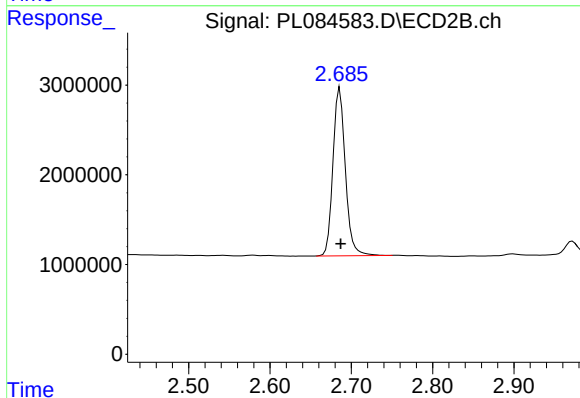


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: 0.000 min
Response: 19868720
Conc: 18.27 ng/ml

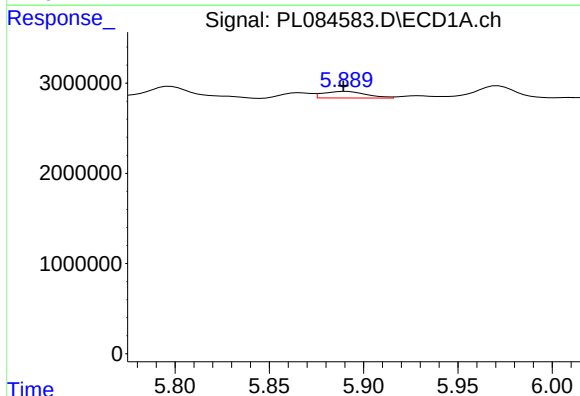


#10 gamma-Chlordane

R.T.: 5.891 min
Delta R.T.: 0.002 min
Response: 1168793
Conc: 0.41 ng/ml

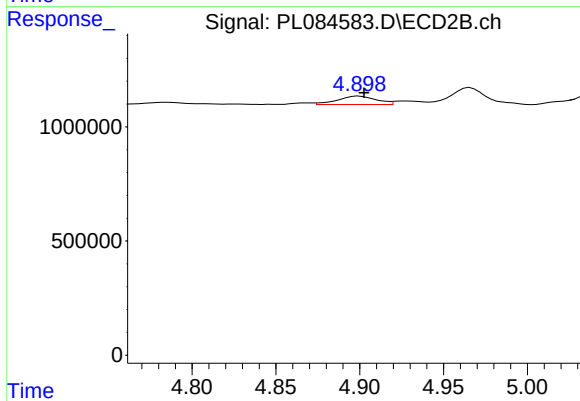

#10 gamma-Chlordane


R.T.: 4.900 min
Delta R.T.: -0.003 min
Response: 588994
Conc: 0.43 ng/ml

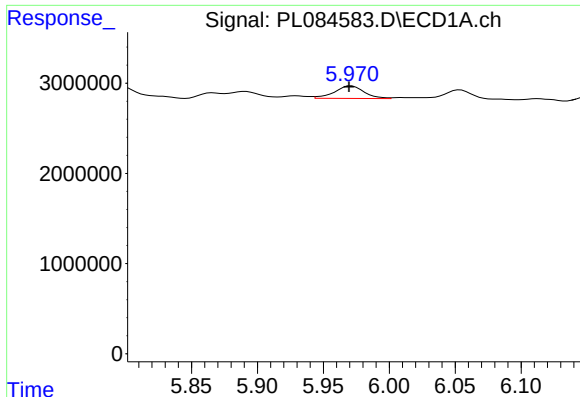

#11 alpha-Chlordane


R.T.: 5.971 min
Delta R.T.: 0.002 min
Response: 2185834
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-PP20

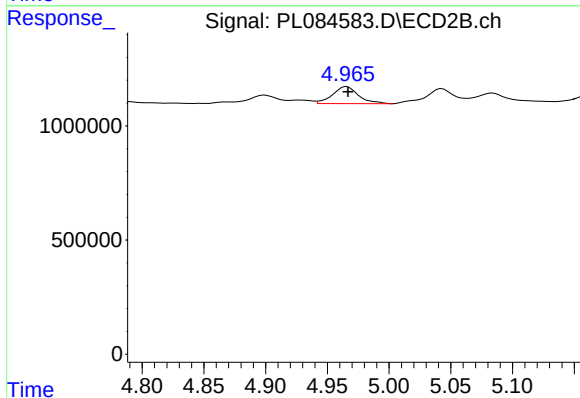


#11 alpha-Chlordane

R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 1095546
Conc: 0.80 ng/ml

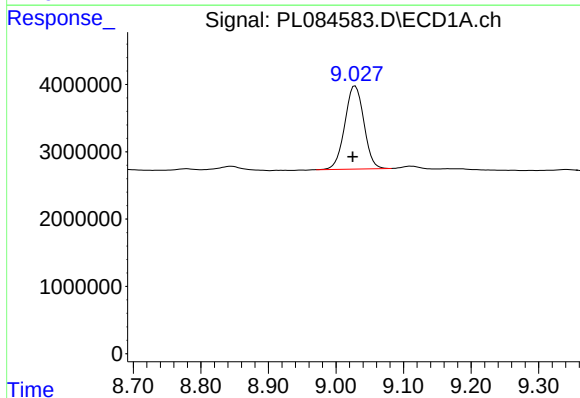

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: 0.003 min
Response: 24207772
Conc: 14.88 ng/ml

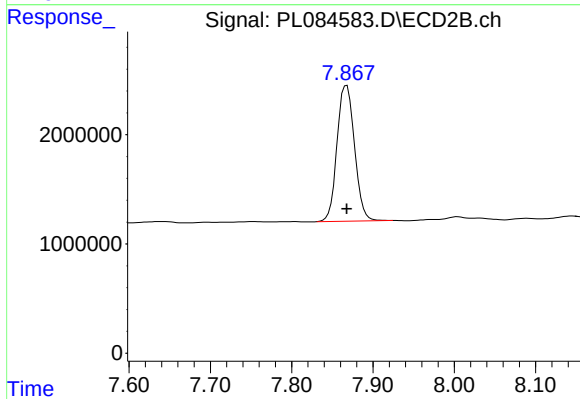

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 18604930
Conc: 14.92 ng/ml