

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080824\
 Data File : PL090863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2024 09:21
 Operator : AR\AJ
 Sample : TOXAPH101
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TOXAPH1300

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 06:46:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 10 06:46:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.786	11293213	9059061	5.104	4.977
27)	SA Decachlor...	9.055	7.927	9442814	8977272	10.269	10.086
Target Compounds							
22)	Toxaphene-1	5.855	5.017	4245125	5686764	531.698	506.538
23)	Toxaphene-2	6.443	5.701	10025409	4403203	558.387	467.501
24)	Toxaphene-3	7.061	6.615	27050093	16494552	522.313	459.769
25)	Toxaphene-4	7.153	6.743	20500912	23457796	523.484	469.725
26)	Toxaphene-5	7.572	7.055	13984673	16033468	510.132	476.932

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080824\
Data File : PL090863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2024 09:21
Operator : AR\AJ
Sample : TOXAPH101
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 06:46:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 10 06:46:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

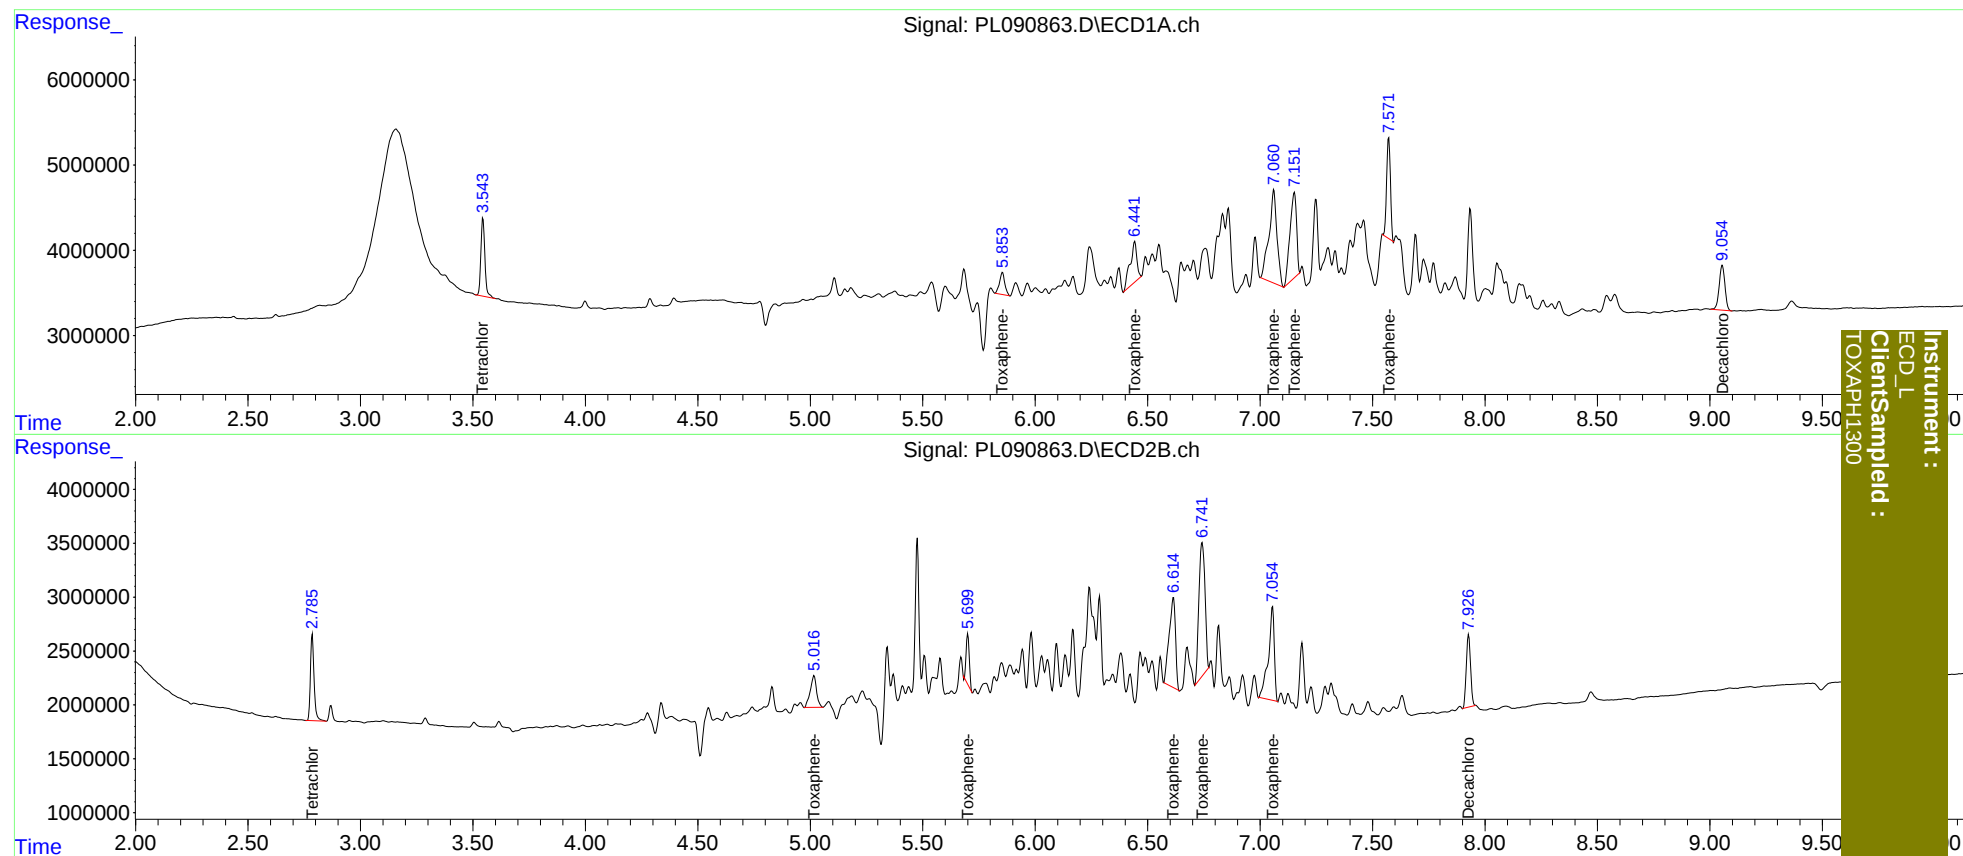

Instrument :
ECD_L
ClientSampled :
TOXAPH1300