

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
 Data File : PL039058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2018 12:39
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:02:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	167.3E6	66912640	22.470	25.491
28)	SA Decachlor...	7.992	8.935	162.5E6	62854688	21.425	25.713
Target Compounds							
3)	MA gamma-BHC...	0.000	4.548f	0	200191	N.D.	0.055 #
7)	B delta-BHC	0.000	4.956	0	2120635	N.D.	0.639 #
8)	B Heptachlo...	0.000	5.801	0	114583	N.D.	0.040 #
15)	B Endosulfa...	0.000	6.823	0	512847	N.D.	0.214 #
23)	Chlordane-1	4.238	4.956	7631941	2120635	22.042	18.299
27)	Chlordane-5	0.000	6.823	0	512847	N.D.	5.725 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
Data File : PL039058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 12:39
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:02:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

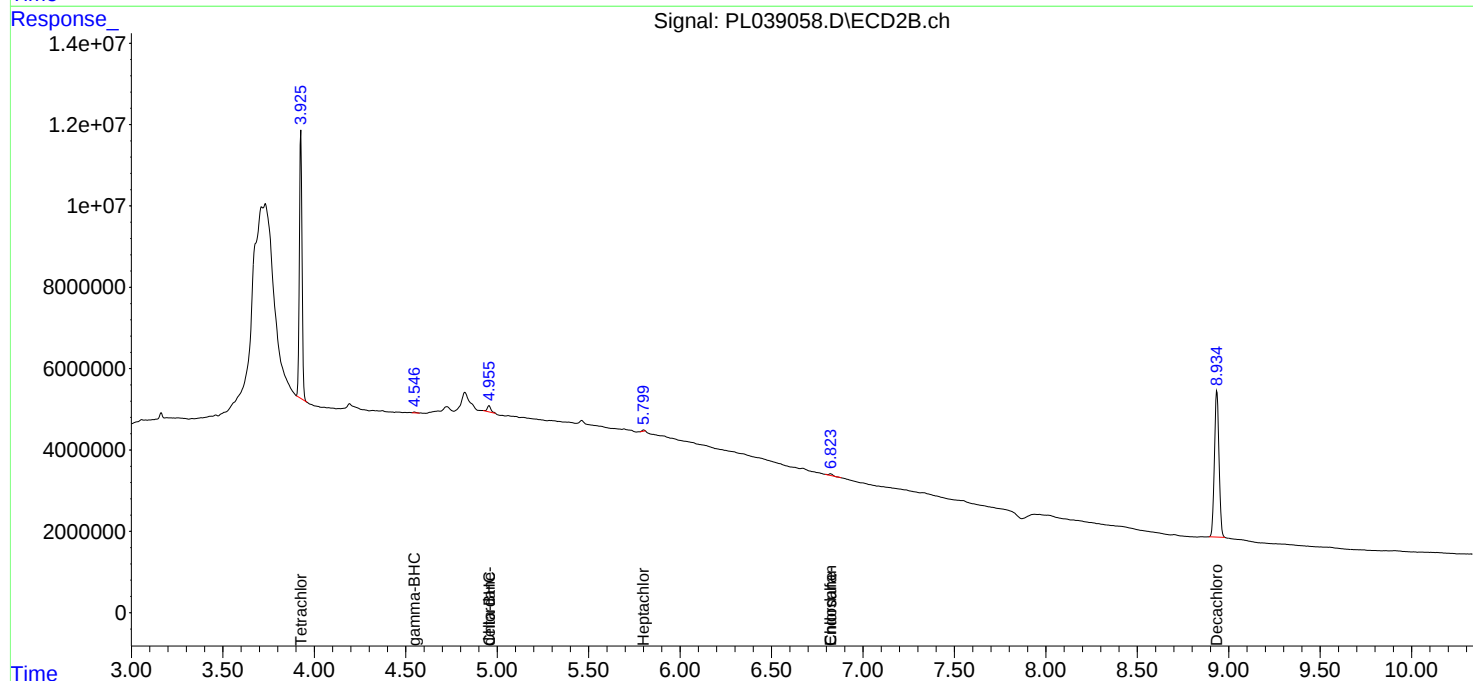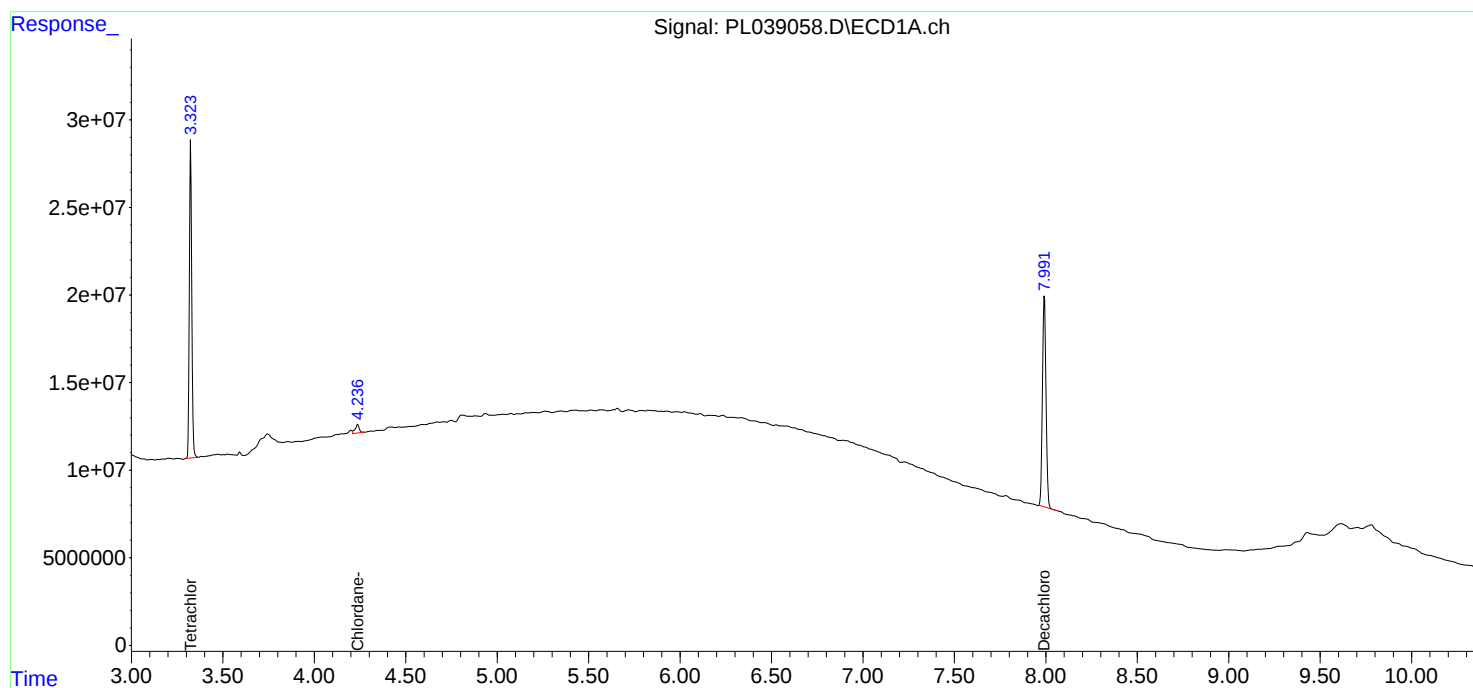


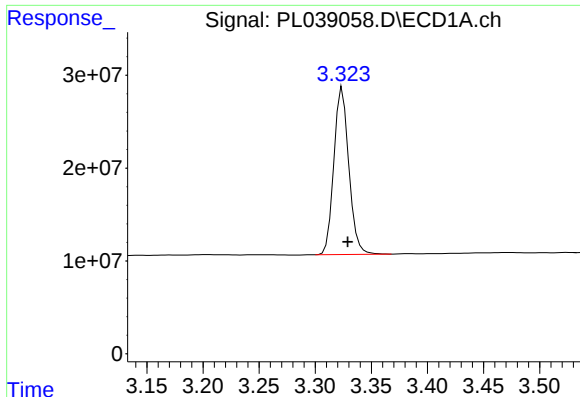

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 167321597
Conc: 22.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

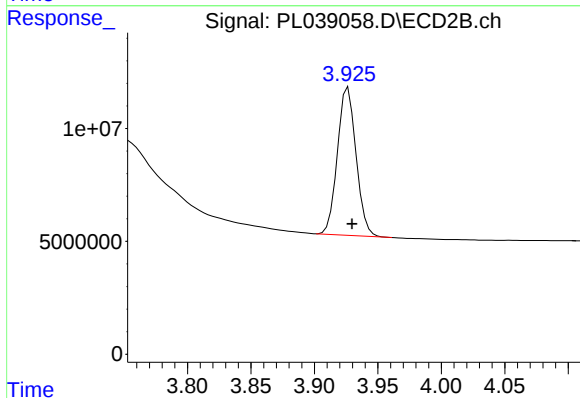


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 66912640
Conc: 25.49 ng/ml

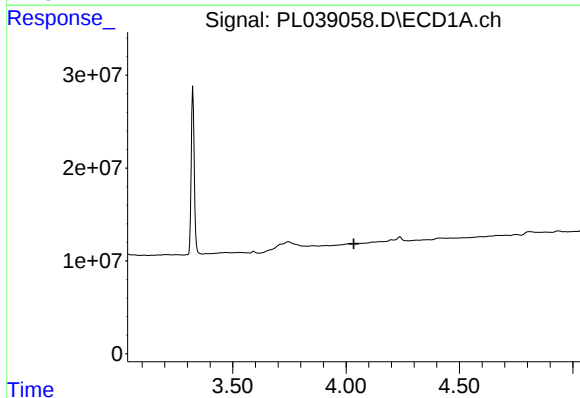


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

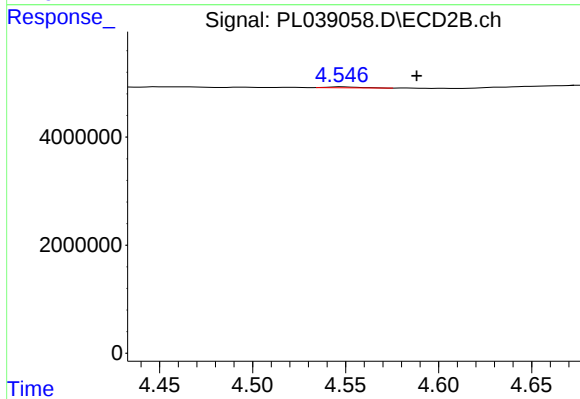

#3 gamma-BHC (Lindane)


R.T.: 4.548 min
Delta R.T.: -0.040 min
Response: 200191
Conc: 0.06 ng/ml

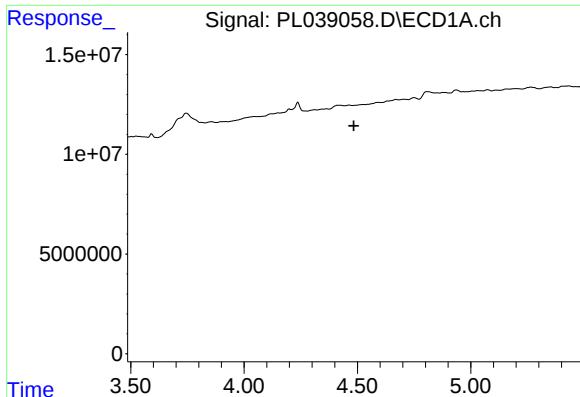

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

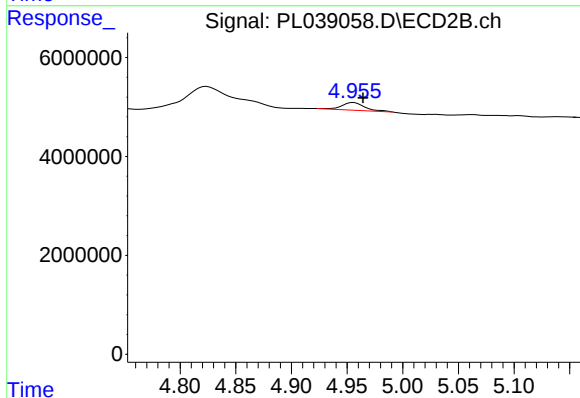


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 2120635
Conc: 0.64 ng/ml

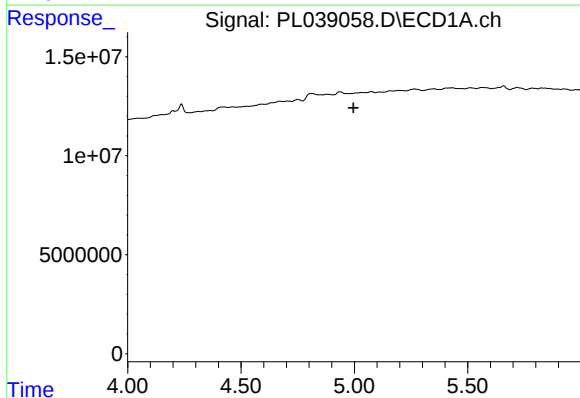


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

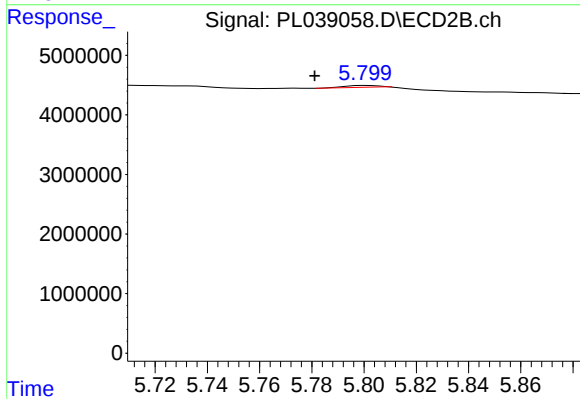

#8 Heptachlor epoxide


R.T.: 5.801 min
Delta R.T.: 0.020 min
Response: 114583
Conc: 0.04 ng/ml

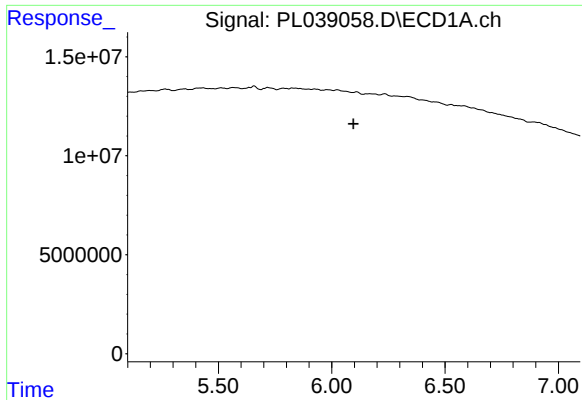

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

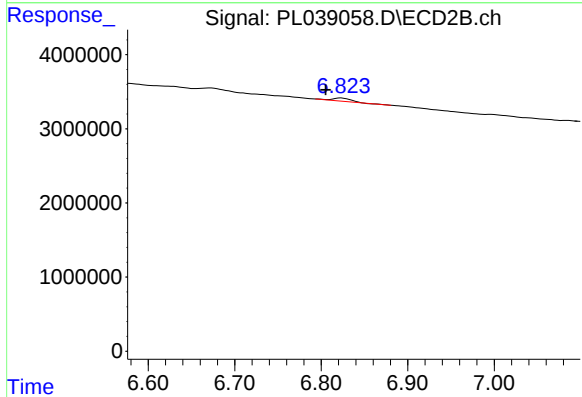


#15 Endosulfan II

R.T.: 6.823 min
Delta R.T.: 0.017 min
Response: 512847
Conc: 0.21 ng/ml

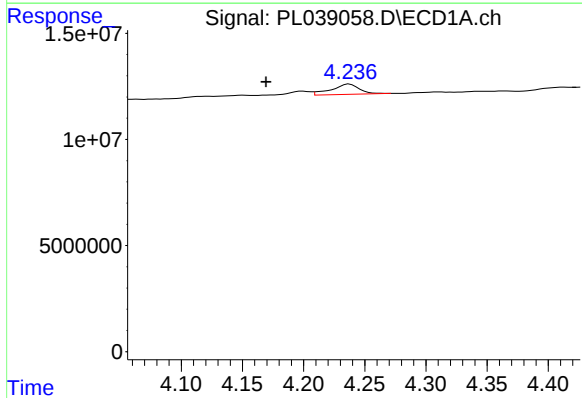


#23 Chlordane-1

R.T.: 4.238 min
Delta R.T.: 0.068 min
Response: 7631941
Conc: 22.04 ng/ml

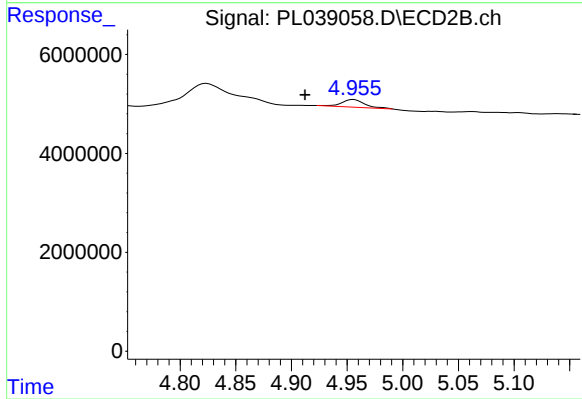

#23 Chlordane-1


R.T.: 4.956 min
Delta R.T.: 0.044 min
Response: 2120635
Conc: 18.30 ng/ml

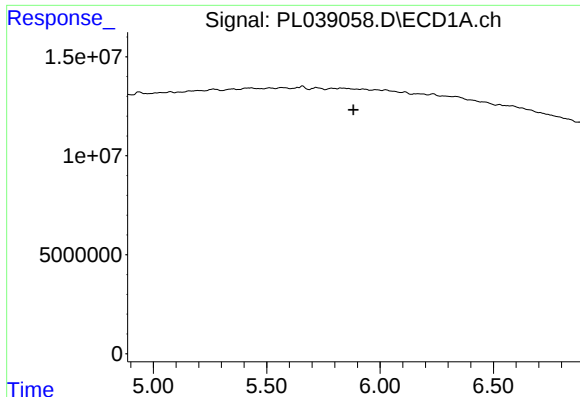

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

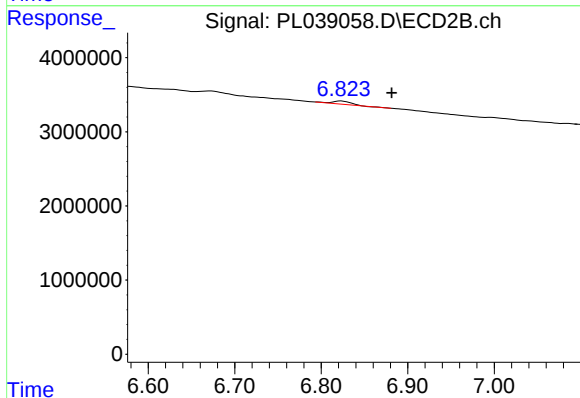


#27 Chlordane-5

R.T.: 6.823 min
Delta R.T.: -0.059 min
Response: 512847
Conc: 5.73 ng/ml

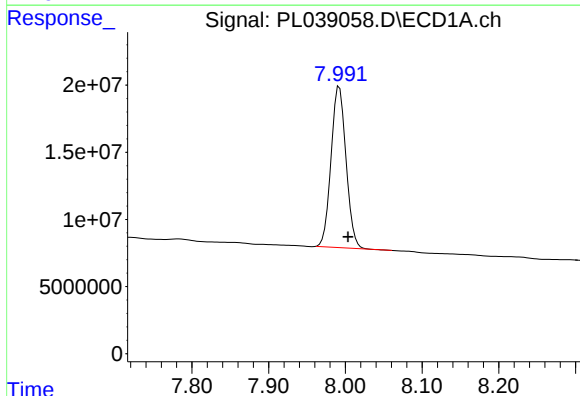

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.011 min
Response: 162530514
Conc: 21.43 ng/ml

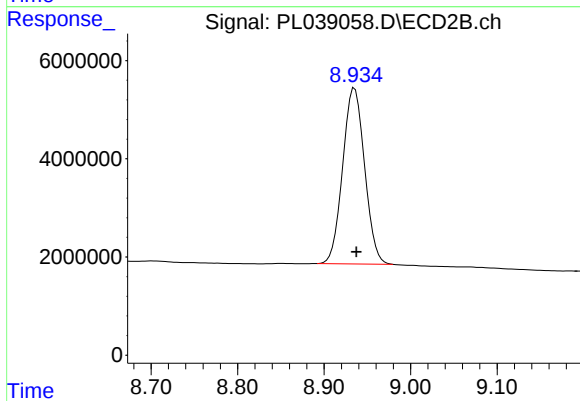

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 62854688
Conc: 25.71 ng/ml