

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
 Data File : PL039065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2018 14:19
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:08:44 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.926	166.0E6	66571614	22.296	25.361
28)	SA Decachlor...	7.990	8.935	157.6E6	61523999	20.779	25.169
Target Compounds							
2)	A alpha-BHC	0.000	4.332	0	1010256	N.D.	0.261 #
3)	MA gamma-BHC...	0.000	4.585	0	152700	N.D.	0.042 #
5)	MB Aldrin	0.000	5.371f	0	187610	N.D.	0.061 #
7)	B delta-BHC	0.000	4.955	0	2352675	N.D.	0.709 #
8)	B Heptachlo...	0.000	5.769	0	49913	N.D.	0.018 #
19)	B Endosulfa...	0.000	7.163	0	405414	N.D.	0.186 #
21)	B Endrin ke...	0.000	7.677f	0	740454	N.D.	0.311 #
23)	Chlordane-1	4.236	4.955	11353389	2352675	32.790	20.302 #
24)	Chlordane-2	0.000	5.371	0	187610	N.D.	1.567 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
Data File : PL039065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 14:19
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:08:44 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

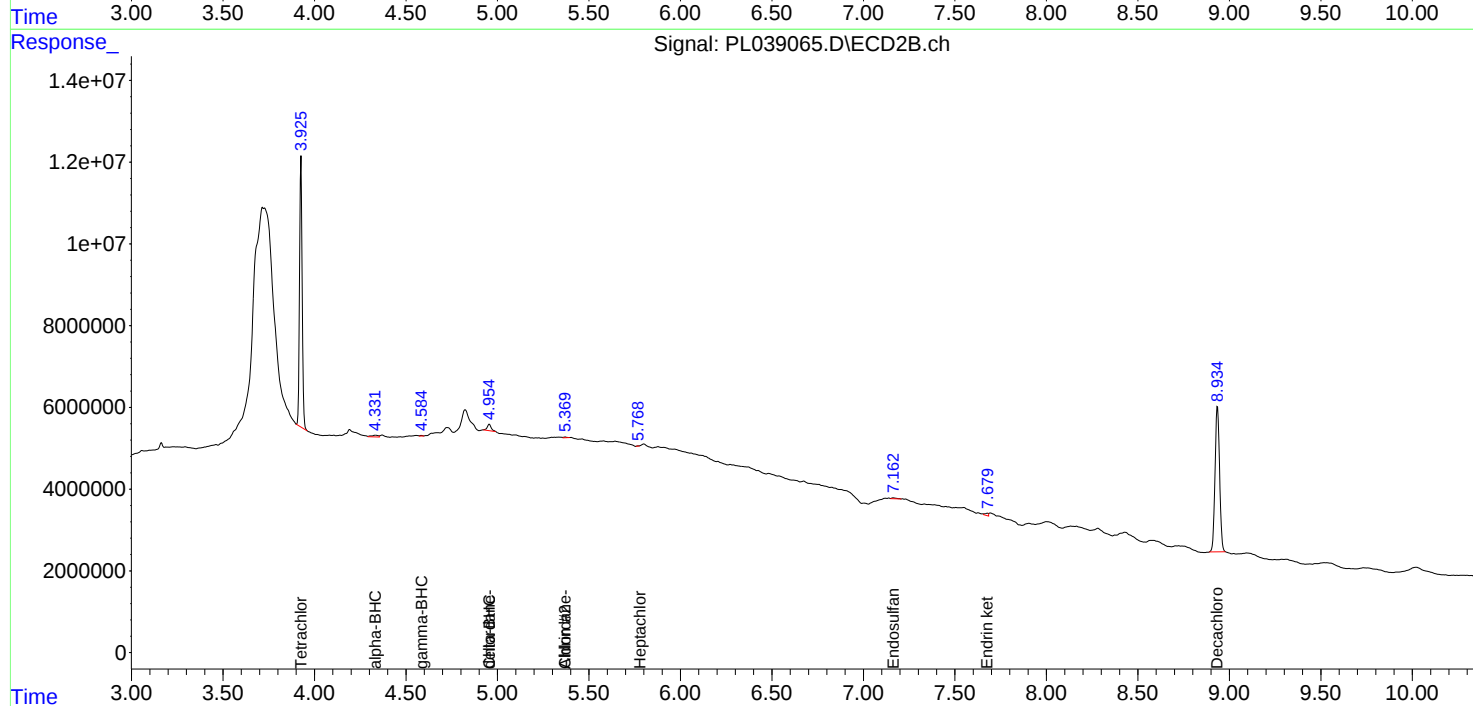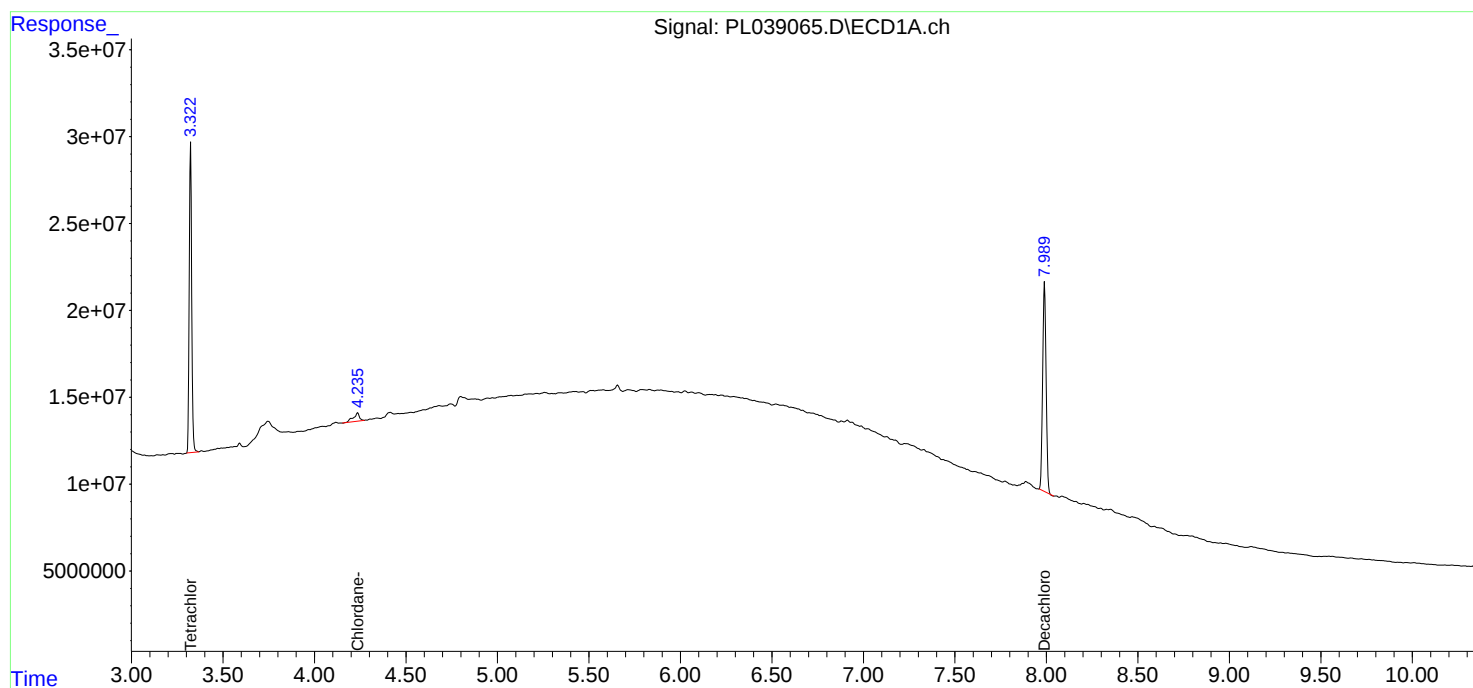


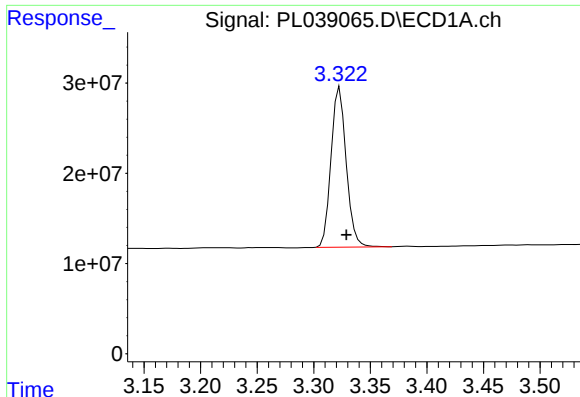

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 166023895
Conc: 22.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

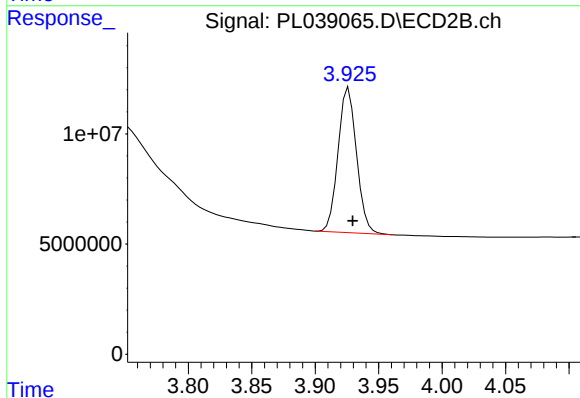


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.003 min
Response: 66571614
Conc: 25.36 ng/ml

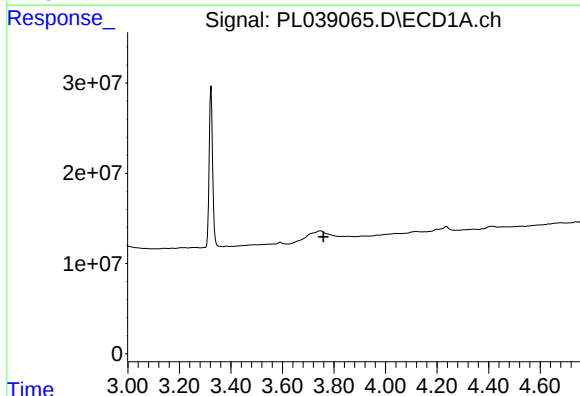


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

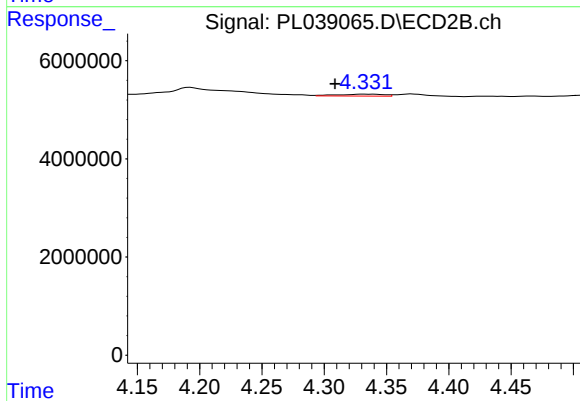

#2 alpha-BHC


R.T.: 4.332 min
Delta R.T.: 0.024 min
Response: 1010256
Conc: 0.26 ng/ml

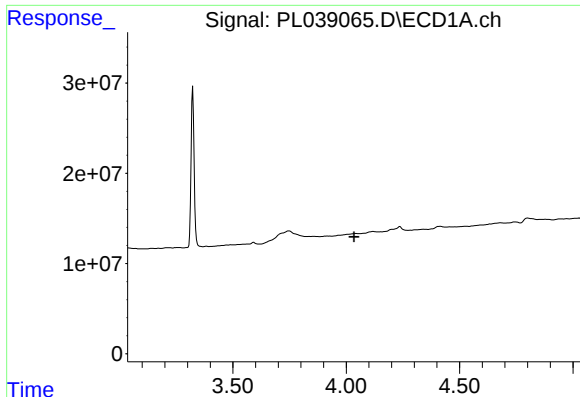

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

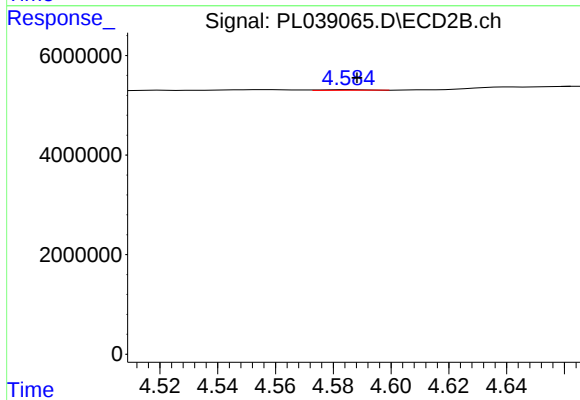


#3 gamma-BHC (Lindane)

R.T.: 4.585 min
Delta R.T.: -0.003 min
Response: 152700
Conc: 0.04 ng/ml

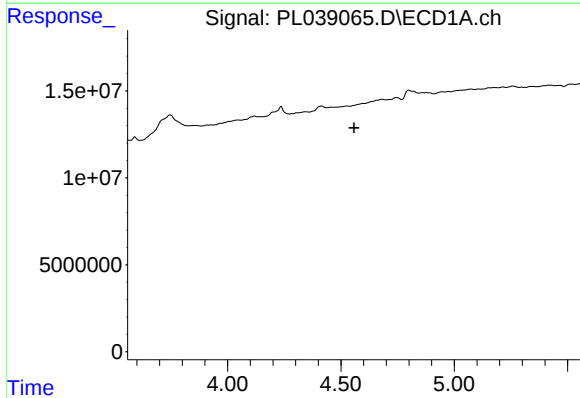


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

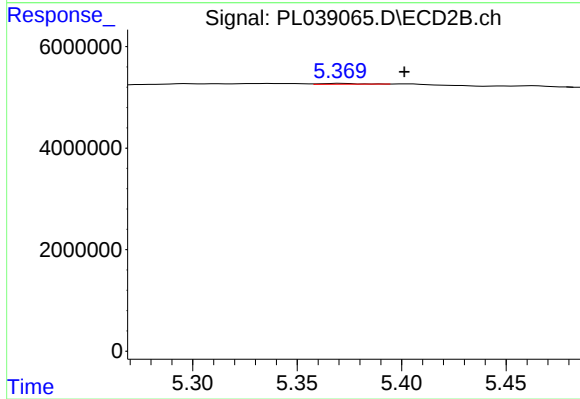

#5 Aldrin


R.T.: 5.371 min
Delta R.T.: -0.031 min
Response: 187610
Conc: 0.06 ng/ml

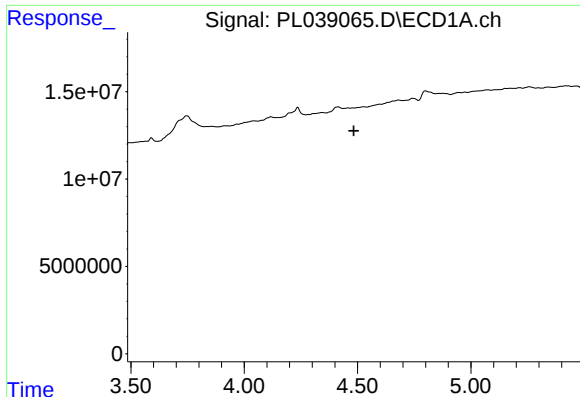

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

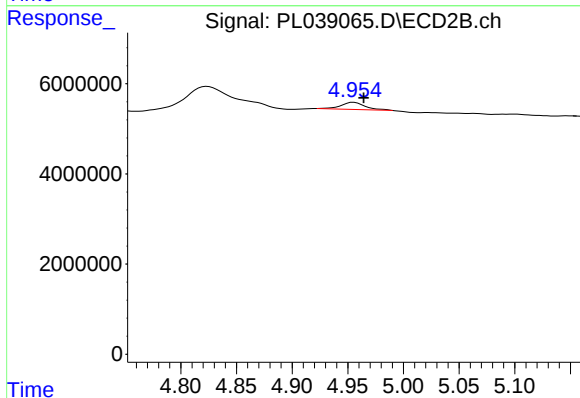


#7 delta-BHC

R.T.: 4.955 min
Delta R.T.: -0.009 min
Response: 2352675
Conc: 0.71 ng/ml

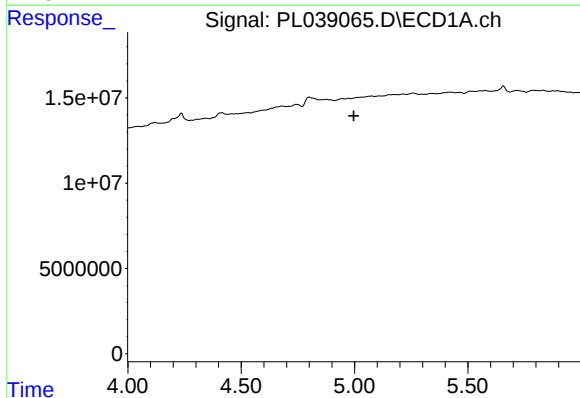


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

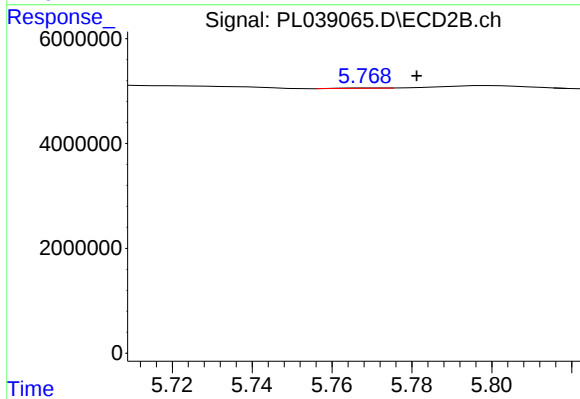

#8 Heptachlor epoxide


R.T.: 5.769 min
Delta R.T.: -0.012 min
Response: 49913
Conc: 0.02 ng/ml

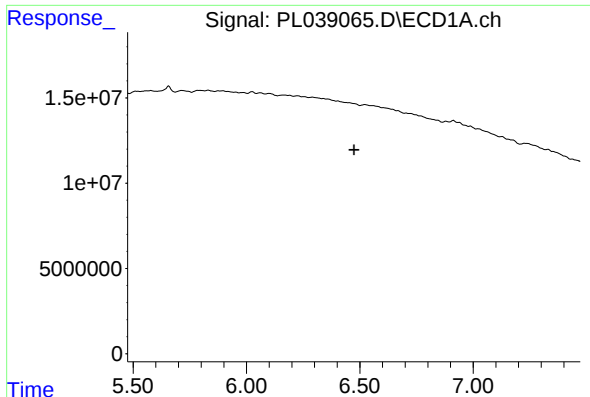

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

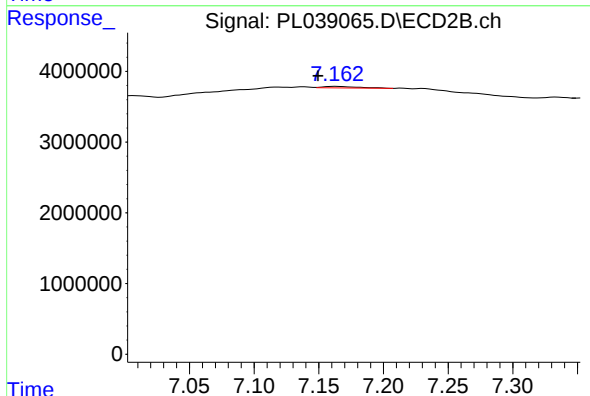


#19 Endosulfan Sulfate

R.T.: 7.163 min
Delta R.T.: 0.014 min
Response: 405414
Conc: 0.19 ng/ml

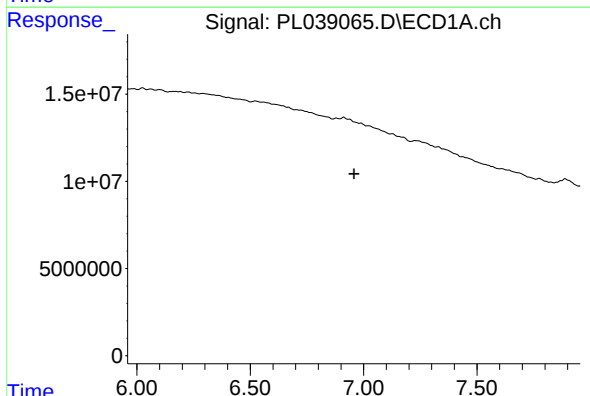


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.958 min
Response: 0
Conc: N.D.

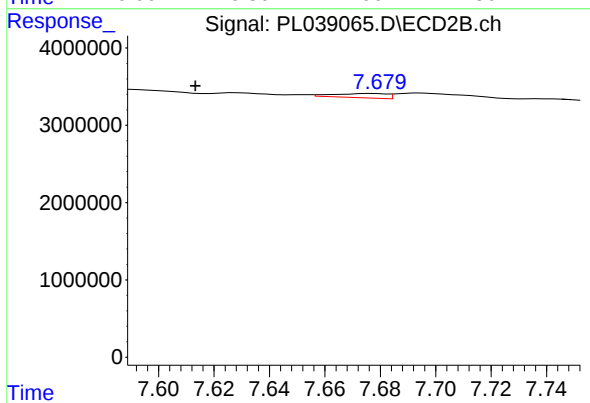

#21 Endrin ketone


R.T.: 7.677 min
Delta R.T.: 0.064 min
Response: 740454
Conc: 0.31 ng/ml

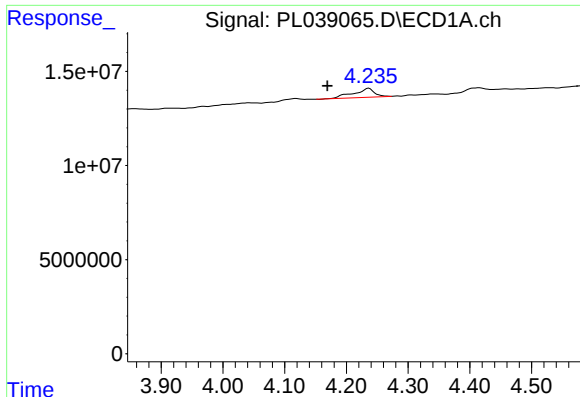

#23 Chlordane-1


R.T.: 4.236 min
Delta R.T.: 0.067 min
Response: 11353389
Conc: 32.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

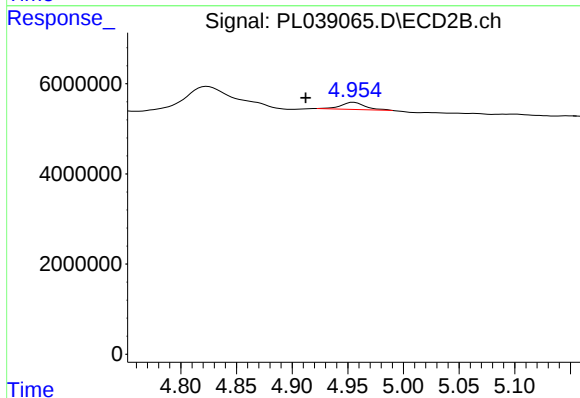


#23 Chlordane-1

R.T.: 4.955 min
Delta R.T.: 0.043 min
Response: 2352675
Conc: 20.30 ng/ml

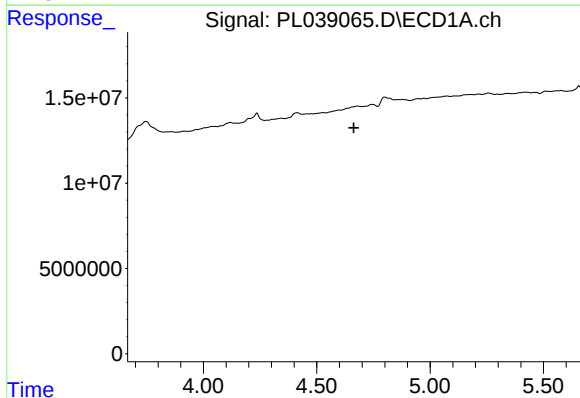


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.663 min
Response: 0
Conc: N.D.

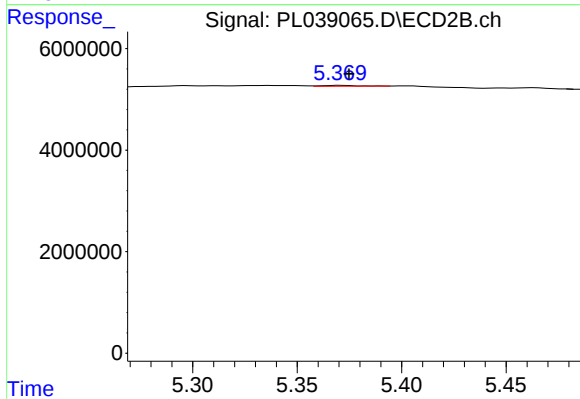

#24 Chlordane-2


R.T.: 5.371 min
Delta R.T.: -0.004 min
Response: 187610
Conc: 1.57 ng/ml

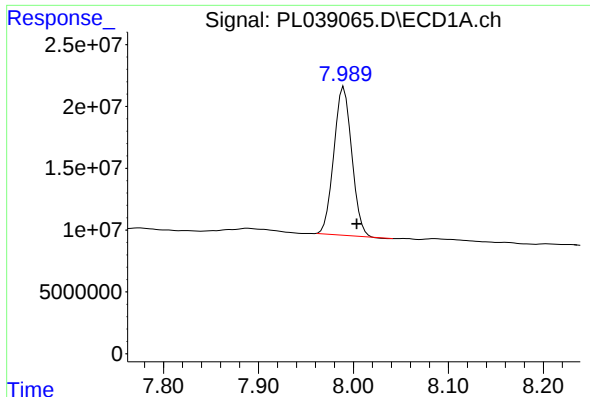

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 157626841
Conc: 20.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

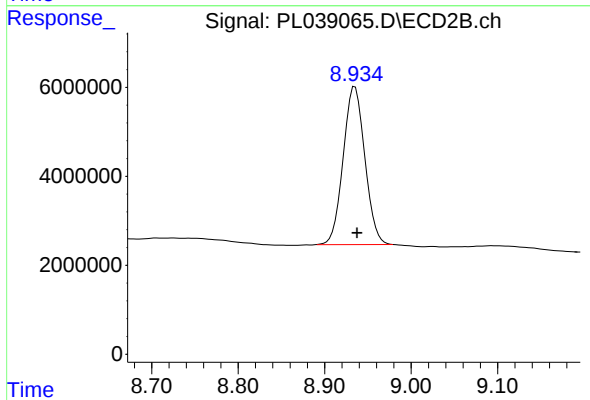

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 61523999
Conc: 25.17 ng/ml