

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
 Data File : PL039089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2018 21:16
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 01:18:18 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	159.2E6	65788259	21.383	25.063
28)	SA Decachlor...	7.990	8.935	134.6E6	58535939	17.750	23.947 #
Target Compounds							
2)	A alpha-BHC	0.000	4.335f	0	280724	N.D.	0.073 #
3)	MA gamma-BHC...	0.000	4.548f	0	716917	N.D.	0.198 #
4)	MA Heptachlor	0.000	5.096	0	560078	N.D.	0.175 #
7)	B delta-BHC	0.000	4.956	0	2471033	N.D.	0.745 #
8)	B Heptachlo...	0.000	5.803	0	189693	N.D.	0.067 #
23)	Chlordane-1	4.236	4.916	17429942	-3953	50.339	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080918\
Data File : PL039089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2018 21:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 01:18:18 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

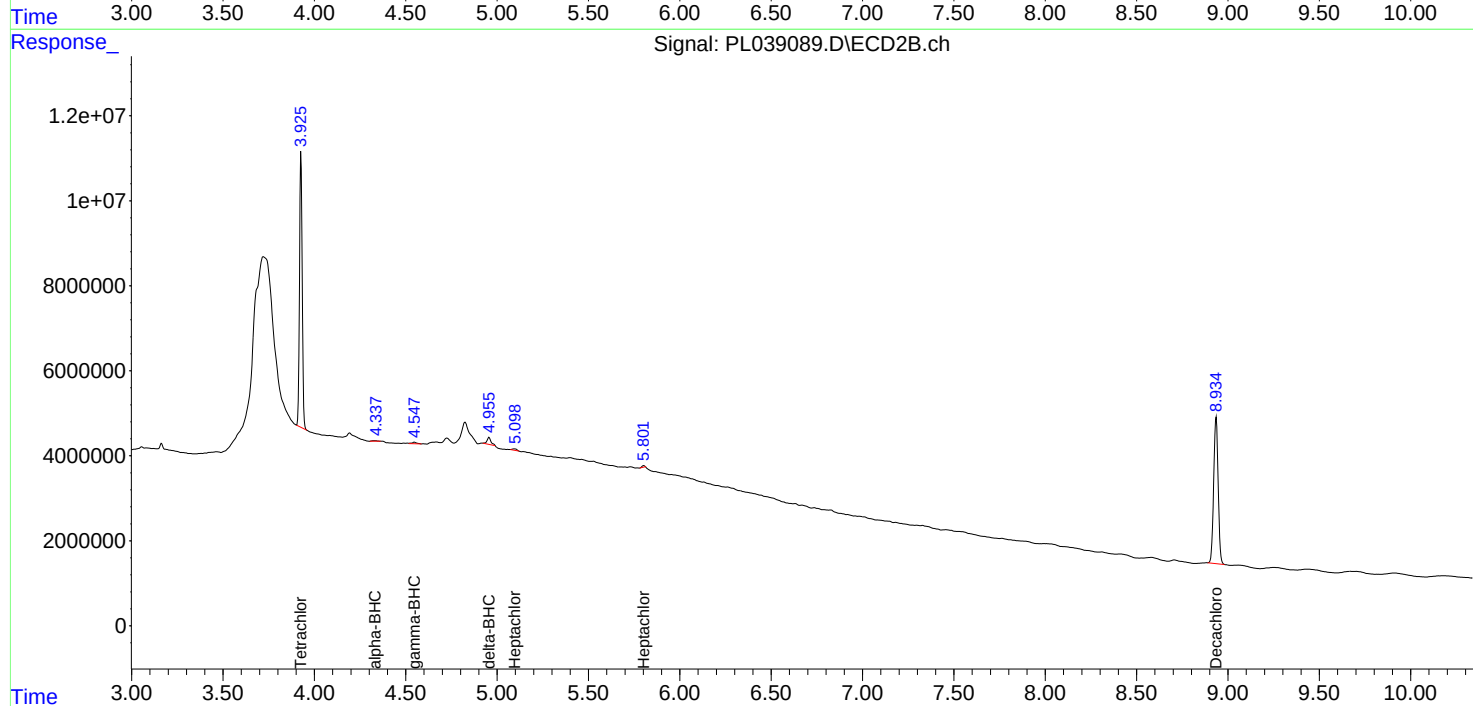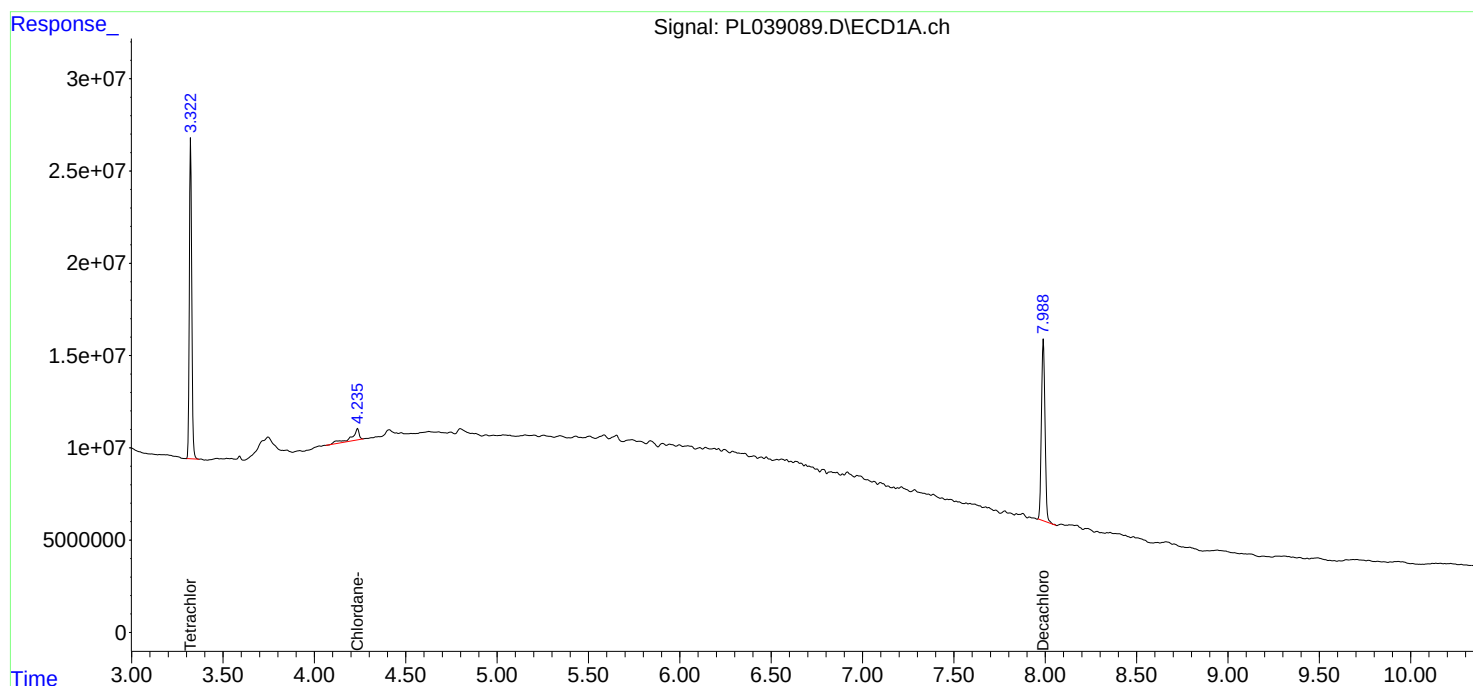


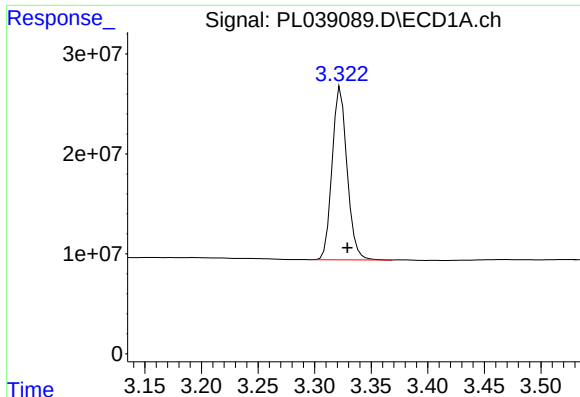

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: -0.006 min
Response: 159228474
Conc: 21.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

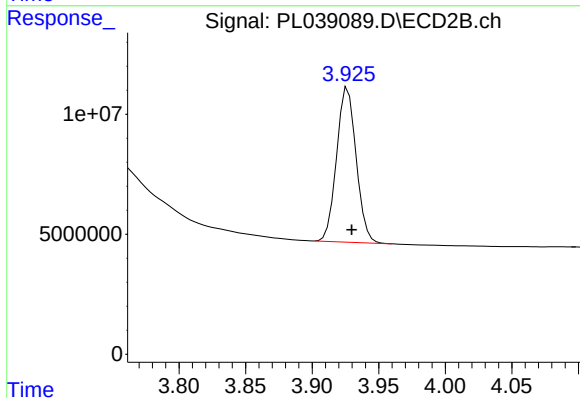


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 65788259
Conc: 25.06 ng/ml

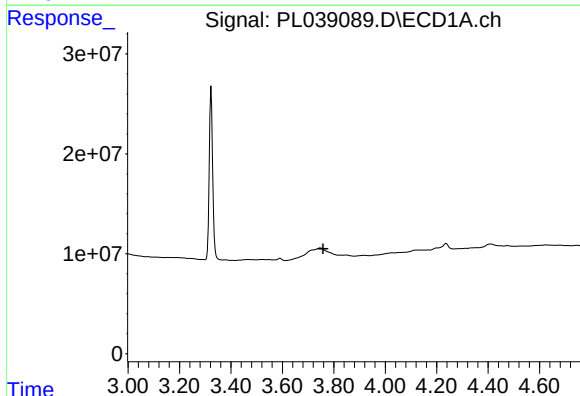


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

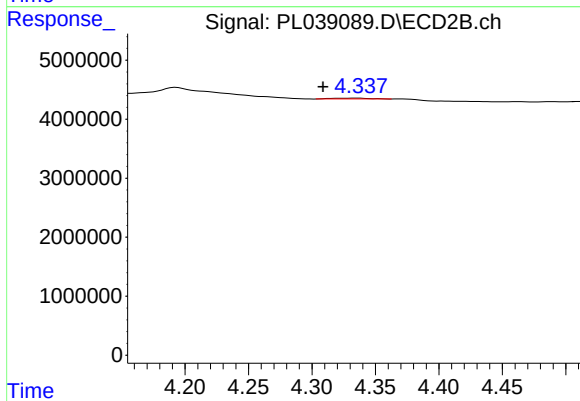

#2 alpha-BHC


R.T.: 4.335 min
Delta R.T.: 0.026 min
Response: 280724
Conc: 0.07 ng/ml

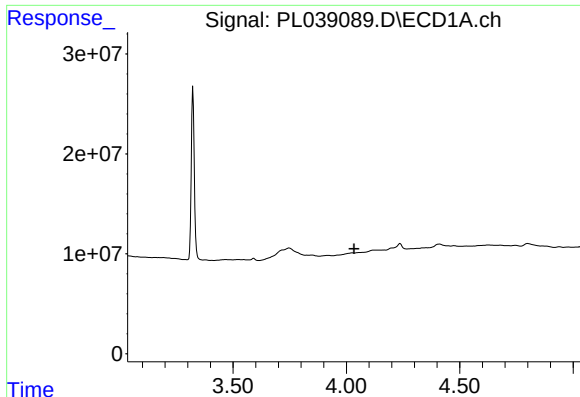

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

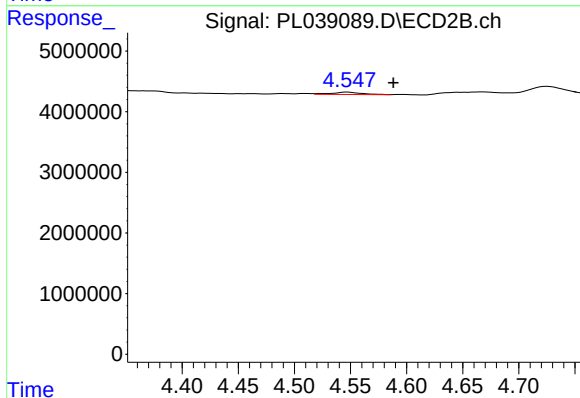


#3 gamma-BHC (Lindane)

R.T.: 4.548 min
Delta R.T.: -0.041 min
Response: 716917
Conc: 0.20 ng/ml

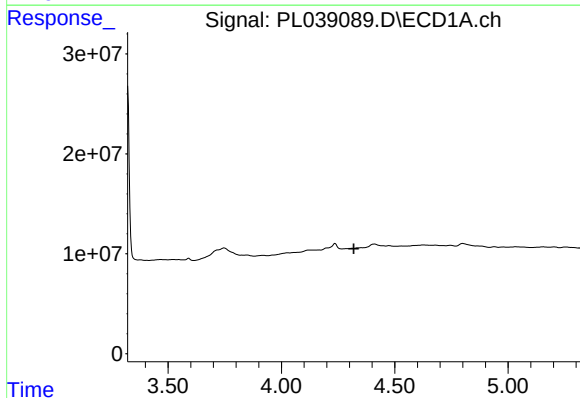


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

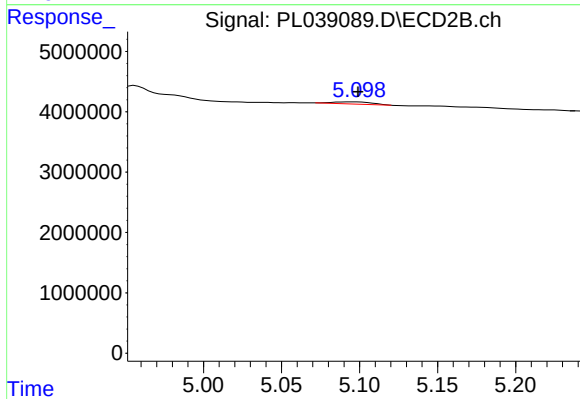

#4 Heptachlor


R.T.: 5.096 min
Delta R.T.: -0.003 min
Response: 560078
Conc: 0.18 ng/ml

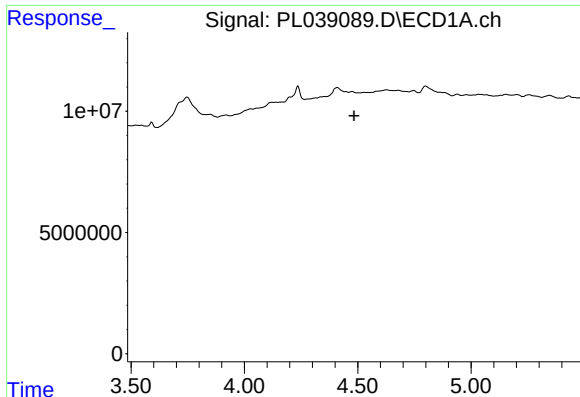

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

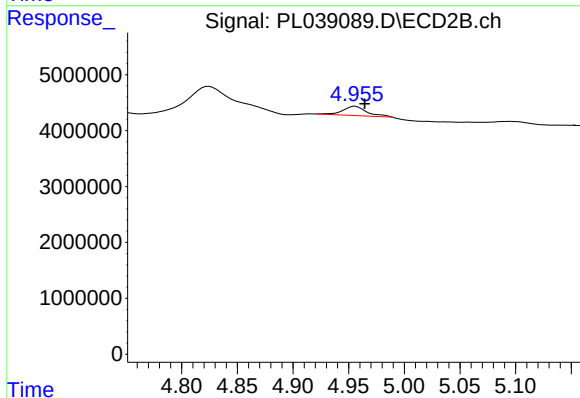


#7 delta-BHC

R.T.: 4.956 min
Delta R.T.: -0.008 min
Response: 2471033
Conc: 0.75 ng/ml

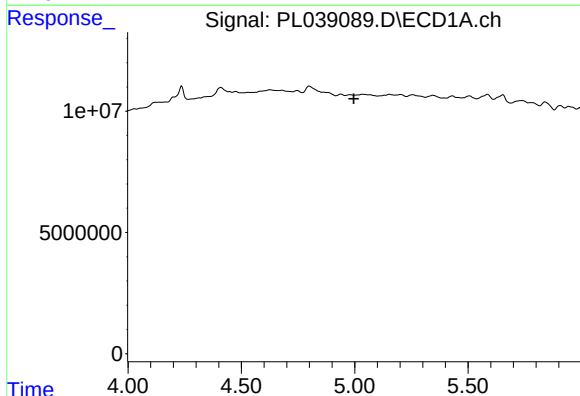


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.997 min
Response: 0
Conc: N.D.

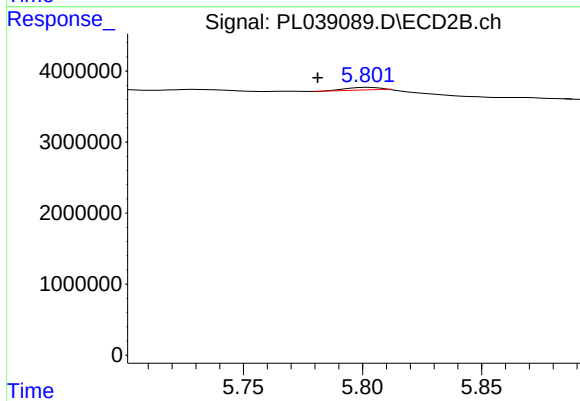

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: 0.021 min
Response: 189693
Conc: 0.07 ng/ml

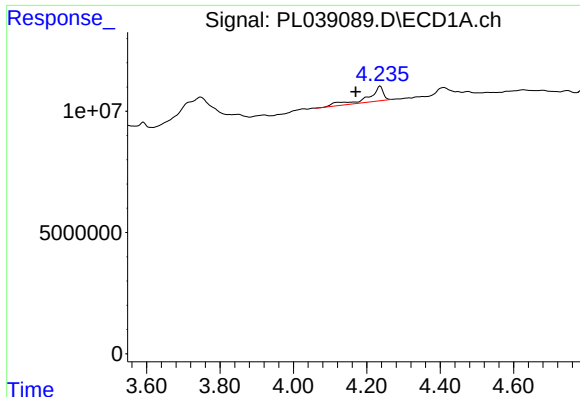

#23 Chlordane-1


R.T.: 4.236 min
Delta R.T.: 0.067 min
Response: 17429942
Conc: 50.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

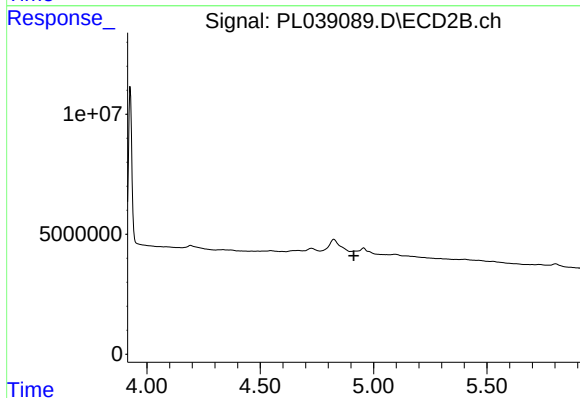


#23 Chlordane-1

R.T.: 4.916 min
Delta R.T.: 0.004 min
Response: -3953
Conc: N.D.

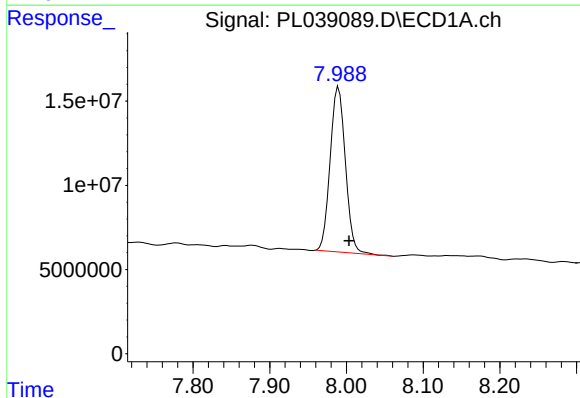

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.014 min
Response: 134648520
Conc: 17.75 ng/ml

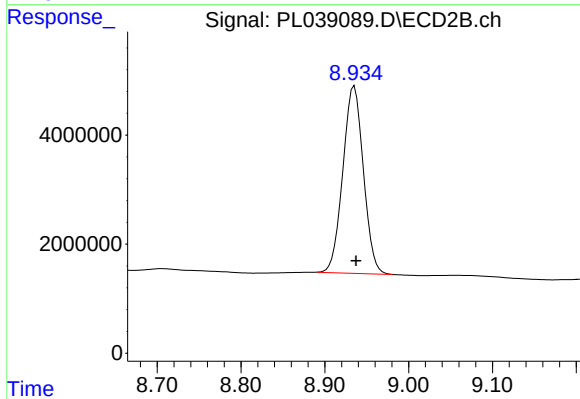

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: -0.002 min
Response: 58535939
Conc: 23.95 ng/ml