

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 11:56
 Operator : SM\AJ
 Sample : PB122080TB
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122080TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:26:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.928	251.2E6	65544399	24.998	22.972
28)	SA Decachlor...	7.978	8.958	225.9E6	64251166	22.308	22.720
Target Compounds							
6)	B beta-BHC	0.000	4.802f	0	5269025	N.D.	3.048 #
8)	B Heptachlo...	0.000	5.804	0	3670389	N.D.	0.960 #
11)	B alpha-Chl...	5.263	0.000	17517058	0	1.148	N.D. #
26)	Chlordane-4	5.263	0.000	17517058	0	13.281	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 11:56
Operator : SM\AJ
Sample : PB122080TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB122080TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:26:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

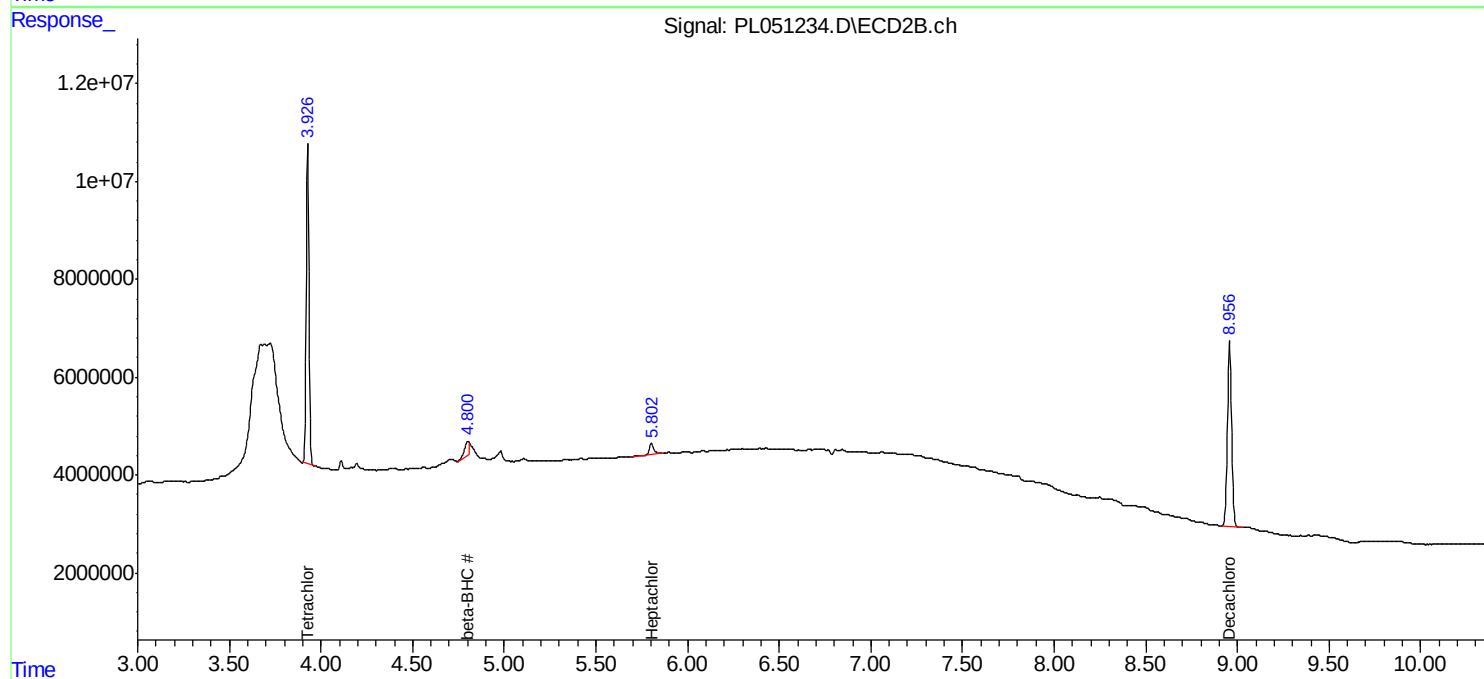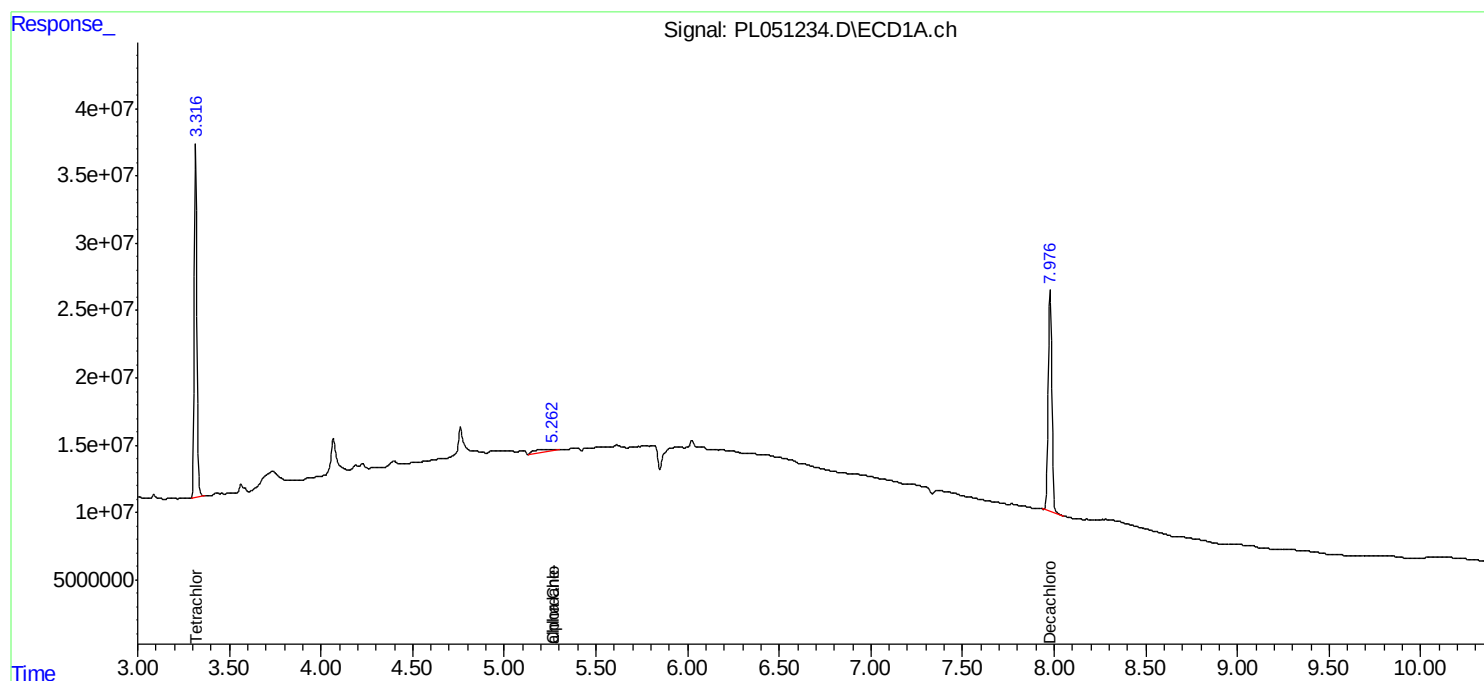


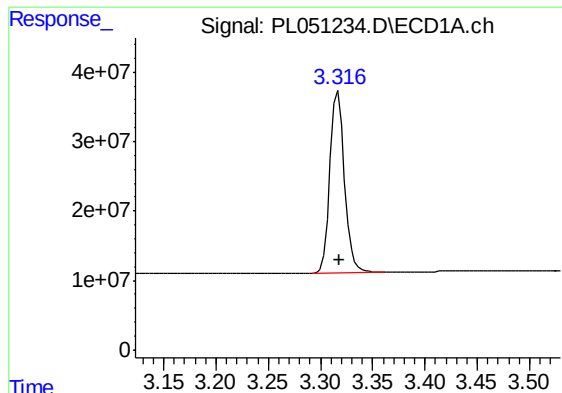

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.001 min
Response: 251178348
Conc: 25.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122080TB

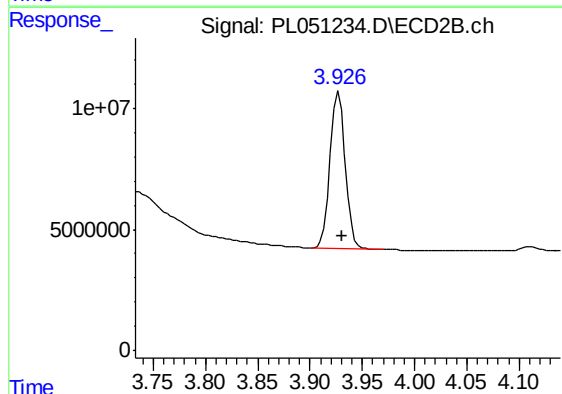


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 65544399
Conc: 22.97 ng/ml

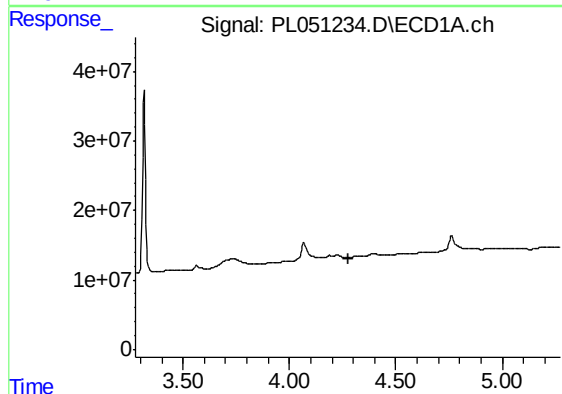


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

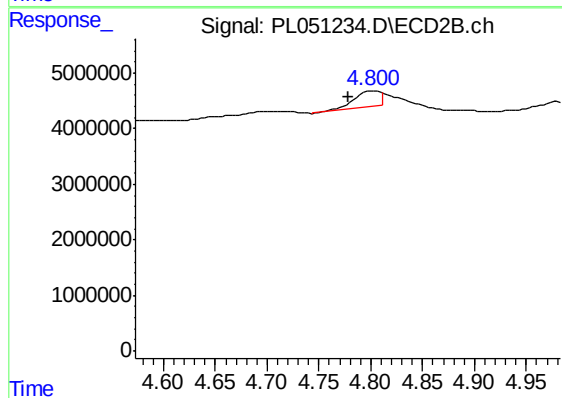

#6 beta-BHC


R.T.: 4.802 min
Delta R.T.: 0.024 min
Response: 5269025
Conc: 3.05 ng/ml

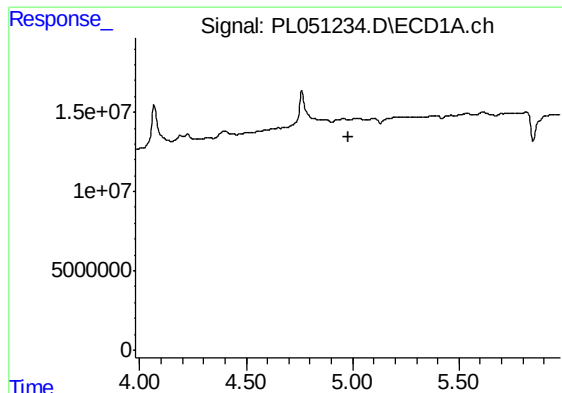

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122080TB

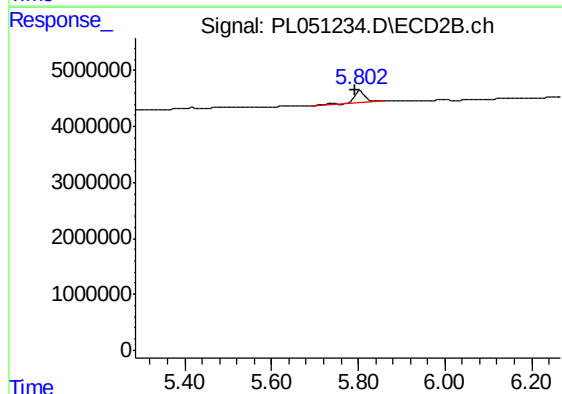


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.011 min
Response: 3670389
Conc: 0.96 ng/ml

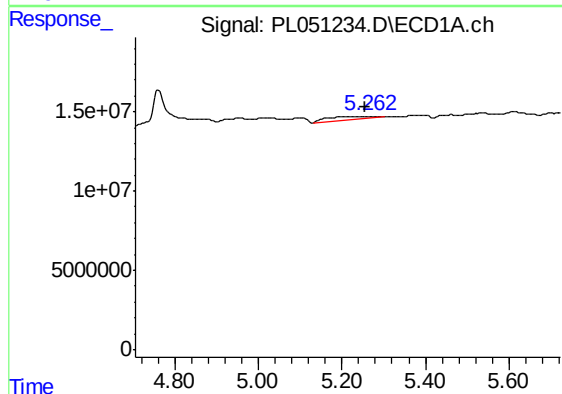


#11 alpha-Chlordane

R.T.: 5.263 min
Delta R.T.: 0.006 min
Response: 17517058
Conc: 1.15 ng/ml

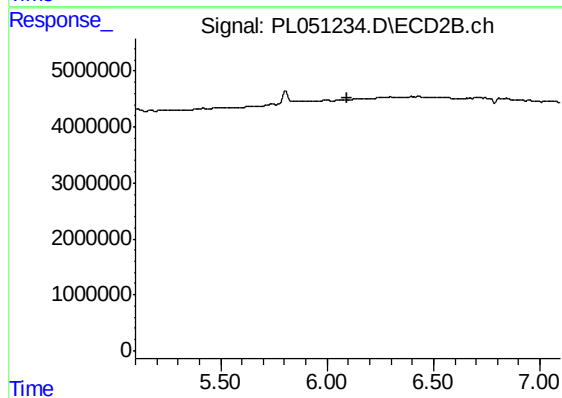

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

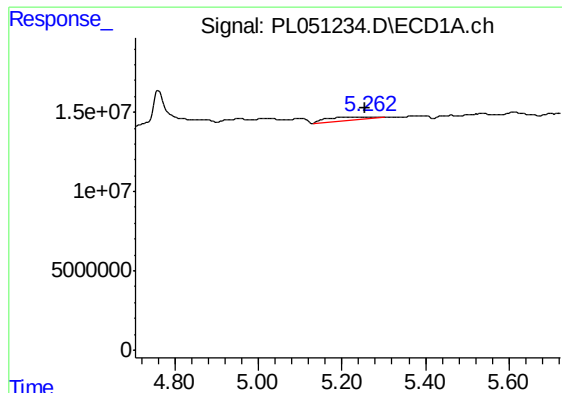

#26 Chlordane-4


R.T.: 5.263 min
Delta R.T.: 0.007 min
Response: 17517058
Conc: 13.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122080TB

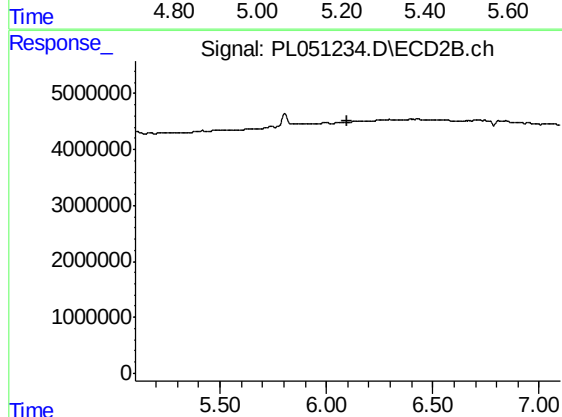


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

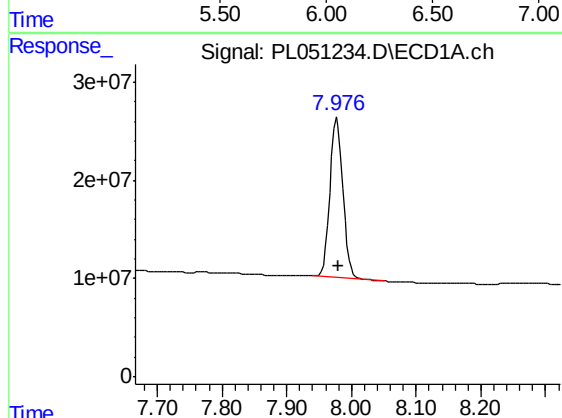

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 225880368
Conc: 22.31 ng/ml

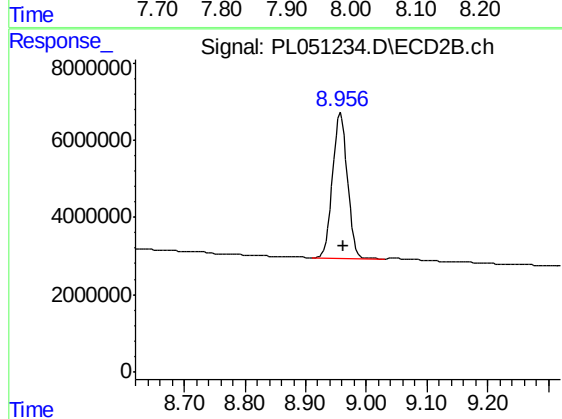

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 64251166
Conc: 22.72 ng/ml