

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 12:11
 Operator : SM\AJ
 Sample : K3613-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-080719-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:27:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.928	232.2E6	62974936	23.109	22.072
28)	SA Decachlor...	7.979	8.957	164.4E6	46213339	16.233	16.342
Target Compounds							
5)	MB Aldrin	4.531	0.000	37511681	0	2.421	N.D. #
6)	B beta-BHC	0.000	4.806f	0	3732152	N.D.	2.159 #
8)	B Heptachlo...	0.000	5.804	0	6761293	N.D.	1.768 #
9)	A Endosulfan I	5.325f	0.000	5832951	0	0.401	N.D. #
10)	B gamma-Chl...	5.196	0.000	30859105	0	1.955	N.D. #
11)	B alpha-Chl...	5.246	0.000	17335909	0	1.136	N.D. #
25)	Chlordane-3	5.196	0.000	30859105	0	22.046	N.D. #
26)	Chlordane-4	5.246	0.000	17335909	0	13.143	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 12:11
Operator : SM\AJ
Sample : K3613-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:27:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

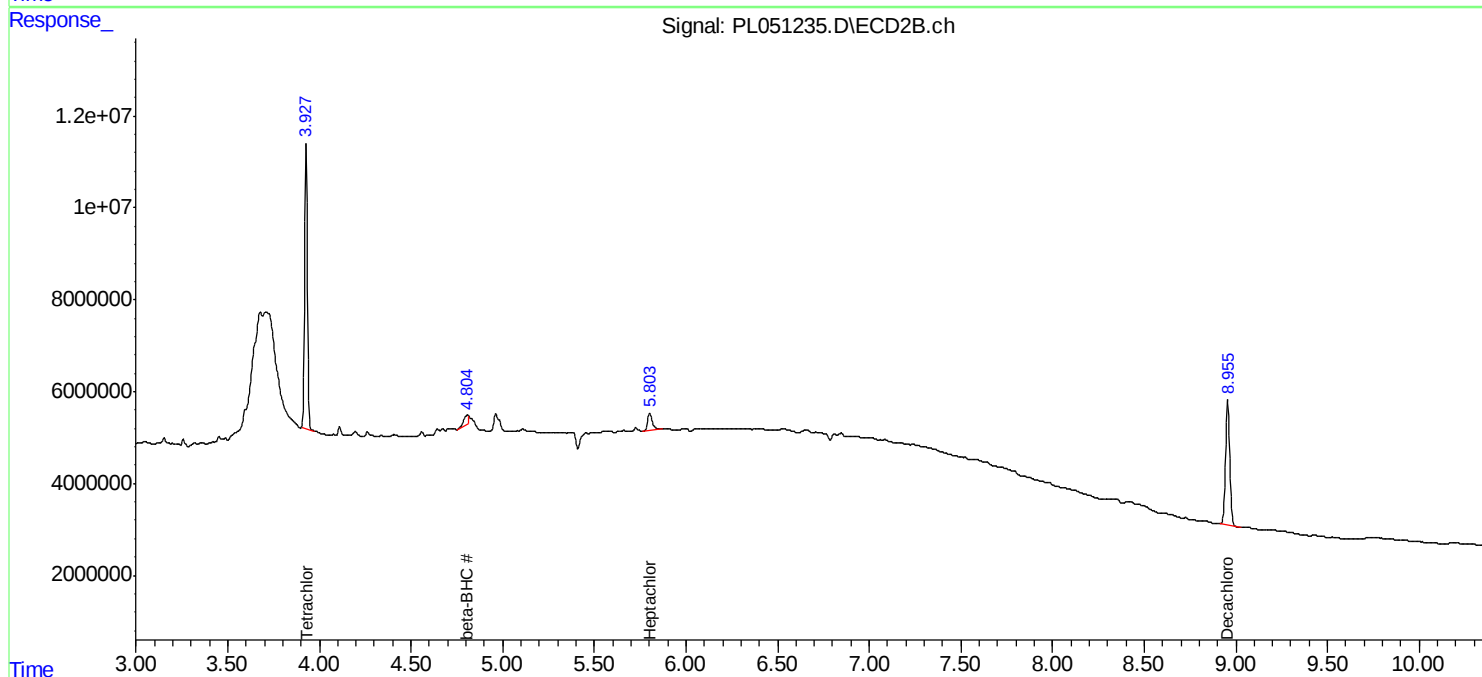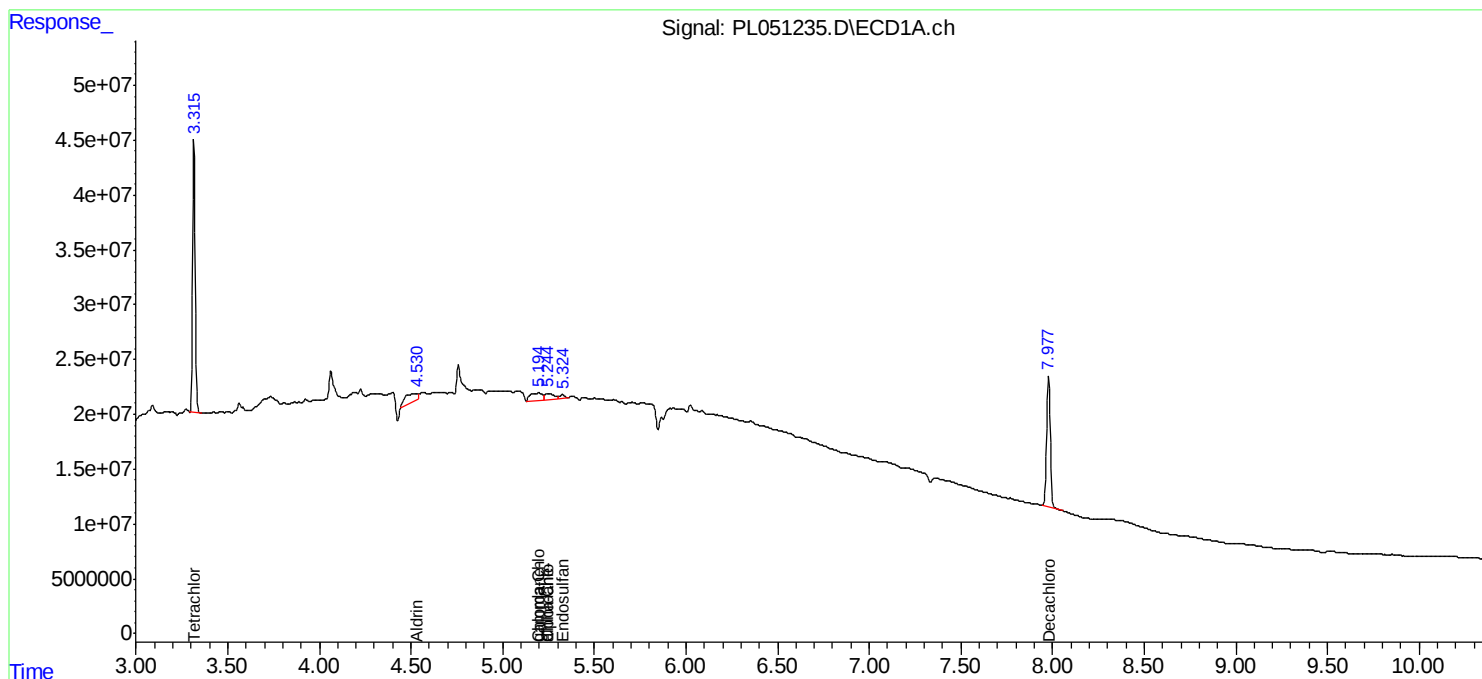


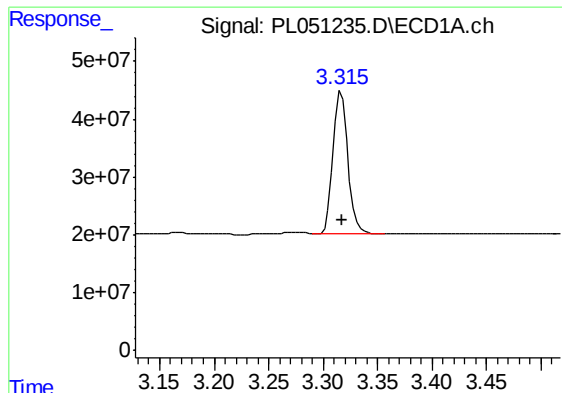

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.001 min
Response: 232197236
Conc: 23.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

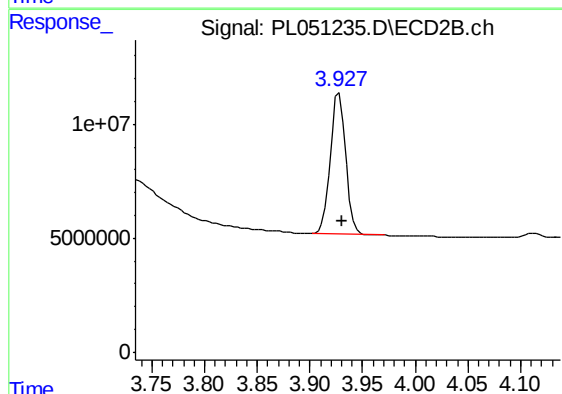


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 62974936
Conc: 22.07 ng/ml

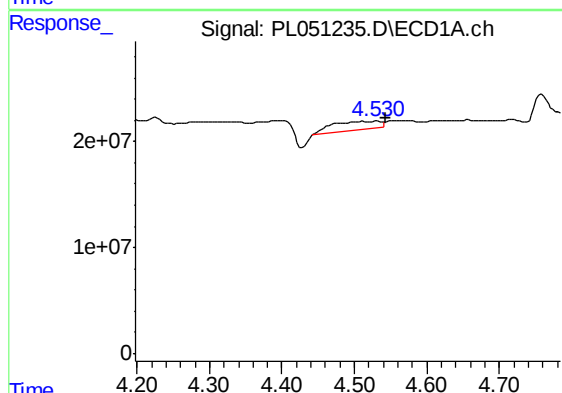


#5 Aldrin

R.T.: 4.531 min
Delta R.T.: -0.012 min
Response: 37511681
Conc: 2.42 ng/ml

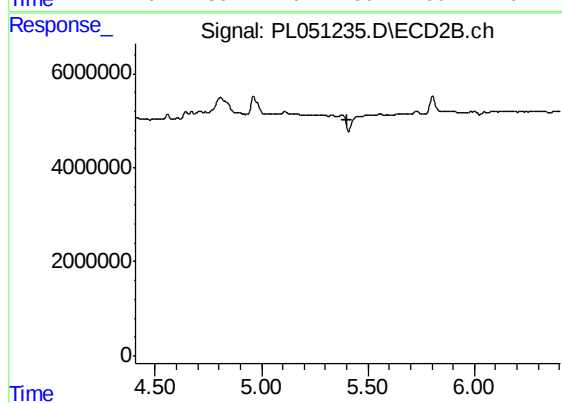

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

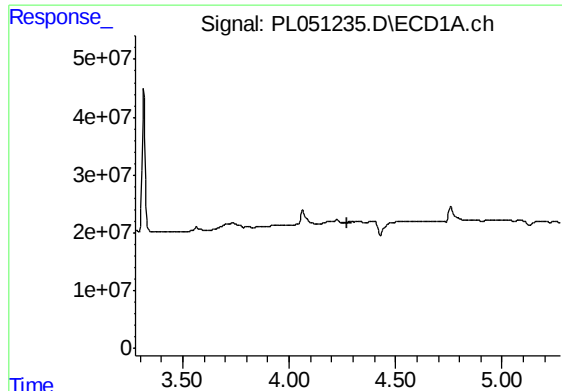

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

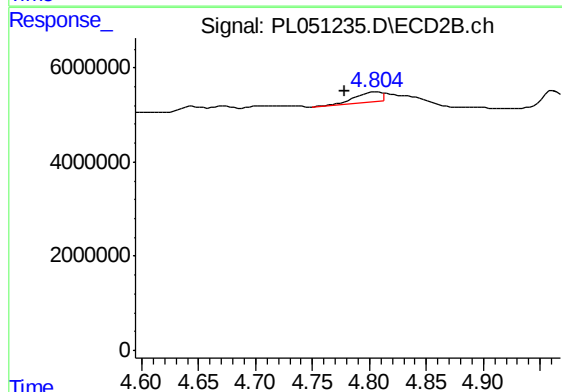


#6 beta-BHC

R.T.: 4.806 min
Delta R.T.: 0.028 min
Response: 3732152
Conc: 2.16 ng/ml

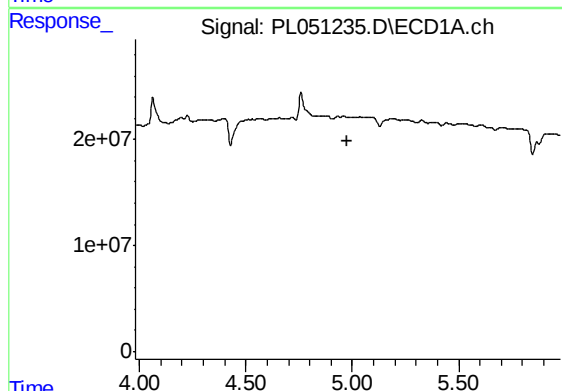


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

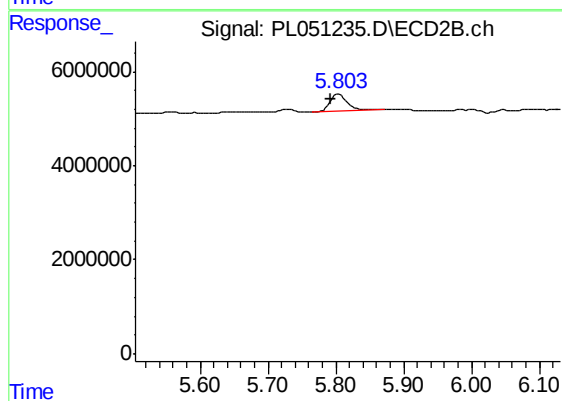

#8 Heptachlor epoxide


R.T.: 5.804 min
Delta R.T.: 0.011 min
Response: 6761293
Conc: 1.77 ng/ml

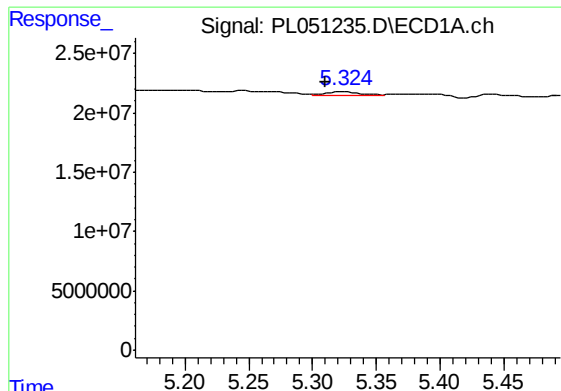

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.015 min
Response: 5832951
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

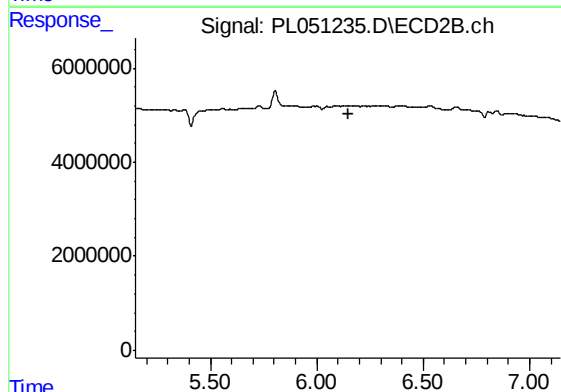


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

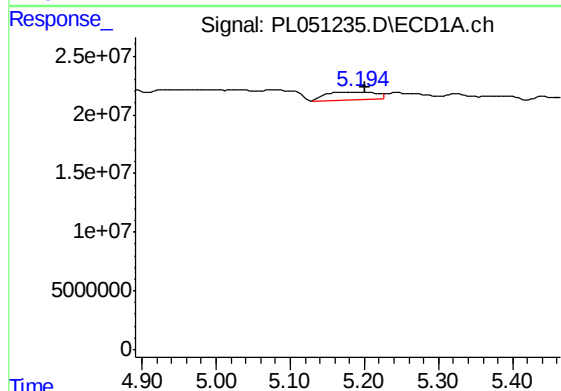


#10 gamma-Chlordane

R.T.: 5.196 min
Delta R.T.: -0.005 min
Response: 30859105
Conc: 1.96 ng/ml

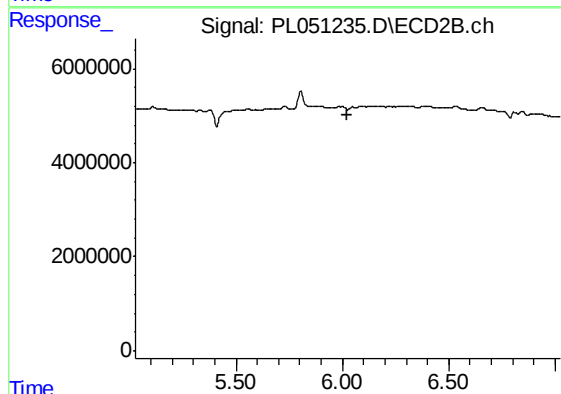

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

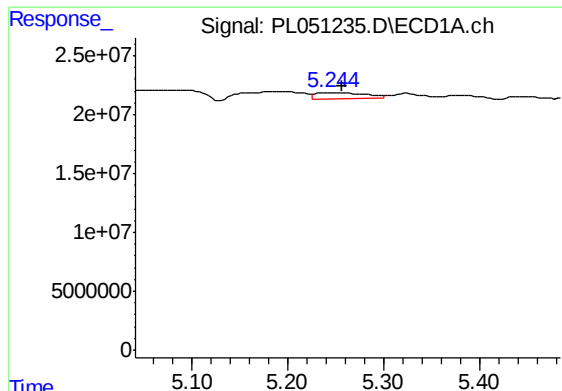

#11 alpha-Chlordane


R.T.: 5.246 min
Delta R.T.: -0.011 min
Response: 17335909
Conc: 1.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

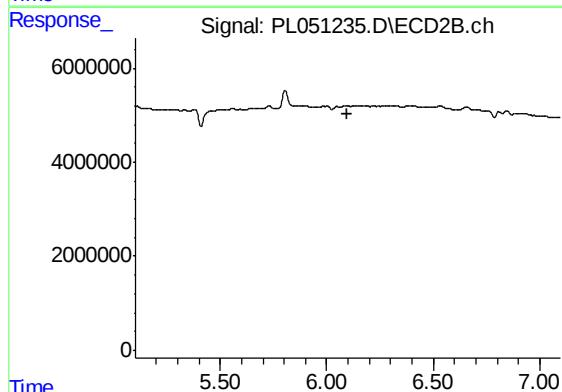


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

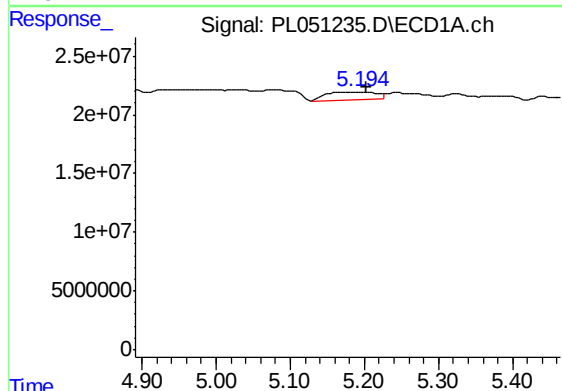


#25 Chlordane-3

R.T.: 5.196 min
Delta R.T.: -0.006 min
Response: 30859105
Conc: 22.05 ng/ml

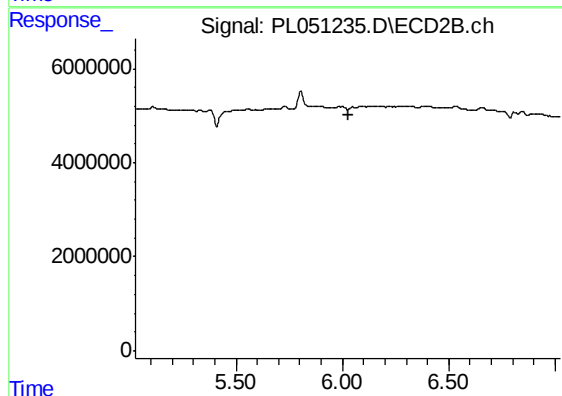

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

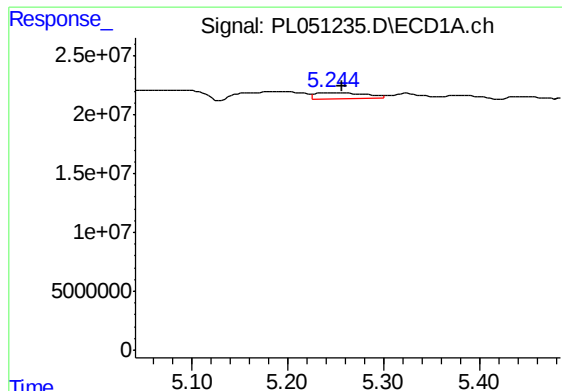

#26 Chlordane-4


R.T.: 5.246 min
Delta R.T.: -0.011 min
Response: 17335909
Conc: 13.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-A

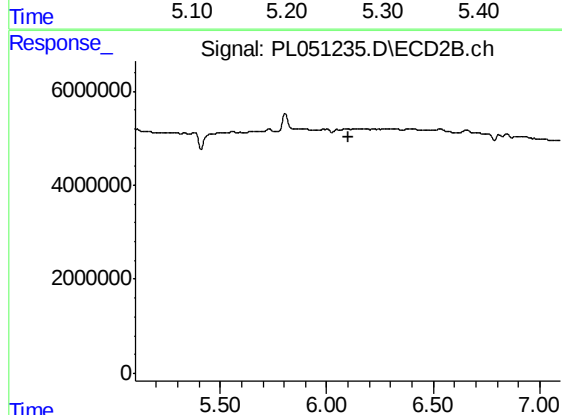


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

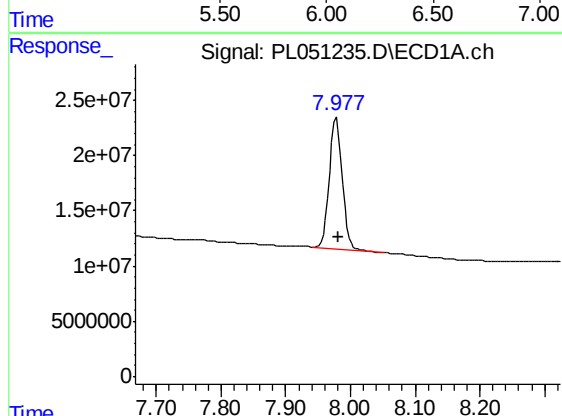

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 164365149
Conc: 16.23 ng/ml

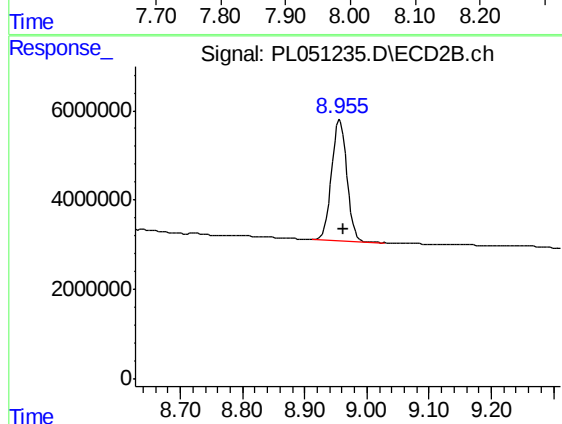

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 46213339
Conc: 16.34 ng/ml