

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 12:55
 Operator : SM\AJ
 Sample : K4092-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-080719-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:27:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	208.7E6	58197623	20.767	20.397
28)	SA Decachlor...	7.979	8.958	196.9E6	56072963	19.443	19.828
Target Compounds							
5)	MB Aldrin	4.513f	0.000	50801872	0	3.279	N.D. #
8)	B Heptachlo...	0.000	5.804	0	5386822	N.D.	1.408 #
9)	A Endosulfan I	5.327f	0.000	13290251	0	0.914	N.D. #
10)	B gamma-Chl...	5.196	0.000	46910419	0	2.972	N.D. #
11)	B alpha-Chl...	5.263	0.000	19332301	0	1.267	N.D. #
13)	MA Dieldrin	5.536	0.000	12560033	0	0.810	N.D. #
25)	Chlordane-3	5.196	0.000	46910419	0	33.513	N.D. #
26)	Chlordane-4	5.263	0.000	19332301	0	14.657	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 12:55
Operator : SM\AJ
Sample : K4092-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
EO-01-080719-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:27:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

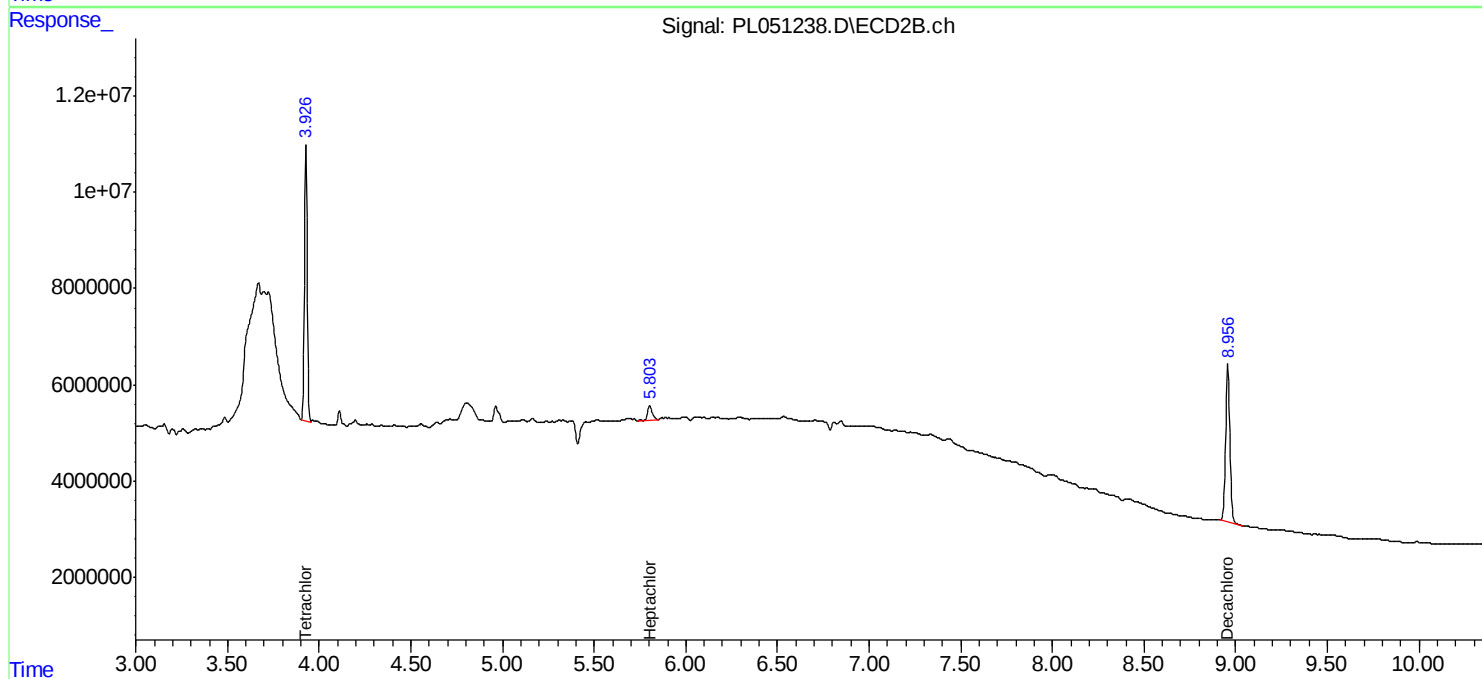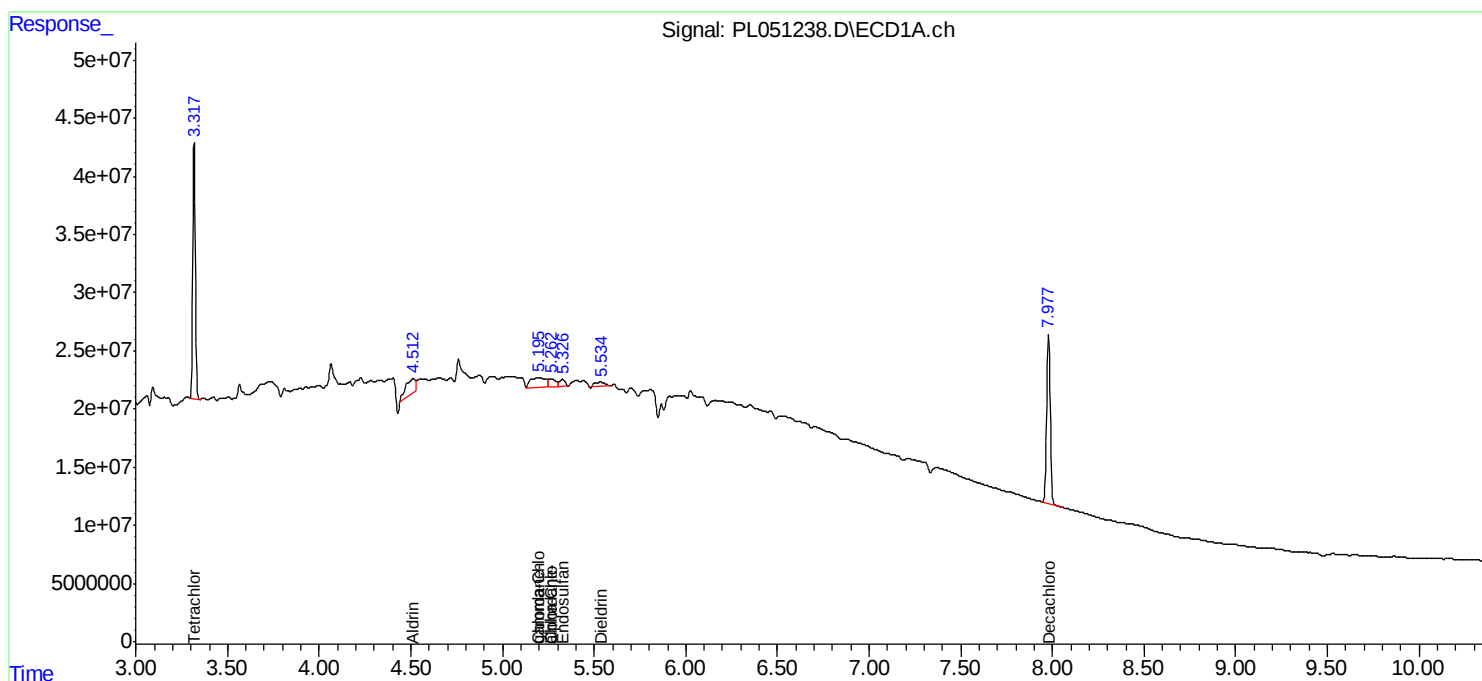


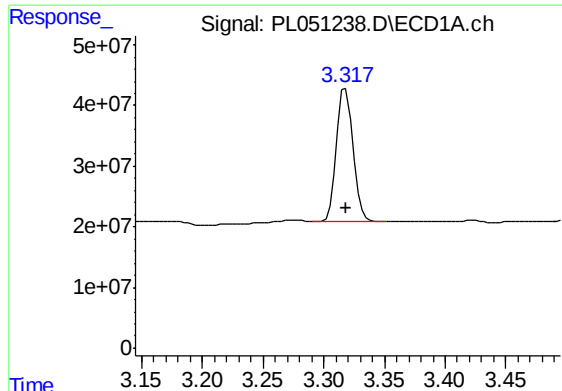

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 208659363
Conc: 20.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-080719-A

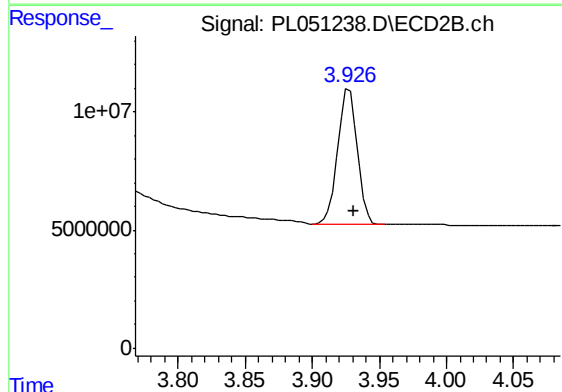


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 58197623
Conc: 20.40 ng/ml

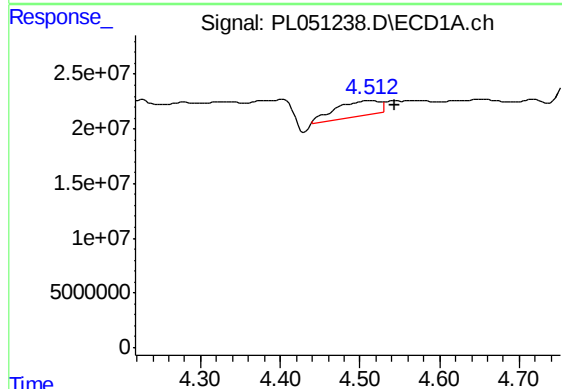


#5 Aldrin

R.T.: 4.513 min
Delta R.T.: -0.030 min
Response: 50801872
Conc: 3.28 ng/ml

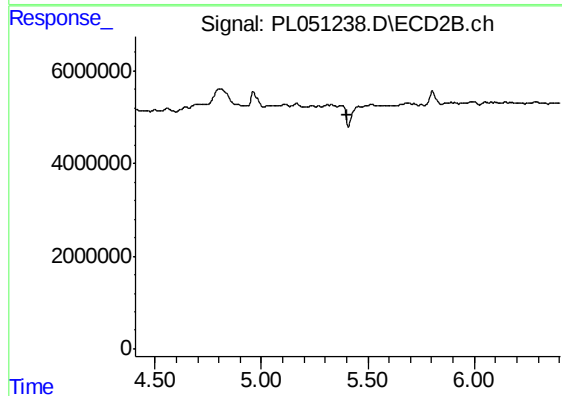

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

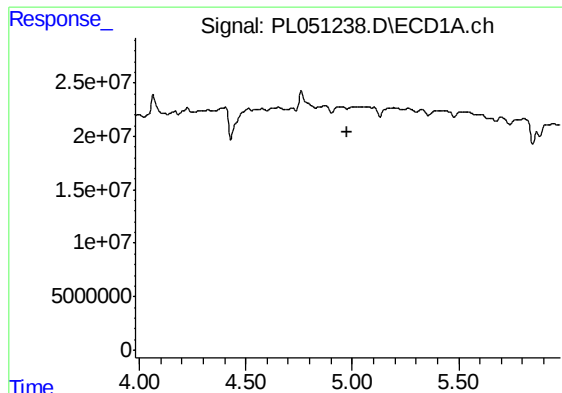

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-01-080719-A

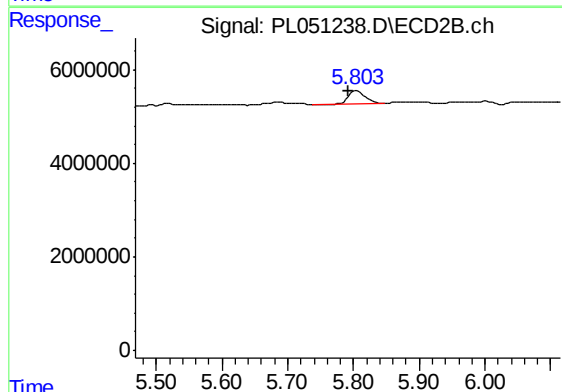


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.012 min
Response: 5386822
Conc: 1.41 ng/ml

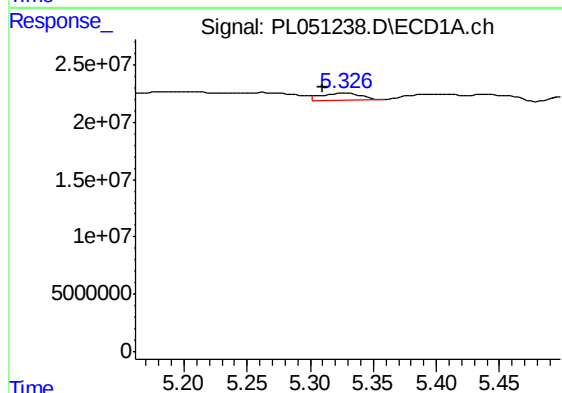


#9 Endosulfan I

R.T.: 5.327 min
Delta R.T.: 0.017 min
Response: 13290251
Conc: 0.91 ng/ml

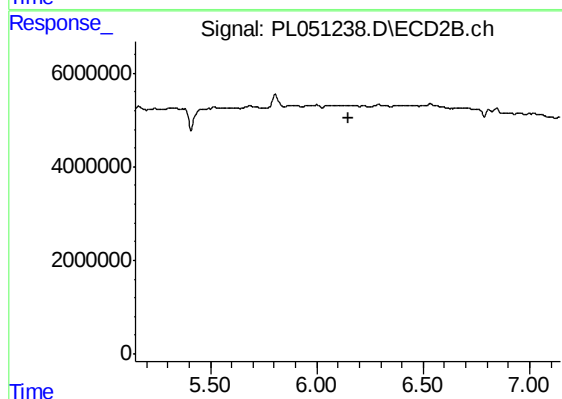

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

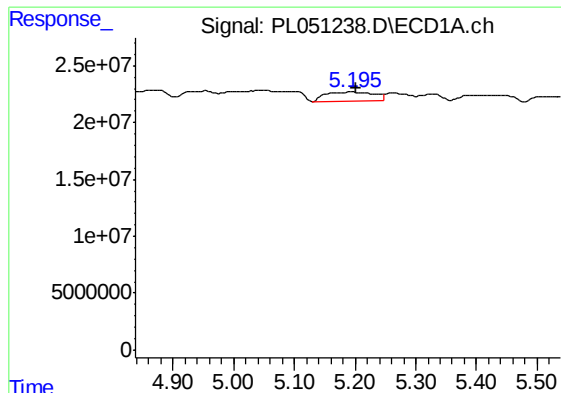

#10 gamma-Chlordane


R.T.: 5.196 min
Delta R.T.: -0.005 min
Response: 46910419
Conc: 2.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-080719-A

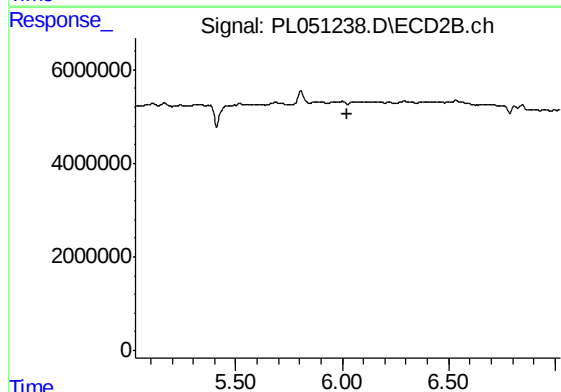


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

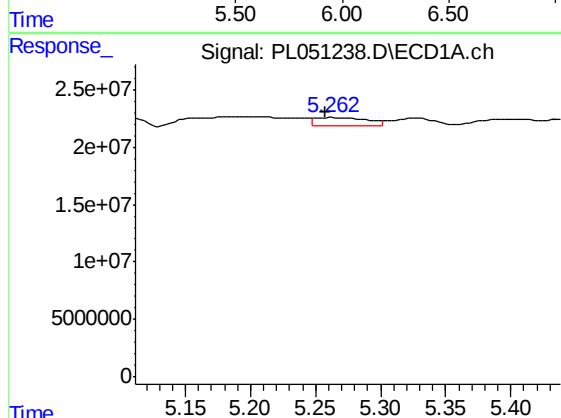


#11 alpha-Chlordane

R.T.: 5.263 min
Delta R.T.: 0.006 min
Response: 19332301
Conc: 1.27 ng/ml

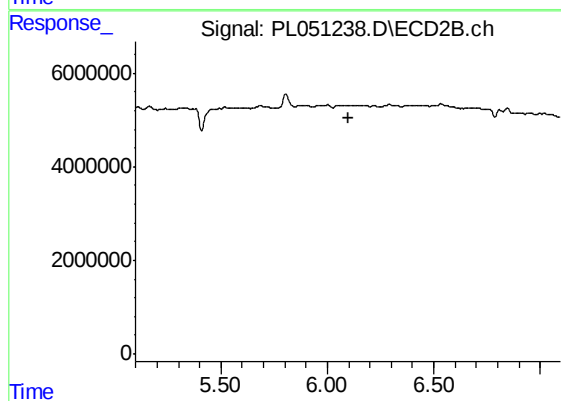

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

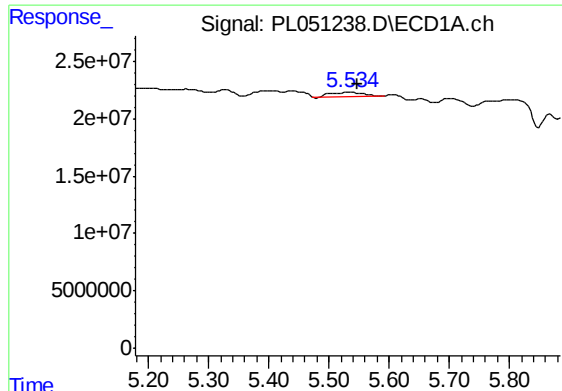

#13 Dieldrin


R.T.: 5.536 min
Delta R.T.: -0.013 min
Response: 12560033
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-080719-A

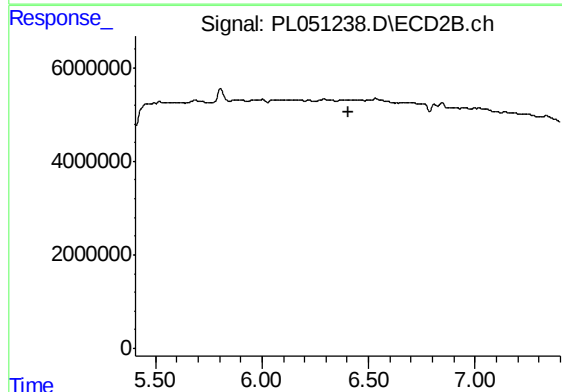


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

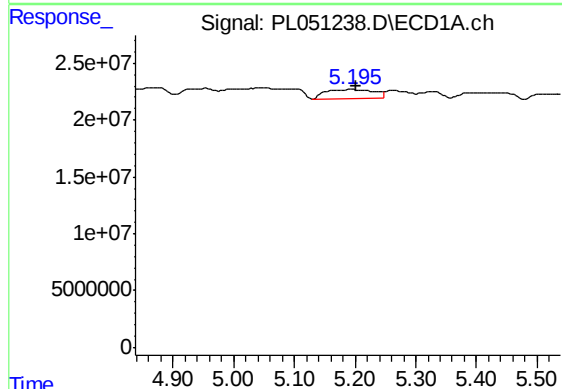


#25 Chlordane-3

R.T.: 5.196 min
Delta R.T.: -0.006 min
Response: 46910419
Conc: 33.51 ng/ml

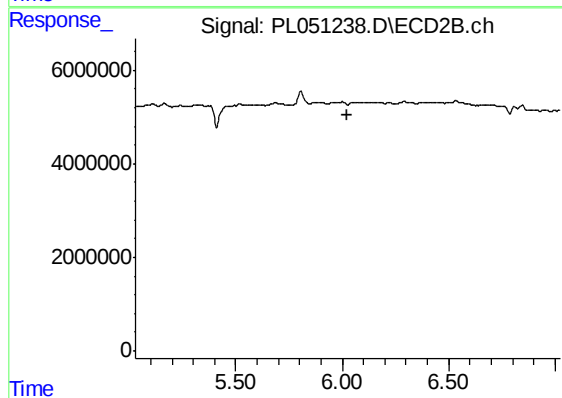

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

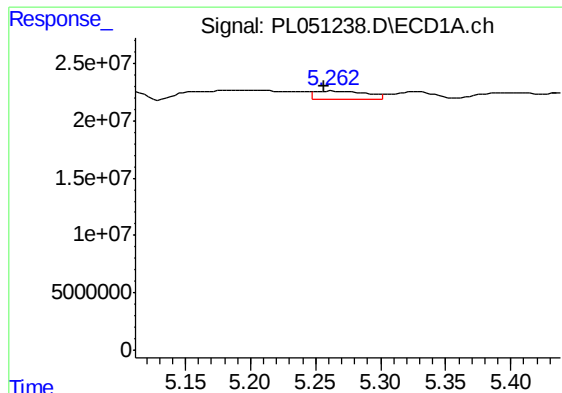

#26 Chlordane-4


R.T.: 5.263 min
Delta R.T.: 0.006 min
Response: 19332301
Conc: 14.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-080719-A

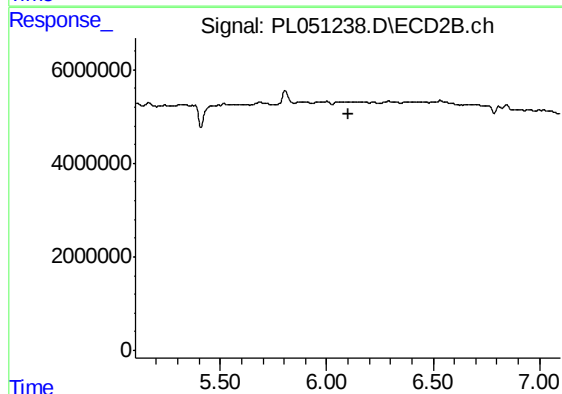


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

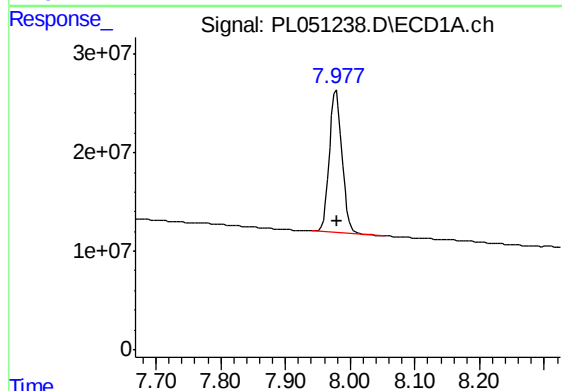

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 196869549
Conc: 19.44 ng/ml

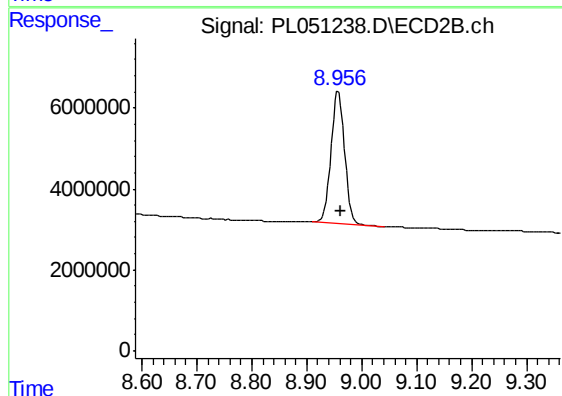

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 56072963
Conc: 19.83 ng/ml