

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 16:30
 Operator : SM\AJ
 Sample : K3613-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-080719-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:32:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.317	3.928	129.4E6	34987911	12.877	12.263
28)	SA Decachlor...	7.978	8.957	100.9E6	31943326	9.964	11.296
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	5059589	N.D.	2.927 #
8)	B Heptachlo...	0.000	5.805	0	6881123	N.D.	1.799 #
10)	B gamma-Chl...	5.219f	0.000	5139874	0	0.326	N.D. #
11)	B alpha-Chl...	0.000	6.095	0	3546322	N.D.	0.968 #
12)	B 4,4'-DDE	5.422	6.253	13108588	4403213	0.875	1.222 #
17)	MA 4,4'-DDT	6.164	0.000	6970008	0	0.563	N.D. #
25)	Chlordane-3	5.219f	0.000	5139874	0	3.672	N.D. #
26)	Chlordane-4	0.000	6.095	0	3546322	N.D.	6.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 16:30
Operator : SM\AJ
Sample : K3613-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:32:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

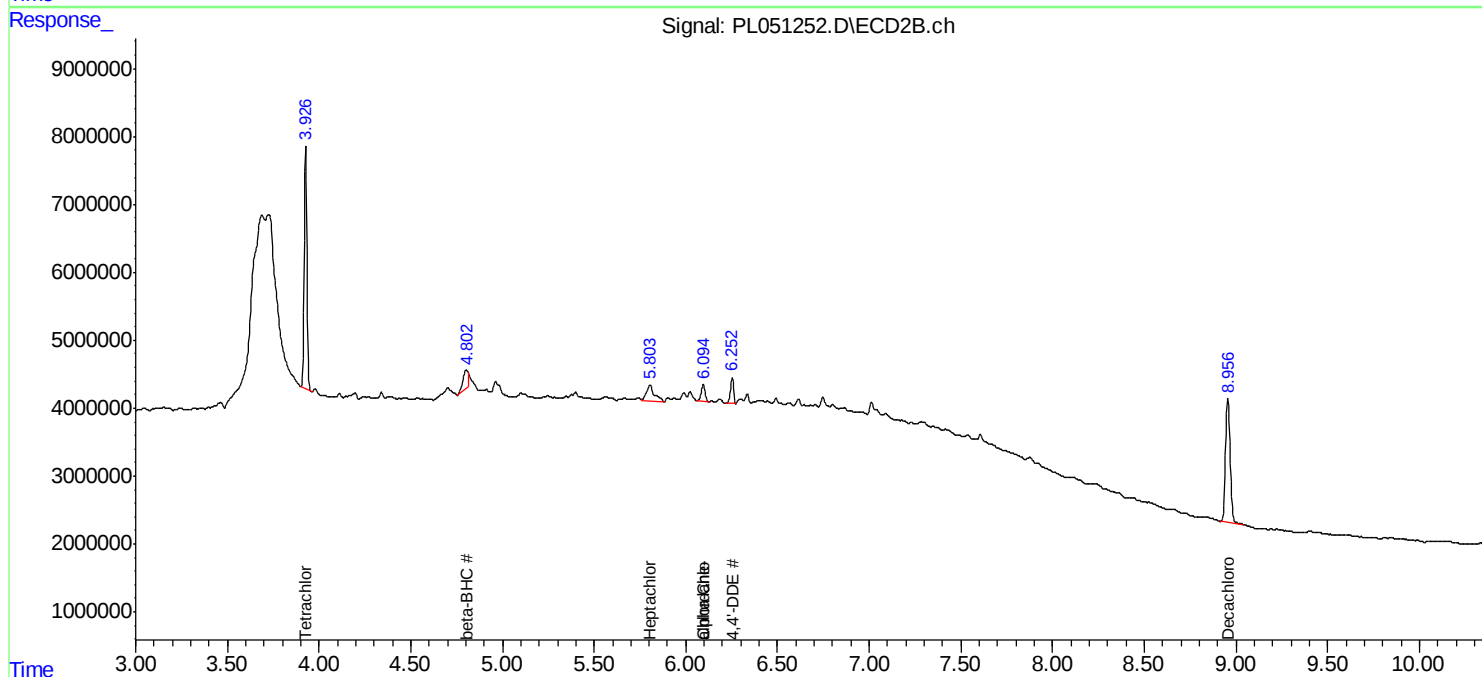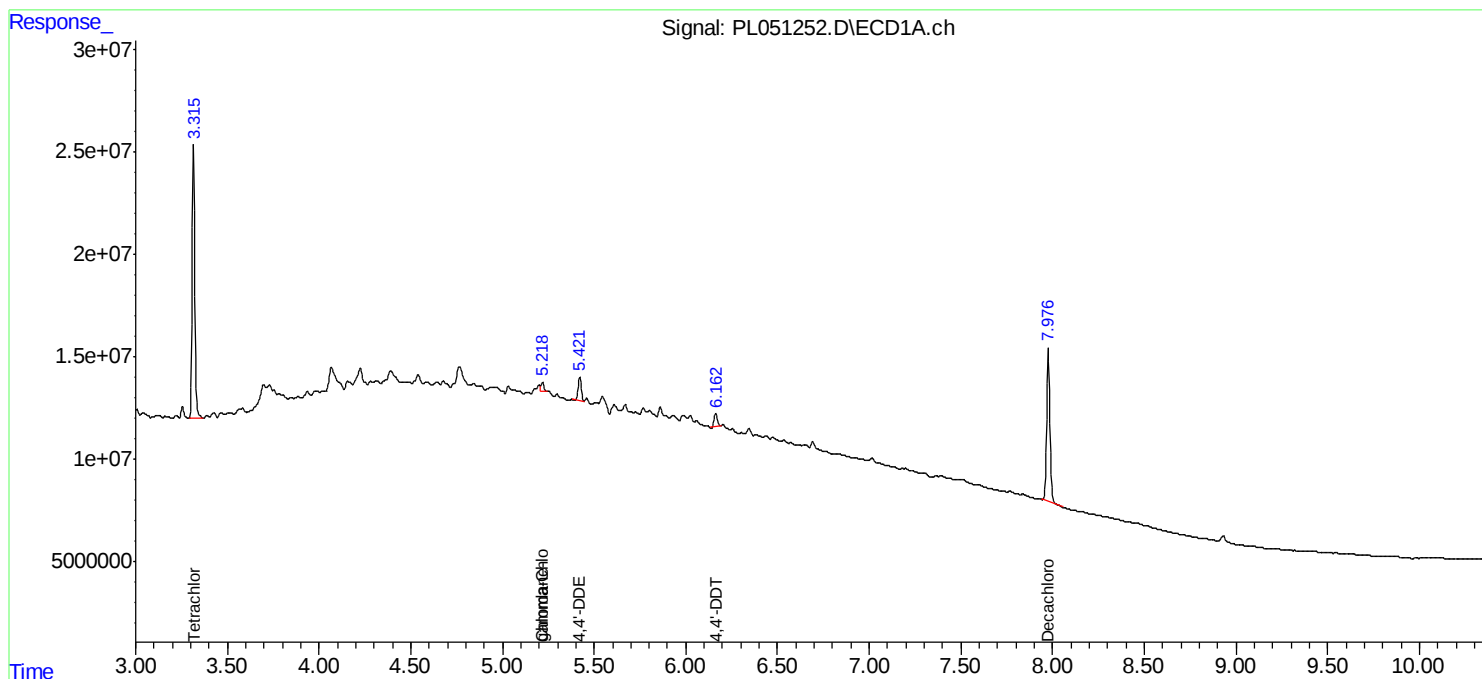


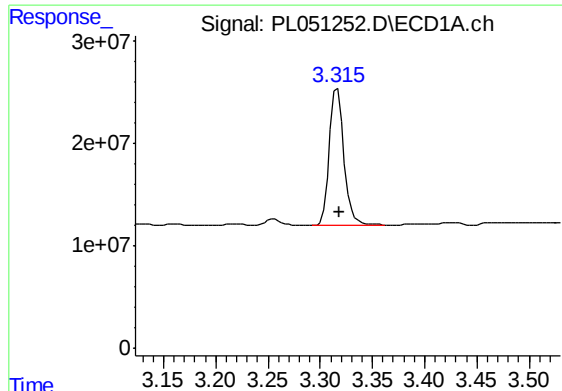

#1 Tetrachloro-m-xylene


R.T.: 3.317 min
Delta R.T.: -0.001 min
Response: 129389119
Conc: 12.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

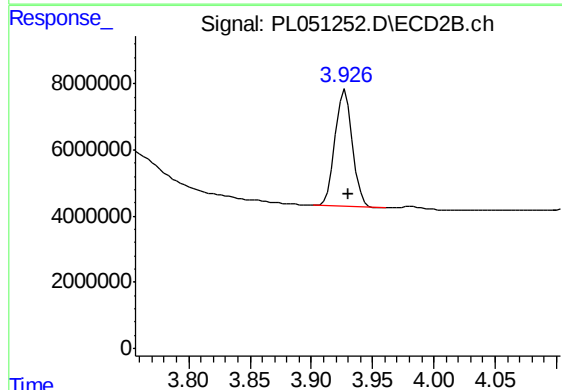


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 34987911
Conc: 12.26 ng/ml

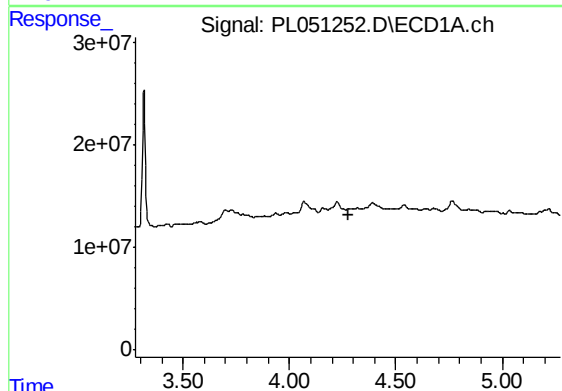


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

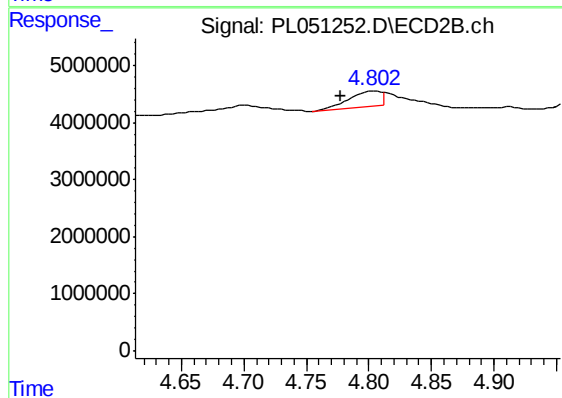

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 5059589
Conc: 2.93 ng/ml

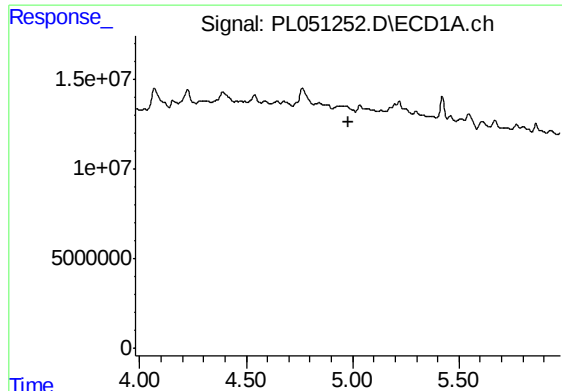

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

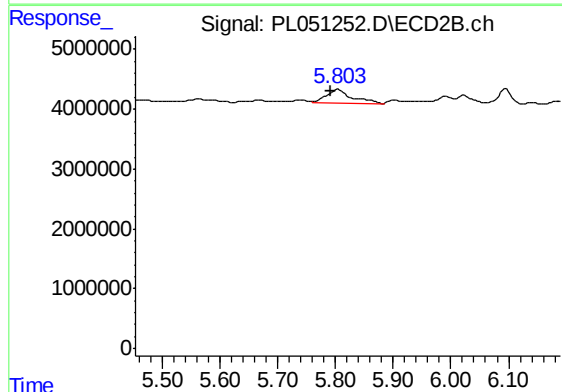


#8 Heptachlor epoxide

R.T.: 5.805 min
Delta R.T.: 0.012 min
Response: 6881123
Conc: 1.80 ng/ml

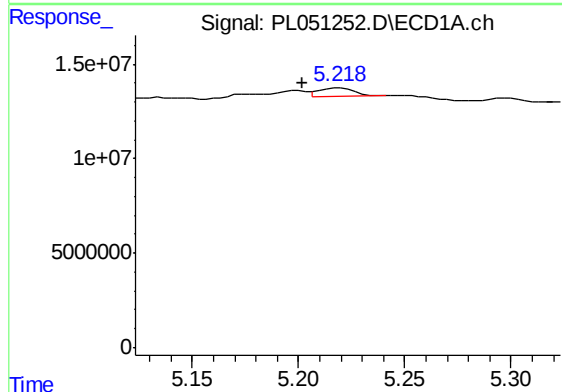


#10 gamma-Chlordane

R.T.: 5.219 min
Delta R.T.: 0.018 min
Response: 5139874
Conc: 0.33 ng/ml

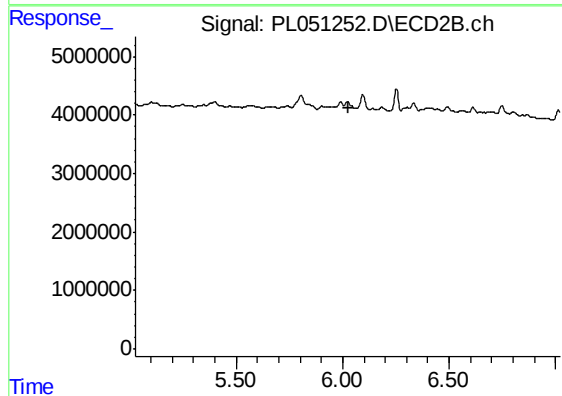

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

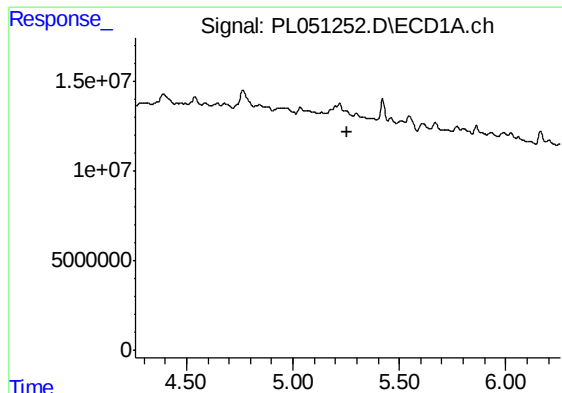

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

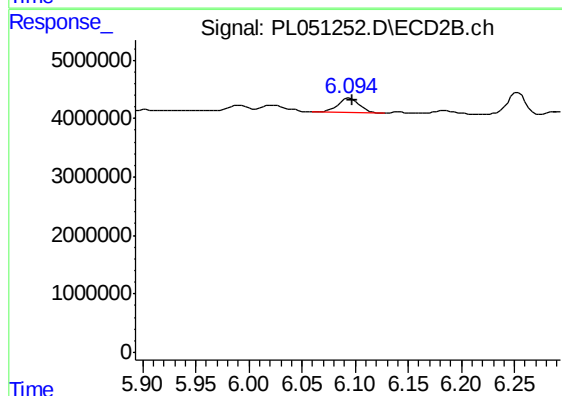


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 3546322
Conc: 0.97 ng/ml

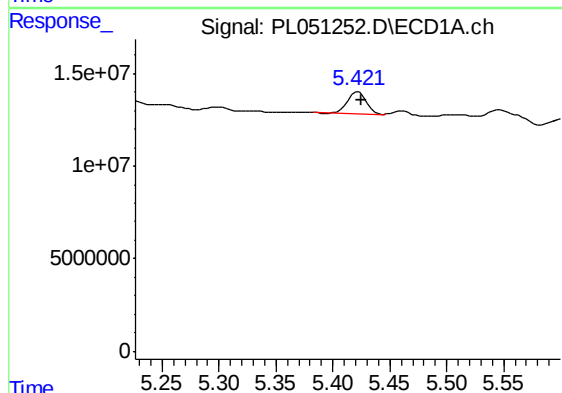


#12 4,4'-DDE

R.T.: 5.422 min
Delta R.T.: -0.002 min
Response: 13108588
Conc: 0.87 ng/ml

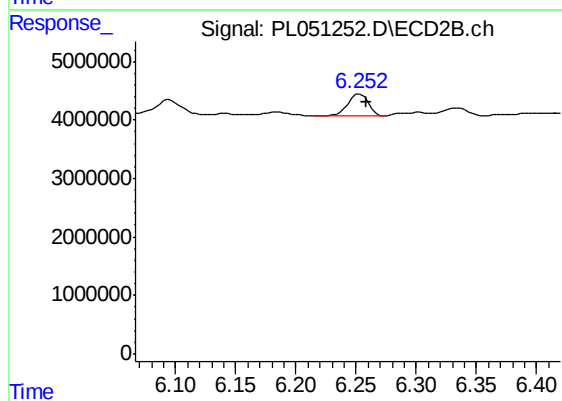

#12 4,4'-DDE


R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 4403213
Conc: 1.22 ng/ml

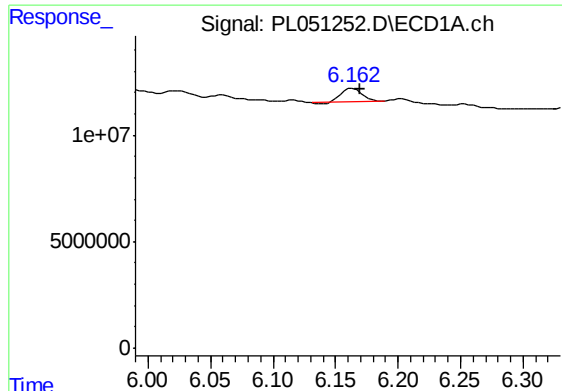

#17 4,4'-DDT


R.T.: 6.164 min
Delta R.T.: -0.006 min
Response: 6970008
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

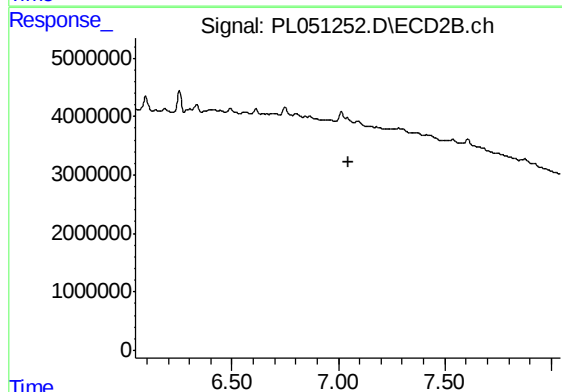


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

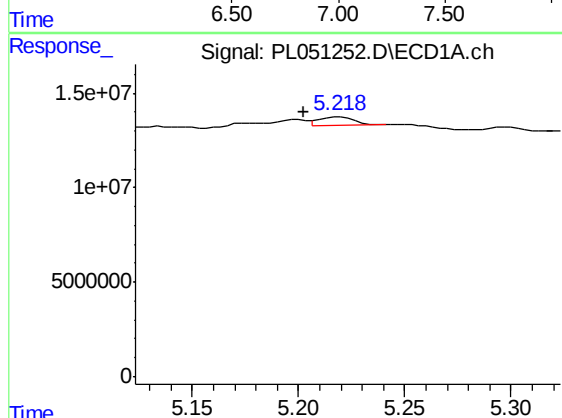


#25 Chlordane-3

R.T.: 5.219 min
Delta R.T.: 0.017 min
Response: 5139874
Conc: 3.67 ng/ml

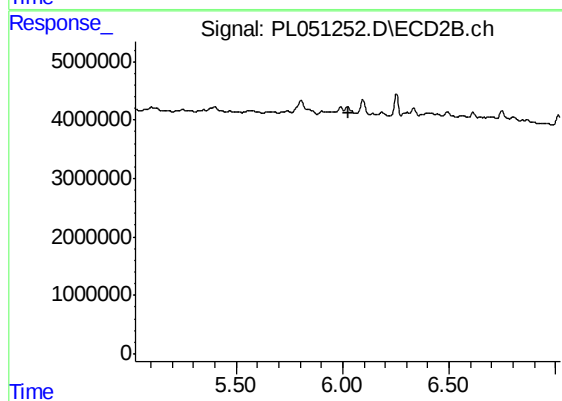

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

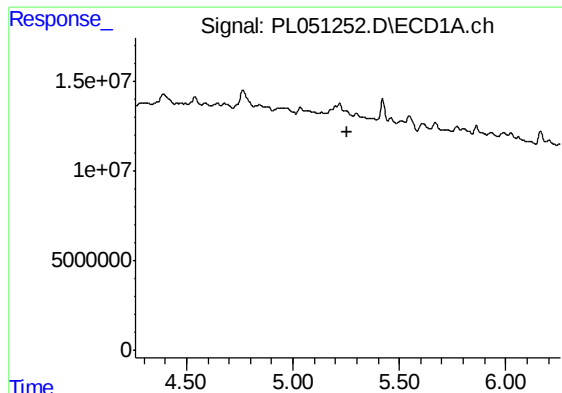

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-080719-B

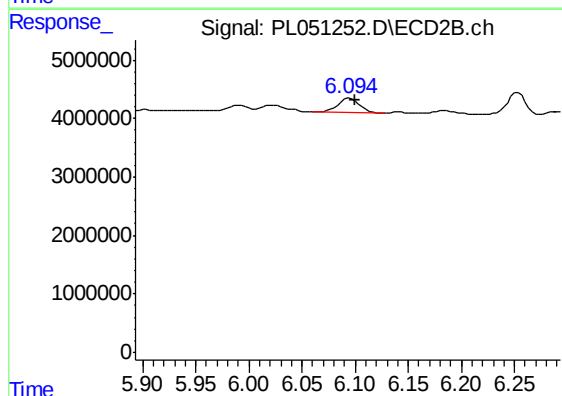


#26 Chlordane-4

R.T.: 6.095 min
Delta R.T.: -0.005 min
Response: 3546322
Conc: 6.10 ng/ml

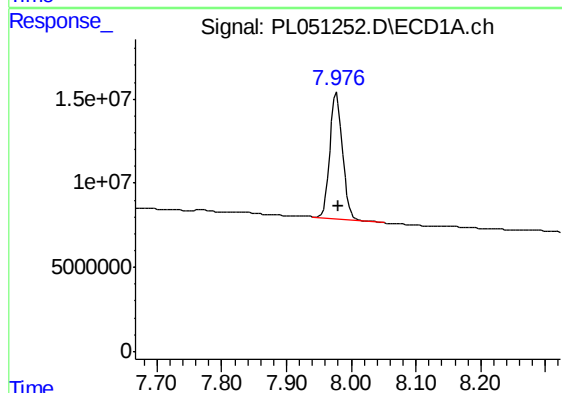

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.003 min
Response: 100891181
Conc: 9.96 ng/ml

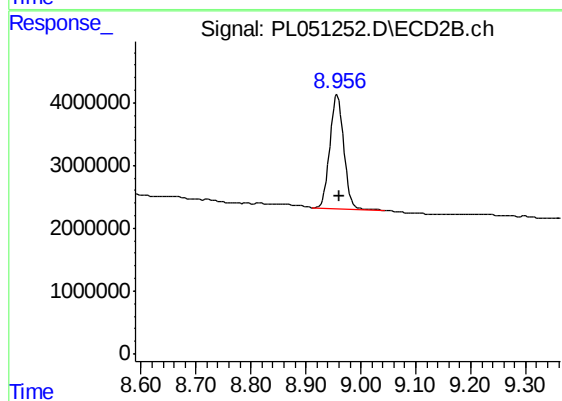

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.004 min
Response: 31943326
Conc: 11.30 ng/ml