

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 10:42
 Operator : SM\AJ
 Sample : K4154-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PS-3

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:21:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:25:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.928	130.8E6	40147882	13.019	14.071
28)	SA Decachlor...	7.979	8.956	69236991	25675602	6.838	9.079m#
Target Compounds							
10)	B gamma-Chl...	5.200	6.022	68922264	17115591	4.367m	4.632
11)	B alpha-Chl...	5.256	6.095	57513548	19290814	3.770	5.263 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 10:42
Operator : SM\AJ
Sample : K4154-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PS-3


Manual Integrations
APPROVED

Ankita
8/12/2019 1:21:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:25:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

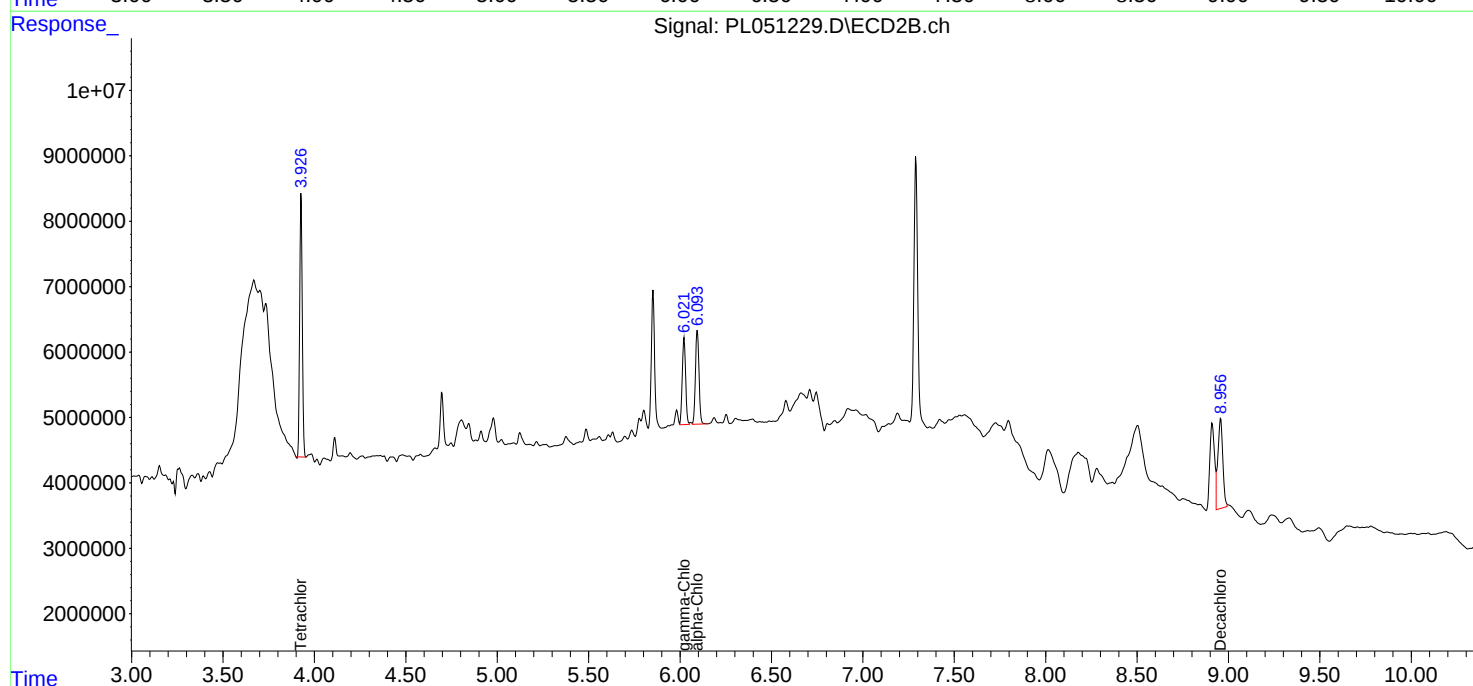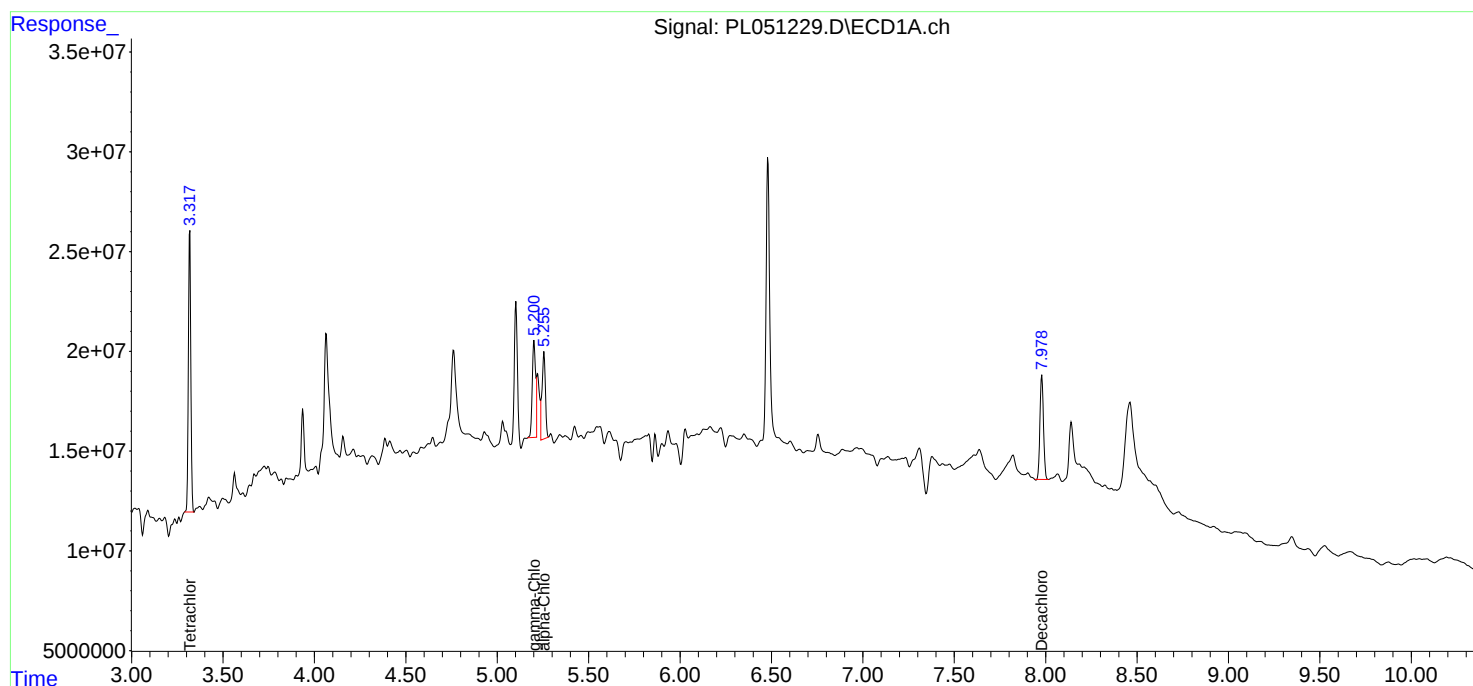

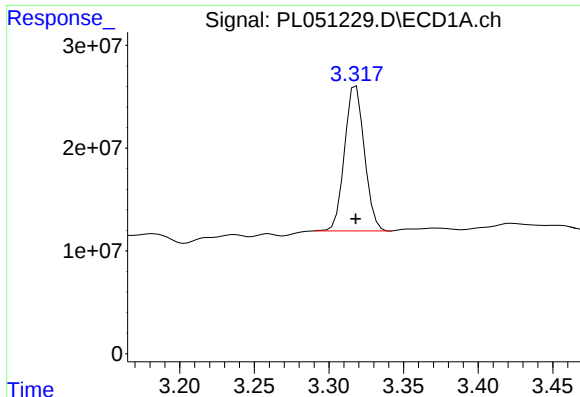


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 130811909
Conc: 13.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-3


Manual Integrations
APPROVED

Ankita
8/12/2019 1:21:32 PM

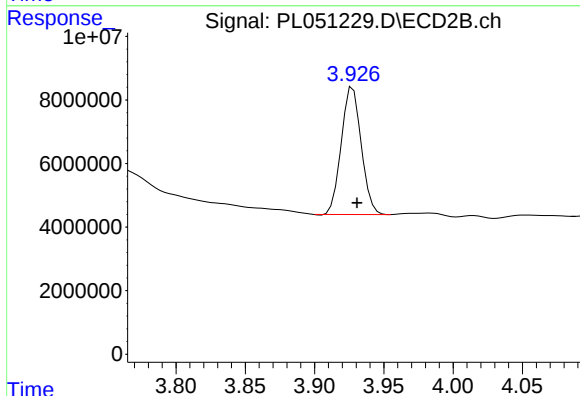


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.003 min
Response: 40147882
Conc: 14.07 ng/ml

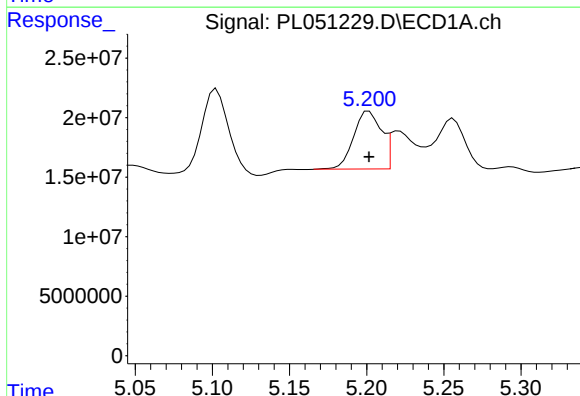


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 68922264
Conc: 4.37 ng/ml m

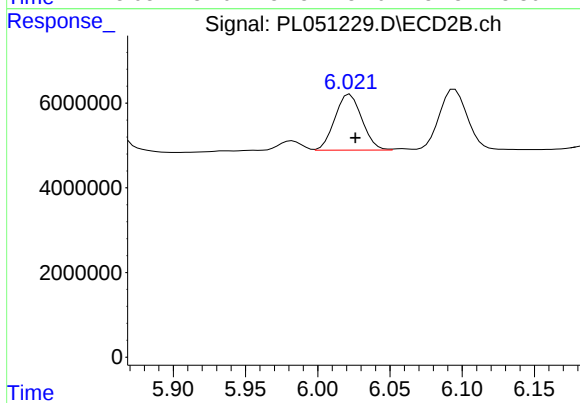

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.004 min
Response: 17115591
Conc: 4.63 ng/ml

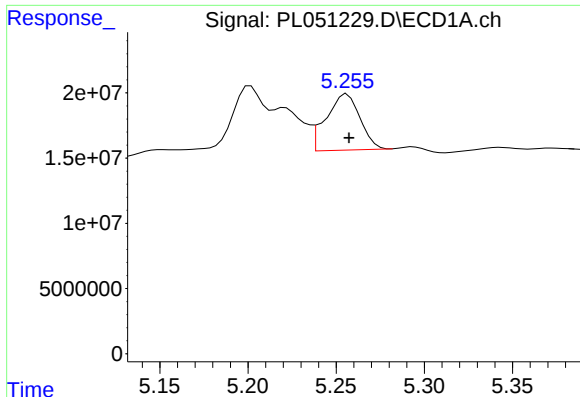


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.001 min
Response: 57513548
Conc: 3.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PS-3


Manual Integrations
APPROVED

Ankita
8/12/2019 1:21:32 PM

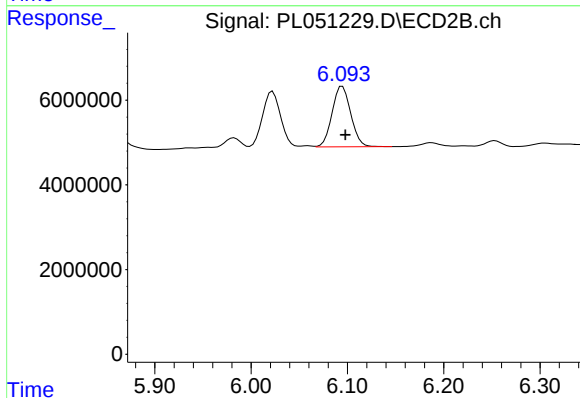


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 19290814
Conc: 5.26 ng/ml

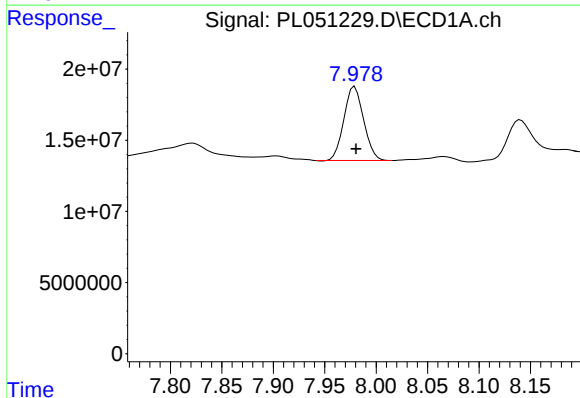

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 69236991
Conc: 6.84 ng/ml

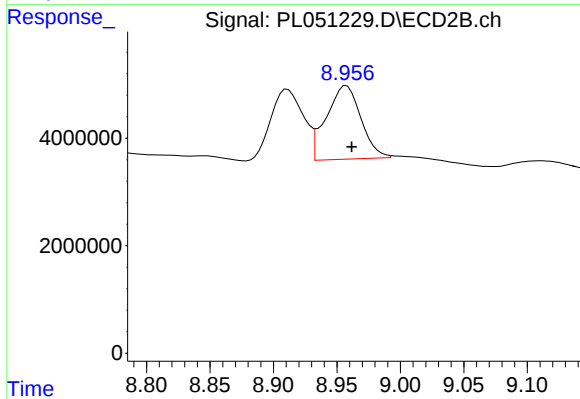

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 25675602
Conc: 9.08 ng/ml m