

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
 Data File : PL051263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2019 19:16
 Operator : SM\AJ
 Sample : K4238-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-18

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:22:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 02:35:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.318	3.928	249.2E6	65636571	24.806	23.004
28) SA Decachlor...	7.979	8.958	206.5E6	56449484	20.396	19.962
Target Compounds						
17) MA 4,4'-DDT	6.166	7.042	24109914	4418926	1.947m	1.637m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080919\
Data File : PL051263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2019 19:16
Operator : SM\AJ
Sample : K4238-05
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-18


Manual Integrations
APPROVED

Ankita
8/12/2019 1:22:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 02:35:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

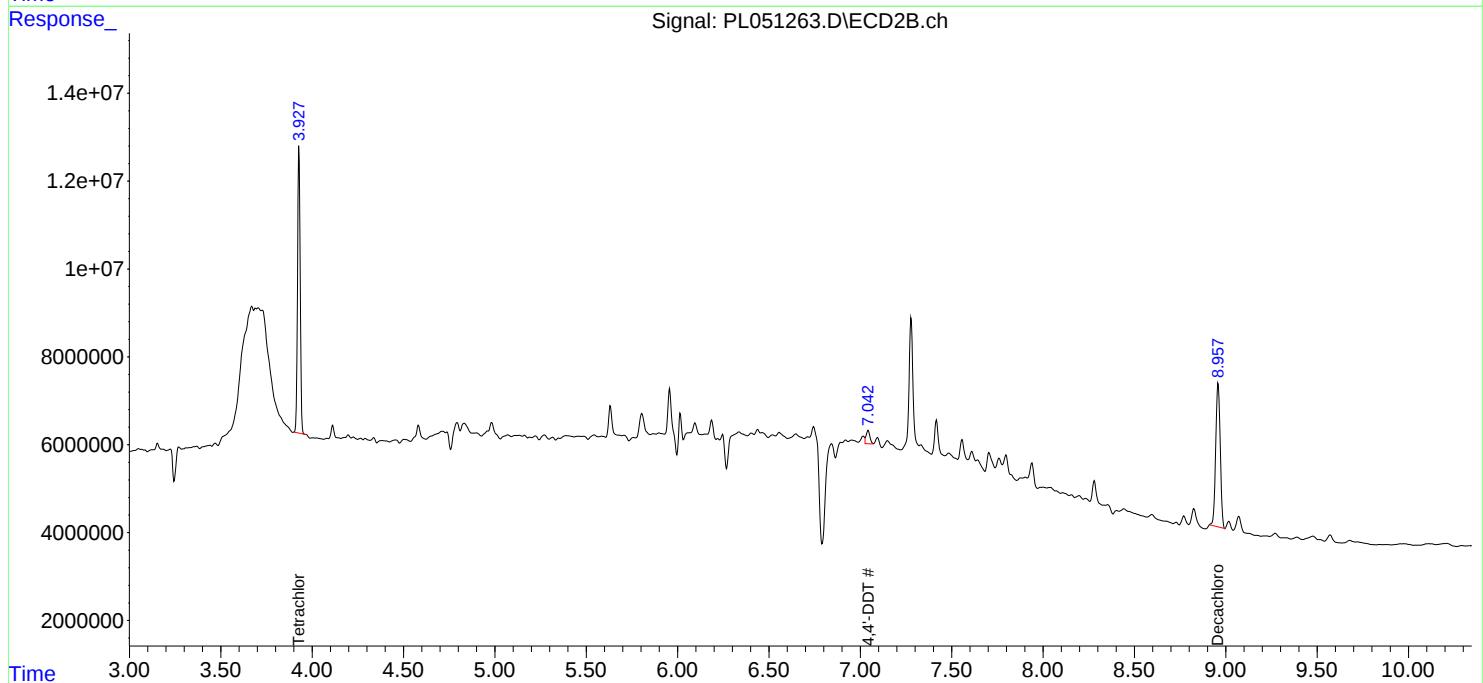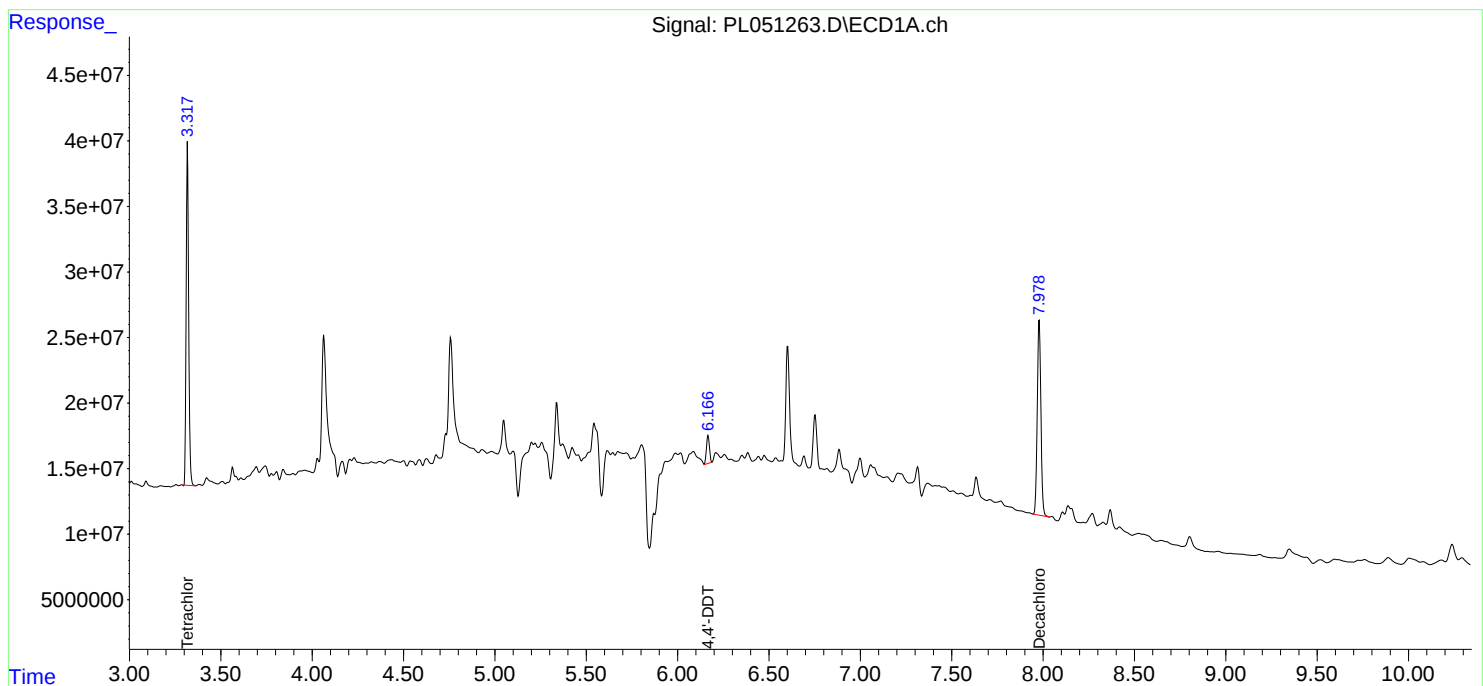

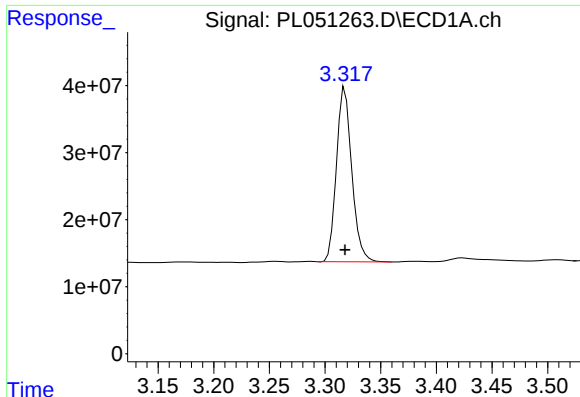


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 249248720
Conc: 24.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-18


Manual Integrations
APPROVED

Ankita
8/12/2019 1:22:19 PM

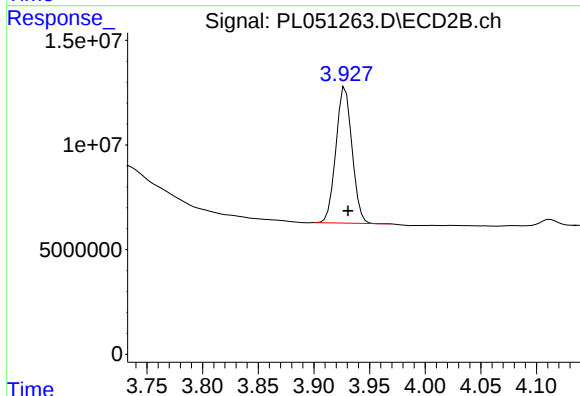


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 65636571
Conc: 23.00 ng/ml

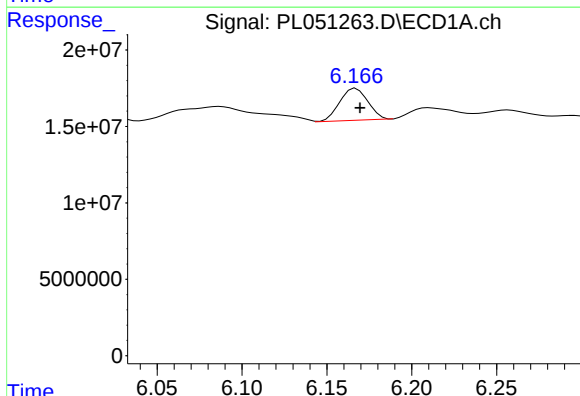


#17 4,4'-DDT

R.T.: 6.166 min
Delta R.T.: -0.004 min
Response: 24109914
Conc: 1.95 ng/ml m

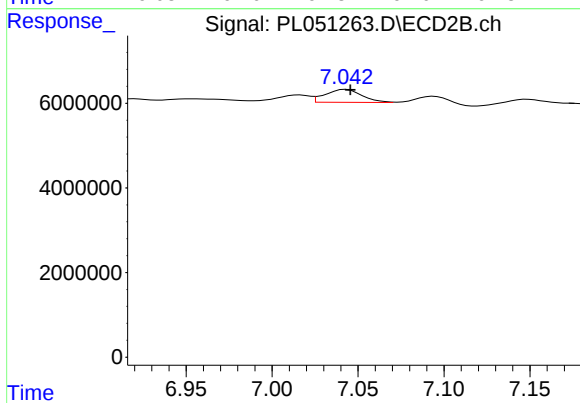

#17 4,4'-DDT

R.T.: 7.042 min
Delta R.T.: -0.004 min
Response: 4418926
Conc: 1.64 ng/ml m

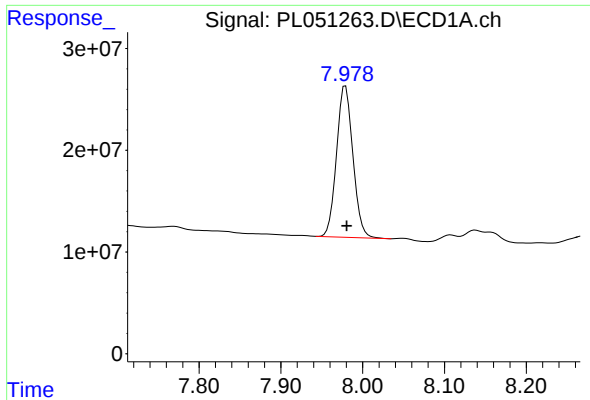


#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 206516958
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-18

Manual Integrations
APPROVED

Ankita
8/12/2019 1:22:19 PM

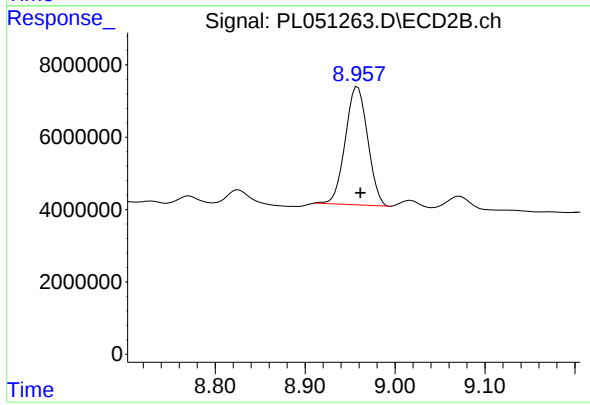

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.003 min
Response: 56449484
Conc: 19.96 ng/ml