

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080922\
 Data File : PL076996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 13:52
 Operator : AR\AJ
 Sample : N4105-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:07:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.639	838073	2546011	0.855	0.889
28)	SA Decachlor...	8.913	7.747	1036986	2862961	1.374	1.272
Target Compounds							
17)	MA 4,4'-DDT	6.886f	5.867	158104	527015	0.206	0.232
19)	B Endosulfa...	0.000	6.165	0	293330	N.D.	0.127 #
20)	A Methoxychlor	0.000	6.423f	0	578845	N.D.	0.481 #
24)	Chlordane-2	0.000	4.191	0	924140	N.D.	8.035 #
27)	Chlordane-5	0.000	5.543	0	384781	N.D.	4.220 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080922\
Data File : PL076996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 13:52
Operator : AR\AJ
Sample : N4105-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:07:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

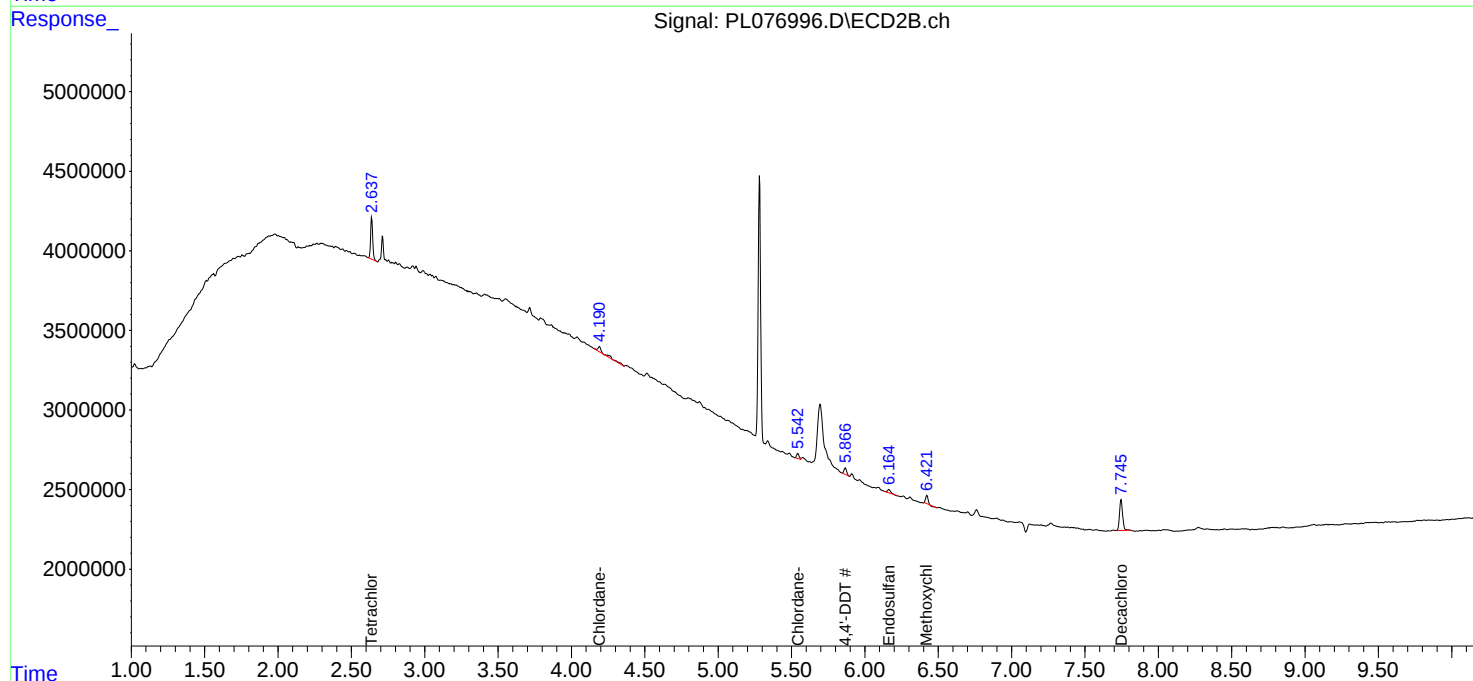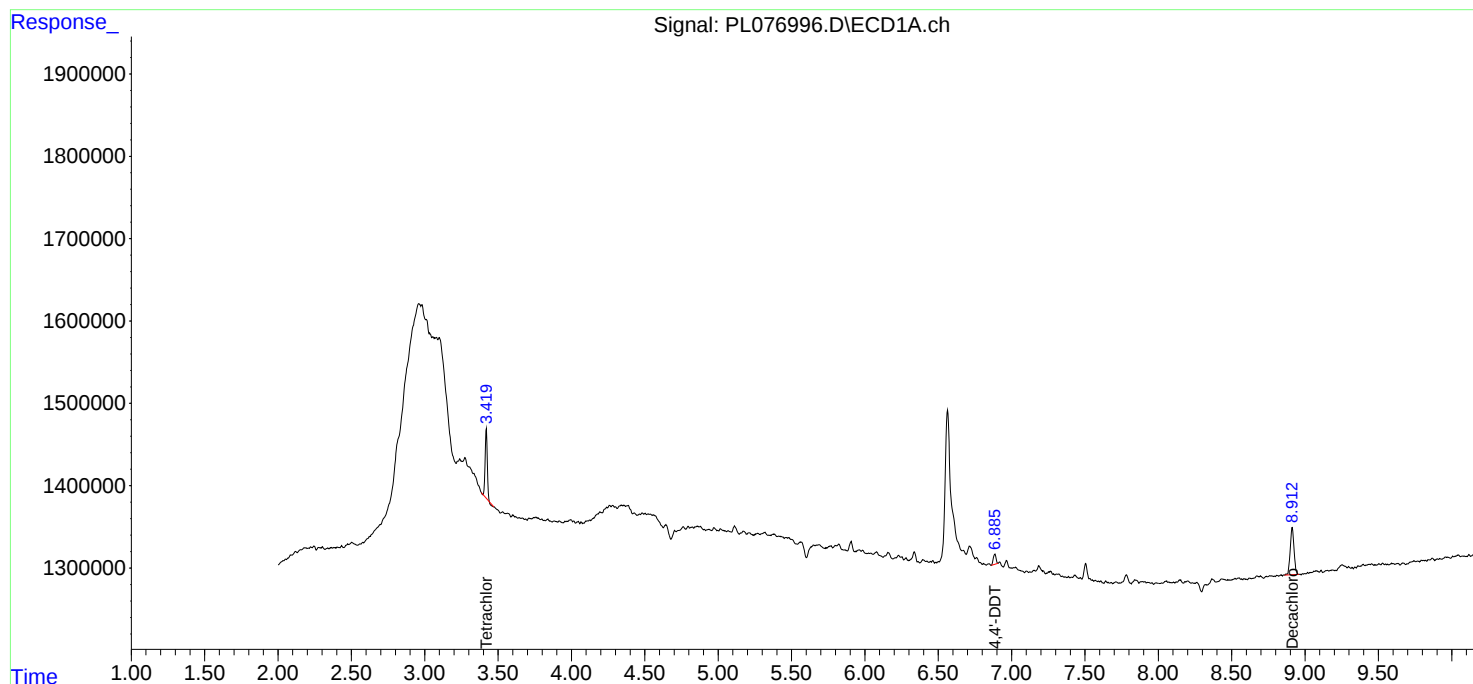


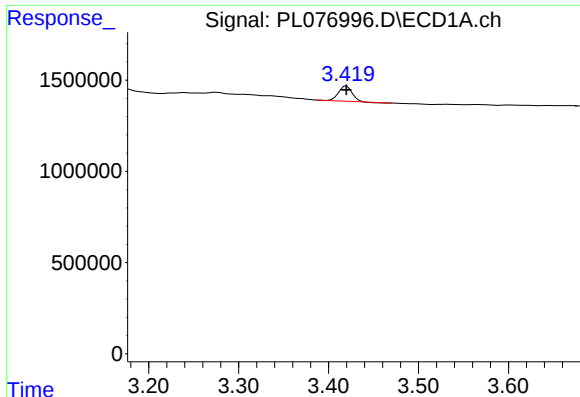

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 838073
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

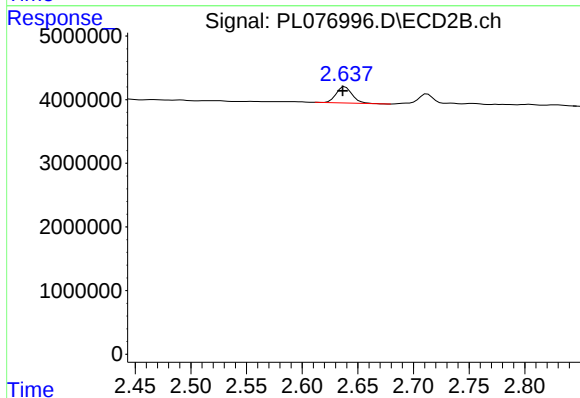


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.002 min
Response: 2546011
Conc: 0.89 ng/ml

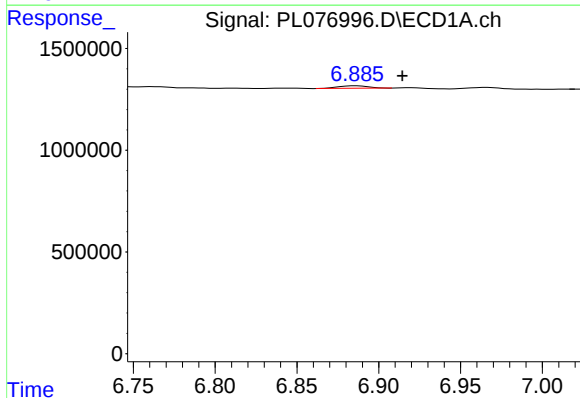


#17 4,4'-DDT

R.T.: 6.886 min
Delta R.T.: -0.028 min
Response: 158104
Conc: 0.21 ng/ml

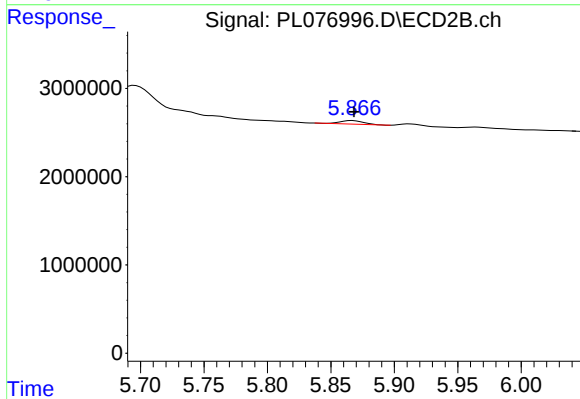

#17 4,4'-DDT


R.T.: 5.867 min
Delta R.T.: -0.001 min
Response: 527015
Conc: 0.23 ng/ml

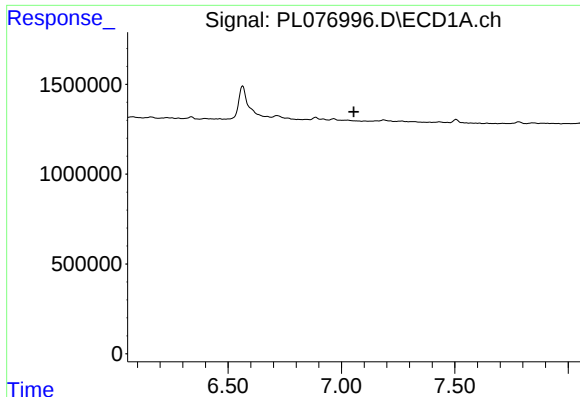

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.055 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

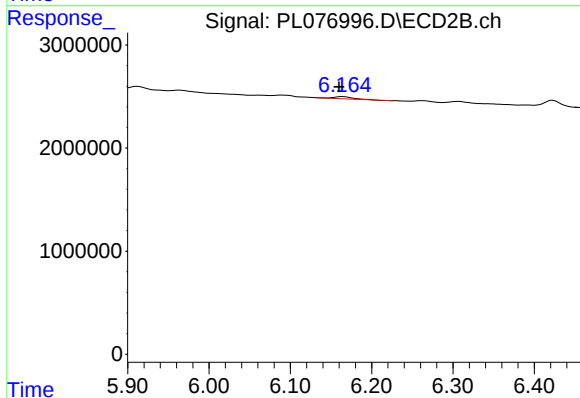


#19 Endosulfan Sulfate

R.T.: 6.165 min
Delta R.T.: 0.005 min
Response: 293330
Conc: 0.13 ng/ml

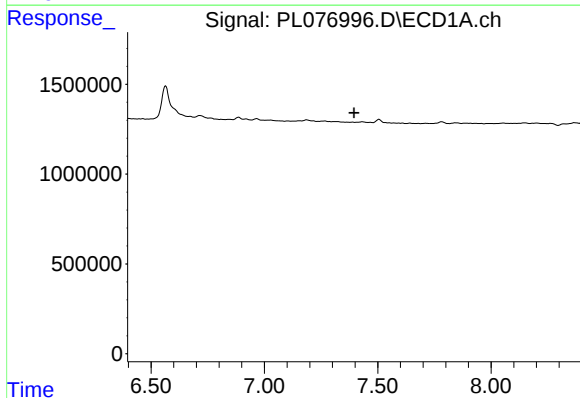


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.396 min
Response: 0
Conc: N.D.

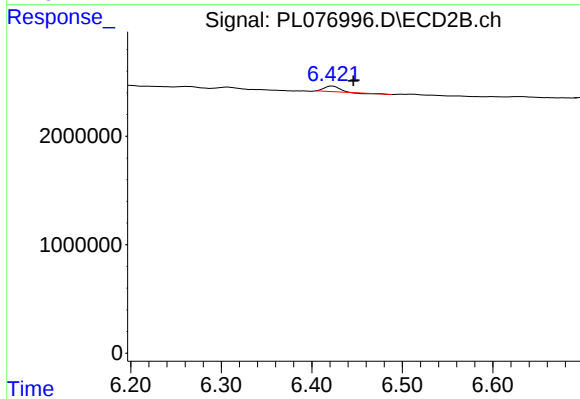

#20 Methoxychlor


R.T.: 6.423 min
Delta R.T.: -0.023 min
Response: 578845
Conc: 0.48 ng/ml

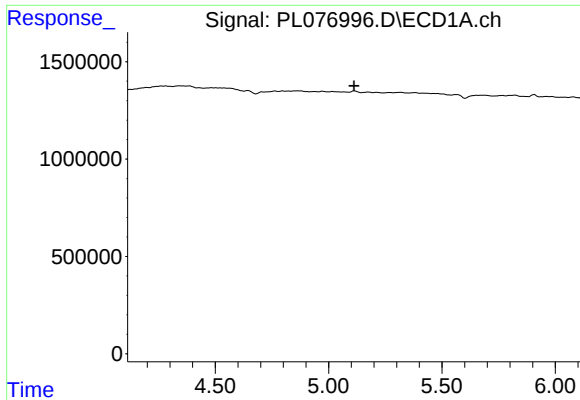

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

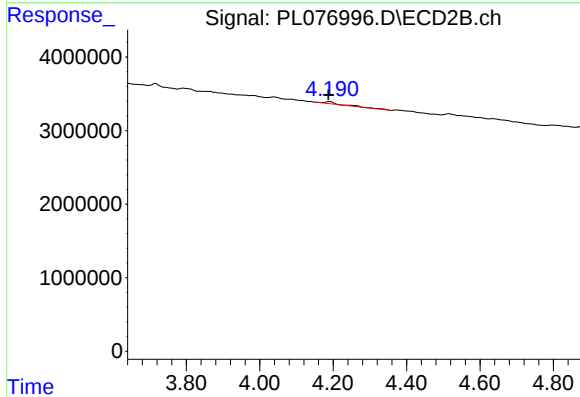


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.004 min
Response: 924140
Conc: 8.04 ng/ml

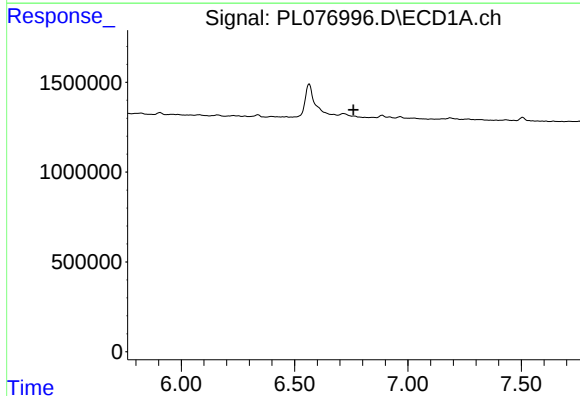


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.760 min
Response: 0
Conc: N.D.

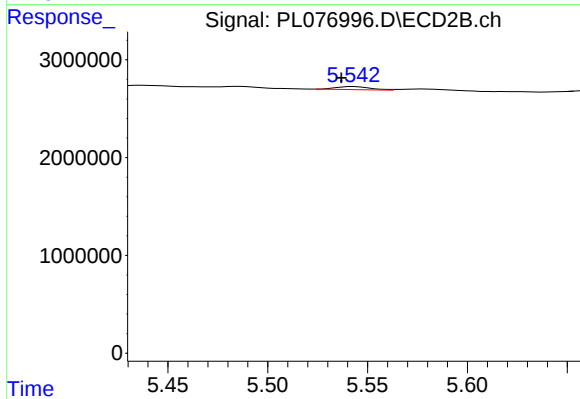

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: 0.006 min
Response: 384781
Conc: 4.22 ng/ml

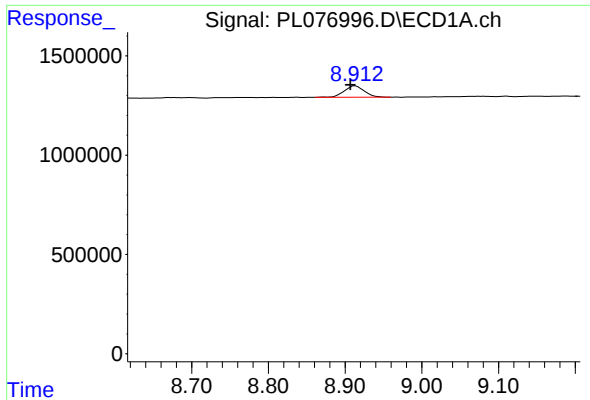

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.006 min
Response: 1036986
Conc: 1.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

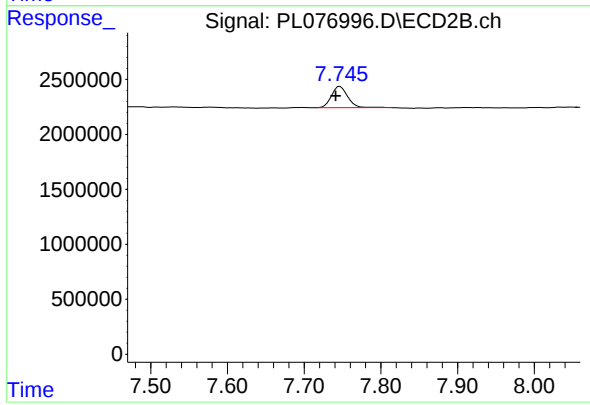

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 2862961
Conc: 1.27 ng/ml