

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080922\
 Data File : PL076996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 13:52
 Operator : AR\AJ
 Sample : N4105-01 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-080822

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:07:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.639	911104	2546011	0.929m	0.889
2)	SA Decachlor...	8.913	7.747	1036986	2862961	1.374	1.272

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080922\
Data File : PL076996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 13:52
Operator : AR\AJ
Sample : N4105-01 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EO-01-080822


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:07:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

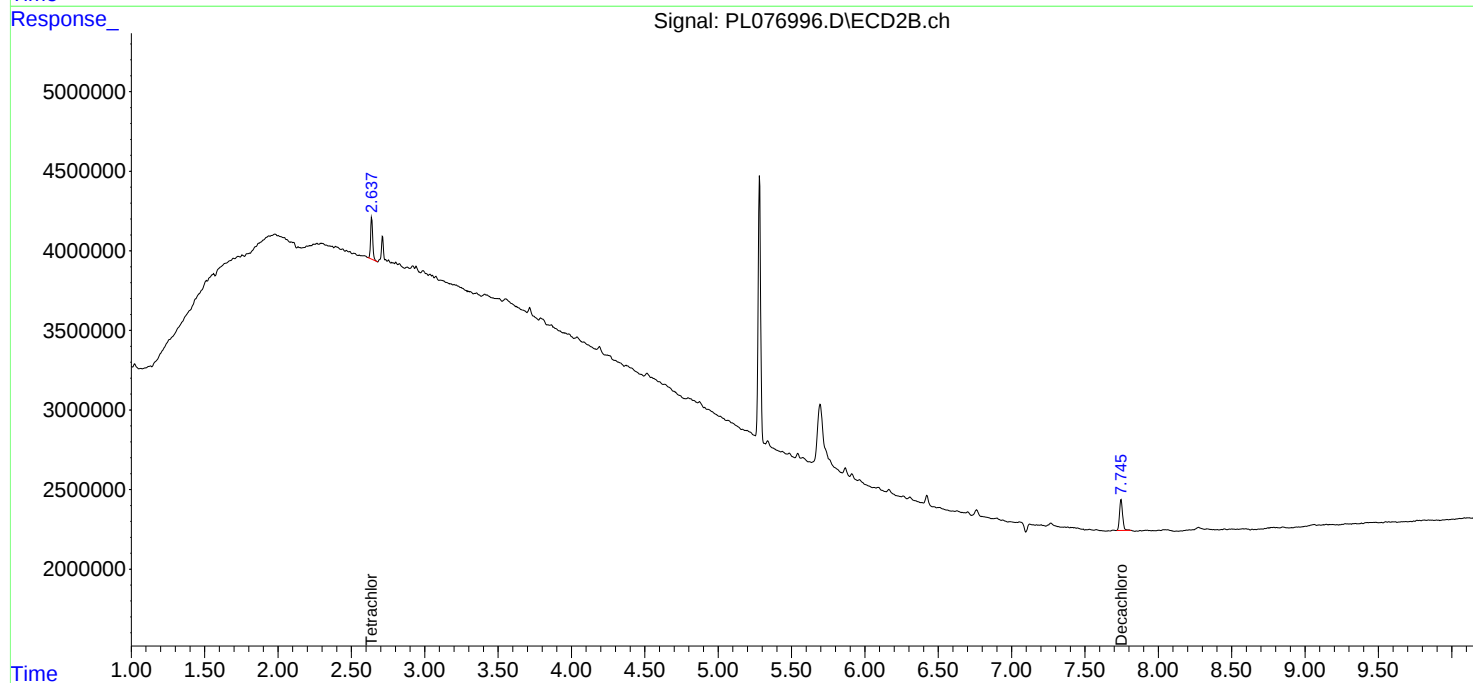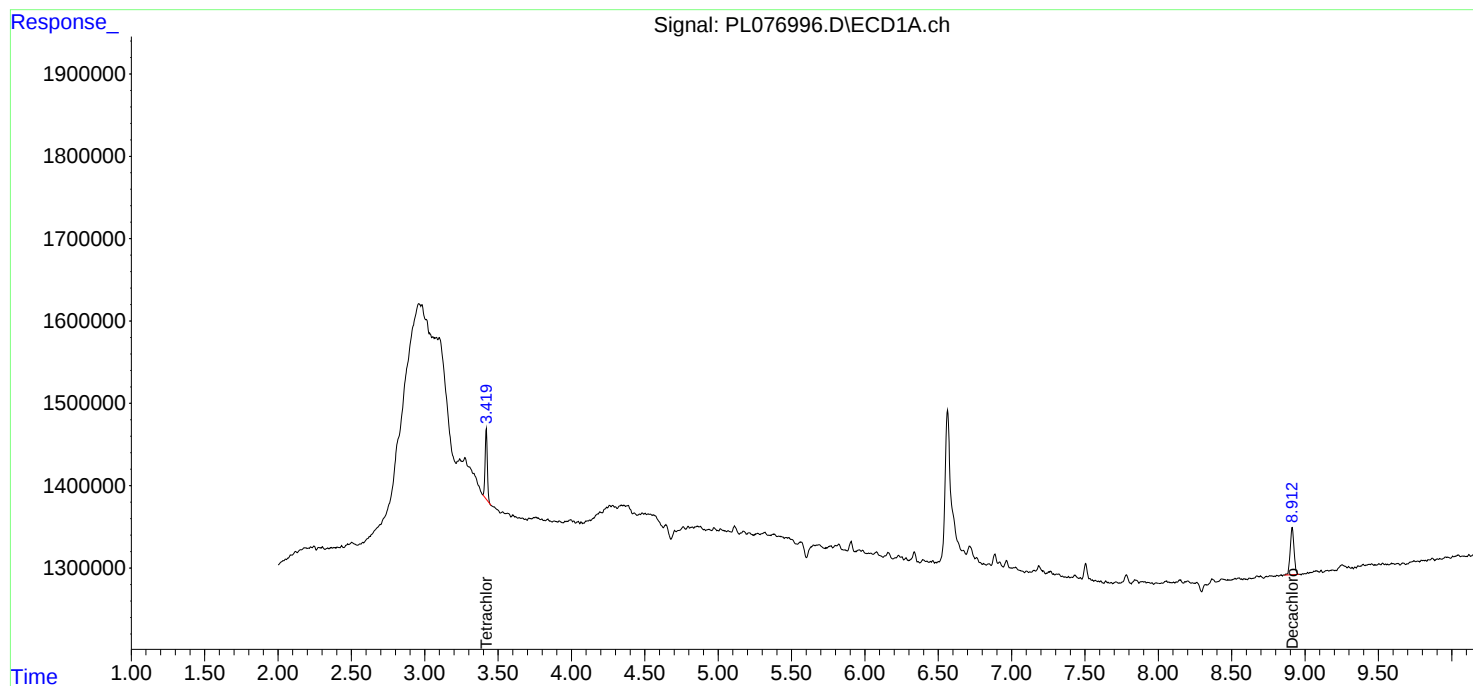

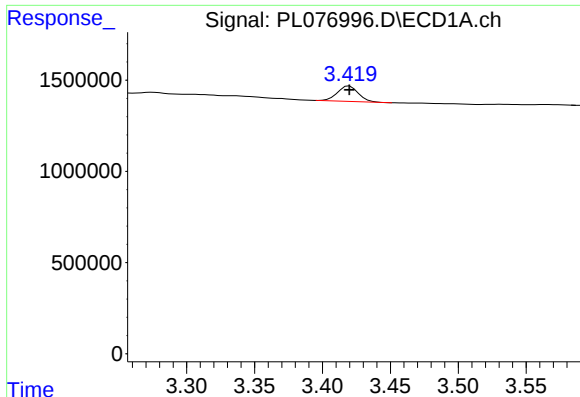

#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 911104
Conc: 0.93 ng/ml

Instrument :

ECD_L


ClientSampleId :

EO-01-080822

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

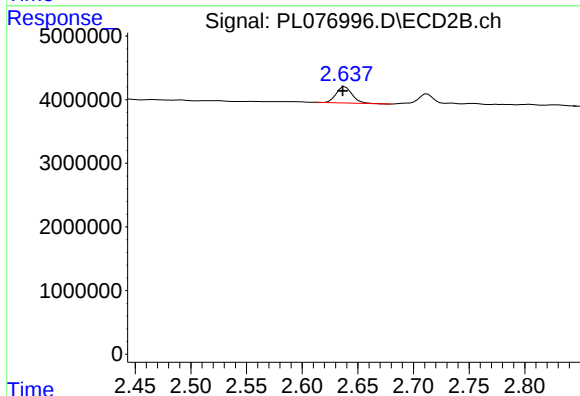


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.002 min
Response: 2546011
Conc: 0.89 ng/ml

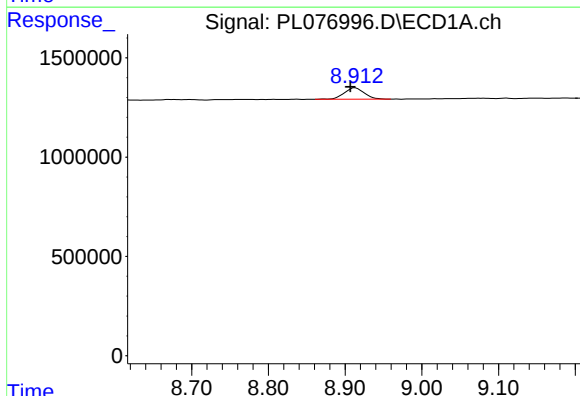

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.006 min
Response: 1036986
Conc: 1.37 ng/ml

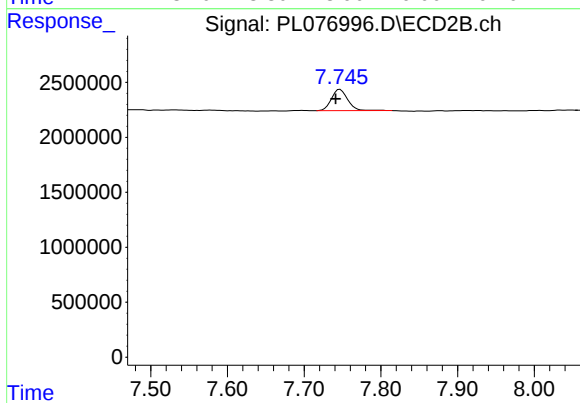

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 2862961
Conc: 1.27 ng/ml