

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080923\
 Data File : PL084613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 16:21
 Operator : AR\AJ
 Sample : 03932-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NEVINS-SB-01-Z30-32

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2023
 Supervised By : Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 04:30:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.686	14120795	6685477	6.077m	6.148m
28) SA Decachlor...	9.037	7.868	17687009	13518198	10.870m	10.842

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080923\
Data File : PL084613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 16:21
Operator : AR\AJ
Sample : 03932-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NEVINS-SB-01-Z30-32


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2023
Supervised By : Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 04:30:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

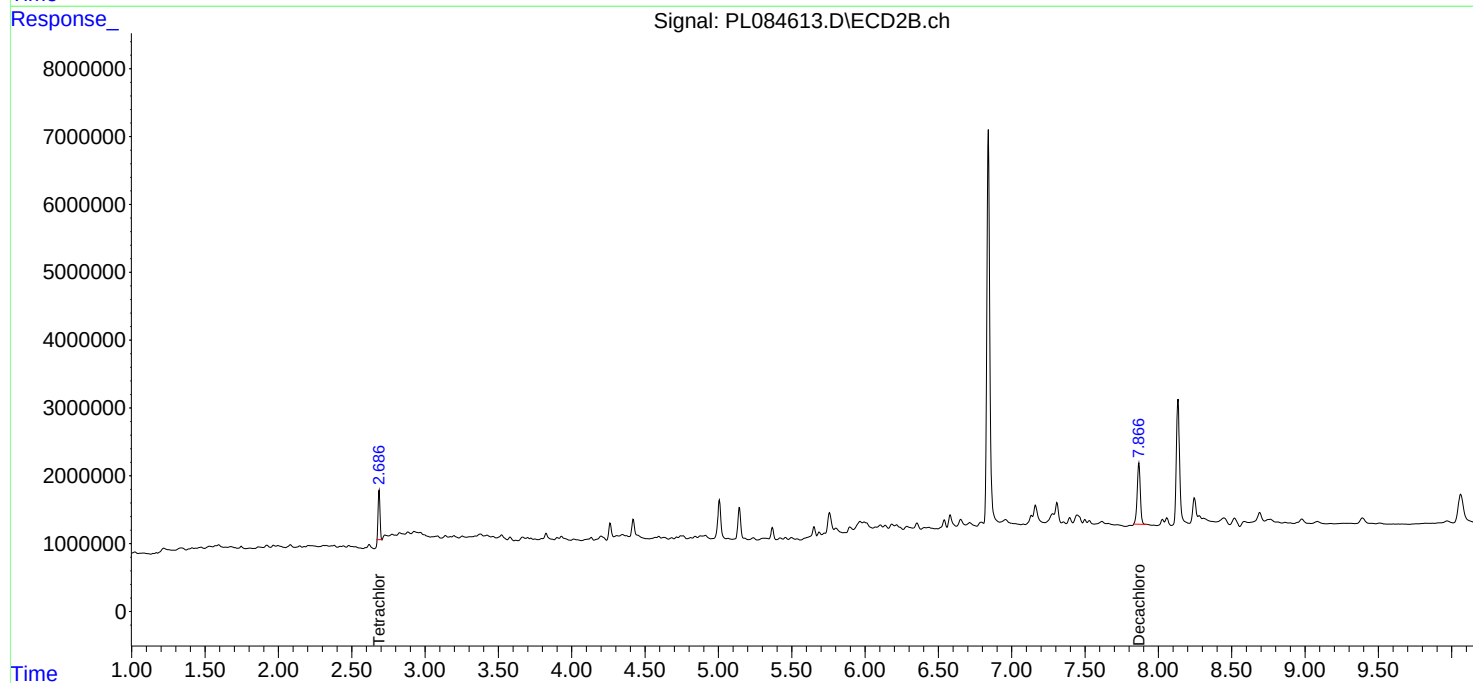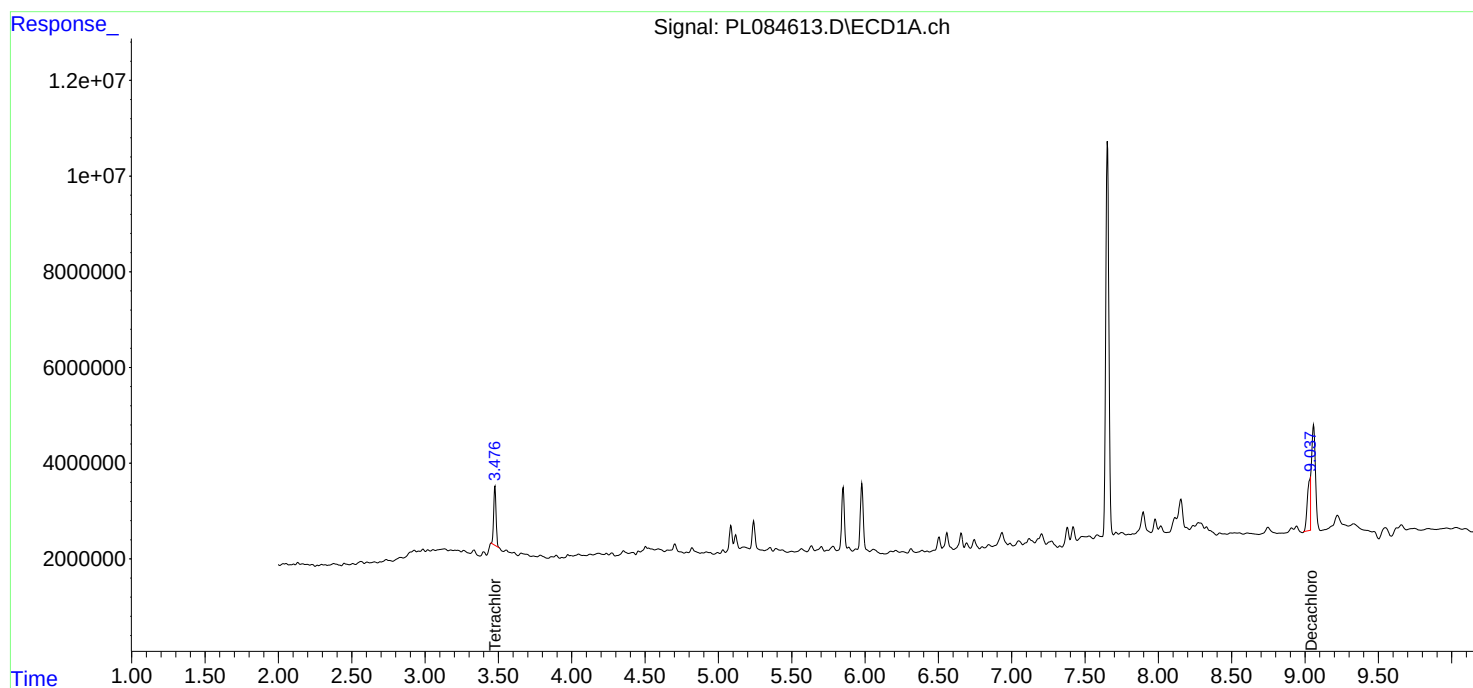

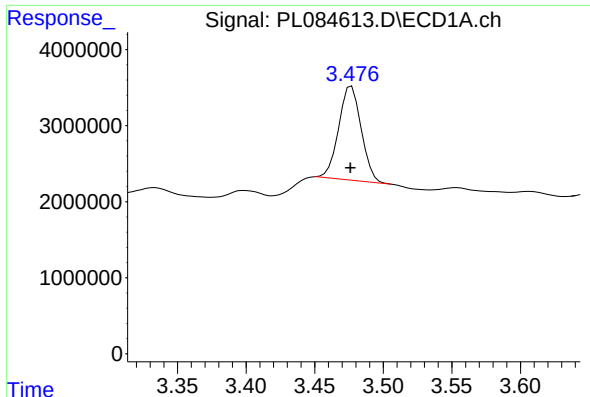


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 14120795
Conc: 6.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEVINS-SB-01-Z30-32


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

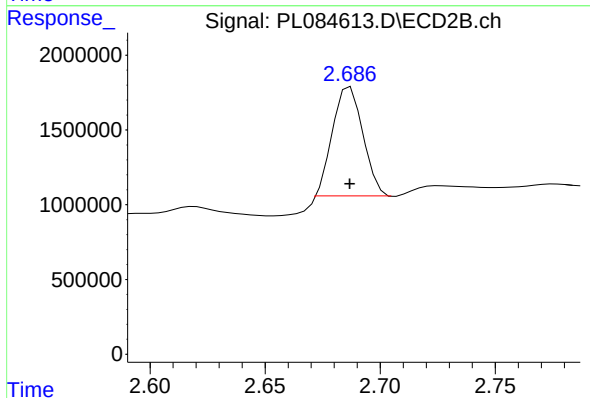


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: -0.001 min
Response: 6685477
Conc: 6.15 ng/ml m

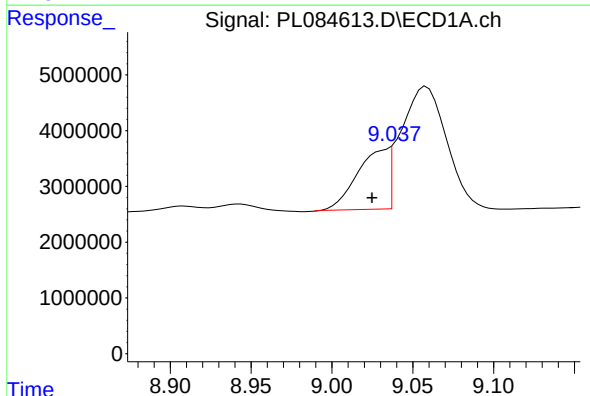

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: 0.012 min
Response: 17687009
Conc: 10.87 ng/ml m

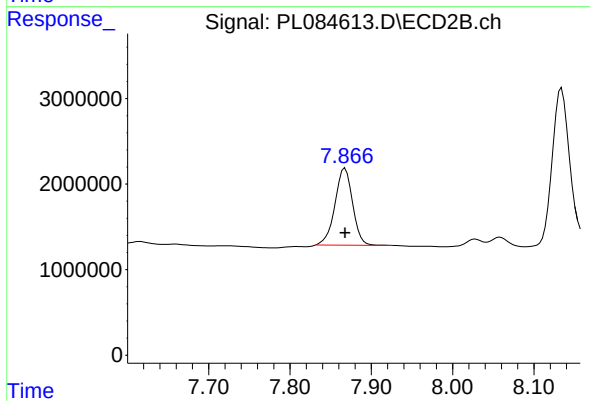

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: 0.000 min
Response: 13518198
Conc: 10.84 ng/ml