

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080923\
 Data File : PL084614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2023 16:35
 Operator : AR\AJ
 Sample : 03932-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NEVINS-SB-01-Z67-69

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/11/2023
 Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 04:30:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.685	14009128	7062866	6.029m	6.495m
28)	SA Decachlor...	9.029	7.867	17450682	14199922	10.725	11.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080923\
Data File : PL084614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2023 16:35
Operator : AR\AJ
Sample : 03932-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NEVINS-SB-01-Z67-69


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2023
Supervised By : Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 04:30:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

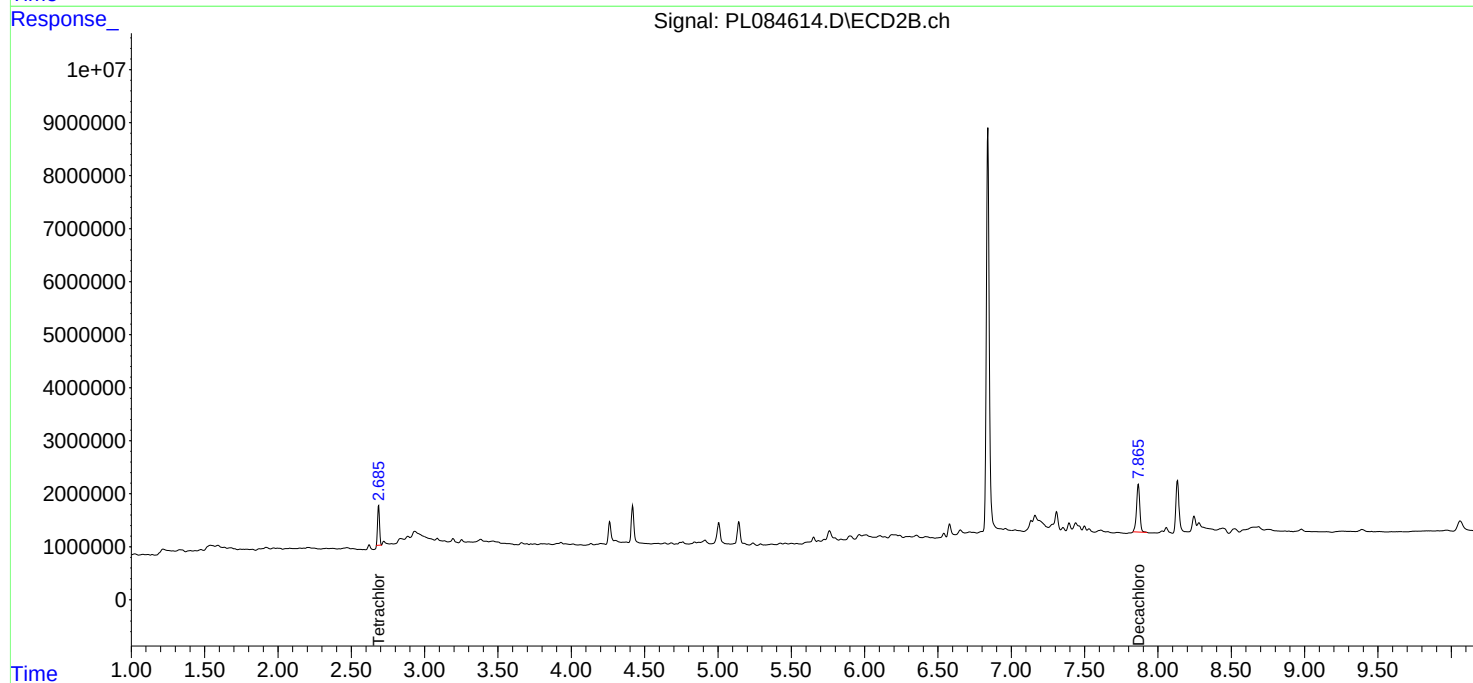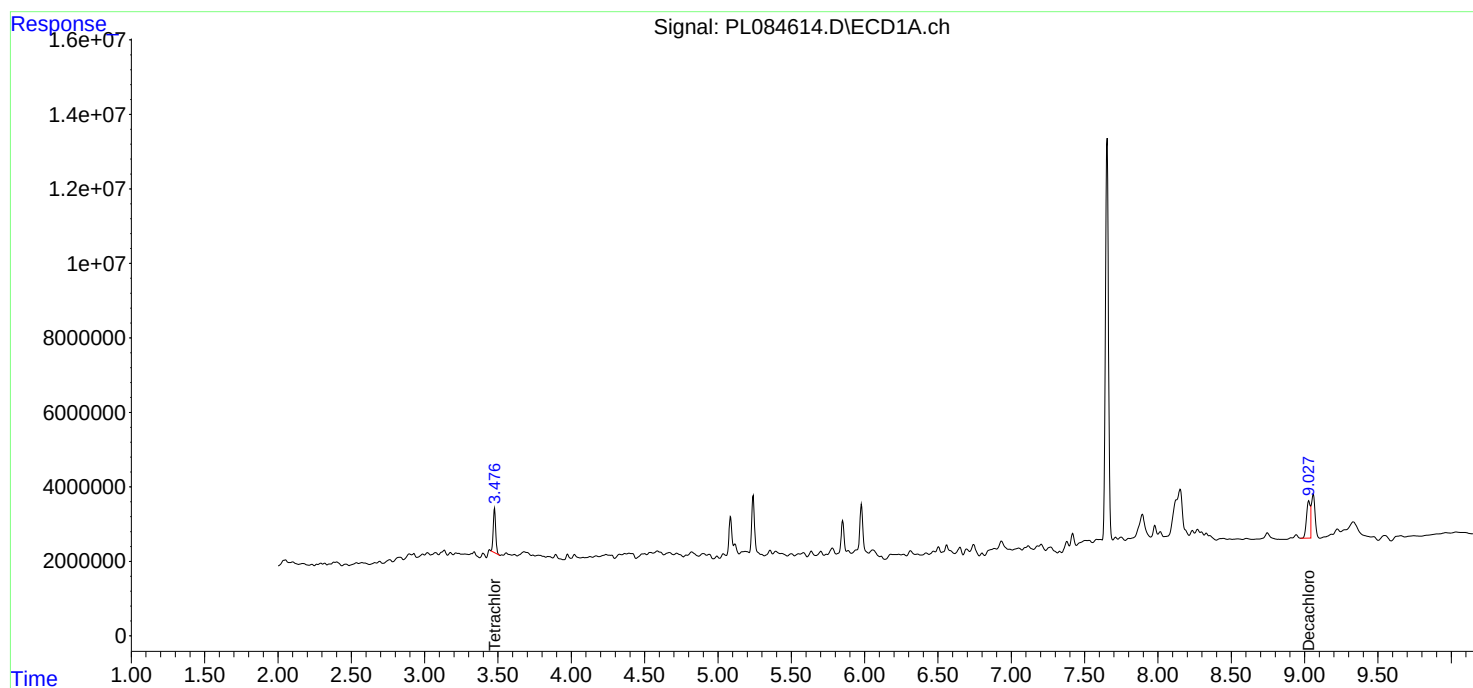

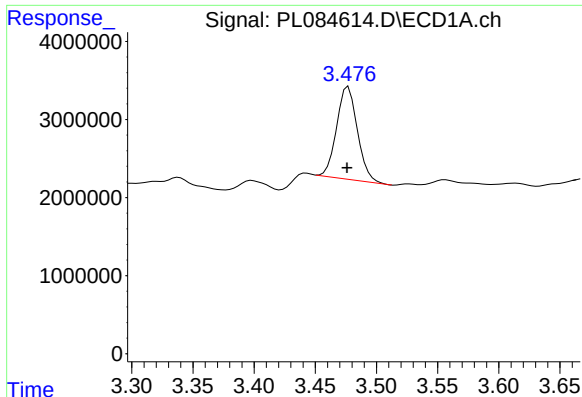


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 14009128
Conc: 6.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEVINS-SB-01-Z67-69


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

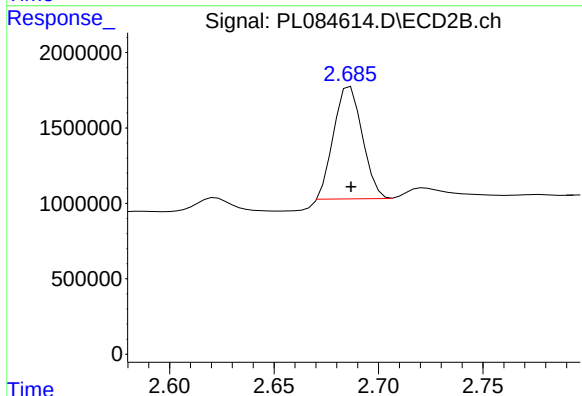


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.002 min
Response: 7062866
Conc: 6.50 ng/ml m

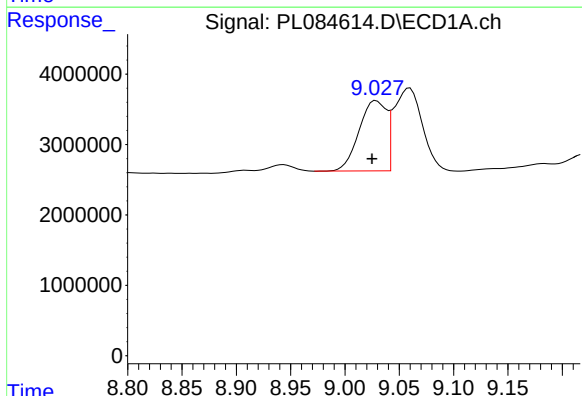

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.004 min
Response: 17450682
Conc: 10.73 ng/ml

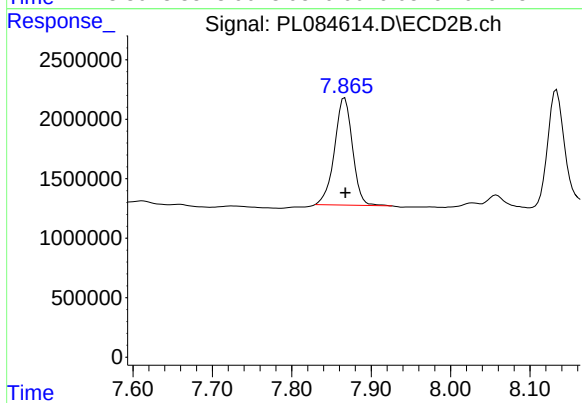

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 14199922
Conc: 11.39 ng/ml