

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080924\
 Data File : PL090911.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2024 22:06
 Operator : AR\AJ
 Sample : P3476-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MUL06

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/09/2024
 Supervised By :Ankita Jodhani 08/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:20:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 06 10:55:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.769f	18280687	498.2E6	9.441m	288.159m#
28)	SA Decachlor...	9.054	7.922	14973779	12878041	10.422m	7.715m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL080924\
Data File : PL090911.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2024 22:06
Operator : AR\AJ
Sample : P3476-05
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MUL06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/09/2024
Supervised By : Ankita Jodhani 08/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:20:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Tue Aug 06 10:55:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

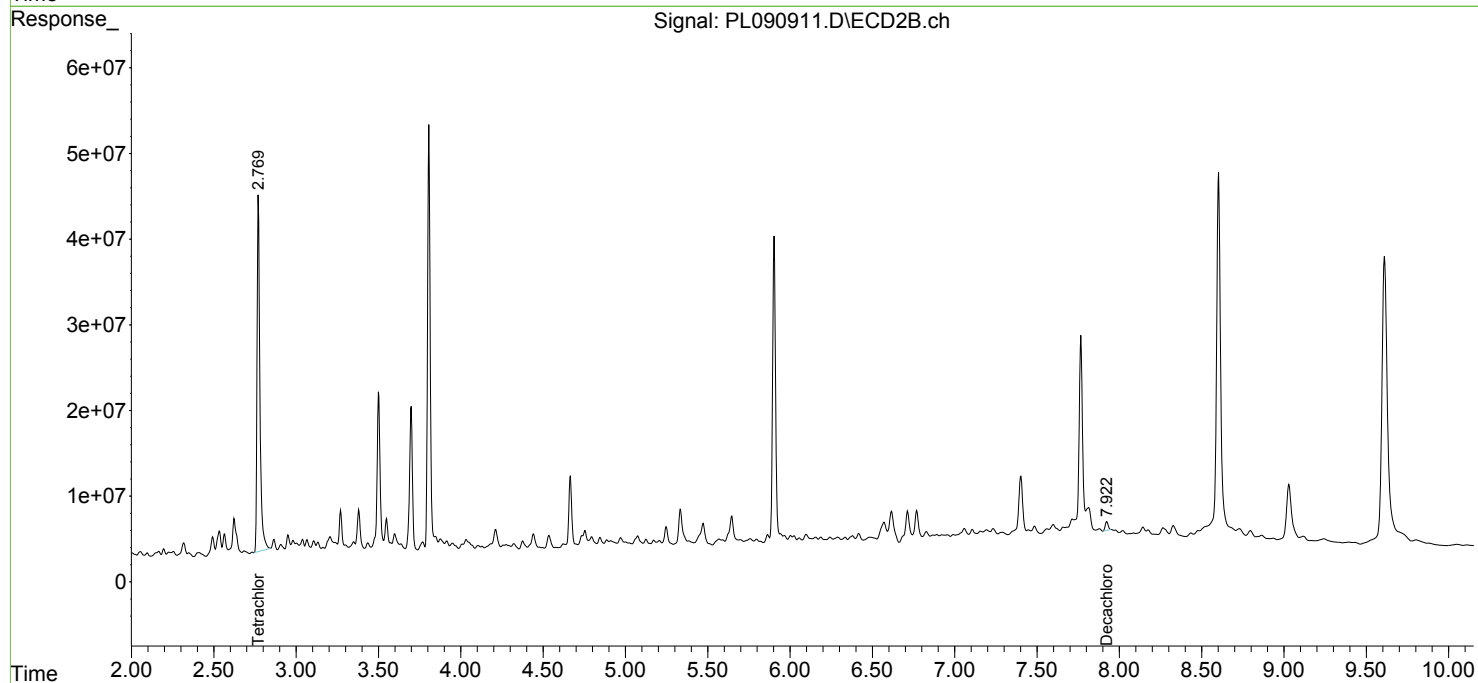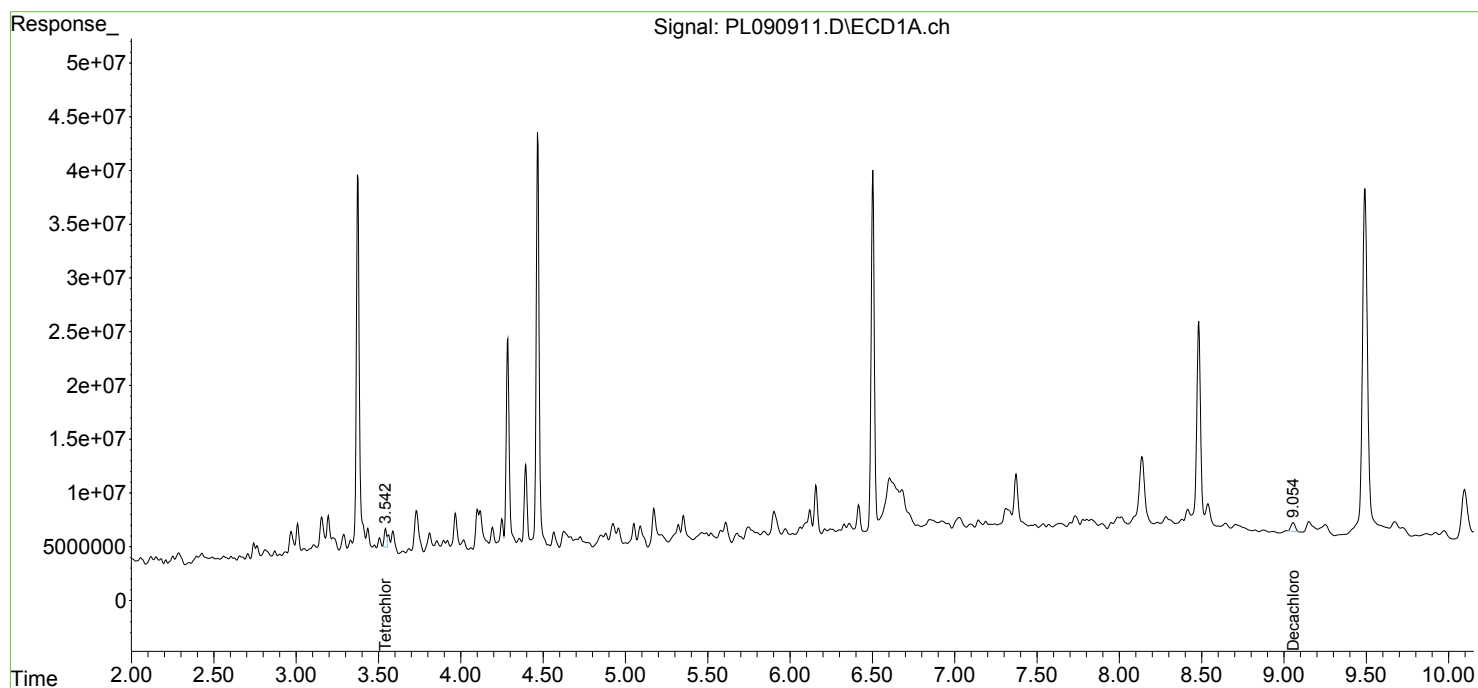

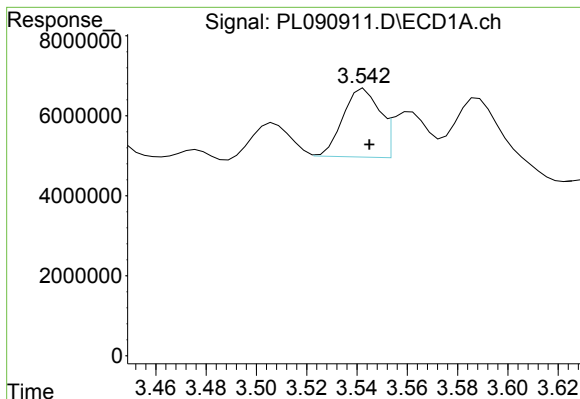


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.003 min
Response: 18280687
Conc: 9.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
MUL06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/09/2024
Supervised By :Ankita Jodhani 08/09/2024

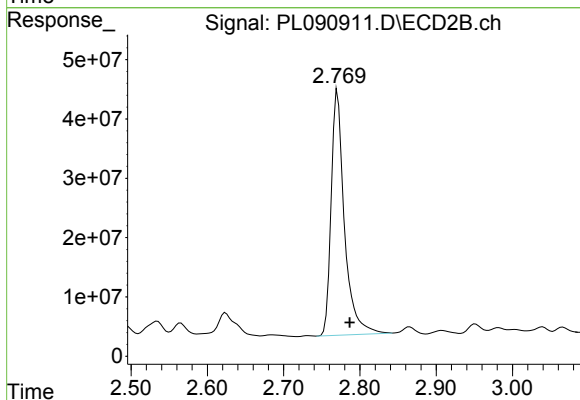


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.017 min
Response: 498170976
Conc: 288.16 ng/ml m

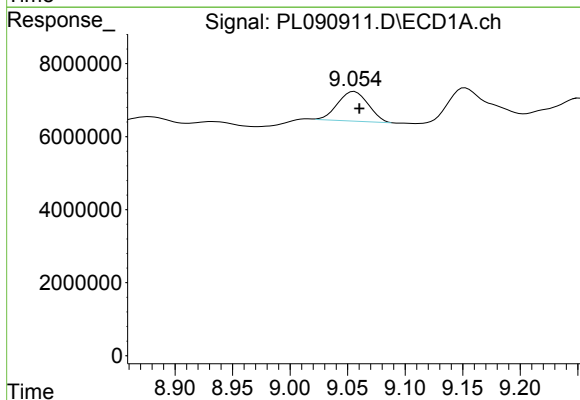

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.006 min
Response: 14973779
Conc: 10.42 ng/ml m

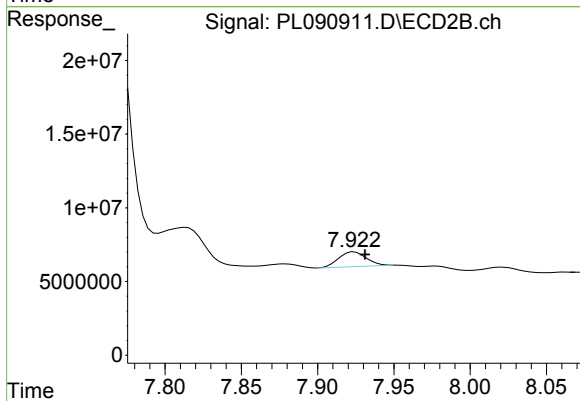

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.009 min
Response: 12878041
Conc: 7.72 ng/ml m