

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081020\
 Data File : PL060580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2020 11:31
 Operator : DD\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:44:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	45693071	64534501	24.373	24.269
28)	SA Decachlor...	8.220	9.097	43814730	45955902	24.004	24.494
Target Compounds							
9)	A Endosulfan I	5.516	6.248	20183910	31255239	10.239	11.035
10)	B gamma-Chl...	5.404	6.125	21587611	43916225	10.182	14.526 #
12)	B 4,4'-DDE	5.628	6.355	39397987	57917439	19.871	20.346
13)	MA Dieldrin	5.759	6.506	42800920	60836358	20.700	20.865
19)	B Endosulfa...	6.670	7.281	37317217	47696121	19.905	19.849
20)	A Methoxychlor	6.930	7.606	104.1E6	127.6E6	103.241	101.304
21)	B Endrin ke...	7.159	7.753	42070888	50050426	20.373	20.538
25)	Chlordane-3	5.404	6.125	21587611	43916225	123.178	121.280



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081020\
Data File : PL060580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2020 11:31
Operator : DD\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:44:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

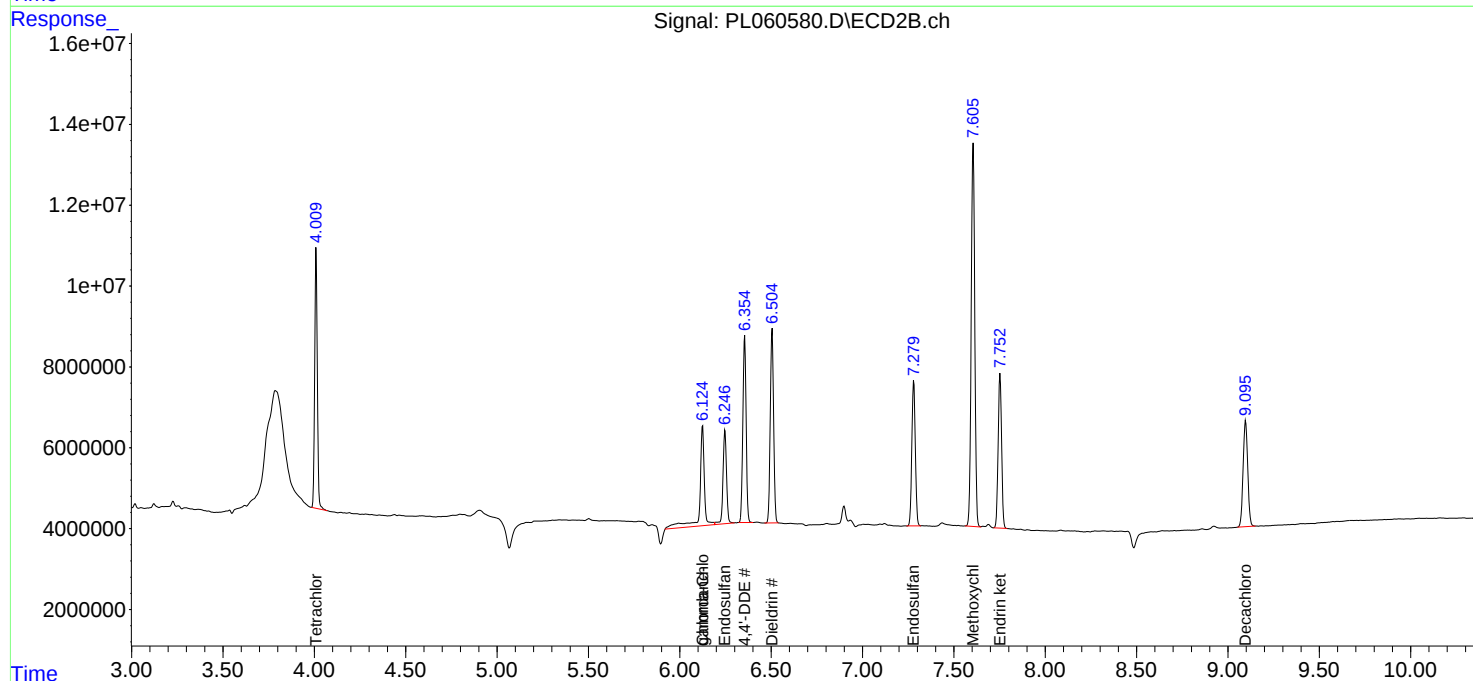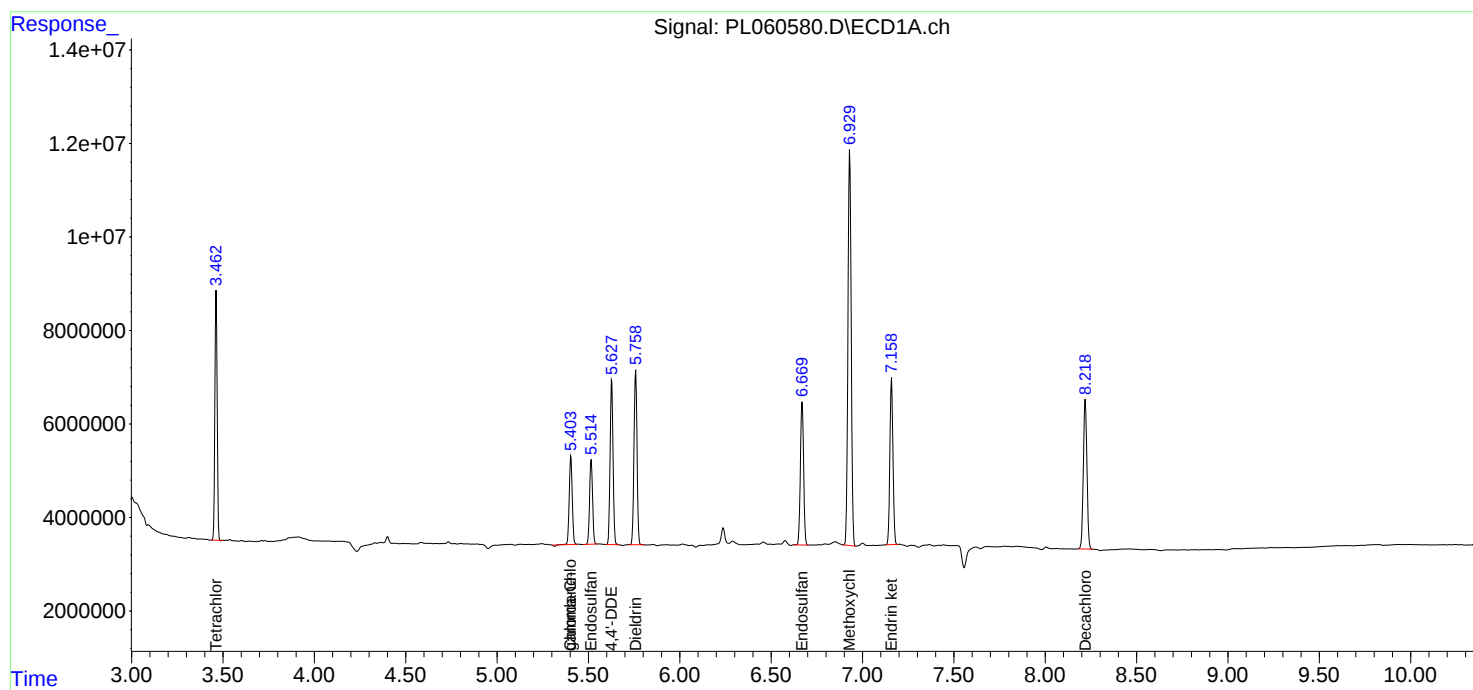


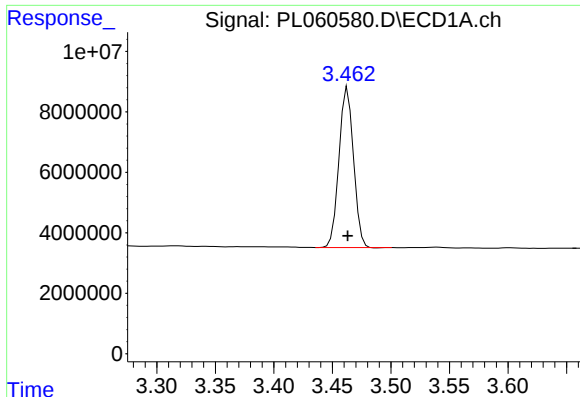

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 45693071
Conc: 24.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

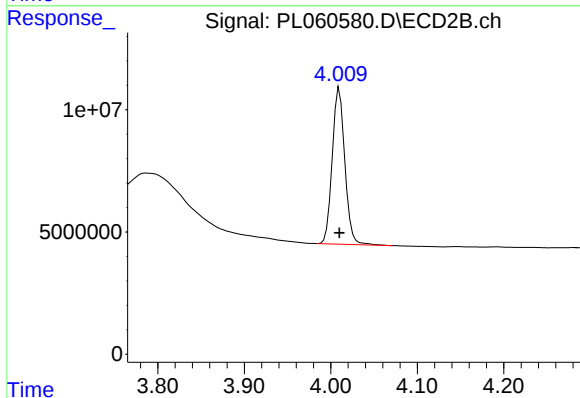


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 64534501
Conc: 24.27 ng/ml

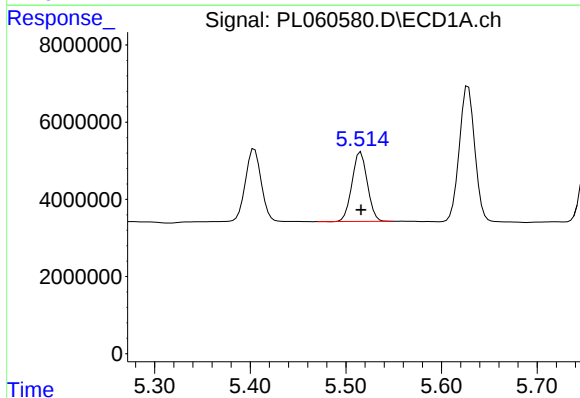


#9 Endosulfan I

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 20183910
Conc: 10.24 ng/ml

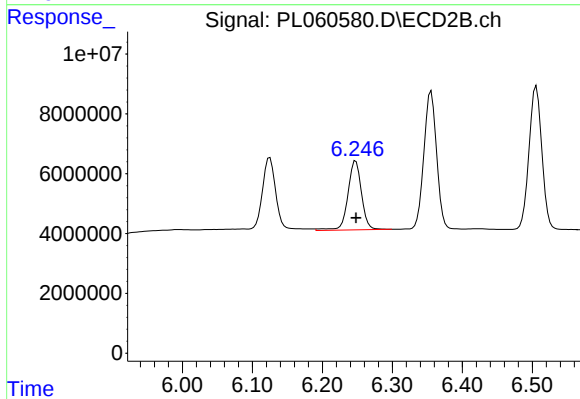

#9 Endosulfan I


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 31255239
Conc: 11.04 ng/ml

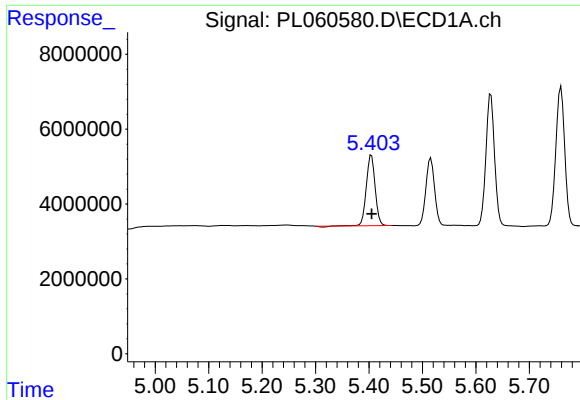

#10 gamma-Chlordane


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 21587611
Conc: 10.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

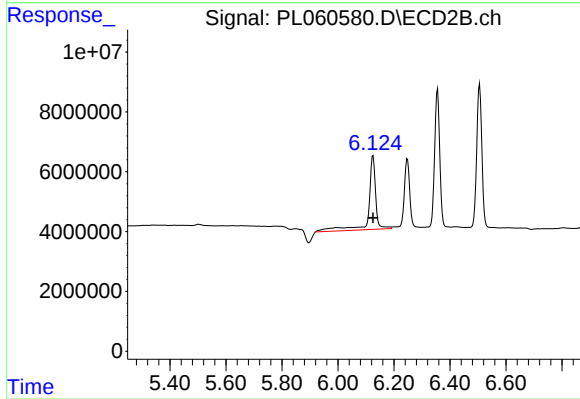


#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 43916225
Conc: 14.53 ng/ml

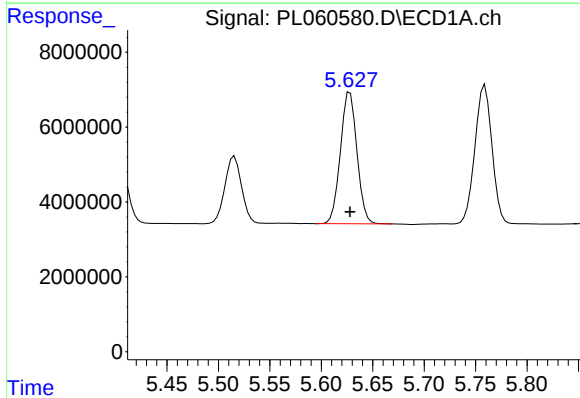


#12 4,4'-DDE

R.T.: 5.628 min
Delta R.T.: 0.000 min
Response: 39397987
Conc: 19.87 ng/ml

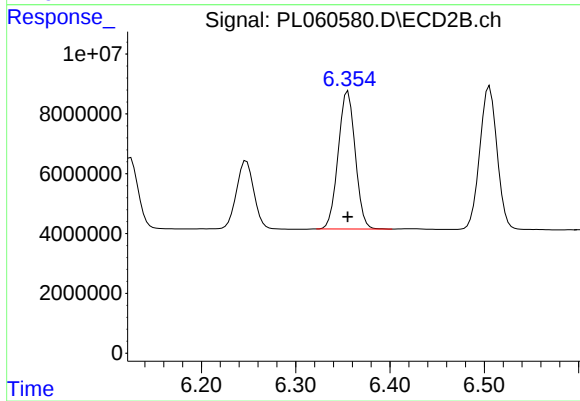

#12 4,4'-DDE


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 57917439
Conc: 20.35 ng/ml

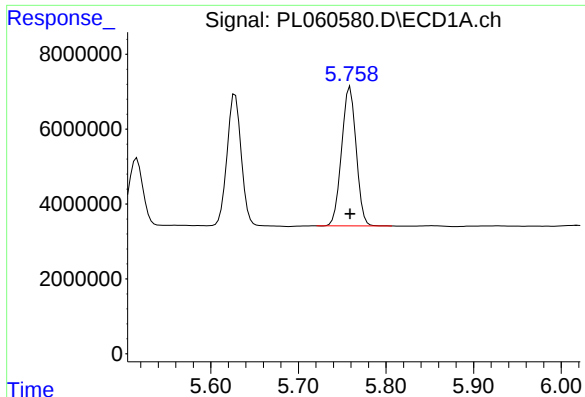

#13 Dieldrin


R.T.: 5.759 min
Delta R.T.: 0.000 min
Response: 42800920
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

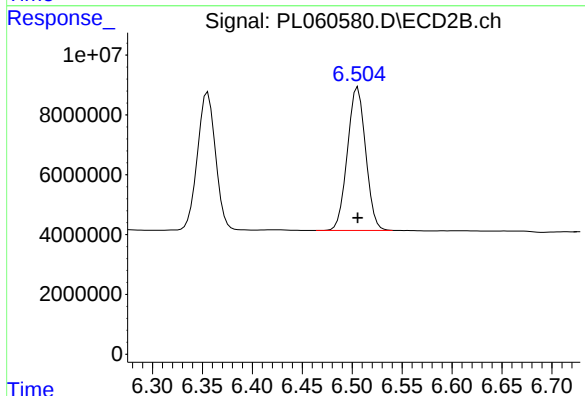


#13 Dieldrin

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 60836358
Conc: 20.86 ng/ml

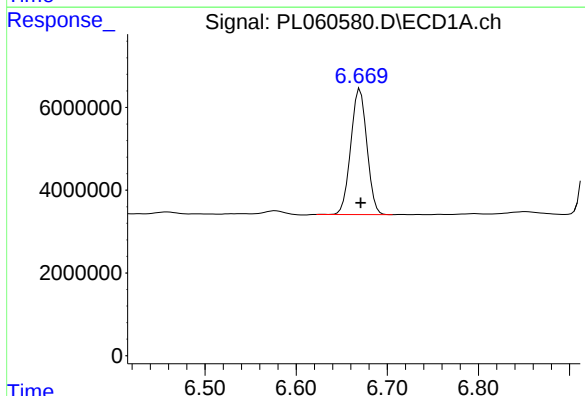


#19 Endosulfan Sulfate

R.T.: 6.670 min
Delta R.T.: 0.000 min
Response: 37317217
Conc: 19.90 ng/ml

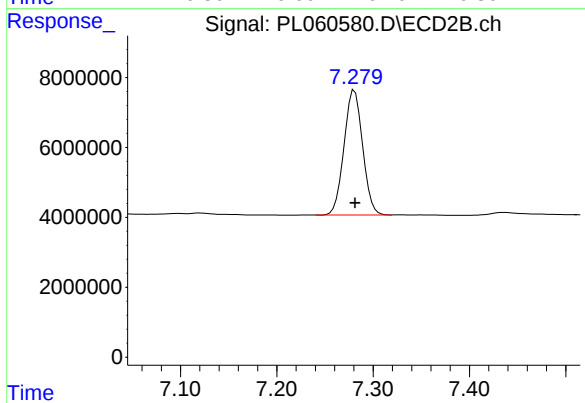

#19 Endosulfan Sulfate


R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 47696121
Conc: 19.85 ng/ml

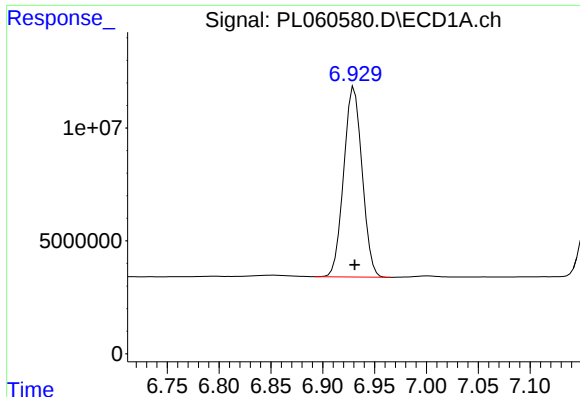

#20 Methoxychlor


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 104123768
Conc: 103.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

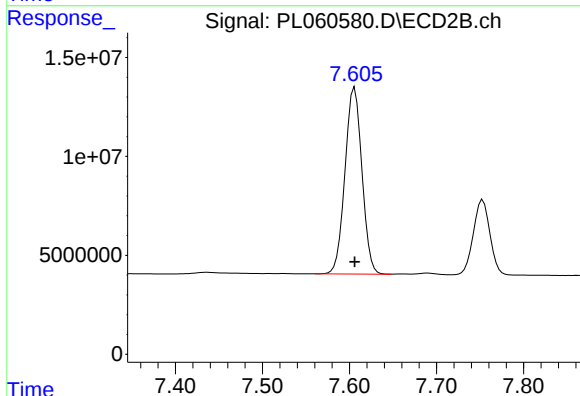


#20 Methoxychlor

R.T.: 7.606 min
Delta R.T.: 0.000 min
Response: 127628499
Conc: 101.30 ng/ml

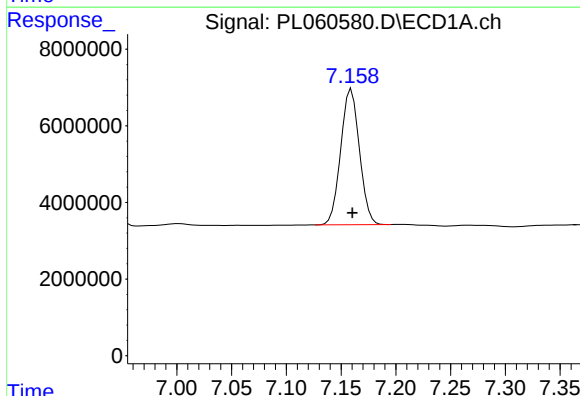


#21 Endrin ketone

R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 42070888
Conc: 20.37 ng/ml

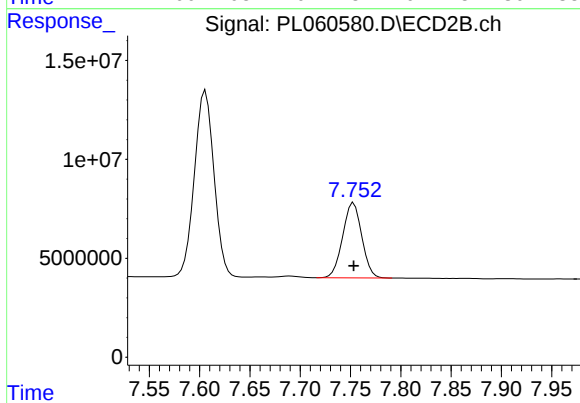

#21 Endrin ketone


R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 50050426
Conc: 20.54 ng/ml

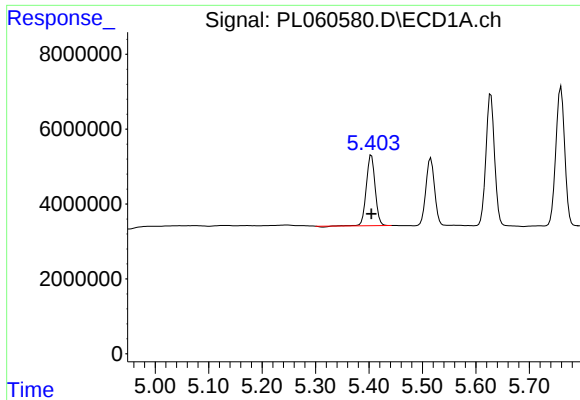

#25 Chlordane-3


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 21587611
Conc: 123.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

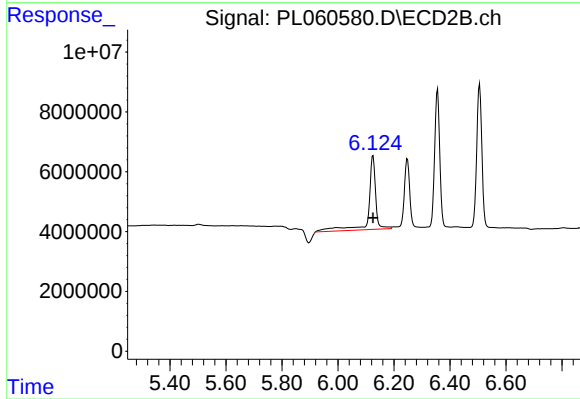


#25 Chlordane-3

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 43916225
Conc: 121.28 ng/ml

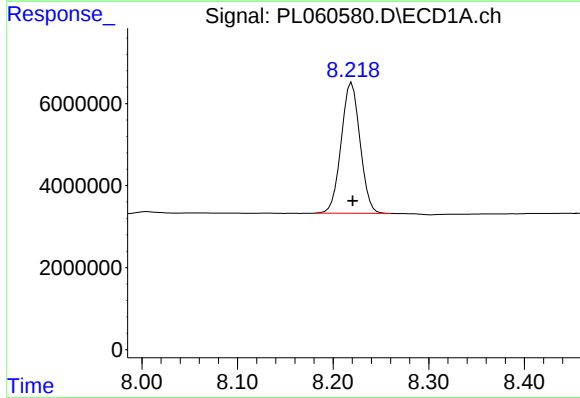

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 43814730
Conc: 24.00 ng/ml

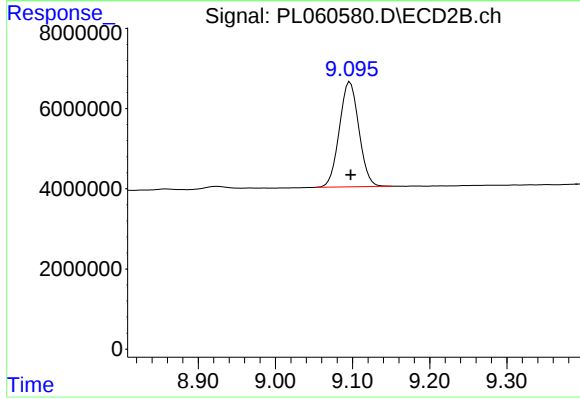

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 45955902
Conc: 24.49 ng/ml